

Nitrite Analyzer *StamoLys CA 70 NO*

Compact photometric analysis system for the nitrite measurement in drinking water and wastewater



Application

- Nitrite monitoring in drinking water
- Nitrite monitoring in wastewater plants

Your benefits

- Direct reaction in photometer at constant temperature
- Low system volume required due to short distances
- Low reagent requirement
- Small sample volume
- Sample heating
- User-friendly interface
- Sample stream monitoring and plain text error menu
- Measured value storage using integrated data logger
- Automatic calibration
- With two channel version: measurement sequences programmable

Quality made by
Endress+Hauser



ISO 9001

Endress + Hauser

The Power of Know How




Function and system design

Measuring principle

Photometric principle

After sample conditioning, the Analyzer sample pump conveys a defined part of the filtrate to a mixing vessel. The reagent pump adds reagent at a specific ratio. As a result of the reaction, the sample turns a characteristic colour. The photometer determines the sample absorption of an emitted light at a specific wavelength (s. Fig., Pos. 2). The wavelength is parameter specific. The absorbed light intensity is proportional to the concentration of the specified parameter in the sample (Pos. 3). Additionally, the absorption of a reference light is determined to receive a genuine measuring result. The reference signal is subtracted from the measuring signal to prevent any effects due to turbidity, contamination and ageing of the LEDs.

The temperature in the photometer is controlled thermostatically so that the reaction is reproducible and takes place within a short period of time.

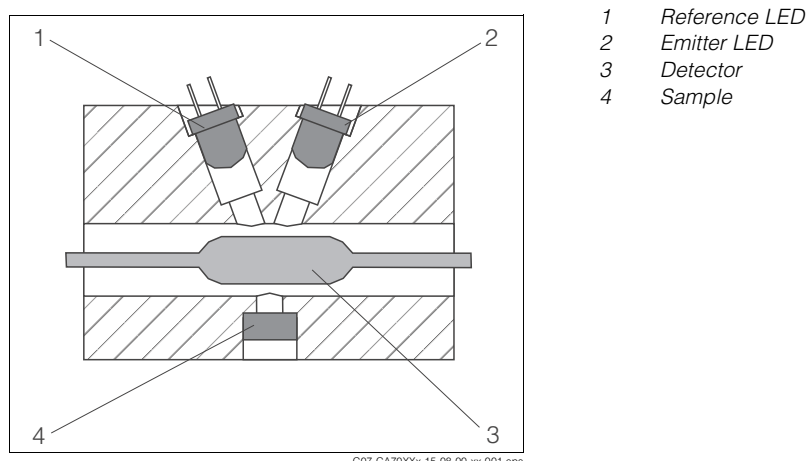

Photometric principle

Naphthylamine method for nitrite determination acc. to DIN 38405-D10

Under acidic conditions, nitrite ions diazotize sulphonamido, which forms a red dye in conjunction with N-(1-naphthyl)-ethylenediamine.

The absorption is determined at a wavelength of 565 nm. The intensity of absorbed light is proportional to the ammonium concentration in the sample.

The reference wavelength is 880 nm.

Sample conditioning

Analyzer in connection with membrane filtration (StamoClean CAT 430, optionally)

A membrane filter element is suspended directly into the wastewater basin or channel. A hose pump is located in a pump box on the basin rim. The pump creates a vacuum between the membrane and the carrier plate of the filter element. This vacuum makes the filtrate pass through the filter membrane. Suspended materials, particles, algae and bacteria are collected on the surface of the membrane.

Due to an alternating pumping periods, intervals of more than one month are achieved between cleaning cycles. Parallel connection of two or four filter elements increases the sampling quantity up to 1 l/h approx.

The hose pump pressure transports the sample to a collecting vessel near the analyzer over a distance of 20 m. For distances up to 100 m the sample is transported to the collecting vessel by means of compressed air. The analyzers suck the needed sample volume from the collecting vessel.

Analyzer without E+H sample conditioning


Before analysis, the sample has to be conditioned and to be transported to an external or to the delivered collecting vessel.

Measuring system

A complete measuring system comprises:

- An analyzer StamoLys CA 70
- A sample conditioning system (optionally):
 - Micro filtration / ultra filtration StamoClean CAT 430 or StamoClean CAT 411
 - Backwash filter StamoClean CAT 220
 - Customer specific solution
- Wall mounting set (optionally)
- Collecting vessel (optionally)


Micro / ultra filtration

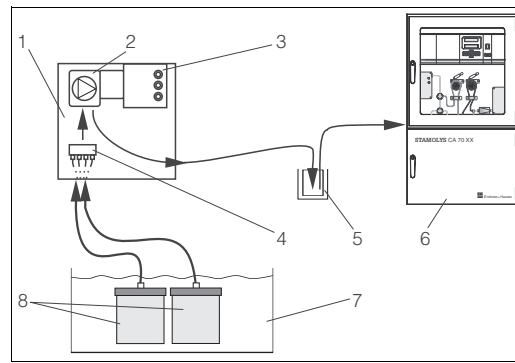

C07-CA70XXx-14-08-00-xx-001.eps

Measuring with StamoClean CAT 430

- 1 Hose pump box
- 2 Hose pump
- 3 Control unit
- 4 Collecting unit (optionally)
- 5 Collecting vessel
- 6 Analyzer
- 7 Aeration basin
- 8 Membrane filter

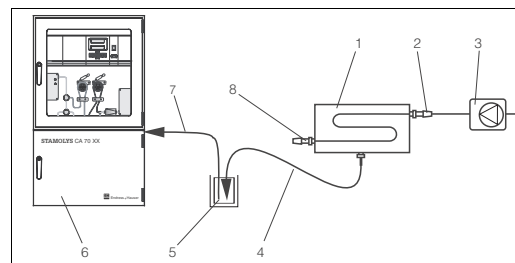


C07-CA70XXx-14-08-00-xx-002.eps

Measuring system with StamoClean CAT 411

- 1 StamoClean CAT 411
- 2 Inlet
- 3 Sample pump or hydraulic main
- 4 Filtrate line
- 5 Collecting vessel
- 6 Analyzer
- 7 Sample line analyzer
- 8 Outlet

Backwash filter

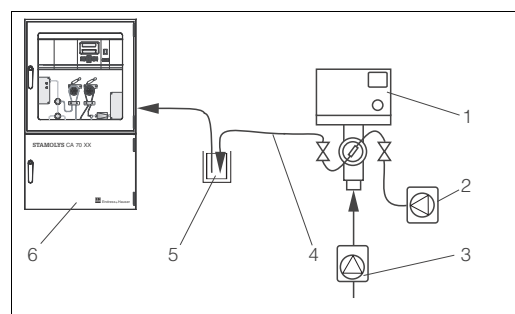

C07-CA70XXx-14-08-00-xx-002.eps

Measuring system with StamoClean CAT 220

- 1 StamoClean CAT 220
- 2 Compressor or compressed air
- 3 Sample pump or hydraulic main
- 4 Sample out
- 5 Collecting vessel
- 6 Analyzer

Input


Measured variable	NO ₂ -N [mg/l]
Measuring ranges	0.01 ... 0.5 mg/l 0.1 ... 1.5 mg/l 0.2 ... 3.0 mg/l
Wavelength	565 nm
Reference wavelength	880 nm

Output


Output signal	0/4 ... 20 mA
Signal on alarm	2 limit contacts (per channel), 1 system alarm contact
Load	max. 500 Ω
Data interface	RS 232 C
Load capacity	30 VA max. 48 V AC, 30 V DC at 0.5 A

Power supply

Electrical connection

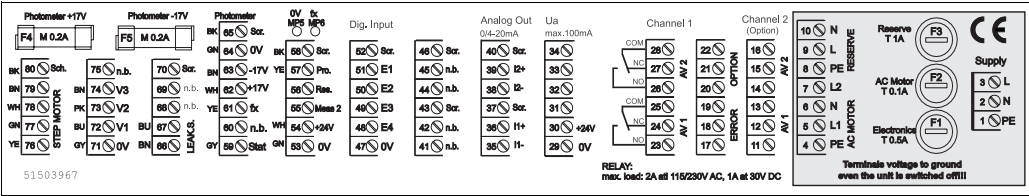

Connection sticker CA 70

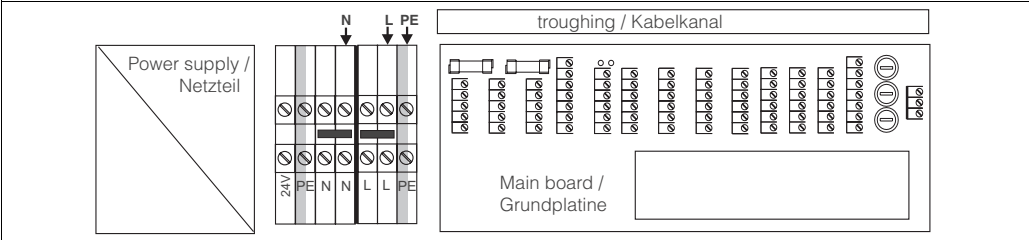

Power supply reagent cooling device

Supply voltage	115 V AC / 230 V AC ±10%, 50/60 Hz
Power consumption	without reagent cooling ca. 40 VA with reagent cooling ca. 200 VA

Current consumption	without reagent cooling	ca. 0.15 A
	with reagent cooling	ca. 0.9 A

Fuses	medium time-lag 0.2 A, time-lag 0.5 A
--------------	---------------------------------------

Performance characteristics

Response time t_{100}	Reaction time + flushing time + waiting time (minimum waiting time = 0 min)
---	---

Maximum measured error	3 % of measuring range scope
-------------------------------	------------------------------

Measuring interval	2 ... 120 min
---------------------------	---------------

Measuring time	6 minutes
-----------------------	-----------

Sample requirement	15 ml per measurement
---------------------------	-----------------------

Reagent requirement	2 x 0.5 ml per measurement
----------------------------	----------------------------

Calibration interval	0 ... 72 h
-----------------------------	------------

Flushing interval	0 ... 72 h
--------------------------	------------


Maintenance interval	3 month
-----------------------------	---------

Servicing requirements	15 minutes a week
-------------------------------	-------------------

Installation


Installation instructions

Wall mounting set (Accessories, with reagent cooling essentially)

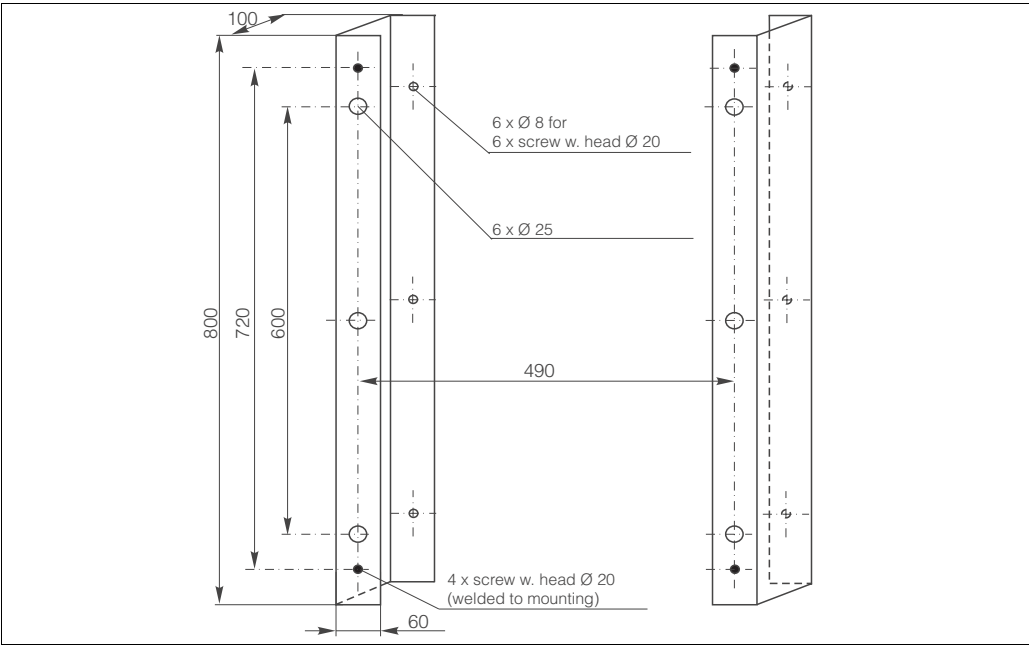

C07-CA70xxxx-17-08-00-xx-001.eps

Wall mounting set for analyzer with reagent cooling device

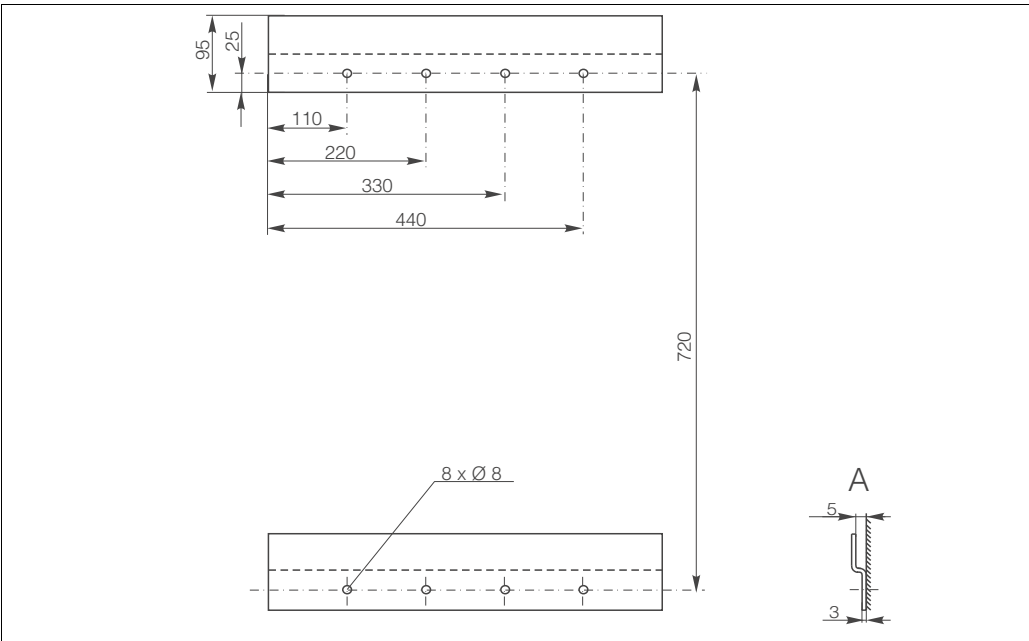

C07-CA70xxxx-17-08-00-xx-002.eps

Wall mounting set for analyzer without reagent cooling device

Environment

Ambient temperature limit 5 ... 40 °C (with temperatures > 25 °C a reagent cooling device is essential)


Ingress protection IP 43

Process


Sample flow rate	min. 5 ml per min
Consistence of the sample	low solid content (< 50 mg/l)
Sample requirement per measurement	20 ml
Sample inlet	pressureless

Mechanical construction

Design, dimensions

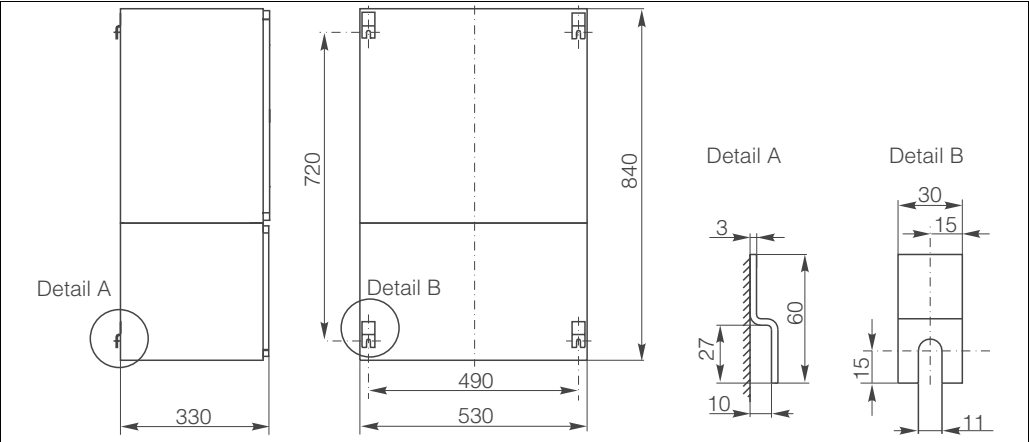

CA 70 dimensions

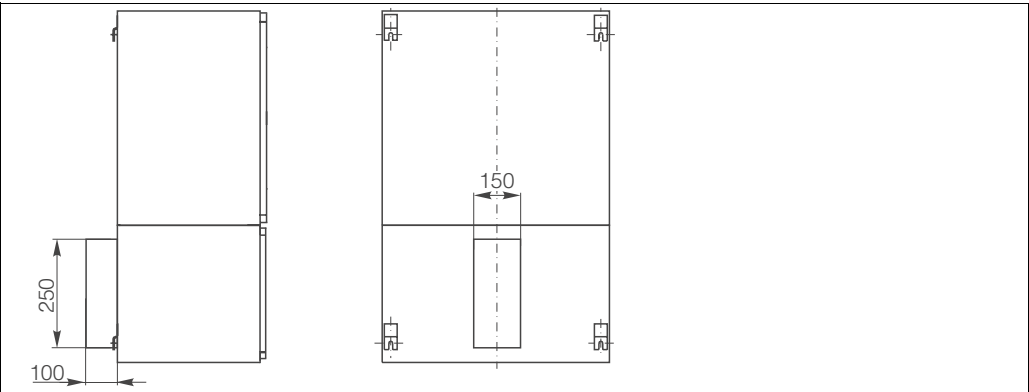


Reagent cooling device dimensions

Weight	Without reagent cooling With reagent cooling	ca. 40 kg ca. 50 kg
Materials	Housing Front windows Endless hose Pump hose	Stainless Steel 1.4573 (AISI 316 Ti) Plexiglas® C-Flex®, Norprene® Tygon®, Viton®

Connection sample line	One channel version	
	Internal collecting vessel	
	Connection	hose ID 3.2 mm
	External collecting vessel	
	Connection	hose ID 1.6 mm
	Max. distance from collecting vessel to analyzer	1 m
	Max. height difference from collecting vessel to analyzer	0.5 m
	Two channel version	
	With option "collecting vessel": two external collecting vessels on a PVC plate mounted	
	Connection collecting vessel to analyzer	2 x hose ID 1.6 mm
Sample outlet	Connection	hose ID 6.4 mm
		– Max. length of closed loop 1 m
		– Open outlet mounted falling
		– No combination of several devices to a closed-loop system
	Min. volume per meas.	20 ml

Human Interface

Display and operating elements

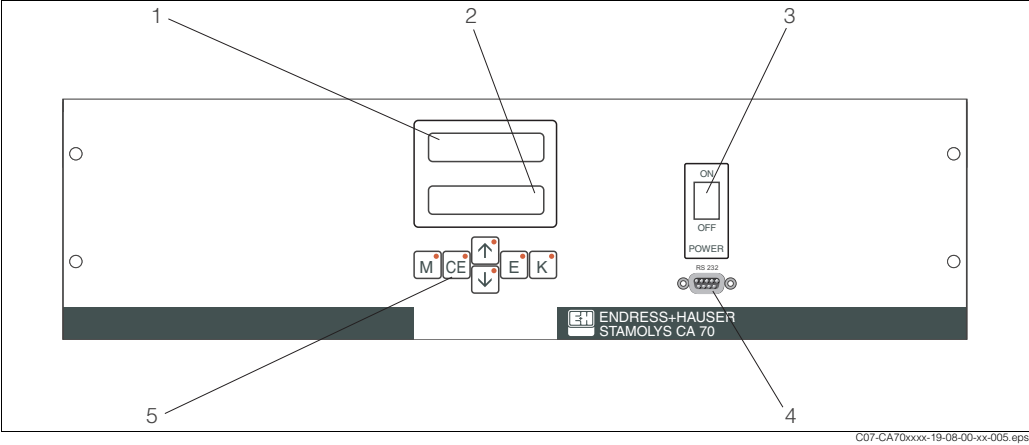

- Display and operating elements CA 70
- 1 LED display (measured value)
 - 2 LC display (measured value + status)
 - 3 Toggle switch on/off
 - 4 RS 232 serial interface
 - 5 Operating keys with indicator LEDs

Certificates and approvals

CE approval

Declaration of conformity

The product meets the legal requirements of the harmonised European standards.
Endress+Hauser confirms compliance with the standards by affixing the **CE** symbol.

Test reports

Quality certificate

Depending on the order code you receive a quality certificate.
With the certificate Endress+Hauser confirms compliance with all technical regulations and the successful testing individually for your product.

Ordering information

Product structure

		Measuring range	
	A	Measuring range 0.01 ... 0.5 mg/l	
	B	Measuring range 0.1 ... 1.0 mg/l	
	C	Measuring range 0.2 ... 3.0 mg/l	
	Y	Special version acc. to customers specification	
		Sample transfer	
	1	Sample transfer from one measuring point (one channel version)	
	2	Alternating sample transfer from two measuring points (two channel version)	
	9	Special version acc. to customers specification	
		Power supply	
	0	Power supply 230 V AC	
	1	Power supply 115 V AC	
	9	Special version acc. to customers specification	
		Collecting vessel	
	A	Without collecting vessel	
	B	With collecting vessel	
	Y	Special version acc. to customers specification	
		Equipment	
	1	Without reagent cooling device	
	2	With reagent cooling device	
	9	Special version acc. to customers specification	
		Communication	
	A	RS 232 + 0/4 ... 20 mA	
	Y	Special version acc. to customers specification	
		Additional equipment	
	1	Quality certificate	
	9	Special version acc. to customers specification	
CA 70 NO-			complete order code

Accessories

Installation accessories

- ☐ Wall mounting set for version without reagent cooling device; order no. 51503061
- ☐ Wall mounting set for version with reagent cooling device; order no. 51503063

Reagents and standard solutions

- ☐ Reagent NO1, 1 l; order no. CAY343-V10AAE
- ☐ Cleaning agent R; order no. CAY344-V10AAE
- ☐ Standard (parent solution) 250 mg/l NO₂ - N; order no. CAY345-V05C25AAE

Documentation

- ☐ Technical Information StamoClean CAT 430, TI 338C/07 (order no. 51508729)
- ☐ Technical Information StamoClean CAT 411, TI 349C/07 (order no. 51508785)
- ☐ Technical Information StamoClean CAT 220, TI 317C/07 (order no. 51509817)

Endress+Hauser GmbH+Co. KG

Instruments International
P.O. Box 2222
D-79574 Weil am Rhein
Germany

Tel. (07621) 975-02
Tx 773926
Fax (07621) 975 345
e-mail: info@ii.endress.com

Internet:

<http://www.endress.com>

Endress + Hauser

The Power of Know How

