

Description of Device Parameters

Proline Promass 10

Coriolis flowmeter
Modbus RS485

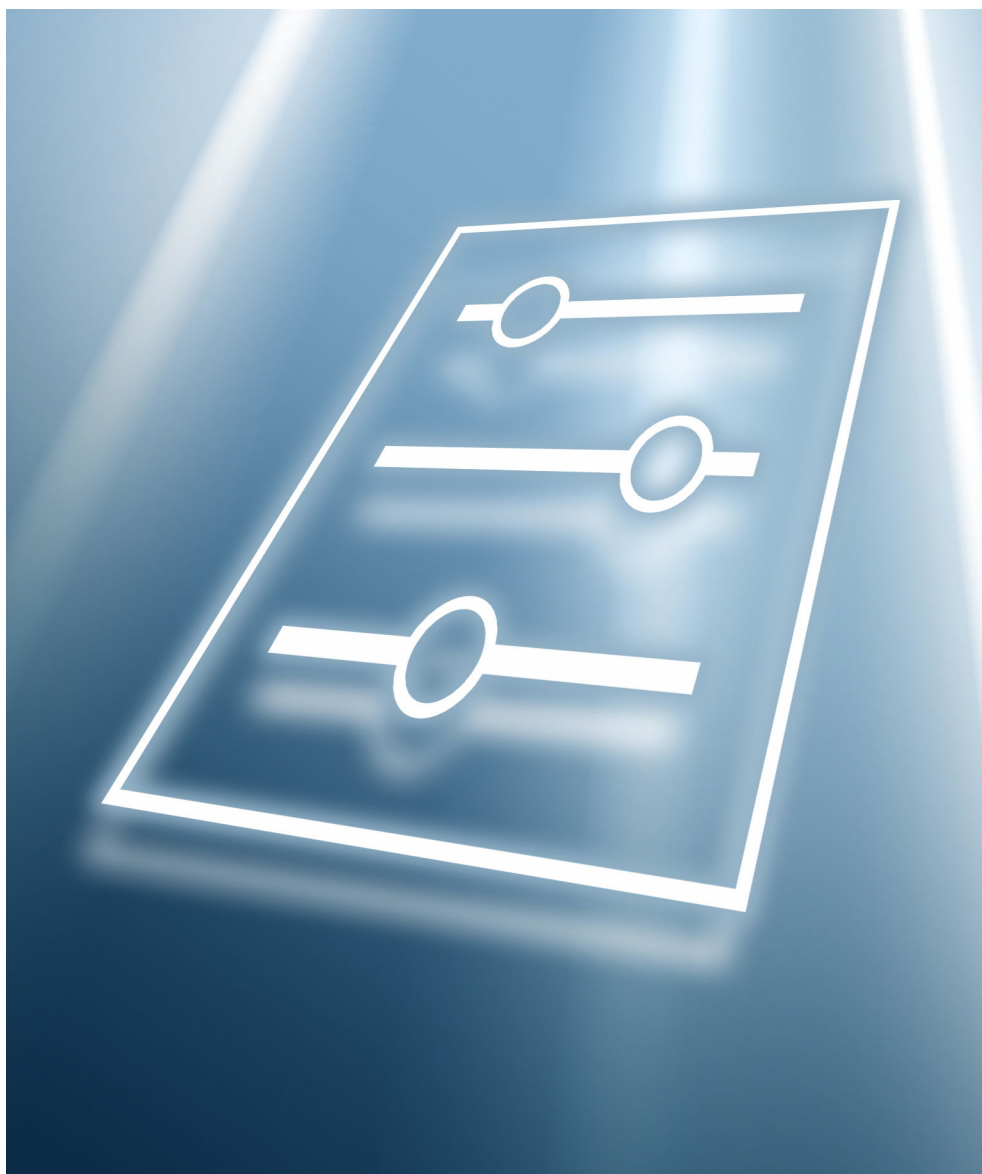


Table of contents

1	About this document	4		
1.1	Document function	4		
1.2	Target group	4		
1.3	Using this document	4		
1.3.1	Symbols	4		
1.3.2	Information on the document structure	4		
1.3.3	Structure of a parameter description	5		
1.4	Associated documentation	5		
2	"Guidance" menu	6		
2.1	"Commissioning" wizard	6		
2.1.1	Device identification	8		
2.1.2	Medium	9		
2.1.3	System units	11		
2.1.4	Totalizer 1 to n	16		
2.1.5	Process parameters	19		
2.1.6	Measuring conditions	19		
2.1.7	Current output	23		
2.1.8	Display	28		
2.1.9	Date/time	30		
3	"Diagnostics" menu	32		
3.1	"Actual diagnostics" submenu	33		
3.2	"Diagnostic list" submenu	35		
3.3	"Simulation" submenu	38		
3.4	"Heartbeat Technology" submenu	41		
3.5	"Diagnostic settings" submenu	42		
3.5.1	"Properties" submenu	42		
3.5.2	"Diagnostic configuration" submenu	42		
4	"Application" menu	53		
4.1	"Measured values" submenu	53		
4.1.1	"Totalizer" submenu	55		
4.2	"System units" submenu	57		
4.3	"Totalizers" submenu	63		
4.3.1	"Totalizer handling" submenu	63		
4.3.2	"Totalizer 1 to n" submenu	63		
4.4	"Sensor" submenu	68		
4.4.1	"Process parameters" submenu	68		
4.4.2	"Low flow cut off" submenu	70		
4.4.3	"Partially filled pipe detection" submenu	71		
4.4.4	"Medium settings" submenu	73		
4.4.5	"Two phase flow" submenu	74		
4.4.6	"External compensation" submenu	77		
4.4.7	"Corrected volume flow calculation" submenu	77		
4.4.8	"Sensor adjustment" submenu	80		
4.4.9	"Calibration" submenu	85		
4.5	"Current output" submenu	87		
4.6	"Communication" submenu	98		
4.6.1	"Modbus configuration" submenu	98		
4.6.2	"Modbus data map" submenu	101		
4.6.3	"Modbus information" submenu	102		
5	"System" menu	103		
5.1	"Device management" submenu	104		
5.2	"User management" submenu	107		
5.2.1	"Define access code" wizard	109		
5.3	"Connectivity" submenu	110		
5.3.1	"Bluetooth configuration" submenu	110		
5.4	"Date / Time" submenu	111		
5.5	"Information" submenu	113		
5.5.1	"Device" submenu	113		
5.5.2	"Sensor electronic module (ISEM)" submenu	116		
5.5.3	"Display module" submenu	116		
5.6	"Display" submenu	118		
5.7	"Software configuration" submenu	122		
6	Modbus RS485 register information	123		
6.1	Notes	123		
6.1.1	Structure of the register information	123		
6.1.2	Address model	123		
6.2	Overview of the operating menu	124		
6.3	Register information	134		
6.3.1	"Guidance" menu	134		
6.3.2	"Diagnostics" menu	144		
6.3.3	"Application" menu	147		
6.3.4	"System" menu	159		
	Index	164		

1 About this document

1.1 Document function

The document is part of the Operating Instructions and serves as a reference for parameters, providing a detailed explanation of each individual parameter of the operating menus.

It is used to perform tasks that require detailed knowledge of the function of the device:

- Optimal adaptation of the measurement to difficult conditions
- Detailed configuration of the communication interface
- Error diagnostics in difficult cases

1.2 Target group

The document is aimed at specialists who work with the device over the entire life cycle and perform specific configurations.

1.3 Using this document

1.3.1 Symbols

Types of information

-  Preferred procedures, processes or actions
-  Permitted procedures, processes or actions
-  Forbidden procedures, processes or actions
-  Additional information
-  Reference to documentation
-  Reference to page
-  Reference to graphic

1.3.2 Information on the document structure

The parameters of all the operating menus and the commissioning wizard are described in this document.

- **Guidance** menu with the **Commissioning** wizard (→  6), which guides the user automatically through all the device parameters that are required for commissioning
- **Application** menu (→  53)
- **Diagnostics** menu (→  32)
- **System** menu (→  103)

1.3.3 Structure of a parameter description

The individual parts of a parameter description are described in the following section:

Complete parameter name		Write-protected parameter = 
Navigation	 Navigation path to the parameter via the operating tool The names of the menus, submenus and parameters are abbreviated to the form in which they appear on the display and in the operating tool.	
Prerequisite	The parameter is only available under these specific conditions	
Description	Description of the parameter function	
Selection	List of the individual options for the parameter ■ Option 1 ■ Option 2	
User entry	Input range for the parameter	
User interface	Display value/data for the parameter	
Additional information	Additional explanations (e.g. in examples): ■ On individual options ■ On display values/data ■ On the input range ■ On the parameter function	

1.4 Associated documentation

Technical Information	Overview of the device with the most important technical data.
Operating Instructions	All the information that is required in the various phases of the life cycle of the device: from product identification, incoming acceptance and storage, to mounting, connection, operation and commissioning through to troubleshooting, maintenance and disposal as well as the technical data and dimensions.
Sensor Brief Operating Instructions	Incoming acceptance, transport, storage and mounting of the device.
Transmitter Brief Operating Instructions	Electrical connection and commissioning of the device.
Description of Parameters	Detailed explanation of the menus and parameters.
Safety Instructions	Documents for the use of the device in hazardous areas.
Special Documentation	Documents with more detailed information on specific topics.
Installation Instructions	Installation of spare parts and accessories.

The related documentation is available online:

W@M Device Viewer	On the www.endress.com/deviceviewer website, enter the serial number of the device: nameplate
Endress+Hauser Operations App	► Scan the Data Matrix code: nameplate ► Enter the serial number of the device: nameplate

2 "Guidance" menu

Main functions for use – from fast and safe commissioning to guided support during operation.

Navigation  Guidance

Guidance

► Commissioning

→  6

2.1 "Commissioning" wizard

Complete this wizard to commission the device. NOTE: If you exit the wizard beforehand, the changes you made will be saved. For this reason, the device may be in an undefined state! In this case, reset the device to the default settings.

Navigation  Guidance → Commissioning

► Commissioning

Device tag

Serial number

Firmware version

Device name

Select medium

Select gas type

Reference sound velocity

Temperature coefficient sound velocity

Pressure compensation

Pressure value

Mass flow unit

Mass unit

Volume flow unit

Volume unit

→  8

→  8

→  9

→  9

→  9

→  9

→  10

→  10

→  11

→  11

→  11

→  12

→  12

→  13

Corrected volume flow unit	→  14
Corrected volume unit	→  14
Density unit	→  15
Reference density unit	→  15
Temperature unit	→  15
Pressure unit	→  16
Assign process variable	→  16
Unit totalizer 1 to n	→  16
Totalizer operation mode	→  18
Failure mode	→  18
Flow damping time	→  19
Low flow cut off	→  20
On value low flow cutoff	→  21
Off value low flow cutoff	→  21
Pressure shock suppression	→  19
Partially filled pipe detection	→  22
Low value partial filled pipe detection	→  22
High value partial filled pipe detection	→  22
Process variable current output	→  23
Current range output	→  23
Lower range value output	→  24
Upper range value output	→  26
Damping current output	→  26
Fixed current	→  26
Failure behavior current output	→  27

Failure current	→  27
Value 1 display	→  28
Value 2 display	→  28
Value 3 display	→  29
Value 4 display	→  29
Display damping	→  30
Time format	→  30
Time zone	→  30
Set date/time	→  31

2.1.1 Device identification

Navigation   Guidance → Commissioning

Device tag

Navigation	  Guidance → Commissioning → Device tag
Description	Enter a unique designation for the measuring point to be able to easily identify it within the plant.
User entry	Character string comprising numbers, letters and special characters (#32)

Serial number

Navigation	  Guidance → Commissioning → Serial number
Description	Displays the serial number of the measuring device. The serial number can be used to identify the measuring device and to retrieve further information on the measuring device, such as the related documentation, via the Device Viewer or Operations app. Additional information: The serial number can also be found on the nameplate of the sensor and transmitter.
User interface	Character string comprising numbers, letters and special characters (#11)

Firmware version

Navigation	  Guidance → Commissioning → Firmware version
Description	Displays the device firmware version installed.
User interface	Character string comprising numbers, letters and special characters (#8)

Device name

Navigation	  Guidance → Commissioning → Device name
Description	Displays the name of the transmitter. Additional information: The name can also be found on the transmitter's nameplate.
User interface	Character string comprising numbers, letters and special characters (#16)

2.1.2 Medium

Navigation   Guidance → Commissioning

Select medium

Navigation	  Guidance → Commissioning → Select medium
Description	Select the medium type.
Selection	■ Liquid ■ Gas

Select gas type

Navigation	  Guidance → Commissioning → Select gas type
Prerequisite	In the Select medium parameter in the Medium settings submenu, the Gas option is selected.
Description	Select the type of gas. Additional information: To achieve accurate measurements, it is necessary to specify the gas.

Selection	■ Air ■ Ammonia NH₃ ■ Argon Ar ■ Sulfur hexafluoride SF₆ ■ Oxygen O₂ ■ Ozone O₃ ■ Nitrogen oxide NO_x ■ Nitrogen N₂ ■ Nitrous oxide N₂O ■ Methane CH₄ ■ Hydrogen H₂ ■ Helium He ■ Hydrogen chloride HCl ■ Hydrogen sulfide H₂S ■ Ethylene C₂H₄ ■ Carbon dioxide CO₂ ■ Carbon monoxide CO ■ Chlorine Cl₂ ■ Butane C₄H₁₀ ■ Propane C₃H₈ ■ Propylene C₃H₆ ■ Ethane C₂H₆ ■ Others
------------------	--

Reference sound velocity	
---------------------------------	---

Navigation	 Guidance → Commissioning → Sound velocity
Prerequisite	In the Select gas type parameter in the Medium settings submenu, the Others option is selected.
Description	Enter sound velocity of the gas at 0 °C (32 °F).
User entry	1 to 99 999.9999 m/s

Temperature coefficient sound velocity	
---	---

Navigation	 Guidance → Commissioning → Temp. coeff. SV
Prerequisite	In the Select gas type parameter in the Medium settings submenu, the Others option is selected.
Description	Enter the temperature coefficient for the gas sound velocity.
User entry	Positive floating-point number

Pressure compensation

Navigation	 Guidance → Commissioning → Pressure compen.
Description	Select the pressure compensation type.
Selection	■ Off ■ Fixed value

Pressure value

Navigation	 Guidance → Commissioning → Pressure value
Prerequisite	In the Pressure compensation parameter in the External compensation submenu, the Fixed value option is selected.
Description	Enter fixed value for the pressure compensation. Additional information: The applicable unit of measure is specified in the "System units" submenu.
User entry	Positive floating-point number

2.1.3 System units

Navigation  Guidance → Commissioning

Mass flow unit

Navigation	 Guidance → Commissioning → Mass flow unit	
Description	Select mass flow unit.	
Selection	<i>SI units</i> ■ g/s ■ g/min ■ g/h ■ g/d ■ kg/s ■ kg/min ■ kg/h ■ kg/d ■ t/s ■ t/min ■ t/h ■ t/d	<i>US units</i> ■ oz/s ■ oz/min ■ oz/h ■ oz/d ■ lb/s ■ lb/min ■ lb/h ■ lb/d ■ STon/s ■ STon/min ■ STon/h ■ STon/d

Mass unit

Navigation	  Guidance → Commissioning → Mass unit		
Description	Select mass unit.		
Selection	<i>SI units</i>		<i>US units</i>
	■ g		■ oz
	■ kg		■ lb
	■ t		■ STon

Volume flow unit

Navigation	  Guidance → Commissioning → Volume flow unit		
Description	Select volume flow unit.		

Selection	<i>SI units</i>	<i>US units</i>	<i>Imperial units</i>
	■ cm ³ /s	■ af/s	■ gal/s (imp)
	■ cm ³ /min	■ af/min	■ gal/min (imp)
	■ cm ³ /h	■ af/h	■ gal/h (imp)
	■ cm ³ /d	■ af/d	■ gal/d (imp)
	■ dm ³ /s	■ ft ³ /s	■ Mgal/s (imp)
	■ dm ³ /min	■ ft ³ /min	■ Mgal/min (imp)
	■ dm ³ /h	■ ft ³ /h	■ Mgal/h (imp)
	■ dm ³ /d	■ ft ³ /d	■ Mgal/d (imp)
	■ m ³ /s	■ MMft ³ /s	■ bbl/s (imp;beer)
	■ m ³ /min	■ MMft ³ /min	■ bbl/min (imp;beer)
	■ m ³ /h	■ MMft ³ /h	■ bbl/h (imp;beer)
	■ m ³ /d	■ Mft ³ /d	■ bbl/d (imp;beer)
	■ ml/s	■ fl oz/s (us)	■ bbl/s (imp;oil)
	■ ml/min	■ fl oz/min (us)	■ bbl/min (imp;oil)
	■ ml/h	■ fl oz/h (us)	■ bbl/h (imp;oil)
	■ ml/d	■ fl oz/d (us)	■ bbl/d (imp;oil)
	■ l/s	■ gal/s (us)	
	■ l/min	■ gal/min (us)	
	■ l/h	■ gal/h (us)	
	■ l/d	■ gal/d (us)	
	■ hl/s	■ Mgal/s (us)	
	■ hl/min	■ Mgal/min (us)	
	■ hl/h	■ Mgal/h (us)	
	■ hl/d	■ Mgal/d (us)	
	■ Ml/s	■ bbl/s (us;liq.)	
	■ Ml/min	■ bbl/min (us;liq.)	
	■ Ml/h	■ bbl/h (us;liq.)	
	■ Ml/d	■ bbl/d (us;liq.)	
		■ bbl/s (us;beer)	
		■ bbl/min (us;beer)	
		■ bbl/h (us;beer)	
		■ bbl/d (us;beer)	
		■ bbl/s (us;oil)	
		■ bbl/min (us;oil)	
		■ bbl/h (us;oil)	
		■ bbl/d (us;oil)	
		■ bbl/s (us;tank)	
		■ bbl/min (us;tank)	
		■ bbl/h (us;tank)	
		■ bbl/d (us;tank)	
		■ kgal/s (us)	
		■ kgal/min (us)	
		■ kgal/h (us)	
		■ kgal/d (us)	

Volume unit
**Navigation**

Guidance → Commissioning → Volume unit

Description

Select volume unit.

Selection	<i>SI units</i>	<i>US units</i>	<i>Imperial units</i>
	■ cm ³	■ af	■ gal (imp)
	■ dm ³	■ ft ³	■ Mgal (imp)
	■ m ³	■ Mft ³	■ bbl (imp;beer)
	■ ml	■ fl oz (us)	■ bbl (imp;oil)
	■ l	■ gal (us)	
	■ hl	■ kgal (us)	
	■ Ml Mega	■ Mgal (us)	
		■ bbl (us;oil)	
		■ bbl (us;liq.)	
		■ bbl (us;beer)	
		■ bbl (us;tank)	

Corrected volume flow unit



Navigation Guidance → Commissioning → Cor.volflow unit

Description Select corrected volume flow unit.

Selection	<i>SI units</i>	<i>US units</i>	<i>Imperial units</i>
	■ Nl/s	■ Sft ³ /s	■ Sgal/s (imp)
	■ Nl/min	■ Sft ³ /min	■ Sgal/min (imp)
	■ Nl/h	■ Sft ³ /h	■ Sgal/h (imp)
	■ Nl/d	■ Sft ³ /d	■ Sgal/d (imp)
	■ Nhl/s	■ Sgal/s (us)	
	■ Nhl/min	■ Sgal/min (us)	
	■ Nhl/h	■ Sgal/h (us)	
	■ Nhl/d	■ Sgal/d (us)	
	■ Nm ³ /s	■ Sbbl/s (us;liq.)	
	■ Nm ³ /min	■ Sbbl/min (us;liq.)	
	■ Nm ³ /h	■ Sbbl/h (us;liq.)	
	■ Nm ³ /d	■ Sbbl/d (us;liq.)	
	■ Sl/s	■ MMSft ³ /s	
	■ Sl/min	■ MMSft ³ /min	
	■ Sl/h	■ MMSft ³ /h	
	■ Sl/d	■ MMSft ³ /d	
	■ Sm ³ /s	■ Sbbl/s (us;oil)	
	■ Sm ³ /min	■ Sbbl/min (us;oil)	
	■ Sm ³ /h	■ Sbbl/h (us;oil)	
	■ Sm ³ /d	■ Sbbl/d (us;oil)	

Corrected volume unit



Navigation Guidance → Commissioning → Corr. vol. unit

Description Select corrected volume unit.

Selection	<i>SI units</i>	<i>US units</i>	<i>Imperial units</i>
	■ NI ■ Nhl ■ Nm³ ■ SI ■ Sm³	■ Sft³ ■ MMSft³ ■ Sgal (us) ■ Sbbl (us;liq.) ■ Sbbl (us;oil)	Sgal (imp)

Density unit



Navigation Guidance → Commissioning → Density unit

Description Select density unit.

Selection	<i>SI units</i>	<i>US units</i>	<i>Imperial units</i>
	■ g/cm³ ■ g/m³ ■ g/ml ■ kg/l ■ kg/dm³ ■ kg/m³	■ lb/ft³ ■ lb/gal (us) ■ lb/bbl (us;liq.) ■ lb/bbl (us;beer) ■ lb/bbl (us;oil) ■ lb/bbl (us;tank)	■ lb/gal (imp) ■ lb/bbl (imp;beer) ■ lb/bbl (imp;oil)
	<i>Other units</i> °API		

Reference density unit



Navigation Guidance → Commissioning → Ref. dens. unit

Description Select reference density unit.

Selection	<i>SI units</i>	<i>US units</i>
	■ kg/Nm³ ■ kg/NI ■ g/Scm³ ■ kg/Sm³ ■ RD15°C ■ RD20°C	■ lb/Sft³ ■ RD60°F

Temperature unit



Navigation Guidance → Commissioning → Temperature unit

Description Select temperature unit.

Selection	<i>SI units</i>	<i>US units</i>
	■ °C ■ K	■ °F ■ °R

Pressure unit

Navigation	  Guidance → Commissioning → Pressure unit	
Description	Select pressure unit.	
Selection	<i>SI units</i>	<i>US units</i>
	■ MPa a ■ MPa g ■ kPa a ■ kPa g ■ Pa a ■ Pa g ■ bar ■ bar g	■ psi a ■ psi g

2.1.4 Totalizer 1 to n

Navigation

  Guidance → Commissioning

Assign process variable

Navigation	  Guidance → Commissioning → Assign variable	
Description	Select process variable for totalizer. Additional information: If the option selected is changed, the device resets the totalizer to "0".	
Selection	■ Off ■ Mass flow ■ Volume flow ■ Corrected volume flow	

Unit totalizer 1 to n

Navigation	  Guidance → Commissioning → Unit totalizer 1 to n	
Prerequisite	A process variable has been selected in the Assign process variable parameter in the Totalizer 1 to n submenu.	
Description	Select process variable totalizer unit.	

Selection

SI units

- g^{*}
- kg^{*}
- t^{*}

US units

- oz^{*}
- lb^{*}
- STon^{*}

* Visibility depends on order options or device settings

or

SI units

- cm³^{*}
- dm³^{*}
- m³^{*}
- ml^{*}
- l^{*}
- hl^{*}
- Ml Mega^{*}

US units

- af^{*}
- ft³^{*}
- Mft³^{*}
- fl oz (us)^{*}
- gal (us)^{*}
- kgal (us)^{*}
- Mgal (us)^{*}
- bbl (us;liq.)^{*}
- bbl (us;beer)^{*}
- bbl (us;oil)^{*}
- bbl (us;tank)^{*}

Imperial units

- gal (imp)^{*}
- Mgal (imp)^{*}
- bbl (imp;beer)^{*}
- bbl (imp;oil)^{*}

* Visibility depends on order options or device settings

or

SI units

- Nl^{*}
- Nhl^{*}
- Nm³^{*}
- Sl^{*}
- Sm³^{*}

US units

- Sft³^{*}
- MMSft³^{*}
- Sgal (us)^{*}
- Sbbl (us;liq.)^{*}
- Sbbl (us;oil)^{*}

Imperial units

- Sgal (imp)^{*}

* Visibility depends on order options or device settings

or

Other units

- None^{*}

* Visibility depends on order options or device settings

Additional information

Description

The unit is selected separately for each totalizer. The unit is independent of the option selected in the **System units** submenu (→  57).

Selection

The selection is dependent on the process variable selected in the **Assign process variable** parameter (→  16).

Totalizer operation mode 	
Navigation	  Guidance → Commissioning → Operation mode
Prerequisite	A process variable has been selected in the Assign process variable parameter in the Totalizer 1 to n submenu.
Description	Select totalizer calculation mode.
Selection	▪ Net flow total ▪ Forward flow total ▪ Reverse flow total
Additional information	<i>Selection</i> ▪ Net flow total option The flow values in the forward and reverse flow directions are totalized and netted against each other. Net flow is recorded in the flow direction. ▪ Forward flow total option Only the flow in the forward flow direction is totalized. ▪ Reverse flow total option Only the flow in the reverse flow direction is totalized (= reverse flow quantity).
Failure mode 	
Navigation	  Guidance → Commissioning → Failure mode
Prerequisite	A process variable has been selected in the Assign process variable parameter in the Totalizer 1 to n submenu.
Description	Specify how the totalizer should behave in the event of a device alarm. Additional information: The failsafe mode that applies to any other totalizers or outputs is specified separately in other parameters and is not impacted by this setting.
Selection	▪ Stop ▪ Actual value ▪ Last valid value
Additional information	<i>Selection</i> ▪ Stop option The totalizer is stopped in the event of a device alarm. ▪ Actual value option The totalizer continues to totalize based on the current value measured; the device alarm is ignored. ▪ Last valid value option The totalizer continues to totalize based on the last valid value measured before the device alarm occurred.

2.1.5 Process parameters

Navigation  Guidance → Commissioning

Flow damping time

Navigation	 Guidance → Commissioning → FlowDampingTime
Description	Enter time constant for flow damping (PT1 element). - Value = 0: No damping - Value > 0: Damping increases Additional information: Damping is implemented by means of a proportional transmission behavior with first order delay (PT1 element).
User entry	0 to 99.9 s


2.1.6 Measuring conditions

Pressure shock suppression

Navigation  Guidance → Commissioning

Pressure shock suppression

Navigation	 Guidance → Commissioning → Pres. shock sup.
Description	Enter time frame for signal suppression (= pressure shock suppression active), for example to prevent the device from registering flow movements in the pipe when a valve is closed. Additional information: Pressure shock suppression is activated when the flow rate drops below the on value for low flow cutoff. Output values when pressure shock suppression is active: - Flow: 0 - Totalizer: Last valid value Pressure shock suppression is deactivated when: - The time frame specified has elapsed and - Flow exceeds the off value for low flow cutoff
User entry	0 to 100 s
Additional information	<i>Example</i> When a valve is closed, momentarily strong fluid movements may occur in the pipeline, which are registered by the device. These totalized flow values lead to a false totalizer status, particularly during batching processes.

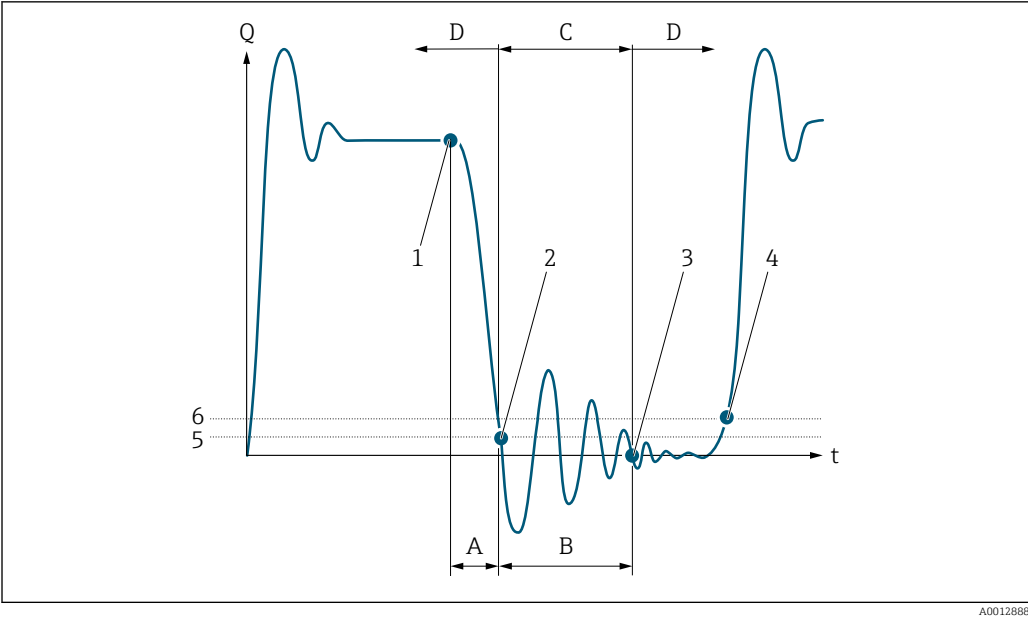

- Q Flow
t Time
A After run
B Pressure shock
C Pressure shock suppression active as specified by the time entered
D Pressure shock suppression inactive
1 Valve closes
2 Flow falls below the on-value of the low flow cut off; pressure shock suppression is activated
3 The time entered has elapsed; pressure shock suppression is deactivated
4 The actual flow value is now displayed and output
5 On-value for low flow cut off
6 Off-value for low flow cut off

Low flow cut off

Navigation  Guidance → Commissioning


Low flow cut off

Navigation  Guidance → Commissioning → Low flow cut off

Description Select process variable for low flow cut off to activate low flow cut off.

- Selection
- Off
 - Mass flow
 - Volume flow
 - Corrected volume flow

Additional information Description

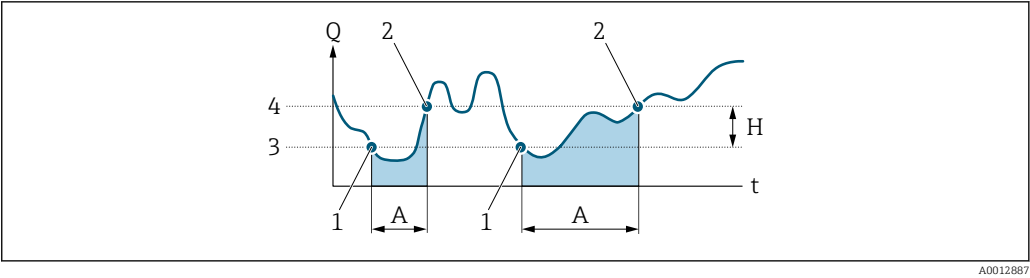

- Q* Flow
- t* Time
- H* Hysteresis
- A* Low flow cut off active
- 1* Low flow cut off is activated
- 2* Low flow cut off is deactivated
- 3* On-value entered
- 4* Off-value entered

On value low flow cutoff

Navigation  Guidance → Commissioning → On value

Description Enter on value to switch on low flow cut off.
Value = 0: No low flow cut off
Value > 0: Low flow cut off is activated

User entry Positive floating-point number

Off value low flow cutoff

Navigation  Guidance → Commissioning → Off value

Description Enter off value to switch off low flow cut off. The off value is entered as a positive hysteresis with respect to the on value.

User entry 0 to 100.0 %

Partially filled pipe detection

Navigation  Guidance → Commissioning

Partially filled pipe detection

Navigation	 Guidance → Commissioning → Partial pipe det
Description	Select process variable for detection of an empty or partially filled pipe. NOTE Due to low density, deactivate partially filled pipe detection for a gas!
Selection	■ Off ■ Density ■ Calculated reference density

Low value partial filled pipe detection

Navigation	 Guidance → Commissioning → Low value
Prerequisite	A process variable has been selected in the Assign process variable parameter in the Empty pipe detection submenu.
Description	Enter the lower limit value for the selected process variable. If the measured value drops below the limit value, diagnostic message "862 Partly filled pipe" is generated. Additional information: - This setting applies only if the "Density unit" parameter is not set to °API. - The lower limit value must be lower than the upper limit value ("High value partial filled pipe detection" parameter).
User entry	Signed floating-point number

High value partial filled pipe detection

Navigation	 Guidance → Commissioning → High value
Prerequisite	A process variable has been selected in the Assign process variable parameter in the Empty pipe detection submenu.
Description	Enter the upper limit value for the selected process variable. If the measured value exceeds the limit value, diagnostic message "862 Partly filled pipe" is generated. Additional information: This setting applies only if the "Density unit" parameter is set to °API.

User entry Signed floating-point number

2.1.7 Current output

Navigation   Guidance → Commissioning

Process variable current output

Navigation   Guidance → Commissioning → Proc.var. outp

Description Select process variable for current output

Selection

- Off *
- Mass flow
- Volume flow
- Corrected volume flow
- Temperature
- Density *
- Index inhomogeneous medium
- Exciter current 0
- Oscillation frequency 0
- Oscillation amplitude 0 *
- Frequency fluctuation 0 *
- Oscillation damping 0
- Oscillation damping fluctuation 0 *
- Signal asymmetry
- HBSI *
- Electronics temperature

Current range output

Navigation   Guidance → Commissioning → Curr.range out

Description Select the current range for the measured value output and the upper and lower fault condition signal level.

Additional information:

- The measured value range is specified in the "Lower range value output" parameter and the "Upper range value output" parameter.
- If the measured value lies outside the scaled measured value range, diagnostic message "441 Current output faulty" is generated.
- In the event of a device alarm, the current output adopts the behavior specified in the "Failure behavior current output" parameter.

* Visibility depends on order options or device settings

- Selection
- 4...20 mA NE (3.8...20.5 mA)

■ 4...20 mA US (3.9...20.8 mA)

■ 4...20 mA (4... 20.5 mA)

■ Fixed value

Additional information

Selection

■ 4...20 mA NE (3.8...20.5 mA) option


Select this option to set the current range in accordance with NAMUR recommendation NE43.

■ Fixed value option

Select this option to set the current output to a current value instead of a range.

The current value is defined in the **Fixed current** parameter (→ ⓘ 26).

The graphic shows the relationship between the current range for the output of the process value and the lower and upper alarm levels:

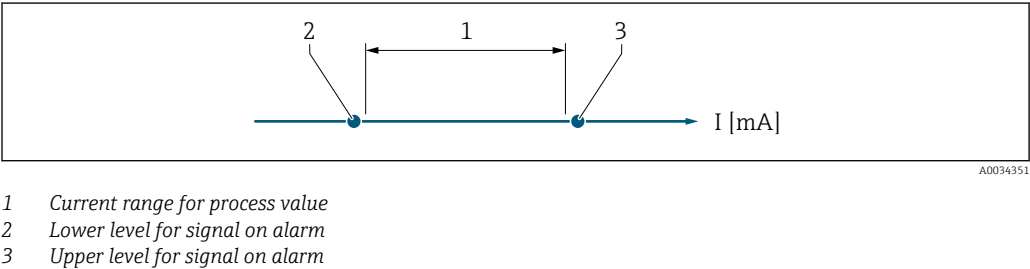

Selection (current range for process value)	Lower level for signal on alarm	Upper level for signal on alarm
4...20 mA NE (3.8...20.5 mA)	< 3.6 mA	> 21.5 mA
4...20 mA US (3.9...20.8 mA)		
4...20 mA (4... 20.5 mA)		

Lower range value output

ⓘ

Navigation

ⓘ ⓘ Guidance → Commissioning → Low.range outp

Prerequisite

In the **Current range output** parameter, one of the following options is selected:

■ 4...20 mA NE (3.8...20.5 mA)

■ 4...20 mA US (3.9...20.8 mA)

■ 4...20 mA (4... 20.5 mA)

Description

Enter lower range value for the measured value range.

Additional information:

- Depending on the setting selected for the "Measuring mode current output " parameter, the value specified for this parameter and the "Upper range value output " parameter must have the same algebraic sign or not.

- As a rule, the lower range value is scaled to be lower than the upper range value. As a result, the behavior of the current output is proportional to the process variable assigned. If the lower range value is scaled to be higher than the upper range value, then the behavior of the current output will be inversely proportional to the process variable assignend.

User entry


Signed floating-point number

Additional information

Examples of the behavior, depending on the option selected in the **Measuring mode current output** parameter (→  88).

Example: Measuring mode with "Forward flow" option

- **Lower range value output** parameter (→  24) = not equal to zero flow (e.g. -250 m³/h)
- **Upper range value output** parameter (→  26) = not equal to zero flow (e.g. +750 m³/h)
- Calculated current value = 8 mA at zero flow

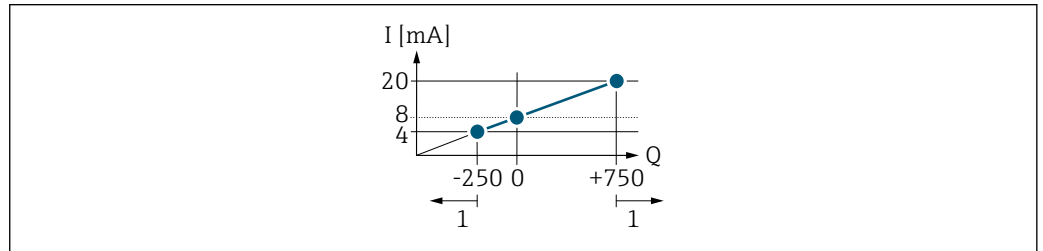


A0013757

Q Flow
I Current
1 Measuring range is exceeded or undershot

The linear operational range of the measuring device is defined by the values entered for the **Lower range value output** parameter (→  24) and **Upper range value output** parameter (→  26), and by the selected current range.

Example: Measuring mode with the "Forward/Reverse flow" option

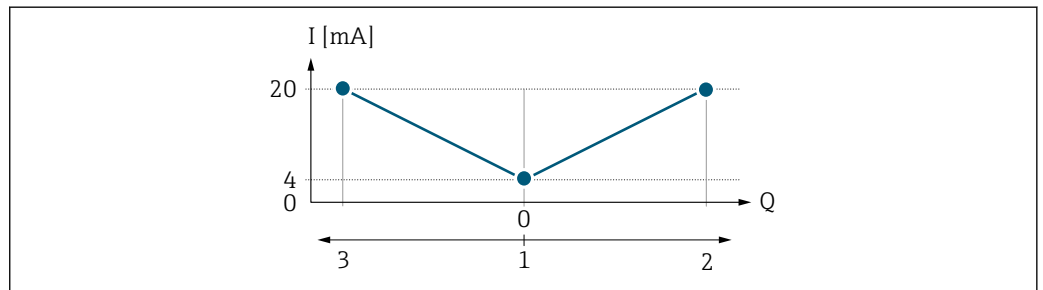

A0013758

Q Flow
I Current
1 Value assigned to 0/4 mA current
2 Forward flow
3 Reverse flow

The current output signal is independent of the direction of flow (absolute amount of the measured variable). The values for the **Lower range value output** parameter (→  24) and **Upper range value output** parameter (→  26) must have the same algebraic sign.

The value for the **Upper range value output** parameter (→  26) (e.g. reverse flow) corresponds to the mirrored value for the **Upper range value output** parameter (→  26) (e.g. forward flow).

Example: Measuring mode with the "Reverse flow compensation" option

If flow is characterized by severe fluctuations (e.g. when using reciprocating pumps), flow components outside the measuring range are buffered, balanced and output after a maximum delay of 60 s.

Upper range value output 	
Navigation	 Guidance → Commissioning → Upp.range outp
Prerequisite	In the Current range output parameter, one of the following options is selected: ■ 4...20 mA NE (3.8...20.5 mA) ■ 4...20 mA US (3.9...20.8 mA) ■ 4...20 mA (4... 20.5 mA)
Description	Enter upper range value for the measured value range.
User entry	Signed floating-point number
Additional information	 Examples of the behavior, depending on the option selected in the Measuring mode current output parameter: Lower range value output parameter (→  24):

Damping current output 	
Navigation	 Guidance → Commissioning → Damp.curr.outp
Prerequisite	A process variable is selected in the Process variable current output parameter and one of the following options is selected in the Current range output parameter: ■ 4...20 mA NE (3.8...20.5 mA) ■ 4...20 mA US (3.9...20.8 mA) ■ 4...20 mA (4... 20.5 mA)
Description	Enter time constant (PT1 element) to set the reaction time of the output signal to fluctuations in the measured value caused by process conditions. Additional information: - The smaller the time constant the faster the output reacts to fluctuations in the measured value. - If the time constant is 0, damping is deactivated.
User entry	0.0 to 999.9 s

Fixed current 	
Navigation	 Guidance → Commissioning → Fixed current
Prerequisite	In the Current range output parameter in the Current output 1 submenu, the Fixed value option is selected.
Description	Enter the value for the "Fixed value" option.
User entry	3.59 to 21.5 mA

Failure behavior current output 	
Navigation	  Guidance → Commissioning → Fail.behav.out
Prerequisite	A process variable is selected in the Process variable current output parameter and one of the following options is selected in the Current range output parameter: ■ 4...20 mA NE (3.8...20.5 mA) ■ 4...20 mA US (3.9...20.8 mA) ■ 4...20 mA (4... 20.5 mA)
Description	Specify how the output should behave in the event of a device alarm.
Selection	■ Min. ■ Max. ■ Last valid value ■ Actual value ■ Fixed value
Additional information	<i>Selection</i> ■ Min. option The current output outputs the lower fault condition signal level for the specified current range. Additional information: The current range is specified in the "Current range output" parameter. ■ Max. option The current output outputs the upper fault condition signal level for the specified current range. Additional information: The current range is specified in the "Current range output" parameter. ■ Last valid value option The current output outputs the last valid value measured before the device alarm occurred. ■ Actual value option The current output outputs the flow value currently measured. The device alarm is ignored. ■ Fixed value option The current output outputs the value specified. Additional information: The value is specified in the "Failure current" parameter.
Failure current 	

Navigation	  Guidance → Commissioning → Fail. current
Prerequisite	In the Failure behavior current output parameter in the Current output 1 submenu, the Fixed value option is selected.
Description	Enter the value for the "Fixed value" option in the "Failure behavior current output" parameter.
User entry	3.59 to 21.5 mA

2.1.8 Display

Navigation   Guidance → Commissioning

Value 1 display

Navigation   Guidance → Commissioning → Value 1 display

Description Select the measured value that is displayed first on the local display.
Additional information:
The applicable unit of measure is specified in the "System units" submenu.

Selection

- Mass flow
- Volume flow
- Corrected volume flow
- Temperature
- Density *
- Totalizer 1
- Totalizer 2
- Totalizer 3
- Index inhomogeneous medium
- Electronics temperature

Value 2 display

Navigation   Guidance → Commissioning → Value 2 display

Description Select the measured value that is shown second on the local display.
Additional information:
The applicable unit of measure is specified in the "System units" submenu.

Selection

- None
- Mass flow
- Volume flow
- Corrected volume flow
- Temperature
- Density *
- Totalizer 1
- Totalizer 2
- Totalizer 3
- Index inhomogeneous medium
- Electronics temperature

* Visibility depends on order options or device settings

Value 3 display

**Navigation**

Guidance → Commissioning → Value 3 display

Description

Select the measured value that is shown third on the local display.

Additional information:

The applicable unit of measure is specified in the "System units" submenu.

Selection

- None
- Mass flow
- Volume flow
- Corrected volume flow
- Temperature
- Density^{*}
- Totalizer 1
- Totalizer 2
- Totalizer 3
- Index inhomogeneous medium
- Electronics temperature

Value 4 display

**Navigation**

Guidance → Commissioning → Value 4 display

Description

Select the measured value that is shown fourth on the local display.

Additional information:

The applicable unit of measure is specified in the "System units" submenu.

Selection

- None
- Mass flow
- Volume flow
- Corrected volume flow
- Temperature
- Density^{*}
- Totalizer 1
- Totalizer 2
- Totalizer 3
- Index inhomogeneous medium
- Electronics temperature

^{*} Visibility depends on order options or device settings

Display damping

Navigation	  Guidance → Commissioning → Display damping
Description	Enter time constant (PT1 element) to set reaction time of the display to fluctuations in the measured value. Additional information: - The smaller the time constant the faster the display reacts to fluctuations in the measured value. - If the time constant is set to 0, damping is deactivated.
User entry	0.0 to 999.9 s

2.1.9 Date/time

Navigation

  Guidance → Commissioning

Time format

Navigation	  Guidance → Commissioning → Time format
Description	Select time format.
Selection	■ 24 h ■ 12 h AM/PM

Time zone

Navigation	  Guidance → Commissioning → Time zone
Description	Select the time zone. Every time the time zone is changed, a logbook entry is created.

Selection

Other units

- UTC-12:00
- UTC-11:00
- UTC-10:00
- UTC-09:30
- UTC-09:00
- UTC-08:00
- UTC-07:00
- UTC-06:00
- UTC-05:00
- UTC-04:00
- UTC-03:30
- UTC-03:00
- UTC-02:00
- UTC-01:00
- UTC 00:00
- UTC+01:00
- UTC+02:00
- UTC+03:00
- UTC+03:30
- UTC+04:00
- UTC+04:30
- UTC+05:00
- UTC+05:30
- UTC+05:45
- UTC+06:00
- UTC+06:30
- UTC+07:00
- UTC+08:00
- UTC+08:45
- UTC+09:00
- UTC+09:30
- UTC+10:00
- UTC+10:30
- UTC+11:00
- UTC+12:00
- UTC+12:45
- UTC+13:00
- UTC+14:00

Set date/time



Navigation



Guidance → Commissioning → Set date/time

Description

Set the date and local time. Every time the date or time is changed, a logbook entry is created.

User entry

Date and time

3 "Diagnostics" menu

Troubleshooting and preventive maintenance – settings for device behavior during process and device events as well as assistance and measures for diagnostic purposes.

Navigation  Diagnostics

Diagnostics		
▶ Active diagnostics	→ 	33
▶ Diagnostic list	→ 	35
▶ Simulation	→ 	38
▶ Heartbeat Technology	→ 	41
▶ Diagnostic settings	→ 	42

3.1 "Actual diagnostics" submenu

Navigation   Diagnostics → Active diagnos.

► Active diagnostics		
Actual diagnostics	→ 	33
Timestamp	→ 	33
Previous diagnostics	→ 	33
Timestamp	→ 	34
Operating time from restart	→ 	34
Operating time	→ 	34

Actual diagnostics

Navigation	  Diagnostics → Active diagnos. → Actual diagnos.
Prerequisite	A diagnostic event has occurred.
Description	Displays the currently active diagnostic message. If there is more than one pending diagnostic event, the message for the diagnostic event with the highest priority is displayed.
User interface	Positive integer

Timestamp

Navigation	  Diagnostics → Active diagnos. → Timestamp
Description	Displays the timestamp for the currently active diagnostic message.
User interface	Days (d), hours (h), minutes (m), seconds (s)

Previous diagnostics

Navigation	  Diagnostics → Active diagnos. → Prev.diagnostics
Prerequisite	At least two diagnostic events have already occurred.

Description Displays the diagnostic message for the last diagnostic event that has ended.

User interface Positive integer

Timestamp

Navigation   Diagnostics → Active diagnos. → Timestamp

Description Displays the timestamp of the diagnostic message generated for the last diagnostic event that has ended.

User interface Days (d), hours (h), minutes (m), seconds (s)

Operating time from restart

Navigation   Diagnostics → Active diagnos. → Time fr. restart

Description Indicates how long the device has been in operation since the last time the device was restarted.

User interface Days (d), hours (h), minutes (m), seconds (s)

Operating time

Navigation   Diagnostics → Active diagnos. → Operating time

Description Indicates how long the device has been in operation.

User interface Days (d), hours (h), minutes (m), seconds (s)

3.2 "Diagnostic list" submenu

Navigation  Diagnostics → Diagnostic list

► Diagnostic list		
Diagnostics 1	→ 	35
Timestamp	→ 	35
Diagnostics 2	→ 	36
Timestamp	→ 	36
Diagnostics 3	→ 	36
Timestamp	→ 	36
Diagnostics 4	→ 	36
Timestamp	→ 	37
Diagnostics 5	→ 	37
Timestamp	→ 	37

Diagnostics 1

Navigation	 Diagnostics → Diagnostic list → Diagnostics 1
Description	Displays the currently active diagnostic message with the highest priority.
User interface	Positive integer

Timestamp

Navigation	 Diagnostics → Diagnostic list → Timestamp
Description	Displays the timestamp for the diagnostic message with the highest priority.
User interface	Days (d), hours (h), minutes (m), seconds (s)

Diagnostics 2

Navigation	 Diagnostics → Diagnostic list → Diagnostics 2
Description	Displays the currently active diagnostic message with the second highest priority.
User interface	Positive integer

Timestamp

Navigation	 Diagnostics → Diagnostic list → Timestamp
Description	Displays the timestamp for the diagnostic message with the second highest priority.
User interface	Days (d), hours (h), minutes (m), seconds (s)

Diagnostics 3

Navigation	 Diagnostics → Diagnostic list → Diagnostics 3
Description	Displays the currently active diagnostic message with the third highest priority.
User interface	Positive integer

Timestamp

Navigation	 Diagnostics → Diagnostic list → Timestamp
Description	Displays the timestamp for the diagnostic message with the third highest priority.
User interface	Days (d), hours (h), minutes (m), seconds (s)

Diagnostics 4

Navigation	 Diagnostics → Diagnostic list → Diagnostics 4
Description	Displays the currently active diagnostic message with the fourth highest priority.
User interface	Positive integer

Timestamp

Navigation	 Diagnostics → Diagnostic list → Timestamp
Description	Displays the timestamp for the diagnostic message with the fourth highest priority.
User interface	Days (d), hours (h), minutes (m), seconds (s)

Diagnostics 5

Navigation	 Diagnostics → Diagnostic list → Diagnostics 5
Description	Displays the currently active diagnostic message with the fifth-highest priority.
User interface	Positive integer

Timestamp

Navigation	 Diagnostics → Diagnostic list → Timestamp
Description	Displays the timestamp for the diagnostic message with the fifth highest priority.
User interface	Days (d), hours (h), minutes (m), seconds (s)

3.3 "Simulation" submenu

Navigation  Diagnostics → Simulation

► Simulation		
Assign simulation process variable	→ 	38
Process variable value	→ 	39
Current output 1 simulation	→ 	39
Current output value	→ 	39
Device alarm simulation	→ 	40
Diagnostic event category	→ 	40
Diagnostic event simulation	→ 	40

Assign simulation process variable



Navigation  Diagnostics → Simulation → Assign proc.var.

Description Select a process variable for the simulation, thereby activating it.

- Selection
- Off
 - Mass flow
 - Volume flow
 - Corrected volume flow
 - Density^{*}
 - Temperature

Additional information *Description*

The display alternates between the measured value and a diagnostics message of the "function check" category (C) when simulation is active.

^{*} Visibility depends on order options or device settings

Process variable value 	
Navigation	  Diagnostics → Simulation → Proc. var. value
Description	Enter the simulation value for the selected process variable. Processing of measured values downstream as well as the signal output follow this value. In this way, it is possible to verify whether the measuring device has been configured correctly. Additional information: The applicable unit of measure is specified in the "System units" submenu.
User entry	Signed floating-point number
Current output 1 simulation 	
Navigation	  Diagnostics → Simulation → Curr.outp 1 sim.
Description	Switch simulation of the current output on or off. Additional information: When simulation is on, the current output signal is set to the value specified in the "Current output value" parameter.
Selection	■ Off ■ On
Additional information	<i>Description</i> The display alternates between the measured value and a diagnostics message of the "function check" category (C) when simulation is active.
Current output value 	
Navigation	  Diagnostics → Simulation → Curr.outp val.
Description	Enter the current value for the simulation. In this manner, it is possible to verify the current output is configured correctly and downstream processing units are functioning properly. Additional information: The valid input range is determined by the "Current range output" parameter.
User entry	3.59 to 21.5 mA

Device alarm simulation

Navigation	  Diagnostics → Simulation → Dev. alarm sim.
Description	Switch the device alarm simulation on or off. While simulation is in progress, the display alternates between the measured value and a diagnostic message of the Function Check (C) category.
Selection	■ Off ■ On

Diagnostic event category

Navigation	 Diagnostics → Simulation → Event category
Description	Select the category of diagnostic events that should be available for selection in the "Diagnostic event simulation" parameter.
Selection	■ Sensor ■ Electronics ■ Configuration ■ Process

Diagnostic event simulation

Navigation	  Diagnostics → Simulation → Diag. event sim.
Description	Select the diagnostic event to simulate.
Selection	Off

3.4 "Heartbeat Technology" submenu

The **Heartbeat Technology** submenu (→  41) is only available with the optional "Heartbeat Verification + Monitoring" application package.

- Order code for: Application package
- Option: EB "Heartbeat Verification + Monitoring"

 Detailed information and all descriptions of the device parameters of the application package are available in the "Heartbeat Verification + Monitoring" Special Documentation

Navigation   Diagnostics → HBT

▶ Heartbeat Technology

3.5 "Diagnostic settings" submenu

Navigation   Diagnostics → Diag. settings

► Diagnostic settings

► Properties

→  42

► Diagnostic configuration

→  42

3.5.1 "Properties" submenu

Navigation   Diagnostics → Diag. settings → Properties

► Properties

Alarm delay

→  42

Alarm delay	
-------------	---

Navigation   Diagnostics → Diag. settings → Properties → Alarm delay

Description Enter a duration for the alarm delay. When a diagnostic event of the "Alarm" category occurs, the diagnostic message is not generated until the delay has elapsed.

User entry 0 to 60 s

3.5.2 "Diagnostic configuration" submenu

Navigation   Diagnostics → Diag. settings → Diag. config.

► Diagnostic configuration

► Sensor

→  43

► Electronics

→  44

► Configuration

→  46

► Process

→  47

"Sensor" submenu

Navigation   Diagnostics → Diag. settings → Diag. config. → Sensor

► Sensor

Assign behavior of diagnostic no. 046

→  43

Assign behavior of diagnostic no. 140

→  43

Assign behavior of diagnostic no. 144

→  44

Assign behavior of diagnostic no. 046

Navigation	  Diagnostics → Diag. settings → Diag. config. → Sensor → Diagnostic no. 046
Description	Select behavior for diagnostic event "046 Sensor limit exceeded".
Selection	■ Off ■ Alarm ■ Warning ■ Logbook entry only
Additional information	<i>Selection</i> ■ Off option The diagnostic event is ignored and no diagnostic message is generated or logged. ■ Alarm option The device stops measuring. The signal outputs and totalizers assume the specified alarm condition. A diagnostic message is generated. ■ Warning option The device continues measuring. The signal outputs and totalizers are not affected. A diagnostic message is generated. ■ Logbook entry only option The device continues measuring. The diagnostic message is only displayed in the "Event logbook" submenu and does not alternate with the standard operational information displayed.

Assign behavior of diagnostic no. 140

Navigation	  Diagnostics → Diag. settings → Diag. config. → Sensor → Diagnostic no. 140
Description	Select behavior for diagnostic event "140 Sensor signal asymmetrical".
Selection	■ Off ■ Alarm ■ Warning ■ Logbook entry only

Additional information

Selection

- **Off** option
The diagnostic event is ignored and no diagnostic message is generated or logged.
- **Alarm** option
The device stops measuring. The signal outputs and totalizers assume the specified alarm condition. A diagnostic message is generated.
- **Warning** option
The device continues measuring. The signal outputs and totalizers are not affected. A diagnostic message is generated.
- **Logbook entry only** option
The device continues measuring. The diagnostic message is only displayed in the "Event logbook" submenu and does not alternate with the standard operational information displayed.

Assign behavior of diagnostic no. 144



Navigation

 Diagnostics → Diag. settings → Diag. config. → Sensor → Diagnostic no. 144

Description

Select diagnostic behavior for the selected diagnostic number.

Selection

- Off
- Alarm
- Warning
- Logbook entry only

Additional information

Selection

- **Off** option
The diagnostic event is ignored and no diagnostic message is generated or logged.
- **Alarm** option
The device stops measuring. The signal outputs and totalizers assume the specified alarm condition. A diagnostic message is generated.
- **Warning** option
The device continues measuring. The signal outputs and totalizers are not affected. A diagnostic message is generated.
- **Logbook entry only** option
The device continues measuring. The diagnostic message is only displayed in the "Event logbook" submenu and does not alternate with the standard operational information displayed.

"Electronics" submenu

Navigation

 Diagnostics → Diag. settings → Diag. config. → Electronics

► Electronics

Assign behavior of diagnostic no. 230 →  45

Assign behavior of diagnostic no. 231 →  45

Assign behavior of diagnostic no. 302	→ 45
Assign behavior of diagnostic no. 374	→ 45

Assign behavior of diagnostic no. 230



Navigation	Diagnostics → Diag. settings → Diag. config. → Electronics → Diagnostic no. 230
Description	Select behavior for diagnostic event "230 Date/time incorrect".
Selection	■ Alarm ■ Warning ■ Logbook entry only

Assign behavior of diagnostic no. 231



Navigation	Diagnostics → Diag. settings → Diag. config. → Electronics → Diagnostic no. 231
Description	Select behavior for diagnostic event "231 Date/time not available".
Selection	■ Alarm ■ Warning ■ Logbook entry only

Assign behavior of diagnostic no. 302



Navigation	Diagnostics → Diag. settings → Diag. config. → Electronics → Diagnostic no. 302
Description	Select behavior for diagnostic event "302 Device verification active".
Selection	■ Off ■ Warning ■ Logbook entry only

Assign behavior of diagnostic no. 374



Navigation	Diagnostics → Diag. settings → Diag. config. → Electronics → Diagnostic no. 374
Description	Select behavior for diagnostic event "374 Sensor electronics (ISEM) faulty".

- Selection**
- Off
 - Alarm
 - Warning
 - Logbook entry only

Additional information

Selection

- **Off** option
The diagnostic event is ignored and no diagnostic message is generated or logged.
- **Alarm** option
The device stops measuring. The signal outputs and totalizers assume the specified alarm condition. A diagnostic message is generated.
- **Warning** option
The device continues measuring. The signal outputs and totalizers are not affected. A diagnostic message is generated.
- **Logbook entry only** option
The device continues measuring. The diagnostic message is only displayed in the "Event logbook" submenu and does not alternate with the standard operational information displayed.

"Configuration" submenu

Navigation   Diagnostics → Diag. settings → Diag. config. → Configuration

► Configuration

Assign behavior of diagnostic no. 441

→  46

Assign behavior of diagnostic no. 441



- Navigation**   Diagnostics → Diag. settings → Diag. config. → Configuration → Diagnostic no. 441
- Description** Select behavior for diagnostic event "441 Current output faulty".
- Selection**
- Off
 - Alarm
 - Warning
 - Logbook entry only

Additional information*Selection*

- **Off** option
The diagnostic event is ignored and no diagnostic message is generated or logged.
- **Alarm** option
The device stops measuring. The signal outputs and totalizers assume the specified alarm condition. A diagnostic message is generated.
- **Warning** option
The device continues measuring. The signal outputs and totalizers are not affected. A diagnostic message is generated.
- **Logbook entry only** option
The device continues measuring. The diagnostic message is only displayed in the "Event logbook" submenu and does not alternate with the standard operational information displayed.

"Process" submenu*Navigation*
 Diagnostics → Diag. settings → Diag. config. → Process

► Process	
Assign behavior of diagnostic no. 832	→  47
Assign behavior of diagnostic no. 833	→  48
Assign behavior of diagnostic no. 834	→  48
Assign behavior of diagnostic no. 835	→  49
Assign behavior of diagnostic no. 842	→  49
Assign behavior of diagnostic no. 862	→  50
Assign behavior of diagnostic no. 912	→  50
Assign behavior of diagnostic no. 913	→  51
Assign behavior of diagnostic no. 944	→  51
Assign behavior of diagnostic no. 948	→  52

Assign behavior of diagnostic no. 832**Navigation**
 Diagnostics → Diag. settings → Diag. config. → Process → Diagnostic no. 832
Description

Select behavior for diagnostic event "832 Electronics temperature too high".

Selection

- Off
- Alarm
- Warning
- Logbook entry only

Additional information

Selection

- **Off** option
The diagnostic event is ignored and no diagnostic message is generated or logged.
- **Alarm** option
The device stops measuring. The signal outputs and totalizers assume the specified alarm condition. A diagnostic message is generated.
- **Warning** option
The device continues measuring. The signal outputs and totalizers are not affected. A diagnostic message is generated.
- **Logbook entry only** option
The device continues measuring. The diagnostic message is only displayed in the "Event logbook" submenu and does not alternate with the standard operational information displayed.

Assign behavior of diagnostic no. 833



Navigation

Diagnostics → Diag. settings → Diag. config. → Process → Diagnostic no. 833

Description

Select behavior for diagnostic event "833 Electronics temperature too low".

Selection

- Off
- Alarm
- Warning
- Logbook entry only

Additional information

Selection

- **Off** option
The diagnostic event is ignored and no diagnostic message is generated or logged.
- **Alarm** option
The device stops measuring. The signal outputs and totalizers assume the specified alarm condition. A diagnostic message is generated.
- **Warning** option
The device continues measuring. The signal outputs and totalizers are not affected. A diagnostic message is generated.
- **Logbook entry only** option
The device continues measuring. The diagnostic message is only displayed in the "Event logbook" submenu and does not alternate with the standard operational information displayed.

Assign behavior of diagnostic no. 834



Navigation

Diagnostics → Diag. settings → Diag. config. → Process → Diagnostic no. 834

Description

Select event category (status signal) for diagnostic event "834 Process temperature too high".

Selection	■ Off ■ Alarm ■ Warning ■ Logbook entry only
Additional information	<i>Selection</i> ■ Off option The diagnostic event is ignored and no diagnostic message is generated or logged. ■ Alarm option The device stops measuring. The signal outputs and totalizers assume the specified alarm condition. A diagnostic message is generated. ■ Warning option The device continues measuring. The signal outputs and totalizers are not affected. A diagnostic message is generated. ■ Logbook entry only option The device continues measuring. The diagnostic message is only displayed in the "Event logbook" submenu and does not alternate with the standard operational information displayed.

Assign behavior of diagnostic no. 835



Navigation	Diagnostics → Diag. settings → Diag. config. → Process → Diagnostic no. 835
Description	Select behavior for diagnostic event "835 Process temperature too low".
Selection	■ Off ■ Alarm ■ Warning ■ Logbook entry only
Additional information	<i>Selection</i> ■ Off option The diagnostic event is ignored and no diagnostic message is generated or logged. ■ Alarm option The device stops measuring. The signal outputs and totalizers assume the specified alarm condition. A diagnostic message is generated. ■ Warning option The device continues measuring. The signal outputs and totalizers are not affected. A diagnostic message is generated. ■ Logbook entry only option The device continues measuring. The diagnostic message is only displayed in the "Event logbook" submenu and does not alternate with the standard operational information displayed.

Assign behavior of diagnostic no. 842



Navigation	Diagnostics → Diag. settings → Diag. config. → Process → Diagnostic no. 842
Description	Select behavior for diagnostic event "842 Process value above limit".

Selection

- Off
- Alarm
- Warning
- Logbook entry only

Additional information

Selection

- **Off** option
The diagnostic event is ignored and no diagnostic message is generated or logged.
- **Alarm** option
The device stops measuring. The signal outputs and totalizers assume the specified alarm condition. A diagnostic message is generated.
- **Warning** option
The device continues measuring. The signal outputs and totalizers are not affected. A diagnostic message is generated.
- **Logbook entry only** option
The device continues measuring. The diagnostic message is only displayed in the "Event logbook" submenu and does not alternate with the standard operational information displayed.

Assign behavior of diagnostic no. 862



Navigation

Diagnostics → Diag. settings → Diag. config. → Process → Diagnostic no. 862

Description

Select behavior for diagnostic event "862 Partly filled pipe".

Selection

- Off
- Alarm
- Warning
- Logbook entry only

Additional information

Selection

- **Off** option
The diagnostic event is ignored and no diagnostic message is generated or logged.
- **Alarm** option
The device stops measuring. The signal outputs and totalizers assume the specified alarm condition. A diagnostic message is generated.
- **Warning** option
The device continues measuring. The signal outputs and totalizers are not affected. A diagnostic message is generated.
- **Logbook entry only** option
The device continues measuring. The diagnostic message is only displayed in the "Event logbook" submenu and does not alternate with the standard operational information displayed.

Assign behavior of diagnostic no. 912



Navigation

Diagnostics → Diag. settings → Diag. config. → Process → Diagnostic no. 912

Description

Select behavior for diagnostic event "912 Medium inhomogeneous".

Selection	■ Off ■ Alarm ■ Warning ■ Logbook entry only
Additional information	<i>Selection</i> ■ Off option The diagnostic event is ignored and no diagnostic message is generated or logged. ■ Alarm option The device stops measuring. The signal outputs and totalizers assume the specified alarm condition. A diagnostic message is generated. ■ Warning option The device continues measuring. The signal outputs and totalizers are not affected. A diagnostic message is generated. ■ Logbook entry only option The device continues measuring. The diagnostic message is only displayed in the "Event logbook" submenu and does not alternate with the standard operational information displayed.

Assign behavior of diagnostic no. 913



Navigation	Diagnostics → Diag. settings → Diag. config. → Process → Diagnostic no. 913
Description	Select behavior for diagnostic event "913 Medium unsuitable".
Selection	■ Off ■ Alarm ■ Warning ■ Logbook entry only
Additional information	<i>Selection</i> ■ Off option The diagnostic event is ignored and no diagnostic message is generated or logged. ■ Alarm option The device stops measuring. The signal outputs and totalizers assume the specified alarm condition. A diagnostic message is generated. ■ Warning option The device continues measuring. The signal outputs and totalizers are not affected. A diagnostic message is generated. ■ Logbook entry only option The device continues measuring. The diagnostic message is only displayed in the "Event logbook" submenu and does not alternate with the standard operational information displayed.

Assign behavior of diagnostic no. 944



Navigation	Diagnostics → Diag. settings → Diag. config. → Process → Diagnostic no. 944
Description	Select behavior for diagnostic event "944 Monitoring failed".

Selection

- Off
- Alarm
- Warning
- Logbook entry only

Additional information

Selection

- **Off** option
The diagnostic event is ignored and no diagnostic message is generated or logged.
- **Alarm** option
The device stops measuring. The signal outputs and totalizers assume the specified alarm condition. A diagnostic message is generated.
- **Warning** option
The device continues measuring. The signal outputs and totalizers are not affected. A diagnostic message is generated.
- **Logbook entry only** option
The device continues measuring. The diagnostic message is only displayed in the "Event logbook" submenu and does not alternate with the standard operational information displayed.

Assign behavior of diagnostic no. 948



Navigation

 Diagnostics → Diag. settings → Diag. config. → Process → Diagnostic no. 948

Description

Select behavior for diagnostic event "948 Oscillation damping too high".

Selection

- Off
- Alarm
- Warning
- Logbook entry only

Additional information

Selection

- **Off** option
The diagnostic event is ignored and no diagnostic message is generated or logged.
- **Alarm** option
The device stops measuring. The signal outputs and totalizers assume the specified alarm condition. A diagnostic message is generated.
- **Warning** option
The device continues measuring. The signal outputs and totalizers are not affected. A diagnostic message is generated.
- **Logbook entry only** option
The device continues measuring. The diagnostic message is only displayed in the "Event logbook" submenu and does not alternate with the standard operational information displayed.

4 "Application" menu

Targeted optimization to the application – comprehensive device settings from sensor technology to system integration for optimum application adaptation.

Navigation  Application

Application		
► Measured values	→ 	53
► System units	→ 	57
► Totalizers	→ 	63
► Sensor	→ 	68
► Current output 1	→ 	87
► Communication	→ 	98

4.1 "Measured values" submenu

Navigation  Application → Measured values

► Measured values		
Mass flow	→ 	53
Volume flow	→ 	54
Corrected volume flow	→ 	54
Density	→ 	54
Temperature	→ 	54
► Totalizer	→ 	55

Mass flow

Navigation  Application → Measured values → Mass flow

Description Displays the mass flow currently measured.
Additional information:
The applicable unit of measure is specified in the "System units" submenu.

User interface Signed floating-point number

Volume flow

Navigation  Application → Measured values → Volume flow

Description Displays the volume flow currently measured.
Additional information:
The applicable unit of measure is specified in the "System units" submenu.

User interface Signed floating-point number

Corrected volume flow

Navigation  Application → Measured values → Correct.vol.flow

Description Displays the currently calculated volume flow compensated for the reference density.
Additional information:
- The reference density can be calculated or fixed.
- The applicable unit of measure is specified in the "System units" submenu.

User interface Signed floating-point number

Density

Navigation  Application → Measured values → Density

Description Displays the density currently measured.
Additional information:
The applicable unit of measure is specified in the "System units" submenu.

User interface Positive floating-point number

Temperature


Navigation  Application → Measured values → Temperature

Description Displays the medium temperature currently measured.
Additional information:
The applicable unit of measure is specified in the "System units" submenu.

User interface Positive floating-point number

4.1.1 "Totalizer" submenu

Navigation   Application → Measured values → Totalizer

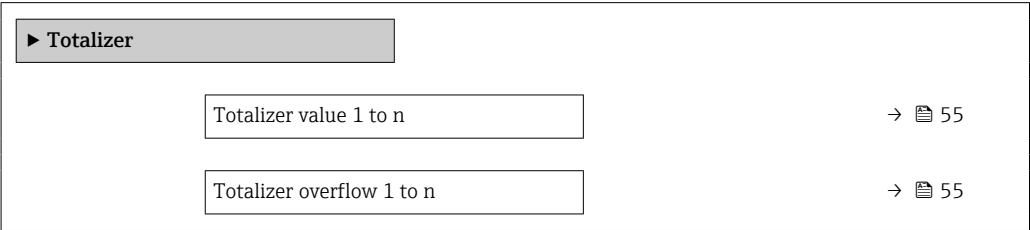

Totalizer value 1 to n

Navigation   Application → Measured values → Totalizer → Totalizer val. 1 to n

Prerequisite A process variable has been selected in the **Assign process variable** parameter in the **Totalizer 1 to n** submenu.

Description Displays the current totalizer counter.

Additional information:

Since the operating tool cannot display figures with more than 7 digits, the current counter above this range equals the sum of the totalizer counter plus the overflow displayed for the "Totalizer overflow" parameter.

Example for how to calculate the current totalizer counter when the value exceeds the 7 digit display range limit of the operating tool:

- Value of "Totalizer value" parameter: 1,968,457 m³
- Value of "Totalizer overflow" parameter: 1 × 10⁷ m³ = 10,000,000 m³
- Current totalizer reading: 11,968,457 m³

In the event of an error, the totalizer behaves as specified in the "Failure mode" parameter.

User interface Signed floating-point number

Totalizer overflow 1 to n

Navigation   Application → Measured values → Totalizer → Tot. overflow 1 to n

Prerequisite A process variable has been selected in the **Assign process variable** parameter in the **Totalizer 1 to n** submenu.

Description

Displays the current totalizer overflow.

Additional information:

If the current totalizer counter exceeds the operating tool's maximum numerical display range of 7 digits, the amount above this range is expressed as an overflow. The current totalizer counter therefore equals the sum of the overflow and the totalizer value displayed in the "Totalizer value" parameter.

Example of how to calculate the current totalizer counter when the value exceeds the 7 digit display limit of the operating tool:

- Value of "Totalizer value" parameter: 1,968,457 m³
- Value of "Totalizer overflow" parameter: $1 \times 10^7 \text{ m}^3 = 10,000,000 \text{ m}^3$
- Current totalizer reading: 11,968,457 m³

User interface

–32 000.0 to 32 000.0

4.2 "System units" submenu

Navigation  Application → System units

► System units		
Mass flow unit	→ 	57
Mass unit	→ 	58
Volume flow unit	→ 	58
Volume unit	→ 	59
Corrected volume flow unit	→ 	60
Corrected volume unit	→ 	60
Density unit	→ 	61
Reference density unit	→ 	61
Temperature unit	→ 	61
Pressure unit	→ 	62

Mass flow unit

Navigation  Application → System units → Mass flow unit

Description Select mass flow unit.

Selection		<i>SI units</i>	<i>US units</i>
		■ g/s	■ oz/s
		■ g/min	■ oz/min
		■ g/h	■ oz/h
		■ g/d	■ oz/d
		■ kg/s	■ lb/s
		■ kg/min	■ lb/min
		■ kg/h	■ lb/h
		■ kg/d	■ lb/d
		■ t/s	■ STon/s
		■ t/min	■ STon/min
		■ t/h	■ STon/h
		■ t/d	■ STon/d

Mass unit

Navigation

  Application → System units → Mass unit

Description

Select mass unit.

- Selection
- SI units*
 - g
 - kg
 - t

US units
 - oz
 - lb
 - STon

Volume flow unit

Navigation

  Application → System units → Volume flow unit

Description

Select volume flow unit.

Selection	<i>SI units</i>	<i>US units</i>	<i>Imperial units</i>
	■ cm ³ /s	■ af/s	■ gal/s (imp)
	■ cm ³ /min	■ af/min	■ gal/min (imp)
	■ cm ³ /h	■ af/h	■ gal/h (imp)
	■ cm ³ /d	■ af/d	■ gal/d (imp)
	■ dm ³ /s	■ ft ³ /s	■ Mgal/s (imp)
	■ dm ³ /min	■ ft ³ /min	■ Mgal/min (imp)
	■ dm ³ /h	■ ft ³ /h	■ Mgal/h (imp)
	■ dm ³ /d	■ ft ³ /d	■ Mgal/d (imp)
	■ m ³ /s	■ MMft ³ /s	■ bbl/s (imp;beer)
	■ m ³ /min	■ MMft ³ /min	■ bbl/min (imp;beer)
	■ m ³ /h	■ MMft ³ /h	■ bbl/h (imp;beer)
	■ m ³ /d	■ Mft ³ /d	■ bbl/d (imp;beer)
	■ ml/s	■ fl oz/s (us)	■ bbl/s (imp;oil)
	■ ml/min	■ fl oz/min (us)	■ bbl/min (imp;oil)
	■ ml/h	■ fl oz/h (us)	■ bbl/h (imp;oil)
	■ ml/d	■ fl oz/d (us)	■ bbl/d (imp;oil)
	■ l/s	■ gal/s (us)	
	■ l/min	■ gal/min (us)	
	■ l/h	■ gal/h (us)	
	■ l/d	■ gal/d (us)	
	■ hl/s	■ Mgal/s (us)	
	■ hl/min	■ Mgal/min (us)	
	■ hl/h	■ Mgal/h (us)	
	■ hl/d	■ Mgal/d (us)	
	■ Ml/s	■ bbl/s (us;liq.)	
	■ Ml/min	■ bbl/min (us;liq.)	
	■ Ml/h	■ bbl/h (us;liq.)	
	■ Ml/d	■ bbl/d (us;liq.)	
		■ bbl/s (us;beer)	
		■ bbl/min (us;beer)	
		■ bbl/h (us;beer)	
		■ bbl/d (us;beer)	
		■ bbl/s (us;oil)	
		■ bbl/min (us;oil)	
		■ bbl/h (us;oil)	
		■ bbl/d (us;oil)	
		■ bbl/s (us;tank)	
		■ bbl/min (us;tank)	
		■ bbl/h (us;tank)	
		■ bbl/d (us;tank)	
		■ kgal/s (us)	
		■ kgal/min (us)	
		■ kgal/h (us)	
		■ kgal/d (us)	

Volume unit


Navigation  Application → System units → Volume unit

Description Select volume unit.

Selection	<i>SI units</i>	<i>US units</i>	<i>Imperial units</i>
	■ cm³ ■ dm³ ■ m³ ■ ml ■ l ■ hl ■ Ml Mega	■ af ■ ft³ ■ Mft³ ■ fl oz (us) ■ gal (us) ■ kgal (us) ■ Mgal (us) ■ bbl (us;oil) ■ bbl (us;liq.) ■ bbl (us;beer) ■ bbl (us;tank)	■ gal (imp) ■ Mgal (imp) ■ bbl (imp;beer) ■ bbl (imp;oil)

Corrected volume flow unit



Navigation Application → System units → Cor.volflow unit

Description Select corrected volume flow unit.

Selection	<i>SI units</i>	<i>US units</i>	<i>Imperial units</i>
	■ l/s ■ l/min ■ l/h ■ l/d ■ Nhl/s ■ Nhl/min ■ Nhl/h ■ Nhl/d ■ Nm³/s ■ Nm³/min ■ Nm³/h ■ Nm³/d ■ Sl/s ■ Sl/min ■ Sl/h ■ Sl/d ■ Sm³/s ■ Sm³/min ■ Sm³/h ■ Sm³/d	■ Sft³/s ■ Sft³/min ■ Sft³/h ■ Sft³/d ■ Sgal/s (us) ■ Sgal/min (us) ■ Sgal/h (us) ■ Sgal/d (us) ■ Sbbl/s (us;liq.) ■ Sbbl/min (us;liq.) ■ Sbbl/h (us;liq.) ■ Sbbl/d (us;liq.) ■ MMSft³/s ■ MMSft³/min ■ MMSft³/h ■ MMSft³/d ■ Sbbl/s (us;oil) ■ Sbbl/min (us;oil) ■ Sbbl/h (us;oil) ■ Sbbl/d (us;oil)	■ Sgal/s (imp) ■ Sgal/min (imp) ■ Sgal/h (imp) ■ Sgal/d (imp)

Corrected volume unit



Navigation Application → System units → Corr. vol. unit

Description Select corrected volume unit.

Selection	<i>SI units</i>	<i>US units</i>	<i>Imperial units</i>
	■ NI ■ Nhl ■ Nm³ ■ SI ■ Sm³	■ Sft³ ■ MMSft³ ■ Sgal (us) ■ Sbbl (us;liq.) ■ Sbbl (us;oil)	Sgal (imp)

Density unit



Navigation Application → System units → Density unit

Description Select density unit.

Selection	<i>SI units</i>	<i>US units</i>	<i>Imperial units</i>
	■ g/cm³ ■ g/m³ ■ g/ml ■ kg/l ■ kg/dm³ ■ kg/m³	■ lb/ft³ ■ lb/gal (us) ■ lb/bbl (us;liq.) ■ lb/bbl (us;beer) ■ lb/bbl (us;oil) ■ lb/bbl (us;tank)	■ lb/gal (imp) ■ lb/bbl (imp;beer) ■ lb/bbl (imp;oil)
	<i>Other units</i> °API		

Reference density unit



Navigation Application → System units → Ref. dens. unit

Description Select reference density unit.

Selection	<i>SI units</i>	<i>US units</i>
	■ kg/Nm³ ■ kg/NI ■ g/Scm³ ■ kg/Sm³ ■ RD15°C ■ RD20°C	■ lb/Sft³ ■ RD60°F

Temperature unit



Navigation Application → System units → Temperature unit

Description Select temperature unit.

Selection	<i>SI units</i>	<i>US units</i>
	■ °C ■ K	■ °F ■ °R

Pressure unit



Navigation Application → System units → Pressure unit

Description Select pressure unit.

- | <i>SI units</i> | <i>US units</i> |
|-----------------|-----------------|
| ■ MPa a | ■ psi a |
| ■ MPa g | ■ psi g |
| ■ kPa a | |
| ■ kPa g | |
| ■ Pa a | |
| ■ Pa g | |
| ■ bar | |
| ■ bar g | |

4.3 "Totalizers" submenu

Navigation  Application → Totalizers

► Totalizers

► Totalizer handling

→  63

► Totalizer 1 to n

→  63

4.3.1 "Totalizer handling" submenu

Navigation  Application → Totalizers → Totalizer

► Totalizer handling

Reset all totalizers

→  63

Reset all totalizers

Navigation	 Application → Totalizers → Totalizer → Reset all tot.
Description	Reset all totalizers to "0" and restart the totaling process. All flow quantities thus far totalized are thereby deleted.
Selection	■ Cancel ■ Reset + totalize

4.3.2 "Totalizer 1 to n" submenu

Navigation  Application → Totalizers → Totalizer 1 to n

► Totalizer 1 to n

Assign process variable

→  64

Unit totalizer 1 to n

→  64

Totalizer operation mode

→  65

Control Totalizer 1 to n

→  66

Preset value 1 to n	→ 66
Failure mode	→ 67

Assign process variable

Navigation

Application → Totalizers → Totalizer 1 to n → Assign variable

Description

Select process variable for totalizer.
Additional information:
If the option selected is changed, the device resets the totalizer to "0".

Selection

- Off
- Mass flow
- Volume flow
- Corrected volume flow

Unit totalizer 1 to n

Navigation

Application → Totalizers → Totalizer 1 to n → Unit totalizer 1 to n

Prerequisite

A process variable has been selected in the **Assign process variable** parameter in the **Totalizer 1 to n** submenu.

Description

Select process variable totalizer unit.

Selection

- | SI units | US units |
|-------------------|---------------------|
| ■ g [*] | ■ oz [*] |
| ■ kg [*] | ■ lb [*] |
| ■ t [*] | ■ STon [*] |

* Visibility depends on order options or device settings

or

<i>SI units</i>	<i>US units</i>	<i>Imperial units</i>
■ cm ³ *	■ af *	■ gal (imp) *
■ dm ³ *	■ ft ³ *	■ Mgal (imp) *
■ m ³ *	■ Mft ³ *	■ bbl (imp;beer) *
■ ml *	■ fl oz (us) *	■ bbl (imp;oil) *
■ l *	■ gal (us) *	
■ hl *	■ kgal (us) *	
■ Ml Mega *	■ Mgal (us) *	
	■ bbl (us;liq.) *	
	■ bbl (us;beer) *	
	■ bbl (us;oil) *	
	■ bbl (us;tank) *	

* Visibility depends on order options or device settings

or

<i>SI units</i>	<i>US units</i>	<i>Imperial units</i>
■ Nl *	■ Sft ³ *	Sgal (imp) *
■ Nhl *	■ MMSft ³ *	
■ Nm ³ *	■ Sgal (us) *	
■ Sl *	■ Sbbl (us;liq.) *	
■ Sm ³ *	■ Sbbl (us;oil) *	

* Visibility depends on order options or device settings

or

Other units
None *

* Visibility depends on order options or device settings

Additional information

Description
The unit is selected separately for each totalizer. The unit is independent of the option selected in the **System units** submenu (→ ⓘ 57).

Selection
The selection is dependent on the process variable selected in the **Assign process variable** parameter (→ ⓘ 16).

Totalizer operation mode ⓘ

Navigation	ⓘ ⓘ Application → Totalizers → Totalizer 1 to n → Operation mode
Prerequisite	A process variable has been selected in the Assign process variable parameter in the Totalizer 1 to n submenu.
Description	Select totalizer calculation mode.

Selection	■ Net flow total ■ Forward flow total ■ Reverse flow total
Additional information	<i>Selection</i> ■ Net flow total option The flow values in the forward and reverse flow directions are totalized and netted against each other. Net flow is recorded in the flow direction. ■ Forward flow total option Only the flow in the forward flow direction is totalized. ■ Reverse flow total option Only the flow in the reverse flow direction is totalized (= reverse flow quantity).

Control Totalizer 1 to n

Navigation	 Application → Totalizers → Totalizer 1 to n → Control Tot. 1 to n
Prerequisite	A process variable has been selected in the Assign process variable parameter in the Totalizer 1 to n submenu.
Description	Operate the totalizer.
Selection	■ Totalize ■ Reset + hold ■ Preset + hold ■ Reset + totalize ■ Hold
Additional information	<i>Selection</i> ■ Totalize option The totalizer is started or continues running. ■ Reset + hold option The totaling process is stopped and the totalizer is reset to "0". ■ Preset + hold option The totaling process is stopped and the totalizer is set to the start value specified in the "Preset value " parameter. ■ Reset + totalize option The totalizer is reset to "0" and the totaling process is restarted. ■ Hold option Totalizing is stopped.

Preset value 1 to n

Navigation	 Application → Totalizers → Totalizer 1 to n → Preset value 1 to n
Prerequisite	A process variable has been selected in the Assign process variable parameter in the Totalizer 1 to n submenu.
Description	Specify start value for totalizer.

User entry Signed floating-point number

Additional information *Description*

The unit of the selected process variable is specified for the totalizer in the **Unit totalizer** parameter (→  16).

Example

This configuration is suitable for applications such as iterative filling processes with a fixed batch quantity.

Failure mode

Navigation   Application → Totalizers → Totalizer 1 to n → Failure mode

Prerequisite A process variable has been selected in the **Assign process variable** parameter in the **Totalizer 1 to n** submenu.

Description Specify how the totalizer should behave in the event of a device alarm.
Additional information:
The failsafe mode that applies to any other totalizers or outputs is specified separately in other parameters and is not impacted by this setting.

Selection

- Stop
- Actual value
- Last valid value

Additional information *Selection*

- **Stop** option
The totalizer is stopped in the event of a device alarm.
- **Actual value** option
The totalizer continues to totalize based on the current value measured; the device alarm is ignored.
- **Last valid value** option
The totalizer continues to totalize based on the last valid value measured before the device alarm occurred.

4.4 "Sensor" submenu

Navigation  Application → Sensor

► Sensor		
► Process parameters	→ 	68
► Low flow cut off	→ 	70
► Partially filled pipe detection	→ 	71
► Medium settings	→ 	73
► Two phase flow	→ 	74
► External compensation	→ 	77
► Corrected volume flow calculation	→ 	77
► Sensor adjustment	→ 	80
► Calibration	→ 	85

4.4.1 "Process parameters" submenu

Navigation  Application → Sensor → Process param.

► Process parameters		
Flow damping time	→ 	69
Flow override	→ 	69
Density damping	→ 	69
Temperature damping	→ 	70

Flow damping time

**Navigation**

Application → Sensor → Process param. → FlowDampingTime

Description

Enter time constant for flow damping (PT1 element).

- Value = 0: No damping
- Value > 0: Damping increases

Additional information:

Damping is implemented by means of a proportional transmission behavior with first order delay (PT1 element).

User entry

0 to 99.9 s

Flow override

**Navigation**

Application → Sensor → Process param. → Flow override

Description

Stops the measuring process. Can be used for example when cleaning the pipeline.

Selection

- Off
- On

Additional information*Selection***"On" option**

Activates flow override. The diagnostic message "453 Flow override active" is generated.

Additional information:

Output values:

- Temperature: Measurement continues
- Totalizers 1 to 3: No longer totalize

Density damping

**Navigation**

Application → Sensor → Process param. → Density damping

Description

Enter time constant for damping (PT1 element) of the measured value for density:

- Value = 0: No damping
- Value > 0: Damping increases

Additional information:

Damping is implemented by means of a proportional transmission behavior with first order delay (PT1 element).

User entry

0 to 999.9 s

Temperature damping



Navigation Application → Sensor → Process param. → Temp. damping

Description Enter time constant for temperature damping (PT1 element).
- Value = 0: No damping
- Value > 0: Damping increases

Additional information:
Damping is implemented by means of a proportional transmission behavior with first order delay (PT1 element).

User entry 0 to 999.9 s

4.4.2 "Low flow cut off" submenu

Navigation Application → Sensor → Low flow cut off

► Low flow cut off

Low flow cut off

→ 70

On value low flow cutoff

→ 71

Off value low flow cutoff

→ 71

Low flow cut off




Navigation Application → Sensor → Low flow cut off → Low flow cut off

Description Select process variable for low flow cut off to activate low flow cut off.

- Selection**
- Off
 - Mass flow
 - Volume flow
 - Corrected volume flow

Additional information Description

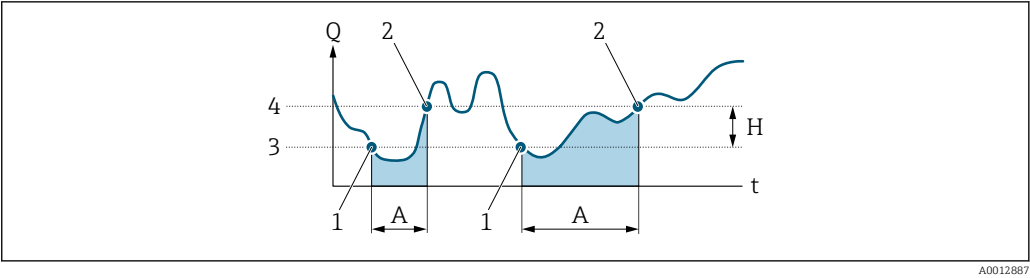

- Q Flow
- t Time
- H Hysteresis
- A Low flow cut off active
- 1 Low flow cut off is activated
- 2 Low flow cut off is deactivated
- 3 On-value entered
- 4 Off-value entered

On value low flow cutoff

Navigation  Application → Sensor → Low flow cut off → On value

Description Enter on value to switch on low flow cut off.
Value = 0: No low flow cut off
Value > 0: Low flow cut off is activated

User entry Positive floating-point number

Off value low flow cutoff

Navigation  Application → Sensor → Low flow cut off → Off value

Description Enter off value to switch off low flow cut off. The off value is entered as a positive hysteresis with respect to the on value.

User entry 0 to 100.0 %

4.4.3 "Partially filled pipe detection" submenu

Navigation  Application → Sensor → Partial pipe det

► Partially filled pipe detection

Partially filled pipe detection

→  72

Low value partial filled pipe detection	→ 72
High value partial filled pipe detection	→ 72

Partially filled pipe detection



Navigation	Application → Sensor → Partial pipe det → Partial pipe det
Description	Select process variable for detection of an empty or partially filled pipe. NOTE Due to low density, deactivate partially filled pipe detection for a gas!
Selection	- Off - Density - Calculated reference density

Low value partial filled pipe detection



Navigation	Application → Sensor → Partial pipe det → Low value
Prerequisite	A process variable has been selected in the Assign process variable parameter in the Empty pipe detection submenu.
Description	Enter the lower limit value for the selected process variable. If the measured value drops below the limit value, diagnostic message "862 Partly filled pipe" is generated. Additional information: - This setting applies only if the "Density unit" parameter is not set to °API. - The lower limit value must be lower than the upper limit value ("High value partial filled pipe detection" parameter).
User entry	Signed floating-point number

High value partial filled pipe detection



Navigation	Application → Sensor → Partial pipe det → High value
Prerequisite	A process variable has been selected in the Assign process variable parameter in the Empty pipe detection submenu.
Description	Enter the upper limit value for the selected process variable. If the measured value exceeds the limit value, diagnostic message "862 Partly filled pipe" is generated. Additional information: This setting applies only if the "Density unit" parameter is set to °API.

User entry Signed floating-point number

4.4.4 "Medium settings" submenu

Navigation  Application → Sensor → Medium settings

► Medium settings

Select medium

→  73

Select gas type

→  73

Reference sound velocity

→  74

Temperature coefficient sound velocity

→  74

Select medium

Navigation  Application → Sensor → Medium settings → Select medium

Description Select the medium type.

- Selection
- Liquid
 - Gas

Select gas type

Navigation  Application → Sensor → Medium settings → Select gas type

Prerequisite In the **Select medium** parameter in the **Medium settings** submenu, the **Gas** option is selected.

Description Select the type of gas.
Additional information:
To achieve accurate measurements, it is necessary to specify the gas.

- Selection
- Air
 - Ammonia NH3
 - Argon Ar
 - Sulfur hexafluoride SF6
 - Oxygen O2
 - Ozone O3
 - Nitrogen oxide NOx
 - Nitrogen N2

- Nitrous oxide N2O
- Methane CH4
- Hydrogen H2
- Helium He
- Hydrogen chloride HCl
- Hydrogen sulfide H2S
- Ethylene C2H4
- Carbon dioxide CO2
- Carbon monoxide CO
- Chlorine Cl2
- Butane C4H10
- Propane C3H8
- Propylene C3H6
- Ethane C2H6
- Others

Reference sound velocity

Navigation	 Application → Sensor → Medium settings → Sound velocity
Prerequisite	In the Select gas type parameter in the Medium settings submenu, the Others option is selected.
Description	Enter sound velocity of the gas at 0 °C (32 °F).
User entry	1 to 99 999.9999 m/s

Temperature coefficient sound velocity

Navigation	 Application → Sensor → Medium settings → Temp. coeff. SV
Prerequisite	In the Select gas type parameter in the Medium settings submenu, the Others option is selected.
Description	Enter the temperature coefficient for the gas sound velocity.
User entry	Positive floating-point number

4.4.5 "Two phase flow" submenu

Navigation  Application → Sensor → Two phase flow

► 2-Phase flow

Gas Fraction Handler

→  75

Index inhomogeneous medium	→ 76
Cut off inhomogeneous wet gas	→ 76
Cut off inhomogeneous liquid	→ 76

Gas Fraction Handler

Navigation	Application → Sensor → Two phase flow → Gas Frac Handler
Description	Activate the Gas Fraction Handler to improve measurement stability and repeatability of a two phase medium. The Gas Fraction Handler continuously tests for the presence of disturbances in single phase flow, i.e. for gas bubbles in liquids or for droplets in gas. In the presence of the second phase, when flow and density become increasingly unstable, the Gas Fraction Handler improves measurement stability with respect to the severity of the disturbances, with no effect under the condition of a single-phase flow. The Gas Fraction Handler stabilizes the output values and enables better readability for operators and interpretation by the process control system. The level of smoothing is adjusted according to the severity of disturbances introduced by the second phase. Additional information: The Gas Fraction Handler applies cumulatively to any fixed damping constants applied to flow and density set elsewhere in the device.
Selection	■ Off ■ Moderate ■ Powerful
Additional information	<i>Selection</i> ■ Off option Deactivates the Gas Fraction Handler. When a second phase is present, large fluctuations of flow and density will occur. ■ Moderate option Use for applications with low level or intermittent levels of second phase. ■ Powerful option Use for applications with very significant levels of second phase.

Index inhomogeneous medium

Navigation	 Application → Sensor → Two phase flow → Index inh.medium
Description	Indicates the severity of the second phase. For applications with entrained gas for example, the index describes the relative amount of entrained gas in the liquid. If there is no entrained gas in the liquid, the value is 0, and for very high levels of gas volume (associated with severe slug flow, for example), the value exceeds 10. Additional information: - The index increases with an increase in the second phase, such as gas volume in a liquid, but scaling is not linear (i.e. no 1:1 correlation of index to gas volume fraction), and with increased flow speed, which results in greater homogeneity, the index value decreases - The index will not saturate with excessive second phase. - The diagnostic is repeatable under the same conditions, and thus can be used to better understand process conditions and the relative severity of the second phase. - This index can also be used to determine the relative level of solids in a liquid or the relative level of a liquid phase in a wet gas.
User interface	Signed floating-point number

Cut off inhomogeneous wet gas

Navigation	 Application → Sensor → Two phase flow → Cut off inh. gas
Description	Enter cut off value for inhomogeneous wet gas applications. Below this value the "Index inhomogeneous medium" is set to 0.
User entry	Positive floating-point number

Cut off inhomogeneous liquid

Navigation	 Application → Sensor → Two phase flow → Cut off liquid
Description	Enter cut off value for inhomogeneous liquid applications. Below this value the "Index inhomogeneous medium" is set to 0. Additional information: This parameter is used for entrained gas in liquid applications or solids in liquid applications.
User entry	Positive floating-point number

4.4.6 "External compensation" submenu

Navigation  Application → Sensor → External comp.

► External compensation

Pressure compensation

→  77

Pressure value

→  77

Pressure compensation

Navigation  Application → Sensor → External comp. → Pressure compen.

Description Select the pressure compensation type.

- Selection
- Off
 - Fixed value

Pressure value

Navigation  Application → Sensor → External comp. → Pressure value

Prerequisite In the **Pressure compensation** parameter in the **External compensation** submenu, the **Fixed value** option is selected.

Description Enter fixed value for the pressure compensation.
Additional information:
The applicable unit of measure is specified in the "System units" submenu.

User entry Positive floating-point number

4.4.7 "Corrected volume flow calculation" submenu

Navigation  Application → Sensor → Corr. vol.flow.

► Corrected volume flow calculation

Select reference density

→  78

Fixed reference density

→  78

Reference temperature	→  78
Linear expansion coefficient	→  79
Square expansion coefficient	→  79

Select reference density

- Navigation  Application → Sensor → Corr. vol.flow. → Select ref. dens
- DescriptionSelect the reference density to use to calculate the corrected volume flow.
- Selection
 - Fixed reference density
 - Calculated reference density

Fixed reference density

- Navigation  Application → Sensor → Corr. vol.flow. → Fix ref.density
- PrerequisiteIn the **Select reference density** parameter (→  78), the **Fixed reference density** option is selected.
- DescriptionEnter a fixed value for the reference density.
- User entryPositive floating-point number

Reference temperature

- Navigation  Application → Sensor → Corr. vol.flow. → Ref. temperature
- PrerequisiteIn the **Select reference density** parameter (→  78), the **Calculated reference density** option is selected.
- DescriptionEnter a reference temperature to calculate the reference density.
- User entry−273.15 to 99 999 °C

Additional information Calculation of the reference density

$$\rho_n = \rho \cdot (1 + \alpha \cdot \Delta t + \beta \cdot \Delta t^2)$$

A0023403

- ρ_n Reference density
- ρ Medium density currently measured
- t Medium temperature currently measured
- t_N Reference temperature at which the reference density is calculated (e.g. 20 °C)
- Δt $t - t_N$
- α Linear expansion coefficient of the medium, unit = [1/K]; K = Kelvin
- β Square expansion coefficient of the medium, unit = [1/K²]

Linear expansion coefficient

Navigation	 Application → Sensor → Corr. vol.flow. → Linear exp coeff
Prerequisite	In the Select reference density parameter (→  78), the Calculated reference density option is selected.
Description	Enter a linear, medium-specific expansion coefficient to calculate the reference density. Additional information: For a medium with a non-linear expansion pattern, use the "Square expansion coefficient" parameter instead.
User entry	Signed floating-point number

Square expansion coefficient

Navigation	 Application → Sensor → Corr. vol.flow. → Square exp coeff
Prerequisite	In the Select reference density parameter (→  78), the Calculated reference density option is selected.
Description	Enter a quadratic, medium-specific expansion coefficient to calculate the reference density. Additional information: For a medium with a linear expansion pattern, use the "Linear expansion coefficient" parameter instead.
User entry	0 to 1 1/K ²

4.4.8 "Sensor adjustment" submenu

Navigation   Application → Sensor → Sensor adjustm.

► Sensor adjustment		
Installation direction	→ 	80
► Zero point adjustment	→ 	80
► Process variable adjustment	→ 	81

Installation direction

Navigation   Application → Sensor → Sensor adjustm. → Install. direct.

Description Select sign of flow direction

- Selection
- Forward flow
 - Reverse flow

"Zero point adjustment" submenu

Navigation   Application → Sensor → Sensor adjustm. → Zero point adj.

► Zero point adjustment		
Zero point adjustment control	→ 	80
Zero point adjustment status	→ 	81
Progress	→ 	81

Zero point adjustment control

Navigation   Application → Sensor → Sensor adjustm. → Zero point adj. → Zero point adj.

Description Start or cancel a zero point adjustment.

Additional information:

The following conditions must be met to perform a zero point adjustment successfully:

- The actual flow rate must be 0.
- The pressure must be at least 1.034 bar.

Selection ■ Cancel
 ■ Start

Zero point adjustment status

Navigation  Application → Sensor → Sensor adjustm. → Zero point adj. → Zero pt adj.stat

Description Displays the status of the zero point adjustment.

User interface ■ Busy
 ■ Zero point adjust failure
 ■ Ok

Progress

Navigation  Application → Sensor → Sensor adjustm. → Zero point adj. → Progress

Description Shows the progress of the process.

User interface 0 to 100 %

"Process variable adjustment" submenu

Navigation  Application → Sensor → Sensor adjustm. → Variable adjust

► Process variable adjustment

Mass flow offset

→  82

Mass flow factor

→  82

Volume flow offset

→  82

Volume flow factor

→  83

Density offset

→  83

Density factor

→  83

Corrected volume flow offset

→  83

Corrected volume flow factor

→  84

Temperature offset	→ 84
Temperature factor	→ 84

Mass flow offset

Navigation	Application → Sensor → Sensor adjustm. → Variable adjust → Mass flow offset
Description	Enter the offset by which to shift the zero point for mass flow. Additional information: The applicable unit of measure is kg/s.
User entry	Signed floating-point number
Additional information	<i>Description</i> Corrected value = (factor × value) + offset

Mass flow factor

Navigation	Application → Sensor → Sensor adjustm. → Variable adjust → Mass flow factor
Description	Enter the multiplication factor to apply to the mass flow value.
User entry	Positive floating-point number
Additional information	<i>Description</i> Corrected value = (factor × value) + offset

Volume flow offset

Navigation	Application → Sensor → Sensor adjustm. → Variable adjust → Vol. flow offset
Description	Enter the offset by which to shift the zero point for volume flow. Additional information: The applicable unit of measure is m3/s.
User entry	Signed floating-point number
Additional information	<i>Description</i> Corrected value = (factor × value) + offset

Volume flow factor



Navigation	Application → Sensor → Sensor adjustm. → Variable adjust → Vol. flow factor
Description	Enter the multiplication factor to apply to the volume flow.
User entry	Positive floating-point number
Additional information	<i>Description</i> Corrected value = (factor × value) + offset

Density offset



Navigation	Application → Sensor → Sensor adjustm. → Variable adjust → Density offset
Description	Enter the offset by which to shift the zero point for density. Additional information: The applicable unit of measure is kg/m ³ .
User entry	Signed floating-point number
Additional information	<i>Description</i> Corrected value = (factor × value) + offset

Density factor



Navigation	Application → Sensor → Sensor adjustm. → Variable adjust → Density factor
Description	Enter the multiplication factor to apply to the density value.
User entry	Positive floating-point number
Additional information	<i>Description</i> Corrected value = (factor × value) + offset

Corrected volume flow offset



Navigation	Application → Sensor → Sensor adjustm. → Variable adjust → Corr. vol offset
Description	Enter the offset by which to shift the zero point for the corrected volume flow. Additional information: The applicable unit of measure is Nm ³ /s.

User entry Signed floating-point number

Additional information *Description*
Corrected value = (factor × value) + offset

Corrected volume flow factor

Navigation   Application → Sensor → Sensor adjustm. → Variable adjust → Corr. vol factor

Description Enter the multiplication factor to apply to the corrected volume flow value.

User entry Positive floating-point number

Additional information *Description*
Corrected value = (factor × value) + offset

Temperature offset

Navigation   Application → Sensor → Sensor adjustm. → Variable adjust → Temp. offset

Description Enter the offset by which to shift the zero point for temperature.
Additional information:
The applicable unit of measure is K.

User entry Signed floating-point number

Additional information *Description*
Corrected value = (factor × value) + offset

Temperature factor

Navigation   Application → Sensor → Sensor adjustm. → Variable adjust → Temp. factor

Description Enter the multiplication factor to apply to the temperature value.

User entry Positive floating-point number

Additional information *Description*
Corrected value = (factor × value) + offset

4.4.9 "Calibration" submenu

Navigation  Application → Sensor → Calibration

► Calibration

Nominal diameter

→  85

Calibration factor

→  85

Zero point

→  85

Nominal diameter

Navigation	 Application → Sensor → Calibration → Nominal diameter
Description	Shows the nominal diameter of the sensor.
User interface	Character string comprising numbers, letters and special characters (#20)

Calibration factor

Navigation	 Application → Sensor → Calibration → Cal. factor
Description	Displays the current calibration factor for the flow rate measuring sensor. Additional information: The factory setting for the calibration factor can be found on the sensor's nameplate.
User interface	Signed floating-point number

Zero point



Navigation	 Application → Sensor → Calibration → Zero point
Description	Displays the zero point correction value for the sensor. NOTE Users logged on in the Service role have write access!
User entry	Signed floating-point number

C0 to 5

Navigation	 Application → Sensor → Calibration → C0 to 5
Description	Displays the current coefficients for density.
User interface	Signed floating-point number

4.5 "Current output" submenu

Navigation  Application → Curr.output 1

► Current output 1

Process variable current output

→  87

Measuring mode current output

→  88

Current range output

→  92

Fixed current

→  93

Lower range value output

→  93

Upper range value output

→  95

Damping current output

→  95

Failure behavior current output

→  96

Failure current

→  96

Output current 1

→  97

Process variable current output

Navigation  Application → Curr.output 1 → Proc.var. outp

Description Select process variable for current output

- Selection
- Off *
 - Mass flow
 - Volume flow
 - Corrected volume flow
 - Temperature
 - Density *
 - Index inhomogeneous medium
 - Exciter current 0
 - Oscillation frequency 0
 - Oscillation amplitude 0 *
 - Frequency fluctuation 0 *
 - Oscillation damping 0
 - Oscillation damping fluctuation 0 *

* Visibility depends on order options or device settings

- Signal asymmetry
- HBSI^{*}
- Electronics temperature

Measuring mode current output



Navigation	 Application → Curr.output 1 → Meas.mode outp
Prerequisite	A process variable is selected in the Process variable current output parameter (→  23).
Description	Select the measuring mode for the output.
Selection	■ Forward flow ■ Forward/Reverse flow[*] ■ Reverse flow compensation

^{*} Visibility depends on order options or device settings

Additional information*Selection*■ **Forward flow** option

The current output signal is proportional to the measured value for the process variable assigned.

Additional information:

- The lower limit value ("Lower range value output " parameter) and the upper limit value ("Upper range value output " parameter) of the measured value range do not have to have the same algebraic sign, i.e. the lower limit value can be negative and the upper limit value positive.
- If the measured value lies outside the scaled measured value range, diagnostic message "441 Current output faulty" is generated.

■ **Forward/Reverse flow** option

The current output outputs the absolute value for the assigned process variable (reflection across the lower limit value of the measured value range).

Additional information:

- The lower limit value ("Lower range value output " parameter) and the upper limit value ("Upper range value output " parameter) of the measured value range must have the same algebraic sign.
- If the absolute value exceeds the upper limit value of the measured value range, diagnostic message "441 Current output faulty" is generated.
- This setting is generally only used for flow-related process variables.

■ **Reverse flow compensation** option


The current output signal is proportional to the measured value for the process variable assigned.

Additional information:

- The lower limit value ("Lower range value output " parameter) and the upper limit value ("Upper range value output " parameter) of the measured value range do not have to have the same algebraic sign, i.e. the lower limit value can be negative and the upper limit value positive.
- Reverse flow (a measured value below the lower limit value of the measured value range) is stored in a buffer and processed after a maximum delay of 60 s with the next forward flow.
- When the flow exceeds the maximum value or the reverse flow stored in the buffer cannot be processed within approx. 60 s, diagnostic message "441 Current output faulty" is generated.
- This option is used e.g. to compensate intermittent reverse flow, which may occur in connection with positive displacement pumps as a result of wear and tear or high viscosity.
- There is no flow damping with this setting.

1. Examples of the behavior of the current output

Defined measuring range: lower range value and upper range value with the **same** algebraic sign.

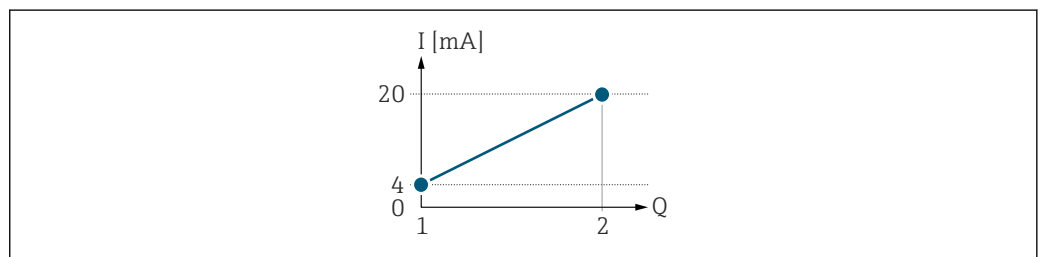

A0028084


I Current

Q Flow

1 Lower range value (value assigned to 0/4 mA current)

2 Upper range value (value assigned to 20 mA current)

With the following flow response:

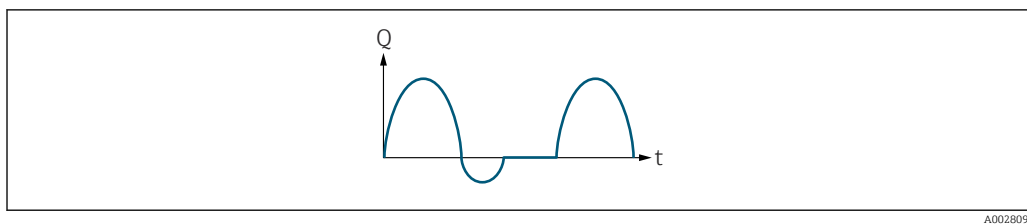


A0028091

Q Flow
 t Time

With the **Forward flow** option

The current output signal is proportional to the process variable assigned. The flow components outside the scaled measuring range are not taken into account for signal output..

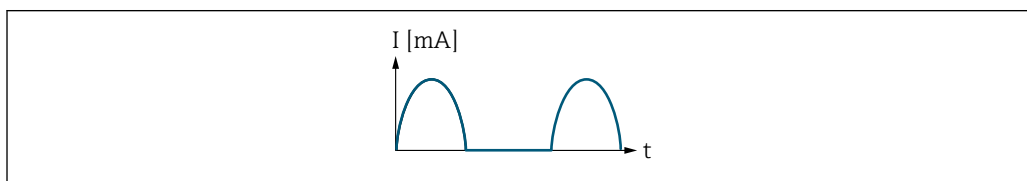


A0028092

I Current
 t Time

With the **Forward/Reverse flow** option

The current output signal is independent of the direction of flow.

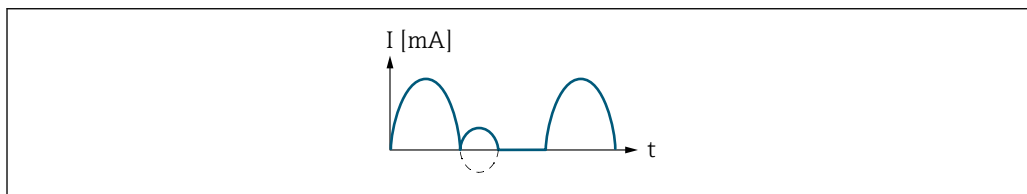


A0028093

I Current
 t Time

With the **Reverse flow compensation** option

Flow components outside the measuring range are buffered, balanced and output after a maximum delay of 60 s.

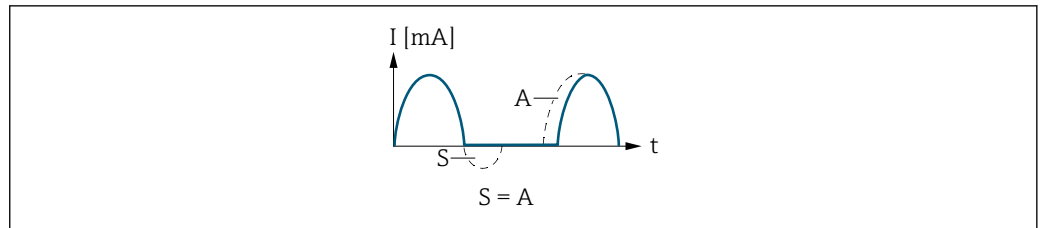


A0028094

- I* Current
t Time
S Flow components saved
A Balancing of saved flow components

2. Examples of the behavior of the current output


Defined measuring range: lower range value and upper range value with **different** algebraic signs.

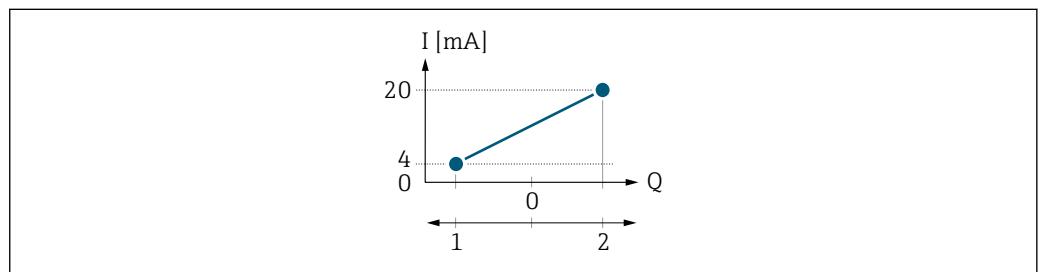

A0028095

- I* Current
Q Flow
 1 Lower range value (value assigned to 0/4 mA current)
 2 Upper range value (value assigned to 20 mA current)

With flow a (–) outside, b (– –) inside the measuring range:

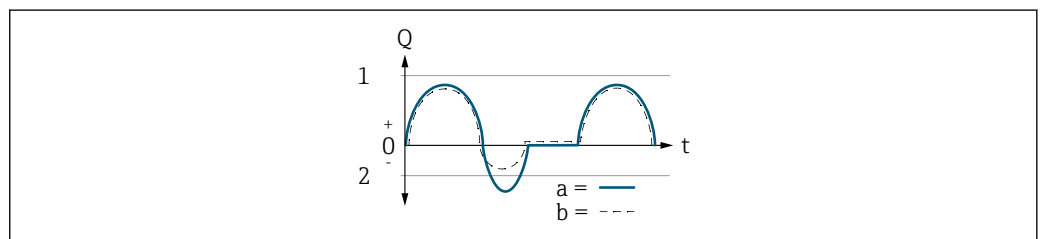


A0028098

- Q* Flow
t Time
a Lower range value (value assigned to 0/4 mA current)
b Upper range value (value assigned to 20 mA current)

With the **Forward flow** option

- a (–): The flow components outside the scaled measuring range cannot be taken into account for signal output. The diagnostic message **△S441 Current output 1 to n** diagnostic message is displayed.
- b (– –): The current output signal is proportional to the process variable assigned.

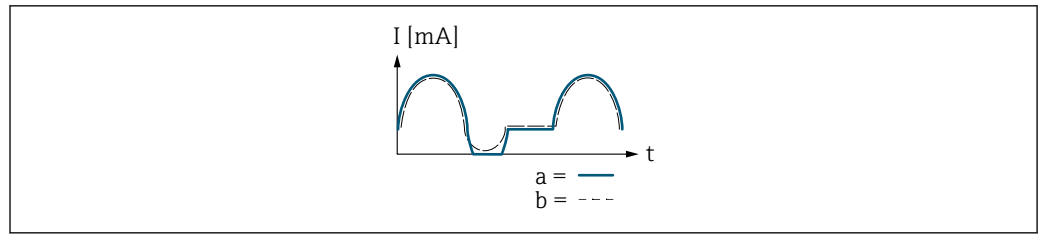

A0028100


I Current
t Time

With the **Forward/Reverse flow** option

This option cannot be selected here since the values for the **20 mA value** parameter (→ 26) and **20 mA value** parameter (→ 26) have different algebraic signs.

With the **Reverse flow compensation** option

Flow components outside the measuring range are buffered, balanced and output after a maximum delay of 60 s.

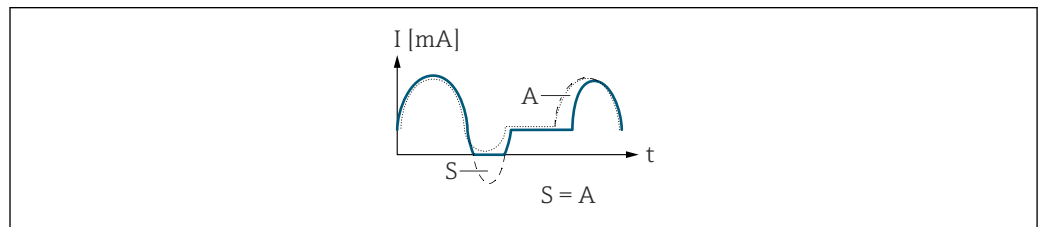

A0028101

I Current
t Time
S Flow components saved
A Balancing of saved flow components

Current range output



Navigation

Application → Curr.output 1 → Curr.range out

Description

Select the current range for the measured value output and the upper and lower fault condition signal level.

Additional information:

- The measured value range is specified in the "Lower range value output" parameter and the "Upper range value output" parameter.
- If the measured value lies outside the scaled measured value range, diagnostic message "441 Current output faulty" is generated.
- In the event of a device alarm, the current output adopts the behavior specified in the "Failure behavior current output" parameter.

Selection

- 4...20 mA NE (3.8...20.5 mA)
- 4...20 mA US (3.9...20.8 mA)
- 4...20 mA (4... 20.5 mA)
- Fixed value


Additional information

Selection

- **4...20 mA NE (3.8...20.5 mA)** option
Select this option to set the current range in accordance with NAMUR recommendation NE43.
- **Fixed value** option
Select this option to set the current output to a current value instead of a range.

The current value is defined in the **Fixed current** parameter (→ 26).

The graphic shows the relationship between the current range for the output of the process value and the lower and upper alarm levels:

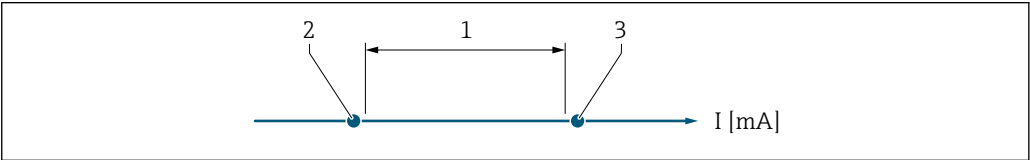

- 1 Current range for process value
- 2 Lower level for signal on alarm
- 3 Upper level for signal on alarm

Selection (current range for process value)	Lower level for signal on alarm	Upper level for signal on alarm
4...20 mA NE (3.8...20.5 mA)	< 3.6 mA	> 21.5 mA
4...20 mA US (3.9...20.8 mA)		
4...20 mA (4... 20.5 mA)		

Fixed current



Navigation

Application → Curr.output 1 → Fixed current

Prerequisite

In the **Current range output** parameter in the **Current output 1** submenu, the **Fixed value** option is selected.

Description

Enter the value for the "Fixed value" option.

User entry

3.59 to 21.5 mA

Lower range value output



Navigation

Application → Curr.output 1 → Low.range outp

Prerequisite

- In the **Current range output** parameter, one of the following options is selected:
- 4...20 mA NE (3.8...20.5 mA)
 - 4...20 mA US (3.9...20.8 mA)
 - 4...20 mA (4... 20.5 mA)

Description

Enter lower range value for the measured value range.

Additional information:

- Depending on the setting selected for the "Measuring mode current output " parameter, the value specified for this parameter and the "Upper range value output " parameter must have the same algebraic sign or not.
- As a rule, the lower range value is scaled to be lower than the upper range value. As a result, the behavior of the current output is proportional to the process variable assigned. If the lower range value is scaled to be higher than the upper range value, then the behavior of the current output will be inversely proportional to the process variable assigned.

User entry


Signed floating-point number

Additional information

Examples of the behavior, depending on the option selected in the **Measuring mode current output** parameter (→  88).

Example: Measuring mode with "Forward flow" option

- **Lower range value output** parameter (→  24) = not equal to zero flow (e.g. -250 m³/h)
- **Upper range value output** parameter (→  26) = not equal to zero flow (e.g. +750 m³/h)
- Calculated current value = 8 mA at zero flow

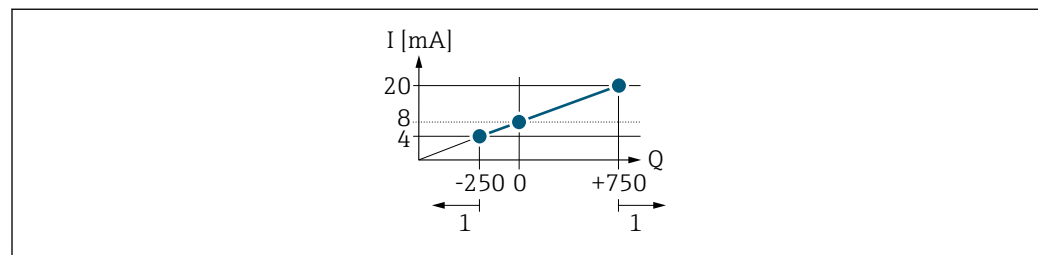


A0013757

Q Flow
I Current
1 Measuring range is exceeded or undershot

The linear operational range of the measuring device is defined by the values entered for the **Lower range value output** parameter (→  24) and **Upper range value output** parameter (→  26), and by the selected current range.

Example: Measuring mode with the "Forward/Reverse flow" option

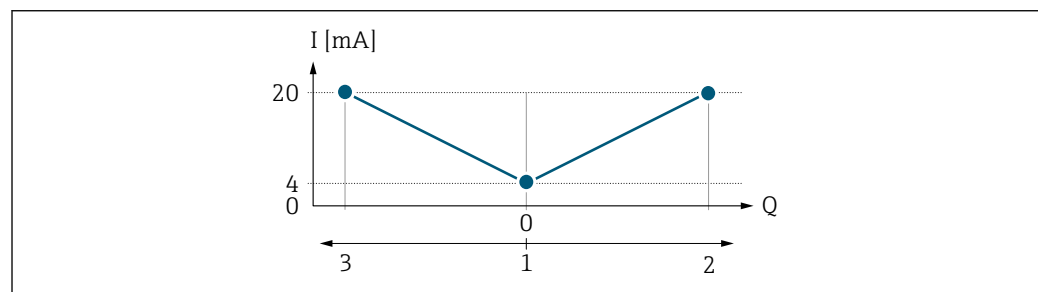

A0013758

Q Flow
I Current
1 Value assigned to 0/4 mA current
2 Forward flow
3 Reverse flow

The current output signal is independent of the direction of flow (absolute amount of the measured variable). The values for the **Lower range value output** parameter (→  24) and **Upper range value output** parameter (→  26) must have the same algebraic sign.

The value for the **Upper range value output** parameter (→  26) (e.g. reverse flow) corresponds to the mirrored value for the **Upper range value output** parameter (→  26) (e.g. forward flow).

Example: Measuring mode with the "Reverse flow compensation" option

If flow is characterized by severe fluctuations (e.g. when using reciprocating pumps), flow components outside the measuring range are buffered, balanced and output after a maximum delay of 60 s.

Upper range value output

Navigation	  Application → Curr.output 1 → Upp.range outp
Prerequisite	In the Current range output parameter, one of the following options is selected: ■ 4...20 mA NE (3.8...20.5 mA) ■ 4...20 mA US (3.9...20.8 mA) ■ 4...20 mA (4... 20.5 mA)
Description	Enter upper range value for the measured value range.
User entry	Signed floating-point number
Additional information	 Examples of the behavior, depending on the option selected in the Measuring mode current output parameter: Lower range value output parameter (→  24):

Damping current output

Navigation	  Application → Curr.output 1 → Damp.curr.outp
Prerequisite	A process variable is selected in the Process variable current output parameter and one of the following options is selected in the Current range output parameter: ■ 4...20 mA NE (3.8...20.5 mA) ■ 4...20 mA US (3.9...20.8 mA) ■ 4...20 mA (4... 20.5 mA)
Description	Enter time constant (PT1 element) to set the reaction time of the output signal to fluctuations in the measured value caused by process conditions. Additional information: - The smaller the time constant the faster the output reacts to fluctuations in the measured value. - If the time constant is 0, damping is deactivated.
User entry	0.0 to 999.9 s

Failure behavior current output 	
Navigation	 Application → Curr.output 1 → Fail.behav.out
Prerequisite	A process variable is selected in the Process variable current output parameter and one of the following options is selected in the Current range output parameter: ■ 4...20 mA NE (3.8...20.5 mA) ■ 4...20 mA US (3.9...20.8 mA) ■ 4...20 mA (4... 20.5 mA)
Description	Specify how the output should behave in the event of a device alarm.
Selection	■ Min. ■ Max. ■ Last valid value ■ Actual value ■ Fixed value
Additional information	<i>Selection</i> ■ Min. option The current output outputs the lower fault condition signal level for the specified current range. Additional information: The current range is specified in the "Current range output " parameter. ■ Max. option The current output outputs the upper fault condition signal level for the specified current range. Additional information: The current range is specified in the "Current range output " parameter. ■ Last valid value option The current output outputs the last valid value measured before the device alarm occurred. ■ Actual value option The current output outputs the flow value currently measured. The device alarm is ignored. ■ Fixed value option The current output outputs the value specified. Additional information: The value is specified in the "Failure current " parameter.
Failure current 	
Navigation	 Application → Curr.output 1 → Fail. current
Prerequisite	In the Failure behavior current output parameter in the Current output 1 submenu, the Fixed value option is selected.
Description	Enter the value for the "Fixed value" option in the "Failure behavior current output " parameter.
User entry	3.59 to 21.5 mA

Output current

Navigation	 Application → Curr.output 1 → Output curr. 1
Description	Displays the current value currently calculated.
User interface	3.59 to 21.5 mA

4.6 "Communication" submenu

Navigation  Application → Communication

► Communication	
► Modbus configuration	→  98
► Modbus data map	→  101
► Modbus information	→  102

4.6.1 "Modbus configuration" submenu

Navigation  Application → Communication → Modbus config.

► Modbus configuration	
Bus address	→  98
Baudrate	→  99
Parity	→  99
Byte order	→  100
Telegram delay	→  100
Failure mode	→  100
Fieldbus writing access	→  101

Bus address	
-------------	---

Navigation	 Application → Communication → Modbus config. → Bus address
Description	Enter device address.
User entry	1 to 247

Baudrate

**Navigation**

Application → Communication → Modbus config. → Baudrate

Description

Define data transfer speed.

Selection

- 1200 BAUD
- 2400 BAUD
- 4800 BAUD
- 9600 BAUD
- 19200 BAUD
- 38400 BAUD
- 57600 BAUD
- 115200 BAUD

Parity

**Navigation**

Application → Communication → Modbus config. → Parity

Description

Select parity bits.

Additional information:

"ASCII" picklist option:

- 0 = "Even" option
- 1 = "Odd" option

"RTU" picklist option:

- 0 = "Even" option
- 1 = "Odd" option
- 2 = "No parity bit/1 stop bit" option
- 3 = "No parity bit/2 stop bits" option

Selection

- Odd
- Even
- None / 1 stop bit
- None / 2 stop bits

Byte order 	
Navigation	  Application → Communication → Modbus config. → Byte order
Description	Select byte transmission sequence. The transmission sequence must be coordinated with the Modbus master. Additional information: The byte sequence is not standardized by the Modbus protocol. However, if the host system and the measuring device do not use the same byte sequence, correct data exchange is not possible. Changing the byte sequence in the host system often requires extensive knowledge and significant programming effort. This parameter can be used to keep the standard settings of the host system, while adjusting the byte sequence on the measuring device by means of trial and error. If it is not possible to achieve correct data exchange in this manner, then it is the host system's settings for the byte sequence that must be modified.
Selection	■ 0-1-2-3 ■ 3-2-1-0 ■ 1-0-3-2 ■ 2-3-0-1
Telegram delay 	
Navigation	  Application → Communication → Modbus config. → Telegram delay
Description	Enter a delay time after which the measuring device replies to the request telegram of the Modbus master. This is to enable communication with slow Modbus RS485 masters.
User entry	0 to 100 ms
Failure mode 	
Navigation	  Application → Communication → Modbus config. → Failure mode
Description	Select the preferred Modbus communication output mode for the measured value, when a diagnostic event of the category specified in the "Assign diagnostic behavior" parameter occurs.
Selection	■ NaN value ■ Last valid value
Additional information	<i>Selection</i> ■ NaN value option The device outputs the NaN value ("Not a number" value). ■ Last valid value option The device displays the last valid measured value before the issue occurred.

Fieldbus writing access

Navigation	 Application → Communication → Modbus config. → Fieldb.writ.acc.
Description	Restrict access to the measuring device via Fieldbus. Additional information: Once read and/or write protection has been enabled, this parameter can only be accessed and reset via local operation. Access via an operating tool is no longer possible. NOTE The cyclical transmission of measured values to the higher-order system is not impacted by these restrictions and always guaranteed!
Selection	■ Read + write ■ Read only

4.6.2 "Modbus data map" submenu

Navigation  Application → Communication → Modbus data map

► Modbus data map

Scan list register 0 to 15

→  101

Scan list register 0 to 15

Navigation	 Application → Communication → Modbus data map → Scan list reg.0 to 15
Description	Enter the scan list register. Additional information: By entering the register address (1-based), it is possible to group up to 16 device parameters, which thereby are assigned to the scan list registers 0 to 15. The data corresponding to the device parameters assigned is read out via the register addresses 5051 to 5081.
User entry	0 to 65 535

4.6.3 "Modbus information" submenu

Navigation  Application → Communication → Modbus info

► Modbus information

Device ID

→  102

Device revision

→  102

Device ID

Navigation	 Application → Communication → Modbus info → Device ID
Description	Displays the device ID to identify the measuring device.
User interface	0 to 65 535

Device revision

Navigation	 Application → Communication → Modbus info → Device revision
Description	Displays device revision.
User interface	0 to 65 535

5 "System" menu

Overall device management and security settings – management of system settings and adaption to operational requirements.

Navigation  System

System		
▶ Device management	→ 	104
▶ User management	→ 	107
▶ Connectivity	→ 	110
▶ Date/time	→ 	111
▶ Information	→ 	113
▶ Display	→ 	118
▶ Software configuration	→ 	122

5.1 "Device management" submenu

Navigation  System → Device manag.

▶ Device management		
Device tag	→	 104
Locking status	→	 104
Configuration counter	→	 105
Device reset	→	 105

Device tag	
------------	---

Navigation  System → Device manag. → Device tag

Description Enter a unique designation for the measuring point to be able to easily identify it within the plant.

User entry Character string comprising numbers, letters and special characters (#32)

Locking status

Navigation  System → Device manag. → Locking status

Description Indicates the write protection with the highest priority that is currently active.

- User interface
- Hardware locked
 - Temporarily locked

Additional information *User interface*

- **Hardware locked** option
The DIP switch for the hardware lock is enabled. As a result write access to the parameters is locked.
- **Temporarily locked** option
Due to internal procedures that are currently in progress (e.g. data upload/download, reset, etc.), write access to the parameters is temporarily locked. The parameters can be modified again, once the internal procedures are complete.

Configuration counter

Navigation
 System → Device manag. → Config. counter
Description

Displays the counter for changes to the device parameters.

Additional information:

- If the value for a static parameter is changed when optimizing or configuring the parameter, the counter is incremented by 1. This is to enable tracking different parameter versions.
- When multiple parameters are changed simultaneously, e.g. when loading parameters into the device from an external source such as FieldCare, the counter may display a higher value. The counter cannot be reset, nor is it reset to a default value on performing a device reset.
- Once the counter has reached the value 65535, it restarts at 0.

User interface

0 to 65 535

Device reset

**Navigation**
 System → Device manag. → Device reset
Description

Reset the device configuration - either entirely or in part - to a defined state.

Selection

- Cancel
- To delivery settings
- Restart device
- Restore S-DAT backup *
- Create T-DAT backup
- Restore T-DAT backup *

Additional information

Selection

- **To delivery settings** option
Every parameter for which a customer-specific default setting was ordered is reset to the customer-specific value. All other parameters are reset to the factory setting.
- **Restart device** option
The restart resets every parameter with data stored in volatile memory (RAM) to the factory setting (e.g. measured value data). The device configuration remains unchanged.
- **Delete powerfail data** option
Deletes the powerfail data segment in the T-DAT or (if applicable) the T-DAT partition of the S-DAT.
Additional information:
This function resolves the following memory content error: "283 Memory content inconsistent" with Service ID 225 and Service ID 721.

* Visibility depends on order options or device settings

- **Delete T-DAT** option

Deletes the T-DAT or (if applicable) the T-DAT partition of the S-DAT. On performing this delete operation, all parameters on the T-DAT are reset to the default values.

Additional information:

This function can be used to resolve any memory content issue on the T-DAT.

NOTE

The powerfail data and device delivery settings will no longer be available on performing this delete operation!

- **Delete flash file system** option

Deletes the flash file system.

Additional information:

This function resolves the following memory content error: "387 HistoROM data faulty" with Service ID 648.

NOTE

The menu structure set up for the SmartBlue app and the files used to perform a firmware restore in the event the firmware is corrupted will no longer be available on performing this delete operation!

- **Reset faulty parameters** option

Resets all faulty parameters to default values when the following memory content error occurs: "283 Memory content inconsistent" with Service ID 367.

Additional information:

Only faulty parameters are reset. All parameters that are reset are logged in the logbook.

- **Delete delivery settings** option

Deletes the delivery settings on the T-DAT or (if applicable) T-DAT partition of the S-DAT.

Additional information:

This function resolves the following memory content error: "311 Sensor electronics (ISEM) faulty" with Service ID 226.

NOTE

The device delivery settings will no longer be available on performing this delete operation!

- **Restore S-DAT backup** option

Restore the data that is saved on the S-DAT. The data record is restored from the electronics memory to the S-DAT.

- **Create T-DAT backup** option

Create T-DAT backup.

5.2 "User management" submenu

Navigation   System → User manag.

► User management	
User role	→  107
Enter access code	→  108
Reset Maintenance code	→  108
► Define Maintenance code	→  109

User role

Navigation	  System → User manag. → User role
Description	Displays the role the user is currently logged on in. The role determines the user's access rights for the parameters. Additional information: - Until a Maintenance code has been set in the "Define Maintenance code" parameter, all users are automatically logged on in the Maintenance role. Once the Maintenance code has been set, all users are automatically logged on in the Operator role. - The access rights can be changed via the "Enter access code" parameter.
User interface	■ Operator ■ Maintenance ■ Service ■ Production ■ Development
Additional information	User interface ■ Operator option Provides only read access to parameters. ■ Maintenance option Provides read and write access to parameters. Additional information: For some parameters, the user must be logged on in the Service role to obtain write access. ■ Service option Provides read and write access to Service parameters.

Enter access code

Navigation	 System → User manag. → Ent. access code
Description	For users logged on in the Operator role, enter the Maintenance code to change the access status to Maintenance and disable write protection of parameters. For users logged on in the Maintenance role, enter the Service code to change the access status to Service and enable read and write access to Service parameters.
User entry	0 to 9 999

Reset Maintenance code

Navigation	 System → User manag. → Reset Maint code
Description	Enter the code provided by Endress+Hauser Technical Support to reset the Maintenance code.
User entry	Character string comprising numbers, letters and special characters (#32)

5.2.1 "Define access code" wizard

Complete this wizard to specify an access code for the Maintenance role.

Navigation  System → User manag. → Def. access code

► Define Maintenance code

Define Maintenance code

→  109

Confirm Maintenance code

→  109

Define Maintenance code

Navigation  System → User manag. → Def. Maint. code → Def. Maint. code

Description Specify an access code that is required to obtain the access rights for the Maintenance role.

User entry 0 to 9 999

Confirm Maintenance code

Navigation  System → User manag. → Def. Maint. code → Conf. Maint code

Description Confirm the access code entered for the Maintenance role.

User entry 0 to 9 999

5.3 "Connectivity" submenu

Navigation   System → Connectivity

► Connectivity

► Bluetooth configuration →  110

5.3.1 "Bluetooth configuration" submenu

Navigation   System → Connectivity → Bluetooth conf.

► Bluetooth configuration

Bluetooth →  110

Communication established →  110

Bluetooth

Navigation   System → Connectivity → Bluetooth conf. → Bluetooth

Description Enable or disable Bluetooth.

- Selection
- Enable
 - Disable
 - Not available *

Communication established

Navigation   System → Connectivity → Bluetooth conf. → Communi. establ.

- User interface
- No
 - Yes

* Visibility depends on order options or device settings

5.4 "Date / Time" submenu

Navigation   System → Date / Time

► Date/time

Set date/time

→  111

Time format

→  111

Time zone

→  111

Set date/time

Navigation	 System → Date/time → Set date/time
Description	Set the date and local time. Every time the date or time is changed, a logbook entry is created.
User entry	Date and time

Time format

Navigation	  System → Date/time → Time format
Description	Select time format.
Selection	■ 24 h ■ 12 h AM/PM

Time zone

Navigation	  System → Date/time → Time zone
Description	Select the time zone. Every time the time zone is changed, a logbook entry is created.

Selection

Other units

- UTC-12:00
- UTC-11:00
- UTC-10:00
- UTC-09:30
- UTC-09:00
- UTC-08:00
- UTC-07:00
- UTC-06:00
- UTC-05:00
- UTC-04:00
- UTC-03:30
- UTC-03:00
- UTC-02:00
- UTC-01:00
- UTC 00:00
- UTC+01:00
- UTC+02:00
- UTC+03:00
- UTC+03:30
- UTC+04:00
- UTC+04:30
- UTC+05:00
- UTC+05:30
- UTC+05:45
- UTC+06:00
- UTC+06:30
- UTC+07:00
- UTC+08:00
- UTC+08:45
- UTC+09:00
- UTC+09:30
- UTC+10:00
- UTC+10:30
- UTC+11:00
- UTC+12:00
- UTC+12:45
- UTC+13:00
- UTC+14:00

5.5 "Information" submenu

Navigation  System → Information

► Information		
► Device		→  113
► Sensor electronic module (ISEM)		→  116
► Display module		→  116

5.5.1 "Device" submenu

Navigation  System → Information → Device

► Device		
Device name		→  113
Device tag		→  114
Serial number		→  114
Order code		→  114
Firmware version		→  114
Extended order code 1		→  115
Extended order code 2		→  115
Extended order code 3		→  115
ENP version		→  115
Manufacturer		→  116

Device name

Navigation

 System → Information → Device → Device name

Description

Displays the name of the transmitter.
Additional information:
The name can also be found on the transmitter's nameplate.

User interface Character string comprising numbers, letters and special characters (#16)

Device tag

Navigation   System → Information → Device → Device tag

Description Displays the name for the measuring point.

User interface Character string comprising numbers, letters and special characters (#32)

Serial number

Navigation   System → Information → Device → Serial number

Description Displays the serial number of the measuring device. The serial number can be used to identify the measuring device and to retrieve further information on the measuring device, such as the related documentation, via the Device Viewer or Operations app.
Additional information:
The serial number can also be found on the nameplate of the sensor and transmitter.

User interface Character string comprising numbers, letters and special characters (#11)

Order code



Navigation   System → Information → Device → Order code

Description Displays the device order code.
Additional information:
The order code can be used for instance to order a replacement or spare device or to verify that the device features specified on the order form match the shipping note.

User interface Character string comprising numbers, letters and special characters (#20)

Firmware version

Navigation   System → Information → Device → Firmware version

Description Displays the device firmware version installed.

User interface Character string comprising numbers, letters and special characters (#8)

Extended order code 1 	
Navigation	  System → Information → Device → Ext. order cd. 1
Description	Displays the first, second and/or third part of the extended order code. Due to character length restrictions, the extended order code is split into a maximum of 3 parameters. The extended order code indicates for each feature in the product structure the selected option, thereby uniquely identifying the device model. Additional information: The extended order code can also be found on the nameplate.
User interface	Character string comprising numbers, letters and special characters (#20)
Extended order code 2 	
Navigation	  System → Information → Device → Ext. order cd. 2
Description	Displays the first, second and/or third part of the extended order code. Due to character length restrictions, the extended order code is split into a maximum of 3 parameters. The extended order code indicates for each feature in the product structure the selected option, thereby uniquely identifying the device model. Additional information: The extended order code can also be found on the nameplate.
User interface	Character string comprising numbers, letters and special characters (#20)
Extended order code 3 	
Navigation	  System → Information → Device → Ext. order cd. 3
Description	Displays the first, second and/or third part of the extended order code. Due to character length restrictions, the extended order code is split into a maximum of 3 parameters. The extended order code indicates for each feature in the product structure the selected option, thereby uniquely identifying the device model. Additional information: The extended order code can also be found on the nameplate.
User interface	Character string comprising numbers, letters and special characters (#20)
ENP version	
Navigation	  System → Information → Device → ENP version
Description	Displays the version of the electronic nameplate (ENP).

User interface

Character string comprising numbers, letters and special characters (#16)

Manufacturer

Navigation

 System → Information → Device → Manufacturer

Description

Displays the manufacturer.

User interface

Character string comprising numbers, letters and special characters (#32)

5.5.2

"Sensor electronic module (ISEM)" submenu

Navigation

 System → Information → Sens. electronic

► Sensor electronic module (ISEM)

Firmware version

→  116

Firmware version

Navigation

 System → Information → Sens. electronic → Firmware version

Description

Displays the firmware version of the module.

User interface

Positive integer

5.5.3

"Display module" submenu

Navigation

 System → Information → Display module

► Display module

Firmware version

→  117

Firmware version

Navigation	 System → Information → Display module → Firmware version
Description	Displays the firmware version of the module.
User interface	Positive integer

5.6 "Display" submenu

Navigation  System → Display

► Display		
Language	→ 	118
Value 1 display	→ 	119
Value 2 display	→ 	119
Value 3 display	→ 	120
Value 4 display	→ 	120
Display damping	→ 	121
Rotation display	→ 	121
Brightness	→ 	121
Color scheme	→ 	121

Language

Navigation  System → Display → Language

Description Set display language.

- Selection
- English
 - Deutsch
 - Français
 - Español
 - Italiano
 - Nederlands
 - Portuguesa
 - Polski
 - русский язык (Russian)
 - Svenska
 - Türkçe
 - 中文 (Chinese)
 - 日本語 (Japanese)
 - 한국어 (Korean)
 - العَرَبِيَّة (Arabic) *
 - Bahasa Indonesia

* Visibility depends on order options or device settings

- ภาษาไทย (Thai) *
- tiếng Việt (Vietnamese)
- čeština (Czech)

Value 1 display
**Navigation**

System → Display → Value 1 display

Description

Select the measured value that is displayed first on the local display.

Additional information:

The applicable unit of measure is specified in the "System units" submenu.

Selection

- Mass flow
- Volume flow
- Corrected volume flow
- Temperature
- Density *
- Totalizer 1
- Totalizer 2
- Totalizer 3
- Index inhomogeneous medium
- Electronics temperature

Value 2 display
**Navigation**

System → Display → Value 2 display

Description

Select the measured value that is shown second on the local display.

Additional information:

The applicable unit of measure is specified in the "System units" submenu.

Selection

- None
- Mass flow
- Volume flow
- Corrected volume flow
- Temperature
- Density *
- Totalizer 1
- Totalizer 2
- Totalizer 3
- Index inhomogeneous medium
- Electronics temperature

* Visibility depends on order options or device settings

Value 3 display

**Navigation** System → Display → Value 3 display**Description**

Select the measured value that is shown third on the local display.

Additional information:

The applicable unit of measure is specified in the "System units" submenu.

Selection

- None
- Mass flow
- Volume flow
- Corrected volume flow
- Temperature
- Density *
- Totalizer 1
- Totalizer 2
- Totalizer 3
- Index inhomogeneous medium
- Electronics temperature

Value 4 display

**Navigation** System → Display → Value 4 display**Description**

Select the measured value that is shown fourth on the local display.

Additional information:

The applicable unit of measure is specified in the "System units" submenu.

Selection

- None
- Mass flow
- Volume flow
- Corrected volume flow
- Temperature
- Density *
- Totalizer 1
- Totalizer 2
- Totalizer 3
- Index inhomogeneous medium
- Electronics temperature

* Visibility depends on order options or device settings

Display damping		
Navigation	  System → Display → Display damping	
Description	Enter time constant (PT1 element) to set reaction time of the display to fluctuations in the measured value. Additional information: - The smaller the time constant the faster the display reacts to fluctuations in the measured value. - If the time constant is set to 0, damping is deactivated.	
User entry	0.0 to 999.9 s	
Rotation display		
Navigation	  System → Display → Rotation display	
Description	Select rotation angle of the display text to optimize local display readability.	
Selection	■ Auto ■ 0 degree ■ 90 degree ■ 180 degree ■ 270 degree	
Brightness		
Navigation	  System → Display → Brightness	
Description	Adjust brightness.	
User entry	0 to 100 %	
Color scheme		
Navigation	  System → Display → Color scheme	
Description	Select preferred color scheme.	
Selection	■ Light ■ Dark	

5.7 "Software configuration" submenu

Navigation  System → Software config.

► Software configuration

Activate SW option

→  122

Software option overview

→  122

Activate SW option

Navigation	 System → Software config. → Activate SW opt.
Description	Enter application package code or code of the functionality ordered separately to activate it. Additional information: - If a measuring device was ordered with an add-on software option, the activation code is programmed into the measuring device ex factory. - After entering the activation code: Check whether the new software option is displayed in the "Software option overview" parameter and therefore active. NOTE If an an invalid code is entered the software options that have already been activated are invalidated! Before entering a new activation code: Create a record of the existing activation code.
User entry	Positive integer

Software option overview

Navigation	 System → Software config. → SW option overv.
Description	Displays all software options included in the order ex factory or ordered at a later date that have been enabled via the operating interface. Additional information: If a new software option is not displayed after entering the activation code, the code entered was inaccurate or invalid. In this case, contact the appropriate Endress+Hauser sales organization to activate the software option.
User interface	■ Density ■ Heartbeat Verification ■ Heartbeat Monitoring

6 Modbus RS485 register information

6.1 Notes

6.1.1 Structure of the register information

The individual parts of a parameter description are described in the following section:

Navigation: navigation path to the parameter					
Parameter	Register	Data type	Access type	Selection/input	→ 
Name of parameter	Indicated in decimal numerical format	- Float length = 4 byte - Integer length = 2 byte - String length, depending on parameter	Possible type of access to parameter: - Read access via function codes 03, 04 or 23 - Write access via function codes 06, 16 or 23	Selection List of the individual options for the parameter - Option 1 Option 2 Option 3 ⁽⁺⁾  - Factory setting highlighted in bold ⁽⁺⁾ = Factory setting depends on country, order options or device settings Input Input range for the parameter	Page number information and cross-reference to the standard parameter description

NOTICE

If non-volatile device parameters are modified via the MODBUS RS485 function codes 06, 16 or 23, the change is saved in the EEPROM of the measuring device.

The number of writes to the EEPROM is technically restricted to a maximum of 1 million.

- Make sure to comply with this limit since, if it is exceeded, data loss and measuring device failure will result.
- Avoid constantly writing non-volatile device parameters via the MODBUS RS485.

6.1.2 Address model

The Modbus RS485 register addresses of the measuring device are implemented in accordance with the "Modbus Applications Protocol Specification V1.1".

In addition, systems are used that work with the register address model "Modicon Modbus Protocol Reference Guide (PI-MBUS-300 Rev. J)".

Depending on the function code used, a number is added at the start of the register address with this specification:

- "3" → "Read" access
- "4" → "Write" access

Function code	Access type	Register in accordance with "Modbus Applications Protocol Specification"	Register in accordance with "Modicon Modbus Protocol Reference Guide"
03 04 23	Read	XXXX Example: mass flow = 2007	3XXXX Example: mass flow = 32007
06 16 23	Write	XXXX Example: reset totalizer = 6401	4XXXX Example: reset totalizer = 46401

6.2 Overview of the operating menu

The following table provides an overview of the menu structure of the operating menu and its parameters. The page reference indicates where the associated description of the submenu or parameter can be found.

Guidance	→ 134
► Commissioning	→ 134
Device tag	→ 134
Serial number	→ 134
Firmware version	→ 134
Device name	→ 135
Select medium	→ 135
Select gas type	→ 135
Reference sound velocity	→ 135
Temperature coefficient sound velocity	→ 135
Pressure compensation	→ 135
Pressure value	→ 135
Mass flow unit	→ 135
Mass unit	→ 136
Volume flow unit	→ 137
Volume unit	→ 138
Corrected volume flow unit	→ 139
Corrected volume unit	→ 139

Density unit	→  140
Reference density unit	→  140
Temperature unit	→  140
Pressure unit	→  140
Assign process variable	→  140
Unit totalizer 1 to n	→  141
Totalizer operation mode	→  141
Failure mode	→  141
Flow damping time	→  141
Low flow cut off	→  141
On value low flow cutoff	→  141
Off value low flow cutoff	→  141
Pressure shock suppression	→  141
Partially filled pipe detection	→  141
Low value partial filled pipe detection	→  141
High value partial filled pipe detection	→  141
Process variable current output	→  142
Current range output	→  142
Lower range value output	→  142
Upper range value output	→  142
Damping current output	→  142
Fixed current	→  142
Failure behavior current output	→  142
Failure current	→  142
Value 1 display	→  142

Value 2 display	→ ⓘ 142
Value 3 display	→ ⓘ 143
Value 4 display	→ ⓘ 143
Display damping	→ ⓘ 143
Time format	→ ⓘ 144
Time zone	→ ⓘ 144
Diagnostics	→ ⓘ 144
▶ Active diagnostics	→ ⓘ 144
Actual diagnostics	→ ⓘ 144
Timestamp	→ ⓘ 144
Previous diagnostics	→ ⓘ 144
Timestamp	→ ⓘ 144
Operating time from restart	→ ⓘ 145
Operating time	→ ⓘ 145
▶ Diagnostic list	→ ⓘ 145
▶ Simulation	→ ⓘ 145
Assign simulation process variable	→ ⓘ 145
Process variable value	→ ⓘ 145
Current output 1 simulation	→ ⓘ 145
Current output value	→ ⓘ 145
Device alarm simulation	→ ⓘ 145
Diagnostic event simulation	→ ⓘ 145

► Heartbeat Technology	→ ⓘ 145
► Diagnostic settings	→ ⓘ 145
► Properties	→ ⓘ 145
Alarm delay	→ ⓘ 145
► Diagnostic configuration	→ ⓘ 146
► Sensor	→ ⓘ 146
Assign behavior of diagnostic no. 046	→ ⓘ 146
Assign behavior of diagnostic no. 140	→ ⓘ 146
Assign behavior of diagnostic no. 144	→ ⓘ 146
► Electronics	→ ⓘ 146
Assign behavior of diagnostic no. 230	→ ⓘ 146
Assign behavior of diagnostic no. 231	→ ⓘ 146
Assign behavior of diagnostic no. 302	→ ⓘ 146
Assign behavior of diagnostic no. 374	→ ⓘ 146
► Configuration	→ ⓘ 146
Assign behavior of diagnostic no. 441	→ ⓘ 146
► Process	→ ⓘ 147
Assign behavior of diagnostic no. 832	→ ⓘ 147
Assign behavior of diagnostic no. 833	→ ⓘ 147
Assign behavior of diagnostic no. 834	→ ⓘ 147
Assign behavior of diagnostic no. 835	→ ⓘ 147
Assign behavior of diagnostic no. 842	→ ⓘ 147
Assign behavior of diagnostic no. 862	→ ⓘ 147
Assign behavior of diagnostic no. 912	→ ⓘ 147
Assign behavior of diagnostic no. 913	→ ⓘ 147

	Assign behavior of diagnostic no. 944	→ ⓘ 147
	Assign behavior of diagnostic no. 948	→ ⓘ 147
Application		→ ⓘ 147
► Measured values		→ ⓘ 147
Mass flow		→ ⓘ 147
Volume flow		→ ⓘ 147
Corrected volume flow		→ ⓘ 147
Density		→ ⓘ 147
Temperature		→ ⓘ 147
► Totalizer		→ ⓘ 148
Totalizer value 1 to n		→ ⓘ 148
Totalizer overflow 1 to n		→ ⓘ 148
► System units		→ ⓘ 148
Mass flow unit		→ ⓘ 148
Mass unit		→ ⓘ 148
Volume flow unit		→ ⓘ 149
Volume unit		→ ⓘ 150
Corrected volume flow unit		→ ⓘ 151
Corrected volume unit		→ ⓘ 151
Density unit		→ ⓘ 152
Reference density unit		→ ⓘ 152
Temperature unit		→ ⓘ 152
Pressure unit		→ ⓘ 152

► Totalizers	→ 152
► Totalizer handling	→ 152
Reset all totalizers	→ 152
► Totalizer 1 to n	→ 153
Assign process variable	→ 153
Unit totalizer 1 to n	→ 153
Totalizer operation mode	→ 153
Control Totalizer 1 to n	→ 153
Preset value 1 to n	→ 153
Failure mode	→ 153
► Sensor	→ 154
► Process parameters	→ 154
Flow damping time	→ 154
Flow override	→ 154
Density damping	→ 154
Temperature damping	→ 154
► Low flow cut off	→ 154
Low flow cut off	→ 154
On value low flow cutoff	→ 154
Off value low flow cutoff	→ 154
► Partially filled pipe detection	→ 154
Partially filled pipe detection	→ 154
Low value partial filled pipe detection	→ 154
High value partial filled pipe detection	→ 154
► Medium settings	→ 155

Select medium	→  155
Select gas type	→  155
Reference sound velocity	→  155
Temperature coefficient sound velocity	→  155
► Two phase flow	→  155
Index inhomogeneous medium	→  155
Cut off inhomogeneous wet gas	→  155
Cut off inhomogeneous liquid	→  155
Gas Fraction Handler	→  155
► External compensation	→  155
Pressure compensation	→  155
Pressure value	→  155
► Corrected volume flow calculation	→  156
Select reference density	→  156
Fixed reference density	→  156
Reference temperature	→  156
Linear expansion coefficient	→  156
Square expansion coefficient	→  156
► Sensor adjustment	→  156
Installation direction	→  156
► Zero point adjustment	→  156
Zero point adjustment control	→  156

Zero point adjustment status	→  156
Progress	→  156
► Process variable adjustment	→  156
Mass flow offset	→  156
Mass flow factor	→  156
Volume flow offset	→  156
Volume flow factor	→  156
Density offset	→  156
Density factor	→  156
Corrected volume flow offset	→  156
Corrected volume flow factor	→  156
Temperature offset	→  156
Temperature factor	→  156
► Calibration	→  157
Nominal diameter	→  157
Calibration factor	→  157
Zero point	→  157
► Current output 1	→  157
Process variable current output	→  157
Measuring mode current output	→  157
Current range output	→  157
Fixed current	→  157
Lower range value output	→  157
Upper range value output	→  157
Damping current output	→  157

Failure behavior current output	→ ⓘ 157
Failure current	→ ⓘ 157
Output current 1	→ ⓘ 157
► Communication	→ ⓘ 158
► Modbus configuration	→ ⓘ 158
Bus address	→ ⓘ 158
Baudrate	→ ⓘ 158
Parity	→ ⓘ 158
Byte order	→ ⓘ 158
Telegram delay	→ ⓘ 158
Failure mode	→ ⓘ 158
Fieldbus writing access	→ ⓘ 158
► Modbus data map	→ ⓘ 158
Scan list register 0 to 15	→ ⓘ 158
► Modbus information	→ ⓘ 158
Device ID	→ ⓘ 158
Device revision	→ ⓘ 158
System	→ ⓘ 159
► Device management	→ ⓘ 159
Device tag	→ ⓘ 159
Locking status	→ ⓘ 159
Configuration counter	→ ⓘ 159
Device reset	→ ⓘ 159
► User management	→ ⓘ 159
User role	→ ⓘ 159

Enter access code	→ ⓘ 159
Reset Maintenance code	→ ⓘ 159
► Define Maintenance code	→ ⓘ 159
Define Maintenance code	→ ⓘ 159
Confirm Maintenance code	→ ⓘ 159
► Connectivity	→ ⓘ 160
► Bluetooth configuration	→ ⓘ 160
Bluetooth	→ ⓘ 160
Communication established	→ ⓘ 160
► Date/time	→ ⓘ 160
Time format	→ ⓘ 160
Time zone	→ ⓘ 160
► Information	→ ⓘ 161
► Device	→ ⓘ 161
Device name	→ ⓘ 161
Device tag	→ ⓘ 161
Serial number	→ ⓘ 161
Order code	→ ⓘ 161
Firmware version	→ ⓘ 161
Extended order code 1	→ ⓘ 161
Extended order code 2	→ ⓘ 161
Extended order code 3	→ ⓘ 161
ENP version	→ ⓘ 161
Manufacturer	→ ⓘ 161

► Sensor electronic module (ISEM)	→ ⓘ 161
Firmware version	→ ⓘ 161
► Display module	→ ⓘ 161
Firmware version	→ ⓘ 161
► Display	→ ⓘ 162
Language	→ ⓘ 162
Value 1 display	→ ⓘ 162
Value 2 display	→ ⓘ 162
Value 3 display	→ ⓘ 162
Value 4 display	→ ⓘ 162
Display damping	→ ⓘ 163
Rotation display	→ ⓘ 163
Brightness	→ ⓘ 163
Color scheme	→ ⓘ 163
► Software configuration	→ ⓘ 163
Activate SW option	→ ⓘ 163
Software option overview	→ ⓘ 163

6.3 Register information

6.3.1 "Guidance" menu

"Commissioning" wizard

Navigation: Guidance → Commissioning					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ ⓘ
Device tag	29243 to 29258	String	Read / Write	Character string comprising numbers, letters and special characters (#32)	8
Serial number	7003 to 7008	String	Read	Character string comprising numbers, letters and special characters (#11)	8
Firmware version	7277 to 7280	String	Read	Character string comprising numbers, letters and special characters (#8)	9

Navigation: Guidance → Commissioning					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Device name	7263 to 7270	String	Read	Character string comprising numbers, letters and special characters (#16)	9
Select medium	2442	Integer	Read / Write	0 = Liquid 1 = Gas	9
Select gas type	5229	Integer	Read / Write	0 = Air 1 = Nitrogen N2 2 = Argon Ar 3 = Helium He 4 = Carbon dioxide CO2 5 = Oxygen O2 6 = Methane CH4 7 = Ammonia NH3 9 = Hydrogen H2 10 = Ethane C2H6 11 = Propane C3H8 12 = Butane C4H10 13 = Chlorine Cl2 14 = Hydrogen chloride HCl 15 = Carbon monoxide CO 16 = Nitrous oxide N2O 17 = Nitrogen oxide NOx 18 = Hydrogen sulfide H2S 19 = Sulfur hexafluoride SF6 20 = Propylene C3H6 21 = Ozone O3 22 = Others 23 = Ethylene C2H4	9
Reference sound velocity	7413 to 7414	Float	Read / Write	1 to 99999.9999 m/s	10
Temperature coefficient sound velocity	7411 to 7412	Float	Read / Write	Positive floating-point number	10
Pressure compensation	5184	Integer	Read / Write	0 = Off 1 = Fixed value	11
Pressure value	5185 to 5186	Float	Read / Write	Positive floating-point number	11
Mass flow unit	2101	Integer	Read / Write	0 = g/s 1 = g/min 2 = g/h 3 = g/d 4 = kg/s 5 = kg/min 6 = kg/h 7 = kg/d 8 = t/s 9 = t/min 10 = t/h 11 = t/d 12 = oz/s 13 = oz/min 14 = oz/h 15 = oz/d 16 = lb/s 17 = lb/min 18 = lb/h 19 = lb/d 20 = STon/s 21 = STon/min 22 = STon/h 23 = STon/d	11

Navigation: Guidance → Commissioning					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Mass unit	2102	Integer	Read / Write	50 = g 51 = kg 52 = t 53 = oz 54 = lb 55 = STon	12

Navigation: Guidance → Commissioning					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Volume flow unit	2103	Integer	Read / Write	0 = cm ³ /s 1 = cm ³ /min 2 = cm ³ /h 3 = cm ³ /d 4 = dm ³ /s 5 = dm ³ /min 6 = dm ³ /h 7 = dm ³ /d 8 = m ³ /s 9 = m ³ /min 10 = m ³ /h 11 = m ³ /d 12 = ml/s 13 = ml/min 14 = ml/h 15 = ml/d 16 = l/s 17 = l/min 18 = l/h 19 = l/d 20 = hl/s 21 = hl/min 22 = hl/h 23 = hl/d 24 = Ml/s 25 = Ml/min 26 = Ml/h 27 = Ml/d 32 = af/s 33 = af/min 34 = af/h 35 = af/d 36 = ft ³ /s 37 = ft ³ /min 38 = ft ³ /h 39 = ft ³ /d 40 = fl oz/s (us) 41 = fl oz/min (us) 42 = fl oz/h (us) 43 = fl oz/d (us) 44 = gal/s (us) 45 = gal/min (us) 46 = gal/h (us) 47 = gal/d (us) 48 = Mgal/s (us) 49 = Mgal/min (us) 50 = Mgal/h (us) 51 = Mgal/d (us) 52 = bbl/s (us;liq.) 53 = bbl/min (us;liq.) 54 = bbl/h (us;liq.) 55 = bbl/d (us;liq.) 56 = bbl/s (us;beer) 57 = bbl/min (us;beer) 58 = bbl/h (us;beer) 59 = bbl/d (us;beer) 60 = bbl/s (us;oil) 61 = bbl/min (us;oil) 62 = bbl/h (us;oil) 63 = bbl/d (us;oil) 64 = bbl/s (us;tank) 65 = bbl/min (us;tank) 66 = bbl/h (us;tank) 67 = bbl/d (us;tank) 68 = gal/s (imp) 69 = gal/min (imp) 70 = gal/h (imp)	12

Navigation: Guidance → Commissioning					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
				71 = gal/d (imp) 72 = Mgal/s (imp) 73 = Mgal/min (imp) 74 = Mgal/h (imp) 75 = Mgal/d (imp) 76 = bbl/s (imp;beer) 77 = bbl/min (imp;beer) 78 = bbl/h (imp;beer) 79 = bbl/d (imp;beer) 80 = bbl/s (imp;oil) 81 = bbl/min (imp;oil) 82 = bbl/h (imp;oil) 83 = bbl/d (imp;oil) 88 = kgal/s (us) 89 = kgal/min (us) 90 = kgal/h (us) 91 = kgal/d (us) 92 = MMft ³ /s 93 = MMft ³ /min 94 = MMft ³ /h 96 = Mft ³ /d	
Volume unit	2104	Integer	Read / Write	0 = cm ³ 1 = dm ³ 2 = m ³ 3 = ml 4 = l 5 = hl 6 = Ml Mega 8 = af 9 = ft ³ 10 = fl oz (us) 11 = gal (us) 12 = Mgal (us) 13 = bbl (us;liq.) 14 = bbl (us;beer) 15 = bbl (us;oil) 16 = bbl (us;tank) 17 = gal (imp) 18 = Mgal (imp) 19 = bbl (imp;beer) 20 = bbl (imp;oil) 22 = kgal (us) 23 = Mft ³	13

Navigation: Guidance → Commissioning					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Corrected volume flow unit	2105	Integer	Read / Write	0 = NI/s 1 = NI/min 2 = NI/h 3 = NI/d 4 = Nm ³ /s 5 = Nm ³ /min 6 = Nm ³ /h 7 = Nm ³ /d 8 = Sm ³ /s 9 = Sm ³ /min 10 = Sm ³ /h 11 = Sm ³ /d 12 = Sft ³ /s 13 = Sft ³ /min 14 = Sft ³ /h 15 = Sft ³ /d 16 = Sgal/s (us) 17 = Sgal/min (us) 18 = Sgal/h (us) 19 = Sgal/d (us) 20 = Sbbbl/s (us;liq.) 21 = Sbbbl/min (us;liq.) 22 = Sbbbl/h (us;liq.) 23 = Sbbbl/d (us;liq.) 24 = Sgal/s (imp) 25 = Sgal/min (imp) 26 = Sgal/h (imp) 27 = Sgal/d (imp) 28 = MMSft ³ /s 29 = MMSft ³ /min 30 = MMSft ³ /h 31 = MMSft ³ /d 32 = Sbbbl/s (us;oil) 33 = Sbbbl/min (us;oil) 34 = Sbbbl/h (us;oil) 35 = Sbbbl/d (us;oil) 36 = Nhl/s 37 = Nhl/min 38 = Nhl/h 39 = Nhl/d 40 = Sl/s 41 = Sl/min 42 = Sl/h 43 = Sl/d	14
Corrected volume unit	2106	Integer	Read / Write	100 = NI 101 = Nm ³ 102 = Sm ³ 103 = Sft ³ 104 = Sl 105 = Sgal (us) 106 = Sbbbl (us;liq.) 107 = Sgal (imp) 108 = Sbbbl (us;oil) 109 = MMSft ³ 110 = Nhl	14

Navigation: Guidance → Commissioning					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Density unit	2107	Integer	Read / Write	0 = g/cm ³ 2 = kg/dm ³ 3 = kg/l 4 = kg/m ³ 11 = lb/ft ³ 12 = lb/gal (us) 13 = lb/bbl (us;liq.) 14 = lb/bbl (us;beer) 15 = lb/bbl (us;oil) 16 = lb/bbl (us;tank) 17 = lb/gal (imp) 18 = lb/bbl (imp;beer) 19 = lb/bbl (imp;oil) 21 = g/m ³ 22 = g/ml 23 = °API	15
Reference density unit	2108	Integer	Read / Write	0 = g/Scm ³ 1 = kg/Nl 2 = kg/Nm ³ 3 = kg/Sm ³ 4 = lb/Sft ³ 6 = RD15°C 7 = RD20°C 8 = RD60°F	15
Temperature unit	2109	Integer	Read / Write	0 = °C 1 = K 2 = °F 3 = °R	15
Pressure unit	2130	Integer	Read / Write	0 = bar 1 = psi a 2 = bar g 3 = psi g 4 = Pa a 5 = kPa a 6 = MPa a 7 = Pa g 8 = kPa g 9 = MPa g	16
Assign process variable	2601	Integer	Read / Write	0 = Off 1 = Mass flow 2 = Volume flow 3 = Corrected volume flow	16

Navigation: Guidance → Commissioning					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Unit totalizer 1 to n	1: 4604 2: 4605 3: 4606	Integer	Read / Write	0 = cm ³ * 1 = dm ³ * 2 = m ³ * 3 = ml * 4 = l * 5 = hl * 6 = Ml Mega * 8 = af * 9 = ft ³ * 10 = fl oz (us) * 11 = gal (us) * 12 = Mgal (us) * 13 = bbl (us;liq.) * 14 = bbl (us;beer) * 15 = bbl (us;oil) * 16 = bbl (us;tank) * 17 = gal (imp) * 18 = Mgal (imp) * 19 = bbl (imp;beer) * 20 = bbl (imp;oil) * 22 = kgal (us) * 23 = Mft ³ * 50 = g * 51 = kg * 52 = t * 53 = oz * 54 = lb * 55 = STon * 100 = Nl * 101 = Nm ³ * 102 = Sm ³ * 103 = Sft ³ * 104 = Sl * 105 = Sgal (us) * 106 = Sbbbl (us;liq.) * 107 = Sgal (imp) * 108 = Sbbbl (us;oil) * 109 = MMSft ³ * 110 = Nhl * 251 = None *	16
Totalizer operation mode	2605	Integer	Read / Write	0 = Net flow total 1 = Forward flow total 2 = Reverse flow total	18
Failure mode	2606	Integer	Read / Write	0 = Stop 1 = Actual value 2 = Last valid value	18
Flow damping time	35954 to 35955	Float	Read / Write	0 to 99.9 s	19
Low flow cut off	5101	Integer	Read / Write	0 = Off 1 = Mass flow 2 = Volume flow 3 = Corrected volume flow	20
On value low flow cutoff	5138 to 5139	Float	Read / Write	Positive floating-point number	21
Off value low flow cutoff	5104 to 5105	Float	Read / Write	0 to 100.0 %	21
Pressure shock suppression	5140 to 5141	Float	Read / Write	0 to 100 s	19
Partially filled pipe detection	5106	Integer	Read / Write	0 = Off 4 = Density 5 = Calculated reference density	22
Low value partial filled pipe detection	5110 to 5111	Float	Read / Write	Signed floating-point number	22
High value partial filled pipe detection	5112 to 5113	Float	Read / Write	Signed floating-point number	22

Navigation: Guidance → Commissioning					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Process variable current output	5927	Integer	Read / Write	0 = Off * 1 = Mass flow 2 = Volume flow 3 = Corrected volume flow 4 = Density * 7 = Temperature 8 = Oscillation amplitude 0 * 9 = Signal asymmetry 32 = Exciter current 0 39 = Electronics temperature 48 = Oscillation frequency 0 63 = Oscillation damping 0 67 = Oscillation damping fluctuation 0 * 68 = Frequency fluctuation 0 * 81 = HBSI * 184 = Index inhomogeneous medium	23
Current range output	5923	Integer	Read / Write	0 = 4...20 mA (4... 20.5 mA) 1 = 4...20 mA US (3.9...20.8 mA) 2 = 4...20 mA NE (3.8...20.5 mA) 4 = Fixed value	23
Lower range value output	6195 to 6196	Float	Read / Write	Signed floating-point number	24
Upper range value output	5915 to 5916	Float	Read / Write	Signed floating-point number	26
Damping current output	5903 to 5904	Float	Read / Write	0.0 to 999.9 s	26
Fixed current	5987 to 5988	Float	Read / Write	3.59 to 21.5 mA	26
Failure behavior current output	5911	Integer	Read / Write	0 = Min. 1 = Max. 4 = Actual value 5 = Last valid value 6 = Fixed value	27
Failure current	5979 to 5980	Float	Read / Write	3.59 to 21.5 mA	27
Value 1 display	34918	Integer	Read / Write	1 = Mass flow 2 = Volume flow 3 = Corrected volume flow 4 = Density * 7 = Temperature 16 = Totalizer 1 17 = Totalizer 2 18 = Totalizer 3 39 = Electronics temperature 184 = Index inhomogeneous medium	28
Value 2 display	34919	Integer	Read / Write	1 = Mass flow 2 = Volume flow 3 = Corrected volume flow 4 = Density * 7 = Temperature 16 = Totalizer 1 17 = Totalizer 2 18 = Totalizer 3 39 = Electronics temperature 184 = Index inhomogeneous medium 251 = None	28

Navigation: Guidance → Commissioning					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Value 3 display	34922	Integer	Read / Write	1 = Mass flow 2 = Volume flow 3 = Corrected volume flow 4 = Density* 7 = Temperature 16 = Totalizer 1 17 = Totalizer 2 18 = Totalizer 3 39 = Electronics temperature 184 = Index inhomogeneous medium 251 = None	29
Value 4 display	34923	Integer	Read / Write	1 = Mass flow 2 = Volume flow 3 = Corrected volume flow 4 = Density* 7 = Temperature 16 = Totalizer 1 17 = Totalizer 2 18 = Totalizer 3 39 = Electronics temperature 184 = Index inhomogeneous medium 251 = None	29
Display damping	27602 to 27603	Float	Read / Write	0.0 to 999.9 s	30

Navigation: Guidance → Commissioning					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Time format	2150	Integer	Read / Write	12 = 12 h AM/PM 24 = 24 h	30
Time zone	27339	Integer	Read / Write	0 = UTC 00:00 1 = UTC+01:00 2 = UTC+02:00 3 = UTC+03:00 4 = UTC+04:00 5 = UTC+05:00 6 = UTC+06:00 7 = UTC+07:00 8 = UTC+08:00 9 = UTC+09:00 10 = UTC+10:00 11 = UTC+11:00 12 = UTC+12:00 13 = UTC+13:00 14 = UTC+14:00 35 = UTC+03:30 45 = UTC+04:30 55 = UTC+05:30 57 = UTC+05:45 65 = UTC+06:30 87 = UTC+08:45 95 = UTC+09:30 105 = UTC+10:30 127 = UTC+12:45 135 = UTC-03:30 195 = UTC-09:30 201 = UTC-01:00 202 = UTC-02:00 203 = UTC-03:00 204 = UTC-04:00 205 = UTC-05:00 206 = UTC-06:00 207 = UTC-07:00 208 = UTC-08:00 209 = UTC-09:00 210 = UTC-10:00 211 = UTC-11:00 212 = UTC-12:00	30

- * Visibility depends on order options or device settings
- * Visibility depends on order options or device settings
- * Visibility depends on order options or device settings

6.3.2 "Diagnostics" menu

"Active diagnostics" submenu

Navigation: Diagnostics → Active diagnostics					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Actual diagnostics	2732	Integer	Read	Positive integer	33
Timestamp	29726	String	Read	Days (d), hours (h), minutes (m), seconds (s)	33
Previous diagnostics	2734	Integer	Read	Positive integer	33
Timestamp	29715	String	Read	Days (d), hours (h), minutes (m), seconds (s)	34

Navigation: Diagnostics → Active diagnostics					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Operating time from restart	2624	String	Read	Days (d), hours (h), minutes (m), seconds (s)	34
Operating time	2631	String	Read	Days (d), hours (h), minutes (m), seconds (s)	34

"Diagnostic list" submenu

"Simulation" submenu

Navigation: Diagnostics → Simulation					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Assign simulation process variable	6813	Integer	Read / Write	0 = Off 1 = Mass flow 2 = Volume flow 3 = Corrected volume flow 4 = Density * 7 = Temperature	38
Process variable value	6814 to 6815	Float	Read / Write	Signed floating-point number	39
Current output 1 simulation	5939	Integer	Read / Write	0 = Off 1 = On	39
Current output value	5995 to 5996	Float	Read / Write	3.59 to 21.5 mA	39
Device alarm simulation	6812	Integer	Read / Write	0 = Off 1 = On	40
Diagnostic event simulation	4259	Integer	Read / Write	0 = Off	40

* Visibility depends on order options or device settings

"Heartbeat Technology" submenu

"Diagnostic settings" submenu

"Properties" submenu

Navigation: Diagnostics → Diagnostic settings → Properties					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Alarm delay	6808 to 6809	Float	Read / Write	0 to 60 s	42

*"Diagnostic configuration" submenu**"Sensor" submenu*

Navigation: Diagnostics → Diagnostic settings → Diagnostic configuration → Sensor					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Assign behavior of diagnostic no. 046	27554	Integer	Read / Write	0 = Off 1 = Logbook entry only 2 = Warning 3 = Alarm	43
Assign behavior of diagnostic no. 140	27622	Integer	Read / Write	0 = Off 1 = Logbook entry only 2 = Warning 3 = Alarm	43
Assign behavior of diagnostic no. 144	27555	Integer	Read / Write	0 = Off 1 = Logbook entry only 2 = Warning 3 = Alarm	44

"Electronics" submenu

Navigation: Diagnostics → Diagnostic settings → Diagnostic configuration → Electronics					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Assign behavior of diagnostic no. 230	27632	Integer	Read / Write	1 = Logbook entry only 2 = Warning 3 = Alarm	45
Assign behavior of diagnostic no. 231	28535	Integer	Read / Write	1 = Logbook entry only 2 = Warning 3 = Alarm	45
Assign behavior of diagnostic no. 302	6484	Integer	Read / Write	0 = Off 1 = Logbook entry only 2 = Warning	45
Assign behavior of diagnostic no. 374	27553	Integer	Read / Write	0 = Off 1 = Logbook entry only 2 = Warning 3 = Alarm	45

"Configuration" submenu

Navigation: Diagnostics → Diagnostic settings → Diagnostic configuration → Configuration					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Assign behavior of diagnostic no. 441	4742	Integer	Read / Write	0 = Off 1 = Logbook entry only 2 = Warning 3 = Alarm	46

"Process" submenu

Navigation: Diagnostics → Diagnostic settings → Diagnostic configuration → Process					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Assign behavior of diagnostic no. 832	6440	Integer	Read / Write	0 = Off 1 = Logbook entry only 2 = Warning 3 = Alarm	47
Assign behavior of diagnostic no. 833	6439	Integer	Read / Write	0 = Off 1 = Logbook entry only 2 = Warning 3 = Alarm	48
Assign behavior of diagnostic no. 834	6438	Integer	Read / Write	0 = Off 1 = Logbook entry only 2 = Warning 3 = Alarm	48
Assign behavior of diagnostic no. 835	6437	Integer	Read / Write	0 = Off 1 = Logbook entry only 2 = Warning 3 = Alarm	49
Assign behavior of diagnostic no. 842	9661	Integer	Read / Write	0 = Off 1 = Logbook entry only 2 = Warning 3 = Alarm	49
Assign behavior of diagnostic no. 862	6441	Integer	Read / Write	0 = Off 1 = Logbook entry only 2 = Warning 3 = Alarm	50
Assign behavior of diagnostic no. 912	27552	Integer	Read / Write	0 = Off 1 = Logbook entry only 2 = Warning 3 = Alarm	50
Assign behavior of diagnostic no. 913	27551	Integer	Read / Write	0 = Off 1 = Logbook entry only 2 = Warning 3 = Alarm	51
Assign behavior of diagnostic no. 944	27557	Integer	Read / Write	0 = Off 1 = Logbook entry only 2 = Warning 3 = Alarm	51
Assign behavior of diagnostic no. 948	27556	Integer	Read / Write	0 = Off 1 = Logbook entry only 2 = Warning 3 = Alarm	52

6.3.3 "Application" menu**"Measured values" submenu**

Navigation: Application → Measured values					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Mass flow	2007 to 2008	Float	Read	Signed floating-point number	53
Volume flow	2009 to 2010	Float	Read	Signed floating-point number	54
Corrected volume flow	35946 to 35947	Float	Read	Signed floating-point number	54
Density	35948 to 35949	Float	Read	Positive floating-point number	54
Temperature	2017 to 2018	Float	Read	Positive floating-point number	54

"Totalizer" submenu

Navigation: Application → Measured values → Totalizer					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Totalizer value 1 to n	1: 2610 to 2611 2: 2810 to 2811 3: 3010 to 3011	Float	Read	Signed floating-point number	55
Totalizer overflow 1 to n	1: 2612 to 2613 2: 2812 to 2813 3: 3012 to 3013	Float	Read	-32 000.0 to 32 000.0	55

"System units" submenu

Navigation: Application → System units					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Mass flow unit	2101	Integer	Read / Write	0 = g/s 1 = g/min 2 = g/h 3 = g/d 4 = kg/s 5 = kg/min 6 = kg/h 7 = kg/d 8 = t/s 9 = t/min 10 = t/h 11 = t/d 12 = oz/s 13 = oz/min 14 = oz/h 15 = oz/d 16 = lb/s 17 = lb/min 18 = lb/h 19 = lb/d 20 = STon/s 21 = STon/min 22 = STon/h 23 = STon/d	57
Mass unit	2102	Integer	Read / Write	50 = g 51 = kg 52 = t 53 = oz 54 = lb 55 = STon	58

Navigation: Application → System units					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Volume flow unit	2103	Integer	Read / Write	0 = cm ³ /s 1 = cm ³ /min 2 = cm ³ /h 3 = cm ³ /d 4 = dm ³ /s 5 = dm ³ /min 6 = dm ³ /h 7 = dm ³ /d 8 = m ³ /s 9 = m ³ /min 10 = m ³ /h 11 = m ³ /d 12 = ml/s 13 = ml/min 14 = ml/h 15 = ml/d 16 = l/s 17 = l/min 18 = l/h 19 = l/d 20 = hl/s 21 = hl/min 22 = hl/h 23 = hl/d 24 = Ml/s 25 = Ml/min 26 = Ml/h 27 = Ml/d 32 = af/s 33 = af/min 34 = af/h 35 = af/d 36 = ft ³ /s 37 = ft ³ /min 38 = ft ³ /h 39 = ft ³ /d 40 = fl oz/s (us) 41 = fl oz/min (us) 42 = fl oz/h (us) 43 = fl oz/d (us) 44 = gal/s (us) 45 = gal/min (us) 46 = gal/h (us) 47 = gal/d (us) 48 = Mgal/s (us) 49 = Mgal/min (us) 50 = Mgal/h (us) 51 = Mgal/d (us) 52 = bbl/s (us;liq.) 53 = bbl/min (us;liq.) 54 = bbl/h (us;liq.) 55 = bbl/d (us;liq.) 56 = bbl/s (us;beer) 57 = bbl/min (us;beer) 58 = bbl/h (us;beer) 59 = bbl/d (us;beer) 60 = bbl/s (us;oil) 61 = bbl/min (us;oil) 62 = bbl/h (us;oil) 63 = bbl/d (us;oil) 64 = bbl/s (us;tank) 65 = bbl/min (us;tank) 66 = bbl/h (us;tank) 67 = bbl/d (us;tank) 68 = gal/s (imp) 69 = gal/min (imp) 70 = gal/h (imp)	58

Navigation: Application → System units					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
				71 = gal/d (imp) 72 = Mgal/s (imp) 73 = Mgal/min (imp) 74 = Mgal/h (imp) 75 = Mgal/d (imp) 76 = bbl/s (imp;beer) 77 = bbl/min (imp;beer) 78 = bbl/h (imp;beer) 79 = bbl/d (imp;beer) 80 = bbl/s (imp;oil) 81 = bbl/min (imp;oil) 82 = bbl/h (imp;oil) 83 = bbl/d (imp;oil) 88 = kgal/s (us) 89 = kgal/min (us) 90 = kgal/h (us) 91 = kgal/d (us) 92 = MMft ³ /s 93 = MMft ³ /min 94 = MMft ³ /h 96 = Mft ³ /d	
Volume unit	2104	Integer	Read / Write	0 = cm ³ 1 = dm ³ 2 = m ³ 3 = ml 4 = l 5 = hl 6 = Ml Mega 8 = af 9 = ft ³ 10 = fl oz (us) 11 = gal (us) 12 = Mgal (us) 13 = bbl (us;liq.) 14 = bbl (us;beer) 15 = bbl (us;oil) 16 = bbl (us;tank) 17 = gal (imp) 18 = Mgal (imp) 19 = bbl (imp;beer) 20 = bbl (imp;oil) 22 = kgal (us) 23 = Mft ³	59

Navigation: Application → System units					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Corrected volume flow unit	2105	Integer	Read / Write	0 = NI/s 1 = NI/min 2 = NI/h 3 = NI/d 4 = Nm ³ /s 5 = Nm ³ /min 6 = Nm ³ /h 7 = Nm ³ /d 8 = Sm ³ /s 9 = Sm ³ /min 10 = Sm ³ /h 11 = Sm ³ /d 12 = Sft ³ /s 13 = Sft ³ /min 14 = Sft ³ /h 15 = Sft ³ /d 16 = Sgal/s (us) 17 = Sgal/min (us) 18 = Sgal/h (us) 19 = Sgal/d (us) 20 = Sbbbl/s (us;liq.) 21 = Sbbbl/min (us;liq.) 22 = Sbbbl/h (us;liq.) 23 = Sbbbl/d (us;liq.) 24 = Sgal/s (imp) 25 = Sgal/min (imp) 26 = Sgal/h (imp) 27 = Sgal/d (imp) 28 = MMSft ³ /s 29 = MMSft ³ /min 30 = MMSft ³ /h 31 = MMSft ³ /d 32 = Sbbbl/s (us;oil) 33 = Sbbbl/min (us;oil) 34 = Sbbbl/h (us;oil) 35 = Sbbbl/d (us;oil) 36 = Nhl/s 37 = Nhl/min 38 = Nhl/h 39 = Nhl/d 40 = Sl/s 41 = Sl/min 42 = Sl/h 43 = Sl/d	60
Corrected volume unit	2106	Integer	Read / Write	100 = NI 101 = Nm ³ 102 = Sm ³ 103 = Sft ³ 104 = Sl 105 = Sgal (us) 106 = Sbbbl (us;liq.) 107 = Sgal (imp) 108 = Sbbbl (us;oil) 109 = MMSft ³ 110 = Nhl	60

Navigation: Application → System units					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Density unit	2107	Integer	Read / Write	0 = g/cm ³ 2 = kg/dm ³ 3 = kg/l 4 = kg/m ³ 11 = lb/ft ³ 12 = lb/gal (us) 13 = lb/bbl (us;liq.) 14 = lb/bbl (us;beer) 15 = lb/bbl (us;oil) 16 = lb/bbl (us;tank) 17 = lb/gal (imp) 18 = lb/bbl (imp;beer) 19 = lb/bbl (imp;oil) 21 = g/m ³ 22 = g/ml 23 = °API	61
Reference density unit	2108	Integer	Read / Write	0 = g/Scm ³ 1 = kg/Nl 2 = kg/Nm ³ 3 = kg/Sm ³ 4 = lb/Sft ³ 6 = RD15°C 7 = RD20°C 8 = RD60°F	61
Temperature unit	2109	Integer	Read / Write	0 = °C 1 = K 2 = °F 3 = °R	61
Pressure unit	2130	Integer	Read / Write	0 = bar 1 = psi a 2 = bar g 3 = psi g 4 = Pa a 5 = kPa a 6 = MPa a 7 = Pa g 8 = kPa g 9 = MPa g	62

"Totalizers" submenu*"Totalizer handling" submenu*

Navigation: Application → Totalizers → Totalizer handling					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Reset all totalizers	2609	Integer	Read / Write	0 = Cancel 1 = Reset + totalize	63

"Totalizer 1 to n" submenu

Navigation: Application → Totalizers → Totalizer 1 to n					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Assign process variable	1: 2601 2: 2801 3: 3001	Integer	Read / Write	0 = Off 1 = Mass flow 2 = Volume flow 3 = Corrected volume flow	64
Unit totalizer 1 to n	1: 4604 2: 4605 3: 4606	Integer	Read / Write	0 = cm ³ * 1 = dm ³ * 2 = m ³ * 3 = ml * 4 = l * 5 = hl * 6 = Ml Mega * 8 = af * 9 = ft ³ * 10 = fl oz (us) * 11 = gal (us) * 12 = Mgal (us) * 13 = bbl (us;liq.) * 14 = bbl (us;beer) * 15 = bbl (us;oil) * 16 = bbl (us;tank) * 17 = gal (imp) * 18 = Mgal (imp) * 19 = bbl (imp;beer) * 20 = bbl (imp;oil) * 22 = kgal (us) * 23 = Mft ³ * 50 = g * 51 = kg * 52 = t * 53 = oz * 54 = lb * 55 = STon * 100 = Nl * 101 = Nm ³ * 102 = Sm ³ * 103 = Sft ³ * 104 = Sl * 105 = Sgal (us) * 106 = Sbbl (us;liq.) * 107 = Sgal (imp) * 108 = Sbbl (us;oil) * 109 = MMSft ³ * 110 = Nhl * 251 = None *	64
Totalizer operation mode	1: 2605 2: 2805 3: 3005	Integer	Read / Write	0 = Net flow total 1 = Forward flow total 2 = Reverse flow total	65
Control Totalizer 1 to n	1: 2608 2: 2808 3: 3008	Integer	Read / Write	0 = Totalize 1 = Reset + totalize 2 = Preset + hold 3 = Reset + hold 5 = Hold	66
Preset value 1 to n	1: 2590 to 2591 2: 2592 to 2593 3: 2594 to 2595	Float	Read / Write	Signed floating-point number	66
Failure mode	1: 2606 2: 2806 3: 3006	Integer	Read / Write	0 = Stop 1 = Actual value 2 = Last valid value	67

* Visibility depends on order options or device settings

"Sensor" submenu*"Process parameters" submenu*

Navigation: Application → Sensor → Process parameters					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Flow damping time	35954 to 35955	Float	Read / Write	0 to 99.9 s	69
Flow override	5503	Integer	Read / Write	0 = Off 1 = On	69
Density damping	35956 to 35957	Float	Read / Write	0 to 999.9 s	69
Temperature damping	37236 to 37237	Float	Read / Write	0 to 999.9 s	70

"Low flow cut off" submenu

Navigation: Application → Sensor → Low flow cut off					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Low flow cut off	5101	Integer	Read / Write	0 = Off 1 = Mass flow 2 = Volume flow 3 = Corrected volume flow	70
On value low flow cutoff	5138 to 5139	Float	Read / Write	Positive floating-point number	71
Off value low flow cutoff	5104 to 5105	Float	Read / Write	0 to 100.0 %	71

"Partially filled pipe detection" submenu

Navigation: Application → Sensor → Partially filled pipe detection					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Partially filled pipe detection	5106	Integer	Read / Write	0 = Off 4 = Density 5 = Calculated reference density	72
Low value partial filled pipe detection	5110 to 5111	Float	Read / Write	Signed floating-point number	72
High value partial filled pipe detection	5112 to 5113	Float	Read / Write	Signed floating-point number	72

"Medium settings" submenu

Navigation: Application → Sensor → Medium settings					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Select medium	2442	Integer	Read / Write	0 = Liquid 1 = Gas	73
Select gas type	5229	Integer	Read / Write	0 = Air 1 = Nitrogen N2 2 = Argon Ar 3 = Helium He 4 = Carbon dioxide CO2 5 = Oxygen O2 6 = Methane CH4 7 = Ammonia NH3 9 = Hydrogen H2 10 = Ethane C2H6 11 = Propane C3H8 12 = Butane C4H10 13 = Chlorine Cl2 14 = Hydrogen chloride HCl 15 = Carbon monoxide CO 16 = Nitrous oxide N2O 17 = Nitrogen oxide NOx 18 = Hydrogen sulfide H2S 19 = Sulfur hexafluoride SF6 20 = Propylene C3H6 21 = Ozone O3 22 = Others 23 = Ethylene C2H4	73
Reference sound velocity	7413 to 7414	Float	Read / Write	1 to 99999.9999 m/s	74
Temperature coefficient sound velocity	7411 to 7412	Float	Read / Write	Positive floating-point number	74

"Two phase flow" submenu

Navigation: Application → Sensor → Two phase flow					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Index inhomogeneous medium	34301 to 34302	Float	Read	Signed floating-point number	76
Cut off inhomogeneous wet gas	34852 to 34853	Float	Read / Write	Positive floating-point number	76
Cut off inhomogeneous liquid	34850 to 34851	Float	Read / Write	Positive floating-point number	76
Gas Fraction Handler	34303	Integer	Read / Write	0 = Off 1 = Moderate 2 = Powerful	75

"External compensation" submenu

Navigation: Application → Sensor → External compensation					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Pressure compensation	5184	Integer	Read / Write	0 = Off 1 = Fixed value	77
Pressure value	5185 to 5186	Float	Read / Write	Positive floating-point number	77

"Corrected volume flow calculation" submenu

Navigation: Application → Sensor → Corrected volume flow calculation					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Select reference density	5129	Integer	Read / Write	0 = Calculated reference density 1 = Fixed reference density	78
Fixed reference density	5130 to 5131	Float	Read / Write	Positive floating-point number	78
Reference temperature	5136 to 5137	Float	Read / Write	-273.15 to 99 999 °C	78
Linear expansion coefficient	5132 to 5133	Float	Read / Write	Signed floating-point number	79
Square expansion coefficient	5134 to 5135	Float	Read / Write	0 to 1 1/K ²	79

"Sensor adjustment" submenu

Navigation: Application → Sensor → Sensor adjustment					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Installation direction	5501	Integer	Read / Write	0 = Forward flow 1 = Reverse flow	80

"Zero point adjustment" submenu

Navigation: Application → Sensor → Sensor adjustment → Zero point adjustment					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Zero point adjustment control	5121	Integer	Read / Write	0 = Cancel 1 = Start	80
Zero point adjustment status	10237	Integer	Read	2 = Zero point adjust failure 5 = Ok 8 = Busy	81
Progress	6797	Integer	Read	0 to 100 %	81

"Process variable adjustment" submenu

Navigation: Application → Sensor → Sensor adjustment → Process variable adjustment					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Mass flow offset	27663 to 27664	Float	Read / Write	Signed floating-point number	82
Mass flow factor	27665 to 27666	Float	Read / Write	Positive floating-point number	82
Volume flow offset	27667 to 27668	Float	Read / Write	Signed floating-point number	82
Volume flow factor	27669 to 27670	Float	Read / Write	Positive floating-point number	83
Density offset	5769 to 5770	Float	Read / Write	Signed floating-point number	83
Density factor	5765 to 5766	Float	Read / Write	Positive floating-point number	83
Corrected volume flow offset	27659 to 27660	Float	Read / Write	Signed floating-point number	83
Corrected volume flow factor	27657 to 27658	Float	Read / Write	Positive floating-point number	84
Temperature offset	6458 to 6459	Float	Read / Write	Signed floating-point number	84
Temperature factor	6452 to 6453	Float	Read / Write	Positive floating-point number	84

"Calibration" submenu

Navigation: Application → Sensor → Calibration					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Nominal diameter	2048 to 2057	String	Read	Character string comprising numbers, letters and special characters (#20)	85
Calibration factor	7513 to 7514	Float	Read	Signed floating-point number	85
Zero point	7527 to 7528	Float	Read / Write	Signed floating-point number	85

"Current output 1" submenu

Navigation: Application → Current output 1					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Process variable current output	5927	Integer	Read / Write	0 = Off * 1 = Mass flow 2 = Volume flow 3 = Corrected volume flow 4 = Density * 7 = Temperature 8 = Oscillation amplitude 0 * 9 = Signal asymmetry 32 = Exciter current 0 39 = Electronics temperature 48 = Oscillation frequency 0 63 = Oscillation damping 0 67 = Oscillation damping fluctuation 0 * 68 = Frequency fluctuation 0 * 81 = HBSI * 184 = Index inhomogeneous medium	87
Measuring mode current output	5899	Integer	Read / Write	0 = Forward flow 2 = Reverse flow compensation 13 = Forward/Reverse flow *	88
Current range output	5923	Integer	Read / Write	0 = 4...20 mA (4... 20.5 mA) 1 = 4...20 mA US (3.9...20.8 mA) 2 = 4...20 mA NE (3.8...20.5 mA) 4 = Fixed value	92
Fixed current	5987 to 5988	Float	Read / Write	3.59 to 21.5 mA	93
Lower range value output	6195 to 6196	Float	Read / Write	Signed floating-point number	93
Upper range value output	5915 to 5916	Float	Read / Write	Signed floating-point number	95
Damping current output	5903 to 5904	Float	Read / Write	0.0 to 999.9 s	95
Failure behavior current output	5911	Integer	Read / Write	0 = Min. 1 = Max. 4 = Actual value 5 = Last valid value 6 = Fixed value	96
Failure current	5979 to 5980	Float	Read / Write	3.59 to 21.5 mA	96
Output current 1	5931 to 5932	Float	Read	3.59 to 21.5 mA	97

* Visibility depends on order options or device settings

"Communication" submenu*"Modbus configuration" submenu*

Navigation: Application → Communication → Modbus configuration					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Bus address	4910	Integer	Read / Write	1 to 247	98
Baudrate	4912	Integer	Read / Write	0 = 1200 BAUD 1 = 2400 BAUD 2 = 4800 BAUD 3 = 9600 BAUD 4 = 19200 BAUD 5 = 38400 BAUD 6 = 57600 BAUD 7 = 115200 BAUD	99
Parity	4914	Integer	Read / Write	0 = Even 1 = Odd 2 = None / 2 stop bits 3 = None / 1 stop bit	99
Byte order	4915	Integer	Read / Write	0 = 0-1-2-3 1 = 3-2-1-0 2 = 2-3-0-1 3 = 1-0-3-2	100
Telegram delay	4916 to 4917	Float	Read / Write	0 to 100 ms	100
Failure mode	4920	Integer	Read / Write	1 = Last valid value 255 = NaN value	100
Fieldbus writing access	6807	Integer	Read / Write	0 = Read + write 1 = Read only	101

"Modbus data map" submenu

Navigation: Application → Communication → Modbus data map					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Scan list register 0 to 15	0: 5001 1: 5002 2: 5003 3: 5004 4: 5005 5: 5006 6: 5007 7: 5008 8: 5009 9: 5010 10: 5011 11: 5012 12: 5013 13: 5014 14: 5015 15: 5016	Integer	Read / Write	0 to 65 535	101

"Modbus information" submenu

Navigation: Application → Communication → Modbus information					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Device ID	2547	Integer	Read	0 to 65 535	102
Device revision	4481	Integer	Read	0 to 65 535	102

6.3.4 "System" menu

"Device management" submenu

Navigation: System → Device management					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Device tag	29243 to 29258	String	Read / Write	Character string comprising numbers, letters and special characters (#32)	104
Locking status	4918	Integer	Read	256 = Hardware locked 512 = Temporarily locked	104
Configuration counter	4818	Integer	Read	0 to 65 535	105
Device reset	6817	Integer	Read / Write	0 = Cancel 1 = Restart device 2 = To delivery settings 5 = Delete powerfail data 21 = Delete T-DAT 22 = Reset faulty parameters 23 = Delete delivery settings 24 = Delete flash file system 25 = Restore S-DAT backup * 35 = Restore T-DAT backup * 36 = Create T-DAT backup	105

* Visibility depends on order options or device settings

"User management" submenu

Navigation: System → User management					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
User role	2178	Integer	Read	0 = Operator 1 = Maintenance 2 = Service 3 = Production 4 = Development	107
Enter access code	2177	Integer	Read / Write	0 to 9999	108
Reset Maintenance code	8880 to 8895	String	Read / Write	Character string comprising numbers, letters and special characters (#32)	108

"Define Maintenance code" wizard

Navigation: System → User management → Define Maintenance code					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Define Maintenance code	29482	Integer	Read / Write	0 to 9999	109
Confirm Maintenance code	29481	Integer	Read / Write	0 to 9999	109

"Connectivity" submenu*"Bluetooth configuration" submenu*

Navigation: System → Connectivity → Bluetooth configuration					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Bluetooth	27662	Integer	Read / Write	0 = Disable 1 = Enable 4 = Not available *	110
Communication established	27927	Integer	Read	0 = Yes 1 = No	110

* Visibility depends on order options or device settings

"Date/time" submenu

Navigation: System → Date/time					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Time format	2150	Integer	Read / Write	12 = 12 h AM/PM 24 = 24 h	111
Time zone	27339	Integer	Read / Write	0 = UTC 00:00 1 = UTC+01:00 2 = UTC+02:00 3 = UTC+03:00 4 = UTC+04:00 5 = UTC+05:00 6 = UTC+06:00 7 = UTC+07:00 8 = UTC+08:00 9 = UTC+09:00 10 = UTC+10:00 11 = UTC+11:00 12 = UTC+12:00 13 = UTC+13:00 14 = UTC+14:00 35 = UTC+03:30 45 = UTC+04:30 55 = UTC+05:30 57 = UTC+05:45 65 = UTC+06:30 87 = UTC+08:45 95 = UTC+09:30 105 = UTC+10:30 127 = UTC+12:45 135 = UTC-03:30 195 = UTC-09:30 201 = UTC-01:00 202 = UTC-02:00 203 = UTC-03:00 204 = UTC-04:00 205 = UTC-05:00 206 = UTC-06:00 207 = UTC-07:00 208 = UTC-08:00 209 = UTC-09:00 210 = UTC-10:00 211 = UTC-11:00 212 = UTC-12:00	111

"Information" submenu*"Device" submenu*

Navigation: System → Information → Device					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Device name	7263 to 7270	String	Read	Character string comprising numbers, letters and special characters (#16)	113
Device tag	2026 to 2041	String	Read	Character string comprising numbers, letters and special characters (#32)	114
Serial number	7003 to 7008	String	Read	Character string comprising numbers, letters and special characters (#11)	114
Order code	2058 to 2067	String	Read	Character string comprising numbers, letters and special characters (#20)	114
Firmware version	7277 to 7280	String	Read	Character string comprising numbers, letters and special characters (#8)	114
Extended order code 1	2212 to 2221	String	Read	Character string comprising numbers, letters and special characters (#20)	115
Extended order code 2	2222 to 2231	String	Read	Character string comprising numbers, letters and special characters (#20)	115
Extended order code 3	2232 to 2241	String	Read	Character string comprising numbers, letters and special characters (#20)	115
ENP version	4003 to 4010	String	Read	Character string comprising numbers, letters and special characters (#16)	115
Manufacturer	8001 to 8016	String	Read	Character string comprising numbers, letters and special characters (#32)	116

"Sensor electronic module (ISEM)" submenu

Navigation: System → Information → Sensor electronic module (ISEM)					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Firmware version	7039	Integer	Read	Positive integer	116

"Display module" submenu

Navigation: System → Information → Display module					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Firmware version	7039	Integer	Read	Positive integer	117

"Display" submenu

Navigation: System → Display					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Language	35001	Integer	Read / Write	0 = English 1 = Deutsch 2 = Français 3 = Español 4 = Italiano 5 = Nederlands 8 = Svenska 10 = Bahasa Indonesia 11 = 日本語 (Japanese) 12 = Portuguesa 13 = Polski 14 = русский язык (Russian) 15 = čeština (Czech) 16 = 中文 (Chinese) 17 = ภาษาไทย (Thai) * 18 = Türkçe 19 = tiếng Việt (Vietnamese) 20 = 한국어 (Korean) 21 = العربية (Arabic) *	118
Value 1 display	34918	Integer	Read / Write	1 = Mass flow 2 = Volume flow 3 = Corrected volume flow 4 = Density * 7 = Temperature 16 = Totalizer 1 17 = Totalizer 2 18 = Totalizer 3 39 = Electronics temperature 184 = Index inhomogeneous medium	119
Value 2 display	34919	Integer	Read / Write	1 = Mass flow 2 = Volume flow 3 = Corrected volume flow 4 = Density * 7 = Temperature 16 = Totalizer 1 17 = Totalizer 2 18 = Totalizer 3 39 = Electronics temperature 184 = Index inhomogeneous medium 251 = None	119
Value 3 display	34922	Integer	Read / Write	1 = Mass flow 2 = Volume flow 3 = Corrected volume flow 4 = Density * 7 = Temperature 16 = Totalizer 1 17 = Totalizer 2 18 = Totalizer 3 39 = Electronics temperature 184 = Index inhomogeneous medium 251 = None	120
Value 4 display	34923	Integer	Read / Write	1 = Mass flow 2 = Volume flow 3 = Corrected volume flow 4 = Density * 7 = Temperature 16 = Totalizer 1 17 = Totalizer 2 18 = Totalizer 3 39 = Electronics temperature 184 = Index inhomogeneous medium 251 = None	120

Navigation: System → Display					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Display damping	27602 to 27603	Float	Read / Write	0.0 to 999.9 s	121
Rotation display	36770	Integer	Read / Write	0 = 0 degree 8 = Auto 9 = 90 degree 18 = 180 degree 27 = 270 degree	121
Brightness	36768 to 36769	Float	Read / Write	0 to 100 %	121
Color scheme	30228	Integer	Read / Write	11 = Light 12 = Dark	121

* Visibility depends on order options or device settings

"Software configuration" submenu

Navigation: System → Software configuration					
Parameter	Register	Data type	Access	Selection / User entry / User interface	→ 
Activate SW option	2795	Integer	Read / Write	Positive integer	122
Software option overview	2902	Integer	Read	1 = Extended HistoROM 256 = Density 16384 = Heartbeat Monitoring 32768 = Heartbeat Verification	122

Index

A

Activate SW option (Parameter)	122
Active diagnostics (Submenu)	33
Actual diagnostics (Parameter)	33
Alarm delay (Parameter)	42
Application (Menu)	53
Assign behavior of diagnostic no. 046 (Parameter)	43
Assign behavior of diagnostic no. 140 (Parameter)	43
Assign behavior of diagnostic no. 144 (Parameter)	44
Assign behavior of diagnostic no. 230 (Parameter)	45
Assign behavior of diagnostic no. 231 (Parameter)	45
Assign behavior of diagnostic no. 302 (Parameter)	45
Assign behavior of diagnostic no. 374 (Parameter)	45
Assign behavior of diagnostic no. 441 (Parameter)	46
Assign behavior of diagnostic no. 832 (Parameter)	47
Assign behavior of diagnostic no. 833 (Parameter)	48
Assign behavior of diagnostic no. 834 (Parameter)	48
Assign behavior of diagnostic no. 835 (Parameter)	49
Assign behavior of diagnostic no. 842 (Parameter)	49
Assign behavior of diagnostic no. 862 (Parameter)	50
Assign behavior of diagnostic no. 912 (Parameter)	50
Assign behavior of diagnostic no. 913 (Parameter)	51
Assign behavior of diagnostic no. 944 (Parameter)	51
Assign behavior of diagnostic no. 948 (Parameter)	52
Assign process variable (Parameter)	16, 64
Assign simulation process variable (Parameter)	38

B

Bluetooth (Parameter)	110
Bluetooth configuration (Submenu)	110
Brightness (Parameter)	121

C

C0 to 5 (Parameter)	86
Calibration (Submenu)	85
Calibration factor (Parameter)	85
Color scheme (Parameter)	121
Commissioning (Wizard)	
.	6, 8, 9, 11, 16, 19, 20, 22, 23, 28, 30
Communication (Submenu)	98
Communication established (Parameter)	110
Configuration (Submenu)	46
Configuration counter (Parameter)	105
Connectivity (Submenu)	110
Control Totalizer 1 to n (Parameter)	66
Corrected volume flow (Parameter)	54
Corrected volume flow calculation (Submenu)	77
Corrected volume flow factor (Parameter)	84
Corrected volume flow offset (Parameter)	83
Corrected volume flow unit (Parameter)	14, 60
Corrected volume unit (Parameter)	14, 60
Current output 1 (Submenu)	87
Current output 1 simulation (Parameter)	39
Current output value (Parameter)	39
Current range output (Parameter)	23, 92
Cut off inhomogeneous liquid (Parameter)	76

Cut off inhomogeneous wet gas (Parameter)	76
---	----

D

Damping current output (Parameter)	26, 95
Date / Time (Submenu)	111
Define access code (Wizard)	109
Density (Parameter)	54
Density damping (Parameter)	69
Density factor (Parameter)	83
Density offset (Parameter)	83
Density unit (Parameter)	15, 61
Device (Submenu)	113
Device alarm simulation (Parameter)	40
Device management (Submenu)	104
Device name (Parameter)	9, 113
Device reset (Parameter)	105
Device tag (Parameter)	8, 104, 114
Diagnostic configuration (Submenu)	42
Diagnostic event category (Parameter)	40
Diagnostic event simulation (Parameter)	40
Diagnostic list (Submenu)	35
Diagnostic settings (Submenu)	42
Diagnostics (Menu)	32
Diagnostics 1 (Parameter)	35
Diagnostics 2 (Parameter)	36
Diagnostics 3 (Parameter)	36
Diagnostics 4 (Parameter)	36
Diagnostics 5 (Parameter)	37
Display (Submenu)	118
Display damping (Parameter)	30, 121
Display module (Submenu)	116
Document	
Target group	4

E

Electronics (Submenu)	44
ENP version (Parameter)	115
Enter access code (Parameter)	108
Extended order code 1 (Parameter)	115
Extended order code 2 (Parameter)	115
Extended order code 3 (Parameter)	115
External compensation (Submenu)	77

F

Failure behavior current output (Parameter)	27, 96
Failure current (Parameter)	27, 96
Failure mode (Parameter)	18, 67
Firmware version (Parameter)	9, 114, 116, 117
Fixed current (Parameter)	26, 93
Fixed reference density (Parameter)	78
Flow damping time (Parameter)	19, 69
Flow override (Parameter)	69

G

Gas Fraction Handler (Parameter)	75
Guidance (Menu)	6

H

Heartbeat Technology (Submenu)	41
High value partial filled pipe detection (Parameter)	22, 72

I

Index inhomogeneous medium (Parameter)	76
Information (Submenu)	113
Installation direction (Parameter)	80

L

Language (Parameter)	118
Linear expansion coefficient (Parameter)	79
Locking status (Parameter)	104
Low flow cut off (Parameter)	20, 70
Low flow cut off (Submenu)	70
Low value partial filled pipe detection (Parameter)	22, 72
Lower range value output (Parameter)	24, 93

M

Manufacturer (Parameter)	116
Mass flow (Parameter)	53
Mass flow factor (Parameter)	82
Mass flow offset (Parameter)	82
Mass flow unit (Parameter)	11, 57
Mass unit (Parameter)	12, 58
Measured values (Submenu)	53
Measuring mode current output (Parameter)	88
Medium settings (Submenu)	73
Menu	
Application	53
Diagnostics	32
Guidance	6
System	103
Modbus configuration (Submenu)	98
Modbus data map (Submenu)	101
Modbus information (Submenu)	102

N

Nominal diameter (Parameter)	85
------------------------------------	----

O

Off value low flow cutoff (Parameter)	21, 71
On value low flow cutoff (Parameter)	21, 71
Operating time (Parameter)	34
Operating time from restart (Parameter)	34
Order code (Parameter)	114
Output current 1 (Parameter)	97

P

Partially filled pipe detection (Parameter)	22, 72
Partially filled pipe detection (Submenu)	71
Preset value 1 to n (Parameter)	66
Pressure compensation (Parameter)	11, 77
Pressure shock suppression (Parameter)	19
Pressure unit (Parameter)	16, 62
Pressure value (Parameter)	11, 77
Previous diagnostics (Parameter)	33
Process (Submenu)	47

Process parameters (Submenu)	68
Process variable adjustment (Submenu)	81
Process variable current output (Parameter)	23, 87
Process variable value (Parameter)	39
Progress (Parameter)	81
Properties (Submenu)	42

R

Reference density unit (Parameter)	15, 61
Reference sound velocity (Parameter)	10, 74
Reference temperature (Parameter)	78
Reset all totalizers (Parameter)	63
Reset Maintenance code (Parameter)	108
Rotation display (Parameter)	121

S

Select gas type (Parameter)	9, 73
Select medium (Parameter)	9, 73
Select reference density (Parameter)	78
Sensor (Submenu)	43, 68
Sensor adjustment (Submenu)	80
Sensor electronic module (ISEM) (Submenu)	116
Serial number (Parameter)	8, 114
Set date/time (Parameter)	31
Simulation (Submenu)	38
Software configuration (Submenu)	122
Software option overview (Parameter)	122
Square expansion coefficient (Parameter)	79
Submenu	
Active diagnostics	33
Bluetooth configuration	110
Calibration	85
Communication	98
Configuration	46
Connectivity	110
Corrected volume flow calculation	77
Current output 1	87
Date / Time	111
Device	113
Device management	104
Diagnostic configuration	42
Diagnostic list	35
Diagnostic settings	42
Display	118
Display module	116
Electronics	44
External compensation	77
Heartbeat Technology	41
Information	113
Low flow cut off	70
Measured values	53
Medium settings	73
Modbus configuration	98
Modbus data map	101
Modbus information	102
Partially filled pipe detection	71
Process	47
Process parameters	68
Process variable adjustment	81

Properties	42
Sensor	43, 68
Sensor adjustment	80
Sensor electronic module (ISEM)	116
Simulation	38
Software configuration	122
System units	57
Totalizer	55
Totalizer 1 to n	63
Totalizer handling	63
Totalizers	63
Two phase flow	74
User management	107
Zero point adjustment	80
System (Menu)	103
System units (Submenu)	57

T

Target group	4
Temperature (Parameter)	54
Temperature coefficient sound velocity (Parameter)	10, 74
Temperature damping (Parameter)	70
Temperature factor (Parameter)	84
Temperature offset (Parameter)	84
Temperature unit (Parameter)	15, 61
Time format (Parameter)	30
Time zone (Parameter)	30
Timestamp (Parameter)	33, 34, 35, 36, 37
Totalizer (Submenu)	55
Totalizer 1 to n (Submenu)	63
Totalizer handling (Submenu)	63
Totalizer operation mode (Parameter)	18, 65
Totalizer overflow 1 to n (Parameter)	55
Totalizer value 1 to n (Parameter)	55
Totalizers (Submenu)	63
Two phase flow (Submenu)	74

U

Unit totalizer 1 to n (Parameter)	16, 64
Upper range value output (Parameter)	26, 95
User management (Submenu)	107
User role (Parameter)	107

V

Value 1 display (Parameter)	28, 119
Value 2 display (Parameter)	28, 119
Value 3 display (Parameter)	29, 120
Value 4 display (Parameter)	29, 120
Volume flow (Parameter)	54
Volume flow factor (Parameter)	83
Volume flow offset (Parameter)	82
Volume flow unit (Parameter)	12, 58
Volume unit (Parameter)	13, 59

W

Wizard	
Commissioning	6, 8, 9, 11, 16, 19, 20, 22, 23, 28, 30
Define access code	109

Z

Zero point (Parameter)	85
Zero point adjustment (Submenu)	80
Zero point adjustment control (Parameter)	80
Zero point adjustment status (Parameter)	81



www.addresses.endress.com
