MCS100FT

FTIR Analyzer System

Everything under control with advanced, proven technology

- Proper HF limit value monitoring
- Only one analyzer for more than 12 measuring components
- Easy integration into the customer network environment
- Long maintenance interval of 6 months for many measuring components
- Type approved measurement of
- greenhouse gases such as N₂O, CH₄ and CO₂
- Low maintenance requirements





Complete Emissions Monitoring

With the MCS100FT, we offer an FTIR analyzer system that provides complete, continuous emissions monitoring. It detects more than 12 measuring components simultaneously, such as HF, HCI, SO $_2$, NO, NO $_2$, CO, NH $_3$, N $_2$ O, CH $_4$ und Corg (VOC). The MCS100FT enables HF limit values to be monitored in accordance with legal requirements. It is equipped with an oxygen sensor as standard and can be supplemented with an integrated total hydrocarbon analyzer.

The MCS100FT is certified for the 2001/80/EC, 2000/76/EC and TA Luft (German Technical Instructions on Air Quality Control) directives and requirements as well as for MCERT, US EPA, and GOST, and has been designed to comply with directive 2010/75/EU. With its very reliable measuring technology, its convenient operation, and low maintenance requirements, the MCS100FT FTIR analyzer system provides a hassle-free solution that offers unequalled opportunities.

EN 15267-3 and EN 14181

- QAL3 inspection and manual adjustment using an internal adjustment filter without expensive test gases – considerable time savings (approx. 1.5 instead of 6 to 7 hours) and increased availability.
- Qualified and experienced support with official inspections
- Meets the minimum requirements of standards EN 15267-3 and EN14181 (QAL1, 2, 3)

Reliable analysis technology


- More than 30 years of experience in spectroscopic emissions
- measurement and more than 2,000 installed systems
- Long-term stability of measured values thanks to automatic spectrum adjustment
- Low maintenance requirements, typical intervals of between 3 and 6 months

Control of HF limit values

- Actual monitoring of strict HF limit values from 0 to 1 mg/m³ or 0 to 2 mg/m³
- Analysis specially optimized for HF, from sampling to the sample gas cell
- Short response time of approx. 170 s, even with a sample gas line up to 35 m in length
- Smallest HF measuring range tested for suitability for multicomponent systems




The Analyzer system – from gas sampling to measurement value evaulation and effective emission data management

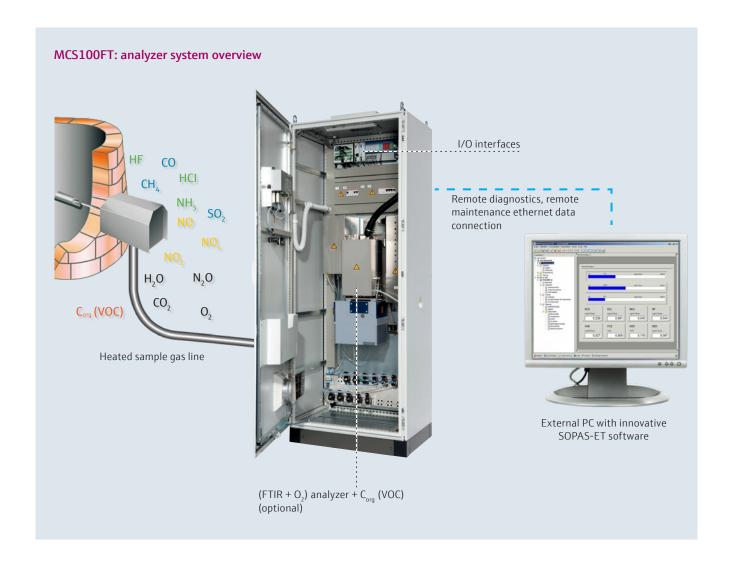

FTIR measurement principle

Infrared spectroscopy according to the Fourier transformation (FTIR) principle ensures high measurement accuracy – especially in combination with the proven sample gas cell. Accurate gas concentrations from the selected gas components are determined from very fast spectrum measurement using chemometric models. The cube corner technique used by the interferometer delivers very reliable and stable measurement results. The principle also involves a RockSolid spectrometer with high spectral resolution and high measuring speed, which is unaffected by vibration and temperature and is permanently adjusted.

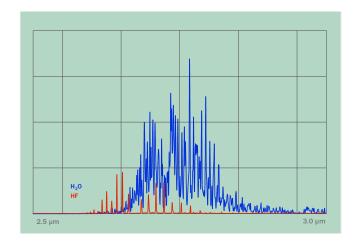

MCS100FT: everything under control with advanced, proven technology



Product description

The FTIR measuring principle allows the simultaneous determination of more than 12 measuring components, tailor-made for the particular requirements of the customer. The MCS100FT FTIR analyzer system with its heated measuring cell enables the monitoring of hydrogen fluoride limits as requested by legislation.

The MCS100FT is equipped with an oxygen sensor as standard and can be supplemented with a total hydrocarbon analyzer. With its reliable measuring technology, its easy operation and low maintenance requirements, the MCS100FT provides a solution that offers unequalled opportunities.

Approved according to EN 15267-3

Remote control and diagnosis via

 Automatic adjustment of analyzer Automatic backflushing and filter

cleaning of sampling unit

software SOPAS ET

At a glance

- Lowest approved HF measuring range of $0 \dots 3 \text{ mg/m}^3$
- Automatic spectrum adjustment via AutoVAL for reliable measuring
- Operation via touchscreen
- Sample gas transport by an ejector without moving parts

Your benefits

- Proper HF limit value monitoring
- Only one analyzer for more than 12 measuring components
- Easy integration into the customer network environment
- components

Fields of application

- Emission monitoring in waste incineration plants
- Effective HF limit value monitoring, e.g. in aluminum production

- Long maintenance interval of 6 months for many measuring
- Type approved measurement of greenhouse gases such as N₂O, CH₄ and CO₂
- Low maintenance requirements
- Monitoring of gaseous emission of cement plants or power station







More Information online

For more information, enter the link or scan the QR code to get direct access to technical data, operating instructions, software, application examples, and much more. www.endress.com/mcs100ft



Technical data

The exact device specifications and performance data of the product may deviate from the information provided here, and depend on the application in which the product is being used and the relevant customer specifications.

Measured values	CH ₄ , CO, CO ₂ , C _{org} , HCl, HF, H ₂ O, NH ₃ , NO, NO ₂ , N ₂ O, O ₂ , SO ₂ , NO _x , C ₃ H ₈ , C ₂ H ₆
Performance tested measurands	CH ₄ , CO, CO ₂ , C _{orq} , HCl, HF, H ₂ O, NH ₃ , NO, NO ₂ , N ₂ O, O ₂ , SO ₂
Measurement principle	FTIR spectroscopy, flame ionization detection, Zirconium dioxide sensor
Sample size	≤ 300 l/h (79.25 gal/h)
Measuring ranges	
CH ₄	0 70 ppm / 0 210 ppm
CO	0 60 ppm / 0 1.200 ppm
CO ₂	0 25 Vol%
C_{org}	0 7,5 ppm / 0 75 ppm
HCI	0 10 ppm / 0 100 ppm
HF	0 3 ppm / 0 10 ppm
H_2O	0 40 Vol%
NH_3	0 13 ppm / 0 65 ppm
NO	0 150 ppm / 0 1.500 ppm
NO_2	0 25 ppm / 0 250 ppm
N_2O	0 25 ppm / 0 250 ppm
O_2	0 21 Vol%
SO ₂	0 25 ppm / 0 525 ppm
NO_x	0 100 ppm / 0 1.000 ppm
C_3H_8	0 25 ppm
C_2H_6	0 40 ppm
	Other measuring ranges and components on request Measuring ranges depend on application and device version
Certified measuring ranges	
CH ₄	$0 \dots 50 \text{ mg/m}^3 / 0 \dots 150 \text{ mg/m}^3 (0 \dots 0.00078 \text{ lb/ft}^3 / 0 \dots 0.00234 \text{ lb/ft}^3)$
СО	0 75 mg/m³ / 0 300 mg/m³ / 0 1.500 mg/m³ (0 0.00117 lb/ft³ / 0 0.00468 lb/ft³ / 0 0.0234 lb/ft³)
CO ₂	0 25 Vol%
C_{org}	0 15 mg/m³ / 0 50 mg/m³ / 0 150 mg/m³ / 0 500 mg/m³ (0 0.00023 lb/ft³ / 0 0.00078 lb/ft³ / 0 0.00234 lb/ft³ / 0 0.00781 lb/ft³
HCI	0 15 mg/m³ / 0 90 mg/m³ / 0 150 mg/m³ (0 0.00023 lb/ft³ / 0 0.00140 lb/ft³ / 0 0.00234 lb/ft³)
HF	0 3 mg/m ³ / 0 10 mg/m ³ (0 0.00005 lb/ft ³ / 0 0.00016 lb/ft ³)
H_2O	0 40 Vol%
NH ₃	0 10 mg/m³ / 0 50 mg/m³ (0 0.00016 lb/ft³ / 0 0.00078 lb/ft³)
NO	0 200 mg/m³ / 0 400 mg/m³ / 0 2.000 mg/m³ (0 0.00312 lb/ft³ / 0 0.00624 lb/ft³ / 0 0.0312 lb/ft³)
NO_2	$0 \dots 100 \ \text{mg/m}^3 \ / \ 0 \dots 500 \ \text{mg/m}^3 \ (0 \dots 0.00156 \ \text{lb/ft}^3 \ / \ 0 \dots 0.00781 \ \text{lb/ft}^3)$
N_2O	$0 \dots 50 \text{ mg/m}^3 / 0 \dots 500 \text{ mg/m}^3 (0 \dots 0.00078 \text{ lb/ft}^3 / 0 \dots 0.00781 \text{ lb/ft}^3)$
O_2	0 21 Vol%
SO ₂	0 75 mg/m³ / 0 300 mg/m³ / 0 1.500 mg/m³

Response time	≤ 200 s FID: ≤ 45 s
Sensitivity drift	< 3 % of measuring range full scale per maintenance interval FID: < 2 % of measuring range full scale per week
Zero point drift	< 3 % of measuring range full scale per maintenance interval FID: < 2 % of measuring range full scale per week
Detection limit	< 2 % of measuring range full scale
Process temperature	≤ +1.300 °C (2372°F)
Sample temperature	≤ +220 °C (428°F)
Process pressure	900 hPa 1.100 hPa (13.05 psi 15.95 psi)
Ambient temperature	+5 °C +35 °C (+41°F +95°F) With cooling device: +5 °C +50 °C (+41°F +122°F)
Storage temperature	−20 °C +60 °C (−4°F +140°F)
Ambient pressure	900 hPa 1.100 hPa (13.05 psi 15.95 psi)
Ambient humidity	≤ 80 %; non-condensing
Conformities	2000/76/EC 2001/80/EC 27. BlmSchV EN 15267 EN 14181
Electrical safety	CE
Enclosure rating	IP 43 Optional: IP 54
Analog outputs	$0/4 \dots 22$ mA, $500~\Omega$ Number depends on system configuration; electrically isolated; max. 32 output
Analog inputs	$0/4 \dots 22$ mA, $100 \ \Omega$ Number depends on system configuration; electrically isolated; max. 32 input
Digital outputs	$48\ V$ AC, 0,5 A, $35\ W$ / $48\ V$ DC, 0,5 A, $24\ W$ Number depends on system configuration; electrically isolated; max. $64\ output$
Digital inputs	3,9 V, 4,5 mA, 0,55 W Number depends on system configuration; max. 64 inputs
Interfaces	RS-422/-485 Ethernet
Bus protocol	Ethernet TCP/IP MODBUS OPC
Indication	LC display Status LEDs: "Power", "Maintenance" and "Fault"
Input	Touchscreen
Operation	Via LC-display or software SOPAS ET Several operating levels, password-protected
Dimensions (W x H x D)	806 mm x 2,165 mm x 605 mm (31.73 in x 85.24 in x 23.82 in) 1,096 mm x 2,165 mm x 605 mm (43.15 in x 85.24 in x 23.82 in) (with cooing device)
Weight	260 kg (573,20 lbs)
Electrical connection	
Power consumption	Analyzer cabinet < 1,000 W: Sample gas line, heated 95 W/m (28.96 W/ft) Gas sampling probe 450 W Heated probe tube 450 W
Auxiliaries	

Zero gas (FTIR/FID)::	\leq 300 l/h \leq 350 l/h (79.25 gal/h \leq 92.46 gal/h) Instrument air; 3±0.2 bar; particle size max. 1 µm; oil content max. 0.1 mg/r pressure dew point max. -30 °C (-22 °F)
Zero gas (O ₂):	\leq 350 l/h (92.46 gal/h) O_2 in N_2 :1 4 Vol%; accuracy \pm 2%; 3 \pm 0.2 bar
Reference g (FTIR):	\leq 350 l/h (92.46 gal/h) Measuring component in N ₂ ; 70% of measuring range full scale; 3 \pm 0.2 bar
Reference gas (O ₂):	≤ 350 l/h (92.46 gal/h) Ambient air
Reference gas (FID):	≤ 450 l/h (118.88 gal/h) Propane in synthetic air: 75% of measuring range full scale; 3 ±0.2 bar
Instrument air:	\leq 2.000 l/h (528.34 gal/h) Instrument air: 5 7 bar; particle size max. 1 μ m; oil content max. 0.1 mg/m pressure dew point max. -30 °C (-22 °F)
Fuel gas:	≤ 4,8 l/h (1.27 gal/h) Hydrogen: 5.0 or higher; 3 ±0.2
Combustion air:	\leq 30 l/h (7.93 gal/h) Instrument air; 3±0.2 bar; particle size max. 1 µm; oil content max. 0.1 mg/n pressure dew point max. -30 °C (-22 °F)
Sample connections	Sample gas inlet: DN 4/6 Exhaust gas outlet: DN 8/10
Auxiliary connections	Test gas: DN 4/6 Fuel gas: DN 4/6 Instrument air: DN 6/8
Corrective functions	Internal adjustment unit (option)
Test functions	Internal zero point check
Options	Integrated total hydrocarbon analyzer

Ordering information

Our regional sales organization will help you to select the optimum device configuration.

Dimensional drawings

MCS100FT (dimensions in mm (inch))

