

Safety Instructions

Cerabar PMC71B, PMP71B

2Ex ec IIC T6...T1 Gc

Ex tc IIIC Txxx°C Dc



Cerabar PMC71B, PMP71B

Table of contents

About this document 4

Associated documentation 4

Supplementary documentation 4

General notes: Combined approval 4

Certificates and declarations 5

Manufacturer address 5

Extended order code 5

Safety instructions: General 8

Safety instructions: Specific conditions of use 8

Safety instructions: Installation 9

Temperature tables 10

Connection data 13

About this document

 The document number of these Safety Instructions (XA) must match the information on the nameplate.





Associated documentation

All documentation is available on the Internet:
www.endress.com/Deviceviewer
(enter the serial number from the nameplate).
To commission the device, please observe the Operating Instructions pertaining to the device:
PMC71B
BA02010P, TI01507P
PMP71B
BA02012P, TI01509P

Supplementary documentation

Explosion protection brochure: CP00021Z
The explosion protection brochure is available on the Internet:
www.endress.com/Downloads

General notes:
Combined approval

					
Ex ec IIC Zone 2	Ex tc IIIC Zone 22	Ex ec IIC Zone 2	Ex tc IIIC Zone 22	Ex tc IIIC Zone 22	Ex ec IIC Zone 2

The device is designed for operation in explosive gas or explosive dust atmosphere as shown in the sketch above. In the event of potentially explosive gas-air and dust-air mixtures occurring simultaneously: Suitability requires further assessment.

-  A sequential change between gas and dust explosion protection is only possible if:
- A period with non-explosive atmosphere is realized during the transition or
 - Special examinations are done which are not covered by the certificate

Certificates and declarations

Certificate of Conformity TP TC 012/2011

Inspection authority:
LLP "T-Standard" (TOO/ЖШС "Т-Стандарт")

Certificate number:
EA9C KZ 7500525.01.01.01734 (Ex ec)
EA9C KZ 7500525.01.01.01735 (Ex tc)

Affixing the certificate number certifies conformity with the following standards (depending on the device version):

- GOST 31610.0-2019 (IEC 60079-0:2017)
- GOST 31610.7-2017 (IEC 60079-7:2015)
- GOST IEC 60079-31-2013

Manufacturer
address

Endress+Hauser SE+Co. KG
Hauptstraße 1
79689 Maulburg, Germany
Address of the manufacturing plant: See nameplate.

Extended
order code

The extended order code is indicated on the nameplate, which is affixed to the device in such a way that it is clearly visible. Additional information about the nameplate is provided in the associated Operating Instructions.

Structure of the extended order code

PMx71B	–	*****	+	A*B*C*D*E*F*G*..
(Device type)		(Basic specifications)		(Optional specifications)

* = Placeholder
At this position, an option (number or letter) selected from the specification is displayed instead of the placeholders.

Basic specifications

The features that are absolutely essential for the device (mandatory features) are specified in the basic specifications. The number of positions depends on the number of features available. The selected option of a feature can consist of several positions.

Optional specifications

The optional specifications describe additional features for the device (optional features). The number of positions depends on the number of features available. The features have a 2-digit structure to aid identification (e.g. JA). The first digit (ID) stands for the feature group and consists of a number or a letter (e.g. J = Test, Certificate). The second digit constitutes the value that stands for the feature within the group (e.g. A = 3.1 material (wetted parts), inspection certificate).

More detailed information about the device is provided in the following tables. These tables describe the individual positions and IDs in the extended order code which are relevant to hazardous locations.

Extended order code: Cerabar

-  The following specifications reproduce an extract from the product structure and are used to assign:
- This documentation to the device (using the extended order code on the nameplate).
 - The device options cited in the document.

Device type

PMC71B, PMP71B

Basic specifications

Position 1, 2 (Approval)		
Selected option		Description
PMC71B PMP71B	GL	EAC 2Ex ec IIC T6...T1 Gc
		EAC Ex tc IIIC Txxx°C Dc

Position 3, 4 (Output)		
Selected option		Description
PMC71B PMP71B	BA	2-wire, 4-20 mA HART
	DA	2-wire, PROFIBUS PA
	FA	2-wire, PROFINET, 10Mbit/s (APL)

Position 5 (Display, Operation)		
Selected option		Description
PMC71B PMP71B	M	Prepared for display FHX50B + Gland M20
	N	Prepared for display FHX50B + Thread NPT1/2
	O	Prepared for display FHX50B + Thread M20

Position 6 (Housing, Material)		
Selected option		Description
PMC71B	B	Single compartment; Alu, coated
PMP71B	J	Dual compartment; Alu, coated
	K	Dual compartment; 316L

Position 7 (Electrical Connection)		
Selected option		Description
PMC71B	B	Gland M20, brass nickel plated, IP66/68 NEMA Type 4X/6P
PMP71B	C	Gland M20, 316L, IP66/68 NEMA Type 4X/6P
	F	Thread M20, IP66/68 NEMA Type 4X/6P
	G	Thread G1/2, IP66/68 NEMA Type 4X/6P
	H	Thread NPT1/2, IP66/68 NEMA Type 4X/6P

Position 10 (Diaphragm Seal Type)		
Selected option		Description
PMP71B	G	Temperature isolator
	M	 m capillary, 316L
	N	 m capillary, PVC>316L
	O	 m capillary, PTFE>316L
	R	 ft capillary, 316L
	S	 ft capillary, PVC>316L
	T	 ft capillary, PTFE>316L

Optional specifications

ID Ex (Application Package)		
Selected option		Description
PMC71B	EC	High temperature version, 150°C/302°F process

ID Px, Rx (Accessory Enclosed)		
Selected option		Description
PMC71B	PA	Weather protection cover, 316L ¹⁾
PMP71B		

1) Only in connection with Position 6 = J, K

Safety instructions: General

- The device is intended to be used in explosive atmospheres as defined in the scope of IEC 60079-0 or equivalent national standards. If no potentially explosive atmospheres are present or if additional protective measures have been taken: The device may be operated according to the manufacturer's specifications.
- Comply with the installation and safety instructions in the Operating Instructions.
- Staff must meet the following conditions for mounting, electrical installation, commissioning and maintenance of the device:
 - Be suitably qualified for their role and the tasks they perform
 - Be trained in explosion protection
 - Be familiar with national regulations
- Install the device according to the manufacturer's instructions and national regulations.
- Do not operate the device outside the specified electrical, thermal and mechanical parameters.
- Only use the device in media to which the wetted materials have sufficient durability.
- Avoid electrostatic charging:
 - Of plastic surfaces (e.g. enclosure, sensor element, special varnishing, attached additional plates, ...)
 - Of isolated capacities (e.g. isolated metallic plates)
- Alterations to the device can affect the explosion protection and must be carried out by staff authorized to perform such work by Endress+Hauser.

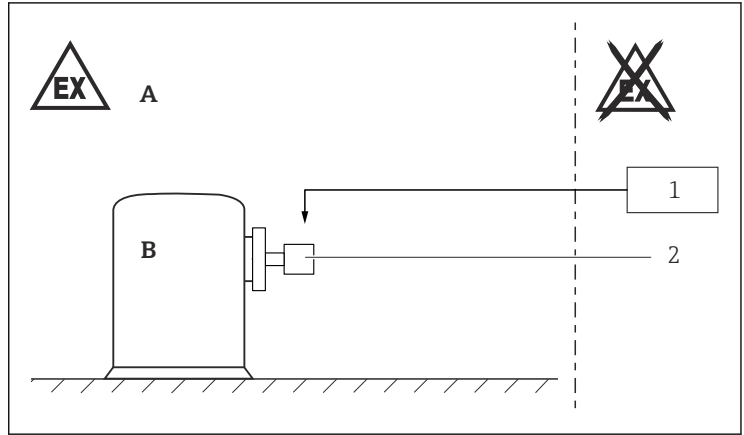
Safety instructions: Specific conditions of use

- To avoid electrostatic charging: Do not rub surfaces with a dry cloth.
- In the event of additional or alternative special varnishing on the enclosure or other metal parts or for adhesive plates:
 - Observe the danger of electrostatic charging and discharge.
 - Do not install in the vicinity of processes (≤ 0.5 m) generating strong electrostatic charges.
- Avoid sparks caused by impact and friction.

Optional specification, ID Px, Rx = PA

Connect the weather protection cover to the local potential equalization.

Safety instructions: Installation



A0041997

- A Zone 2 or Zone 22, Electronic
 B Zone 2 or Zone 22, Process
 1 Power supply
 2 PMC71B, PMP71B

- After aligning (rotating) the enclosure, retighten the fixing screw.
- Perform the following to achieve the degree of protection IP66/67:
 - Screw the cover tight.
 - Mount the cable entry correctly.
- In potentially explosive atmospheres:
 - Do not disconnect the electrical connection of the power supply circuit when energized.
 - Do not open the connection compartment cover and the electronics compartment cover when energized.
- Continuous service temperature of the connecting cable: $\geq T_a + 20\text{ K}$.
- Observe the maximum process conditions according to the manufacturer's Operating Instructions.
- Install the device to exclude any mechanical damage or friction during the application. Pay particular attention to flow conditions and tank fittings.
- Seal unused entry glands with approved sealing plugs that correspond to the type of protection. The plastic transport sealing plug does not meet this requirement and must therefore be replaced during installation.
- Supplied cable glands and metallic sealing plugs comply with the requirements of type of protection marked on the nameplate.
- Before operation:
 - Screw in the cover all the way.
 - Tighten the securing screw on the cover.

Basic specification, Position 5 = N
Observe the requirements according to IEC/EN 60079-14 for conduit systems and the wiring and installation instructions of the suitable Safety Instructions (XA). In addition, observe national regulations and standards for conduit systems.

Potential equalization

Integrate the device into the local potential equalization.

Temperature tables

2Ex ec IIC T6...T1 Gc

- 
- The specified ambient and process temperature ranges exclusively refer to the explosion protection and must not be exceeded. Operationally permitted ambient temperature ranges can be restricted depending on the version: See Operating Instructions.
 - Do not exceed the max. ambient temperature at the enclosure.
 - The process temperatures refer to the temperature at the separation membrane.

Device Type PMC71B

Temperature class	Process temperature range	Ambient temperature range
T6	$-40\text{ °C} \leq T_p \leq +80\text{ °C}$	$-40\text{ °C} \leq T_a \leq +55\text{ °C}$
T4	$-40\text{ °C} \leq T_p \leq +55\text{ °C}$	$-40\text{ °C} \leq T_a \leq +65\text{ °C}$
T4	$-40\text{ °C} \leq T_p \leq +100\text{ °C}$	$-40\text{ °C} \leq T_a \leq +60\text{ °C}$
T4...T1	$-40\text{ °C} \leq T_p \leq +125\text{ °C}$	$-40\text{ °C} \leq T_a \leq +50\text{ °C}$

Optional specification, ID Ex = EC

Temperature class	Process temperature range	Ambient temperature range
T6	$-40\text{ °C} \leq T_p \leq +80\text{ °C}$	$-40\text{ °C} \leq T_a \leq +65\text{ °C}$
T4	$-40\text{ °C} \leq T_p \leq +125\text{ °C}$	$-40\text{ °C} \leq T_a \leq +60\text{ °C}$
T3...T1	$-40\text{ °C} \leq T_p \leq +150\text{ °C}$	$-40\text{ °C} \leq T_a \leq +50\text{ °C}$

Device Type PMP71B

Temperature class	Process temperature range	Ambient temperature range
T6	$-40\text{ }^{\circ}\text{C} \leq T_p \leq +80\text{ }^{\circ}\text{C}$	$-40\text{ }^{\circ}\text{C} \leq T_a \leq +60\text{ }^{\circ}\text{C}$
	$-40\text{ }^{\circ}\text{C} \leq T_p \leq +70\text{ }^{\circ}\text{C}$	$-40\text{ }^{\circ}\text{C} \leq T_a \leq +65\text{ }^{\circ}\text{C}$
T4...T1	$-40\text{ }^{\circ}\text{C} \leq T_p \leq +125\text{ }^{\circ}\text{C}$	$-40\text{ }^{\circ}\text{C} \leq T_a \leq +50\text{ }^{\circ}\text{C}$
	$-40\text{ }^{\circ}\text{C} \leq T_p \leq +100\text{ }^{\circ}\text{C}$	$-40\text{ }^{\circ}\text{C} \leq T_a \leq +60\text{ }^{\circ}\text{C}$

Basic specification, Position 10 = G

Temperature class	Process temperature range	Ambient temperature range
T6	$-40\text{ }^{\circ}\text{C} \leq T_p \leq +80\text{ }^{\circ}\text{C}$	$-40\text{ }^{\circ}\text{C} \leq T_a \leq +65\text{ }^{\circ}\text{C}$
T4	$-40\text{ }^{\circ}\text{C} \leq T_p \leq +130\text{ }^{\circ}\text{C}$	$-40\text{ }^{\circ}\text{C} \leq T_a \leq +70\text{ }^{\circ}\text{C}$
T3	$-40\text{ }^{\circ}\text{C} \leq T_p \leq +190\text{ }^{\circ}\text{C}$	$-40\text{ }^{\circ}\text{C} \leq T_a \leq +65\text{ }^{\circ}\text{C}$
T2	$-40\text{ }^{\circ}\text{C} \leq T_p \leq +290\text{ }^{\circ}\text{C}$	$-40\text{ }^{\circ}\text{C} \leq T_a \leq +60\text{ }^{\circ}\text{C}$
T1	$-40\text{ }^{\circ}\text{C} \leq T_p \leq +400\text{ }^{\circ}\text{C}$	$-40\text{ }^{\circ}\text{C} \leq T_a \leq +55\text{ }^{\circ}\text{C}$

Basic specification, Position 10 = M, N, O, R, S, T

Temperature class	Process temperature range	Ambient temperature range
T6	$-40\text{ }^{\circ}\text{C} \leq T_p \leq +80\text{ }^{\circ}\text{C}$	$-40\text{ }^{\circ}\text{C} \leq T_a \leq +65\text{ }^{\circ}\text{C}$
T4	$-40\text{ }^{\circ}\text{C} \leq T_p \leq +130\text{ }^{\circ}\text{C}$	$-40\text{ }^{\circ}\text{C} \leq T_a \leq +70\text{ }^{\circ}\text{C}$
T3	$-40\text{ }^{\circ}\text{C} \leq T_p \leq +190\text{ }^{\circ}\text{C}$	
T2	$-40\text{ }^{\circ}\text{C} \leq T_p \leq +290\text{ }^{\circ}\text{C}$	
T1	$-40\text{ }^{\circ}\text{C} \leq T_p \leq +400\text{ }^{\circ}\text{C}$	

Ex tc IIIC Txxx°C Dc

- 
 - The specified surface temperature takes into account all direct heat influences from process heat and self-heating at the enclosure.
 - Surface temperatures at the process side maybe higher and must be considered by the user (e.g. at high temperature process connections).
 - The T-marking is based on the process temperature of the compact designs.
 - The specified ambient and process temperature ranges exclusively refer to the explosion protection and must not be exceeded. Operationally permitted temperature ranges can be restricted depending on the version: See Operating Instructions.
 - Do not exceed the max. ambient temperature at the enclosure.
 - The process temperatures refer to the temperature at the separation membrane.

For detailed information see Technical Information.

- 

Basic specification, Position 6 = K
When using the stainless steel enclosure: Reduce the admissible ambient temperature by 5 K.
- 

Protection type of enclosure: IP66/67

Device Type PMC71B

Ex tc IIIC T125°C Dc

Maximum surface temperature	Process temperature range	Ambient temperature range
T125 °C	-40 °C ≤ T _p ≤ +70 °C	-40 °C ≤ T _a ≤ +65 °C
	-40 °C ≤ T _p ≤ +100 °C	-40 °C ≤ T _a ≤ +60 °C
	-40 °C ≤ T _p ≤ +125 °C	-40 °C ≤ T _a ≤ +55 °C

Ex tc IIIC T150°C Dc

Optional specification, ID Ex = EC

Maximum surface temperature	Process temperature range	Ambient temperature range
T150 °C	-40 °C ≤ T _p ≤ +125 °C	-40 °C ≤ T _a ≤ +60 °C
	-40 °C ≤ T _p ≤ +150 °C	-40 °C ≤ T _a ≤ +55 °C

Device Type PMP71B

Ex tc IIIC T125°C Dc

Maximum surface temperature	Process temperature range	Ambient temperature range
T125 °C	$-40\text{ °C} \leq T_p \leq +80\text{ °C}$	$-40\text{ °C} \leq T_a \leq +65\text{ °C}$
	$-40\text{ °C} \leq T_p \leq +100\text{ °C}$	$-40\text{ °C} \leq T_a \leq +60\text{ °C}$
	$-40\text{ °C} \leq T_p \leq +125\text{ °C}$	$-40\text{ °C} \leq T_a \leq +50\text{ °C}$

Basic specification, Position 10 = G

Maximum surface temperature	Process temperature range	Ambient temperature range
T125 °C	$-40\text{ °C} \leq T_p \leq +190\text{ °C}$	$-40\text{ °C} \leq T_a \leq +60\text{ °C}$
	$-40\text{ °C} \leq T_p \leq +290\text{ °C}$	$-40\text{ °C} \leq T_a \leq +55\text{ °C}$
	$-40\text{ °C} \leq T_p \leq +400\text{ °C}$	$-40\text{ °C} \leq T_a \leq +50\text{ °C}$

Basic specification, Position 10 = M, N, O, R, S, T

Maximum surface temperature	Process temperature range	Ambient temperature range
T125 °C	$-40\text{ °C} \leq T_p \leq +190\text{ °C}$	$-40\text{ °C} \leq T_a \leq +70\text{ °C}$
	$-40\text{ °C} \leq T_p \leq +290\text{ °C}$	
	$-40\text{ °C} \leq T_p \leq +400\text{ °C}$	

Connection data

Basic specification, Position 3 = BA

Power supply
$U \leq 35\text{ V}_{DC}$ $P \leq 1\text{ W}$

Basic specification, Position 3 = DA

Power supply
$U \leq 32\text{ V}_{DC}$ $P \leq 0.7\text{ W}$

Basic specification, Position 3 = FA

Power supply
$U \leq 15\text{ V}_{DC}$ $P \leq 0.7\text{ W}$

In connection with: *Basic specification, Position 5 = M, N, O*
Installation according to the specifications of FHX50B.

 Only the type of protection suitable for the device shall be connected!

Cable entry parameters

Cable gland: *Basic specification, Position 7 = B*

Thread	Clamping range	Material	Sealing insert	O-ring
M20x1,5	ø 8 to 10.5 mm	Ms, nickel-plated	Silicone	EPDM (ø 17x2)

Cable gland: *Basic specification, Position 7 = C*

Thread	Clamping range	Material	Sealing insert	O-ring
M20x1,5	ø 7 to 12 mm	1.4404	NBR	EPDM (ø 17x2)

-  ■ The tightening torque refers to cable glands installed by the manufacturer:
- Recommended: 3.5 Nm
 - Maximum: 10 Nm
 - This value may be different depending on the type of cable. However, the maximum value must not be exceeded.
- Only suitable for fixed installation. The operator must pay attention to a suitable strain relief of the cable.
- The cable glands are suitable for a low risk of mechanical danger (4 Joule) and must be mounted in a protected position if larger impact energy levels are expected.
- To maintain the ingress protection of the enclosure: Install the enclosure cover, cable glands and blind plugs correctly.



71675082

www.addresses.endress.com
