Safety Instructions **Gammapilot FMG50**

Ex db ia IIC T6...T1 Gb







Gammapilot FMG50

Table of contents

About this document	4
Associated documentation	4
Supplementary documentation	4
Certificates and declarations	4
Manufacturer address	4
Extended order code	4
Safety instructions: General	7
Safety instructions: Specific conditions of use	7
Safety instructions: Installation	3
Safety instructions: Ex d joints	9
Temperature tables	9
Connection data 10	O

About this document



The document number of these Safety Instructions (XA) must match the information on the nameplate.

Associated documentation

All documentation is available on the Internet:

www.endress.com/Deviceviewer

(enter the serial number from the nameplate).

To commission the device, please observe the Operating Instructions pertaining to the device:

BA01966F

Supplementary documentation

Explosion protection brochure: CP00021Z

The explosion protection brochure is available on the Internet:

www.endress.com/Downloads

Certificates and declarations

Certificate of Conformity

Certificate number: TÜV 20.1811 X

Affixing the certificate number certifies conformity with the following standards (depending on the device version):

- ABNT NBR IEC 60079-0:2020
- ABNT NBR IEC 60079-1:2020
- ABNT NBR IEC 60079-11:2017

Manufacturer address

Endress+Hauser SE+Co. KG

Hauptstraße 1

79689 Maulburg, Germany

Address of the manufacturing plant: See nameplate.

Extended order code

The extended order code is indicated on the nameplate, which is affixed to the device in such a way that it is clearly visible. Additional information about the nameplate is provided in the associated Operating Instructions.

Structure of the extended order code

FMG50	_	*****	+	A*B*C*D*E*F*G*.
(Device		(Basic		(Optional
type)		specifications)		specifications)

* = Placeholder

At this position, an option (number or letter) selected from the specification is displayed instead of the placeholders.

Basic specifications

The features that are absolutely essential for the device (mandatory features) are specified in the basic specifications. The number of positions depends on the number of features available.

The selected option of a feature can consist of several positions.

Optional specifications

The optional specifications describe additional features for the device (optional features). The number of positions depends on the number of features available. The features have a 2-digit structure to aid identification (e.g. JA). The first digit (ID) stands for the feature group and consists of a number or a letter (e.g. J = Test, Certificate). The second digit constitutes the value that stands for the feature within the group (e.g. A = 3.1 material (wetted parts), inspection certificate).

More detailed information about the device is provided in the following tables. These tables describe the individual positions and IDs in the extended order code which are relevant to hazardous locations.

Extended order code: Gammapilot



The following specifications reproduce an extract from the product structure and are used to assign:

- This documentation to the device (using the extended order code on the nameplate).
- The device options cited in the document.

Device type

FMG50

Basic specifications

Position 1,	Position 1, 2 (Approval)			
Selected option		Description		
FMG50 MP		INMETRO Ex db ia IIC T6T1 Gb 1)		

1) Protection type "Ex db" only available inside the detector pipe

Position 3, 4 (Output)			
Selected option Description		Description	
FMG50	BA	2-wire, 4-20 mA HART	
DA 2-wire, PROFIBUS PA		2-wire, PROFIBUS PA	
FA 2-wire, PROFINET, 10Mbit/s (APL)		2-wire, PROFINET, 10Mbit/s (APL)	

Position 5 (Display, Operation)			
Selected option		Description	
FMG50	А	W/o; via communication	
	С	Segment display w/o buttons	
	D	Segment display w/o buttons + Bluetooth	
	Е	Graphic display	
	F	Graphic display + Bluetooth	
	L	Prepared for display FHX50B + M12 connection	
	M	Prepared for display FHX50B + Gland M20	
	N	Prepared for display FHX50B + Thread NPT1/2	
	0	Prepared for display FHX50B + Thread M20	

Position 8 (Application)			
Selected option Description			
FMG50	А	Ambient temperature -4060°C/ -40140°F (PVT)	
	В	Ambient temperature -2080°C/ -4176°F (PVT HT)	
C Ambient temperature -4080°C/ -40176°F (NaI)		Ambient temperature -4080°C/ -40176°F (NaI)	

Optional specifications

ID Nx (Accessory Mounted)				
Selected option		Description		
FMG50 NA		Overvoltage protection		

ID Px, Rx (Accessory Enclosed)				
Selected option		Description		
FMG50 PA		Weather protection cover, 316L		

Safety instructions: General


- The device is intended to be used in explosive atmospheres as defined in the scope of IEC 60079-0 or equivalent national standards. If no potentially explosive atmospheres are present or if additional protective measures have been taken: The device may be operated according to the manufacturer's specifications.
- Comply with the installation and safety instructions in the Operating Instructions.
- Staff must meet the following conditions for mounting, electrical installation, commissioning and maintenance of the device:
 - Be suitably qualified for their role and the tasks they perform
 - Be trained in explosion protection
 - Be familiar with national regulations
- Install the device according to the manufacturer's instructions and national regulations.
- Do not operate the device outside the specified electrical, thermal and mechanical parameters.
- Avoid electrostatic charging:
 - Of plastic surfaces (e.g. enclosure, sensor element, special varnishing, attached additional plates, ...)
 - Of isolated capacities (e.g. isolated metallic plates)
- Alterations to the device can affect the explosion protection and must be carried out by staff authorized to perform such work by Endress+Hauser.

Safety instructions: Specific conditions of use

- To avoid electrostatic charging: Do not rub surfaces with a dry cloth.
- In the event of additional or alternative special varnishing on the enclosure or other metal parts or for adhesive plates:
 - Observe the danger of electrostatic charging and discharge.
 - Do not install in the vicinity of processes generating strong electrostatic charges.


Optional specification, ID Px, Rx = PAConnect the weather protection cover to the local potential equalization.

Safety instructions: Installation

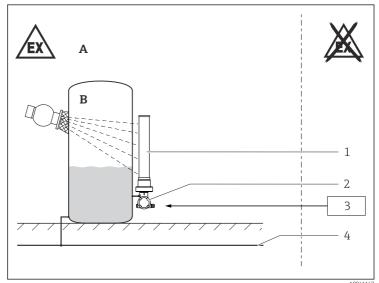

AU04116

- A Zone 1, Zone 2
- B Zone 0, Zone 1, Zone 2
- 1 Detector pipe (in Ex d)
- 2 Enclosure
- 3 Certified associated apparatus
- 4 Local potential equalization
- After aligning (rotating) the enclosure, retighten the fixing screw.
- The safety screws at the pipe enclosure must not be loosened:



10041226

- Continuous service temperature of the connecting cable: $\geq T_a+20 \text{ K}$.
- Observe the pertinent guidelines when interconnecting intrinsically safe circuits

Basic specification, Position 5 = N

Observe the requirements according to IEC/EN 60079-14 for conduit systems and the wiring and installation instructions of the suitable Safety Instructions (XA). In addition, observe national regulations and standards for conduit systems.

Intrinsic safety

- \blacksquare The intrinsically safe input power circuit of the device is isolated from ground. The dielectric strength is at least 500 $V_{\rm rms}.$
- When the device is connected to certified intrinsically safe circuits of Category Ex ib for Equipment Groups IIC and IIB, the type of protection changes to Ex ib IIC and Ex ib IIB.
- Associated devices with galvanic isolation between the intrinsically safe and non-intrinsically safe circuits are preferred.

Potential equalization

Integrate the device into the local potential equalization.

Overvoltage protection

Optional specification, ID Nx = NA

The intrinsically safe input power circuit of the device is isolated from ground. The dielectric strength is at least 290 $V_{\rm rms}$.

Safety instructions: Ex d joints

- If required or if in doubt: ask manufacturer for specifications.
- Flameproof joints are not intended to be repaired.

Temperature tables

Basic specification, Position 3, 4 = BA

	Temperature	Ambient temperature T _a (ambient)		
with Basic	class	with Basic specification		
specification, Position 8		Position 5 = A, L, M, N, O	Position 5 = C, D, E, F	
= A	T6T1	-40 °C ≤ T _a ≤ +60 °C	$-40 ^{\circ}\text{C} \le T_a \le +60 ^{\circ}\text{C}$	
= B	T6	$-20 ^{\circ}\text{C} \le \text{T}_{\text{a}} \le +70 ^{\circ}\text{C}$	$-20 ^{\circ}\text{C} \le T_{a} \le +60 ^{\circ}\text{C}$	
	T5T1	$-20 ^{\circ}\text{C} \le \text{T}_{\text{a}} \le +75 ^{\circ}\text{C}$	$-20 ^{\circ}\text{C} \le T_{\text{a}} \le +65 ^{\circ}\text{C}$	
= C	Т6	$-40 ^{\circ}\text{C} \le \text{T}_{\text{a}} \le +70 ^{\circ}\text{C}$	$-40 ^{\circ}\text{C} \le T_{a} \le +60 ^{\circ}\text{C}$	
	T5T1	-40 °C ≤ T _a ≤ +75 °C	$-40 ^{\circ}\text{C} \le T_{a} \le +65 ^{\circ}\text{C}$	

Basic specification, Position 3, 4 = DA

with Basic	Temperature class	Ambient temperature T_a (with Basic specification	(ambient)
specification, Position 8		Position 5 = A, L, M, N, O	Position 5 = C, D, E, F
= A	T6T1	$-40 ^{\circ}\text{C} \le T_{a} \le +60 ^{\circ}\text{C}$	$-40 ^{\circ}\text{C} \le T_a \le +60 ^{\circ}\text{C}$
= B	T6	$-20 ^{\circ}\text{C} \le T_a \le +60 ^{\circ}\text{C}$	$-20 ^{\circ}\text{C} \le T_a \le +60 ^{\circ}\text{C}$
	T5T1	$-20 ^{\circ}\text{C} \le \text{T}_{\text{a}} \le +65 ^{\circ}\text{C}$	$-20 ^{\circ}\text{C} \le T_a \le +65 ^{\circ}\text{C}$
= C	T6	-40 °C ≤ T _a ≤ +60 °C	-40 °C ≤ T _a ≤ +60 °C
	T5T1	$-40 ^{\circ}\text{C} \le \text{T}_{\text{a}} \le +65 ^{\circ}\text{C}$	-40 °C ≤ T _a ≤ +65 °C

Basic specification, Position 3, 4 = FA

with Basic	Temperature class	Ambient temperature T_a (ambient) with Basic specification	
Position 8		Position 5 = A, L, M, N, O	Position 5 = C, D, E, F
= A	T6T1	$-40 ^{\circ}\text{C} \le \text{T}_{\text{a}} \le +60 ^{\circ}\text{C}$	$-40 ^{\circ}\text{C} \le T_a \le +60 ^{\circ}\text{C}$
= B	T6	$-20 ^{\circ}\text{C} \le \text{T}_{\text{a}} \le +70 ^{\circ}\text{C}$	$-20 ^{\circ}\text{C} \le T_a \le +60 ^{\circ}\text{C}$
	T5T1	$-20 ^{\circ}\text{C} \le \text{T}_{\text{a}} \le +75 ^{\circ}\text{C}$	$-20 ^{\circ}\text{C} \le T_a \le +65 ^{\circ}\text{C}$
= C	T6	-40 °C ≤ T _a ≤ +70 °C	$-40 ^{\circ}\text{C} \le T_{a} \le +60 ^{\circ}\text{C}$
	T5T1	-40 °C ≤ T _a ≤ +75 °C	-40 °C ≤ T _a ≤ +65 °C

Connection data

Basic specification, Position 3, 4 = BA

ower supply	
$\begin{array}{l} J_i \leq 30 \ V_{DC} \\ \leq 300 \ mA \end{array}$	
$P_i \le 1 \text{ W}$	
$C_i \le 10 \text{ nF}$	
$r_i = 0$	

Basic specification, Position 3, 4 = DA

Power supply	
FISCO	Entity
$\begin{split} &U_{i} \leq 17.5 \ V_{DC} \\ &I_{i} \leq 380 \ mA \\ &P_{i} \leq 5.32 \ W \\ &C_{i} \leq 5 \ nF \\ &L_{i} = 0 \end{split}$	$\begin{split} &U_{l} \leq 24 \; V_{DC} \\ &I_{i} \leq 300 \; mA \\ &P_{i} \leq 1.2 \; W \\ &C_{i} \leq 5 \; nF \\ &L_{i} = 0 \end{split}$

Basic specification, Position 3, 4 = FA

Power supply	
2-WISE	Entity
$\begin{split} &U_{i} \leq 17.5 \ V_{DC} \\ &I_{i} \leq 380 \ mA \\ &P_{i} \leq 5.32 \ W \\ &C_{i} \leq 5 \ nF \\ &L_{i} = 0 \end{split}$	$\begin{split} &U_i \leq 17.5 \ V_{DC} \\ &I_i \leq 300 \ mA \\ &P_i \leq 1.2 \ W \\ &C_i \leq 5 \ nF \\ &L_i = 0 \end{split}$

In connection with: Basic specification, Position 5 = L, M, N, O Installation according to the specifications of FHX50B.



Only the type of protection suitable for the device shall be connected!



www.addresses.endress.com