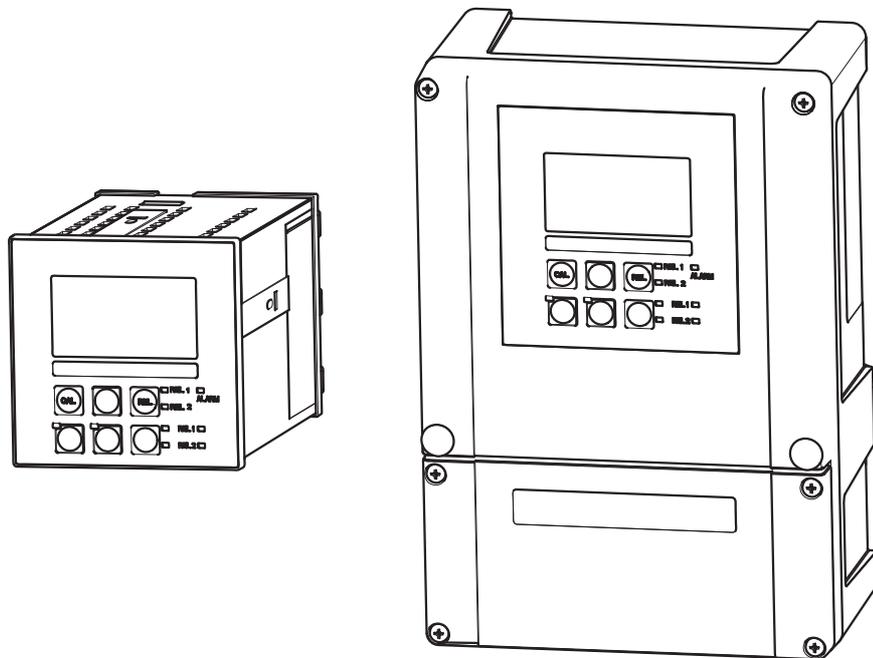


Operating Instructions

Liquisys M COM223/253

Transmitter for Dissolved Oxygen



About this document

Safety messages

The structure, signal words and safety colors of the signs comply with the specifications of ANSI Z535.6 ("Product safety information in product manuals, instructions and other collateral materials").

Safety message structure	Meaning
 DANGER Cause (/consequences) Consequences if safety message is not heeded ▶ Corrective action	This symbol alerts you to a dangerous situation. Failure to avoid the situation will result in a fatal or serious injury.
 WARNING Cause (/consequences) Consequences if safety message is not heeded ▶ Corrective action	This symbol alerts you to a dangerous situation. Failure to avoid the situation can result in a fatal or serious injury.
 CAUTION Cause (/consequences) Consequences if safety message is not heeded ▶ Corrective action	This symbol alerts you to a dangerous situation. Failure to avoid this situation can result in minor or medium injury.
 NOTICE Cause/situation Consequences if safety message is not heeded ▶ Action/note	This symbol alerts you to situations that can result in damage to property and equipment.

Symbols

-  Additional information, tips
-  Permitted or recommended
-  Forbidden or not recommended

Table of contents

1	Basic Safety instructions	5	6	Commissioning	32
1.1	Requirements for the personnel	5	6.1	Function check	32
1.2	Designated use	5	6.2	Switching on	32
1.3	Workplace safety	5	6.3	Quick start-up	34
1.4	Operational safety	5	6.4	System configuration	36
1.5	Product safety	6	6.4.1	Setup 1 (Oxygen)	36
1.6	Electrical symbols	6	6.4.2	Setup 2 (Salinity and temperature)	37
2	Incoming acceptance and product identification	7	6.4.3	Current input	38
2.1	Incoming acceptance	7	6.4.4	Current outputs	41
2.2	Scope of delivery	7	6.4.5	Monitoring functions	46
2.3	Product identification	8	6.4.6	Relay contact configuration	51
2.3.1	Nameplate	8	6.4.7	Service	62
2.3.2	Identifying the product	8	6.4.8	E+H Service	63
2.4	Certificates and approvals	8	6.4.9	Interfaces	64
2.4.1	CE mark	8	6.5	Communication	64
2.4.2	CSA general purpose	8	6.6	Calibration	65
3	Installation	9	7	Diagnostics and troubleshooting	69
3.1	Quick installation guide	9	7.1	Troubleshooting instructions	69
3.1.1	Measuring system	9	7.2	System error messages	69
3.2	Installation conditions	10	7.3	Process specific errors	72
3.2.1	Field instrument	10	7.4	Instrument specific errors	75
3.2.2	Panel-mounted instrument	11	8	Maintenance	77
3.3	Installation instructions	12	8.1	Maintenance of the entire measuring point	77
3.3.1	Field instrument	12	8.1.1	Cleaning the transmitter	77
3.3.2	Panel-mounted instrument	15	8.1.2	Test variant 1 (DX/DS with COS41)	78
3.4	Post-installation check	15	8.1.3	Test variant 2 (WX/WS with COS31 or COS71)	79
4	Electrical connection	16	8.1.4	Maintenance oxygen sensors	79
4.1	Wiring	16	8.1.5	Maintenance assembly	79
4.1.1	Electrical connection variant 1 (DX/DS with COS41)	17	8.1.6	Connecting lines and junction boxes	80
4.1.2	Electrical connection variant 2 (WX/WS with COS31/71)	21	9	Repair	81
4.1.3	Alarm contact	24	9.1	Spare parts	81
4.2	Post-connection check	24	9.2	Dismantling the panel-mounted instrument ...	81
5	Operability	25	9.3	Dismantling the field instrument	84
5.1	Quick operation guide	25	9.4	Replacing the central module	87
5.2	Display and operating elements	25	9.5	Return	88
5.2.1	Display	25	9.6	Disposal	88
5.2.2	Operating elements	26	10	Accessories	89
5.2.3	Key assignment	27	10.1	Sensors	89
5.3	Local operation	29	10.2	Connection accessories	89
5.3.1	Automatic/manual mode	29	10.3	Mounting accessories	90
5.3.2	Operating concept	30	10.4	Software and hardware add-ons	91

11	Technical data.....	92
11.1	Input.....	92
11.2	Output.....	93
11.3	Power supply.....	96
11.4	Performance characteristics.....	97
11.5	Environment.....	98
11.6	Mechanical construction.....	98
12	Appendix.....	100
	Index.....	113

1 Basic safety instructions

1.1 Requirements for the personnel

- ▶ Installation, commissioning, operation and maintenance of the measuring system must only be carried out by trained technical personnel.
 - ▶ The technical personnel must be authorized by the plant operator to carry out the specified activities.
 - ▶ The electrical connection may only be performed by an electrical technician.
 - ▶ The technical personnel must have read and understood these Operating Instructions and must follow the instructions they contain.
 - ▶ Measuring point faults may only be rectified by authorized and specially trained personnel.
-  Repairs not described in the enclosed Operating Instructions may only be carried out directly at the manufacturer's or by the service organization.

1.2 Designated use

Liquisys M is a transmitter for determining the oxygen concentration of a liquid medium.

The transmitter is particularly suited for use in the following areas:

- Sewage treatment plants
- Sewage treatment
- Drinking water
- Water conditioning and monitoring
- Surface water (rivers, lakes, oceans)
- Fish farming

Any other use than the one described here compromises the safety of persons and the entire measuring system and is not permitted.

The manufacturer is not liable for damage caused by improper or non-designated use.

1.3 Workplace safety

As the user, you are responsible for complying with the following safety conditions:

- Regulations for explosion protection
- Installation instructions
- Local standards and regulations

Electromagnetic compatibility

With regard to electromagnetic compatibility, this device has been tested in accordance with the applicable European standards for industrial applications.

The electromagnetic compatibility indicated only applies to a device that has been connected in accordance with the instructions in these Operating Instructions.

1.4 Operational safety

- ▶ Before commissioning the entire measuring point, make sure all the connections are correct. Ensure that electrical cables and hose connections are not damaged.
- ▶ Do not operate damaged products, and safeguard them to ensure that they are not operated inadvertently. Mark the damaged product as defective.
- ▶ If faults cannot be rectified, the products must be taken out of service and secured against unintentional commissioning.

1.5 Product safety

The product is designed to meet state-of-the-art safety requirements, has been tested and left the factory in a condition in which it is safe to operate. Relevant regulations and European standards have been observed.

1.6 Electrical symbols



Direct Current (DC)

A terminal at which DC is applied or through which DC flows.



Alternating Current (AC)

A terminal at which (sine-form) AC is applied or through which AC flows.



Ground connecting

A terminal which, from the user's point of view, is already grounded using a grounding system.



Protective ground terminal

A terminal which must be grounded before other connections may be set up.



Class II (isolated) device

Double insulation



Alarm relay



Input



Output



DC voltage source



Temperature sensor

2 Incoming acceptance and product identification

2.1 Incoming acceptance

- ▶ Make sure the packaging is undamaged!
- ▶ Inform the supplier about any damage to the packaging.
Keep the damaged packaging until the matter has been settled.
- ▶ Make sure the contents are undamaged!
- ▶ Inform the supplier about damage to the contents. Keep the damaged products until the matter has been settled.
- ▶ Check that the order is complete and agrees with your shipping documents.
- ▶ The packaging material used to store or to transport the product must provide shock protection and humidity protection. The original packaging offers the best protection. Also, keep to the approved ambient conditions (see "Technical data").
- ▶ If you have any questions, please contact your supplier or your local sales center.

2.2 Scope of delivery

The delivery of the field instrument includes:

- 1 transmitter COM253
- 1 plug-in screw terminal
- 1 cable gland Pg 7
- 1 cable gland Pg 16 reduced
- 2 cable glands Pg 13.5
- 1 Operating Instructions BA00199C/07/EN
- 1 Operating Instructions
 - versions with HART communication:
 - 1 Operating Instructions Field Communication with HART, BA00208C/07/EN
 - versions with PROFIBUS communication:
 - 1 Operating Instructions Field Communication with PROFIBUS PA/DP, BA00209C/07/EN

The delivery of the panel mounted instrument includes:

- 1 transmitter COM223
- 1 set of plug-in screw terminals
- 2 tensioning screws
- 1 BNC-plug (solder-free)
- 1 Operating Instructions BA00199C/07/EN
- 1 Operating Instructions
 - versions with HART communication:
 - 1 Operating Instructions Field Communication with HART, BA00208C/07/EN
 - versions with PROFIBUS communication:
 - 1 Operating Instructions Field Communication with PROFIBUS PA/DP, BA00209C/07/EN

If you have any questions, please contact your supplier or your local sales center.

2.3 Product identification

2.3.1 Nameplate

The nameplate contains the following information:

- Manufacturer data
- Order code
- Extended order code
- Serial number
- Operating conditions
- Safety icons

Compare the order code on the nameplate with your order.

2.3.2 Identifying the product

The order code and serial number of your device can be found in the following locations:

- On the nameplate
- In the delivery papers

 To find out the version of your device, enter the order code indicated on the nameplate in the search screen at the following address: www.products.endress.com/order-ident

2.4 Certificates and approvals

2.4.1 CE mark

Declaration of conformity

The product meets the requirements of the harmonized European standards. It thus complies with the legal requirements of the EC directives.

The manufacturer confirms successful testing of the product by affixing the **CE** symbol.

2.4.2 CSA general purpose

CSA General Purpose

The products listed below are eligible to bear the CSA Mark shown with adjacent indicators "C" and "US":

Version	Approval
COM253-..2... COM253-..3... COM253-..7...	CSA Mark for Canada and USA
COM223-..2... COM223-..3... COM223-..7...	CSA Mark for Canada and USA

3 Installation

3.1 Quick installation guide

Proceed as follows to completely install the measuring point:

- Install the transmitter (see "Installation instructions" section).
- If the sensor is not yet installed in the measuring point, install it (see Technical Information of the sensor).
- Connect the sensor to the transmitter as illustrated in the "Electrical connection" section.
- Connect the transmitter as illustrated in the "Electrical connection" section.
- Commission the transmitter as explained in the "Commissioning" section.

3.1.1 Measuring system

A complete measuring system comprises:

Variant 1 (DX/DS with COS41)

- The transmitter Liquisys M COM223 or COM253 in version DX or DS
- An oxygen sensor COS41
- An immersion, flow or retractable assembly

Options: extension cable CMK, junction box VBM

Variant 2 (WX/WS with COS31, COS61 or COS71)

- The transmitter Liquisys M COM223 or COM253 in version WX or WS
- An oxygen sensor COS31, COS61 or COS71
- An immersion, flow or retractable assembly

Options: extension cable OMK, junction box VS

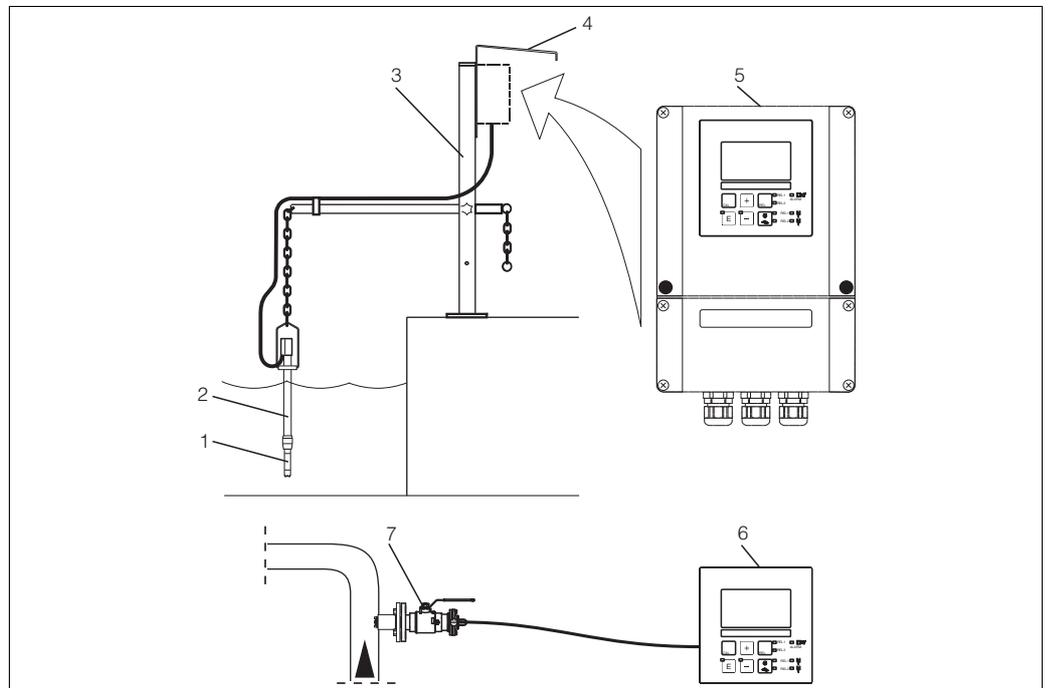


Fig. 1: Complete measuring system Liquisys M COM223/253

- | | |
|--|-------------------------------|
| 1 Oxygen sensor | 5 Liquisys M COM253 |
| 2 Immersion assembly CYA611 | 6 Liquisys M COM223 |
| 3 Universal hanging assembly holder CYH101 | 7 Retractable assembly COA451 |
| 4 Weather protection cover CYY101 | |

C07-COM2x3xx-14-06-00-xx-002.eps

3.2 Installation conditions

3.2.1 Field instrument

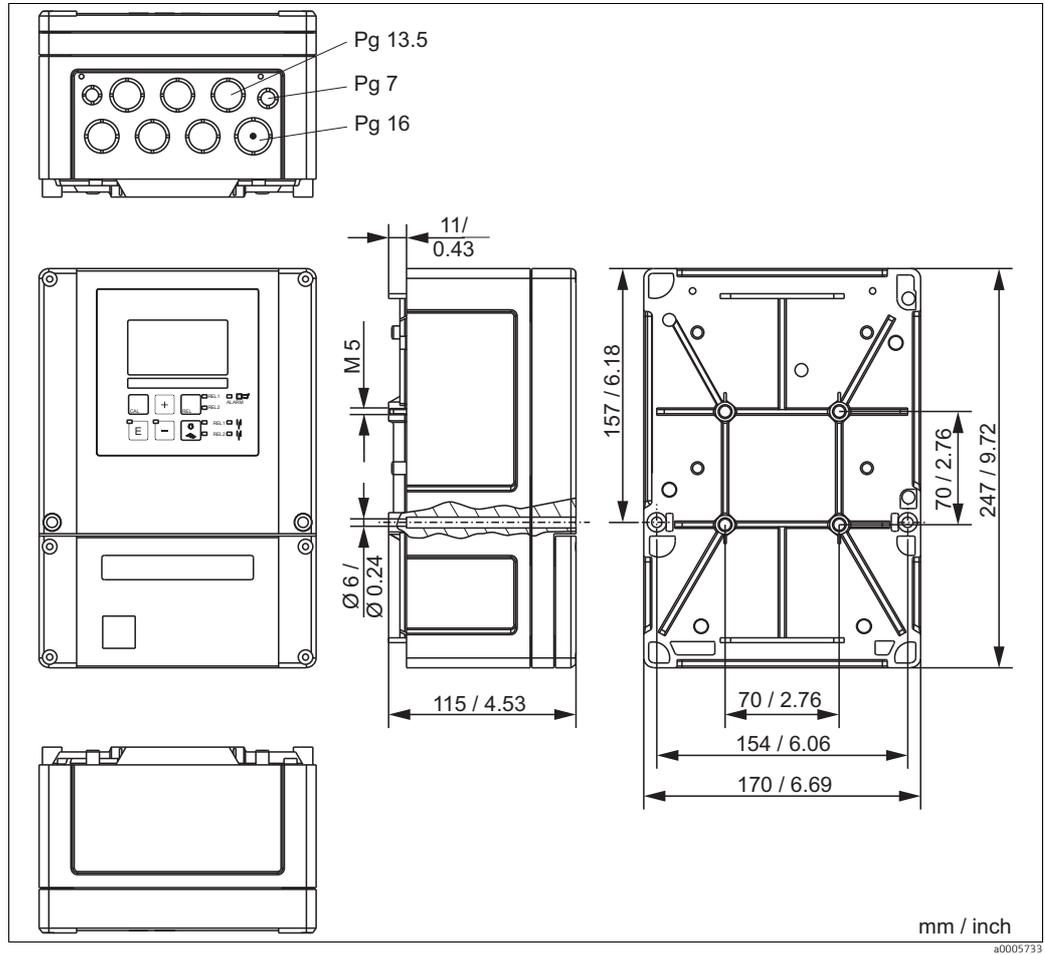
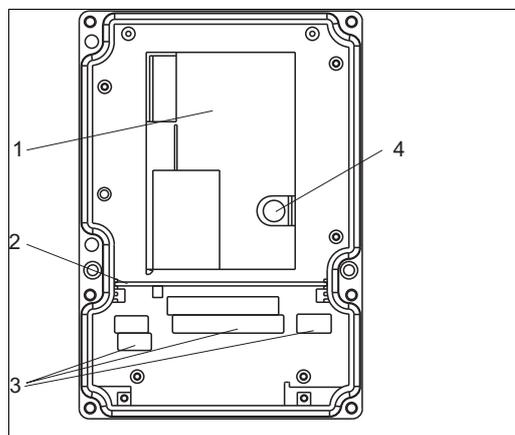


Fig. 2: Field instrument

i There is a hole in the punching for the cable entry (connection of supply voltage). It serves as a pressure balance during air freight dispatching. Make sure no moisture penetrates the inside of the housing before the cable installation. The housing is completely air-tight after the cable installation.



- 1 Removable electronics box
- 2 Partition plate
- 3 Terminals
- 4 Fuse

Fig. 3: View into the field housing

3.2.2 Panel-mounted instrument

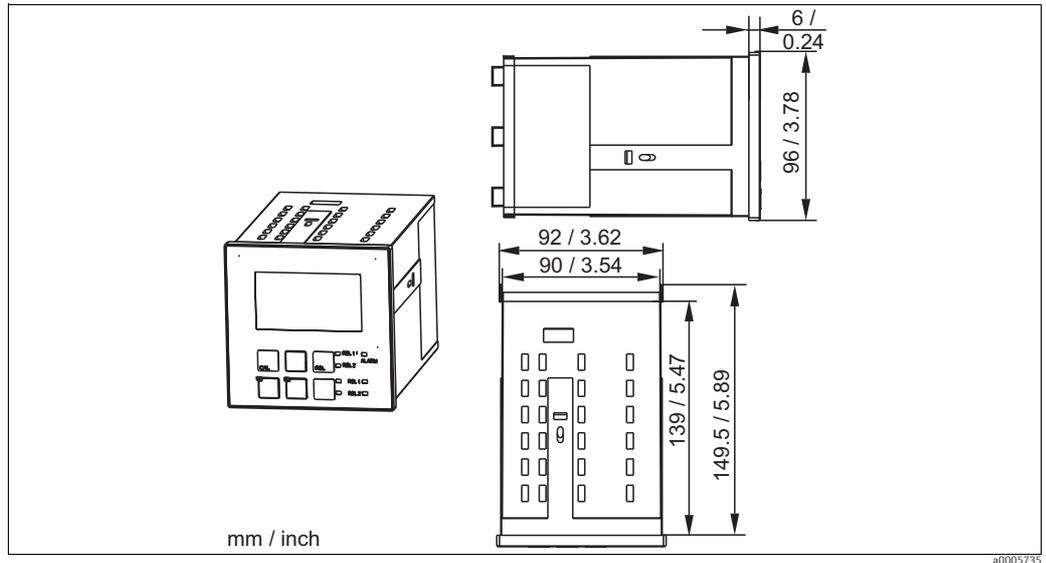


Fig. 4: Panel-mounted instrument

a0005735

3.3 Installation instructions

3.3.1 Field instrument

There are several ways of securing the field housing:

- Wall mounting with fixing screws
- Post mounting to cylindrical pipes
- Post mounting to square securing masts

NOTICE

Effect of climate conditions (rain, snow, direct sun etc.)

Impaired operation to complete transmitter failure

- ▶ When installing outside, always use the weather protection cover (accessory).

Transmitter wall mounting

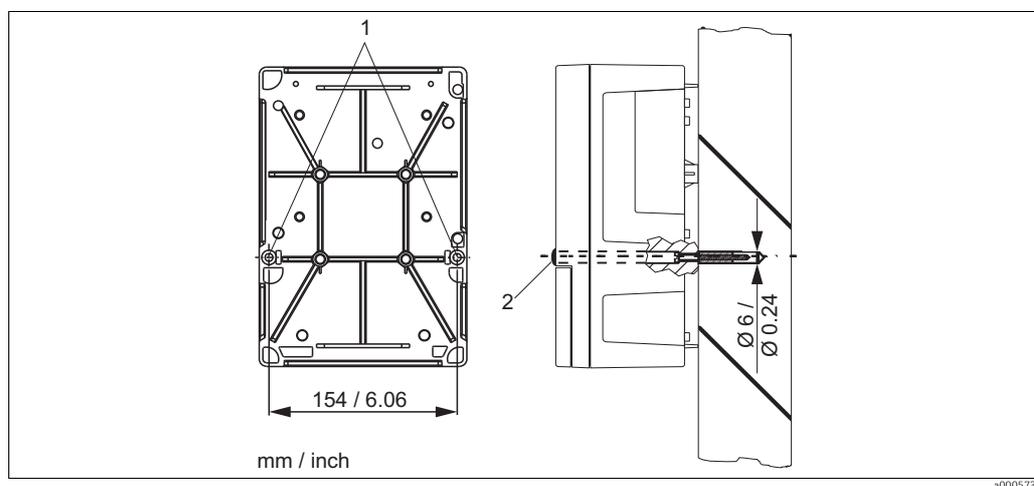


Fig. 5: Wall mounting field device

For wall mounting the transmitter, proceed as follows:

1. Drill the bores as shown in → 5.
2. Drive the two fixing screws through the securing bores (1) from the front.
3. Mount the transmitter on the wall as shown.
4. Cover the bores with plastic caps (2).

Transmitter post mounting

- i** You require a post mounting kit to secure the field device to horizontal and vertical posts or pipes (max. \varnothing 60 mm (2.36")). The kit can be acquired as an accessory (see "Accessories" section).

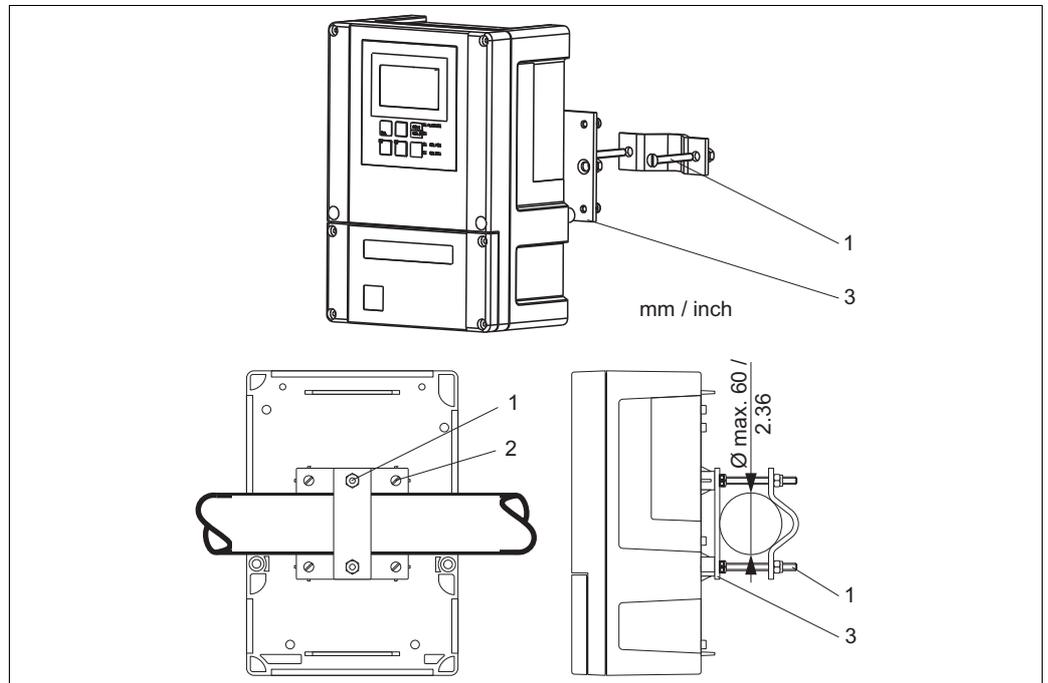


Fig. 6: Post mounting field device to cylindrical pipes

For post mounting the transmitter, proceed as follows:

1. Guide the two securing screws (1) of the mounting kit through the openings of the securing plate (3).
2. Screw the securing plate onto the transmitter using the four fixing screws (2).
3. Secure the retainer with the field device on the post or pipe using the clip.

You can also secure the field device to a square universal post in conjunction with the weather protection cover. These can be acquired as accessories, see "Accessories" section.

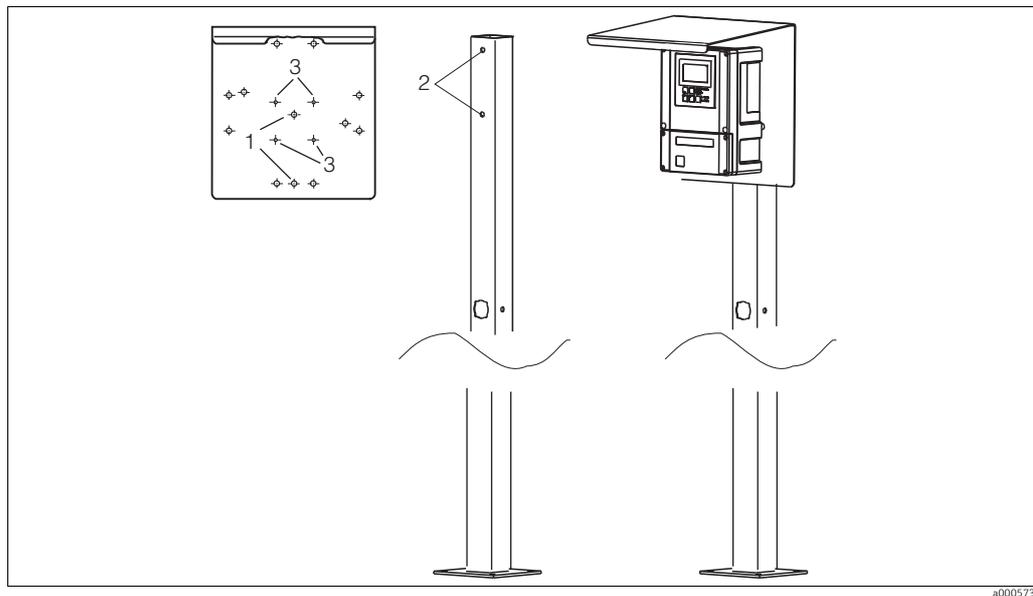


Fig. 7: Mounting field device with universal posts and weather protection cover

For mounting the weather protection cover, proceed as follows:

1. Screw the weather protection cover with 2 screws (bores 1) to the upright post (bores 2).
2. Secure the field device to the weather protection cover. To do so, use the bores (3).

3.3.2 Panel-mounted instrument

The panel-mounted instrument is secured with the clamping screws supplied (see →  8). The necessary installation depth is approx. 165 mm (6.50").

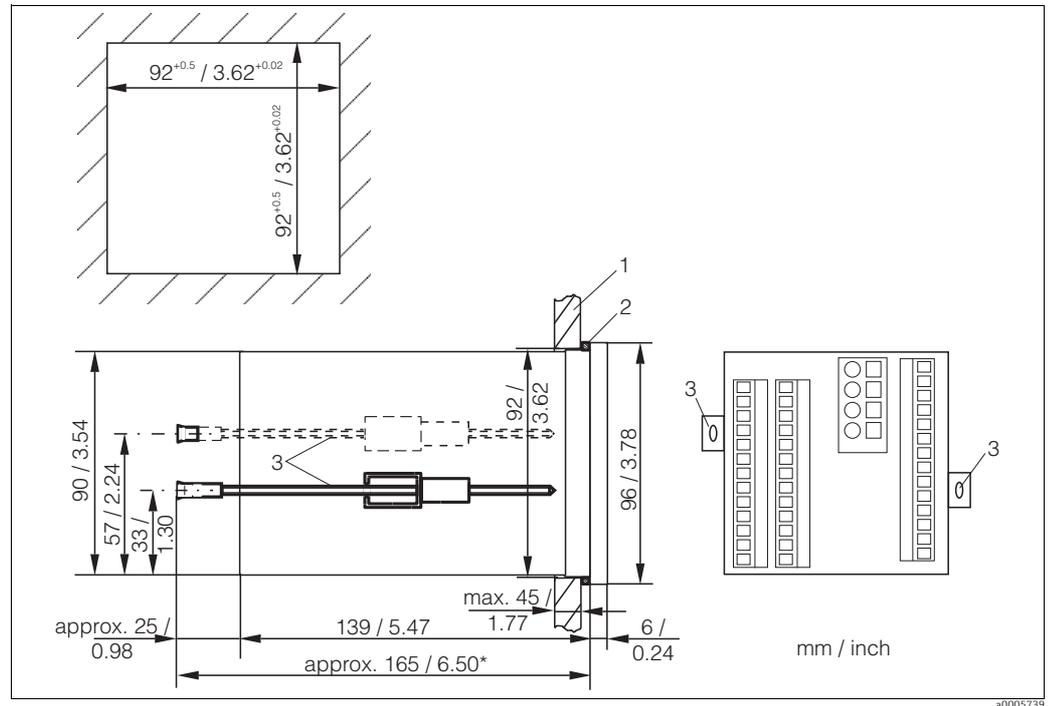


Fig. 8: Securing the panel-mounted instrument

- 1 Wall of the cabinet
- 2 Seal
- 3 Clamping screws
- * Required installation depth

3.4 Post-installation check

- After installation, check the transmitter for damage.
- Check whether the transmitter is protected against moisture and direct sunlight (e.g. by the weather protection cover).

4 Electrical connection

⚠ WARNING

Device is energized

Improper connection can cause injury or death.

- ▶ The electrical connection must only be carried out by a certified electrician.
- ▶ Technical personnel must have read and understood the instructions in this manual and must adhere to them.
- ▶ **Prior to beginning** any wiring work, make sure voltage is not applied to any of the cables.

4.1 Wiring

NOTICE

The device does not have a power switch

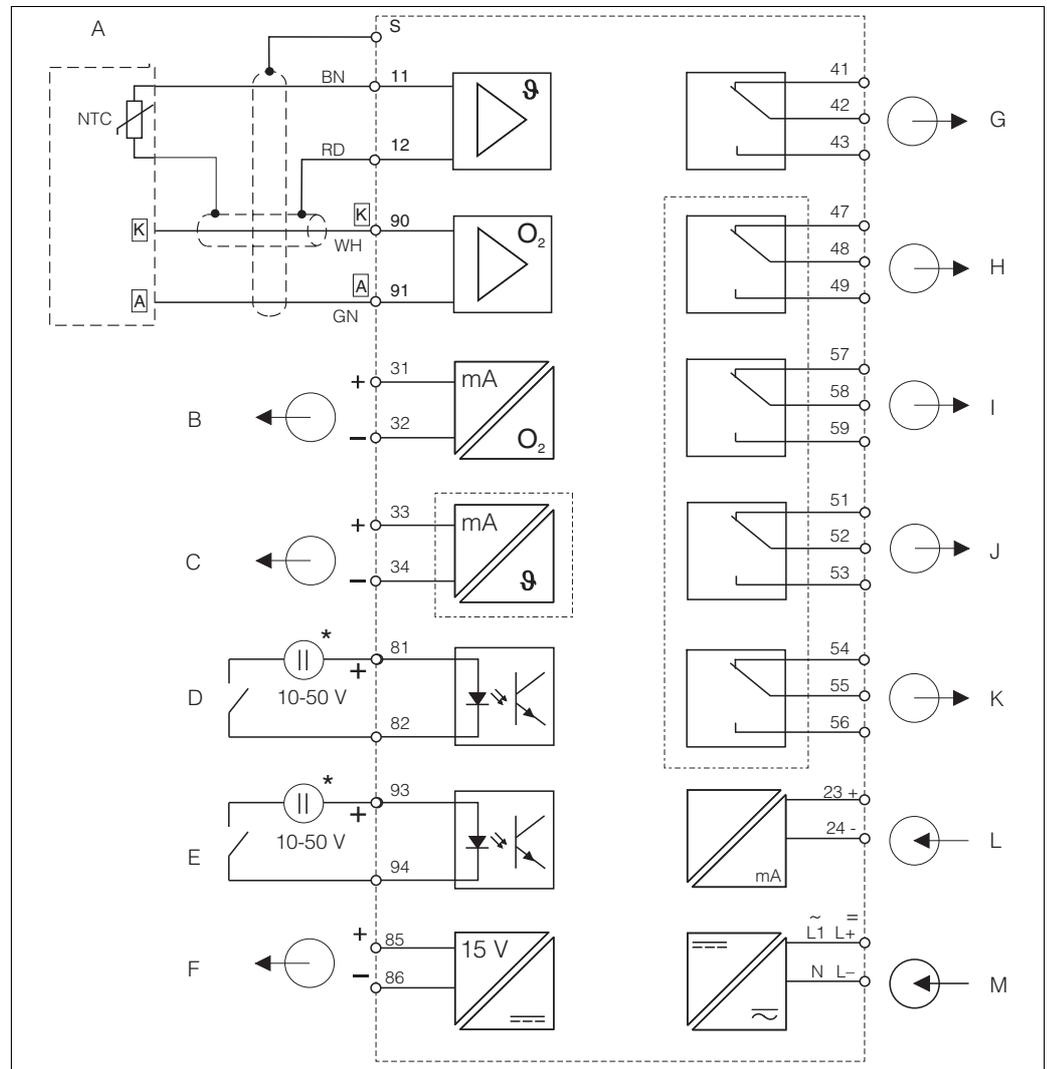
- ▶ You must provide a protected circuit breaker in the vicinity of the device.
- ▶ This must be a switch or a power-circuit breaker and you must label it as the circuit breaker for the device.
- ▶ At the supply point, the power supply for the 24 V versions must be isolated from dangerous live cables by double or reinforced insulation.

The electrical connection of the transmitter differs depending on the device version:

- If you are using the device version DX/DS (with COS41), please read the instructions in the "Electrical connection variant 1" section.
- If you are using the device version WX/WS (with COS31, COS61 or COS71), please read the instructions in the "Electrical connection variant 2" section.

4.1.1 Electrical connection variant 1 (DX/DS with COS41)

The wiring diagram depicted in →  9 shows the connections of the transmitter with all the options.



C07-COM2x3xx-04-06-00-xx-001.eps

Fig. 9: Electrical connection of the transmitter in version DX or DS

- | | | | |
|---|--|---|---|
| A | Oxygen sensor COS41 | G | Alarm (current-free contact position) |
| B | Signal output 1 oxygen | H | Relay 1 (current-free contact position) |
| C | Signal output 2 temperature/controller | I | Relay 2 (current-free contact position) |
| D | Binary input 1 (Hold) | J | Relay 3 (current-free contact position) |
| E | Binary input 2 (Chemoclean) | K | Relay 4 (current-free contact position) |
| F | Aux. voltage output | L | Current input 4 ... 20 mA |
| | | M | Power supply |

* Aux. voltage output terminal 85/86 applicable

 The device is approved for protection class II and is generally operated without a protective earth connection. The circuits "C" and "F" are not galvanically isolated from each other.

Field instrument connection version DX/DS

To connect the field instrument proceed as follows:

1. Open the front cover to get access to the terminals.
2. Cut out the marked PG gland hole of the housing. Mount a PG gland and guide the measuring cable through the PG gland into the housing.
3. Connect the measuring cable in accordance with the connection diagram.
4. Fix the PG gland.

NOTICE**Nonobservance could cause incorrect measurement**

- ▶ Make sure to protect the connectors, cable ends and terminals against moisture.
- ▶ Terminals marked NC may not be wired.
- ▶ Unmarked terminals may not be wired.

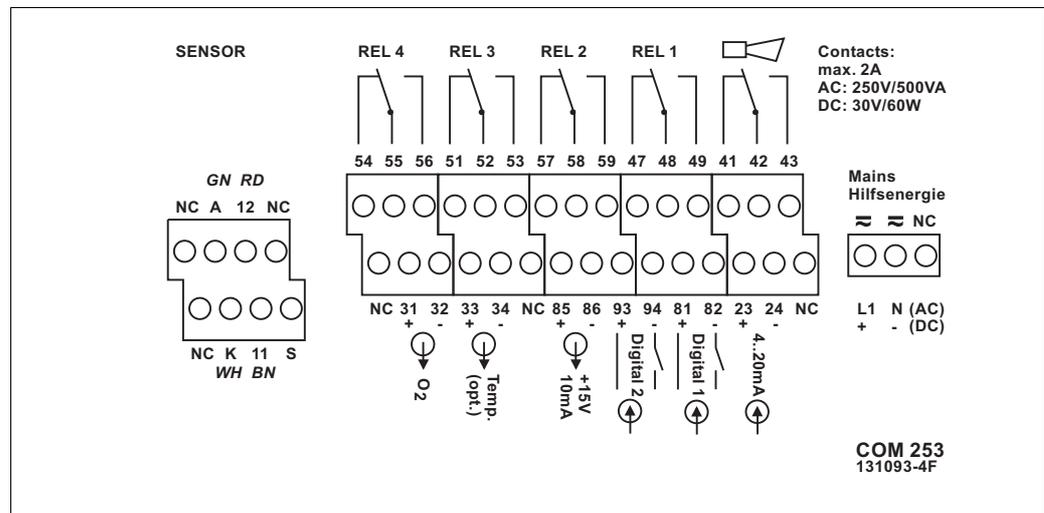


Fig. 10: Field instrument connection compartment sticker

 Please label the sensor terminal block with the sticker provided.

Panel-mounted instrument connection

Connect the cables in accordance with the connection diagram.

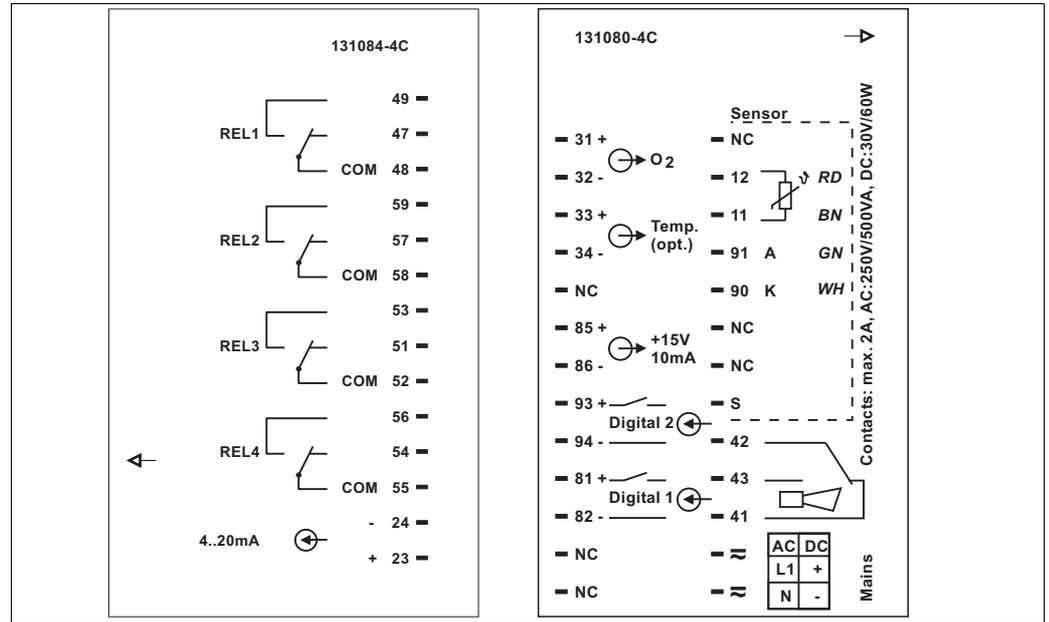


Fig. 11: Panel mounted instrument connection sticker

NOTICE

Nonobservance could cause incorrect measurement

- ▶ Make sure to protect the connectors, cable ends and terminals against moisture.
- ▶ Terminals marked NC may not be wired.
- ▶ Unmarked terminals may not be wired.

Measuring cable and sensor connection

You require screened special measuring cables to connect oxygen sensor COS41 to the transmitter. To extend the measuring cable, use junction box and extension cable:

Sensor	Sensor cable	Extension
COS41	CYK71	VBM junction box + CYK71 cable

You can also use measuring cable CMK.

Maximum cable length	
COS41	50 m (164 ft) with CMK / CYK71 cable

Structure of the measuring cable

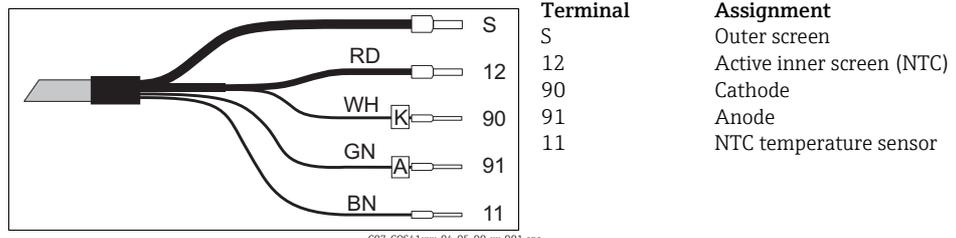


Fig. 12: Measuring cable CMK or CYK71

i For further information on cables and junction boxes refer to chapter "Accessories".

Example of connecting an oxygen sensor

Connection of the oxygen sensor COS41:

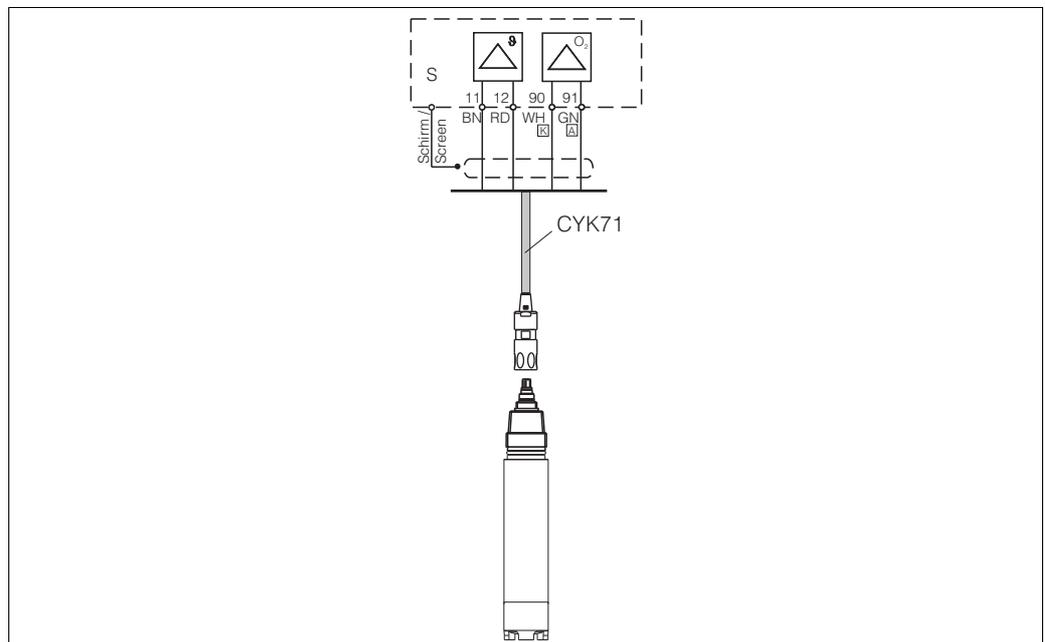


Fig. 13: Connection of COS41 with CYK71 cable

4.1.2 Electrical connection variant 2 (WX/WS with COS31/71)

The wiring diagram depicted in → Fig. 14 shows the connections of the transmitter with all the options.

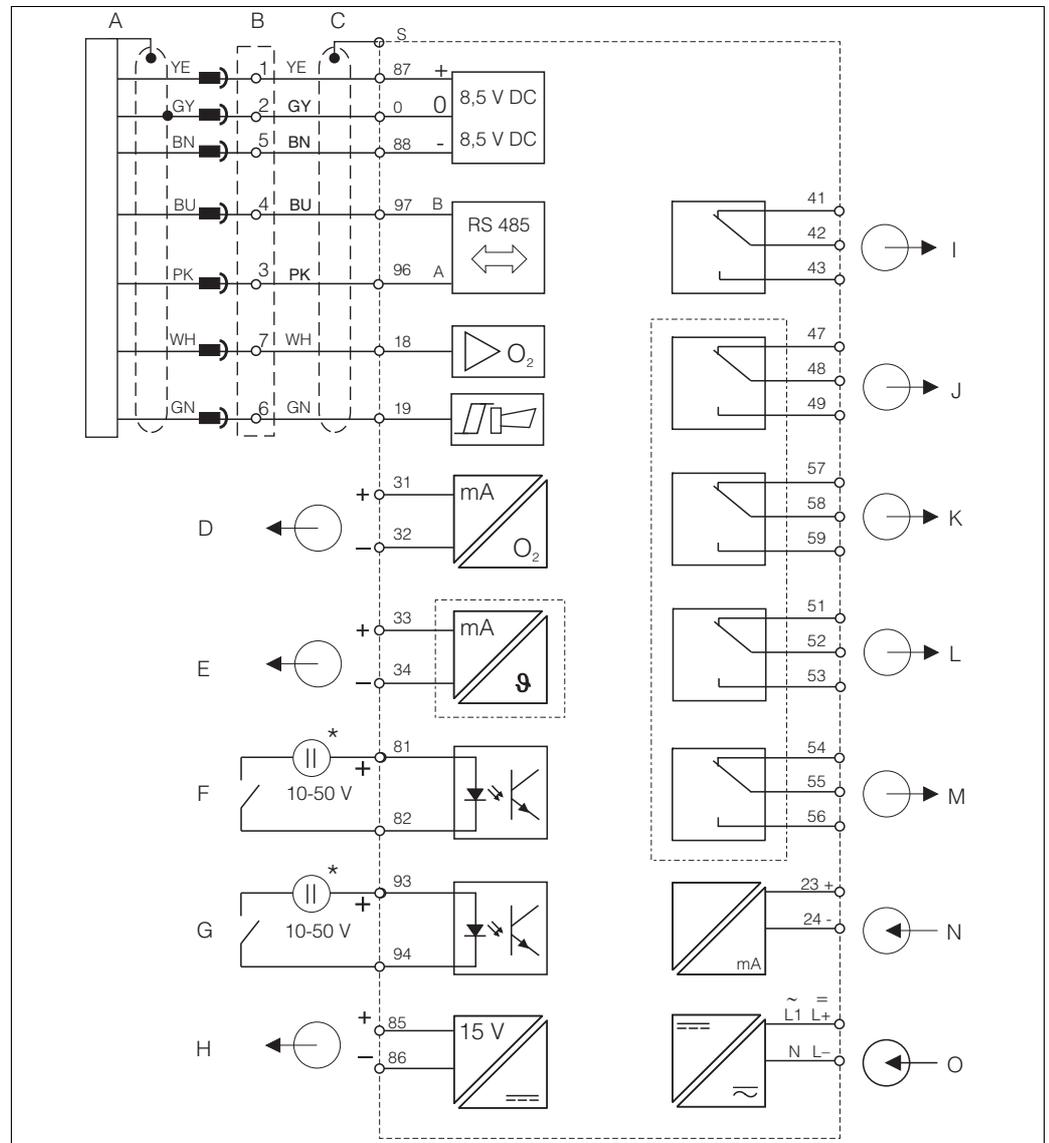


Fig. 14: Electrical connection of the transmitter version WX or WS

A	Oxygen sensor COS31/61/71	H	Aux. voltage output
B	Junction box VS with extension	I	Alarm (current-free contact position)
C	COM253: Plug connection for oxygen sensor COM223: the sensor cable plug must be removed or junction box VS used	J	Relay 1 (current-free contact position)
D	Signal output 1 oxygen	K	Relay 2 (current-free contact position)
E	Signal output 2 temperature/controller	L	Relay 3 (current-free contact position)
F	Binary input 1 (Hold)	M	Relay 4 (current-free contact position)
G	Binary input 2 (Chemoclean)	N	Current input 4 ... 20 mA
		O	Power supply

* Aux. voltage output terminal 85/86 applicable

Pay attention to the following:

- The device is approved for protection class II and is generally operated without a protective earth connection.
- The circuits "E" and "H" are not galvanically isolated from each other.
- The signals "Sensor signal" (18) and "Alarm" (19) are not used at the TOP68 version.

Field instrument connection

For connection, the measuring cables are introduced through the cable glands on the field instrument and connected according to the following diagram. The sensor is plugged in from the outside (7-pin socket SXB).

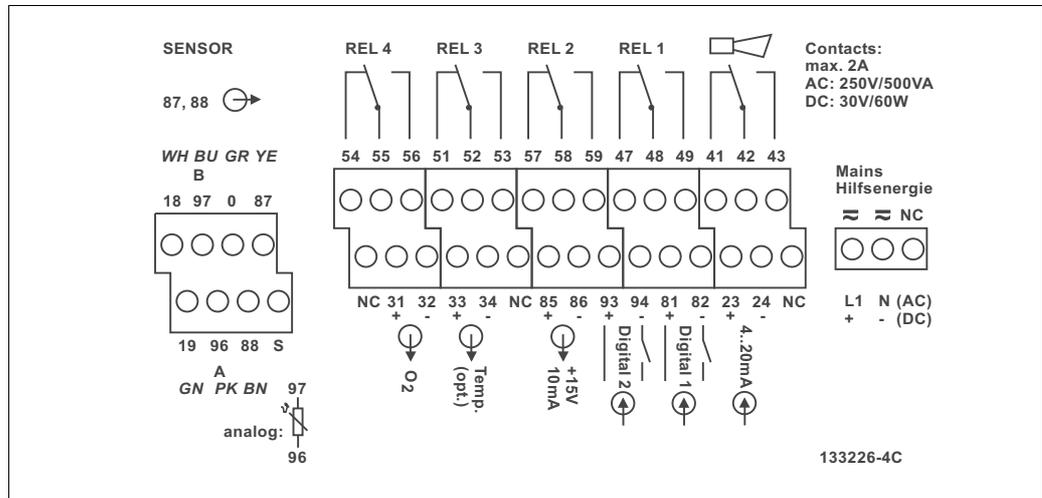


Fig. 15: Field instrument connection compartment sticker version WX/WS

NOTICE

Nonobservance could cause incorrect measurement

- ▶ Terminals marked NC may not be wired.
- ▶ Unmarked terminals may not be wired.

i Please label the sensor terminal block with the sticker provided.

Panel-mounted instrument connection

To connect a sensor to the panel mounted instrument you have to take off the sensor plug. Connect the cable conductors directly to the terminals of the transmitter. If you need a pluggable connection you can install a VS junction box between sensor and transmitter.

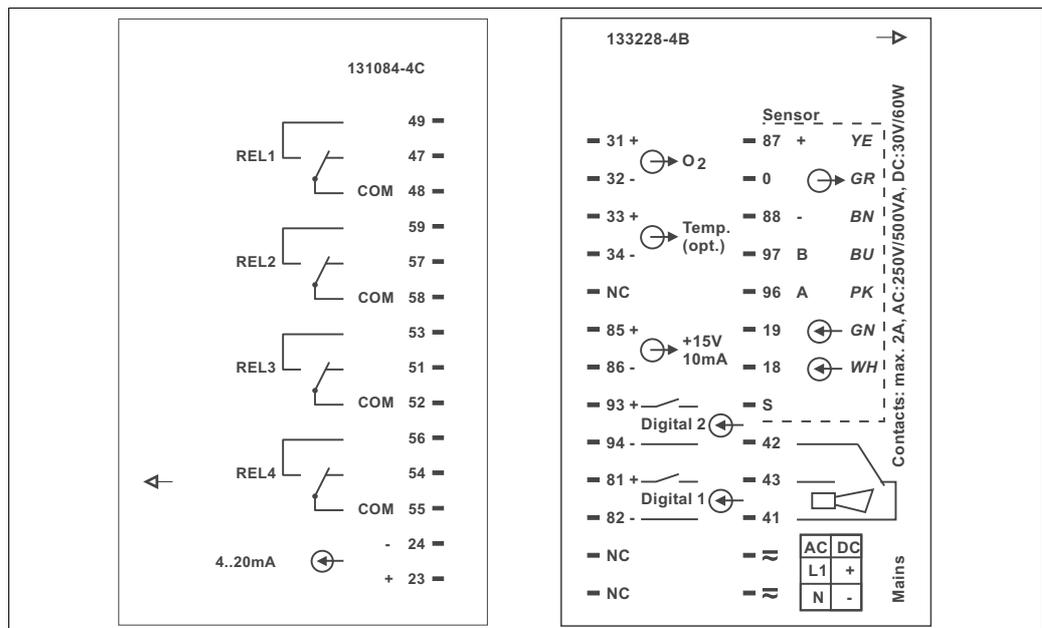


Fig. 16: Panel mounted instrument connection sticker

NOTICE

Nonobservance could cause incorrect measurement

- ▶ Terminals marked NC may not be wired.
- ▶ Unmarked terminals may not be wired.

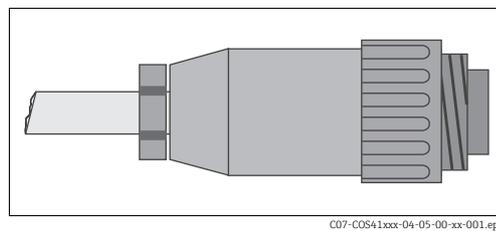
Measuring cable and sensor connection

To extend the measuring cable you require a junction box and an extension cable:

Sensor	Sensor cable	Extension
COS31/61/71 with fixed cable connection	OMK with SXP plug	VS junction box + OMK cable
COS31/61/71 with TOP68 connection	CYK71 with SXP plug	VS junction box + OMK cable

Maximum cable length	
COS31/61/71	100 m (328 ft) with OMK / CYK71 cable

Pin assignment of the SXP plug with OMK cable



	OMK		CYK
1 yellow	+UB	+UB	yellow
2 grey	0 V	0 V	white
3 pink	RS 485 (NTC)	RS 485 (NTC)	green
4 blue	RS 485 (NTC)	RS 485 (NTC)	brown
5 brown	-UB	-UB	coax inner
6 green	Alarm	NC	
7 white	Sensor signal	NC	

Fig. 17: Sensor plug with special measuring cable OMK

i For further information on cables and junction boxes refer to chapter "Accessories".

Example of connecting an oxygen sensor

Connection of the oxygen sensor COS31/61/71.

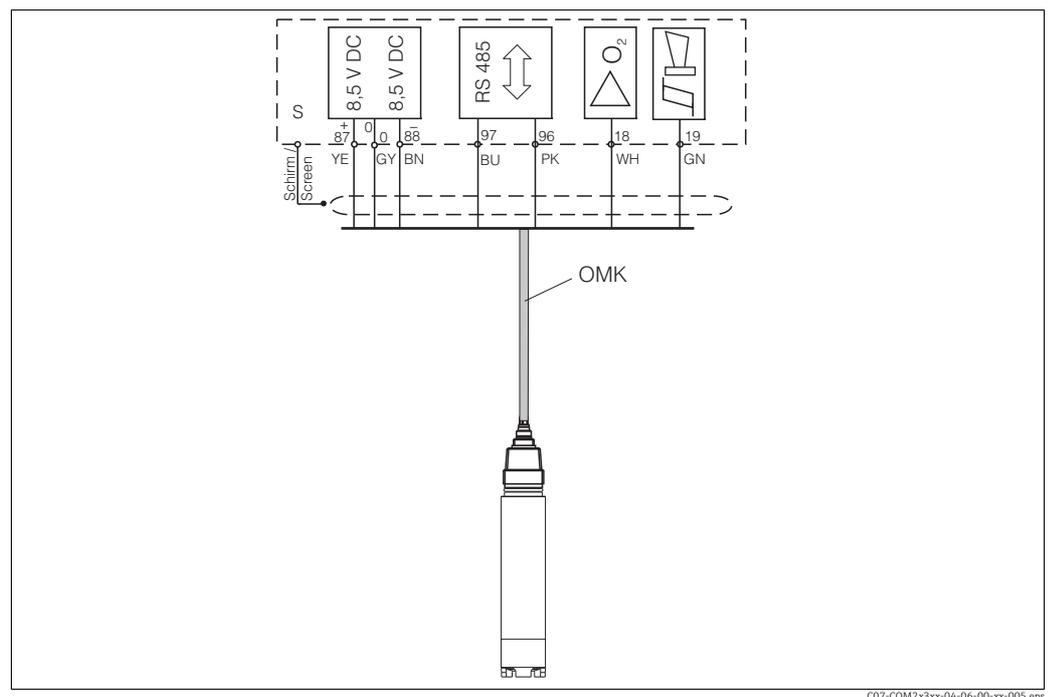


Fig. 18: Connection of COS31/71 with OMK cable

i The signals **Sensor signal** and **Alarm** are not used by COS61 and the TOP68-versions.

4.1.3 Alarm contact

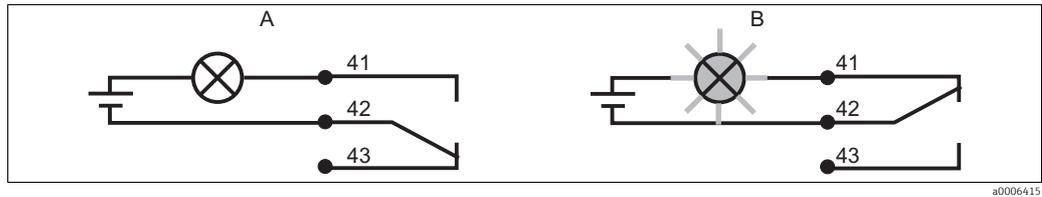


Fig. 19: Recommended fail-safe switching for the alarm contact

A Normal operating status

B Alarm condition

Normal operating status:

Device in operation and no error message present (alarm LED off)

- Relay energized
- Contact 42/43 closed

Alarm condition

Error message present (alarm LED red) or device defective or voltage-free (alarm LED off)

- Relay de-energized
- Contact 41/42 closed

4.2 Post-connection check

After the electrical connection, carry out the following checks:

Device condition and specifications	Notes
Are the transmitter and cables damaged on the outside?	Visual inspection

Electrical connection	Notes
Are the mounted cables strain relieved?	
Cable run without loops and cross-overs?	
Are the signal lines correctly connected in accordance with the wiring diagram?	
Are all screw terminals tightened?	
Are all cable entries installed, tightened and sealed?	

5 Operability

5.1 Quick operation guide

You have the following ways of operating the transmitter:

- On site via the key field
- Via the HART interface (optional, with corresponding order version) per:
 - HART handheld terminal or
 - PC with HART modem and the FieldCare software package
- Via PROFIBUS PA/DP (optional, with corresponding order version) with:
 - PC with corresponding interface and the FieldCare software package (see Accessories) or
 - via a programmable logic controller (PLC)

 For operation via HART or PROFIBUS PA/DP, please read the relevant sections in the additional Operating Instructions:


- PROFIBUS PA/DP, field communication for Liquisys M CXM223/253, BA00209C/07/EN
- HART, field communication for Liquisys M CXM223/253, BA00208C/07/EN

The following section only explains operation via the keys.

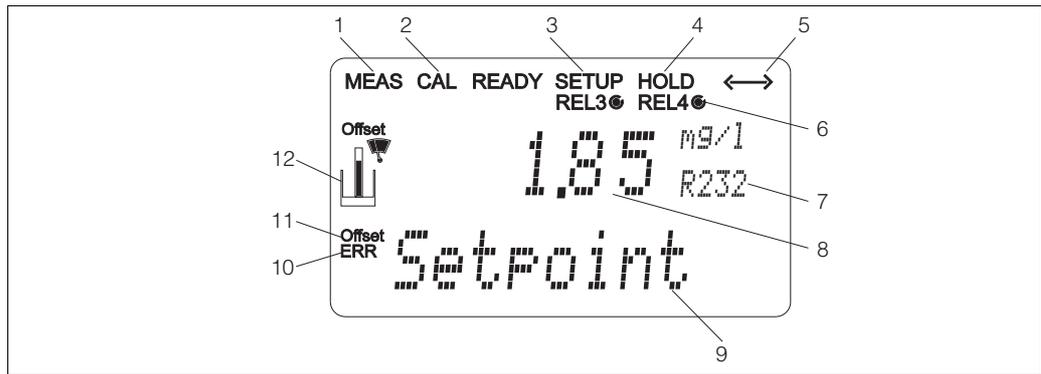
5.2 Display and operating elements

5.2.1 Display

LED display

	Indicates the current operating mode, "Auto" (green LED) or "Manual" (yellow LED)
	Indicates the activated relay in the "Manual" mode (red LED)
	Indicates the working status of relay 1 and 2 LED green: measured value within the permitted limit, relay inactive LED red: measured value outside the permitted limit, relay active
	Alarm display, e.g. for continuous limit value overshoot, temperature sensor failure or system error (see error list)

LC display

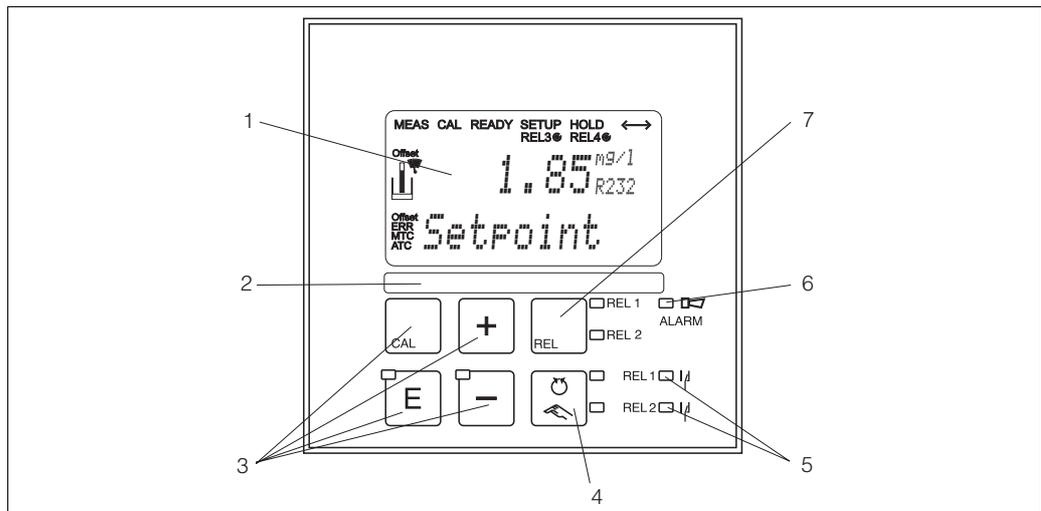


C07-COM2x3xx-07-06-00-en-001.eps

Fig. 20: LC display of transmitter

- | | | | |
|---|--|----|---|
| 1 | Indicator for measuring mode (normal operation) | 7 | Function code display |
| 2 | Indicator for calibration mode | 8 | In measuring mode: measured variable |
| 3 | Indicator for setup mode (configuration) | | In setup mode: configured variable |
| 4 | Indicator for "Hold" mode (current outputs remain at last current state) | 9 | In measuring mode: secondary measured value |
| 5 | Indicator for receipt of a message for devices with communication | | In setup/calibr. mode: e.g. setting value |
| 6 | Indicator of working status of relays 3/4:
○ inactive, ● active | 10 | "Error": error display |
| | | 11 | Temperature offset |
| | | 12 | Sensor symbol |

5.2.2 Operating elements






C07-COM2x3xx-19-06-00-en-001.eps

Fig. 21: Operating elements

- | | |
|---|---|
| 1 | LC display for displaying the measured values and configuration data |
| 2 | Field for user labelling |
| 3 | 4 main operating keys for calibration and device configuration |
| 4 | Changeover switch for automatic/manual mode of the relays |
| 5 | LEDs for limit contactor relay (switch status) |
| 6 | LED for alarm function |
| 7 | Display of the active contact and key for relay changeover in manual mode |

5.2.3 Key assignment

	<p>CAL key When you press the CAL key, the device first prompts you for the calibration access code:</p> <ul style="list-style-type: none"> ▪ Code 22 for calibration ▪ Code 0 or any other code for reading the last calibration data <p>Use the CAL key to accept the calibration data or to switch from field to field within the calibration menu.</p>
	<p>ENTER key When you press the ENTER key, the device first prompts you for the setup mode access code:</p> <ul style="list-style-type: none"> ▪ Code 22 for setup and configuration ▪ Code 0 or any other code for reading all configuration data. <p>The ENTER key has several functions:</p> <ul style="list-style-type: none"> ▪ Calls up the Setup menu from the measuring mode. ▪ Saves (confirms) data entered in the setup mode. ▪ Moves on within function groups.
 	<p>PLUS key and MINUS key In the setup mode, the PLUS and MINUS keys have the following functions:</p> <ul style="list-style-type: none"> ▪ Selection of function groups. <ul style="list-style-type: none">  Press the MINUS key to select the function groups in the order given in the "System configuration" section. ▪ Configuration of parameters and numerical values ▪ Operation of the relay in manual mode <p>In the measuring mode, you get the following sequence of functions by repeatedly pressing the PLUS key:</p> <ol style="list-style-type: none"> 1. Temperature display in F 2. Temperature display hidden 3. Measured value display in mg/l 4. Measured value display in %SAT 5. Measured value display in hPa 6. Sensor current in nA/mA 7. Current input signal in % 8. Current input signal in mA 9. Return to basic settings <p>In the measuring mode, the following is displayed in sequence by repeatedly pressing the MINUS key:</p> <ol style="list-style-type: none"> 1. Current errors are displayed in rotation (max. 10). 2. Once all the errors have been displayed, the standard measurement display appears. In the function group F, an alarm can be defined separately for each error code.





 <p>REL 1 REL 2</p>	<p>REL key</p> <p>In the manual mode, you can use the REL key to switch between the relay and the manual start of cleaning.</p> <p>In the automatic mode, you can use the REL key to read out the switch-on points (for limit contactor) or set points (for PID controller) assigned to the relay in question.</p> <p>Press the PLUS key to jump to the settings of the next relay. Use the REL key to get back to the display mode (automatic return after 30 s).</p>
	<p>AUTO key</p> <p>You can use the AUTO key to switch between automatic mode and manual mode.</p>
	<p>Escape function</p> <p>If you press the PLUS and MINUS key simultaneously, you return to the main menu or are taken to the end of calibration if calibrating. If you press the PLUS and MINUS key again, you return to the measuring mode.</p>
	<p>Locking the keyboard</p> <p>Press the PLUS and ENTER key for at least 3 s to lock the keyboard against any unauthorized data entry. All the settings can continue to be read.</p> <p>The code prompt displays the code 9999.</p>
	<p>Unlocking the keyboard</p> <p>Press the CAL and MINUS key for at least 3 s to unlock the keyboard.</p> <p>The code prompt displays the code 0.</p>

5.3 Local operation

5.3.1 Automatic/manual mode

The transmitter normally operates in automatic mode. Here, the relays are triggered by the transmitter. In the manual mode, you can trigger the relays using the REL key or start the cleaning function.

How to change the operating mode:

	<p>1. The transmitter is in Automatic mode. The top LED beside the AUTO key is lit.</p>
	<p>2. Press the AUTO key.</p>
	<p>3. To enable the manual mode, enter the code 22 via the PLUS and MINUS keys. The bottom LED beside the AUTO key lights up.</p>
	<p>4. Select the relay or the function. You can use the REL key to switch between the relays. The relay selected and the switch status (ON/OFF) is displayed on the second line of the display. In the manual mode, the measured value is displayed continuously (e.g. for measured value monitoring for dosing functions).</p>
	<p>5. Switch the relay. It is switched on with PLUS and switched off with MINUS. The relay remains in its switched state until it is switched over again.</p>
	<p>6. Press the AUTO key to return to the measuring mode, i.e. to the automatic mode. All the relays are triggered again by the transmitter.</p>

Pay attention to the following:

- The selected operating mode remains in effect even after a power failure.
- The manual mode has priority over all automatic functions (Hold).
- Hardware locking is not possible in the manual mode.
- The manual settings are kept until they are actively reset.
- Error code E102 is signalled in the manual mode.

5.3.2 Operating concept

Operating modes

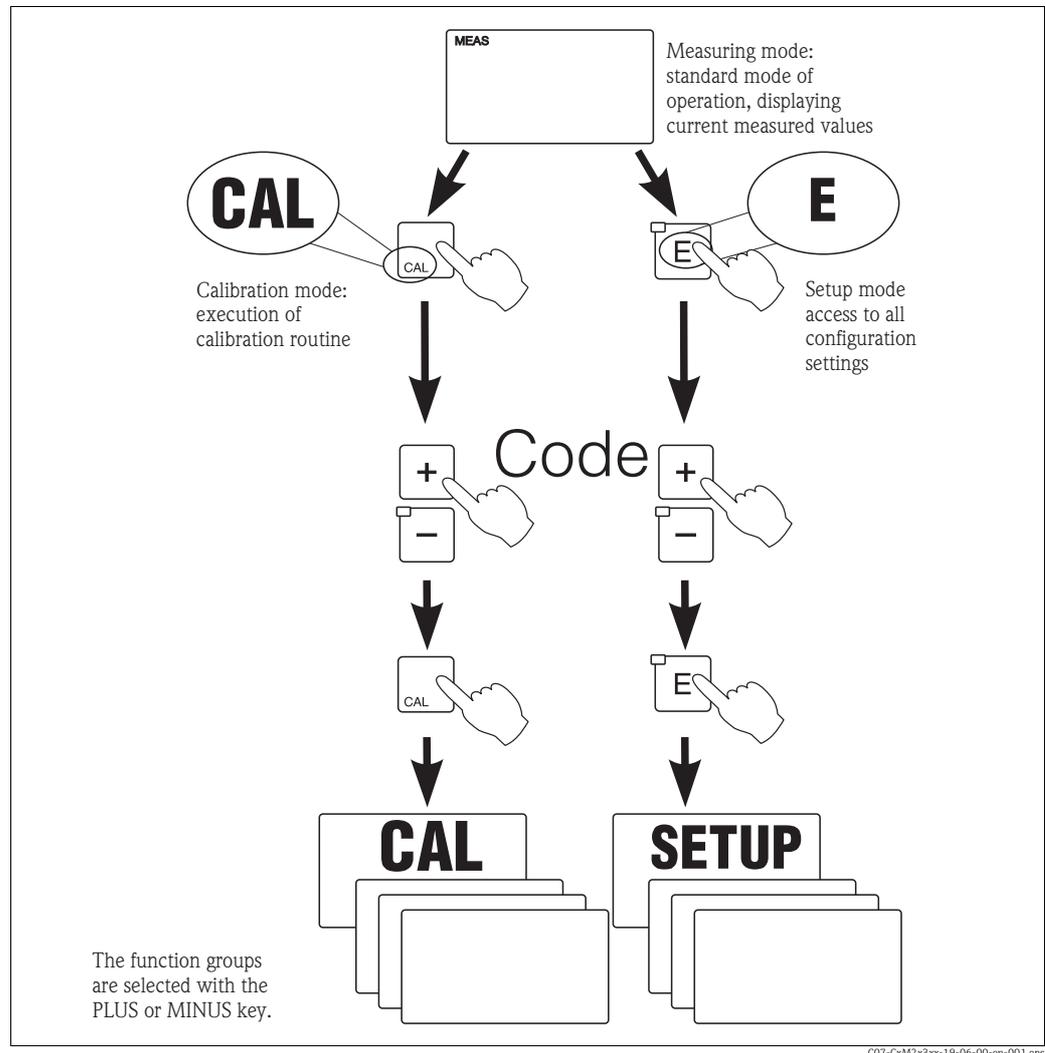


Fig. 22: Description of the possible operating modes

- i** If no key is pressed in the setup mode for approx. 15 min, the device automatically returns to the measuring mode. Any active Hold (Hold during setup) is reset.

Access codes

All device access codes are fixed and cannot be altered. When the device requests the access code, it distinguishes between different codes.

- **Key CAL + Code 22:** access to Calibration and Offset menu
- **Key ENTER + Code 22:** access to the setup menus
- **Keys PLUS + ENTER:** locks the keyboard
- **Keys CAL + MINUS:** unlocks the keyboard
- **Key CAL or ENTER + any code:** access to read mode, i.e. all the settings can be read but not modified.

The device continues measuring in the read mode. It does not shift to the Hold status. The current output and the controllers remain active.

Menu structure

The configuration and calibration functions are arranged in function groups.

- In setup mode, select a function group with the PLUS and MINUS keys.
 - In the function group itself, switch from function to function with the ENTER key.
 - Within the function, select the desired option with the PLUS and MINUS keys or edit the settings with these keys. Then confirm with the ENTER key and continue.
 - Press the PLUS and MINUS keys simultaneously (Escape function) to exit programming (return to the main menu).
 - Press the PLUS and MINUS simultaneously keys again to switch to the measuring mode.
- i** If a modified setting is not confirmed with ENTER, the old setting is retained.
An overview of the menu structure is provided in the Appendix to these Operating Instructions.

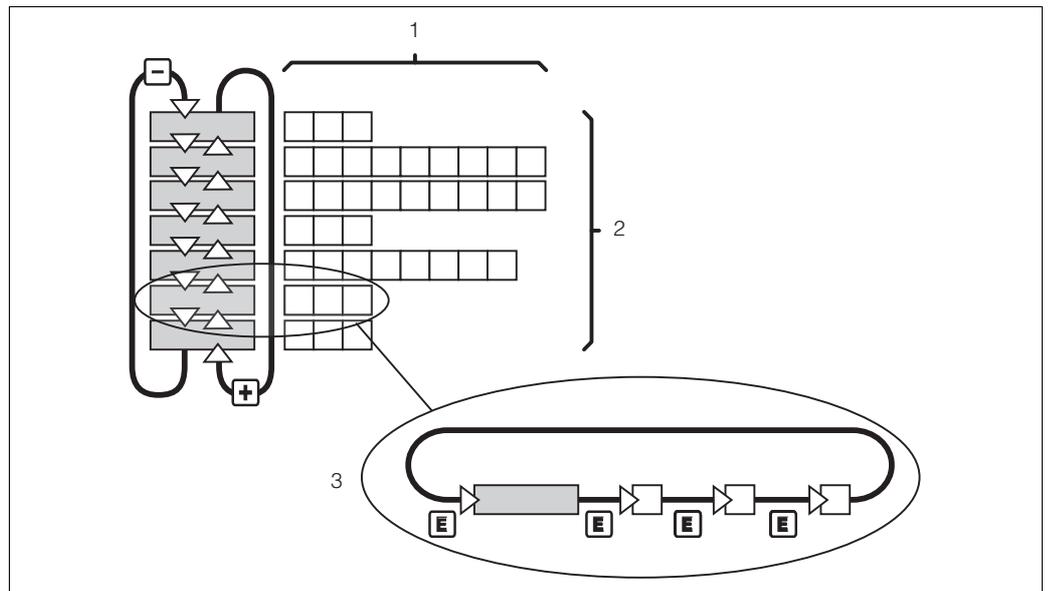


Fig. 23: Diagram of the menu structure

- 1 Functions (parameters selected, numbers entered)
- 2 Function groups, scroll backwards and forwards with the PLUS and MINUS keys
- 3 Switch from function to function with the ENTER key

Hold function: "freezing" of the outputs

During setup and calibration, the current output can be "frozen". It constantly retains its current status. "HOLD" appears on the display. If the controller actuating variable (steady control 4 to 20 mA) is output via current output 2, it is set to 0/4 mA in Hold.

Pay attention to the following:

- Hold settings can be found in the "Service" section.
- During Hold, all contacts will go to their normal positions.
- An active Hold has priority over all other functions.
- With every Hold, the I-component of the controller is set to zero.
- Any alarm delay is reset to "0".
- This function can also be activated externally via the Hold input (see Wiring diagram; binary input 1).
- The manual Hold (field S3) remains active even after a power failure.

6 Commissioning

6.1 Function check

▲ WARNING

Incorrect connection, incorrect supply voltage

Safety risks for staff and incorrect operation of the device

- ▶ Check that all connections have been established correctly in accordance with the wiring diagram.
- ▶ Make sure that the supply voltage matches the voltage indicated on the nameplate.

6.2 Switching on

Familiarize yourself with the operation of the transmitter before it is first switched on.

Please refer in particular to the "Safety instructions" and "Operation" sections.

After power-up, the device performs a self-test and then goes to the measuring mode.

Now calibrate the sensor in accordance with the instructions in the "Calibration" section.

i During commissioning, the sensor must be calibrated so that the measuring system can return precise measurement data.

Then perform the first configuration in accordance with the instructions in the "Quick start-up" section. The values set by the user are kept even in the event of a power failure.

The following function groups are available in the transmitter (the groups only available in the Plus Package are marked accordingly in the functional description):

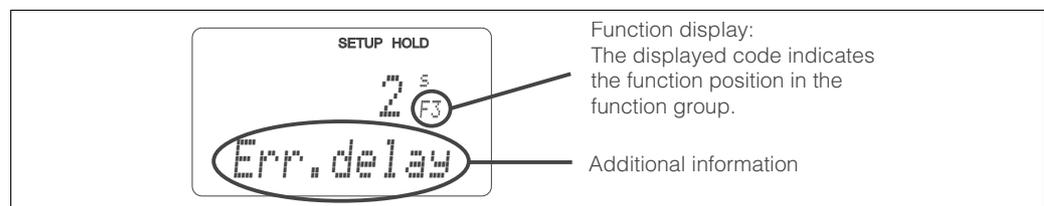
Setup mode

- SETUP 1 (A)
- SETUP 2 (B)
- CURRENT INPUT (Z)
- CURRENT OUTPUT (O)
- ALARM (F)
- CHECK (P)
- RELAY (R)
- SERVICE (S)
- E+H SERVICE (E)
- INTERFACE (I)

Calibration and offset mode

- CALIBRATION (C)

A detailed explanation of the function groups available in the transmitter can be found in the "System configuration" section.



C07-CLD132xx-07-06-00-en-003.eps

Fig. 24: Example for display in setup mode

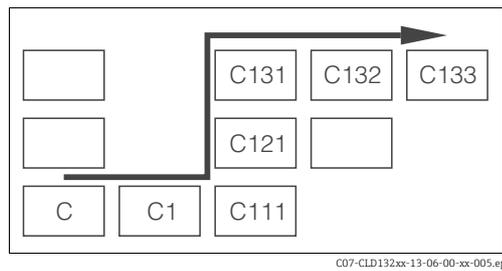


Fig. 25: Function coding

Selecting and locating functions is facilitated by a code displayed for each function in a special display field → 24.

The structure of this coding is given in → 25.

The first column indicates the function group as a letter (see group designations). The functions in the individual groups are counted from the top to the bottom and from the left to the right.

Factory settings

The first time it is switched on, the device has the factory setting for all functions. The table below provides an overview of the most important settings.









All other factory settings can be found in the description of the individual function groups in the "System configuration" section (the factory setting is highlighted in **bold**).

Function	Factory setting
Type of measurement	Oxygen concentration in mg/l Temperature in °C
Automatic pressure compensation*	Off (only with version WX/WS/DS)
Altitude	0 m above sea level
Salinity	0.0 % salt concentration
Current outputs 1* and 2*	4 to 20 mA
Current output 1: measured value for 4 mA signal current*	0.00 mg/l 0.000 mg/l (only with sensor COS71)
Current output 1: measured value for 20 mA signal current*	10.00 mg/l 10.000 mg/l (only with sensor COS71)
Current output 2: temperature value for 4 mA signal current*	0.0 °C (32 °F)
Current output 2: temperature value for 20 mA signal current*	40.0 °C (104 °F)
Alarm contact	Latching contact
Alarm delay	Setting in minutes
Error current for alarm	22 mA
Check functions*	Off. Can be switched on as required.
Setpoint for oxygen	5.00 mg/l 5.000 mg/l (only with sensor COS71)
Language	English

* For corresponding version

6.3 Quick start-up

After power-up, you must make some settings to configure the most important functions of the transmitter which are required for correct measurement. The following section gives an example of this.







User input	Setting range (Factory settings, bold)	Display
1. Press the [E] key. 2. Enter the code 22 to edit the setup. Press [E] .		
3. Press [−] until you get to the "Service" function group. 4. Press [E] to be able to make your settings.		 <p>SETUP HOLD 5 SERVICE</p>
5. In S1, select your language, e.g. "ENG" for English. Press [E] to confirm.	ENG = English GER = German FRA = French ITA = Italian NEL = Dutch ESP = Spanish	 <p>SETUP HOLD ENG S1 Language</p>
6. Press [+] simultaneously to exit the "Service" function group.		
7. Press [−] until you get to the "Setup 1" function group. 8. Press [E] to be able to make your settings for "Setup 1".		 <p>SETUP HOLD A SETUP 1</p>
9. In A1, select the desired mode of operation, e.g. "mg/l" = oxygen concentration. Press [E] to confirm.	mg/l %SAT hPA	 <p>SETUP HOLD mg/l A1 Unit</p>
10. In A2, select display unit and press [E] to confirm.	mg/l ppm ppb	 <p>SETUP HOLD mg/l A2 Unit</p>
11. In A3, switch automatic pressure compensation on or off (version WX/WS/DS). Compensation takes account of both the altitude dependent and the weather dependent proportion of the air pressure. Press [E] to confirm.	off on	 <p>SETUP HOLD off A3 PressComp</p>
12. In A4, enter altitude if automatic pressure compensation is not available (version DX) or switched off. Press [E] to confirm.	0 m 0 to 4000 m	 <p>SETUP HOLD 0 A4 Altitude</p>
13. In A5, enter measured value damping. Measured value damping causes averaging over the specified number of individual measured values. This is used for example, to stabilise the display if the measurement is unstable. Enter "1" if no damping is required. Press [E] to confirm.	1 1 to 60	 <p>SETUP HOLD 1 A5 Damping</p>

User input	Setting range (Factory settings, bold)	Display
14. In A6, enter oxygen measuring range: COS41, COS61 or COS71: select "20 mg/l" / "200 %SAT" / "400 hPa" COS31: All measuring ranges possible Press [E] to confirm. Display returns to "Setup 1".	20 mg/l 60 mg/l 200 %SAT 600 %SAT 400 hPa 1200 hPa	<p>SETUP HOLD 20 mg/l A6 Range</p>
15. Press [←] to go to the "Setup 2" function group. 16. Press [E] to edit "Setup 2".		<p>SETUP HOLD B SETUP 2</p>
17. In B1, select salinity of the medium. Press [E] to confirm.	0.0 % 0.0 to 4.0 %	<p>SETUP HOLD 0.0 % B1 Salinity</p>
18. In B2, enter correct process temperature. Press [E] to confirm.	current meas. value -10 to 60 °C	<p>SETUP HOLD 0.0 °C B2 RealTemp</p>
19. The difference between measured and entered temperature will be displayed. Press [E] . The display returns to "Setup 2".	current meas. value -5.0 to 5.0 °C	<p>SETUP HOLD 0.0 °C B3 Temp. Offs</p>
20. Press [+] simultaneously to switch to the measuring mode.		

6.4 System configuration





6.4.1 Setup 1 (Oxygen)

In the SETUP 1 function group, you can change the operating mode and the sensor settings.

Coding	Field	Selection or range (factory settings bold)	Display	Info
A	Function group SETUP 1			Basic settings.
A1	Select operating mode	mg/l %SAT hPa		mg/l = oxygen concentration %SAT = oxygen saturation index hPa = oxygen partial pressure  Any change in operating mode causes an automatic reset of user settings. If the oxygen value only needs to read switch display using the PLUS key.
A2	Select display unit	mg/l ppm ppb		
A3	Switch automatic pressure compensation on or off	off on		Field only available with WX/WS or DS versions. The absolute air pressure is measured. Compensation takes account of both the altitude dependent and the weather dependent proportion of the air pressure.
A4	Enter altitude	0 m 0 to 4000m		Only available if the pressure compensation in A2 is switched off or not available.
A5	Enter measured value damping	1 1 to 60		Measured value damping causes averaging over the specified number of individual measured values. It is used, for example, to stabilise the display with applications that fluctuate a great deal. There is no damping if "1" is entered.
A6	Enter oxygen measuring range	20 mg/l, 20 ppm, 20000 ppb 60 mg/l, 60 ppm, 60000 ppb (depends on selected display unit) 200 % SAT 600 %SAT 400 hPa 1200 hPa		Sensor COS41/61/71: Measuring must be 0 to 20 mg/l (0 to 200 %SAT, 0 to 400 hPa) Sensor COS31: Both measuring ranges possible.

6.4.2 Setup 2 (Salinity and temperature)

In the SETUP 2 function group, you can change the salinity and the temperature settings.

Coding	Field	Selection of range (factory settings bold)	Display	Info
B	Function group SETUP 2		 The display shows 'SETUP HOLD' at the top, 'B' in the middle, and 'SETUP 2' at the bottom.	Setups for salinity and temperature.
B1	Enter salinity	0.0 % 0.0 to 4.0 %	 The display shows 'SETUP HOLD' at the top, '0.0%' with a small 'B1' below it in the middle, and 'Salinity' at the bottom.	Input of salinity.
B2	Enter correct process temperature	current meas. value -10.0 to 60.0 °C	 The display shows 'SETUP HOLD' at the top, '0.0 °C' with a small 'B2' below it in the middle, and 'RealTemp' at the bottom.	The display value can be edited. You can make an adjustment of max. ±5 °C. Due to the high accuracy, adjustment is not usually necessary.
B3	Displays temperature difference (offset)	Current offset -5.0 to 5.0 °C	 The display shows 'SETUP HOLD' at the top, '0.0 °C' with a small 'B3' below it in the middle, and 'Temp. Offs' at the bottom.	The offset is the difference between measured and entered temperature.

6.4.3 Current input

To use the "Current input" function group, you need a relay board with current input which is not part of the basic version. With this function group you can monitor process parameters and use these for feedforward control. For this purpose, you must connect the current output of an external measured variable (e.g. flowmeter) to the 4 to 20 mA input of the transmitter. The following assignment applies:

Flow in main stream	Current signal in mA	Current input signal in %
Flowmeter start of measuring range	4	0
Flowmeter end of measuring range	20	100

Monitoring of flow in main stream

This arrangement is particularly practical if the sample flow through a flow assembly in an open outlet is completely independent of the flow in the main stream.

This permits signalling of an alarm condition in the main stream (flow too low or has completely stopped) and triggers dosing switch-off even if the medium flow is retained due to the method of installation.

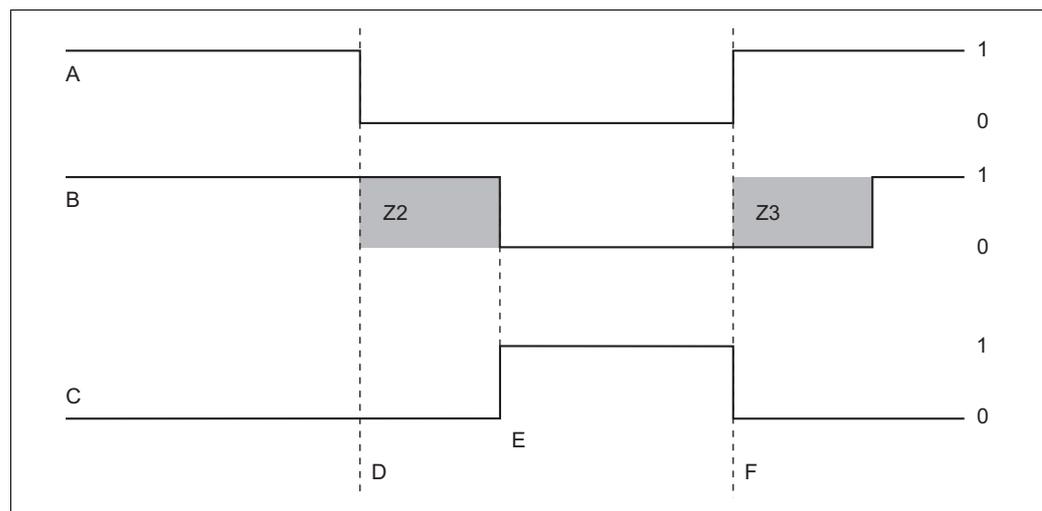


Fig. 26: Alarm signalling and dosing switch-off by the main stream

A	Flow in main stream	F	Flow restoration
B	Relay contacts of PID controller	Z2	Delay for controller switch-off, see field Z2
C	Alarm relay	Z3	Delay for controller switch-on, see field Z3
D	Flow below switch-off limit Z4 or flow failure	0	Off
E	Flow alarm	1	On

Feedforward control to PID controller

For control systems with very short reaction times, you can optimise the control. Additionally you measure the flow rate of the medium. This flow rate value (0/4 to 20 mA) you apply as feedforward control to the PID controller.

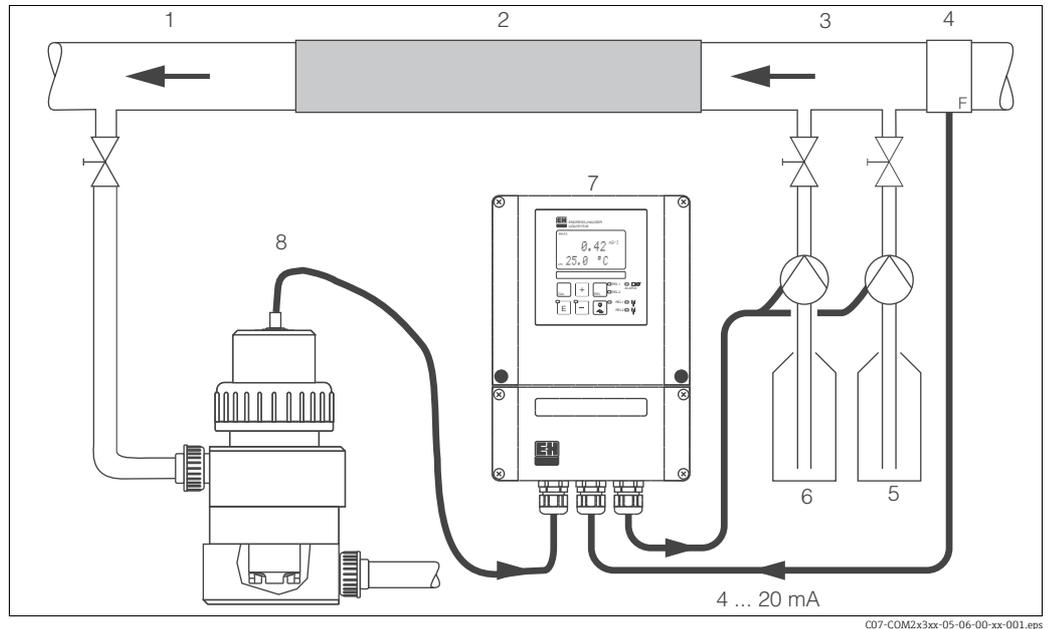


Fig. 27: Arrangement example for feedforward control of the flow rate in the main stream to the PID controller

- | | |
|------------------------------------|---------------------|
| 1 Measuring water extraction point | 5 Reducing agent |
| 2 Static mixer | 6 Oxidising agent |
| 3 Injection points | 7 Liquisys M COM253 |
| 4 Flowmeter | 8 COA250 with COS31 |

Feedforward control is a multiplying function as illustrated in the figure below (example with factory setting):

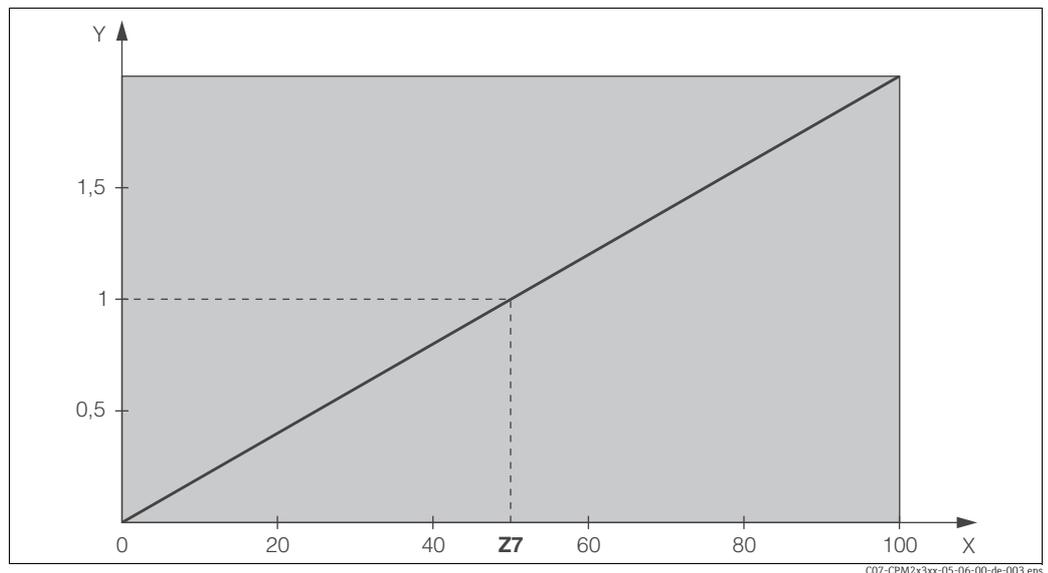


Fig. 28: Multiplying feedforward control

- | | |
|----|---------------------------------------|
| Y | Gain K_{infl} |
| X | Current input signal [%] |
| Z7 | Input value, when gain $K_{infl} = 1$ |

The basic version does not include functions in *italic*.

Coding	Field	Setting range (Factory settings, bold)	Display	Info
Z	CURRENT INPUT function group			Current input settings.
Z1	Select flow monitoring of main stream (with controller switch-off)	Off On		Flow monitoring may only be switched on if the flowmeter is connected in the main stream. If Z1 = off, fields Z2 to Z5 are not available.
Z2	Enter the delay for controller switch-off through current input	0 s 0 to 2000 s		Brief flow shortfalls can be suppressed by a delay and do not result in controller switch-off.
Z3	Enter the delay for controller switch-on through current input	0 s 0 to 2000 s		In the case of a controller, a delay until a representative measured value is received is useful if the flow fails for an extended period.
Z4	Enter the switch-off limit value for the current input	50% 0 to 100%		0 to 100% corresponds to 4 to 20 mA at the current input. Observe measured value assignment to the current output of the flowmeter.
Z5	Enter the switch-off direction for the current input	Low High		The controller is switched off if the value entered in Z4 is undershot or overshoot.
Z6	Select feedforward control to PID controller	Off <i>Lin = linear</i> <i>Basic</i>		If Z6 = off, the field Z7 is not available. Z6 = basic: disturbance variable only affects the basic load (alternatively dosing in proportion to quantity can be used if usual PID controlling is not possible, due to a defective sensor, for example).
Z7	Enter value for feedforward control at which gain = 1 applies	50% 0 to 100%		When the value is set, the controller actuating variable is the same size when feedforward control is switched on as when feedforward control is switched off.

6.4.4 Current outputs

Use the "Current output" function group to configure the individual outputs. You can enter either a linear characteristic (O3 (1)) or a user-defined current output characteristic in conjunction with the Plus Package (O3 (3)). Exception: if you have chosen a "continuous controller" for current output 2, you cannot enter a user-defined current output characteristic for this current output.

In addition, you can simulate a current output value (O3 (2)) to check the current outputs. If a second current output is present, you can output the controller actuating variable in accordance with field R 237 via the current output.

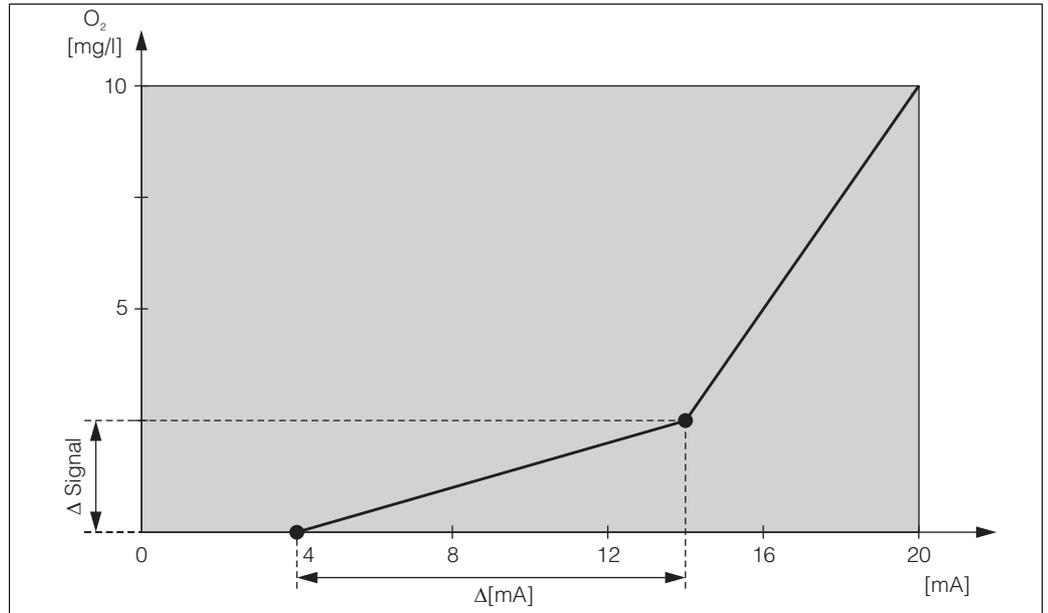


Fig. 29: User-defined current output characteristic (example)

The current output characteristic must be strictly monotonously increasing or strictly monotonously decreasing.

The distance per mA between two table value pairs must be greater than:

	Measuring range	Minimum distance per mA
Oxygen	0 to 20 mg/l	0.13 mg/l
	0 to 60 mg/l	0.38 mg/l
	0 to 200 % SAT	1.30 % SAT
	0 to 600 % SAT	3.80 % SAT
	0 to 400 hPa	2.50 hPa
	0 to 1200 hPa	7.50 hPa
Temperature	-10 to 60 °C (14 to 140 °F)	0.45 °C (0.81 °F)

The values for the sample characteristic (→  29) are entered in the following table. The distance per mA can be calculated from $\Delta \text{ signal} / \Delta \text{ mA}$.







Value pair	Current output 1			Current output 2		
	[mg/l; %SAT; hPa]	Current [mA]	Distance per mA	[mg/l; %SAT; hPa]	Current [mA]	Distance per mA
1	0	4				
2	2.5	14	0.25			
3	10	20	1.25			

First enter the desired current output configuration into the following blank table with a pencil. Calculate the resulting signal distance per mA to observe the necessary minimum slope. Then enter the values in the device.

Value pair	Current output 1			Current output 2		
	[mg/l; %SAT; hPa]	Current [mA]	Distance per mA	[mg/l; %SAT; hPa]	Current [mA]	Distance per mA
1						
2						
3						
4						
5						
6						
7						
8						
9						

Basic version does not include functions in *italic*.

Coding	Field	Setting range (Factory settings, bold)	Display	Info
0	CURRENT OUTPUT function group			Configuration of the current output (does not apply for PROFIBUS).
01	Select current output	Out1 <i>Out 2</i>		A characteristic can be selected for every output.
02	Select measured variable for 2nd current output	°C <i>mg/l</i> <i>ppm</i> <i>Contr</i>		R237 = curr (current output 2) can only be selected if O2 = Contr is selected (relay board required).
03 (1)	Enter or output linear characteristic	Lin = linear (1) <i>Sim = simulation (2)</i> <i>Tab = table (3)</i>		The characteristic can have a positive or negative slope for the measured value output. In the case of actuating variable output (O2 = Contr), an increasing current corresponds to an increasing actuating variable.
0311	Select current range	4 to 20 mA <i>0 to 20 mA</i>		
0312	0/4 mA value: Enter corresponding O ₂ or temperature value	- Version DX/DS or WX/WS with COS61: 0.00 mg/l* 0.00 to 20.00 mg/l 0.0 %SAT 0.0 to 200.0 %SAT 0 hPa 0 to 400 hPa - WX/WS with COS31: 0.00 mg/l* 0.00 to 60.00 mg/l 0.0 %SAT 0.0 to 600.0 %SAT 0 hPa 0 to 1200 hPa - WX/WS with COS71: 0.000 mg/l* 0.000 to 20.000 mg/l 0.0 %SAT 0.0 to 200.0 %SAT 0 hPa 0 to 400 hPa 0.0 °C -10.0 to 60.0 °C		Here you can enter the O ₂ or temperature value at which the min. current value (0/4 mA) is applied at the transmitter output. Minimum distance between 0/4 mA and 20 mA value: see field O313 * Display depends on setting in A2



Coding		Field	Setting range (Factory settings, bold)	Display	Info
	0313	20 mA value: Enter corresponding O ₂ or temperature value	<ul style="list-style-type: none"> Version DX/DS or WX/WS with COS61: 10.00 mg/l* 0.00 to 20.00 mg/l 100.0 %SAT 0.0 to 200.0 %SAT 200 hPa 0 to 400 hPa WX/WS with COS31: 10.00 mg/l* 0.00 to 60.00 mg/l 100.0 %SAT 0.0 to 600.0 %SAT 200 hPa 0 to 1200 hPa WX/WS with COS71: 10.000 mg/l* 0.000 to 20.000 mg/l 100.0 %SAT 0.0 to 200.0 %SAT 200 hPa 0 to 400 hPa 40.0 °C -10.0 to 60.0 °C		Here you can enter the O ₂ or temperature value at which the max. current value (20 mA) is applied at the transmitter output. Minimum distance between 0/4 mA and 20 mA value must be: Oxygen: - DX/DS or WX/WS with COS61: 0.2 mg/l / 2 %SAT / 4 hPa - WX/WS with COS31: 0.6 mg/l / 6 %SAT / 12 hPa - WX/WS with COS71: 0.02 mg/l / 0.2 %SAT / 0.4 hPa Temperature: All versions: 7 °C * Display depends on setting in A2
O3 (2)		Simulate current output	Lin = linear (1) Sim = simulation (2) Tab = table (3)		Simulation is not ended until (1) or (3) is selected. For further characteristics, see O3 (1), O3(3).
	0321	Enter simulation value	Current value 0.00 to 22.00 mA		Entering a current value results in this value being directly output at the current output.
O3 (3)		Enter current output table (only for Plus Package)	Lin = linear (1) Sim = simulation (2) Tab = table (3)		Values can also be added or altered at a later stage. The values entered are automatically sorted by increasing current value. For further characteristics, see O3 (1), O3 (2).
	0331	Select table options	Read Edit		
	0332	Enter number of table value pairs	1 1 to 10		Enter the number of pairs from the x and y value (measured value and current value) here.
	0333	Select table value pair	1 1 to No. elem. Assign		The function chain O333 ... O335 will run through as many times as correspond to the value in O332. "Assign" appears as the last step. After confirmation the system jumps to O336.

Coding		Field	Setting range (Factory settings, bold)	Display	Info
		0334 <i>Enter x value</i>	– <i>Version DX/DS or WX/WS with COS61:</i> 0.00 mg/l* <i>0.00 to 20.00 mg/l</i> 0.0 %SAT <i>0.0 to 200.0 %SAT</i> 0 hPa <i>0 to 400 hPa</i> – <i>WX/WS with COS31:</i> 0.00 mg/l* <i>0.00 to 60.00 mg/l</i> 00.0 %SAT <i>0.0 to 600.0 %SAT</i> 0 hPa <i>0 to 1200 hPa</i> – <i>WX/WS with COS71:</i> 0.000 mg/l* <i>0.000 to 20.000 mg/l</i> 0.0 %SAT <i>0.0 to 200.0 %SAT</i> 0 hPa <i>0 to 400 hPa</i> 0.0 °C <i>-10.0 to 60.0 °C</i>		x value = measured value specified by user. * Display depends on setting in A2
		0335 <i>Enter y value</i>	4.00 mA <i>0.00 to 20.00 mA</i>		y value = current value belonging to 0334 specified by user. Return to 0333 until all values are entered.
		0336 <i>Message as to whether table status is OK</i>	yes <i>no</i>		Back to 03. If status = no, correct table (all settings made up until now are retained) or back to measuring mode (table is deleted).

6.4.5 Monitoring functions

The monitoring functions are used to define various alarms and configure output contacts. Each individual error can be defined to be effective or not (at the contact or as an error current). An alarm condition can be defined to activate a cleaning function (F8)

Coding	Field	Setting range (Factory settings, bold)	Display	Info
F	ALARM function group			Alarm function settings.
F1	Select contact type	Latch = latching contact Momen = momentary contact		The contact type selected only applies to the alarm contact.
F2	Select time unit	s min		
F3	Enter alarm delay	0 s (min) 0 to 2000 s (min)		Depending on the option selected in F2, the alarm delay is entered in s or min.
F4	Select error current	22 mA 2.4 mA		This selection must be made even if all error reporting is switched off in F5. If "0-20 mA" was selected in O311, "2.4 mA" may not be used.
F5	Select error	1 1 to 255		Here you can select all the errors which should trigger an alarm. The errors are selected via the error numbers. Please refer to the table in section 9.2 "System error messages" for the meaning of the individual error numbers. The factory settings remain in effect for all errors not edited.
F6	Set alarm contact to be effective for the selected error	yes no		If "no" is selected, all the other alarm settings are deactivated (e.g. alarm delay). The settings themselves are retained. This setting only applies to the error selected in F5.
F7	Set error current to be effective for the selected error	no yes		The option selected in F4 is effective or ineffective in the event of an error. This setting only applies to the error selected in F5.

Coding		Field	Setting range (Factory settings, bold)	Display	Info
	F8	Automatic cleaning function start	no yes		This field is not available for certain errors, see "Troubleshooting and fault elimination" section.
	F9	Select return to menu or next error	next = next error ←R		If ←R is selected, you return to F, if next is selected, you go to F5.

Check

The CHECK function group is only available for devices with a Plus Package.

In the CHECK function group, you can select different monitoring functions for the measurement.

All the monitoring functions are off in the factory setting. The Sensor Check System adapts to the current application conditions by adding and setting suitable functions.

Alarm threshold monitoring

For oxygen measurement without entry control (ventilation) sensor errors lead to a measured value error, but have no impact on the process medium (examples: monitoring measurement in surface waters or in water-works). Sensor errors normally cause high or low readings that are implausible. This is detected and signalled by user-definable alarm thresholds.

Controller monitoring

For oxygen measurement with simultaneous entry control, sensor errors not only lead to incorrect measured values but also have a direct impact on the state of the process medium. Particularly in the case of oxygenation control in sewage treatment works, the risk exists due to the control loop that the ventilation does not switch on if the measured value is constantly too high. A too low oxygen supply creates a considerable risk for the microbes and their cleaning performance. On the other hand, a measured value which is permanently too low due to the uninterrupted operation of the ventilation units leads to increased operating costs. Such cases are recognised and signalled using freely settable monitoring times for the maximum permitted controller switch-on and switch-off periods.

Sensor activity monitoring

The process medium can also have an effect on the sensor leading to incorrect measured values. The collection of solid matter at the sensor or a strong coating on the sensor membrane can lead to a strongly-delayed or completely passive measuring signal. Constant monitoring of the signal activity recognises and signals such passivity.






SCS monitoring functions at a glance

	Functional description	Setting possibility	Alarm event	Application
Alarm threshold monitoring (P1 to P4)	<ul style="list-style-type: none"> - Freely adjustable lower alarm threshold (AT) - Freely adjustable upper alarm threshold (AT) 	off	–	Applications with or without oxygenation control
		only lower AT	Lower AT reached or dropped below	
		only upper AT	Upper AT reached or exceeded	
		lower and upper AT	Lower AT reached or dropped below or upper AT reached or exceeded	
Controller monitoring (CC: Controller Check, P5 to P8)	<ul style="list-style-type: none"> - Switch-on period monitoring - Switch-off period monitoring 	off	–	Applications with oxygenation control
		on	Set maximum period for permanent switch-on or switch-off exceeded	
Sensor activity monitoring (AC: Alternation Check, P5 to P8)	Monitoring for signal change	off	–	Applications with or without oxygenation control
		on	Change within 1 hour < ± 0.1 mg/l or ± 1 %SAT or ± 2 hPa	

The function group "Check" is used to monitor the lower and upper limits of the measured value and to initiate alarms.

Basic version does not include functions in *italic*.

Coding	Field	Setting range (Factory settings, bold)	Display	Info
P	CHECK function group			Settings for sensor and process monitoring
P1	Select alarm threshold monitoring	Off Low High Lo+Hi Low! High! Lo+Hi!		Alarm signalling optionally with or without simultaneous controller switch-off. XXXX = without controller switch-off XXXX! = with controller switch-off
P2	Enter alarm delay	0 s (min) 0 to 2000 s (min)		Depending on your selection in F2, you can enter the error delay in min or s. Only after this delay does a high or low limit violation cause an alarm as per field P3/P4.
P3	Enter lower alarm threshold	<ul style="list-style-type: none"> - Version DX/DS or WX/WS with COS61: 0.00 mg/l* 0.00 to 19.00 mg/l 0.0 %SAT 0.0 to 190.0 %SAT 0 hPa 0 to 380 hPa - WX/WS with COS31: 0.00 mg/l* 0.00 to 59.00 mg/l 0.0 %SAT 0.0 to 590.0 %SAT 0 hPa 0 to 1180 hPa - WX/WS with COS71: 0.000 mg/l* 0.000 to 19.000 mg/l 0.0 %SAT 0.0 to 190.0 %SAT 0 hPa 0 to 380 hPa 		* Display depends on setting in A2

Coding	Field	Setting range (Factory settings, bold)	Display	Info
P4	Enter upper alarm threshold	<ul style="list-style-type: none"> - Version DX/DS or WX/WS with COS61: 20.00 mg/l* 1.00 to 20.00 mg/l 200.0 %SAT 0.0 to 200.0 %SAT 400 hPa 20 to 400 hPa - WX/WS with COS31: 20.00 mg/l* 1.00 to 60.00 mg/l 200.0 %SAT 10.0 to 600.0 %SAT 400 hPa 20 to 1200 hPa - WX/WS with COS71: 20.000 mg/l* 0.010 to 20.000 mg/l 200.0 %SAT 0.5 to 200.0 %SAT 400 hPa 20 to 400 hPa 		* Display depends on setting in A2
P5	Select process monitoring (PCS alarm)	<ul style="list-style-type: none"> Off AC CC AC+CC AC! CC! AC+CC! 		AC = sensor activity check CC = controller check AC checking limits: ±0.1 mg/l or ±1 %SAT or ±2 hPa in 1 h XXXX = without controller switch-off XXXX! = with controller switch-off
P6	Enter maximum permissible duration for lower CC setpoint limit violation (field P8)	480 min 0 to 2000 min		Only when P6 = CC or AC+CC
P7	Enter maximum permissible duration for upper CC setpoint limit violation (field P8)	240 min 0 to 2000 min		Only when P6 = CC or AC+CC
P8	Enter CC setpoint (for P6/P7)	<ul style="list-style-type: none"> - Version DX/DS or WX/WS with COS61: 5.00 mg/l* 0.00 to 20.00 mg/l 50.0 %SAT 0.0 to 200.0 %SAT 200 hPa 0 to 400 hPa - WX/WS with COS31: 5.00 mg/l* 0.00 to 60.00 mg/l 50.0 %SAT 0.0 to 600.0 %SAT 200 hPa 0 to 1200 hPa - WX/WS with COS71: 1.000 mg/l* 0.000 to 20.000 mg/l 10.0 %SAT 0.0 to 200.0 %SAT 20 hPa 0 to 400 hPa 		Setpoint for external controller (process control system) must match with setpoint in P8. * Display depends on setting in A2

6.4.6 Relay contact configuration

To use the RELAY function group, you need a relay board which is not part of the basic version.

The following relay contacts can be selected and configured as desired (max. four contacts, depending on options installed):

- Limit contactor for measured oxygen value: R2 (1)
- Limit contactor for temperature: R2 (2)
- PID controller: R2 (3)
- Timer for cleaning function: R2 (4)
- Chemoclean function: R2 (5)

Limit contactor for measured oxygen value and temperature

The transmitter has different ways of assigning a relay contact. Switch-on and switch-off points and pick-up and drop-out delays can be assigned to the limit contactor. In addition, you can configure an alarm threshold to output an error message and to start a cleaning function in conjunction with this.

These functions can be used both for oxygen measurement and for temperature measurement.

Please refer to Fig. 30 for a clear illustration of the relay contact states.

- When the measured values increase (maximum function), the relay contact is closed as of t_2 after the switch-on point (t_1) has been overshoot and the pick-up delay has elapsed ($t_2 - t_1$).
The alarm contact switches if the alarm threshold (t_3) is reached and the alarm delay ($t_4 - t_3$) has also elapsed.
- When the measured values decrease, the alarm contact is reset when the alarm threshold (t_5) is undershot as is the relay contact (t_7) after the drop-out delay ($t_7 - t_6$).
- If the pick-up and drop-out delays are set to 0 s, the switch-on and switch-off points are also switch points of the contacts.

Settings can also be made for a minimum function in the same way as for a maximum function.

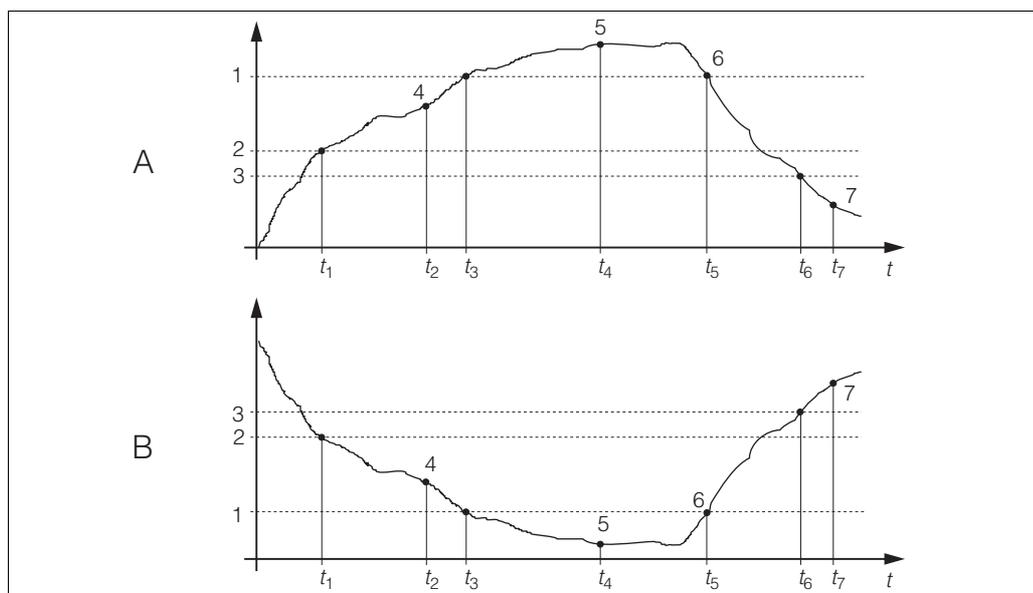


Fig. 30: Illustration of the alarm and limit value functions

A	Switch-on point > switch-off point: Max. function	1	Alarm threshold	5	Alarm ON
B	Switch-on point < switch-off point: Min. function	2	Switch-on point	6	Alarm OFF
		3	Switch-off point	7	Contact OFF
		4	Contact ON		

P(ID) controller

You can define various controller functions for the transmitter. On the basis of the PID controller, P, PI, PD and PID controllers can be implemented. For an optimum control system, use the controller that best suits your application. Depending on the option selected in the R 237/R 266 field, the actuating signal can be output via relays or via current output 2 (if available).

- **P controller**

Used for simple linear control purposes with small system deviations. Where major changes are to be controlled, overshooting may occur. In addition, a lasting control deviation is to be expected.

- **PI controller**

Is used for control systems where overshooting is to be avoided and no lasting control deviation should occur.

- **PD controller**

Is used for processes that require quick changes and where peaks are to be corrected.

- **PID controller**

Is used for processes where a P, PI or PD controller does not control sufficiently.

Configuration options of the PID controller

The following configuration options are available for a PID controller:

- Change control gain K_p (P influence)
- Set integral action time T_n (I influence)
- Set derivative action time T_v (D influence)

Basic load dosing (Basic)

The basic load dosing (field R231) is used to set a constant dosage (field R2311)

PID controlling plus basic load dosing

If you select this function (PID + Basic) in field R231 the PID controlled dosage will not be lower than the basic load value entered in field R2311.

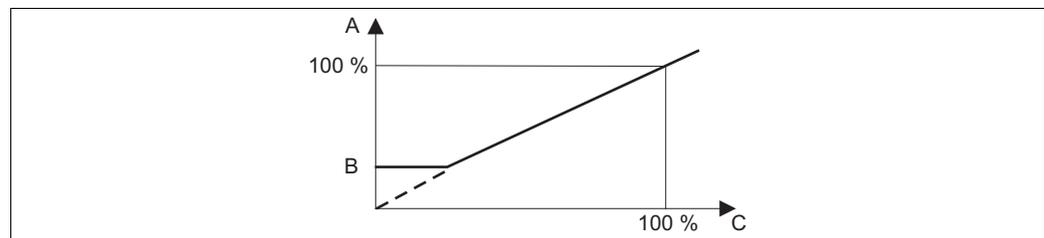


Fig. 31: Control characteristic PID controller with basic load dosing

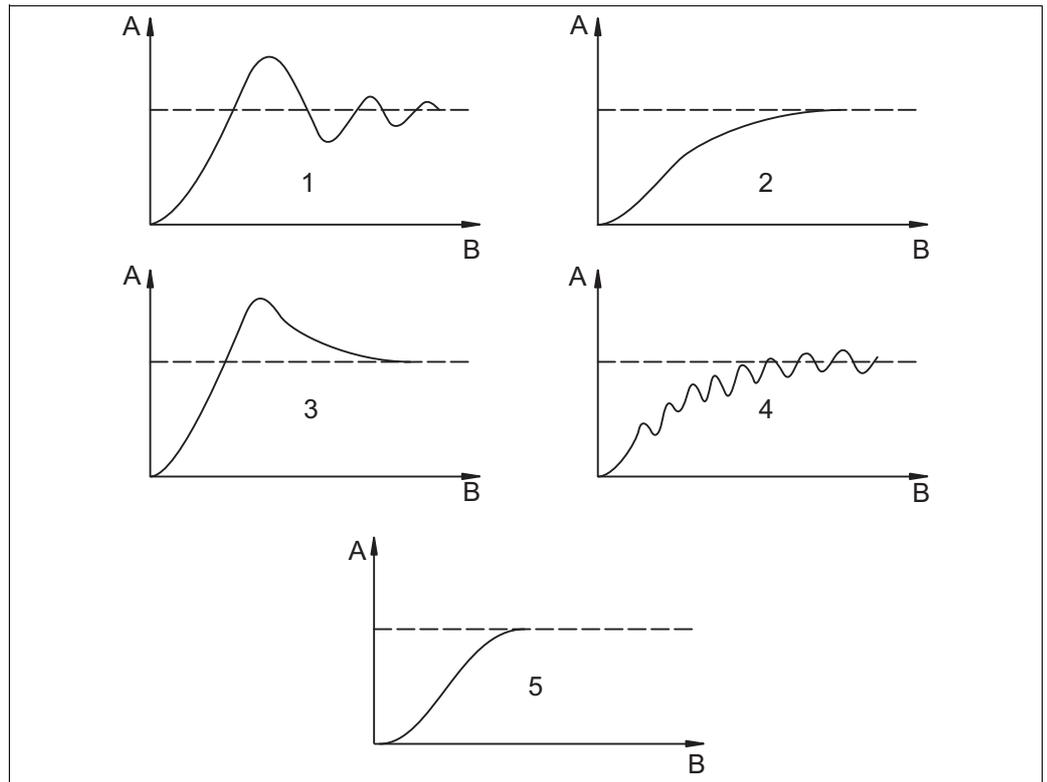
A PID with basic load
 B Basic load
 C PID

Commissioning

If you do not yet have any experience for setting the control parameters, set the values that yield the greatest possible stability in the control circuit. Proceed as follows to optimize the control circuit further:

- Increase the control gain K_p until the controlled variable just starts to overshoot.
- Reduce K_p slightly and then reduce the integral action time T_n so that the shortest possible correction time without overshooting is achieved.
- To reduce the response time of the controller, also set the derivative action time T_v .

Control and fine optimization of the set parameters with a recorder



Optimization of settings T_n and K_p

A Actual value
B Time

- | | |
|-------------------|-------------------|
| 1 T_n too small | 4 K_p too small |
| 2 T_n too large | 5 Optimum setting |
| 3 K_p too large | |

Actuating signal outputs (R237 ... R2310)

Each control contact outputs a cyclical signal whose intensity corresponds to the controller's manipulated variable. A distinction is made according to the type of signal cycle:

- Pulse length modulation
The bigger the calculated manipulated variable is, the longer the contact affected remains picked up. The period T can be adjusted between 0.5 and 99 s (field R238). Outputs with pulse length modulation are used to activate solenoid valves.
- Pulse frequency modulation
The bigger the calculated manipulated variable is, the higher the switching frequency of the contact affected. The maximum switching frequency $1/T$ can be set between 60 and 180 min^{-1} . The on-time t_{ON} is constant. It depends on the set maximum frequency and is approx. 0.5 s for 60 min^{-1} and approx. 170 ms for 180 min^{-1} . Outputs with pulse frequency modulation are used to activate directly controlled solenoid dosing pumps.

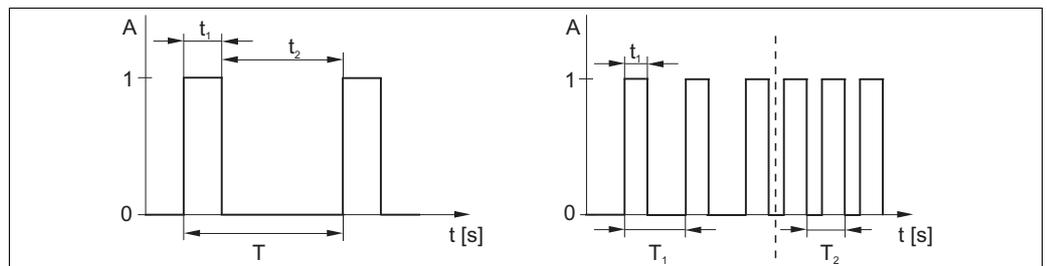


Fig. 32: Signal of a pulse-length modulated controller contact (left) and of a pulse-frequency modulated controller contact (right)
A Contact 1 = on, 0 = off
T Period length
B Time [s] $t_1 = t_{on}$ $t_2 = t_{off}$
 T_1 T_2 Impulse period length (impulse freq. $1/T_1$ and $1/T_2$)

Constant controller

Via the current output 2, the minimum actuating variable (0 %) of the controller is output with 0/4 mA and the maximum actuating variable (100%) of the controller is output with 20 mA.

Control characteristic for direct and inverse control action

You can choose between two control characteristics in the R236 field:

- Direct control action = maximum function
- Inverse control action = minimum function

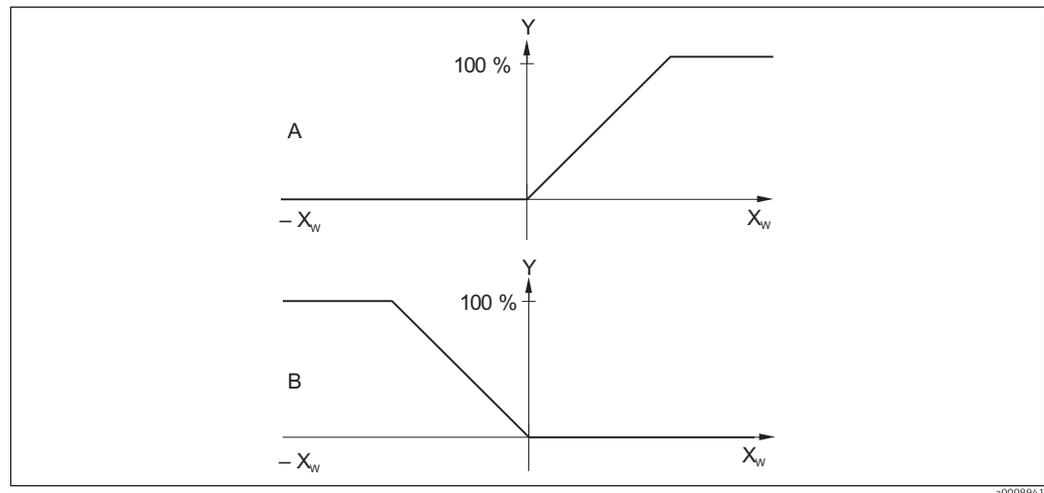


Fig. 33: Control characteristic of a proportional controller with direct and inverse control action

A Direct = max. function
B Inverse = min. function

Timer for cleaning function

This function includes a simple cleaning option. You can set the time interval after which cleaning should start. So you can only select a constant interval sequence.

Other cleaning functions are available for selection in conjunction with the Chemoclean function (version with four contacts, see "Chemoclean function" section).

- i** Timer and Chemoclean do not work independently of one another. While one of the two functions is active, the other cannot be started.

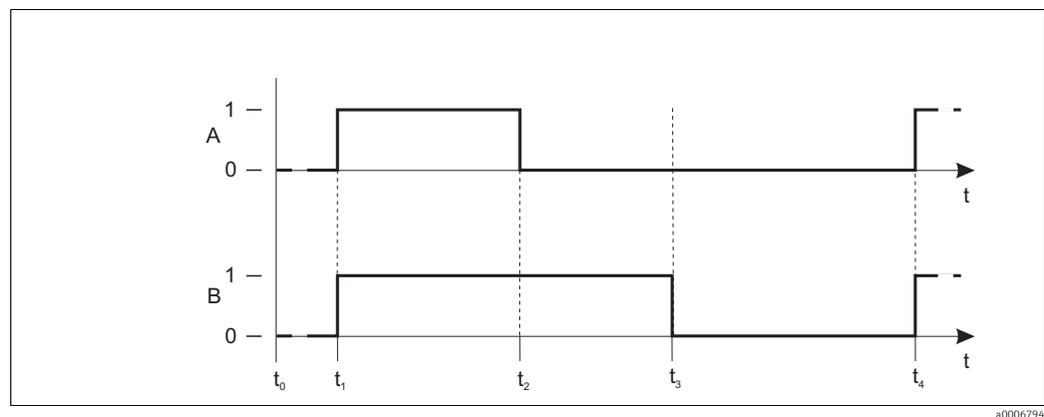


Fig. 34: Correlation of cleaning time, pause time and hold dwell period

A Wiper and/or spray cleaning system
B Hold function
0 Inactive
1 Active

t_0 Normal mode
 t_1 Cleaning start
 $t_2 - t_1$ Cleaning time
 $t_3 - t_2$ Clean hold dwell period (0 to 999 s)
 $t_4 - t_3$ Pause time between two cleaning intervals (1 to 7200 min)

Chemoclean function

Just like the timer function, Chemoclean can also be used to start a cleaning cycle. However, Chemoclean also gives you the added option of defining different cleaning and rinsing intervals.

As a result, it is possible to clean irregularly with different repeat cycles and to separately set the cleaning times with post rinse times.

Pay attention to the following:

- To use the Chemoclean function the transmitter has to be equipped with a designated relay board (see product structure or chapter "accessories").
- Timer and Chemoclean do not work independently of one another. While one of the two functions is active, the other cannot be started.
- For the Chemoclean function, the relays 3 (water) and 4 (cleaner) are used.
- If cleaning is prematurely aborted, a post rinse time always follows.
- If the setting is "Economy", cleaning only takes place with water.

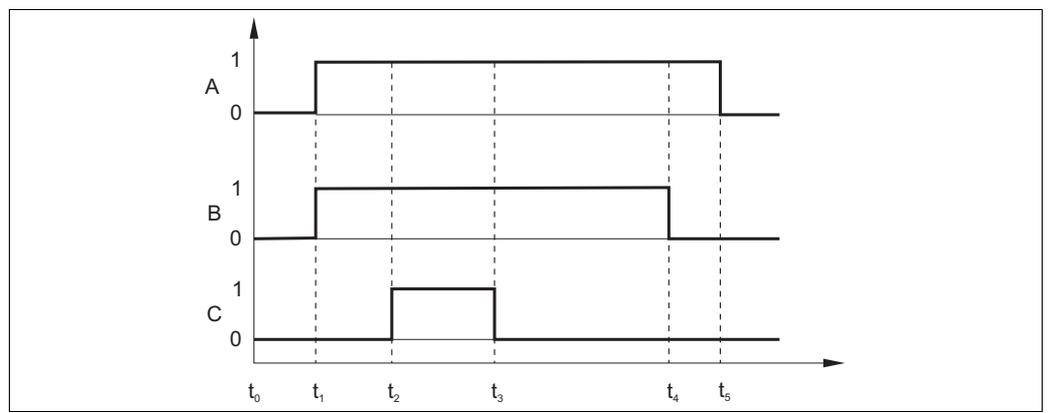


Fig. 35: Sequence of a cleaning cycle




- A Hold
- B Water
- C Cleaner
- 0 Contact on
- 1 Contact off










- t₀ Normal mode
- t₁ Cleaning start
- t₂ - t₁ Pre-rinse time
- t₃ - t₂ Cleaning time
- t₄ - t₃ Post rinse time
- t₅ - t₄ Hold dwell period

a0006793

Basic version does not include functions in *italic*.

Coding	Field	Setting range (Factory settings, bold)	Display	Info
R	RELAY function group			Relay contact settings.
R1	Select contact to be configured	Rel1 <i>Rel2</i> <i>Rel3</i> <i>Rel4</i>		Rel3 (water) and Rel4 (cleaner) are only available with the relevant version of the transmitter. If Chemoclean is used as the cleaning method, Rel4 is not available.
R2 (1)	Configuration limit contactor for O ₂ measurement	LC PV = limit contactor O₂ (1) LC °C = limit contactor T (2) PID controller (3) Timer (4) <i>Clean = Chemoclean (5)</i>		PV = process value If Rel4 is selected in the R1 field, Clean = Chemoclean cannot be selected. By confirming with ENTER, another relay function already switched on is switched off and its settings are reset to the factory settings.
R211	Switch function of R2 (1) off or on	Off On		All the settings are retained.
R212	Enter the switch-on point of the contact	<ul style="list-style-type: none"> - Version DX/DS or WX/WS with COS61: 20.00 mg/l* 0.00 to 20.00 mg/l 200.0 %SAT 0.0 to 200.0 %SAT 400 hPa 0 to 400 hPa - WX/WS with COS31: 20.00 mg/l* 0.00 to 60.00 mg/l 200.0 %SAT 0.0 to 600.0 %SAT 400 hPa 0 to 1200 hPa - WX/WS with COS71: 20.000 mg/l* 0.000 to 20.000 mg/l 200.0 %SAT 0.0 to 200.0 %SAT 400 hPa 0 to 400 hPa 		Never set the switch-on point and the switch-off point to the same value! (Only the operating mode selected in A1 is displayed.) * Display depends on setting in A2

Coding		Field	Setting range (Factory settings, bold)	Display	Info
	R213	Enter the switch-off point of the contact	<ul style="list-style-type: none"> - Version DX/DS or WX/WS with COS61: 20.00 mg/l* 0.00 to 20.00 mg/l 200.0 %SAT 0.0 to 200.0 %SAT 400 hPa 0 to 400 hPa - WX/WS with COS31: 20.00 mg/l* 0.00 to 60.00 mg/l 200.0 %SAT 0.0 to 600.0 %SAT 400 hPa 0 to 1200 hPa - WX/WS with COS71: 20.000 mg/l* 0.000 to 20.000 mg/l 200.0 %SAT 0.0 to 200.0 %SAT 400 hPa 0 to 400 hPa 		<p>Entering a switch-off point selects either a Max contact (switch-off point < switch-on point) or a Min contact (switch-off point > switch-on point), thereby implementing a hysteresis that is constantly required (see "Illustration of the alarm and limit functions" figure).</p> <p>(Only the operating mode selected in A1 is displayed.)</p> <p>* Display depends on setting in A2</p>
	R214	Enter pick-up delay	0 s 0 to 2000 s		
	R215	Enter drop-out delay	0 s 0 to 2000 s		
	R216	Enter alarm threshold	<ul style="list-style-type: none"> - Version DX/DS or WX/WS with COS61: 20.00 mg/l* 0.00 to 20.00 mg/l 200.0 %SAT 0.0 to 200.0 %SAT 400 hPa 0 to 400 hPa - WX/WS with COS31: 20.00 mg/l* 0.00 to 60.00 mg/l 200.0 %SAT 0.0 to 600.0 %SAT 400 hPa 0 to 1200 hPa - WX/WS with COS71: 20.000 mg/l* 0.000 to 20.000 mg/l 200.0 %SAT 0.0 to 200.0 %SAT 400 hPa 0 to 400 hPa 		<p>If the alarm threshold is undershot/overshot, this triggers an alarm with the error message and error current at the transmitter (note alarm delay in field F3). If defined as a Min contact, the alarm threshold must be < switch-off point. (Only the operating mode selected in A1 is displayed.)</p> <p>* Display depends on setting in A2</p>
	R217	Display status for limit contactor	MAX MIN		Display only.







Coding	Field	Setting range (Factory settings, bold)	Display	Info
R2 (2)	Configure limit contactor for temperature measurement	LC PV = limit contactor O ₂ (1) LC °C = limit contactor T (2) PID controller (3) Timer (4) <i>Clean = Chemoclean (5)</i>		By confirming with ENTER, another relay function already switched on is switched off and its settings are reset to the factory settings.
R221	Switch function of R2 (2) off or on	Off On		Settings made for the limit contactor are not deleted by switching the function off.
R222	Enter switch-on temperature	60.0 C (140 °F) -10.0 to 60.0 C (14 to 140 °F)		Never set the switch-on point and the switch-off point to the same value!
R223	Enter switch-off temperature	60.0 C (140 °F) -10.0 to 60.0 C (14 to 140 °F)		Entering a switch-off point selects either a Max contact (switch-off point < switch-on point) or a Min contact (switch-off point > switch-on point), thereby implementing a hysteresis that is constantly required (see "Illustration of the alarm and limit functions" figure).
R224	Enter pick-up delay	0 s 0 to 2000 s		
R225	Enter drop-out delay	0 s 0 to 2000 s		
R226	Enter alarm threshold (as absolute value)	60.0 C (140 °F) -10.0 to 60.0 C (14 to 140 °F)		If the alarm threshold is undershot/overshot, this triggers an alarm with the error message and error current at the transmitter (note alarm delay in field F3). If defined as a Min contact, the alarm threshold must be < switch-off point.
R227	Display status for limit contactor	MAX MIN		Display only.
R2 (3)	Configure P(ID) controller	LC PV = limit contactor O ₂ (1) LC °C = limit contactor T (2) PID controller (3) Timer (4) <i>Clean = Chemoclean (5)</i>		By confirming with ENTER, another relay function already switched on is switched off and its settings are reset to the factory settings.




Coding	Field	Setting range (Factory settings, bold)	Display	Info
R231	Switch function of R2 (3) off or on	Off On Basic PID+B		On = PID controller Basic = basic load dosing PID+B = PID controller + basic load dosing
R232	Enter set point	<ul style="list-style-type: none"> - Version DX/DS or WX/WS with COS61: 5.00 mg/l* 0.00 to 20.00 mg/l 50.0 %SAT 0.0 to 200.0 %SAT 200 hPa 0 to 400 hPa - WX/WS with COS31: 5.00 mg/l* 0.00 to 60.00 mg/l 50.0 %SAT 0.0 to 600.0 %SAT 200 hPa 0 to 1200 hPa - WX/WS with COS71: 5.000 mg/l* 0.000 to 20.000 mg/l 50.0 %SAT 0.0 to 200.0 %SAT 200 hPa 0 to 400 hPa 		The set point is the value to be maintained by the control system. Using this control process, this value is restored upwards or downwards when a deviation occurs. (Only the operating mode selected in A1 is displayed.) * Display depends on setting in A2
R233	Enter control gain K_p	1.00 0.01 to 20.00		See "P(ID) controller" section.
R234	Enter integral action time T_n (0.0 = no I-component)	0.0 min 0.0 to 999.9 min		See "P(ID) controller" section. With every Hold, the I-component is set to zero. Although Hold can be deactivated in field S2, this does not apply for Chemoclean and timer!
R235	Enter derivative action time T_v (0.0 = no D-component)	0.0 min 0.0 to 999.9 min		See "P(ID) controller" section.
R236	Select controller characteristic	dir = direct inv = inverse		dir = Max. function inv = Min. function The setting is required depending on the control deviation (upward or downward deviation, see "P(ID) controller" section).
R237	Select pulse length or pulse frequency	len = pulse length freq = pulse frequency curr = current output 2		Pulse length e.g. for solenoid valve, pulse frequency e.g. for solenoid dosing pump, see "Actuating signal outputs" section. Curr = current output 2 can only be selected if O2 = Contr.

Coding		Field	Setting range (Factory settings, bold)	Display	Info
	R238	Enter pulse interval	10.0 s 0.5 to 999.9 s		This field only appears if pulse length is selected in R237. If pulse frequency is selected, R238 is skipped and entries continue with R239.
	R239	Enter maximum pulse frequency of the adjuster	120 min⁻¹ 60 to 180 min ⁻¹		This field only appears if pulse frequency is selected in R237. If pulse length is selected, R239 is skipped and entries continue with R2310.
	R2310	Enter minimum switch-on time t _{ON}	0.3 s 0.1 to 5.0 s		This field only appears if pulse length is selected in R237.
	R2311	Enter basic load	0 % 0 to 40 %		When you select the basic load, you enter the desired dosing quantity. 100% basic load would correspond to: – Constantly on for R237 = len – Fmax at R237 = freq (field R239) – 20 mA at R237 = curr
R2 (4)		Configure cleaning function (timer)	LC PV = limit contactor O ₂ (1) LC °C = limit contactor T (2) PID controller (3) Timer (4) Clean = Chemoclean (5)		Cleaning only takes place with one cleaning agent (usually water). By confirming with ENTER, another relay function already switched on is switched off and its settings are reset to the factory settings.
	R241	Switch function of R2 (4) off or on	Off On		Settings made for the timer are not deleted by switching the function off.
	R242	Enter rinsing/cleaning time	30 s 0 to 999 s		Settings for Hold and relay are active for this time.
	R243	Enter pause time	360 min 1 to 7200 min		The pause time is the time between two cleaning cycles (see "Timer for cleaning function" section).
	R244	Enter minimum pause time	120 min 1 to R243 min		The minimum pause time prevents constant cleaning if a cleaning trigger is present.







Coding	Field	Setting range (Factory settings, bold)	Display	Info
R2 (5)	Configure cleaning with Chemoclean (for version with four contacts, Chemoclean option and contacts 3 and 4 assigned)	LC PV = limit contactor O2 (1) LC °C = limit contactor T (2) PID controller (3) Timer (4) Clean = Chemoclean (5)		See "Chemoclean function" section. By confirming with ENTER, another relay function already switched on is switched off and its settings are reset to the factory settings.
R251	Switch function of R2 (5) off or on	Off On		Settings made for the timer are not deleted by switching the function off.
R252	Select type of start pulse	Int = internal (time-controlled) Ext = external (digital input 2) I+ext = internal + external I+stp = internal, suppressed by external		The cycle for the "int" function is started by the end of the pause time (R257). No real time clock is available. External suppression is required for irregular time intervals (e.g. weekends).
R253	Enter pre-rinse time	20 s 0 to 999 s		Rinsing with water takes place.
R254	Enter cleaning time	10 s 0 to 999 s		Cleaning with cleaning agent and water takes place.
R255	Enter post rinse time	20 s 0 to 999 s		Rinsing with water takes place.
R256	Enter number of repeat cycles	0 0 to 5		R253 to R255 is repeated.
R257	Enter pause time	360 min 1 to 7200 min		The pause time is the time between two cleaning cycles (see "Timer function" section).
R258	Enter minimum pause time	120 min 1 to R257 min		The minimum pause time prevents constant cleaning if an external cleaning start is present.
R259	Enter number of cleaning cycles without cleaning agent (economy function)	0 0 to 9		After cleaning with cleaner, up to 9 cleaning sessions can be carried out with water only until the next cleaning session with cleaner takes place.

6.4.7 Service




Coding	Field	Setting range (Factory settings, bold)	Display	Info
S	SERVICE function group			Service function settings.
S1	Select language	ENG = English GER = German FRA = French ITA = Italian NL = Dutch ESP = Spanish		
S2	Configure Hold	S+C = Hold during configuration and calibration Cal = Hold during calibration Setup = Hold during configuration None = no Hold		S = setup C = calibration
S3	Manual Hold	Off On		The setting is retained even in the event of a power failure.
S4	Enter Hold dwell period	10 s 0 to 999 s		
S5	Enter SW upgrade release code (Plus Package)	0000 0000 to 9999		The code is located on the nameplate. If an incorrect code is entered, you are taken back to the measurement menu. The number is edited with the PLUS or MINUS key and confirmed with the ENTER key. "1" is displayed if the code is active.
S6	Enter SW upgrade release code Chemoclean	0000 0000 to 9999		The code is located on the nameplate. If an incorrect code is entered, you are taken back to the measurement menu. The number is edited with the PLUS or MINUS key and confirmed with the ENTER key. "1" is displayed if the code is active.
S7	Order number is displayed	COM253-W		If the device is upgraded, the order code is not automatically adjusted.
S8	Serial number is displayed	4A135705G00		

Coding	Field	Setting range (Factory settings, bold)	Display	Info
S9	Reset the device to the basic settings 	No Sens = sensor data Facy = factory settings		Sens = last calibration is deleted and is reset to factory setting. Facy = all data (apart from A1 a. S1) are deleted and reset to the factory setting!
S10	Perform device test	No Displ = display test		
S11	Absolute air pressure will be displayed	Current value		Do not compare with the barometer. This shows the relative air pressure (related to sea level).

6.4.8 E+H Service

Coding	Field	Setting range (Factory settings, bold)	Display	Note
E	E+H SERVICE function group			Information on the device version
E1	Select module	Contr = controller (1) Trans = transmitter (2) Main = power unit (3) Rel = relay module (4) Sens = sensor (5)		"Sens" only with version WX or WS
	E111 E121 E131 E141 E151 Software version is displayed			If E1 = contr: instrument software If E1 = trans, main, rel: module firmware If E1 = sens: sensor software
	E112 E122 E132 E142 E152 Hardware version is displayed			Only display function
	E113 E123 E133 E143 E153 Serial number is displayed			Only display function
	E114 E124 E134 E144 E154 Module ID is displayed			Only display function

6.4.9 Interfaces

Coding	Field	Setting range (Factory settings, bold)	Display	Info
I	INTERFACE function group			Communication settings (only for device version HART or PROFIBUS).
I1	Enter bus address	Address HART: 0 to 15 or PROFIBUS: 0 to 126		Each address may only be used once in a network. If a device address ≠ 0 is selected, the current output is automatically set to 4 mA and the device is set to multi-drop operation.
I2	Display of measuring point			

6.5 Communication

For devices with a communication interface, please also refer to the separate Operating Instructions BA00208C/07/EN (HART) or BA00209C/07/EN (PROFIBUS).

6.6 Calibration





To access the "Calibration" function group, press the CAL key.
 This function group is used to calibrate and adjust the measuring point. The sensor is calibrated in air or in the medium.

Pay attention to the following:


- At first start-up, sensor calibration of amperometric sensors is absolutely required in order for the measuring system to be able to generate accurate measuring values.
- The optical oxygen sensor COS61 does not need a calibration at first start-up.
- If the calibration procedure is aborted by pressing the PLUS and MINUS keys at the same time (return to C113 or C124) or if the calibration is faulty, then the previous calibration data are reinstated. A calibration error is indicated by the "ERR" message and flashing of the sensor symbol on the display.
 Repeat calibration!
- The instrument is automatically switched to hold during calibration (factory setting).
- After calibration, the system jumps back to the measuring mode. During the hold dwell period the hold symbol is displayed.

The slope calibration of the oxygen sensor COS61 will be performed in air or in air saturated water. The calibration of the zero point will be performed in nitrogen or in oxygen-free water (water enriched with zero solution). The sensor identifies unassisted the slope calibration (75 to 140 % SAT) and the calibration of the zero point (0 to 10 %SAT). No further selection is necessary. These limits are valid for the three types of calibration "air", "water" and "ref".

Coding	Field	Selection or range (factory settings bold)	Display	Info
C	Function group CALIBRATION	Calibration oxygen		Calibration settings.
C1 (1)	Calibration in air	Air (1) H ₂ O (2) Ref (3)		Calibration in air is only possible if air temperature is ≥-5 °C (≥23 °F).
	Remove sensor from the medium and dry completely .			

Coding		Field	Selection or range (factory settings bold)	Display	Info
	C111	Start calibration	Last sensor slope Counter in second row counts down: 600 s → 0 s		COS31/41/71: After 530 s the sensor slope is checked for 10 s. Permitted range 75 % to 140 % (for COS41: 50 % to 150 %), otherwise error E032 occurs and calibration is aborted. The stability of the signal is checked during the last 60 s of the calibration (< 1%), if greater: error E044 and calibration is aborted. COS61: The calibration procedure lasts between 60 and 600 seconds. The stability of the signal (< 1%) and the slope (75 to 140 %) each of them will be tested for 60 s. If o. k. the data will be transferred, if not, the test starts again. After 600 s the calibration procedure will be aborted and error E032 (slope) or E044 (stability) will be displayed.
	C112	Calibration status is displayed	o.k. E xxx		If the calibration status is not o.k., see chapter "System error messages".
		Immerse sensor in medium, if C112 = o. k.			If C112 = E xxx, then only no or new . If new, return to C. If yes/no, return to "Measurement".
	C113	Store calibration results?	yes no new		If C113 = E xxx, then only no or new . If new, return to C. If yes/no, return to "Measurement".
C1 (2)		Calibration in air-saturated water	Air (1) H₂O (2) Ref (3)		
		Remove sensor from medium and immerse in air-saturated water			

Coding		Field	Selection or range (factory settings bold)	Display	Info
	C121	Start calibration	Last sensor slope Counter in second row counts down: 600 s → 0 s		COS31/41/71: After 530 s the sensor slope is checked for 10 s. Permitted range 75 % to 140 % (for COS41: 50 % to 150 %), otherwise error E032 occurs and calibration is aborted. The stability of the signal is checked during the last 60 s of the calibration (< 1%), if greater: error E044 and calibration is aborted. COS61: The calibration procedure lasts between 60 and 600 seconds. The stability of the signal (< 1%) and the slope (75 to 140 %) each of them will be tested for 60 s. If o. k. the data will be transferred, if not, the test starts again. After 600 s the calibration procedure will be aborted and error E032 (slope) or E044 (stability) will be displayed.
	C122	Calibration status is displayed	o. k. Exxx		If the calibration status is not o.k., see chapter "System error messages".
		Remove sensor from air-saturated water and reimmerse in medium, if C122 = o. k.			
	C123	Store calibration results?	yes no new		If C122 = E xxx, then only no or new . If new, return to C. If yes/no, return to "Measurement".
C1 (3)		Single-point calibration in medium	Air (1) H ₂ O (2) Ref (3)		The calibration value must be determined using an external method, e. g.: <ul style="list-style-type: none"> ▪ Oxygen handheld measuring device ▪ Winkler titration
	C131	Enter calibration value	Current value		Minimum value is 0.2 mg/l
	C132	Slope is displayed	100.0 % 75.0 to 140 %		
	C133	Calibration status is displayed	o.k. Exxx		If the calibration status is not o.k., see chapter "System error messages".

Coding			Field	Selection or range (factory settings bold)	Display	Info
		C134	Store calibration results?	yes no new		<p>If C133 = E xxx, then only no or new. If new, return to C. If yes/no, return to "Measurement".</p>

7 Diagnostics and troubleshooting

7.1 Troubleshooting instructions

The transmitter constantly monitors its functions itself. If an error occurs which the device recognizes, this is indicated on the display. The error number is shown below the display of the main measured value. If more than one error occurs, you can call these up with the MINUS key.

Refer to the "System error messages" table for the possible error numbers and remedial measures.

Should a malfunction occur without any transmitter error message, please refer to the "Process-specific errors" or the "Device-specific errors" tables to localize and rectify the error. These tables provide you with additional information on any spare parts required.

7.2 System error messages

The system error messages can be called up and selected with the MINUS key.

Error no.	Display	Tests and/or remedial measures	Alarm contact		Error current		Automatic cleaning start		PROFIBUS status	
			factory	user	factory	user	factory	user	PV ¹⁾	Temp
E001	EEPROM memory error	1. Switch device off and then on again.	Yes		No		—	— ²⁾	0C	0C
E002	Instrument not calibrated, calibration data invalid, no user data, user data invalid (EEPROM error), instrument software not suitable to hardware (controller)	2. Load device software compatible with the hardware (with optoscope, see "Optoscope service tool" section). 3. Load measurement-parameter specific device software. 4. If the error persists, send in the device for repair to your local service organisation or replace the device.	Yes		No		—	— ²⁾	0C	0C
E003	Download error	Invalid configuration. Repeat download, check optoscope.	Yes		No		No		0C	0C
E004	Instrument software version not compatible with module hardware version	Load software compatible with hardware.	Yes		No		No		0C	0C
E007	Transmitter malfunction, instrument software not compatible with transmitter version	Load measurement-parameter specific device software.	Yes		No		—	— ²⁾	0C	0C
E008	Sensor or sensor connection faulty	Check sensor and sensor connection (Service).	Yes		Yes		—	—	0C	80
E010	Temperature sensor defective	Send in sensor for repair.	Yes		No		—	—	80	0C
E017	Sensor electrode section defective	COS31/41/71: Send in sensor for repair. COS61: Replace membrane cap, calibrate sensor.	Yes		Yes		—	—	0C	0C
E018	Sensor membrane damaged (not sealed) or membrane cap not completely screwed on	COS31/41/71: Replace membrane cap. Completely screw on membrane cap. COS61: Replace membrane cap during the next preventive maintenance.	Yes		Yes		—	—	0C	80
E020	Signal range of sensor undershot	Check medium and sensor.	Yes		No		—	—	44	80

Error no.	Display	Tests and/or remedial measures	Alarm contact		Error current		Automatic cleaning start		PROFIBUS status	
			factory	user	factory	user	factory	user	PV ¹⁾	Temp
E022	Signal range of sensor exceeded	Check medium and sensor.	No		No		—	—	44	80
E032	During calibration signal outside permitted slope range 75 to 140 % (for COS41: 50 to 150 %)	Check sensor and recalibrate.	Yes		No		—	— ²⁾	80	80
E044	During calibration sensor unstable	Check sensor and recalibrate.	No		No		No		80	80
E057	Main parameter measuring range exceeded	Check measurement, control and connections.	Yes		No		No		44	80
E059	Below temperature measuring range		Yes		No		No		80	44
E061	Temperature measuring range exceeded		Yes		No		No		80	44
E063	Below current output range 1	Check configuration.	Yes		No		No		80	80
E064	Current output range 1 exceeded	Check measured value and current assignment.	Yes		No		No		80	80
E065	Below current output range 2		Yes		No		No		80	80
E066	Current output range 2 exceeded		Yes		No		No		80	80
E067	Alarm threshold limit contactor 1 exceeded	Check configuration.	Yes		No		No		80	80
E068	Alarm threshold limit contactor 2 exceeded		Yes		No		No		80	80
E069	Alarm threshold limit contactor 3 exceeded		Yes		No		No		80	80
E070	Alarm threshold limit contactor 4 exceeded		Yes		No		No		80	80
E080	Current output 1 range too small	Increase range in "Current outputs" menu.	Yes		No		—	— ²⁾	80	80
E081	Current output 2 range too small		Yes		No		—	— ²⁾	80	80
E082	Air pressure range undershot (<500 hPa)	Measurement only possible when uncompensated or with altitude data	Yes		No		No		80	80
E083	Air pressure range exceeded (>1100 hPa)		Yes		No		No		80	80
E085	Incorrect setting for error current	If the current range "0 to 20 mA" was selected in field O311, the error current "2.4 mA" may not be set.	Yes		No		No		80	80
E100	Current simulation active		No		No		—	— ²⁾	80	80
E101	Service function active	Switch off service function or switch device off and then on again.	No		No		—	— ²⁾	80	80
E102	Manual mode active		No		No		—	— ²⁾	80	80
E106	Download active	Wait for download to finish.	No		No		—	— ²⁾	80	80
E116	Download error	Repeat download.	Yes		No		—	— ²⁾	0C	0C
E152	Measuring signal of main parameter delayed or frozen (AC function / alternation check)	Inspect sensor and connection line, repair or replace.	Yes		No		No		44	44

Error no.	Display	Tests and/or remedial measures	Alarm contact		Error current		Automatic cleaning start		PROFIBUS status	
			factory	user	factory	user	factory	user	PV ¹⁾	Temp
E154	Below lower alarm threshold for period exceeding alarm delay	Perform manual comparison measurement if necessary. Service sensor and recalibrate.	Yes		No		No		- ³⁾	-
E155	Above upper alarm threshold for period exceeding alarm delay		Yes		No		No		-	-
E156	Actual value undershoots alarm threshold (CC setpoint) for longer than the set permissible maximum period		Yes		No		No		-	-
E157	Actual value exceeds alarm threshold (CC setpoint) for longer than the set permissible maximum period		Yes		No		No		-	-
E162	Dosage stop	Check settings in the CURRENT INPUT and CHECK function groups.	Yes		No		No		-	-
E171	Flow in main stream too low or zero	Restore flow.	Yes		No		No		-	-
E172	Switch-off limit for current input exceeded	Check process variables at sending measuring instrument. Change range assignment if necessary.	Yes		No		No		-	-
E173	Current input < 4 mA	Check process variables at sending measuring instrument.	Yes		No		No		-	-
E174	Current input > 20 mA	Check process variables at sending measuring instrument. Change range assignment if necessary.	Yes		No		No		-	-

- 1) PV = Process variable
- 2) If this error occurs, there is no possibility of starting a cleaning session (field F8 not applicable with this error).
- 3) Current error messages not applicable via PROFIBUS

7.3 Process specific errors

Use the following table to locate and correct errors.

Error	Possible cause	Tests and / or remedial measures	Equipment, spare parts, personnel
Value indicated 0.0	Incorrect sensor	Check sensor type.	COS41 for COM2x3-DX/DS. COS31/71 for COM2x3-WX/WS.
	Sensor defective	<ul style="list-style-type: none"> - Test with new sensor. - Instrument test with sensor diagram. - Sensor current test. 	Sensor type acc. to instrument version. Sensor simulation see chapter "Maintenance of the entire measuring point".
	Sensor extension line interrupted	Check junction boxes and line.	Sensor simulation see chapter "Maintenance of the entire measuring point".
	Incorrect sensor connection	Check connection.	See chapter "Wiring".
	Instrument input defective	Replace module MKO1 (DX/DS). Replace module MKO5 (WX/WS).	See spare parts list.
No or creeping display change	Sensor soiled	Clean sensor membrane.	See instructions for COSxx. Heavily soiled media: use spray cleaning.
	Sensor installed in dead zone	Check installation conditions, move sensor to area with optimal flow conditions.	
Value indicated too small / sensor can probably not be calibrated	Membrane soiled	Clean sensor membrane.	See instructions for COSxx. Heavily soiled media: use spray cleaning.
	Incorrect temperature measurement	Check temperature value.	Ref. measurement / thermometer.
	Incorrect altitude setting	Check altitude value.	
	Incorrect air pressure measurement	Check pressure value in field S11. sea level: approx. 1013 hPa. 500 m above sea level: approx. 950 hPa.	Only with version WX/WS/DS. Caution: display value = absolute atmospheric pressure.
	Electrolyte used up or soiled	Replace electrolyte.	See instructions for COSxx.
	Flow rate too low	Check installation conditions, move sensor to area with optimal flow conditions.	
	Sensor type recognition (COS31/61/71) unsuccessful	Calibrate sensor to air.	See chapter "Calibration".
	Polarisation incomplete	After sensor commissioning (also after interruption to operation) wait for polarisation time.	Polarisation is complete when the measured value is stable, max. approx. 60 minutes.
Value indicated too high / sensor can probably not be calibrated	Incorrect altitude setting	Check altitude value.	
	Incorrect air pressure measurement	Check pressure value in field S11. sea level: approx. 1013 hPa. 500 m above sea level: approx. 950 hPa.	Only with version WX/WS/DS. Caution: display value = absolute atmospheric pressure.
	Electrolyte or soiled	Replace electrolyte.	See instructions for COSxx.
	Air cushion under membrane	Install new membrane cap.	For procedures and spare parts ordering see instructions for COSxx.
	Anode coating worn off (silver coloured)	Sensor regeneration at factory.	Normal anode colour is brownish.
	"S" membrane on standard sensor	Install correct membrane cap.	"S" membrane cap recognisable by white colour (COS31). With COS31 self-recognition of S version.
	Sensor type recognition (COS31/61/71) unsuccessful	Calibrate sensor in air.	See chapter "Calibration".
Simulation with sensor incorrect	Incorrect sensor voltage	Required sensor voltage 6.5 to 8.5 VDC.	See chapter "Function, simulation and test with COS31 and COS71".

Error	Possible cause	Tests and / or remedial measures	Equipment, spare parts, personnel
Fixed incorrect measured value	Impermissible instrument operating state (no response to key actuation)	Switch instrument off and back on.	EMC problem: check line routing. If problem persists, check for possible sources of interference.
Incorrect temperature value	Incorrect sensor connection	Verify connections using connection diagram.	Connection diagram in chapter "Electrical connection".
	Measuring cable defective	Check cable for interruption/short circuit/ shunt.	Ohmmeter or on-site simulation.
	Temp. probe in sensor defective	Measure resistance value in sensor (red and brown sensor lines) only possible with COS41.	Ohmmeter / values see chapter "Simulation temperature sensor".
Measured value variations	Faults on measuring cable	Connect cable screening according to circuit diagram.	See chapter "Wiring".
	Faults on signal output line	Check line routing, possibly route line separately.	Separate signal output, measuring input and power supply lines.
	Irregular flow/turbulences/large air bubbles	Select a better installation site or calm turbulences. Possibly use large measured value damping factor.	Measured value damping see field A5.
Controller or timer cannot be activated	No relay module available	Install module LSR1-2 or LSR1-4.	
Controller/limit contact does not work	Controller switched off	Activate controller.	See fields R2xx.
	Controller in "Manual/Off" mode	Choose "Auto" or "Manual/On" mode.	Keyboard, REL-key
	Pickup delay setting too long	Disable or shorten pickup delay.	See fields R2xx.
	"Hold" function active	"Automatic Hold" during calibration, "Hold" input activated; "Hold" via keyboard active.	See fields S2 to S4.
Controller/limit contact works continuously	Controller in "Manual/On" mode	Set controller to "Manual/Off" or "Auto".	Keyboard, REL and AUTO keys.
	Dropout delay setting too long	Shorten dropout delay.	See field R2xx.
	Control loop interruption	Check measured value, current output, actuators, chemical supply.	
No O ₂ current output signal	Line open or short-circuited	Disconnect line and measure directly on instrument.	mA meter 0–20 mA.
	Instrument with PROFIBUS PA/DP	PA/DP instruments have no current output.	
Fixed current output signal	Current simulation active	Switch off simulation.	See field O3.
	Impermissible operating state of processor system	Switch instrument off and back on.	EMC problem: check installation, screen, grounding if problem persists.
Incorrect current output signal	Incorrect current assignment	Check current assignment: 0–20 mA or 4–20 mA?	Field O311
	Total load in current loop excessive (> 500 Ω.)	Disconnect output and measure directly on instrument.	mA meter for 0–20 mA DC.
Current output table not accepted	Value interval too small	Select practical intervals.	
No temperature output signal	Instrument does not have 2nd current output	Refer to nameplate for variant; change LSCH-x1 module if necessary.	Module LSCH-x2, see chapter "Spare parts".
	Instrument with PROFIBUS PA	PA instrument has no current output!	
Chemoclean function not available	No relay module (LSR1-x) installed or only LSR1-2 available Additional function not enabled	Install LSR1-4 module. Chemoclean is enabled using the release code supplied by E+H in the Chemoclean retrofit kit.	Module LSR1-4, see chapter "Spare parts".

Error	Possible cause	Tests and / or remedial measures	Equipment, spare parts, personnel
Plus package functions not available	Plus package not enabled (enable with code that depends on serial number and is received from E+H with order of extension package)	<ul style="list-style-type: none"> - When upgrading instrument with Plus package: code received from E+H ⇒ enter. - After replacing defective LSCH/LSCP module: first enter instrument serial number (s. nameplate) manually, then enter code. 	For a detailed description, see chapter "Replacement of central module".
No HART communication	No central HART module	Verify by looking at nameplate: HART = -xxx5xx and -xxx6xx.	Upgrade to LSCH-H1 / -H2.
	No or wrong DD (device description)	For further information see BA00208C/07/EN, "HART® - Field communication with Liquisys M CxM223/253".	
	HART interface missing		
	Instrument not registered with HART server		
	Load too low (load > 230 Ω required)		
	HART receiver (e.g. FXA 191) not connected via load but via power supply		
	Incorrect device address (addr. = 0 for single operation, addr. > 0 for multi-drop operation)		
	Line capacitance too high		
	Line interferences		
Several devices set to same address	Set addresses correctly.	Communication not possible with several devices set to same address.	
No PROFIBUS® communication	No central PA/DP module	Verify by looking at nameplate: PA = -xxx3xx /DP = xxx4xx.	Upgrade to LSCP module, see chapter "Spare parts".
	Incorrect instrument software version (without PROFIBUS)	For further information, see BA00209C/07/EN "PROFIBUS PA/DP - Field communication with Liquisys M CxM223/253".	
	Commuwin (CW) II: Incompatible CW II and instrument software versions		
	No or incorrect DD/DLL		
	Incorrect baud rate setting for segment coupler in DPV-1 server		
	Incorrect station (master) addressed or duplicate address		
	Incorrect station (slaves) address		
	Bus line not terminated		
	Line problems (too long, cross section too small; not shielded, screen not grounded, wires not twisted)		
	Bus voltage too low (bus supply voltage typ. 24 V DC for non-Ex)		

7.4 Instrument specific errors

The following table helps you during the diagnosis and points to any spare parts required. Depending on the degree of difficulty and the measuring equipment present, diagnosis is carried out by:

- Trained operator personnel
- The user's trained electrical technicians
- Company responsible for system installation/operation
- Endress+Hauser Service

Information on the exact spare part designations and on how to install these parts can be found in the "Spare parts" section.

Error	Possible cause	Tests and/or remedial measures	Execution, tools, spare parts
Device cannot be operated, display value 9999	Operation locked	Press CAL and MINUS keys simultaneously.	See "Function of keys" section.
Display dark, no light-emitting diode active	No line voltage	Check whether line voltage is present.	Electrical technician/e.g. multimeter
	Supply voltage wrong/too low	Compare actual line voltage and nameplate data.	User (data for energy supply company or multimeter)
	Connection faulty	Terminal not tightened; insulation jammed; wrong terminals used.	Electrical technician
	Device fuse defective	Compare line voltage and the nameplate data and replace fuse.	Electrical technician/suitable fuse; see drawing in "Spare parts" section.
	Power unit defective	Replace power unit, note variant.	On-site diagnosis by Endress+Hauser Service, test module necessary
	Central module defective	Replace central module, note variant.	On-site diagnosis by Endress+Hauser Service, test module necessary
	COM253: ribbon cable item 310 loose or defective	Check ribbon cable, renew if necessary.	See "Spare parts" section.
Display dark, light-emitting diode active	Central module defective (module: LSCH/LSCP)	Renew central module, note variant.	On-site diagnosis by Endress+Hauser Service, test module necessary
Display is on but – No change in display and/or – Device cannot be operated – Missing pixels in display	Device or module in device not correctly mounted	COM223: reinstall module. COM253: reinstall display module.	Perform with the aid of the installation drawings in the "Spare parts" section.
	Operating system in unpermitted mode	Switch device off and then on again.	Poss. EMC problem: if this persists, check the installation.
	Conductive rubber soiled	Replace LSCxx module. Clean conductive rubber and printed conductor.	Only in emergency, with alcohol and glass fibre brush
	Contact pressure too low	Lay paper strips in frame.	Only in emergency, better: replace LSCxx.
Device gets hot	Voltage wrong/too high	Compare line voltage and nameplate data.	User, electrical technician
	Power unit defective	Replace power unit.	Diagnosis only by Endress+Hauser Service
Incorrect meas. O ₂ and/or temperature	Transmitter module defective (module: MKO1/MKO5), please first carry out tests and take measures as per the "Process errors without messages" section to make sure that the error is not in the cabling or in the sensor	Measuring input test MKO1: – Connect resistors for oxygen and temperature, see chapter "Simulation oxygen measurement". Measuring input test MKO5: – See chapter "Function, simulation and test with COS31 and COS71".	If test negative: replace module (note variant). Perform with the aid of the exploded drawings in the "Spare parts" section. Only possible with intact sensor as digital data transfer sensor <-> instrument. If test positive: check peripherals once more.
	Incorrect sensor current	Sensor current readable in the display in measurement mode by pressing PLUS key 3x.	Display in nA. Nominal value in air for 20 °C and 1013 hPa: 290 nA

Error	Possible cause	Tests and/or remedial measures	Execution, tools, spare parts
Pressure value incorrect / unreadable	Defective pressure sensor	Module MKO1 defective Module MKO5 defective	Pressure readable in field S11 Caution: The absolute air pressure is displayed.
	No pressure sensor available	WX/WS/DS always with pressure sensor DX with MKO1 always without pressure sensor	
Current output, current value incorrect	Adjustment not correct	Check with installed current simulation, connect mA meter directly to current output.	If simulation value incorrect: adjustment in factory or new module LSCxx required. If simulation value correct: check current loop for load and shunts.
	Load too big		
	Shunt/short to ground in current loop		
	Incorrect mode of operation	Check whether 0–20 mA or 4–20 mA is selected.	
No current output signal	Current output stage defective (module LSCH/LSCP)	For safety reasons, first completely disconnect the auxiliary power output. Check with installed current simulation, connect mA meter directly to current output.	If test negative: Renew central module LSCH/LSCP (note variant).
No function of additional relay	COM253: ribbon cable item 320 loose or defective	Check ribbon cable seating, renew cable if required.	See "Spare parts" section.
Only 2 additional relays can be triggered	Relay module LSR1-2 installed with 2 relays	Upgrade to LSR1-4 with 4 relays.	User or Endress+Hauser Service
Additional functions (Plus package) missing	No or incorrect release code used	If retrofitting: check whether the correct serial number was quoted when ordering the Plus package.	Handled by Endress+Hauser Sales
	Incorrect device serial number saved in LSCH/LSCP module	Check whether serial number on the nameplate matches SNR in LSCH/ LSCP (field E112).	The serial number of the device is definitive for the Plus package.
	Changed product strategy	From introduction WX/WS: – WX/WS/DS always with pressure sensor – DX always without pressure sensor	For DS: Use altitude setting.
Additional functions (Plus package and/or Chemoclean) missing after LSCH/LSCP module replaced	Replacement modules LSCH or LSCP have the device serial number 0000 when they leave the factory. The Plus package or Chemoclean are not enabled on leaving the factory.	In the case of LSCH/LSCP with SNR 0000, a device serial number can be entered once in fields E114 to E116. Then enter the release code for the Plus package and/or Chemoclean.	For a detailed description, see "Replacing central module" section.
No HART or PROFIBUS-PA/-DP interface function	Incorrect central module	HART: LSCH-H1 or H2 module, PROFIBUS-PA: LSCP-PA module, PROFIBUS-DP: LSCP-DP module, see field E112.	Replace central module; user or Endress+Hauser Service.
	Wrong software	SW version see field E111.	SW can be modified with optoscope.
	Bus problem	Remove some devices and repeat the test.	Contact Endress+Hauser Service.
No sensor data in E151 to E159	Analog sensor connected	For COS3 and compatible sensors, no data exchange possible	

8 Maintenance

Take all the necessary measures in time to guarantee the operational safety and reliability of the entire measuring system.

Maintenance work at the transmitter comprises:

- Calibration (see "Calibration" section)
- Cleaning of assembly and sensor
- Cable and connection check

When performing any work on the device, bear in mind any potential impact this may have on the process control system or on the process itself.

NOTICE

Electrostatic discharge (ESD)

Risk of damage to electronic components

- ▶ Take personal protective measures to avoid ESD, such as discharging beforehand at PE or permanent grounding with a wrist strap.
- ▶ For your own safety, use only genuine spare parts. With genuine spare parts, the function, accuracy and reliability are also guaranteed after repair.

8.1 Maintenance of the entire measuring point

8.1.1 Cleaning the transmitter

Clean the front of the housing with usual commercial cleaning agents.

In accordance with DIN 42 115, the front is resistant to:

- Ethanol (short periods)
- Diluted acids (max. 2% HCl)
- Diluted bases (max. 3% NaOH)
- Soap-based household cleaners

NOTICE

Prohibited cleaning agents

Damage to the housing surface or housing seal

- ▶ For cleaning purposes, never use concentrated mineral acids or bases.
- ▶ Never use organic cleaners such as benzyl alcohol, methanol, methylene chloride, xylene or concentrated glycerol cleaner.
- ▶ Never use high-pressure steam for cleaning purposes.

8.1.2 Test variant 1 (DX/DS with COS41)

Simulation of oxygen measurement

The instrument versions DX/DS work with the sensor COS41, i.e. with amperometric sensors without a preamp.

To perform a functional test of the instrument, the COS41 sensor can be simulated by resistors. Since the display value greatly depends on the sensor slope setting and on temperature, the following values should be considered as reference values:

Simulation resistance	Display value
∞ (open)	0 mg O ₂ /l
1.9 M Ω	7 to 13 mg O ₂ /l
With 1.9 M Ω and a temperature equivalent resistance of 37.3 k Ω after calibration	9.0 to 9.2 mg O ₂ /l
4.06 M Ω	3 to 6 mg O ₂ /l

Simulation temperature sensor

The COS41 sensor uses an NTC sensor (30.0 k Ω /25 °C) for temperature measurement. Use the following equivalent resistances to test the temperature measurement:

Simulation resistance	Display value
95.0 k Ω	0.0 °C (32 °F)
58.7 k Ω	10.0 °C (50 °F)
37.3 k Ω	20.0 °C (68 °F)
30.0 k Ω	25.0 °C (77 °F)
24.3 k Ω	30.0 °C (86 °F)

Test procedure

1. Connect the O₂ equivalent resistance (e. g. decade resistor) to terminals 90 and 91.
2. Connect the temperature equivalent resistance (e. g. decade resistor) to terminals 11 and 12.
3. Air pressure measurement:
The air pressure measured can be checked in field S11 (absolute air pressure). There is no air pressure compensation for the DX version. Use the location altitude setting to compensate for the air pressure influence.

8.1.3 Test variant 2 (WX/WS with COS31 or COS71)

Function, simulation and test with COS31 and COS71

The instrument versions WX/WS work preferably with the sensors COS31, COS31-S and COS71. These sensors have digital data transfer using the interface RS485. The sensors COS31 or COS31-S are automatically recognised internally after calibration. All the sensor data are forwarded to the transmitter by data exchange. After a mains supply interruption, the data are resent to the transmitter. The sensors require a 6.5 to 8.5 VDC voltage supply from the transmitter.

Due to the digital data, **no simulation** of sensor signals is possible.

Test possibilities in digital mode:

- Measure supply voltage (6.5 to 8.5 VDC, see connection diagram).
- Connect intact sensor COS31, COS31-S or COS71.
- Check O₂ measured value and temperature value on transmitter.
- The O₂ input can be tested by measuring the output DC voltage.
 - The reference is terminal 0, O₂ input is terminal 18:
 - 0 mV = 0.0 mg O₂/l
 - -750 mV = O₂ saturation = 8.1 mg O₂/l (at 25 °C). Value indicated depends on last calibration.
- Measure sensor current consumption (max. ± 5 mA).
- The sensor data can be read off in the fields "E+H Service" E151 to E159.
- In measurement mode, the sensor current can be displayed in nA by pressing the PLUS key.

Guide values:

- COS31: approx. 40 nA correspond to 1 mg O₂/l at 25 °C
- COS31-S: approx. 120 nA correspond to 1 mg O₂/l at 25 °C
- COS61: approx. 1300 nA correspond to 8 mg O₂/l at 25 °C
- COS71: approx. 800 nA correspond to 1 mg O₂/l at 25 °C

8.1.4 Maintenance oxygen sensors

Please refer to the operating instructions for your sensor with regard to sensor maintenance and troubleshooting:

COS31	BA00285/07/EN
COS41	BA00284/07/EN
COS61	BA00387/07/EN
COS71	BA00286/07/EN

The operating instructions contain detailed information including:

- Sensor design and function
- Mounting and installation
- Electrical connection
- Start-up and calibration
- Calculation examples and tables for verification of measured values
- Maintenance, regeneration, cleaning
- Trouble-shooting table
- Accessories and spare parts
- Technical data and ordering information

8.1.5 Maintenance assembly

Please refer to the corresponding assembly Operating Instructions for information on maintaining and trouble-shooting the assembly. Here you can find a description for assembling and disassembling, sensor replacement, seal replacement, as well as information on stability and spare parts and accessories.

8.1.6 Connecting lines and junction boxes

Since COS41 works with low measuring currents, shunts in connecting cables and junction boxes may cause considerable inaccuracy.

The following is to be assured:

- Intact gaskets on lids and cable glands
- Dry and clean inner compartment (if necessary dry, clean and insert a dehydrating bag)
- Lines ferrules, terminals and connectors must be free of corrosion
- Terminal screws must be tightened firmly
- Cables must enter junction boxes and instruments from below
- Make a downward cable loop in case of lateral cable entries to allow water to drip off

 If the function test explained in the previous chapter is performed on a junction box instead of the instrument, the junction box, terminals and connecting line to the instrument are automatically included in the test.

COS31, COS61 and COS71 sensors work with a digital interface and therefore are not sensitive to electrical faults and shunting by humidity. Nevertheless, follow the recommendations mentioned above.

9 Repair

9.1 Spare parts

Spare parts are to be ordered from your sales center responsible. Specify the order numbers listed in the chapter "Spare parts kits".

To be on the safe side, you should **always** specify the following data with your spare part orders:

- Instrument order code (order code)
- Serial number (serial no.)
- Software version where available

Refer to the nameplate for the order code and serial number.

The software version is displayed in the instrument software (see chapter "Instrument configuration") if the instrument processor system is functional.

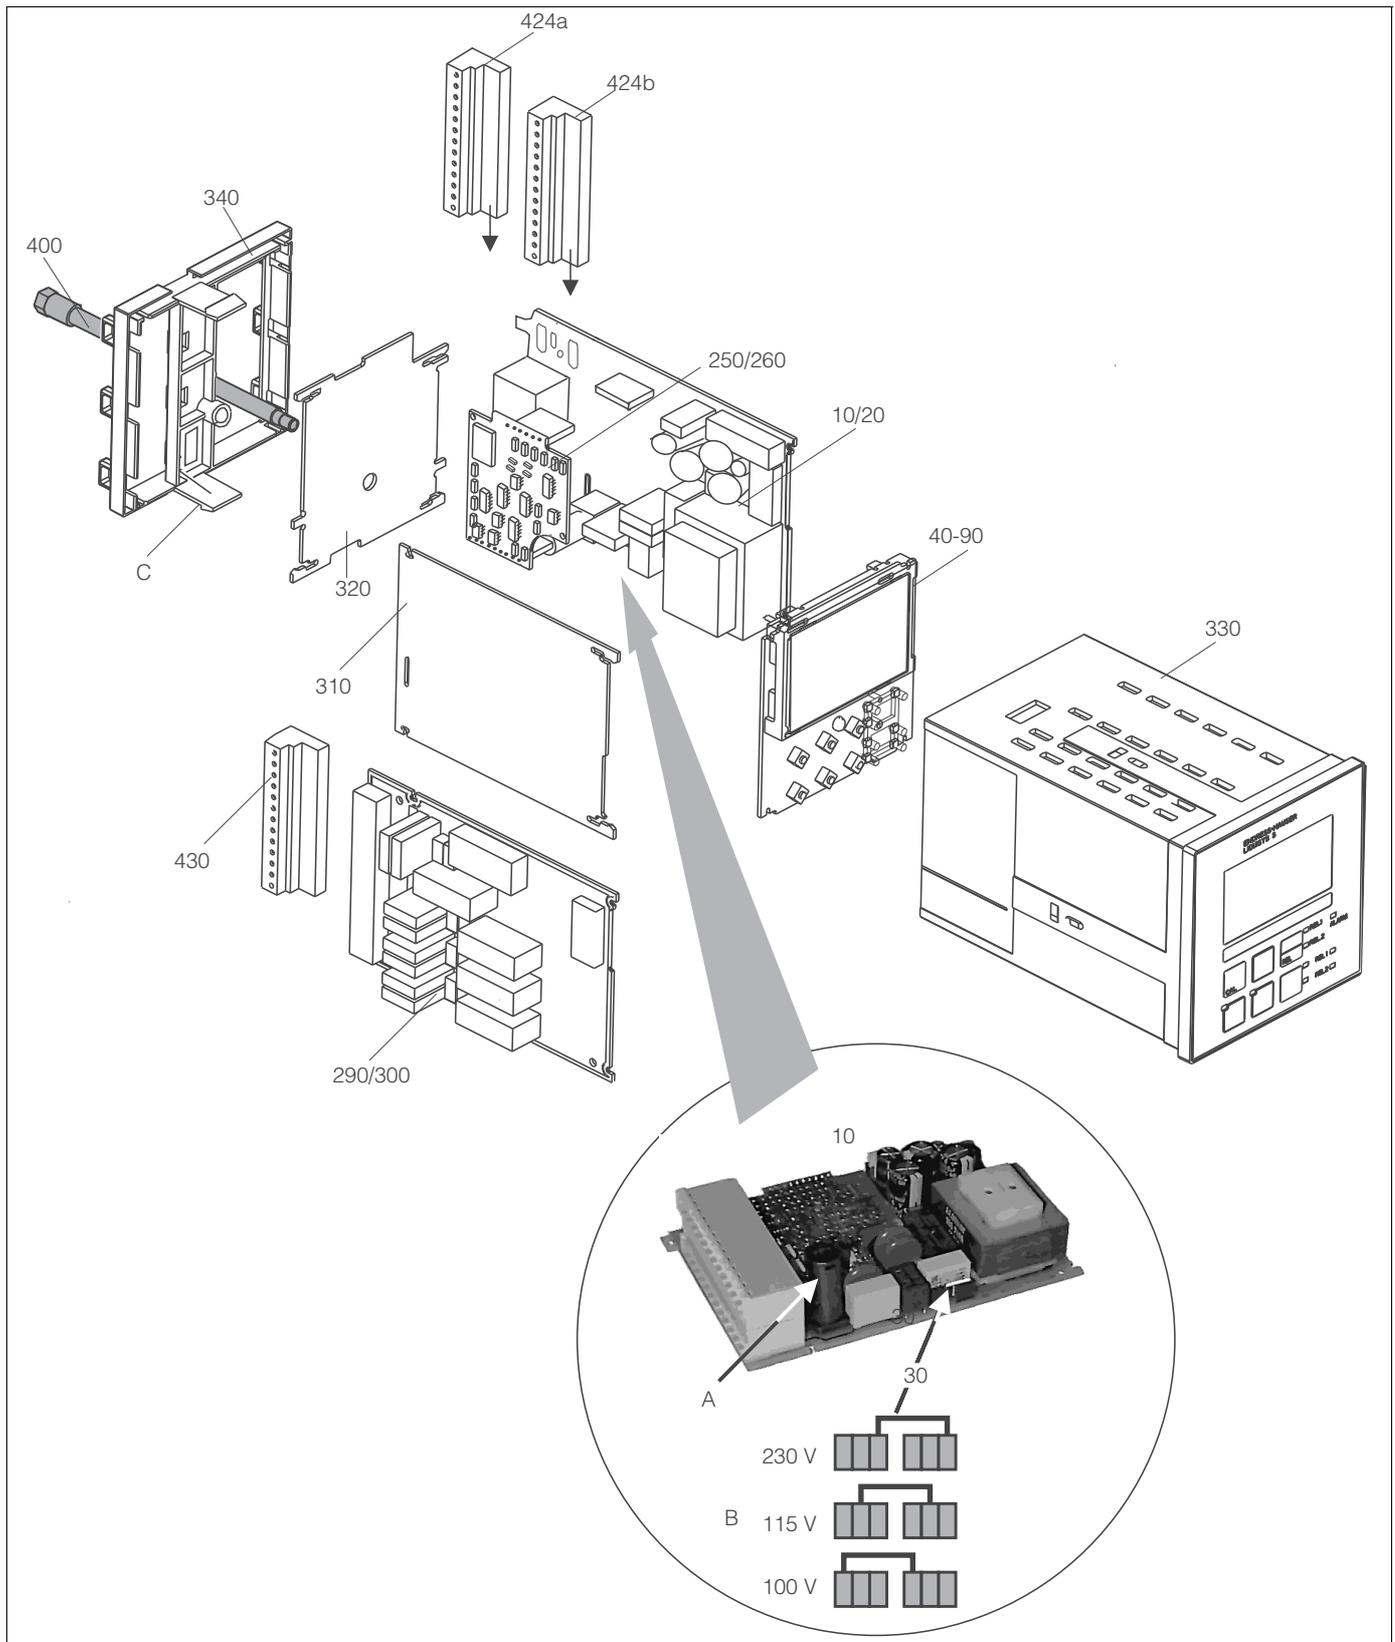
9.2 Dismantling the panel-mounted instrument

 Please note the effects on the process if the device is taken out of service!

Please refer to the following diagram for the item numbers.

1. Disconnect the terminal block (item 424 b) from the rear of the device to de-energize the device.
2. Then remove the terminal blocks (item 424 a and possibly 430) from the rear of the device. Now you can disassemble the device.
3. Press in the latches of the end frame (item 340) and remove the frame from the rear.
4. Release the special screw (item 400) by turning it counter-clockwise.
5. Remove the entire electronics block from the housing. The modules are only mechanically connected and can be easily separated:
 - Simply remove the processor/display module from the front.
 - Pull out the brackets of the rear plate (item 320) slightly.
 - Now you can remove the side modules.
6. Remove the O₂ transmitter (item 250/260) as follows:
 - Using fine side-cutting pliers, nip off the heads of the synthetic distance holders.
 - Then remove the module from above.

Assembly is the reverse of the disassembly sequence. Tighten the special screw hand-tight without a tool.



C07-COM223xx-09-06-00-xx-001.eps

Fig. 36: Exploded drawing of panel mounted instrument

The exploded drawing contains the components and spare parts of the panel-mounted instrument. You can take the spare parts and the corresponding order number from the following section using the item numbers.

Item	Kit description	Name	Function/contents	Order number
10	Power unit (main module)	LSGA	100 / 115 / 230 V AC	51500317
20	Power unit (main module)	LSGD	24 V AC + DC	51500318
30	Jumper		Part of power unit item 10	
40	Central module (controller)	LSCH-S1	1 current output	51501225
50	Central module (controller)	LSCH-S2	2 current outputs	51501222
60	Central module (controller)	LSCH-H1	1 current output + HART	51501223
70	Central module (controller)	LSCH-H2	2 current outputs + HART	51501226
80	Central module (controller)	LSCP-PA	PROFIBUS PA/no current output	51501227
90	Central module (controller)	LSCP-DP	PROFIBUS DP/no current output	51502500
90	Kit COM2x3 Central module PROFIBUS DP	LSCP-DP	Central module PROFIBUS DP Relay module + 2 relays Current input and terminals valid of: hardware version 2.10	71134729
250	O ₂ transmitter	MK01 (-DX/DS)	O ₂ + temperature O ₂ + temperature + air pressure	51501207 51501208
260	O ₂ transmitter	MK05 (-WX/ WS)	O ₂ + temperature + air pressure	51506938
290	Relay module	LSR1-2	2 relays	51500320
290	Relay module	LSR2-2i	2 relays + current input 4 to 20 mA	51504304
290	Kit CxM2x3 Relay module PROFIBUS DP	LSR2-DP	Relay module + 2 relays Current input and terminals DP valid of: hardware version 2.10	71134732
300	Relay module	LSR1-4	4 relays	51500321
300	Relay module	LSR2-4i	4 relays + current input 4 to 20 mA	51504305
310	Side panel		Kit with 10 parts	51502124
310, 320, 340, 400	Housing mechanical parts		Rear plate, side panel, end frame, special screw	51501076
330, 400	Housing module		Housing with front membrane, sensory tappets, gasket, special screw, tensioning dogs, connection plates and nameplates	51501075
340	End frame PROFIBUS-DP		Rear frame for PROFIBUS DP, with D-submin plug connector	51502513
345	Grounding terminal strip		PE and screening connections	51501086
424a, 424b	Terminal strip set Standard + HART / DX + DS		Complete terminal strip set, standard + HART	51501204
424a, 424b	Terminal strip set PROFIBUS PA / DX + DS		Complete terminal strip set, PROFIBUS PA	51502127
424a, 424b	Terminal strip set PROFIBUS DP / DX + DS		Complete terminal strip set, PROFIBUS DP	51502492
430	Terminal strip		Terminal strip for relay module	51501078
A	Fuse		Part of power unit, item 10	
B	Choice of line voltage		Position of jumper on power unit, item 10 depending on line voltage	
C	End frame latches		Part of the end frame	

9.3 Dismantling the field instrument

 Please note the effects on the process if the device is taken out of service!

To dismantle the field instrument you need the following tools:

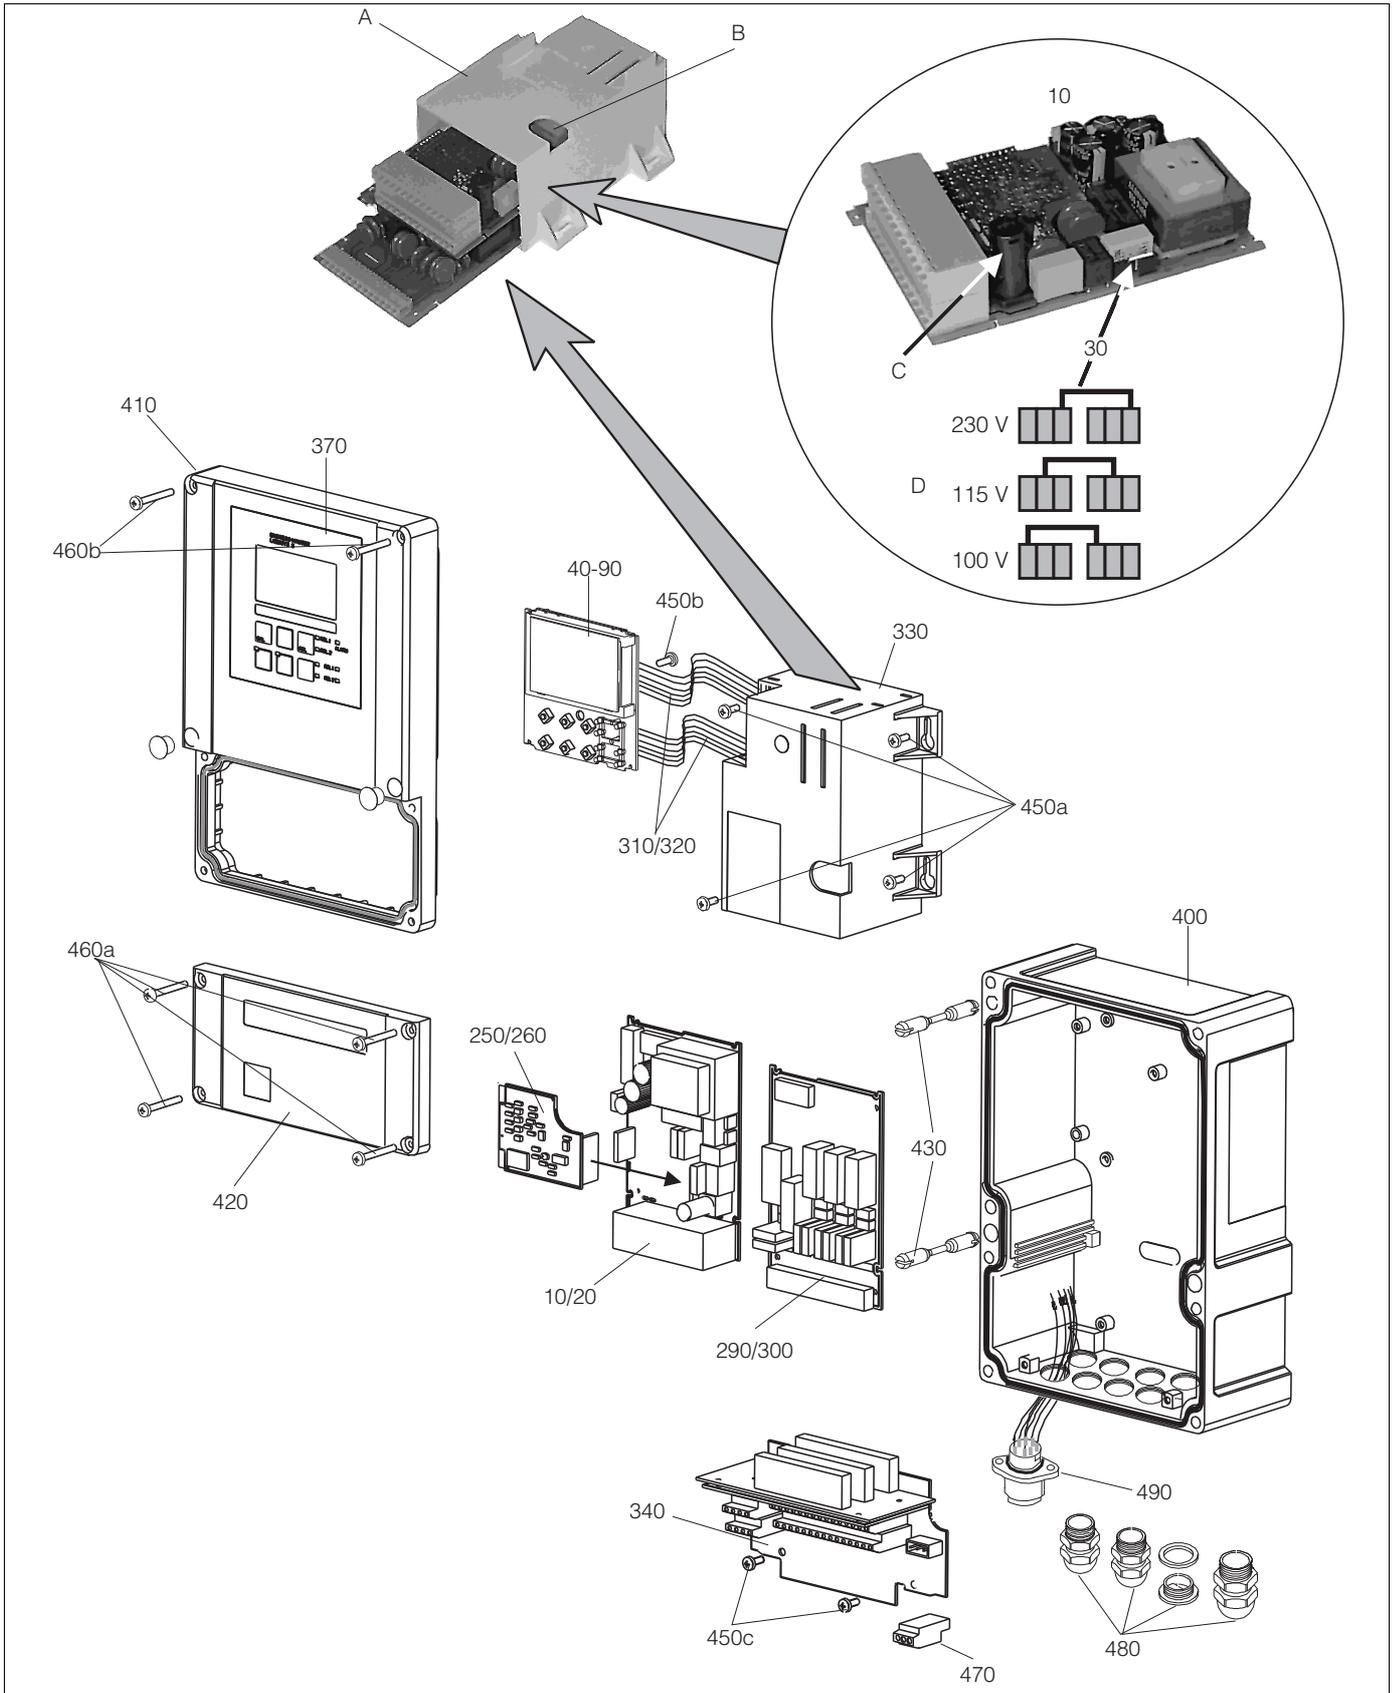
- Standard set of screwdrivers
- Torx-screwdriver size TX 20

Proceed as follows:

1. Open and remove the cover of the connection compartment (item 420).
2. Disconnect the mains terminal (item 470) to de-energize the device.
3. Open the display cover (item 410) and loosen the ribbon cables (item 310/320) on the side of the central module (item 40 to 90).
4. To remove the central module (item 40), loosen the screw in the display cover (item 450 b).
5. Proceed as follows to remove the electronics box (item 330):
 - Release the screws in the housing base (item 450 a) with two revolutions.
 - Then push the entire box backwards and remove it from above.
 - Make sure that module locks do not open!
 - Loosen the ribbon cables (item 310/320).
 - Bend the module locks out and remove the modules.
6. To remove the docking module (item 340), remove the screws in the housing base (item 450 c) and remove the entire module from above.
7. Proceed as follows to remove the O₂ transmitter (item 250/260):
 - Using fine side-cutting pliers, nip off the heads of the synthetic distance sleeves.
 - Then remove the module from above.

To assemble, carefully push the modules into the trolley tracks of the electronics box and let them engage in the side box noses.

 Incorrect mounting is not possible. Modules inserted in the electronics box incorrectly are not operable since the ribbon cables cannot be connected.
Make sure the cover seals are intact to guarantee IP 65 ingress protection.



C07-COM253xx-09-06-00-xx-001.eps

Fig. 37: Exploded drawing of field instrument

The exploded drawing contains the components and spare parts of the field device. You can take the spare parts and the corresponding order number from the following section using the item numbers.

Item	Kit description	Name	Function/contents	Order number
10	Power unit (main module)	LSGA	100 / 115 / 230 V AC	51500317
20	Power unit (main module)	LSGD	24 V AC + DC	51500318
30	Jumper		Part of power unit item 10	
40	Central module (controller)	LSCH-S1	1 current output	51501225
50	Central module (controller)	LSCH-S2	2 current outputs	51501222
60	Central module (controller)	LSCH-H1	1 current output + HART	51501223
70	Central module (controller)	LSCH-H2	2 current outputs + HART	51501226
80	Central module (controller)	LSCP	PROFIBUS PA/no current output	51501227
90	Central module (controller)	LSCP-DP	PROFIBUS DP/no current output	51502500
90	Kit COM2x3 Central module PROFIBUS DP	LSCP-DP	Central module PROFIBUS DP Relay module + 2 relays Current input and terminals valid of: hardware version 2.10	71134729
250	O ₂ transmitter	MKO1 (-DX/DS)	O ₂ + temperature O ₂ + temperature + air pressure	51501207 51501208
260	O ₂ transmitter	MKO5 (-WX/ WS)	O ₂ + temperature + air pressure	51506938
290	Relay module	LSR1-2	2 relays	51500320
290	Relay module	LSR2-2i	2 relays + current input 4 to 20 mA	51504304
290	Kit CxM2x3 Relay module PROFIBUS DP	LSR2-DP	Relay module + 2 relays Current input and terminals DP valid of: hardware version 2.10	71134732
300	Relay module	LSR1-4	4 relays	51500321
300	Relay module	LSR2-4i	4 relays + current input 4 to 20 mA	51504305
310, 320	Ribbon cable lines		2 ribbon cable lines	51501074
330, 340, 450	Internal housing parts		Docking assembly, empty electronics box, small parts	51501073
450a, 450c	Torx screws K4x10		Internal housing parts	
450b	Torx screw for central module		Internal housing parts	
370, 410, 420, 430, 460	Housing cover		Display cover, connection compartment cover, front membrane, hinges, cover screws, small parts	51501068
460a, 460c	Screws for housing cover		Parts of housing cover	
400, 480	Housing base		Base, threaded joints	51501072
430	Hinges		2 pairs of hinges	51501069
470	Terminal strip		Terminal strip for connection to mains	51501079
490	Sensor socket SXB		Sensor connection	51506966
A	Electronics box with relay module LSR1-x (bottom) and power unit LSGA/LSGD (top)			
B	Fuse also accessible if electronics box installed			
C	Fuse		Part of power unit, item 10	
D	Choice of line voltage		Position of jumper on power unit, item 10 depending on desired line voltage	

9.4 Replacing the central module

-  Generally, when a central module has been replaced, all data which can be changed are set to the factory setting.

Proceed as described below if a central module is replaced:

1. If possible, note the customized settings of the device, such as:
 - Calibration data
 - Current assignment, main parameter and temperature
 - Relay function selections
 - Limit value/controller settings
 - Cleaning settings
 - Monitoring functions
 - Interface parameters
2. Disassemble the device as explained in the "Dismantling the panel-mounted instrument" or "Dismantling the field instrument" section.
3. Use the part number on the central module to check whether the new module has the same part number as the previous module.
4. Assemble the device with the new module.
5. Start up the device again and check the basic functions (e.g. measured value and temperature display, operation via keyboard).
6. Enter the serial number:
 - Read the serial number ("ser-no.") on the nameplate of the device.
 - Enter this number in the fields E115 (year, one-digit), E116 (month, one-digit), E117 (consecutive number, four-digit).
 - In the field E118, the complete number is displayed again so you can check it is correct.

 You can only enter the serial number for new modules with the serial number 0000. This can only be done **once!** For this reason, make sure the number entered is correct before you confirm with ENTER!
Entry of an incorrect code will prevent the additional functions from being enabled. An incorrect serial number can only be corrected at the factory!

Press ENTER to confirm the serial number or cancel the entry to enter the number again.

7. If available, enter the release codes for the Plus Package and/or Chemoclean in the "Service" menu.
8. Check the Plus Package release (e.g. by opening the function group CHECK / Code P) or the Chemoclean function.
9. Make the customer device settings again.

9.5 Return

The device must be returned if repairs or a factory calibration are required, or if the wrong device has been ordered or delivered. According to legal regulations, Endress+Hauser, as an ISO-certified company, is required to follow certain procedures when handling returned products that are in contact with medium.

To ensure swift, safe and professional device returns, please read the return procedures and conditions on the internet site:

www.services.endress.com/return-material

9.6 Disposal

The device contains electronic components and must therefore be disposed of in accordance with regulations on the disposal of electronic waste.

Please observe local regulations.

10 Accessories

10.1 Sensors

Oxymax W COS31

- Oxygen sensor for drinking water and wastewater measurements, SS 1.4571 , potentiostatic amperometric principle
- Ordering acc. to product structure, www.products.endress.com/cos31
- Technical Information TI00285/07/EN

Oxymax W COS41

- Oxygen sensor for drinking water and wastewater measurements, POM, amperometric principle
- Ordering acc. to product structure, www.products.endress.com/cos41
- Technical Information TI00284/07/EN

Oxymax W COS61

- Optical oxygen sensor for drinking water and wastewater measurements, SS 1.4571, fluorescence quenching principle
- Ordering acc. to product structure, www.products.endress.com/cos61
- Technical Information TI00387/07/EN

Oxymax W COS71

- Oxygen sensor for trace measurement, SS 1.4571, potentiostatic amperometric principle
- Ordering acc. to product structure, www.products.endress.com/cos71
- Technical Information TI00286/07/EN

10.2 Connection accessories

OMK measuring cable

- non-terminated measuring cable for oxygen sensors COS31, COS61 and COS71, for extension between junction box VS and transmitter
- Sold by the meter, order no. 50004124

CMK measuring cable

- non-terminated measuring cable for oxygen sensor COS41, for extension between junction box VBM and transmitter
- Sold by the meter, order no. 50005374

VS junction box

- With plug-in socket and 7-pole plug
- For cable extension from sensor (COS71, COS61, COS31, COS3 with SXP connector) to transmitter, IP 65;
- Order no. 50001054

Junction box VBM

- for cable extension for sensors COS41, COS4 (fixed cable versions)
- with 10 terminals, IP 65 / NEMA 4X
- Order numbers:
 - Cable entry Pg 13.5: 50003987
 - Cable entry NPT ½": 51500177

10.3 Mounting accessories

CYY101 weather protection cover for field devices, absolutely essential if operating the unit outdoors

- Material: stainless steel 1.4031 (AISI 304)
- Order No. CYY101-A

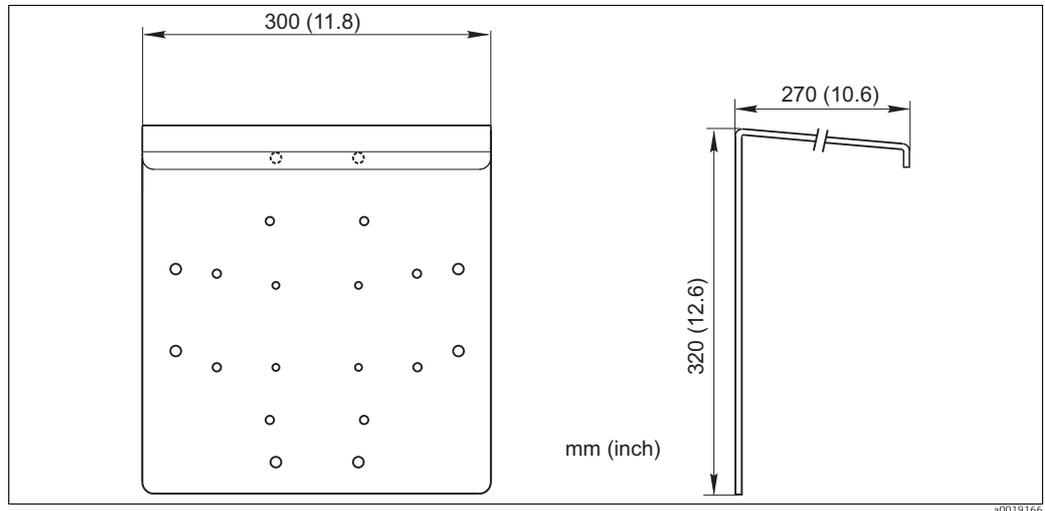


Fig. 38: Weather protection cover for field devices

CYY102 universal post

- Square pipe for mounting transmitters
- Material: stainless steel 1.4301 (AISI 304)
- Order No. CYY102-A

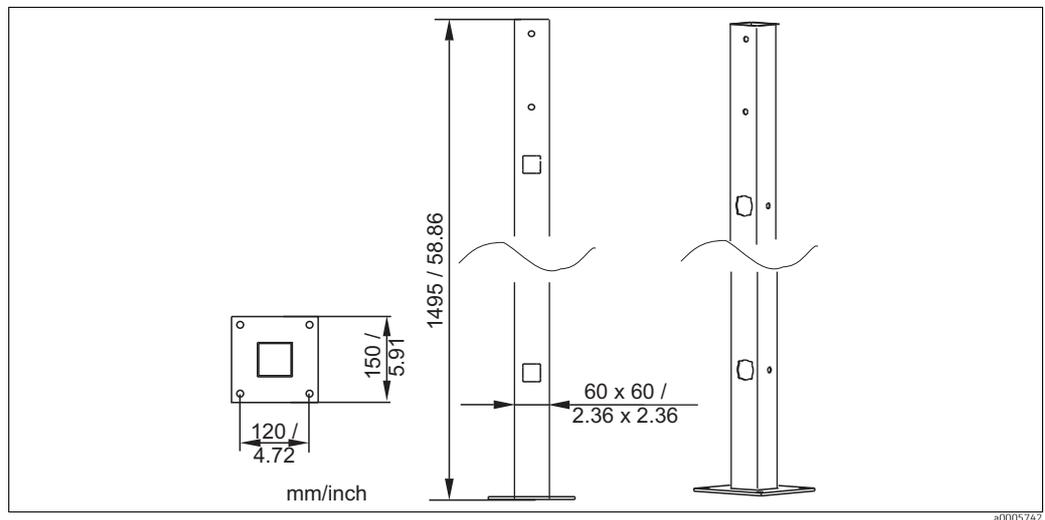


Fig. 39: Universal post

Post mounting kit

- For mounting of field housing on horizontal or vertical pipes (\varnothing max. 60 mm (2.36"))
- Material: stainless steel 1.4301
- order no. 50086842

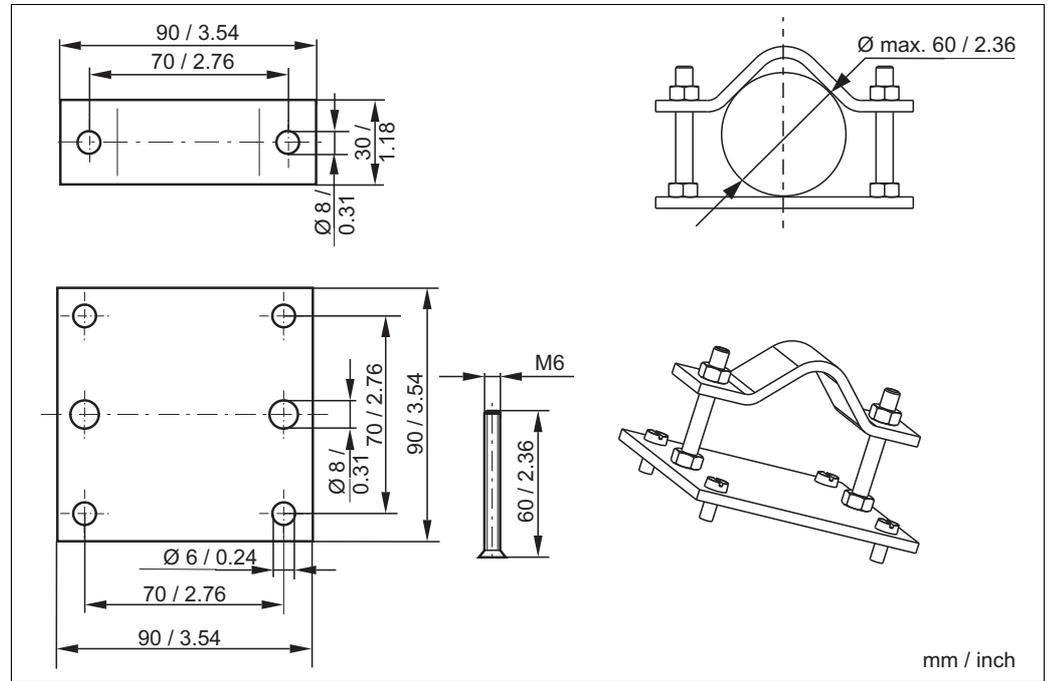


Fig. 40: Post mounting kit

10.4 Software and hardware add-ons

The add-ons can only be ordered by quoting the serial number of the device in question.

- Plus Package
Order no. 51501679
- Chemoclean
Order no. 51500963
- Two-relay card
Order no. 51500320
- Four-relay card
Order no. 51500321
- Two-relay card with current input
Order no. 51504304
- Four-relay card with current input
Order no. 51504305

11 Technical data

11.1 Input

Measured variables	Oxygen Temperature
Measuring range	<p>COS31: Oxygen concentration 0 to 20 / 0 to 60 mg/l Oxygen saturation index 0 to 200 / 0 to 600 % SAT Oxygen partial pressure 0 to 400 / 0 to 1200 hPa</p> <p>COS41, COS61: Oxygen concentration 0 to 20 mg/l Oxygen saturation index 0 to 200 % SAT Oxygen partial pressure 0 to 400 hPa</p> <p>COS71: Oxygen concentration 0 to 20 mg/l Oxygen saturation index 0 to 200 % SAT Oxygen partial pressure 0 to 400 hPa</p> <p>Temperature: -10 to 60 °C (14 to 140 °F)</p>
Cable specification	<p>Cable length: COS31, COS61, COS71 max. 100 m (328 ft) COS41 max. 50 m (164 ft)</p>
O₂ Signal input	<p>Version DX/DS: 0 to 3000 nA Version WX/WS: digital communication or 0 to -7500 mV</p>
Binary inputs	<p>Voltage: 10 to 50 V Power consumption: max. 10 mA</p>
Current input	<p>4 to 20 mA, galvanically separated Load: 260 Ω at 20 mA (voltage drop 5.2 V)</p>

11.2 Output

Output signal 0/4 to 20 mA, galvanically separated, active

HART	
Signal coding	Frequency Shift Keying (FSK) + 0.5 mA via current output signal
Data transfer rate	1200 Baud
Galvanic isolation	yes

PROFIBUS PA	
Signal coding	Manchester Bus Powered (MBP)
Data transfer rate	31.25 kBit/s, voltage mode
Galvanic isolation	yes (IO-Module)

PROFIBUS DP	
Signal coding	RS485
Data transfer rate	9.6 kBd, 19.2 kBd, 93.75 kBd, 187.5 kBd, 500 kBd, 1.5 MBd
Galvanic isolation	yes (IO-Module)

Signal on alarm 2.4 or 22 mA in case of an error

Load maximum 500 Ω

Transmission range

COS31:

- Oxygen concentration Δ 0.2 to Δ 20 / Δ 0.6 to Δ 60 mg/l
- Oxygen saturation index Δ 2 to Δ 200 / Δ 6 to Δ 600 % SAT
- Oxygen partial pressure Δ 4 to Δ 400 / Δ 12 to Δ 1200 hPa

COS41, COS61:

- Oxygen concentration Δ 0.2 to Δ 20 mg/l
- Oxygen saturation index Δ 2 to Δ 200 % SAT
- Oxygen partial pressure Δ 4 to Δ 400 hPa

COS71:

- Oxygen concentration Δ 0.02 to Δ 20 mg/l
- Oxygen saturation index Δ 0.2 to Δ 200 % SAT
- Oxygen partial pressure Δ 0.4 to Δ 400 hPa

Temperature: Δ 7 to Δ 70 °C

Resolution max. 700 digits/mA

Isolation voltage max. 350 V_{RMS}/500 V DC

Overvoltage protection according to EN 61000-4-5

Auxiliary voltage output

Output voltage:	15 V \pm 0.6
Output current:	max. 10 mA

Contact outputs	Switching current with ohmic load ($\cos \varphi = 1$):	max. 2 A
	Switching current with inductive load ($\cos \varphi = 0.4$):	max. 2 A
	Switching voltage:	max. 250 V AC, 30 V DC
	Switching power with ohmic load ($\cos \varphi = 1$):	max. 500 VA AC, 60 W DC
	Switching power with inductive load ($\cos \varphi = 0.4$):	max. 500 VA AC, 60 W DC
	Limit contactor	Pickup/dropout delay:
Controller	Function (adjustable):	pulse length/pulse frequency controller
	Controller response:	PID
	Control gain K_p :	0.01 to 20.00
	Integral action time T_n :	0.0 to 999.9 min
	Derivative action time T_v :	0.0 to 999.9 min
	Period for pulse length controller:	0.5 to 999.9 s
	Frequency for pulse frequency controller:	60 to 180 min^{-1}
Basic load:	0 to 40% of max. set value	
Alarm	Function (switchable):	latching/momentary contact
	Alarm threshold adjustment range:	O_2 / temperature: entire measuring range, depending on sensor type
	Alarm delay:	0 to 2000 s (min)
	Monitoring time lower limit violation:	0 to 2000 min
	Monitoring time upper limit violation:	0 to 2000 min

Protocol specific data

HART	
Manufacturer ID	11 _h
Device type code	0094 _h
Transmitter specific revision	0001 _h
HART specification	5.0
DD files	www.products.endress.com/hart
Load HART	250 Ω
Device variables	None (dynamic variables PV, SV, only)
Features supported	-

PROFIBUS PA	
Manufacturer ID	11 _h
Ident number	1518 _h
Device revision	11 _h
Profile version	2.0
GSD files	www.products.endress.com/profibus
GSD file version	
Output values	Main value, temperature value
Input values	Display value of PLC
Features supported	Device locking: The device can be locked by hardware or software.

PROFIBUS DP	
Manufacturer ID	11 _h
Ident number	151E _h
Profile version	2.0
GSD files	www.products.endress.com/profibus
GSD file version	
Output values	Main value, temperature value
Input values	Display value of PLC
Features supported	Device locking: The device can be locked by hardware or software.

11.3 Power supply

Supply voltage Depending on ordered version:
 100/115/230 V AC +10/-15 %, 48 to 62 Hz
 24 V AC/DC +20/-15 %

Fieldbus connection

HART	
Supply voltage	n/a, active current outputs
Integrated reverse voltage protection	n/a, active current outputs

PROFIBUS PA	
Supply voltage	9 V to 32 V, max. 35 V
Polarity sensitive	no
FISCO/FNICO compliant acc. to IEC 60079-27	no

PROFIBUS DP	
Supply voltage	9 V to 32 V, max. 35 V
Polarity sensitive	n/a
FISCO/FNICO compliant acc. to IEC 60079-27	no

Power consumption max. 7.5 VA

Mains protection Fine-wire fuse, medium-slow blow 250 V/3.15 A

11.4 Performance characteristics

Resolution	Oxygen: COS31, COS41, COS61: COS71: Temperature:	0.01 mg/l / 0.1 % SAT / 1 hPa 0.001 mg/l / 0.1 % SAT / 1 hPa 0.1 °C
Maximum measured error¹⁾	Display Oxygen: Temperature: Signal output Oxygen: Temperature:	max. 0.5 % of measuring range max. 1.0 % of measuring range max. 0.75 % of measuring range max. 1.25 % of measuring range
Repeatability^a	max. 0.2 % of measuring range	
Temperature compensation range	0 to 50 °C (32 to 104 °F)	
Pressure compensation range	500 to 1100 hPa	
Altitude adjustment range	0 to 4000 m (0 to 13124 ft)	
Salinity adjustment range	0 to 4 ‰	
Slope adjustment range	COS31: COS41: COS61: COS71:	75 to 140 % (nominal 290 nA, in air, 20 °C (68 °F), 1013 hPa) 50 to 150 % (nominal 290 nA, in air, 20 °C (68 °F), 1013 hPa) 75 to 140 % (nominal 1340 nA, in air, 20 °C (68 °F), 1013 hPa) 50 to 150 % (nominal 8000 nA, in air, 20 °C (68 °F), 1013 hPa)

1) acc. to IEC 746-1, for nominal operating conditions

11.5 Environment

Ambient temperature	-10 to +55 °C (+14 to +131 °F)	
Storage temperature	-25 to +65 °C (-13 to +149 °F)	
Electromagnetic compatibility	Interference emission and interference immunity as per EN 61326-1:2006, EN 61326-2-3:2006	
Ingress protection	Panel mounted instrument: Field instrument:	IP 54 (front), IP 30 (housing) IP 65 / tightness acc. to NEMA 4X
Electrical safety	according EN/IEC 61010-1:2001, Installation Category II, for use up to 2000 m above sea level	
CSA	Apparatus with CSA General Purpose Approval are certified for indoor use.	
Relative humidity	10 to 95%, non-condensing	
Pollution degree	The product is suitable for pollution degree 2.	

11.6 Mechanical construction

Dimensions	Panel mounted instrument: Field instrument:	96 x 96 x 145 mm (3.78 x 3.78 x 5.71 inches) Installation depth: approx. 165 mm (6.50") 247 x 170 x 115 mm (9.72 x 6.69 x 4.53 inches)
Weight	Panel mounted instrument: Field instrument:	max. 0.7 kg (1.5 lb) max. 2.3 kg (5.1 lb)
Material	Housing of panel mounted instrument: Field housing: Front membrane:	Polycarbonate ABS PC Fr Polyester, UV-resistant
Terminals	Cross section	max. 2.5 mm ²

12 Appendix

Operating matrix COM223/253 - DX/DS with COS41 - WX/WS with COS61

CALIBRATION C	Ref = entry of reference value C1 (3)	Entry of calibration value current value C131	Slope is displayed 100.0 % 75.0 ... 140.0 % C132	Calibration status is displayed o.k. Exxx C133	Store calibration results yes: no: new C134
	H ₂ O = water C1 (2)	Start calibration Countdown 600 s --> 0 s C121	Calibration status is displayed o.k. Exxx C122	Store calibration results yes: no: new C123	
	on air C1 (1)	Start calibration Countdown 600 s --> 0 s C111	Calibration status is displayed o.k. Exxx C112	Store calibration results yes: no: new C113	
Edit: Code 22 Read: any code MEAS. VAL. DISPLAY with TEMPERATURE DISPLAY in °C Edit: Code 22 Read: any code	+ -	Temperature display in °F 1st error is displayed (if present)	Temperature display suppressed Other errors are displayed (up to max. 10 errors)	Measured value in mg/l	Measured value in % Sat
SETUP 1 A	Selection of operating mode mg/l % SAT hPa A1	Selection of display unit mg/l ppm ppb A2	* ----- A3	Entry of altitude 0 m 0 ... 4000 m A4	Entry of measured value damping 1 (no damping) 1 ... 60 A5
SETUP 2 B	Entry of salt concentration 0.0 % 0.0 ... 4.0 % B1	Entry of process temperature current meas. value -10.0 ... 60.0 °C B2	Display of temp. difference (Offset) current offset -5.0 ... +5.0 °C B3	* these fields are not available with DX versions	
CURRENT INPUT Z	Controller switch-off by current input Off; Input Z1	Delay for controller switch-off by current input 0 s 0 ... 2000 s Z2	Delay for controller switch-on by current input 0 s 0 ... 2000 s Z3	Switch-off limit value for current input 50% 0 ... 100% Z4	Switch-off direction for current input Low; High Z5
CURRENT OUTPUT O	Selection of current output Out 1, Out 2 O1	Select meas. unit for 2nd current output °C; mg/l; % Sat, hPa; Contr O2	Tab = Table O3 (3)	Selection of table option read edit O331	Enter number of value pairs in table 1 1 ... 10 O332
			sim = Simulation O3 (2)	Entry of simulation value current value 0 ... 22.00 mA O321	Selection of current range 4-20 mA; 0-20 mA O311
ALARM F	Selection of contact type Latch=latching Momen=momentary F1	Selection of alarm delay unit min; s F2	Alarm delay 0 min (s) 0 ... 2000 min (s) (depends on F2) F3	Setting of error current 22 mA; 2.4 mA F4	Selection of error number 1 1 ... 255 F5
CHECK P	Selection of alarm threshold monitoring Off; Low; High; Lo+Hi=low and high P1	Alarm delay 0 min (s) 0 ... 2000 min (s) (depends on F2) P2	Setting of lower alarm threshold 0.00 mg/l; 0...19 mg/l 0.0%SAT; 0...190%SAT 0 hPa; 0...380 hPa P3	Setting of upper alarm threshold 20.00 mg/l; 1...20 mg/l 200.0%SAT; 10...200%SAT 400 hPa; 20...400hPa P4	Selection of process monitoring off; AC; CC monitoring limit (AC): AC+CC ±0.1 mg/l ±1 % SAT ±2 hPa (in 1 h) P5

C07-COM2x3xx-13-06-00-en-001.eps

Measured value in hPa	Measured value Sensor signal in nA / mV	Measured value Current input in %	Measured value Current input in mA
--------------------------	--	--------------------------------------	---------------------------------------

only display switch!!

Selection of measuring range	
20 mg/l	60 mg/l
200%Sat	600% Sat
400 hPa	1200 hPa
A6	

Feedforward control to PID controller Off ; lin = linear Basic = basic load	Feedforward control gain = 1 at 50% 0 ... 100%		
Z6	Z7		
Selection of value pair in table 1 1 ... no. of value pairs assign	Entry of x-value (measured value) 0.00 mg/l ; 0...20 mg/l 0.0%SAT ; 0...200%SAT 0 hPa ; 0...400 hPa	Entry of y-value (current) 0.00mA ; 0...20.00mA	Table status o.k. yes ; no
O333	O334	O335	O336

Enter 20mA value 10.00 mg/l ; 0...20 mg/l 100.0%SAT ; 0...200%SAT 200 hPa ; 0...400hPa 40.0 °C ; -10...60 °C
O313

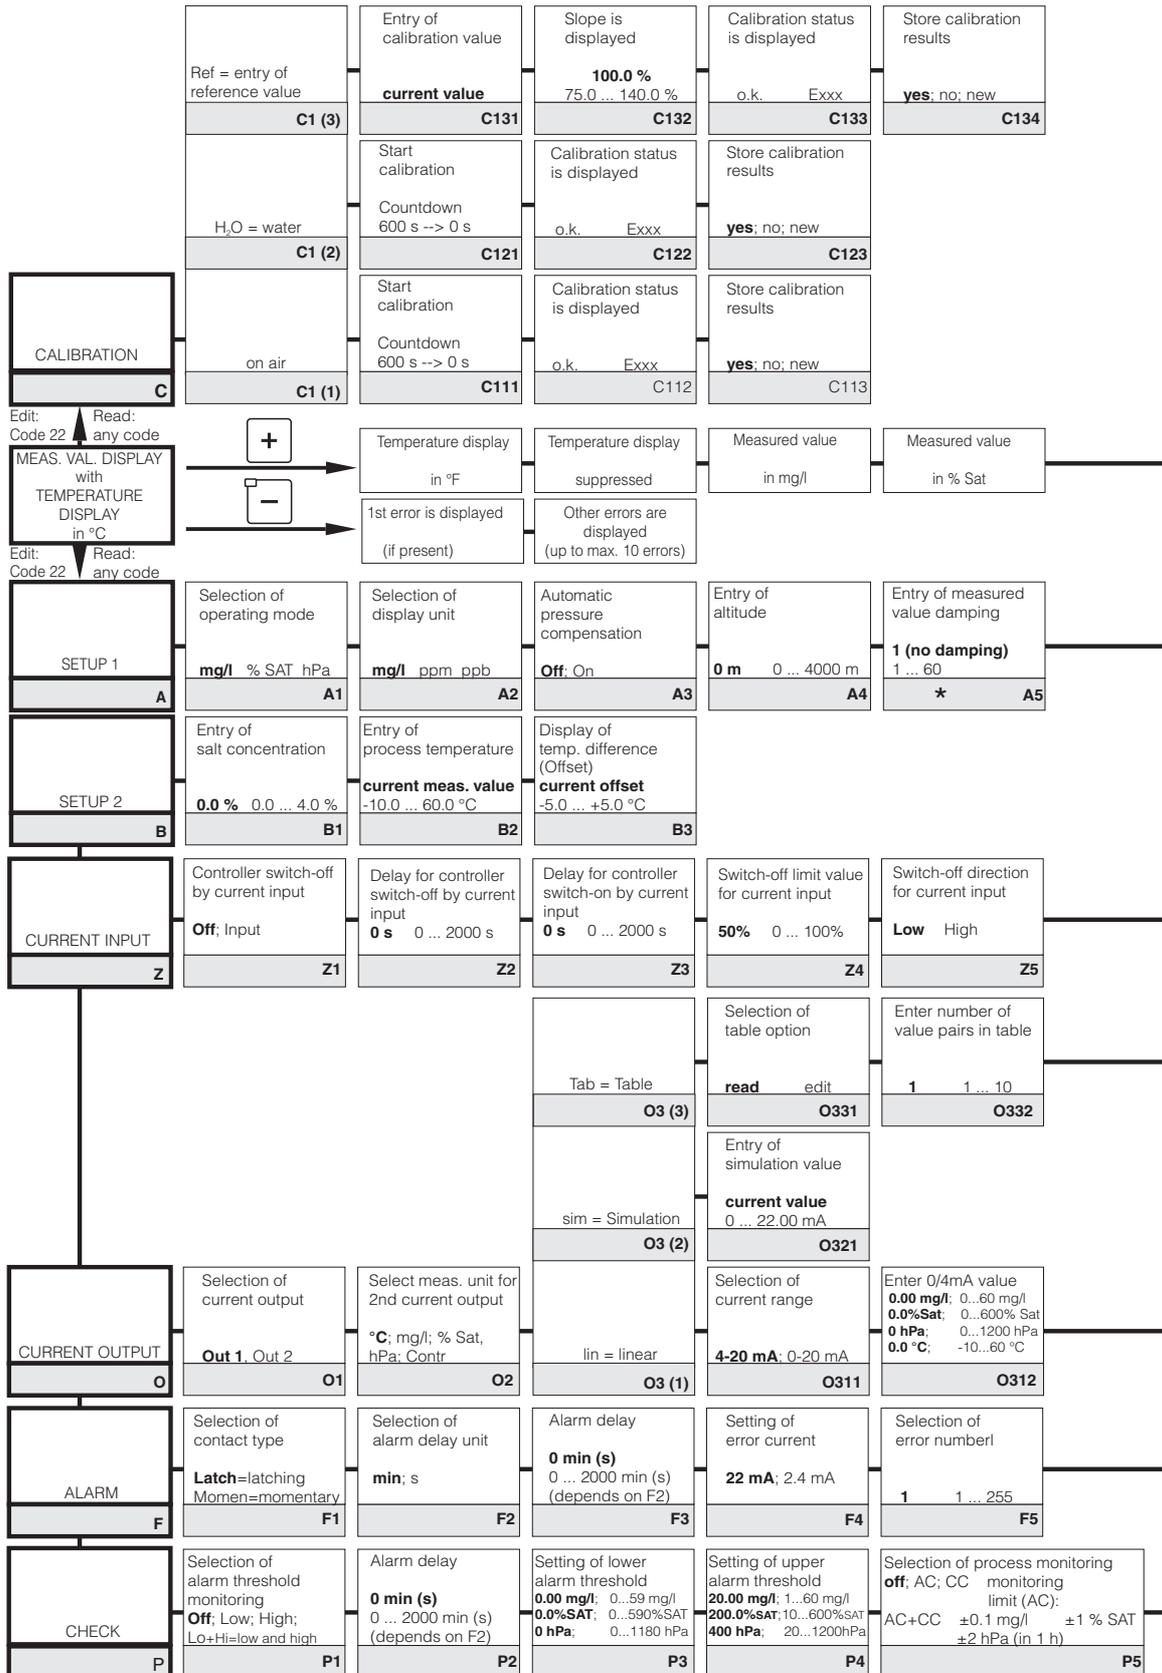
Activate alarm contact yes ; no	Activate error current for previously set error no ; yes	Automatic start of cleaning function no ; yes	Selection "next error" or return to menu Next=next error <--- R
F6	F7	F8	F9
Setting of maximum permissible limit violation period (below limit) 480 min ; 0...2000 min	Setting of maximum permissible limit violation period (upper limit) 240 min ; 0...2000 min	Setting of limit value 5.00 mg/l ; 0...20 mg/l 50.0 %SAT ; 0...200%SAT 200 hPa ; 0...400 hPa	
P6	P7	P8	

Field for customer settings

RELAY R	Clean = Chemoclean (with Rel3 a. Rel4 only)	Function R2 (5) switch on or off	Selection of start pulse int = internal i+ext = internal + external ext = external i+stp = internal suppressed by external		
		Off On	R251	R252	
	Timer	Function R2 (4) switch on or off	Setting of rinse time	Setting of pause time	
		Off On	30 s 0 ... 999 s	360 min 1 ... 7200 min	R241
	PID controller	Function R2 (3) switch on or off	Entry of set point	Entry of control gain K_p	
	Aus ; Ein; Basic: PID+B	R231	5.00 mg/l ; 0...20 mg/l 50.0 %SAT ; 0...200%SAT 200 hPa ; 0...400 hPa	1.00 0.01 ... 20.00	
	LC °C = limit contacter T	Function R2 (2) switch on or off	Entry of switch-on temperature	Entry of switch-off temperature	
	Off On	R221	60 °C -10 ... 60 °C	60 °C -10 ... 60 °C	
	Select contact to be configured	Function R2 (1) switch on or off	Select switch-on contact point	Select switch-off contact point	
	Rel1 ; Rel2; Rel3; Rel4	Off On	20.00 mg/l ; 0...20 mg/l 200.0%SAT ; 0...200%SAT 400 hPa ; 0...400 hPa	20.00 mg/l ; 0...20 mg/l 200.0%SAT ; 0...200%SAT 400 hPa ; 0...400 hPa	
	LC PV = limit contacter O ₂	R2(1)	R212	R213	
SERVICE S	Selection of language	Hold configuration none = no hold Cal = during calibration S+C = during setup + calibration Setup = during setup	Manual hold	Entry of hold dwell period	
	Eng ; Ger; Ita; Fra; Esp; Nel	S1	Off On	10 s 0 ... 999 s	
		S2	S2	S3	
	*	*	*	*	
	E1 (5)	E151	E152	E153	
	Rel = relay	Software version	Hardware version	Serial number is displayed	
	E1 (4)	E141	E142	E143	
	SW version	HW version	Module ID is displayed	E144	
E+H SERVICE E	MainB = main board	Software version	Hardware version	Serial number is displayed	
	E1 (3)	E131	E132	E133	
	SW version	HW version	Module ID is displayed	E134	
	Trans = transmitter	Software version	Hardware version	Serial number is displayed	
	E1 (2)	E121	E122	E123	
	SW version	HW version	Module ID is displayed	E124	
	Contr = controller	Software version	Hardware version	Serial number is displayed	
	E1 (1)	E111	E112	E113	
	SW version	HW version	Module ID is displayed	E114	
INTERFACE F	Entry of address	Tag description			
	Hart: 0 ... 15 or PROFIBUS: 1...126	@@@@@			
	F1	F2			

C07-COM2x3xx-13-06-00-en-003.eps

Operating matrix COM223/253 - WX/WS with COS31



C07-COM2x3xx-13-06-00-en-005.eps

Measured value in hPa	Measured value Sensor signal in nA / mV	Measured value Current input in %	Measured value Current input in mA
--------------------------	--	--------------------------------------	---------------------------------------

only display switch!!

Selection of measuring range	
20 mg/l	60 mg/l
200%Sat	600% Sat
400 hPa	1200 hPa
A6	

Feedforward control to PID controller Off ; lin = linear Basic = basic load Z6	Feedforward control gain = 1 at 50% 0 ... 100% Z7	Selection of value pair in table 1 1 ... no. of value pairs assign O333	Entry of x-value (measured value) 0.00 mg/l ; 0...60 mg/l 0.0%SAT ; 0...600%SAT 0 hPa ; 0...1200 hPa O334	Entry of y-value (current) 0.00mA ; 0...20.00mA O335	Table status o.k. yes ; no O336
--	--	---	--	---	--

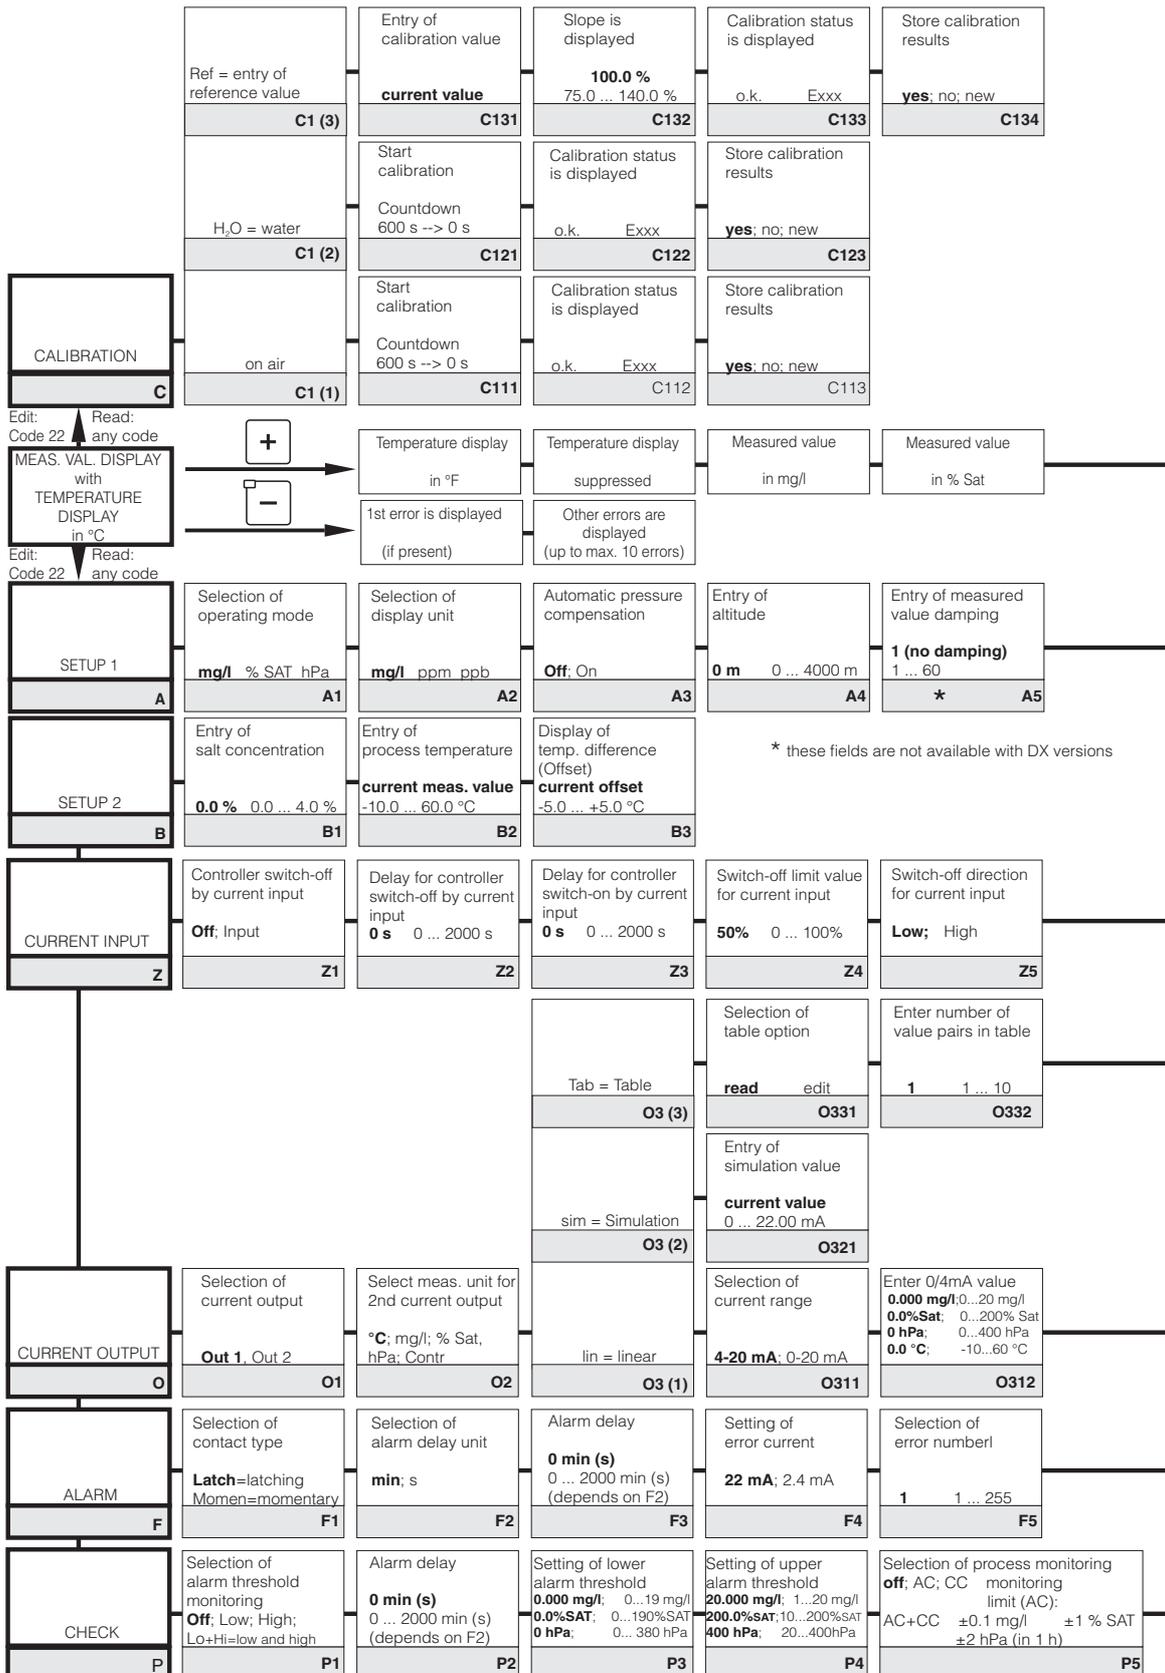
Enter 20mA value 10.00 mg/l ; 0...60 mg/l 100.0%SAT ; 0...600%SAT 200 hPa ; 0...1200hPa 40.0 °C ; -10...60 °C O313

Activate alarm contact yes ; no F6	Activate error current for previously set error no ; yes F7	Automatic start of cleaning function no ; yes F8	Selection "next error" or return to menu Next=next error <--- R F9
Setting of maximum permissible limit violation period (below limit) 480 min ; 0...2000 min P6	Setting of maximum permissible limit violation period (upper limit) 240 min ; 0...2000 min P7	Setting of limit value 5.00 mg/l ; 0...60 mg/l 50.0 %SAT ; 0...600%SAT 200 hPa ; 0...1200 hPa P8	Field for customer settings

RELAY R	Clean = Chemoclean (with Rel3 a. Rel4 only)	Function R2 (5) switch on or off	Selection of start pulse int = internal i+ext = internal + external ext = external i+stp = internal suppressed by external		
	R2 (5)	R251	R252		
	Timer	Function R2 (4) switch on or off	Setting of rinse time 30 s 0 ... 999 s		
	R2 (4)	R241	R242		
	PID controller	Function R2 (3) switch on or off	Setting of pause time 360 min 1 ... 7200 min		
R2 (3)	R231	R243	Entry of set point 5.00 mg/l: 0...60 mg/l 50.0 %SAT: 0...600%SAT 200 hPa: 0...1200 hPa		
LC °C = limit contacter T	Function R2 (2) switch on or off	Entry of control gain K_p 1.00 0.01 ... 20.00	R233		
R2(2)	R221	Entry of switch-on temperature 60 °C -10 ... 60 °C	R222		
Select contact to be configured Rel1; Rel2; Rel3; Rel4	Function R2 (1) switch on or off	Entry of switch-off temperature 60 °C -10 ... 60 °C	R223		
R1	R2(1)	R211	R212		
LC PV = limit contacter O ₂	Function R2 (1) switch on or off	Select switch-on contact point 20.00 mg/l: 0...60 mg/l 200.0%SAT: 0...600%SAT 400 hPa: 0...1200 hPa	Select switch-off contact point 20.00 mg/l: 0...60 mg/l 200.0%SAT: 0...600%SAT 400 hPa: 0...1200 hPa		
R1	R211	R212	R213		
SERVICE S	Selection of language Eng: Ger; Ita; Fra: Esp; Nel	Hold configuration none = no hold Cal = during calibration S+C = during setup + calibration Setup = during setup	Manual hold Off On		
	S1	S2	S2		
E+H SERVICE E	Sens = sensor	Software version	Hardware version	Serial number is displayed	Module ID is displayed
	E1 (5)	E151	E152	E153	E154
	Rel = relay	SW version	HW version	Serial number is displayed	Module ID is displayed
	E1 (4)	E141	E142	E143	E144
	MainB = main board	Software version	Hardware version	Serial number is displayed	Module ID is displayed
E1 (3)	E131	E132	E133	E134	
Trans = transmitter	SW version	HW version	Serial number is displayed	Module ID is displayed	
E1 (2)	E121	E122	E123	E124	
Contr = controller	Software version	Hardware version	Serial number is displayed	Module ID is displayed	
E1 (1)	E111	E112	E113	E114	
INTERFACE F	Entry of address Hart: 0 ... 15 or PROFIBUS: 1...126	Tag description @@@@@			
	F1	F2			

C07-COM2x3cc-13-06-00-en-007.eps

Operating matrix COM223/253 - WX/WS with COS71



C07-COM2x3xx-13-06-00-en-009.eps

Measured value in hPa	Measured value Sensor signal in nA / mV	Measured value Current input in %	Measured value Current input in mA
--------------------------	--	--------------------------------------	---------------------------------------

only display switch!!

Selection of measuring range	
20 mg/l	60 mg/l
200%Sat	600% Sat
400 hPa	1200 hPa
A6	

Feedforward control to PID controller Off ; lin = linear Basic = basic load Z6	Feedforward control gain = 1 at 50% 0 ... 100% Z7	Selection of value pair in table 1 1 ... no. of value pairs assign O333	Entry of x-value (measured value) 0.00 mg/l ; 0...20 mg/l 0.0%SAT ; 0...200%SAT 0 hPa ; 0...400 hPa O334	Entry of y-value (current) 0.00mA ; 0...20.00mA O335	Table status o.k. yes ; no O336
--	--	---	---	---	--

Enter 20mA value 10.000 mg/l ; 0...20 mg/l 100.0%SAT ; 0...200%SAT 200 hPa ; 0...400hPa 40.0 °C ; -10...60 °C O313

Activate alarm contact yes ; no F6	Activate error current for previously set error no ; yes F7	Automatic start of cleaning function no ; yes F8	Selection "next error" or return to menu Next=next error <--- R F9
Setting of maximum permissible limit violation period (below limit) 480 min ; 0...2000 min P6	Setting of maximum permissible limit violation period (upper limit) 240 min ; 0...2000 min P7	Setting of limit value 1.000 mg/l ; 0...20 mg/l 50.0 %SAT ; 0...200%SAT 20 hPa ; 0...400 hPa P8	Field for customer settings

RELAY R	Clean = Chemoclean (with Rel3 a. Rel4 only)	Function R2 (5) switch on or off	Selection of start pulse int = internal i+ext = internal + external ext = external i+stp = internal suppressed by external		
	R2 (5)	R251	R252		
	Timer	Function R2 (4) switch on or off	Setting of rinse time		
	R2 (4)	R241	R242		
	PID controller	Function R2 (3) switch on or off	Setting of pause time		
R2 (3)	R231	R243	R233		
LC °C = limit contacter T	Function R2 (2) switch on or off	Entry of set point	Entry of control gain K _p		
R2(2)	R221	R232	R233		
LC PV = limit contacter O ₂	Function R2 (1) switch on or off	Entry of switch-on temperature	Entry of switch-off temperature		
R2(1)	R211	R222	R223		
Select contact to be configured	LC PV = limit contacter O ₂	Select switch-on contact point	Select switch-off contact point		
Rel1; Rel2; Rel3; Rel4	R1	R212	R213		
SERVICE S	Selection of language	Hold configuration none = no hold Cal = during calibration S+C = during setup + calibration Setup = during setup	Manual hold		
	Eng; Ger; Ita; Fra; Esp; Nel	S1	S2		
E+H SERVICE E	Sens = sensor	Software version	Hardware version	Serial number is displayed	Module ID is displayed
	E1 (5)	E151	E152	E153	E154
	Rel = relay	SW version	HW version	Serial number is displayed	Module ID is displayed
	E1 (4)	E141	E142	E143	E144
	MainB = main board	Software version	Hardware version	Serial number is displayed	Module ID is displayed
E1 (3)	E131	E132	E133	E134	
Trans = transmitter	SW version	HW version	Serial number is displayed	Module ID is displayed	
E1 (2)	E121	E122	E123	E124	
Contr = controller	Software version	Hardware version	Serial number is displayed	Module ID is displayed	
E1 (1)	E111	E112	E113	E114	
INTERFACE F	Entry of address	Tag description			
	Hart: 0 ... 15 or PROFIBUS: 1...126	@@@@@@@@			
F1	F2				

C07-COM2x3xx-13-06-00-en-011.eps

Entry of pre-rinse time 30 s 0 ... 999 s R253	Entry of cleaning time 10 s 0 ... 999 s R254	Entry of post-rinse time 30 s 0 ... 999 s R255	Number of repeat cycles 0 0 ... 5 R256	Setting of interval between 2 cleaning cycles (pause time) 360 min 1...7200 min R257	Setting of minimum pause time 120 min 1...3600 min R258	Number of cleaning cycles without cleaning agent 0 0 ... 9 R259			
Setting of minimum pause time 120 min 1...3600 min R244	Chemoclean: uses 2 contacts, only permissible for contacts 3 (+4)								
Entry of integral action time Tn (0,0=no I component) 0.0 s 0,0...999,9 min R234	Entry of derivative action time Tv (0,0=no D component) 0.0 s 0,0...999,9 min R235	Selection of control characteristics inv = invers dir = direct R236	Selection len = pulse length freq = pulse frequency curr = current output R237	Entry of pulse interval 10.0 s 0,5...999,9 s R238	Entry of pulse frequency 120 min⁻¹ 60 ... 180 min ⁻¹ R239	Entry of minimum on time t _{on} 0.3 s 0.1 ... 5.0 s R2310	Entry of basic load 0% 0 ... 40% R2311		
Setting of pick-up delay 0 s 0 ... 2000 s R224	Setting of drop-out delay 0 s 0 ... 2000 s R225	Setting of alarm threshold (absolute value) 60 °C -10 ... 60 °C R226	LC status MIN; MAX R227						
Setting of pick-up delay 0 s 0 ... 2000 s R214	Setting of drop-out delay 0 s 0 ... 2000 s R215	Setting of alarm threshold (abs. value) 20.000 mg/l: 0...60 mg/l 200.0%SAT: 0...600%SAT 400 hPa: 0...1200 hPa R216	LC status MIN; MAX R217						
Entry of SW upgrade release code (Plus package) 0000 0000 ... 9999 S2	Entry of SW upgrade release code Chemoclean 0000 0000 ... 9999 S6	Display of order number S7	Display of serial number S8	Reset instrument to default values no: sens; factory S9	Perform instrument test no: display S10	Display of absolute air pressure S11			
Serial number sensor head existing serial no. 00000000...99999999 E155	Serial number sensor existing serial no. 00000000...99999999 E156	Order number sensor existing order no. COS71-...COS71-ZZZZ E157	Display of minimum temperature E158	Display of maximum temperature E159					

Index

A

Access codes	30
Accessories	89
Alarm	94
Alarm contact	24
Alarm threshold monitoring	47
Altitude adjustment range	97
Ambient temperature	98
Appendix	
Operating matrix	100
Automatic mode	29
Auxiliary voltage output	93

B

Binary inputs	92
---------------------	----

C

Cable specification	92
Calibration	65–68
CE mark	8
Central module	87
Check	47
Checking	
Connections	24
Function	32
Installation	15
Chemoclean function	55
Cleaning	
Transmitter	77
Commissioning	32
Quick setup	34
Switching on	32
Communication	64
Connection diagram	17
Contact outputs	94
Controller	94
Controller monitoring	47
CSA	98
CSA general purpose	8
Current	92
Current input	38
Current outputs	41

D

Declaration of conformity	8
Designated use	5
Diagnosis code	69
Dimensions	98
Dismantling	
Field instrument	84
Panel-mounted instrument	81
Display	25
Disposal	88

E

E+H Service	63
Electrical safety	98
Electrical connection	16
Electrical icons	6
Electrical symbols	6
Electromagnetic compatibility	5
EMC	98
Environment	98

F

Factory settings	33
Field device connection	18, 22
Fieldbus	96
Freezing of outputs	31

H

Hold function	31, 62
---------------------	--------

I

Icons	
Electrical	6
Incoming acceptance	7
Ingress protection	98
Input	92
Installation	12
Installation instructions	10–15
Quick guide	9
Interfaces	64
Isolation voltage	93

K

Key assignment	27
----------------------	----

L

Limit	94
Limit contactor	51
Load	93

M

Mains	96
Maintenance	77
Assembly	79
Connecting lines and junction boxes	80
Entire measuring point	77
Oxygen sensors	79
Manual mode	29
Material	98
Maximum	97
Measured	92
Measuring range	92
Measuring cable	
Variant 1	19
Measuring system	9
Mechanical construction	98
Menu	
Current input	38
Current outputs	41
E+H Service	63
Interfaces	64
Monitoring functions	46
Relay	55
Service	62
Setup 1	36
Setup 2	37
Menu structure	31
Monitoring functions	46

N

Nameplate	8
-----------	---

O

Operating elements	26
Operating matrix	100
Operating modes	30
Operation	
Display	25
Operating concept	29
Operating elements	26
Operational safety	5
Output	93–95
Overvoltage protection	93

P

P controller	52
PD controller	52
Performance characteristics	97
PI controller	52
PID controller	52
Pollution degree	98
Post mounting	13
Power consumption	96
Power supply	96
Pressure compensation range	97
Product safety	6
Protocol specific data	95

Q

Quick setup	34
Quick start-up	25, 34

R

Relative humidity	98
Relay contact configuration	51
Repeatability	97
Replacing the central module	87
Requirements for the personnel	5
Resolution	93, 97
Return	88

S

Salinity	97
Scope of delivery	7
Sensor activity monitoring	47
Service	62
Setup 1 (oxygen)	36
Setup 2 (salinity and temperature)	37
Signal	92–93
Slope	97
Spare parts	81
Storage	98
Supply voltage	96
Switching on	32
System configuration	36–64

T

Technical data	92–98
Temperature compensation range	97
Terminals	98
Test	
Variant 1 (DX/DS)	78
Variant 2 (WX/WS)	79
Timer for cleaning function	54
Transmission	93
Troubleshooting	
Instrument specific errors	75
Process specific errors	72
System error messages	69

W

Wall mounting	12
Weight	98
Wiring	16
Workplace safety	5



71212633

www.addresses.endress.com
