# Technical Information **Proline Cubemass C 500**

Coriolis flowmeter



# Compact sensor for smallest quantities, with a transmitter remote version with up to $4\ \text{I/Os}$

#### Application

- Measuring principle operates independently of physical fluid properties such as viscosity or density
- Measuring accurately smallest quantities of liquids and gases

#### Device properties

- Nominal diameter: DN 1 to 6 ( $\frac{1}{24}$  to  $\frac{1}{4}$ ")
- Process pressure up to 400 bar (5800 psi)
- Medium temperature up to +205 °C (+401 °F)
- Remote version with up to 4 I/Os
- Backlit display with touch control and WLAN access
- Standard cable between sensor and transmitter

#### Your benefits

- Space-saving installation compact single-tube design
- Fewer process measuring points multivariable measurement (flow, density, temperature)
- Suitable for skids lightweight sensor
- Full access to process and diagnostic information numerous, freely combinable I/Os and Ethernet
- Reduced complexity and variety freely configurable I/O functionality
- Integrated verification Heartbeat Technology



# Table of contents

About this document		Special installation instructions	68
		Environment	71
Function and system design	5	Ambient temperature range	
Measuring principle		Storage temperature	71
Measuring system		Climate class	71
Equipment architecture		Relative humidity	71
Reliability		Operating height	72
		Degree of protection	72
Input	12	Vibration resistance and shock resistance	
Measured variable		Mechanical load	
Measuring range		Electromagnetic compatibility (EMC)	72
Operable flow range			
Input signal		Process	73
input signal	10	Medium temperature range	
		Medium density	
<b>-</b>	15	Pressure-temperature ratings	
Output and input variants		Sensor housing	
Output signal		Rupture disk	
Signal on alarm		Internal cleaning	
		Flow limit	75
Ex connection data	27	Pressure loss	75
Low flow cut off	31	Static pressure	75
Galvanic isolation	31	Thermal insulation	76
Protocol-specific data	34	Heating	76
		Vibrations	76
11 3	39		
Terminal assignment	39	Mechanical construction	77
Available device plugs Proline 500	41	Dimensions in SI units	
Available device plugs Proline 500 digital	43	Dimensions in US units	
Pin assignment, device plug		Weight	
Supply voltage	46	Materials	
Power consumption		Process connections	
Current consumption		Surface roughness	
Power supply failure	47	3	
Overcurrent protection element	47	Operability	07
Electrical connection	47		
Potential equalization	55	Operation concept	
Terminals	55 56	Onsite operation	
Cable entries		Remote operation	
			104
Overvoltage protection	01	Network integration	
			107
Performance characteristics	61		108
Reference operating conditions	61	Instance auta management	100
Maximum measurement error	61		110
Repeatability	62	* *	110
Response time	63		110
Influence of ambient temperature	63	5	110
Influence of medium temperature	I	3	110
Influence of medium pressure	64	11	110
Design fundamentals	64	· · · · · · · · · · · · · · · · · · ·	110
			110
Installation	65		111
Mounting location			111
Orientation	66		111
Inlet and outlet runs	66	Certification PROFINET	
Installing the transmitter housing	67		111
		Radio approval	111

2

Additional certification	111
External standards and guidelines	112
Ordering information	112
Application packages	112
Diagnostic functionality	113
Heartbeat Technology	113
Concentration measurement	113
Special density	113
OPC-UA Server	114
Accessories	114
Device-specific accessories	114
Communication-specific accessories	115
Service-specific accessories	
System components	116
Documentation	117
Standard documentation	117
Device-dependent additional documentation	118
Registered trademarks	119

# About this document

#### Symbols Electrical symbols

Symbol	Meaning
	Direct current
~	Alternating current
$\overline{}$	Direct current and alternating current
<u></u>	Ground connection A grounded terminal which, as far as the operator is concerned, is grounded via a grounding system.
	Protective earth (PE) Ground terminals that must be connected to ground prior to establishing any other connections.
	The ground terminals are located on the interior and exterior of the device:  Interior ground terminal: protective earth is connected to the mains supply.  Exterior ground terminal: device is connected to the plant grounding system.

#### Communication-specific symbols

Symbol	Meaning
<b></b>	Wireless Local Area Network (WLAN) Communication via a wireless, local area network
•	LED LED is off.
<u></u>	LED LED is on.
	LED LED flashing.

#### $Symbols \ for \ certain \ types \ of \ information$

Symbol	Meaning
<b>✓</b>	Permitted Procedures, processes or actions that are permitted.
	Preferred Procedures, processes or actions that are preferred.
X	Forbidden Procedures, processes or actions that are forbidden.
i	Tip Indicates additional information.
[i	Reference to documentation
A=	Reference to page
	Reference to graphic
	Visual inspection

#### Symbols in graphics

Symbol	Meaning
1, 2, 3,	Item numbers
1., 2., 3.,	Series of steps
A, B, C,	Views
A-A, B-B, C-C,	Sections
EX	Hazardous area
×	Safe area (non-hazardous area)
≋➡	Flow direction

## Function and system design

#### Measuring principle

The measuring principle is based on the controlled generation of Coriolis forces. These forces are always present in a system when both translational and rotational movements are superimposed.

 $F_c = 2 \cdot \Delta m (v \cdot \omega)$ 

 $F_c$  = Coriolis force

 $\Delta m = moving mass$ 


 $\omega$  = rotational velocity

 $v = radial \ velocity \ in \ rotating \ or \ oscillating \ system$ 

The amplitude of the Coriolis force depends on the moving mass  $\Delta m$ , its velocity v in the system and thus on the mass flow. Instead of a constant rotational velocity  $\omega$ , the sensor uses oscillation.

In the sensor, an oscillation is produced in the measuring tube loop. The Coriolis forces produced at the measuring tube loop cause a phase shift in the tube oscillations (see illustration):

- If there is zero flow (i.e. when the medium is at a standstill), the oscillation measured at points A and B has the same phase (no phase shift) (1).
- Mass flow causes deceleration of the oscillation at the inlet of the tubes (2) and acceleration at the outlet (3).

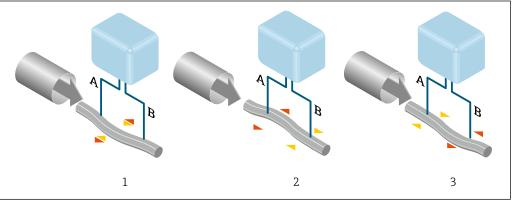

A002993

The phase shift (A-B) increases with increasing mass flow. Electrodynamic sensors register the tube oscillations at the inlet and outlet. System balance is ensured by the antiphase oscillation of the two measuring tubes. The measuring principle operates independently of temperature, pressure, viscosity, conductivity and flow profile.

#### **Density measurement**

The measuring tube is continuously excited at its resonance frequency. A change in the mass and thus the density of the oscillating system (comprising measuring tube and medium) results in a corresponding, automatic adjustment in the oscillation frequency. The resonance frequency is thus a function of the medium density. The microprocessor utilizes this relationship to obtain a density signal.

#### Volume measurement


Together with the measured mass flow, this is used to calculate the volume flow.


#### Temperature measurement

The temperature of the measuring tube is determined in order to calculate the compensation factor due to temperature effects. This signal corresponds to the process temperature and is also available as an output signal.

#### Gas Fraction Handler (GFH)

The Gas Fraction Handler is a Promass software function that improves measurement stability and repeatability. The function continuously checks for the presence of disturbances in single-phase flow, i.e. gas bubbles in liquids. In the presence of the second phase, flow and density become increasingly unstable. The Gas Fraction Handler function improves measurement stability with respect to the severity of the disturbances, without any effect under single-phase flow conditions.






#### Measuring system

The measuring system consists of a transmitter and a sensor. The transmitter and sensor are mounted in physically separate locations. They are interconnected by connecting cables.

#### Transmitter

Two versions of the transmitter are available.

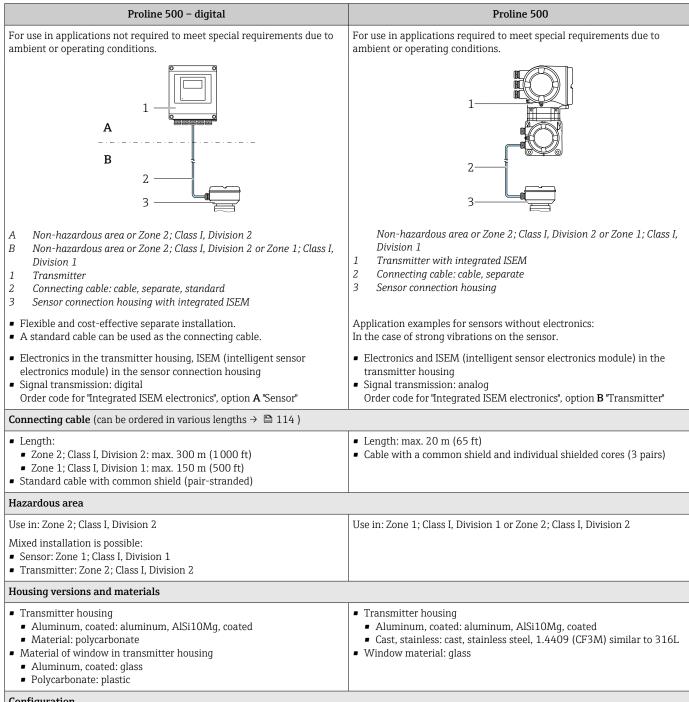

#### Configuration


- External operation via 4-line, illuminated graphic local display (LCD) with touch control and guided menus ("Make-it-run" wizards) for applicationspecific commissioning.
- Via service interface or WLAN interface:
  - Operating tools (e.g. FieldCare, DeviceCare)
  - Web server (access via web browser)

#### Sensor connection housing


Different versions of the connection housing are available.

Order code for "Sensor connection housing", option A, "Aluminum, coated": Aluminum, AlSi10Mg, coated  This device version is only available in conjunction with the Proline 500 – digital transmitter.
Order code for "Sensor connection housing", option B, "Stainless":  Hygienic version, stainless steel 1.4301 (304)  Optional: order code for "Sensor feature", option CC "Hygienic version, for maximum corrosion resistance": stainless steel 1.4404 (316L)
Order code for "Sensor connection housing", option C, "Ultra-compact hygienic, stainless":  Hygienic version, stainless steel 1.4301 (304)  Optional: order code for "Sensor feature", option CC "Hygienic version, for maximum corrosion resistance": stainless steel 1.4404 (316L)  This device version is only available in conjunction with the Proline 500 – digital transmitter.
Order code for "Sensor connection housing", option L, "Cast, stainless": 1.4409 (CF3M) similar to 316L

#### Sensor

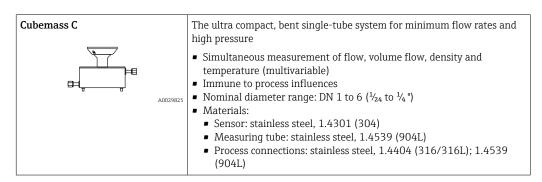

#### Equipment architecture

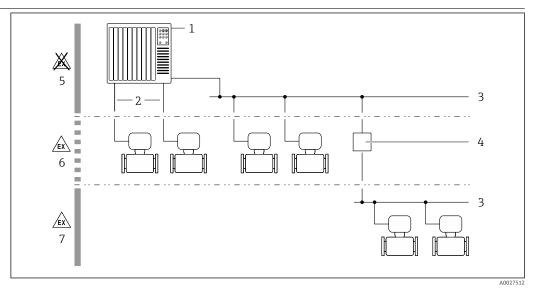

 $\blacksquare 1$  Possibilities for integrating measuring instruments into a system

- 1 Automation system (e.g. PLC)
- 2 Connection cable (0/4 to 20 mA HART etc.)
- 3 Fieldbus
- 4 Coupler
- 5 Non-hazardous area
- 6 Hazardous area: Zone 2; Class I, Division 2
- 7 Hazardous area: Zone 1; Class I, Division 1

#### Reliability

#### IT security

The manufacturer warranty is valid only if the product is installed and used as described in the Operating Instructions. The product is equipped with security mechanisms to protect it against any inadvertent changes to the settings.

IT security measures, which provide additional protection for the product and associated data transfer, must be implemented by the operators themselves in line with their security standards.

#### **Device-specific IT security**

The device offers a range of specific functions to support protective measures on the operator's side. These functions can be configured by the user and guarantee greater in-operation safety if used correctly. The following list provides an overview of the most important functions:

Function/interface	Factory setting	Recommendation
Write protection via hardware write protection switch $\rightarrow \stackrel{ riangle}{ riangle} 10$	Not enabled	On an individual basis following risk assessment
Access code (also applies to web server login or FieldCare connection) → 🖺 10	Not enabled (0000)	Assign a customized access code during commissioning
WLAN (order option in display module)	Enabled	On an individual basis following risk assessment
WLAN security mode	Enabled (WPA2- PSK)	Do not change
WLAN passphrase (Password) → 🖺 10	Serial number	Assign an individual WLAN passphrase during commissioning
WLAN mode	Access point	On an individual basis following risk assessment
Web server → 🗎 10	Enabled	On an individual basis following risk assessment
Service interface CDI-RJ45 → 🗎 11	Enabled	-

Protecting access via hardware write protection

Write access to the parameters of the device via the local display, web browser or operating tool (e.g. FieldCare, DeviceCare) can be disabled via a write protection switch (DIP switch on the main electronics module). When hardware write protection is enabled, only read access to the parameters is possible.

Hardware write protection is disabled when the device is delivered.

#### Protecting access via a password

Different passwords are available to protect write access to the device parameters or access to the device via the WLAN interface.

User-specific access code

Protect write access to the device parameters via the local display, web browser or operating tool (e.g. FieldCare, DeviceCare). Access authorization is clearly regulated through the use of a user-specific access code.

WLAN passphrase

The network key protects a connection between an operating unit (e.g. notebook or tablet) and the device via the WLAN interface which can be ordered as an option.

• Infrastructure mode

When the device is operated in infrastructure mode, the WLAN passphrase corresponds to the WLAN passphrase configured on the operator side.

User-specific access code

Local display, web browser and operating tool (e.g. FieldCare, DeviceCare)

- Write access to the device parameters via the local display, web browser or operating tool (e.g. FieldCare, DeviceCare) can be protected by the modifiable, user-specific access code.
- When delivered, the device does not have an access code; the default value is 0000 (open).

WLAN passphrase: Operation as WLAN access point

A connection between an operating unit (e.g. notebook or tablet) and the device via the WLAN interface, which can be ordered as an optional extra, is protected by the network key. The WLAN authentication of the network key complies with the IEEE 802.11 standard.

When the device is delivered, the network key is pre-defined depending on the device. It can be changed via the **WLAN settings** submenu in the **WLAN passphrase** parameter.

Infrastructure mode

A connection between the device and WLAN access point is protected by means of an SSID and passphrase on the system side. Please contact the relevant system administrator for access.

General notes on the use of passwords

- The access code and network key supplied with the device should be changed during commissioning for security reasons.
- Follow the general rules for generating a secure password when defining and managing the access code or network key.
- The user is responsible for the management and careful handling of the access code and network key.

Access via web server

The integrated web server can be used to operate and configure the device via a web browser. The connection is established via the service interface (CDI-RJ45) or WLAN interface . For device versions with the Ethernet/IP and PROFINET communication protocols, the connection can also be established via the terminal connection for signal transmission with Ethernet/IP, PROFINET (RJ45 plug), PROFINET over Ethernet-APL (two-wire) or Modbus TCP over Ethernet-APL.

The web server is enabled when the device is delivered. The web server can be disabled if necessary via the **Web server functionality** parameter (e.g., after commissioning).

The device and status information can be hidden on the login page. This prevents unauthorized access to the information.

For detailed information on device parameters, see: Description of Device Parameters.

#### Access via OPC UA



The device can communicate with OPC UA clients using the "OPC UA Server" application package.

The OPC UA server integrated in the device can be accessed via the WLAN access point using the WLAN interface - which can be ordered as an optional extra - or the service interface (CDI-RJ45) via Ethernet network. Access rights and authorization as per separate configuration.

The following Security Modes are supported as per the OPC UA Specification (IEC 62541):

- Without
- Basic128Rsa15 signed
- Basic128Rsa15 signed and encrypted

Access via service interface (port 2): CDI-RJ45

The device can be connected to a network via the service interface. Device-specific functions quarantee the secure operation of the device in a network.

The use of relevant industrial standards and guidelines that have been defined by national and international safety committees, such as IEC/ISA62443 or the IEEE, is recommended. This includes organizational security measures such as the assignment of access authorization as well as technical measures such as network segmentation.



#### PROFINET, Ethernet/IP:



For detailed information on connecting transmitters with an Ex de approval, see separate document "Safety instructions" (XA) for the device.

#### Advanced safety requirements

If the specified requirements for measures cannot be met, alternative measures may need to be put in place. This may involve, for example, mechanical protection of the product against tampering, the cabling, or organizational measures. The Proline measuring instruments can be used in the open field for example. Measures to combat physical tampering of the Proline measuring instruments must be arranged by the customer.

Additional analysis is required if Proline measuring instruments are integrated into a different system. Please note the following:

- The fieldbus network (OT) and company network (IT) must be strictly separated.
- Endress+Hauser recommends the segmentation of the fieldbus networks according to DIN IEC 62443-3-3.

#### Network

Pay particular attention to the network components used, the router and switches for example. The operator must guarantee the integrity of the components. Access to the network must be restricted by the operator, if necessary.

#### FDI Packages

Signed FDI Packages can be obtained via www.endress.com for the configuration of the field device.

#### User training

Depending on the application scenario, users who are not specialized in this area may come in contact with the instrument. We recommend that these users be trained in the safe use of the relevant terminals, components and/or interfaces and be made aware of security issues.

# **Input**

#### Measured variable

#### Direct measured variables

- Mass flow
- Density
- Temperature

#### Calculated measured variables

- Volume flow
- Corrected volume flow
- Reference density

#### Measuring range

#### Measuring range for liquids

DN		Measuring range full scale values $\dot{m}_{min(F)}$ to $\dot{m}_{max(F)}$	
[mm]	[in]	[kg/h]	[lb/min]
1	1/24	0 to 20	0 to 0.735
2	1/12	0 to 100	0 to 3.675
4	1/8	0 to 450	0 to 16.54
6	1/4	0 to 1000	0 to 36.75

#### Measuring range for gases

The full scale value depends on the density and the speed of sound of the gas used. The full scale value can be calculated with the following formulas:

$$\dot{m}_{\;max\,(G)}=minimum\;of \qquad \qquad (\dot{m}_{max(F)}\cdot \rho_G:x\;)$$
 and

$$(\rho_G\cdot (c_G/2)\cdot d_i{}^2\cdot (\pi/4)\cdot 3600\cdot n)$$

m <sub>max(G)</sub>	Maximum full scale value for gas [kg/h]	
m <sub>max(F)</sub>	Maximum full scale value for liquid [kg/h]	
$\dot{m}_{\max(G)} < \dot{m}_{\max(F)}$	$\dot{m}_{ max(G)}$ can never be greater than $\dot{m}_{ max(F)}$	
$\rho_{G}$	Gas density in [kg/m³] at operating conditions	
х	Limitation constant for max. gas flow [kg/m³]	
$c_G$	Speed of sound (gas) [m/s]	
d <sub>i</sub>	Measuring tube internal diameter [m]	
π	Pi	
n = 1	Number of measuring tubes	

DN		х
[mm]	[in]	[kg/m³]
1	1/24	20
2	1/12	20
4	1/8	20
6	1/4	20

i

If calculating the full scale value using the two formulas:

- 1. Calculate the full scale value with both formulas.
- 2. The smaller value is the value that must be used.

#### Recommended measuring range



Flow limit → 🖺 75

#### Operable flow range

Over 1000:1.

Flow rates above the preset full scale value do not override the electronics unit, with the result that the totalizer values are registered correctly.

#### Input signal


#### Output and input variants

→ 🖺 15

#### External measured values

To increase the measurement accuracy of certain measured variables or to calculate the corrected volume flow for gases, the automation system can continuously write different measured values to the measuring instrument:

- Operating pressure to increase measurement accuracy (Endress+Hauser recommends the use of a pressure measuring instrument for absolute pressure, e.g. Cerabar M or Cerabar S)
- Medium temperature to increase measurement accuracy (e.g. iTEMP)
- Reference density for calculating the corrected volume flow for gases



It is recommended to read in external measured values to calculate the corrected volume flow.

#### HART protocol

The measured values are written from the automation system to the measuring device via the HART protocol. The pressure transmitter must support the following protocol-specific functions:

- HART protocol
- Burst mode

#### Current input

#### Digital communication

The measured values can be written by the automation system via:

- FOUNDATION Fieldbus
- PROFIBUS DP
- PROFIBUS PA
- Modbus RS485
- Modbus TCP over Ethernet-APL
- EtherNet/IP
- PROFINET
- PROFINET over Ethernet-APL

#### Current input 0/4 to 20 mA

Current input	0/4 to 20 mA (active/passive)
Current span	<ul><li>4 to 20 mA (active)</li><li>0/4 to 20 mA (passive)</li></ul>
Resolution	1 μΑ
Voltage drop	Typically: 0.6 to 2 V for 3.6 to 22 mA (passive)
Maximum input voltage	≤ 30 V (passive)

Open-circuit voltage	≤ 28.8 V (active)
Possible input variables	<ul><li>Pressure</li><li>Temperature</li><li>Density</li></ul>

#### Status input

Maximum input values	■ DC $-3$ to 30 V ■ If status input is active (ON): $R_i > 3 \text{ k}\Omega$		
Response time Configurable: 5 to 200 ms			
Input signal level	<ul> <li>Low signal: DC -3 to +5 V</li> <li>High signal: DC 12 to 30 V</li> </ul>		
Assignable functions	<ul> <li>Off</li> <li>Reset the individual totalizers separately</li> <li>Reset all totalizers</li> <li>Flow override</li> </ul>		

# Output

#### Output and input variants

Depending on the option selected for output/input 1, different options are available for the other outputs and inputs. Only one option can be selected for each output/input 1 to 4. The following tables must be read vertically  $(\downarrow)$ .

Example: If the option BA "4-20 mA HART" was selected for output/input 1, one of the options A, B, D, E, F, H, I or J is available for output 2 and one of the options A, B, D, E, F, H, I or J is available for output 3 and 4.

#### Output/input 1 and options for output/input 2



Options for output/input 3 and 4  $\rightarrow$   $\stackrel{\triangle}{=}$  16

Order code for "Output; input 1" (020) →							Poss	ible o	ption	s					
Current output 4 to 20 mA HART	ВА														
Current output 4 to 20 mA HART Ex i passive	<b>4</b>	CA													
Current output 4 to 20 mA HART Ex i active		<b>4</b>	СС												
FOUNDATION fieldbus			<b>4</b>	SA											
FOUNDATION fieldbus Ex i				4	TA										
PROFIBUS DP					<b>\</b>	LA									
PROFIBUS PA						<b>\</b>	GA								
PROFIBUS PA Ex i							<b>\</b>	НА							
Modbus RS485								<b>\</b>	MA						
Ethernet/IP 2-port switch integrated									<b>\</b>	NA					
PROFINET 2-port switch integrated										4	RA				
PROFINET over Ethernet-APL											4	RB			
PROFINET over Ethernet-APL Ex i												1	RC		
Modbus TCP over Ethernet-APL 10 Mbit/s, SPE 10 Mbit/s, Ethernet 100 Mbit/s													<b>\</b>	МВ	
Modbus TCP over Ethernet-APL, Ex i, 10 Mbit/s, Ethernet 100 Mbit/s														4	МС
Order code for "Output; input 2" (021) →	<b>\</b>	4	<b>\</b>	4	<b>\</b>	<b>\</b>	<b>\</b>	<b>\</b>	<b>\</b>	4	1	1	<b>\</b>	<b>\</b>	<b>\</b>
Not used	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α
Current output 4 to 20 mA	В			В		В	В		В	В	В	В		В	
Current output 4 to 20 mA Ex i passive		С	С		С			С					С		С
User-configurable input/output 1)	D			D		D	D		D	D	D	D		D	
Pulse/frequency/switch output	Е			Е		Е	Е		Е	Е	Е	Е		Е	
Double pulse output <sup>2)</sup>	F								F						
Pulse/frequency/switch output Ex i passive		G	G		G			G					G		G
Relay output	Н			Н		Н	Н		Н	Н	Н	Н		Н	
Current input 0/4 to 20 mA	I			I		I	I		I	I	I	I		I	
Status input	J			J		J	J		J	J	J	J		J	

<sup>2)</sup> If double pulse output (F) is selected for output/input 2 (021), only the double pulse output (F) option is available for selection for output/input 3 (022).

#### Output/input 1 and options for output/input 3 and 4

Options for output/input  $2 \rightarrow \triangleq 15$ 

Order code for "Output; input 1" (020) →	Possible options														
Current output 4 to 20 mA HART	ВА														
Current output 4 to 20 mA HART Ex i passive	<b>\</b>	CA													
Current output 4 to 20 mA HART Ex i active		<b>\</b>	СС												
FOUNDATION fieldbus			<b>\</b>	SA											
FOUNDATION fieldbus Ex i				<b>\</b>	TA										
PROFIBUS DP					<b>\</b>	LA									
PROFIBUS PA						<b>\</b>	GA								
PROFIBUS PA Ex i							<b>\</b>	НА							
Modbus RS485								<b>\</b>	MA						
Ethernet/IP 2-port switch integrated									<b>\</b>	NA					
PROFINET 2-port switch integrated										4	RA				
PROFINET over Ethernet-APL 10 Mbit/s, 2-wire											4	RB			
PROFINET over Ethernet-APL Ex i, 10 Mbit/s, 2-wire												<b>4</b>	RC		
Modbus TCP over Ethernet-APL 10 Mbit/s, SPE 10 Mbit/s, Ethernet 100 Mbit/s													<b>\</b>	МВ	
Modbus TCP over Ethernet-APL, Ex i, 10 Mbit/s, Ethernet 100 Mbit/s														4	МС
Order code for "Output; input 3" (022), "Output; input 4" (023) $^{1)}$ $\rightarrow$	<b>\</b>	<b>\</b>	<b>\</b>	<b>\</b>	<b>\</b>	<b>\</b>	<b>\</b>	<b>\</b>	<b>+</b>	4	4	4	4	<b>\</b>	<b>→</b>
Not used	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α
Current output 4 to 20 mA	В					В			В	В	В	В		В	
Current output 4 to 20 mA Ex i passive <sup>2)</sup>		С	С												
User-configurable input/output	D					D			D	D	D	D		D	
Pulse/frequency/switch output	Е					Е			Е	Е	Е	Е		Е	
Double pulse output (slave) 3)	F								F						
Pulse/frequency/switch output Ex i passive 4)		G	G												
Relay output	Н					Н			Н	Н	Н	Н		Н	
Current input 0/4 to 20 mA	I					I			I	I	I	I		I	
Status input	J					J			J	J	J	J		J	

The order code for "Output; input 4" (023) is only available for the Proline 500-digital transmitter, order code for "Integrated ISEM electronics", 1) option A.

The current output 4 to 20 mA Ex i passive (C) option is not available for input/output 4.

The double pulse output (F) option is not available for input/output 4. 3)

The pulse/frequency/switch output Ex i passive (G) option is not available for input/output 4.

#### Output signal

#### Current output 4 to 20 mA HART

Order code	"Output; input 1" (20): Option BA: current output 4 to 20 mA HART
Signal mode	Can be set to: Active Passive
Current range	Can be set to:  4 to 20 mA NAMUR  4 to 20 mA US  4 to 20 mA  0 to 20 mA  for the signal mode is active)  Fixed current
Open-circuit voltage	DC 28.8 V (active)
Maximum input voltage	DC 30 V (passive)
Load	250 to 700 Ω
Resolution	0.38 μΑ
Damping	Configurable: 0 to 999.9 s
Assignable measured variables	<ul> <li>Mass flow</li> <li>Volume flow</li> <li>Corrected volume flow</li> <li>Density</li> <li>Reference density</li> <li>Temperature</li> <li>Electronics temperature</li> <li>Oscillation frequency 0</li> <li>Oscillation damping 0</li> <li>Signal asymmetry</li> <li>Exciter current 0</li> <li>The range of options increases if the measuring device has one or more application packages.</li> </ul>

#### Current output 4 to 20 mA HART Ex i

Order code	"Output; input 1" (20) choose from:  ■ Option CA: current output 4 to 20 mA HART Ex i passive  ■ Option CC: current output 4 to 20 mA HART Ex i active
Signal mode	Depends on the selected order version.
Current range	Can be set to:  4 to 20 mA NAMUR  4 to 20 mA US  4 to 20 mA  0 to 20 mA  for independent of the signal mode is active)  Fixed current
Open-circuit voltage	DC 21.8 V (active)
Maximum input voltage	DC 30 V (passive)
Load	<ul> <li>250 to 400 Ω (active)</li> <li>250 to 700 Ω (passive)</li> </ul>
Resolution	0.38 μΑ

Damping	Configurable: 0 to 999.9 s
Assignable measured variables	<ul> <li>Mass flow</li> <li>Volume flow</li> <li>Corrected volume flow</li> <li>Density</li> <li>Reference density</li> <li>Temperature</li> <li>Electronics temperature</li> <li>Oscillation frequency 0</li> <li>Oscillation damping 0</li> <li>Signal asymmetry</li> <li>Exciter current 0</li> <li>The range of options increases if the measuring device has one or more application packages.</li> </ul>

#### FOUNDATION Fieldbus

FOUNDATION Fieldbus H1, IEC 61158-2, galvanically isolated			
Data transfer	31.25 kbit/s		
<b>Current consumption</b>	10 mA		
Permitted supply voltage	9 to 32 V		
Bus connection	With integrated reverse polarity protection		

#### PROFIBUS DP

Signal encoding	NRZ code
Data transfer	9.6 kBaud12 MBaud
Terminating resistor	Integrated, can be activated via DIP switches

#### PROFIBUS PA

PROFIBUS PA	In accordance with EN 50170 Volume 2, IEC 61158-2 (MBP), galvanically isolated
Data transmission	31.25 kbit/s
<b>Current consumption</b>	10 mA
Permitted supply voltage	9 to 32 V
Bus connection	With integrated reverse polarity protection

#### Modbus RS485

Physical interface	RS485 in accordance with EIA/TIA-485 standard
Terminating resistor	Integrated, can be activated via DIP switches

#### Modbus TCP over Ethernet-APL

Port 1: Modbus TCP over Et	Port 1: Modbus TCP over Ethernet-APL 10 Mbit/s					
Device usage	Device connection to an APL field switch (terminal 26/27)  The device may only be operated according to the following APL port classifications:  If used in hazardous areas: SLAA or SLAC 1)  If used in non-hazardous areas: SLAX					
	Connection values of APL field switch (corresponds to APL port classification SPCC or SPAA, for instance):					
	<ul> <li>Maximum input voltage: 15 V<sub>DC</sub></li> <li>Minimum output values: 0.54 W</li> </ul>					
	<ul> <li>Device connection to an SPE switch</li> <li>In non-hazardous areas, the device can be used with an appropriate SPE switch:</li> <li>Maximum output voltage: 30 V<sub>DC</sub></li> <li>Minimum output power: 1.85 W</li> <li>The SPE switch must support the 10BASE-T1L standard and PoDL power classes 10, 11 or 12 and have a function to disable power class detection.</li> </ul>					
Standards	According to IEEE 802.3cg, APL port profile specification v1.0, galvanically isolated					
Data transfer	Full-duplex (APL/SPE)					
Current consumption	Terminal 26/27 max. approx. 45 mA					
Permitted supply voltage	9 to 30 V					
Bus connection	Terminal 26/27 with integrated reverse polarity protection					

 $1) \qquad \hbox{For more information on using the device in the hazardous area, see the Ex-specific Safety Instructions}$ 

Port 2: Modbus TCP over Ethernet 100 Mbit/s	
Device usage	Device connection to a Fast Ethernet (RJ45) switch In non-hazardous areas, the Ethernet switch must support the standard 100BASE-TX.
Standards	In accordance with IEEE 802.3u
Data transfer	Half-duplex, full-duplex
Current consumption	-
Permitted supply voltage	-
Bus connection	Service interface (RJ45)

#### EtherNet/IP

Standards	In accordance with IEEE 802.3
-----------	-------------------------------

#### PROFINET

Standards	In accordance with IEEE 802.3
-----------	-------------------------------

#### PROFINET over Ethernet-APL

Device use	Device connection to an APL field switch  The device may only be operated according to the following APL port classifications:  ■ If used in hazardous areas: SLAA or SLAC ¹¹  ■ If used in non-hazardous areas: SLAX  Connection values of APL field switch (corresponds to APL port classification SPCC or SPAA, for instance):  ■ Maximum input voltage: 15 V <sub>DC</sub>
	<ul> <li>Minimum output values: 0.54 W</li> <li>Device connection to an SPE switch</li> <li>In non-hazardous areas, the device can be used with an appropriate SPE switch: The device can be connected to an SPE switch with a maximum voltage of 30 V<sub>DC</sub> and a minimum output power of 1.85 W connected.</li> <li>The SPE switch must support the 10BASE-T1L standard and PoDL power classes 10, 11 or 12 and have a function to disable power class detection.</li> </ul>
PROFINET	According to IEC 61158 and IEC 61784
Ethernet-APL	According to IEEE 802.3cg, APL port profile specification v1.0, galvanically isolated
Data transfer	10 Mbit/s
Current consumption	Transmitter  • Max. 400 mA(24 V)  • Max. 200 mA (110 V, 50/60 Hz; 230 V, 50/60 Hz)
Permitted supply voltage	9 to 30 V
Network connection	With integrated reverse polarity protection

1) For more information on using the device in the hazardous area, see the Ex-specific Safety Instructions

#### Current output 4 to 20 mA

Order code	"Output; input 2" (21), "Output; input 3" (022) or "Output; input 4" (023): Option B: current output 4 to 20 mA
Signal mode	Can be set to: Active Passive
Current range	Can be set to:  4 to 20 mA NAMUR  4 to 20 mA US  4 to 20 mA  0 to 20 mA  for independent of the signal mode is active)  Fixed current
Maximum output values	22.5 mA
Open-circuit voltage	DC 28.8 V (active)
Maximum input voltage	DC 30 V (passive)
Load	$0$ to $700~\Omega$
Resolution	0.38 μΑ

Damping	Configurable: 0 to 999.9 s
Assignable measured variables	<ul> <li>Mass flow</li> <li>Volume flow</li> <li>Corrected volume flow</li> <li>Density</li> <li>Reference density</li> <li>Temperature</li> <li>Electronics temperature</li> <li>Oscillation frequency 0</li> <li>Oscillation damping 0</li> <li>Signal asymmetry</li> <li>Exciter current 0</li> <li>The range of options increases if the measuring device has one or more application packages.</li> </ul>

#### Current output 4 to 20 mA Ex i passive

Order code	"Output; input 2" (21), "Output; input 3" (022): Option C: current output 4 to 20 mA Ex i passive
Signal mode	Passive
Current range	Can be set to:  4 to 20 mA NAMUR  4 to 20 mA US  4 to 20 mA  Fixed current
Maximum output values	22.5 mA
Maximum input voltage	DC 30 V
Load	0 to 700 $\Omega$
Resolution	0.38 μΑ
Damping	Configurable: 0 to 999 s
Assignable measured variables	<ul> <li>Mass flow</li> <li>Volume flow</li> <li>Corrected volume flow</li> <li>Density</li> <li>Reference density</li> <li>Temperature</li> <li>Electronics temperature</li> <li>Oscillation frequency 0</li> <li>Oscillation damping 0</li> <li>Signal asymmetry</li> <li>Exciter current 0</li> <li>The range of options increases if the measuring device has one or more application packages.</li> </ul>

#### Pulse/frequency/switch output

Function	Can be configured as pulse, frequency or switch output
Version	Open collector  Can be set to:     Active     Passive     Passive NAMUR  Ex-i, passive
Maximum input values	DC 30 V, 250 mA (passive)
Open-circuit voltage	DC 28.8 V (active)
Voltage drop	For 22.5 mA: ≤ DC 2 V

Pulse output	
Maximum input values	DC 30 V, 250 mA (passive)
Maximum output current	22.5 mA (active)
Open-circuit voltage	DC 28.8 V (active)
Pulse width	Configurable: 0.05 to 2 000 ms
Maximum pulse rate	10 000 Impulse/s
Pulse value	Configurable
Assignable measured variables	<ul> <li>Mass flow</li> <li>Volume flow</li> <li>Corrected volume flow</li> <li>The range of options increases if the measuring device has one or more</li> </ul>
	The range of options increases if the measuring device has one or more application packages.
Frequency output	
Maximum input values	DC 30 V, 250 mA (passive)
Maximum output current	22.5 mA (active)
Open-circuit voltage	DC 28.8 V (active)
Output frequency	Configurable: end value frequency 2 to $10000Hz(f_{max} = 12500Hz)$
Damping	Configurable: 0 to 999.9 s
Pulse/pause ratio	1:1
Assignable measured variables	<ul> <li>Mass flow</li> <li>Volume flow</li> <li>Corrected volume flow</li> <li>Density</li> <li>Reference density</li> <li>Temperature</li> <li>Electronics temperature</li> <li>Oscillation frequency 0</li> <li>Oscillation damping 0</li> <li>Signal asymmetry</li> <li>Exciter current 0</li> <li>The range of options increases if the measuring device has one or more application packages.</li> </ul>
Switch output	
Maximum input values	DC 30 V, 250 mA (passive)
Open-circuit voltage	DC 28.8 V (active)
Switching behavior	Binary, conductive or non-conductive
Switching delay	Configurable: 0 to 100 s

Number of switching cycles	Unlimited
Assignable functions	<ul> <li>Disable</li> <li>On</li> <li>Diagnostic behavior</li> <li>Limit</li> <li>Mass flow</li> <li>Volume flow</li> <li>Corrected volume flow</li> <li>Density</li> <li>Reference density</li> <li>Temperature</li> <li>Totalizer 1-3</li> <li>Flow direction monitoring</li> <li>Status</li> <li>Partially filled pipe detection</li> <li>Low flow cut off</li> <li>The range of options increases if the measuring device has one or more application packages.</li> </ul>

#### Double pulse output

Function	Double pulse
Version	Open collector
	Can be set to: Active Passive Passive NAMUR
Maximum input values	DC 30 V, 250 mA (passive)
Open-circuit voltage	DC 28.8 V (active)
Voltage drop	For 22.5 mA: ≤ DC 2 V
Output frequency	Configurable: 0 to 1000 Hz
Damping	Configurable: 0 to 999 s
Pulse/pause ratio	1:1
Assignable measured variables	<ul> <li>Mass flow</li> <li>Volume flow</li> <li>Corrected volume flow</li> <li>Density</li> <li>Reference density</li> <li>Temperature</li> <li>The range of options increases if the measuring device has one or more application packages.</li> </ul>

### Relay output

Function	Switch output
Version	Relay output, galvanically isolated
Switching behavior	Can be set to: NO (normally open), factory setting NC (normally closed)

Maximum switching capacity (passive)	<ul> <li>DC 30 V, 0.1 A</li> <li>AC 30 V, 0.5 A</li> </ul>
Assignable functions	<ul> <li>Disable</li> <li>On</li> <li>Diagnostic behavior</li> <li>Limit</li> <li>Mass flow</li> <li>Volume flow</li> <li>Corrected volume flow</li> <li>Density</li> <li>Reference density</li> <li>Temperature</li> <li>Totalizer 1-3</li> <li>Flow direction monitoring</li> <li>Status</li> <li>Partially filled pipe detection</li> <li>Low flow cut off</li> <li>The range of options increases if the measuring device has one or more application packages.</li> </ul>

#### User-configurable input/output

**One** specific input or output is assigned to a user-configurable input/output (configurable I/O) during device commissioning.

The following inputs and outputs are available for assignment:

- Choice of current output: 4 to 20 mA (active), 0/4 to 20 mA (passive)
- Pulse/frequency/switch output
- Choice of current input: 4 to 20 mA (active), 0/4 to 20 mA (passive)
- Status input

The technical values correspond to those of the inputs and outputs described in this section.

#### Signal on alarm

Depending on the interface, failure information is displayed as follows:

#### **HART** current output

Device diagnostics	Device condition can be read out via HART Command 48
--------------------	--

#### **PROFIBUS PA**

Status and alarm messages	Diagnostics in accordance with PROFIBUS PA Profile 3.02
Failure current FDE (Fault Disconnection Electronic)	0 mA

#### PROFIBUS DP

Status and alarm	Diagnostics in accordance with PROFIBUS PA Profile 3.02
messages	

#### EtherNet/IP

Device diagnostics	Device condition can be read out in Input Assembly
--------------------	--

#### **PROFINET**

#### PROFINET over Ethernet-APL

Device diagnostics	Diagnostics according to PROFINET PA Profile 4.02

#### FOUNDATION Fieldbus

Status and alarm messages	Diagnostics in accordance with FF-891
Failure current FDE (Fault Disconnection Electronic)	0 mA

#### Modbus RS485

Failure mode	Choose from:
	■ NaN value instead of current value
	■ Last valid value

#### Modbus TCP over Ethernet-APL/SPE/Fast Ethernet

Failure mode	Choose from:
	■ NaN value instead of current value
	■ Last valid value

#### **Current output**

Current output 4-20 mA	
Failure mode	Configurable:  4 to 20 mA in accordance with NAMUR recommendation NE 43  4 to 20 mA in accordance with US  Min. value: 3.59 mA  Max. value: 22.5 mA  Definable value between: 3.59 to 22.5 mA  Actual value  Last valid value
Current output 4-20 mA	
Failure mode	Configurable:  ■ Maximum alarm: 22 mA  ■ Definable value between: 0 to 20.5 mA

#### Pulse/frequency/switch output

Pulse output	
Failure mode	Configurable:
Frequency output	
Failure mode	Configurable:     Actual value     O Hz     Definable value between: 2 to 12 500 Hz
Switch output	
Failure mode	Configurable:

#### Relay output

Failure mode	Choose from:
	<ul> <li>Current status</li> </ul>
	■ Open
	■ Closed

#### Local display

Plain text display	With information on cause and remedial measures
Backlight	Red lighting indicates a device error.



Status signal as per NAMUR recommendation NE 107  $\,$ 

#### Interface/protocol

- Via digital communication:
  - HART protocol
  - FOUNDATION Fieldbus
  - PROFIBUS PA
  - PROFIBUS DP
  - Modbus RS485
  - Modbus TCP over Ethernet-APL
  - EtherNet/IP
  - PROFINET
  - PROFINET over Ethernet-APL
- Via service interface
  - Service interface CDI-RJ45
  - Via service interface/port 2: (RJ45)
  - WLAN interface
- Plain text display
  - With information on cause and remedial actions
  - Modbus TCP

#### Web browser

Plain text display	With information on cause and remedial measures
--------------------	---

#### LEDs

Status information	Status indicated by various LEDs
	The following information is displayed depending on the device version:  Supply voltage active  Data transmission active  Device alarm/error has occurred  Network available <sup>1)</sup> Connection established <sup>1)</sup> Diagnostic status <sup>2)</sup> PROFINET blinking feature <sup>3)</sup>

- 1) Only available for PROFINET, PROFINET over Ethernet-APL, Modbus over Ethernet-APL, Ethernet/IP
- 2) Only available for Modbus over Ethernet-APL
- 3) Only available for PROFINET, PROFINET over Ethernet-APL,

**Load** Output signal  $\rightarrow \blacksquare 17$ 

#### Ex connection data Safety-related values

Order code for	Output type	Safety-related values	
"Output; input 1"		Output; input 1 (Port 1)	Service interface (Port 2)
Option <b>BA</b>	Current output 4-20 mA HART	$U_{N} = 30 V_{DC}$ $U_{M} = 250 V_{AC}$	$U_N = 3.3 V_{AC}$ $U_M = 250 V_{AC}$
Option <b>GA</b>	PROFIBUS PA	$U_N = 32 V_{DC}$ $U_M = 250 V_{AC}$	$U_N = 3.3 V_{AC}$ $U_M = 250 V_{AC}$
Option <b>LA</b>	PROFIBUS DP	$U_{N} = 5 V$ $U_{M} = 250 V_{AC}$	$U_N = 3.3 V_{AC}$ $U_M = 250 V_{AC}$
Option <b>MA</b>	Modbus RS485	$U_{N} = 5 V$ $U_{M} = 250 V_{AC}$	$U_N = 3.3 V_{AC}$ $U_M = 250 V_{AC}$
Option <b>MB</b>	Modbus TCP over Ethernet-APL 10 Mbit/s, SPE 10 Mbit/s, Ethernet 100 Mbit/s	APL port profile SLAX SPE PoDL classes 10, 11, 12 $U_N = 30 \ V_{DC}$ $U_M = 250 \ V_{AC}$	$U_{N} = 3.3 V_{AC}$ $U_{M} = 250 V_{AC}$
Option <b>NA</b>	EtherNet/IP	$U_N = 3.3 V_{AC}$ $U_M = 250 V_{AC}$	U <sub>N</sub> = 3.3 V <sub>AC</sub> U <sub>M</sub> = 250 V <sub>AC</sub>
Option <b>RA</b>	PROFINET	$U_N = 3.3 V_{AC}$ $U_M = 250 V_{AC}$	$U_N = 3.3 V_{AC}$ $U_M = 250 V_{AC}$
Option <b>RB</b>	PROFINET over Ethernet-APL/SPE, 10Mbit/s	APL port profile SLAX SPE PoDL classes 10, 11, 12 $U_N = 30 \ V_{DC}$ $U_M = 250 \ V_{AC}$	$U_{N} = 3.3 V_{AC}$ $U_{M} = 250 V_{AC}$
Option <b>SA</b>	FOUNDATION Fieldbus	$\begin{array}{l} U_N = 32 \ V_{DC} \\ U_M = 250 \ V_{AC} \end{array}$	$U_{N} = 3.3 V_{AC}$ $U_{M} = 250 V_{AC}$

The specifications for  $U_M$  only apply to devices with Ex i circuits. Zone 1; Class I, Division 1 devices; Zone 2; Class I Division 2 devices with Ex i sensor.

Order code for	Output type		Safety-related values	
"Output; input 2" "Output; input 3" "Output; input 4"		Output; input 2	Output; input 3	Output; input 4
Option <b>B</b>	Current output 4-20 mA	$U_{N} = 30 V_{DC}$ $U_{M} = 250 V_{AC}$		
Option <b>D</b>	Configurable I/O initial setting off	$U_{N} = 30 V_{DC}$ $U_{M} = 250 V_{AC}$		
Option <b>E</b>	Pulse/frequency/switch output	$U_{N} = 30 V_{DC}$ $U_{M} = 250 V_{AC}$		
Option <b>F</b>	Double pulse output	$U_{N} = 30 V_{DC}$ $U_{M} = 250 V_{AC}$		
Option <b>H</b>	Relay output	$U_N = 30 V_{DC}$ $I_N = 100 \text{ mA}_{DC} / 500 \text{ mA}_{AC}$ $U_M = 250 V_{AC}$		
Option <b>I</b>	Current input 4-20 mA	$U_{N} = 30 V_{DC}$ $U_{M} = 250 V_{AC}$		
Option <b>J</b>	Status input	$U_{\rm N} = 30  V_{\rm DC}$ $U_{\rm M} = 250  V_{\rm AC}$		

#### Intrinsically safe values

Zone 1, Zone 21	Zone 1, Zone 21			
Order code for "Output; input 1"	Output type	Intrinsically safe values		
Output, input 1		Output; input 1 (Port 1)	Service interface (Port 2)	
Option CA	Current output 4-20mA HART Ex-i passive	$ \begin{aligned} & \textbf{Ex ic} \\ & \textbf{Ex ia} & ^{1)} \\ & \textbf{U}_i = 30 \ \textbf{V} \\ & \textbf{I}_i = 100 \ \textbf{mA} \\ & \textbf{P}_i = 1.25 \ \textbf{W} \\ & \textbf{L}_i = 0 \ \mu \textbf{H} \\ & \textbf{C}_i = 6 \ \textbf{nF} \end{aligned} $	$\begin{aligned} &\textbf{Ex ia}^{\ 1)} \\ &U_i = 10 \ V \\ &I_i = n. \ a. \\ &P_i = n. \ a. \\ &L_i = 0 \ \mu H \\ &C_i = 200 \ nF \end{aligned}$	
		Ex ic $^{2)}$ Ex ic (NIFW) $^{3)}$ $U_i = 30 \text{ V}$ $I_i = 100 \text{ mA}$ $P_i = 1.25 \text{ W}$ $L_i = 0 \mu\text{H}$ $C_i = 6 \text{ nF}$	Non-intrinsically safe <sup>4)</sup>	
Option CC	Current output 4-20mA HART Ex-i active	$ \begin{aligned} &\textbf{Ex ia}^{1} \\ &\textbf{U}_0 = 21.8  \text{V} \\ &\textbf{I}_0 = 90  \text{mA} \\ &\textbf{P}_0 = 491  \text{mW} \\ &\textbf{L}_0 = 4.1  \text{mH(IIC)/15 mH(IIB)} \\ &\textbf{C}_0 = 160  \text{nF(IIC)/1160 nF(IIB)} \\ &\textbf{U}_i = 30  \text{V} \\ &\textbf{I}_i = 10  \text{mA} \\ &\textbf{P}_i = 0.3  \text{W} \\ &\textbf{L}_i = 5  \mu \text{H} \\ &\textbf{L}_i = 4.1  \mu \text{H} \\ &\textbf{C}_i = 6  \text{nF} \end{aligned} $	$ \begin{aligned}                                   $	
		Ex ic $^{2)}$ Ex ic (NIFW) $^{3)}$ $U_0 = 21.8 \text{ V}$ $I_0 = 90 \text{ mA}$ $P_i = 491 \text{ mW}$ $L_0 = 9 \text{ mH}(\text{IIC})/39 \text{ mH}(\text{IIB})$ $C_0 = 600 \text{ nF}(\text{IIC})/4000 \text{ nF}(\text{IIB})$ $U_i = 30 \text{ V}$ $I_i = 10 \text{ mA}$ $P_i = 0.3 \text{ W}$ $L_i = 5 \text{ \muH}$ $L_i = 4.1 \text{ \muH}$ $C_i = 6 \text{ nF}$	Non-intrinsically safe <sup>4)</sup>	
Option HA	PROFIBUS PA Ex i (STANDARD + FISCO)	Ex ia $^{1)}$ $U_i = 30 \text{ V}$ $I_i = 570 \text{ mA}$ $P_i = 8.5 \text{ W}$ $L_i = 10 \mu\text{H}$ $C_i = 5 \text{ nF}$ Ex ic $^{2)}$ Ex ic (NIFW) $^{3)}$ $U_i = 32 \text{ V}$ $I_i = 570 \text{ mA}$ $P_i = 8.5 \text{ W}$ $L_i = 10 \mu\text{H}$ $C_i = 5 \text{ nF}$	$ \begin{aligned} &\textbf{Ex ia}^{\ 1)} \\ &U_i = 10 \ V \\ &I_i = n. \ a. \\ &P_i = n. \ a. \\ &L_i = 0 \ \mu H \\ &C_i = 200 \ nF \end{aligned} $ Non-intrinsically safe $^{4)}$	

Zone 1, Zone 21				
Order code for	Output type	Intrinsically safe values		
"Output; input 1"		Output; input 1 (Port 1)	Service interface (Port 2)	
Option MC	Modbus TCP over Ethernet-APL, Ex-i, 10Mbit/s	2-WISE power load, APL port profile SLAA $^{5)}$ Ex ia $^{1)}$ $U_i = 17.5 \text{ V}$ $I_i = 380 \text{ mA}$ $P_i = 5.32 \text{ W}$ $L_i = 10 \mu\text{H}$ $C_i = 5 \text{ nF}$ Cable specifications according to 2-WISE: $R_c = 15 \text{ to } 150 \Omega/\text{km}$ $L_c = 0.4 \text{ to } 1 \text{ mH/km}$ $C_c = 45 \text{ to } 200 \text{ nF/km}$ $C_c = C_c \text{ line/line} + 0.5 C_c \text{ line/screen, if both lines are floating, or C_c = C_c \text{ line/line} + C_c \text{ line/screen, if the screen is connected to one line} Length of cable (not including cable stubs): \leq 200 \text{ m} (656.2 ft) Length of cable stubs: \leq 1 \text{ m} (3.3 ft)$	Ex ia $^{1)}$ $U_i = 10 \text{ V}$ $I_i = n. \text{ a.}$ $P_i = n. \text{ a.}$ $L_i = 0  \mu\text{H}$ $C_i = 200  n\text{F}$	
			Non-intrinsically safe <sup>4)</sup>	
Option RC	PROFINET over Ethernet-APL, Ex-i, 10Mbit/s	2-WISE power load, APL port profile SLAA $^{5)}$ Ex ia $^{1)}$ $U_i = 17.5 \text{ V}$ $I_i = 380 \text{ mA}$ $P_i = 5.32 \text{ W}$ $L_i = 10 \mu\text{H}$ $C_i = 5 \text{ nF}$ Cable specifications according to 2-WISE: $R_c = 15 \text{ to } 150 \Omega/\text{km}$ $L_c = 0.4 \text{ to } 1 \text{ mH/km}$ $C_c = 45 \text{ to } 200 \text{ nF/km}$ $C_c = 45 \text{ to } 200 \text{ nF/km}$ $C_c = C_c \text{ line/line} + 0.5 C_c \text{ line/screen, if both lines are floating, or C_c = C_c \text{ line/line} + C_c \text{ line/screen, if the screen is connected to one line} Length of cable (not including cable stubs): \leq 200 \text{ m } (656.2 \text{ ft}) Length of cable stubs: \leq 1 \text{ m } (3.3 \text{ ft})$	Ex ia $^{1)}$ $U_i = 10 \text{ V}$ $I_i = n. \text{ a.}$ $P_i = n. \text{ a.}$ $L_i = 0  \mu\text{H}$ $C_i = 200  n\text{F}$	

Zone 1, Zone 21	Zone 1, Zone 21			
Order code for	Output type	Intrinsically safe values		
"Output; input 1"		Output; input 1 (Port 1)	Service interface (Port 2)	
		2-WISE power load, APL port profile SLAC $^{5)}$ Ex ic $^{2)}$ Ex ic (NIFW) $^{3)}$ U <sub>i</sub> = 17.5 V I <sub>i</sub> = 380 mA P <sub>i</sub> = 5.32 W L <sub>i</sub> = 10 $\mu$ H C <sub>i</sub> = 5 nF Cable specifications according to 2-WISE: R <sub>c</sub> = 15 to 150 $\Omega$ /km L <sub>c</sub> = 0.4 to 1 mH/km C <sub>c</sub> = 45 to 200 nF/km C <sub>c</sub> = C <sub>c</sub> line/line + 0,5 C <sub>c</sub> line/screen, if both lines are floating, or C <sub>c</sub> = C <sub>c</sub> line/line + C <sub>c</sub> line/screen, if the screen is connected to one line Length of cable (not including cable stubs): $\leq$ 200 m (656.2 ft) Length of cable stubs: $\leq$ 1 m (3.3 ft)	Non-intrinsically safe <sup>4)</sup>	
Option TA	FOUNDATION Fieldbus Ex i (STANDARD + FISCO)	Ex ia $^{1)}$ $U_{i} = 30 \text{ V}$ $I_{i} = 570 \text{ mA}$ $P_{i} = 8.5 \text{ W}$ $L_{i} = 10  \mu\text{H}$ $C_{i} = 5 \text{ nF}$ Ex ic $^{2)}$ Ex ic (NIFW) $^{3)}$ $U_{i} = 32 \text{ V}$ $I_{i} = 570 \text{ mA}$ $P_{i} = 8.5 \text{ W}$ $L_{i} = 10  \mu\text{H}$ $C_{i} = 5 \text{ nF}$	Ex ia $^{1)}$ $U_i = 10 \text{ V}$ $I_i = n. \text{ a.}$ $P_i = n. \text{ a.}$ $L_i = 0  \mu\text{H}$ $C_i = 200 \text{ nF}$ Non-intrinsically safe $^{4)}$	

- Only for the order code for "Approval", option BB, BD MB, MD NB, ND JD KB, KD GB, GD, BB, BDC2, C4 CD UB, UD For approved options only: See separate document "Safety Instructions" (XA) for the device. For approved options only: See separate document "Safety Instructions" (XA) for the device. Connection to or operation with Service interface (Port 2) is not permitted in potentially explosive atmospheres. For further options see Ethernet-APL Installation Drawing HE\_01622. 1)
- 2)
- 3)
- 4)

Zone 2	Zone 2			
Order code for "Output; input 1"	Output type	Intrinsically safe values or NIFW values Output; input 1 (Port 1)		
Option HA	PROFIBUS PA Ex i (STANDARD + FISCO)	Ex ic AEx ic, Ex ic, NIFW $U_i = 32 \text{ V}$ $I_i = 570 \text{ mA}$ $P_i = 8.5 \text{ W}$ $L_i = 10 \mu\text{H}$ $C_i = 5 \text{ nF}$		
Option MC	Modbus TCP over Ethernet-APL, Ex-i, 10Mbit/s	2-WISE power load, APL port profile SLAC <sup>1)</sup> Ex ic		
Option RC	PROFINET over Ethernet-APL, Ex-i, 10Mbit/s	AEx ic, Ex ic, NIFW $ U_i = 17.5 \text{ V} $ $ I_i = 380 \text{ mA} $ $ P_i = 5.32 \text{ W} $ $ L_i = 10  \mu\text{H} $ $ C_i = 5 \text{ nF} $ Cable specifications according to 2-WISE: $ R_c = 15 \text{ to } 150  \Omega/\text{km} $ $ L_c = 0.4 \text{ to } 1 \text{ mH/km} $ $ C_c = 45 \text{ to } 200 \text{ nF/km} $ $ C_c = C_c \text{ line/line} + 0.5  C_c \text{ line/screen, if both lines are floating, or } $ $ C_c = C_c \text{ line/line} + C_c \text{ line/screen, if the screen is connected to one line } $ $ \text{Length of cable (not including cable stubs): } \leq 200 \text{ m } (656.2 \text{ ft}) $ $ \text{Length of cable stubs: } \leq 1 \text{ m } (3.3 \text{ ft}) $		
Option TA	FOUNDATION Fieldbus Ex i (STANDARD + FISCO)	Ex ic AEx ic, Ex ic, NIFW $U_i = 32 \text{ V}$ $I_i = 570 \text{ mA}$ $P_i = 8.5 \text{ W}$ $L_i = 10 \mu\text{H}$ $C_i = 5 \text{ nF}$		

1) For further options see Ethernet-APL Installation Drawing HE\_01622.

Order code for	Output type	Intrinsically safe values or NIFW values		
"Output; input 2" "Output; input 3" "Output; input 4"		Output; input 2	Output; input 3	Output; input 4
Option C	Current output 4-20mA Ex-i passive	Ex ia or Ex ic (NIFW) Ex ic AEx ic, Ex ic, NIFW $U_i = 30 \text{ V}$ $I_i = 100 \text{ mA}$ $P_i = 1.25 \text{ W}$ $L_i = 0$ $C_i = 0$		
Option G	Pulse/frequency/switch output Ex-i passive	Ex ia or Ex ic (NIFW) Ex ic AEx ic, Ex ic, NIFW $U_i = 30 \text{ V}$ $I_i = 100 \text{ mA}$ $P_i = 1.25 \text{ W}$ $L_i = 0$ $C_i = 0$		

Low flow cut off	The switch points for low flow cut off are user-selectable.
Galvanic isolation	The outputs are galvanically isolated:  from the power supply from one another from the protective ground connection (PE)

#### Protocol-specific data

#### HART

Manufacturer ID	0x11
Device type ID	0x3B
HART protocol revision	7
Device description files (DTM, DD)	Information and files under: www.endress.com
HART load	Min. 250 Ω
System integration	Information on system integration: Operating Instructions → 🗎 117.  • Measured variables via HART protocol • Burst Mode functionality

#### FOUNDATION Fieldbus

Manufacturer ID	0x452B48 (hex)
Ident number	0x103B (hex)
Device revision	1
DD revision	Information and files under:
CFF revision	<ul><li>www.endress.com</li><li>www.fieldcommgroup.org</li></ul>
Interoperability Test Kit (ITK)	Version 6.2.0
ITK Test Campaign Number	Information:  www.endress.com  www.fieldcommgroup.org
Link Master capability (LAS)	Yes
Choice of "Link Master" and "Basic Device"	Yes Factory setting: Basic Device
Node address	Factory setting: 247 (0xF7)
Supported functions	The following methods are supported:  Restart  ENP Restart  Diagnostic  Set to OOS  Set to AUTO  Read trend data  Read event logbook
Virtual Communication Relation	nships (VCRs)
Number of VCRs	44
Number of link objects in VFD	50
Permanent entries	1
Client VCRs	0
Server VCRs	10
Source VCRs	43
Sink VCRs	0
Subscriber VCRs	43
Publisher VCRs	43
Device Link Capabilities	
Slot time	4
Min. delay between PDU	8

Max. response delay	16
System integration	Information regarding system integration: Operating Instructions $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $
	<ul><li>Cyclic data transmission</li><li>Description of the modules</li></ul>
	<ul><li>Execution times</li><li>Methods</li></ul>

#### PROFIBUS DP

Manufacturer ID	0x11
Ident number	0x156F
Profile version	3.02
Device description files (GSD, DTM, DD)	Information and files under:  ■ https://www.endress.com/download On the device product page: PRODUCTS → Product Finder → Links ■ https://www.profibus.com
Supported functions	Identification & Maintenance Simplest device identification on the part of the control system and nameplate PROFIBUS upload/download Reading and writing parameters is up to ten times faster with PROFIBUS upload/download Condensed status Simplest and self-explanatory diagnostic information by categorizing diagnostic messages that occur
Configuration of the device address	<ul> <li>DIP switches on the I/O electronics module</li> <li>Via operating tools (e.g. FieldCare)</li> </ul>
Compatibility with earlier model	If the device is replaced, the measuring device Promass 500 supports the compatibility of the cyclic data with previous models. It is not necessary to adjust the engineering parameters of the PROFIBUS network with the Promass 500 GSD file.  Previous model:  Previous model:  Promass 83 PROFIBUS DP  ID No.: 1529 (hex)  Extended GSD file: EH3x1529.gsd  Standard GSD file: EH3_1529.gsd  Description of the function scope of compatibility:  Operating Instructions →  117.
System integration	Information regarding system integration: Operating Instructions → 🖺 117.  Cyclic data transmission  Block model  Description of the modules

#### PROFIBUS PA

Manufacturer ID	0x11
Ident number	0x156D
Profile version	3.02
Device description files (GSD, DTM, DD)	Information and files under:  ■ https://www.endress.com/download On the device product page: PRODUCTS → Product Finder → Links ■ https://www.profibus.com

Supported functions	Identification & Maintenance Simplest device identification on the part of the control system and nameplate PROFIBUS upload/download Reading and writing parameters is up to ten times faster with PROFIBUS upload/download Condensed status Simplest and self-explanatory diagnostic information by categorizing diagnostic messages that occur
Configuration of the device address	<ul> <li>DIP switches on the I/O electronics module</li> <li>Local display</li> <li>Via operating tools (e.g. FieldCare)</li> </ul>
Compatibility with earlier model	If the device is replaced, the measuring device Promass 500 supports the compatibility of the cyclic data with previous models. It is not necessary to adjust the engineering parameters of the PROFIBUS network with the Promass 500 GSD file.  Earlier models:  ■ Promass 80 PROFIBUS PA  ■ ID No.: 1528 (hex)  ■ Extended GSD file: EH3x1528.gsd  ■ Standard GSD file: EH3_1528.gsd  ■ Promass 83 PROFIBUS PA  ■ ID No.: 152A (hex)  ■ Extended GSD file: EH3x152A.gsd  ■ Standard GSD file: EH3x152A.gsd  ■ Standard GSD file: EH3x152A.gsd  ■ Standard GSD file: EH3_152A.gsd  ■ Description of the function scope of compatibility: Operating Instructions →   ■ 117.
System integration	Information regarding system integration: Operating Instructions → 🖺 117.  Cyclic data transmission  Block model  Description of the modules

#### Modbus RS485

Protocol	Modbus Applications Protocol Specification V1.1
Response times	<ul> <li>Direct data access: typically 25 to 50 ms</li> <li>Auto-scan buffer (data range): typically 3 to 5 ms</li> </ul>
Device type	Slave
Slave address range	1 to 247
Broadcast address range	0
Function codes	<ul> <li>03: Read holding register</li> <li>04: Read input register</li> <li>06: Write single registers</li> <li>08: Diagnostics</li> <li>16: Write multiple registers</li> <li>23: Read/write multiple registers</li> </ul>
Broadcast messages	Supported by the following function codes:  O6: Write single registers  16: Write multiple registers  23: Read/write multiple registers
Supported baud rate	<ul> <li>1200 BAUD</li> <li>2400 BAUD</li> <li>4800 BAUD</li> <li>9600 BAUD</li> <li>19200 BAUD</li> <li>38400 BAUD</li> <li>57600 BAUD</li> <li>115200 BAUD</li> </ul>
Data transmission mode	■ ASCII ■ RTU

34

Data access	Each device parameter can be accessed via Modbus RS485.  For Modbus register information
Compatibility with earlier model	If the device is replaced, the measuring instrument Promass 500 supports the compatibility of the Modbus registers for the process variables and the diagnostic information with the previous model Promass 83. It is not necessary to change the engineering parameters in the automation system.  □ Description of the function scope of compatibility:  Operating Instructions → ■ 117.
System integration	Information regarding system integration: Operating Instructions → 🗎 117.  • Modbus RS485 information  • Function codes  • Register information  • Response time  • Modbus data map

#### Modbus TCP over Ethernet-APL

Port 1: Modbus TCP over Ethernet-APL 10 Mbit/s, SPE 10 Mbit/s	
Protocol	<ul><li>Modbus application protocol V1.1</li><li>TCP</li></ul>
Response times	On Modbus client request: Typically 3 to 5 ms
TCP port	502
Modbus TCP connections	Maximum 4
Communication type	Ethernet Advanced Physical Layer 10BASE-T1L
Data transfer	Full-duplex
Polarity	Automatic correction of crossed "APL signal + " and "APL signal -" signal lines
Device type	Address
Device type ID	0xC43B
Function codes	<ul> <li>03: Read holding register</li> <li>04: Read input register</li> <li>06: Write single registers</li> <li>16: Write multiple registers</li> <li>23: Read/write multiple registers</li> <li>43: Read device identification</li> </ul>
Broadcast support for function codes	<ul> <li>06: Write single registers</li> <li>16: Write multiple registers</li> <li>23: Read/write multiple registers</li> <li>43: Read device identification</li> </ul>
Supported transfer speed	10 Mbit/s (Ethernet-APL)
Supported features	Address can be configured using DHCP, web server or software
Device description files (FDI)	Information and files available at: www.endress.com → Downloads area
Configuration options for measuring instrument	<ul> <li>Asset management software (FieldCare, DeviceCare, Field Expert)</li> <li>Integrated web server via web browser and IP address</li> <li>Onsite operation</li> </ul>

Supported functions	<ul> <li>Device identification using:         Nameplate     </li> <li>Measured value status         The process variables are communicated with a measured value status     </li> <li>Blinking feature via the local display for simple device identification and assignment</li> <li>Device operation via asset management software (e.g. FieldCare, DeviceCare)</li> </ul>
System integration	Information regarding system integration: Operating Instructions → 🗎 117.  • Overview and description of the supported function codes  • Status coding  • Factory setting

Port 2: Modbus TCP over Ether	Port 2: Modbus TCP over Ethernet 100 Mbit/s	
Protocol	<ul><li>Modbus application protocol V1.1</li><li>TCP</li></ul>	
Response times	On Modbus client request: Typically 3 to 5 ms	
TCP port	502	
Modbus TCP connections	Maximum 4	
Communication type	■ 10BASE-T ■ 100BASE-TX	
Data transfer	Half-duplex, full-duplex	
Polarity	Auto-MDIX	
Device type	Address	
Device type ID	0xC43B	
Function codes	<ul> <li>03: Read holding register</li> <li>04: Read input register</li> <li>06: Write single registers</li> <li>16: Write multiple registers</li> <li>23: Read/write multiple registers</li> <li>43: Read device identification</li> </ul>	
Broadcast support for function codes	<ul> <li>06: Write single registers</li> <li>16: Write multiple registers</li> <li>23: Read/write multiple registers</li> <li>43: Read device identification</li> </ul>	
Supported transfer speed	■ 10 Mbit/s ■ 100 Mbit/s (Fast-Ethernet)	
Supported features	Address can be configured using DHCP, web server or software	
Device description files (FDI)	Information and files available at: www.endress.com → Downloads area	
Configuration options for measuring instrument	<ul> <li>Asset management software (FieldCare, DeviceCare, Field Expert)</li> <li>Integrated web server via web browser and IP address</li> <li>Onsite operation</li> </ul>	
Supported functions	<ul> <li>Device identification using:         Nameplate     </li> <li>Measured value status         The process variables are communicated with a measured value status     </li> <li>Device operation via asset management software (e.g. FieldCare, DeviceCare)</li> </ul>	
System integration	Information regarding system integration: Operating Instructions → 🗎 117.  Overview and description of the supported function codes  Status coding  Factory setting	

# EtherNet/IP

Protocol	<ul> <li>The CIP Networks Library Volume 1: Common Industrial Protocol</li> <li>The CIP Networks Library Volume 2: EtherNet/IP Adaptation of CIP</li> </ul>							
Communication type	■ 10Base-T ■ 100Base-TX							
Device profile	Generic device (product type: 0x2B)							
Manufacturer ID	0x000049E							
Device type ID	0x103B							
Baud rates	Automatic <sup>10</sup> / <sub>100</sub> Mbit with half-duplex and full-duplex detection							
Polarity	Auto-polarity for automatic correction of crossed TxD and RxD pairs							
Supported CIP connections	Max. 3 connections							
Explicit connections	Max. 6 connections							
I/O connections	Max. 6 connections (scanner)							
Configuration options for measuring device	<ul> <li>DIP switches on the electronics module for IP addressing</li> <li>Manufacturer-specific software (FieldCare)</li> <li>Add-on Profile Level 3 for Rockwell Automation control systems</li> <li>Web browser</li> <li>Electronic Data Sheet (EDS) integrated in the measuring device</li> </ul>							
Configuration of the EtherNet interface	<ul> <li>Speed: 10 MBit, 100 MBit, auto (factory setting)</li> <li>Duplex: half-duplex, full-duplex, auto (factory setting)</li> </ul>							
Configuration of the device address	<ul> <li>DIP switches on the electronics module for IP addressing (last octet)</li> <li>DHCP</li> <li>Manufacturer-specific software (FieldCare)</li> <li>Add-on Profile Level 3 for Rockwell Automation control systems</li> <li>Web browser</li> <li>EtherNet/IP tools, e.g. RSLinx (Rockwell Automation)</li> </ul>							
Device Level Ring (DLR)	Yes							
System integration	Information regarding system integration: Operating Instructions $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $							
	<ul><li>Cyclic data transmission</li><li>Block model</li><li>Input and output groups</li></ul>							

# PROFINET

Protocol	Application layer protocol for decentral device periphery and distributed automation, Version 2.3
Communication type	100 Mbit/s
Conformity class	Conformance class B
Netload Class	Netload Class 2 100 Mbit/s
Baud rates	Automatic 100 Mbit/s with full-duplex detection
Periods	From 8 ms
Polarity	Auto-polarity for automatic correction of crossed TxD and RxD pairs
Media Redundancy Protocol (MRP)	Yes
System redundancy support	System redundancy S2 (2 AR with 1 NAP)
Device profile	Application interface identifier 0xF600 Generic device
Manufacturer ID	0x11
Device type ID	0x843B

Device description files (GSD, DTM, DD)	Information and files available at:  ■ www.endress.com  On the product page for the device: Documents/Software → Device drivers  ■ www.profibus.com
Supported connections	<ul> <li>2 x AR (IO Controller AR)</li> <li>1 x AR (IO-Supervisor Device AR connection allowed)</li> <li>1 x Input CR (Communication Relation)</li> <li>1 x Output CR (Communication Relation)</li> <li>1 x Alarm CR (Communication Relation)</li> </ul>
Configuration options for measuring instrument	<ul> <li>DIP switches on the electronics module, for device name assignment (last part)</li> <li>Asset management software (FieldCare, DeviceCare, Field Xpert)</li> <li>Integrated web server via web browser and IP address</li> <li>Device master file (GSD), can be read out via the integrated web server of the measuring instrument.</li> <li>Onsite operation</li> </ul>
Configuration of the device name	<ul> <li>DIP switches on the electronics module, for device name assignment (last part)</li> <li>DCP protocol</li> <li>Asset management software (FieldCare, DeviceCare, Field Xpert)</li> <li>Integrated web server</li> </ul>
Supported functions	<ul> <li>Identification &amp; Maintenance, simple device identifier via:</li> <li>Control system</li> <li>Nameplate</li> <li>Measured value status         The process variables are communicated with a measured value status     </li> <li>Blinking feature via the local display for simple device identification and assignment</li> <li>Device operation via asset management software (e.g. FieldCare, DeviceCare, SIMATIC PDM)</li> </ul>
System integration	Information regarding system integration: Operating Instructions → 🖺 117.  Cyclic data transmission  Overview and description of the modules  Status coding  Startup configuration  Factory setting

# PROFINET over Ethernet-APL

Protocol	Application layer protocol for decentral device periphery and distributed automation, Version 2.43					
Communication type	Ethernet Advanced Physical Layer 10BASE-T1L					
Conformance Class	Conformance Class B (PA)					
Netload Class	PROFINET Netload Robustness Class 2 10 Mbit/s					
Data transfer	10 Mbit/s Full-duplex					
Cycle times	64 ms					
Polarity	Automatic correction of crossed "APL signal +" and "APL signal -" signal lines					
Media Redundancy Protocol (MRP)	Not possible (point-to-point connection to APL field switch)					
System redundancy support	System redundancy S2 (2 AR with 1 NAP)					
Device profile	PROFINET PA profile 4.02 (Application interface identifier API: 0x9700)					
Manufacturer ID	17					
Device type ID	0xA43B					
Device description files (GSD, DTM, FDI)	Information and files available at:  ■ www.endress.com → Downloads area  ■ www.profibus.com					

Supported connections	■ 2x AR (IO Controller AR)
	2x AR (IO Supervisor Device AR connection allowed)
Configuration options for measuring instrument	<ul> <li>DIP switches on the electronics module, for device name assignment (last part)</li> <li>Asset management software (FieldCare, DeviceCare, Field Xpert)</li> <li>Integrated Web server via Web browser and IP address</li> <li>Device master file (GSD), can be read out via the integrated Web server of the measuring instrument.</li> <li>Onsite operation</li> </ul>
Configuration of the device name	<ul> <li>DIP switches on the electronics module, for device name assignment (last part)</li> <li>DCP protocol</li> <li>Asset management software (FieldCare, DeviceCare, Field Xpert)</li> <li>Integrated web server</li> </ul>
Supported functions	<ul> <li>Identification &amp; Maintenance, simple device identifier via:</li> <li>Control system</li> <li>Nameplate</li> <li>Measured value status         The process variables are communicated with a measured value status     </li> <li>Blinking feature via the local display for simple device identification and assignment</li> <li>Device operation via asset management software (e.g. FieldCare, DeviceCare, SIMATIC PDM with FDI package)</li> </ul>
System integration	Information regarding system integration: Operating Instructions → 🗎 117.  Cyclic data transmission Overview and description of the modules Status coding Factory setting

# **Power supply**

Transmitter: supply voltage, input/outputs

# HART

Supply	Supply voltage		Input/output 1 (port 1)		Input/output 2		Input/output 3		output	Service interface (Port 2)		
1 (+)	2 (-)	26 (+)	27 (-)	24 (+)	25 (-)	22 (+)	23 (-)	20 (+)	21 (-)	CDI-RJ45		
				The tern	The terminal assignment depends on the specific device version ordered  → 🗎 15.							

1) Input/output only available for Proline 500 - digital.

# FOUNDATION fieldbus

Terminal assignment

Supply voltage		Input/output 1 (port 1)		Input/output 2		Input/output 3		Input/output 4 1)		Service interface (Port 2)		
1 (+)	2 (-)	26 (A)	27 (B)	24 (+)	25 (-)	22 (+)	23 (-)	20 (+)	21 (-)	CDI-RJ45		
				The term	The terminal assignment depends on the specific device version ordered $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $							

1) Input/output only available for Proline 500 - digital.

# PROFIBUS DP

Supply voltage		Input/output 1 (port 1)		Input/output 2		Input/output 3		Input/output 4 1)		Service interface (Port 2)	
1 (+)	2 (-)	26 (B)	27 (A)	24 (+)	25 (-)	22 (+)	23 (-)	20 (+)	21 (-)	CDI-RJ45	
				The term	The terminal assignment depends on the specific device version ordered $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $						

Input/output only available for Proline 500 - digital. 1)

#### PROFIBUS PA

Supp	oly voltage		Input/output 1 (port 1)		Input/output 2		Input/output 3		output	Service interface (Port 2)	
1 (+)	2 (-)	26 (B)	27 (A)	24 (+)	25 (-)	22 (+)	23 (-)	20 (+)	21 (-)	CDI-RJ45	
				The tern	The terminal assignment depends on the specific device version ordered $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $						

Input/output only available for Proline 500 - digital. 1)

# Modbus RS485

Supply voltage		Input/output 1 (port 1)		Input/output 2		Input/output 3		Input/output 4 1)		Service interface (Port 2)		
1 (+)	2 (-)	26 (B)	27 (A)	24 (+)	25 (-)	22 (+)	23 (-)	20 (+)	21 (-)	CDI-RJ45		
				The tern	The terminal assignment depends on the specific device version ordered $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $							

1) Input/output only available for Proline 500 - digital.

# Modbus TCP

Supply voltage Input/output 1 (Port 1 1)		Input/output 2		Input/	output 3		output (2)	Service interface (Port 2) <sup>1)</sup>		
1 (+)	2 (-)	26 (+)	27 (-)	24 (+)	25 (-)	22 (+)	23 (-)	20 (+)	21 (-)	CDI-RJ45
				The term	inal assignme					

- 1) For Modbus TCP communication, either port 1 OR port 2 can be used.
- Input/output only available for Proline 500 digital. 2)

# **PROFINET**

Supply	voltage	Input/output 1 (Port 1) <sup>1)</sup>	Input/output 2		Input/output 3		Input/output 4 <sup>2)</sup>		Service interface (Port 2) 1)		
1 (+)	2 (-)	RJ45	24 (+)	25 (-)	22 (+)	23 (-)	20 (+)	21 (-)	CDI-RJ45		
			The tern	The terminal assignment depends on the specific device version ordered $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $							

- Port can be used for communication or as a service interface (CDI-RJ45). Input/output only available for Proline 500 digital. 1)
- 2)

#### PROFINET over Ethernet-APL

Supply	y voltage	•	output 1 rt 1)	Input/	output 2	Input/	output 3	Input/	output	Service interface (Port 2 <sup>2)</sup> )
1 (+)	2 (-)	26 (+)	27 (-)	24 (+)	25 (-)	22 (+)	23 (-)	20 (+)	21 (-)	CDI-RJ45
				The tern	The terminal assignment depends on the specific d  → 🖺 15.		device version	ordered		

- 1) Input/output only available for Proline 500 digital.
- 2) No PROFINET communication available on port 2

# Ethernet/IP

Supply voltage		Input/output 1 (Port 1) <sup>1)</sup>	Input/	output 2	Input/	output 3		output	Service interface (Port 2) 1)
1 (+)	2 (-)	RJ45	24 (+)	25 (-)	22 (+)	23 (-)	20 (+)	21 (-)	CDI-RJ45
			The terminal assign			n the specific 15.	device versior	ordered	

- 1) Port can be used for communication or as a service interface (CDI-RJ45).
- 2) Input/output only available for Proline 500 digital.

#### Transmitter and sensor connection housing: connecting cable

The sensor and transmitter, which are mounted in separate locations, are interconnected by a connecting cable. The cable is connected via the sensor connection housing and the transmitter housing.

Terminal assignment and connection of the connecting cable:

- Proline 500 digital  $\rightarrow$  🖺 47
- Proline 500 → 🖺 48

# Available device plugs Proline 500



Device plugs may not be used in hazardous areas!

### Device plugs for Proline 500:

Order code for "Input; output 1"

- Option **SA** "FOUNDATION Fieldbus" → 🖺 41
- Option **GA** "PROFIBUS PA" → 🖺 41
- Option **NA** "EtherNet/IP" → 🖺 42
- Option **RA** "PROFINET" → 🖺 42
- Option **RB** "PROFINET over Ethernet-APL"  $\rightarrow$   $\stackrel{\triangle}{=}$  42
- Option **MB** "Modbus TCP" → 🖺 42

# Device plug for connecting to the service interface:

Order code for "Accessory mounted"

Option NB, RJ45 M12 adapter (service interface)  $\rightarrow$   $\stackrel{\triangle}{=}$  46

#### Order code for "Input; output 1", option SA "FOUNDATION fieldbus"

Order code for	Cable entry/connection → 🖺 48		
"Electrical connection"	2	3	
M, 3, 4, 5	7/8" plug	-	

# Order code for "Input; output 1", option GA "PROFIBUS PA"

Order code for	Cable entry/connection → 🖺 48		
"Electrical connection"	2	3	
L, N, P, U	Connector M12×1	-	

# Order code for "Input; output 1", option NA "EtherNet/IP"

Order code for	Cable entry/connection → 🗎 48			
"Electrical connection"	2	3		
L, N, P, U	Connector M12×1	-		
R <sup>1)2)</sup> S <sup>1)2)</sup> , T <sup>1)2)</sup> , V <sup>1)2)</sup>	Connector M12×1	Connector M12×1		

- Not compatible with an external WLAN antenna (order code for "Accessory enclosed", option P8), an RJ45 M12 adapter for the service interface (order code for "Accessory mounted", option NB)
- 2) Suitable for integrating the device into a ring topology.

# Order code for "Input; output 1", option RA "PROFINET"

Order code for	Cable entry/connection → 🖺 48			
"Electrical connection"	2	3		
L, N, P, U	Connector M12×1	-		
R <sup>1)2)</sup> , S <sup>1)2)</sup> , T <sup>1)2)</sup> , V <sup>1)2)</sup>	Connector M12×1	Connector M12×1		

- Not compatible with an external WLAN antenna (order code for "Accessory enclosed", option P8), an RJ45 M12 adapter for the service interface (order code for "Accessory mounted", option NB)
- 2) Suitable for integrating the device into a ring topology.

# Order code for "Input; output 1", option RB "PROFINET over Ethernet-APL"

Order code for	Cable entry/connection → 🗎 48			
"Electrical connection"	2	3		
L, N, P, U	Connector M12×1	-		

# Order code for "Input; output 1", option MB "Modbus TCP over Ethernet-APL"

Order code for	Accessories	Cable entry/connection → 🖺 48		
"Electrical connection"	Accessories	2	2 3  or M12×1 - coded  or M12×1   Connector M12×1 1) coded   D-coded   Connector M12×1	
L, N, P, U	-	Connector M12×1 A-coded	-	
L, N, P, U	NB <sup>1)</sup>	Connector M12×1 A-coded		
1 <sup>2)</sup> , 2 <sup>2)</sup> , 7 <sup>2)</sup> , 8 <sup>2)</sup>	-	-	Connector M12×1 D-coded	

- 1) Cannot be used as a Modbus TCP port.
- Not compatible with an external WLAN antenna (order code for "Accessory enclosed", option P8, an RJ45 M12 adapter for the service interface (order code for "Accessory mounted", option NB)

# Order code for "Accessory mounted", option NB: "Adapter RJ45 M12 (service interface)"

Order code for	Cable entry/connection → 🖺 48		
"Accessory mounted"	Cable entry 2	Cable entry 3	
NB 1)	-	Connector M12×1	

1) Not compatible with electrical connection option 1, 2, 7, 8  $\,$ 

# Available device plugs Proline 500 digital

#### Device plugs for Proline 500 digital:

Order code for "Input; output 1"

- Option **SA** "FOUNDATION Fieldbus" → 🖺 41
- Option **GA** "PROFIBUS PA" → 🖺 41
- Option **NA** "Ethernet/IP"  $\rightarrow$  🖺 42
- Option **RA** "PROFINET" → 🖺 42
- Option **RB** "PROFINET over Ethernet-APL"  $\rightarrow$   $\stackrel{\triangle}{=}$  42

### • Option MB "Modbus TCP over Ethernet-APL"

# Device plug for connecting to the service interface:

Order code for "Accessory mounted"

Option NB, RJ45 M12 adapter (service interface) → 

46

### Order code for "Input; output 1", option SA "FOUNDATION fieldbus"

Order code for		Cable entry/connection → 🖺 48			
"Electrical connection"	2	3	4	4 5	
M, 3, 4, 5	-	7/8" connector	-	-	

# Order code for "Input; output 1", option GA "PROFIBUS PA"

Order code for		Cable entry/con	nection → 🖺 48	
"Electrical connection"	2	3	4	5
L, N, P, U	_	Connector M12×1	_	_

# Order code for "Input; output 1", option NA "Ethernet/IP"

Order code for	Cable entry/connection → 🗎 48				
"Electrical connection"	2	3	4	5	
L, N, P, U	Connector M12×1	-	_	_	
R <sup>1) 2)</sup> , S <sup>1) 2)</sup> , T <sup>1) 2)</sup> , V <sup>1) 2)</sup>	Connector M12×1	-	-	Connector M12×1	

Not compatible with an external WLAN antenna (order code for "Accessory enclosed", option P8), an RJ45 M12 adapter for the service interface (order code for "Accessory mounted", option NB)

# Order code for "Input; output 1", option RA "PROFINET"

Order code for	Cable entry/connection → 🖺 48							
"Electrical connection"	2	3	4	5				
L, N, P, U	Connector M12×1	_	_	-				
R <sup>1) 2)</sup> , S <sup>1) 2)</sup> , T <sup>1) 2)</sup> , V <sup>1) 2)</sup>	Connector M12×1	-	-	Connector M12×1				

Not compatible with an external WLAN antenna (order code for "Accessory enclosed", option P8), an RJ45 M12 adapter for the service interface (order code for "Accessory mounted", option NB)

2) Suitable for integrating the device into a ring topology.

<sup>2)</sup> Suitable for integrating the device into a ring topology.

# Order code for "Input; output 1", option RB "PROFINET over Ethernet-APL"

Order code for	Cable entry/connection → 🗎 48					
"Electrical connection"	2	3	4	5		
L, N, P, U	-	Connector M12×1 A-coded	-	-		

# Order code for "Input; output 1", option MB "Modbus TCP over Ethernet-APL"

Order code for		Cable entry/connection → 🗎 48					
"Electrical connection"	Accessories	2	3	4	5		
L, N, P, U	-	-	Connector M12×1 A-coded	-	-		
L, N, P, U	NB 1)	-	Connector M12×1 A-coded	-	Connector M12×1 <sup>1)</sup> D-coded		
1 2), 2 2), 7 2), 8 2)	-	-	-	-	Connector M12×1 D-coded		

- 1) Cannot be used as a Modbus TCP port.
- Not compatible with an external WLAN antenna (order code for "Accessory enclosed", option P8, an RJ45 M12 adapter for the service interface (order code for "Accessory mounted", option NB)

# Order code for "Accessory mounted", option NB: "Adapter RJ45 M12 (service interface)"

Order code for		Cable entry/connection → 🗎 48					
"Electrical connection"	2	3	4	5			
NB 1)	-	-	-	M12x1 plug D-coded			

1) Not compatible with electrical connection option 1, 2, 7, 8

# Pin assignment, device plug

# **FOUNDATION Fieldbus**

	Pin		Assignment	Coding	Plug/socket
2 3	1	+	Signal +	А	Plug
1 4	2	-	Signal –		
	3		Cable shield <sup>1</sup>		
	4		Not used		
	Metal plug housing		Cable shield		
		<sup>1</sup> If a cable shield is used			

# **PROFIBUS PA**

	Pin		Assignment	Coding	Plug/socket
2 3	1	+	PROFIBUS PA +	A	Plug
1 4	2		Grounding		
	3	-	PROFIBUS PA -		

4	Not used	
Met al	Cable shield	
plug hous ing		

# Recommended plug:

- Binder, series 713, part no. 99 1430 814 04
- Phoenix, part no. 1413934 SACC-FS-4QO SH PBPA SCO


#### **PROFINET**

2	Pin		Assignment	Coding	Plug/socket
	1	+	TD +	D	Socket
1 3	2	+	RD +		
	3	-	TD -		
	4	-	RD -		
4 A0032047					
	Metal plug housing		Cable shield		

# Recommended plug:

- Binder, series 825, part no. 99 3729 810 04
- Phoenix, part no. 1543223 SACC-M12MSD-4Q


# PROFINET over Ethernet-APL

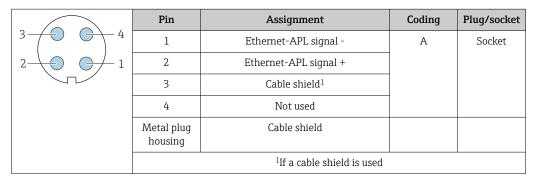

# Recommended plug:

- Binder, series 713, part no. 99 1430 814 04
- Phoenix, part no. 1413934 SACC-FS-4QO SH PBPA SCO

# Modbus TCP over Ethernet-APL 10 Mbit/s

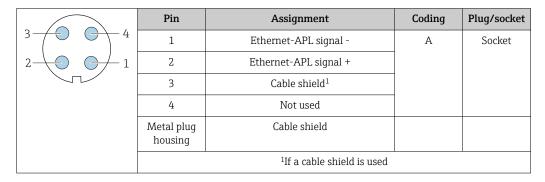

- Recommended plug:
  Binder, series 713, part no. 99 1430 814 04
  - Phoenix, part no. 1413934 SACC-FS-4QO SH PBPA SCO

# Modbus TCP over Ethernet 100 Mbit/s

2	Pin		Assignment	Coding	Plug/socket
	1	+	Tx	D	Socket
1 3	2	+	Rx		
	3	-	Tx		
	4	-	Rx		
4 A0032047					

# EtherNet/IP

2	Pin		Assignment	Coding	Plug/socket
	1	+	Tx	D	Socket
1 3	2	+	Rx		
	3	-	Tx		
	4	-	Rx		
4 A0032047					
	Met al		Cable shield		
	plug hous ing				

- Recommended plug:
  Binder, series 825, part no. 99 3729 810 04
  - Phoenix, part no. 1543223 SACC-M12MSD-4Q

#### Service interface

Order code for "Accessory mounted", option NB: "Adapter RJ45 M12 (service interface)"

2	Pin		Assignment	Coding	Plug/socket
	1	+	Tx	D	Socket
1 3	2	+	Rx		
	3	-	Tx		
	4	-	Rx		
4 A0032047					

- Recommended plug:
  Binder, series 825, part no. 99 3729 810 04
  - Phoenix, part no. 1543223 SACC-M12MSD-4Q

# Supply voltage

Order code for "Power supply"	Terminal voltage		Frequency range
Option <b>D</b>	DC 24 V	±20%	_
Option E	AC 100 to 240 V	-15 to 10%	50/60 Hz
Option I	DC 24 V	±20%	-
Option I	AC 100 to 240 V	-15 to 10%	50/60 Hz

# Power consumption

#### Transmitter

Max. 10 W (active power)

switch-on current	Max. 36 A (<5 ms) as per NAMUR Recommendation NE 21
-------------------	---

#### **Current consumption**

#### Transmitter

- Max. 400 mA (24 V)
- Max. 200 mA (110 V, 50/60 Hz; 230 V, 50/60 Hz)

# Power supply failure

- Totalizers stop at the last value measured.
- Depending on the device version, the configuration is retained in the device memory or in the plug-in memory (HistoROM DAT).
- Error messages (incl. total operated hours) are stored.


# Overcurrent protection element

The device must be operated with a dedicated circuit breaker, as it does not have an ON/OFF switch of its own.

- The circuit breaker must be easy to reach and labeled accordingly.
- Permitted nominal current of the circuit breaker: 2 A up to maximum 10 A.

#### **Electrical connection**

# Connection of connecting cable: Proline 500 - digital

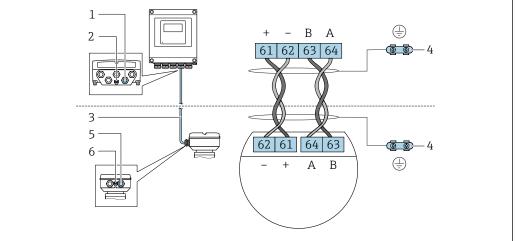

A002819

- 1 Cable entry for cable on transmitter housing
- 2 Protective ground connection (PE)
- 3 Connecting cable ISEM communication
- 4 Grounding via ground connection; in the version with a device plug, grounding is ensured through the plug itself
- 5 Cable entry for cable or connection of device plug on sensor connection housing
- 6 Protective ground connection (PE)

Depending on the device version of the sensor connection housing, the connecting cable is connected via terminals or device plugs.

Sensor connection housing Order code for "Housing"	Connection to sensor connection housing via	Connection to transmitter housing via
Option <b>A</b> : aluminum coated	Terminals	Terminals
Option <b>B</b> : stainless	Terminals	Terminals
Option <b>C</b> : ultra-compact, hygienic, stainless	Device plug	Terminals
Option <b>L</b> : cast, stainless	Terminals	Terminals

Pin assignment, device plug

Device plugs are only available for device version, order code for "Housing":

Option C: ultra-compact, hygienic, stainless

For connection to sensor connection housing.


2	Pin	Color 1)		Assignment	Connection to terminal
	1	Brown	+	Supply voltage	61
3 0 0 0 1	2	White	A	ISEM communication	64
_5	3	Blue	В		63
4	4	Black	-	Supply voltage	62
	5	-		-	-
	Coding			Plug/socket	
	A			Plug	

1) Cable colors of connecting cable



# Connection of the connecting cable: Proline 500

The connecting cable is connected via terminals.

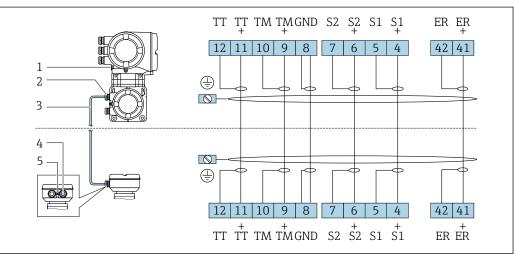


A002819

- 1 Protective ground connection (PE)
- 2 Cable entry for connecting cable on transmitter connection housing
- 3 Connecting cable
- 4 Cable entry for connecting cable on sensor connection housing
- 5 Protective ground connection (PE)

# **Transmitter connection**

### Transmitter connection: Proline 500 - digital

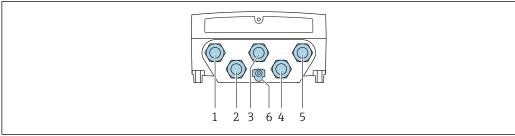


A0028200

- 1 Terminal connection for supply voltage
- 2 Terminal connection for signal transmission, input/output
- 3 Terminal connection for signal transmission, input/output
- 4 Terminal connection for connecting cable between sensor and transmitter
- 5 Terminal connection for signal transmission, input/output or terminal for network connection (DHCP client) via service interface (CDI-RJ45); optional: terminal connection for external WLAN antenna
- 6 Protective ground connection (PE)
- An adapter for the RJ45 to the M12 plug is optionally available:
  Order code for "Accessories", option **NB**: "Adapter RJ45 M12 (service interface)"

The adapter connects the service interface (CDI-RJ45) to an M12 plug mounted in the cable entry. The connection to the service interface can be established via an M12 plug without opening the device.

Connecting the transmitter: Proline 500

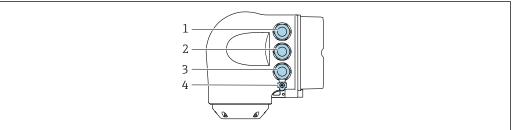

A0026781

- 1 Terminal connection for supply voltage
- 2 Terminal connection for signal transmission, input/output
- 3 Terminal connection for signal transmission, input/output or terminal for network connection (DHCP client) via service interface (CDI-RJ45); optional: terminal connection for external WLAN antenna
- 4 Protective ground connection (PE)
- An adapter for the RJ45 to the M12 plug is optionally available:
  Order code for "Accessories", option **NB**: "Adapter RJ45 M12 (service interface)"

The adapter connects the service interface (CDI-RJ45 to an M12 plug mounted in the cable entry. The connection to the service interface can be established via an M12 plug without opening the device.

# Connecting in a ring topology


Device versions with EtherNet/IP and PROFINET communication protocols can be integrated into a ring topology. The device is integrated via the terminal connection for signal transmission (output 1) and the connection to the service interface (CDI-RJ45).

For detailed information on connecting transmitters with an Ex de approval, see separate document "Safety instructions" (XA) for the device.

Integrating the transmitter into a ring topology:

EtherNet/IPPROFINET


Transmitter: Proline 500 - digital

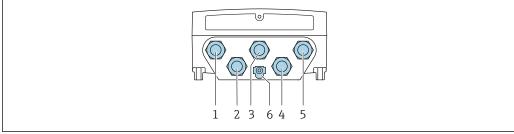

A0028200

- 1 Terminal connection for supply voltage
- 2 Terminal connection for signal transmission, input/output
- 2 Terminal connection for signal transmission: PROFINET or Ethernet/IP (RJ45 plug)
- 4 Terminal connection for connecting cable between sensor and transmitter
- 5 Connection to service interface (CDI-RJ45)
- 6 Protective ground connection (PE)

Transmitter: Proline 500

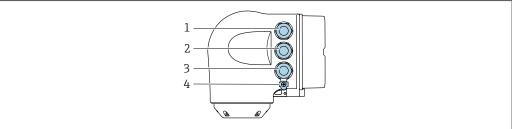

A002678


- 1 Terminal connection for supply voltage
- 2 Terminal connection for signal transmission: PROFINET or Ethernet/IP (RJ45 plug)
- 3 Connection to service interface (CDI-RJ45)
- 4 Protective ground connection (PE)

If the device has additional inputs/outputs, these are routed in parallel via the cable entry for connection to the service interface (CDI-RJ45).

50


# **Connection examples**

Current output 4 to 20 mA (without HART)

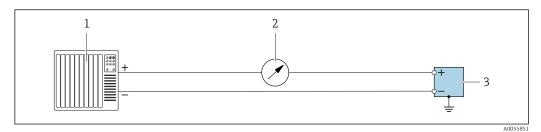


**₽** 2 Connection example for 4 to 20 mA current output (active)

- Automation system with current input (e.g. PLC)
- 2 Optional additional display unit: Observe maximum load
- Flowmeter with current output (active)

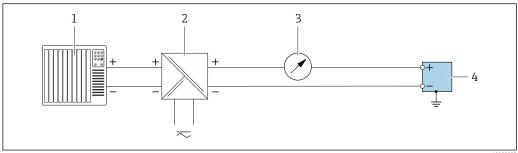


- ₩ 3 Connection example for 4 to 20 mA current output (passive)
- Automation system with current input (e.g. PLC)
- 2 Power supply
- Optional additional display unit: Observe maximum load
- Transmitter with current output (passive)

# Current input 4 to 20 mA

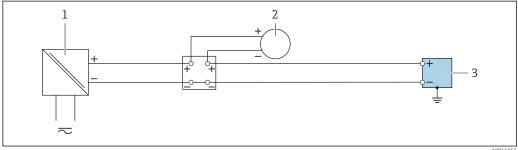


- € 4 Connection example for 4 to 20 mA current input
- Power supply
- External measuring instrument with 4 to 20 mA passive current output. e.g. pressure or temperature)
- Transmitter with 4 to 20 mA current input

# *Pulse output/frequency output/switch output*

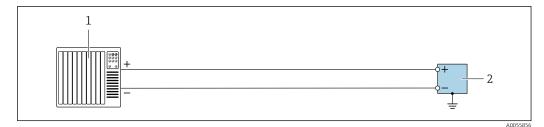

■ 5 Connection example for pulse output/frequency output/switch output (active)


- 1 Automation system with pulse input/frequency input/switch input (e.g. PLC)
- 2 Transmitter with pulse output/frequency output/switch output (active)

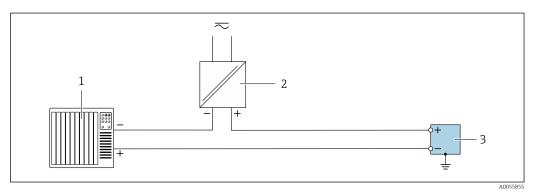

 $\blacksquare$  6 Connection example for pulse output/frequency output/switch output (passive)

- 1 Automation system with pulse input/frequency input/switch input (e.g. PLC)
- 2 Power supply
- 3 Transmitter with pulse output/frequency output/switch output (passive)


# Relay output

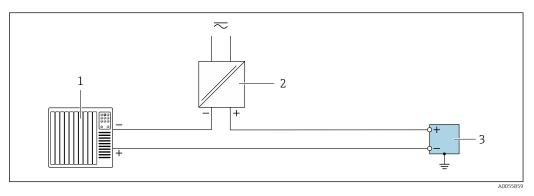

 $\blacksquare$  7 Connection example for relay output

- 1 Automation system with switch input (e.g. PLC)
- 2 Power supply
- 3 Transmitter with relay output


# Status input

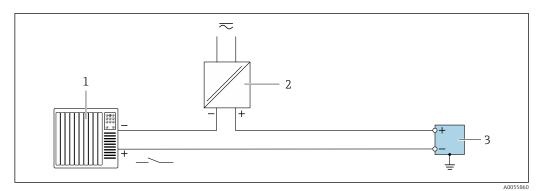

■ 8 Connection example for status input


- 1 Automation system with switch output passive e.g. PLC)
- 2 Power supply
- 3 Transmitter with status input

# Current output 4 to 20 mA HART

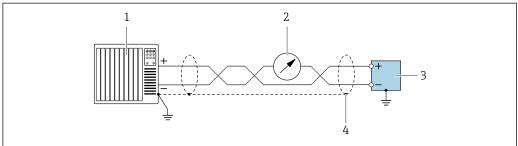

A0055862


- 9 Connection example for 4 to 20 mA current output with HART (active)
- 1 Automation system with 4 to 20 mA current input with HART (e.g. PLC)
- 2 Optional display unit: Note maximum load
- *Transmitter with 4 to 20 mA current output with HART (active)*
- 4 Ground cable shield at one end. For installations in compliance with NAMUR NE 89, grounding of the cable shield on both sides is required.

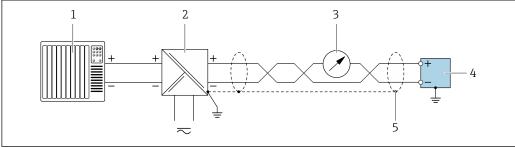

A005586

- 10 Connection example for 4 to 20 mA current output with HART (passive)
- 1 Automation system with 4 to 20 mA current input with HART (e.g. PLC)
- 2 Power supply
- 3 Optional display unit: Note maximum load
- 4 Transmitter with 4 to 20 mA current output with HART (passive)
- Ground cable shield at one end. For installations in compliance with NAMUR NE 89, grounding of the cable shield on both sides is required.

# Modbus RS485

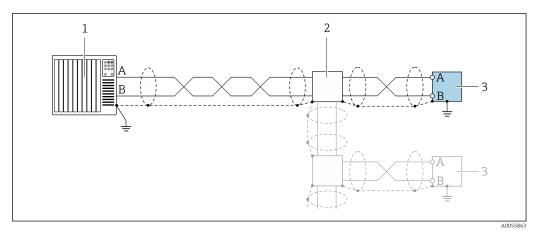

■ 11 Connection example for Modbus RS485

- Automation system with Modbus master (e.g. PLC)
- 2 Optional distribution box
- Transmitter with Modbus RS485

# PROFIBUS PA




See https://www.profibus.com "PROFIBUS Installation Guidelines".

# PROFIBUS DP



See https://www.profibus.com "PROFIBUS Installation Guidelines".

#### FOUNDATION Fieldbus

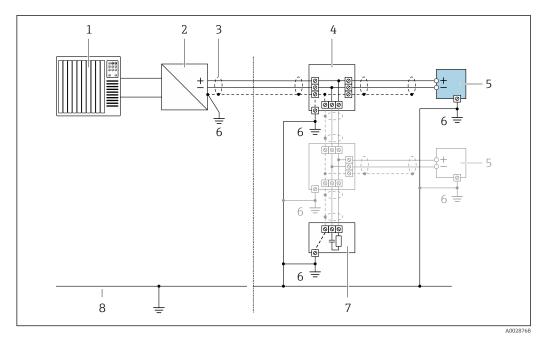

12 Connection example for FOUNDATION Fieldbus

- 1 Automation system (e.g. PLC)
- 2 Power Conditioner (FOUNDATION Fieldbus)
- 3 Cable shield provided at one end. The cable shield must be grounded at both ends to comply with EMC requirements; observe cable specifications
- 4 T-box
- 5 Measuring instrument
- 6 Local grounding
- 7 Bus terminator
- 8 Potential equalization conductor

#### **PROFINET**



See https://www.profibus.com "PROFINET Planning guideline".

### EtherNet/IP



See https://www.odva.org"EtherNet/IP Media Planning & Installation Manual".

# Ethernet-APL



See https://www.profibus.com Ethernet-APL White Paper "

### Potential equalization

### Requirements

For potential equalization:

- Pay attention to in-house grounding concepts
- Take account of operating conditions like the pipe material and grounding
- Connect the medium, sensor and transmitter to the same electric potential
- $\blacksquare$  Use a ground cable with a minimum cross-section of 6 mm  $^2$  (10 AWG) and a cable lug for potential equalization connections

# Terminals

Spring-loaded terminals: Suitable for strands and strands with ferrules. Conductor cross-section 0.2 to 2.5 mm $^2$  (24 to 12 AWG).

#### Cable entries

- Cable gland: M20 × 1.5 with cable Ø 6 to 12 mm (0.24 to 0.47 in)
- Thread for cable entry:
  - NPT 1/2"
  - G 1/2"
  - M20
- Device plug for digital communication: M12 Only available for certain device versions  $\rightarrow \triangleq 41$ .
- Device plug for connecting cable: M12

A device plug is always used for the device version with the order code for "Sensor connection housing", option **C** "Ultra-compact, hygienic, stainless".

#### Cable specification

#### Permitted temperature range

- The installation guidelines that apply in the country of installation must be observed.
- The cables must be suitable for the minimum and maximum temperatures to be expected.

# Power supply cable (incl. conductor for the inner ground terminal)

Standard installation cable is sufficient.

# Protective grounding cable for the outer ground terminal

Conductor cross-section < 6 mm<sup>2</sup> (10 AWG)

Larger cross-sections can be connected using a cable lug.

The grounding impedance must be less than 2  $\Omega$ .

#### Signal cable

4 to 20 mA current input

Standard installation cable is sufficient.

Pulse/frequency/switch output

Standard installation cable is sufficient.

Relay output

Standard installation cable is sufficient.

Status input

Standard installation cable is sufficient.

Current output 4 to 20 mA HART

Shielded twisted-pair cable.



See https://www.fieldcommgroup.org "HART PROTOCOL SPECIFICATIONS".

### Modbus RS485

Shielded twisted-pair cable.



 $See \ https://modbus.org \ "MODBUS \ over Serial \ Line \ Specification \ and \ Implementation \ Guide".$ 

#### PROFIBUS PA

Shielded twisted-pair cable. Cable type A is recommended.



See https://www.profibus.com "PROFIBUS Installation Guidelines".

#### PROFIBUS DP

Shielded twisted-pair cable. Cable type A is recommended.



See https://www.profibus.com "PROFIBUS Installation Guidelines".

#### **PROFINET**

Only PROFINET cables.



See https://www.profibus.com "PROFINET Planning guideline".

# EtherNet/IP

Twisted-pair Ethernet CAT 5 or better.



 $See \ \ https://www.odva.org'' Ether Net/IP\ Media\ Planning\ \&\ Installation\ Manual''.$ 

#### Ethernet-APL

Shielded twisted-pair cable. Cable type A is recommended.



See https://www.profibus.com Ethernet-APL White Paper "

#### FOUNDATION Fieldbus

Twisted, shielded two-wire cable.




For further information on planning and installing FOUNDATION Fieldbus networks see:

- Operating Instructions for "FOUNDATION Fieldbus Overview" (BA00013S)
- FOUNDATION Fieldbus Guideline
- IEC 61158-2 (MBP)

# Choice of connecting cable between the transmitter and sensor

Depends on the type of transmitter and the installation zones

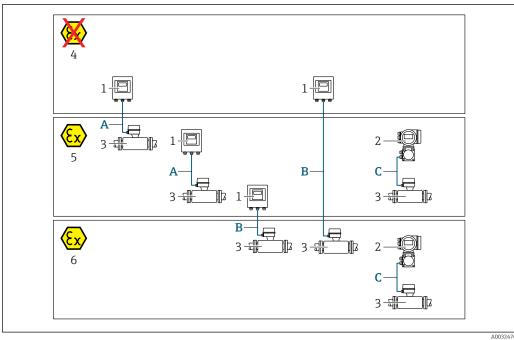

- Proline 500 digital transmitter 1
- Proline 500 transmitter 2
- 3 Sensor Cubemass
- 4 Non-hazardous area
- 5 Hazardous area: Zone 2; Class I, Division 2
- Hazardous area: Zone 1; Class I, Division 1 6
- Standard cable to 500 digital transmitter  $\rightarrow \implies 58$ Transmitter installed in the non-hazardous area or hazardous area: Zone 2; Class I, Division 2/sensor installed in the hazardous area: Zone 2; Class I, Division 2
- Standard cable to 500 digital transmitter  $\rightarrow \implies 59$ В Transmitter installed in the hazardous area: Zone 2; Class I, Division 2/sensor installed in the hazardous area: Zone 1; Class I, Division 1
- Signal cable to 500 transmitter  $\rightarrow \triangleq 61$ Transmitter and sensor installed in the hazardous area: Zone 2; Class I, Division 2 or Zone 1; Class I, Division 1

# A: Connecting cable between sensor and transmitter: Proline 500 – digital

# Standard cable

A standard cable with the following specifications can be used as the connecting cable.

Design	4 cores (2 pairs); uninsulated stranded CU wires; pair-stranded with common shield	
Shield	Tin-plated copper braid, optical cover $\geq$ 85 %	
Loop resistance	Power supply line (+, –): maximum 10 $\Omega$	
Cable length	Maximum 300 m (900 ft), see the following table.	
Device plug, side 1	M12 socket, 5-pin, A-coded.	
Device plug, side 2	M12 plug, 5-pin, A-coded.	
Pins 1+2	Connected cores as twisted pair.	
Pins 3+4	Connected cores as twisted pair.	

Cross-section	Cable length [max.]
0.34 mm <sup>2</sup> (AWG 22)	80 m (240 ft)
0.50 mm <sup>2</sup> (AWG 20)	120 m (360 ft)
0.75 mm <sup>2</sup> (AWG 18)	180 m (540 ft)

58

Cross-section	Cable length [max.]
1.00 mm <sup>2</sup> (AWG 17)	240 m (720 ft)
1.50 mm <sup>2</sup> (AWG 15)	300 m (900 ft)

# Optionally available connecting cable

Design	$2 \times 2 \times 0.34 \text{ mm}^2$ (AWG 22) PVC cable $^{1)}$ with common shield (2 pairs, uninsulated stranded CU wires; pair-stranded)	
Flame resistance	According to DIN EN 60332-1-2	
Oil resistance	According to DIN EN 60811-2-1	
Shield	Tin-plated copper braid, optical cover $\geq$ 85 %	
Continuous operating temperature	When mounted in a fixed position: $-50$ to $+105$ °C ( $-58$ to $+221$ °F); when cable can move freely: $-25$ to $+105$ °C ( $-13$ to $+221$ °F)	
Available cable length	Fixed: 20 m (60 ft); variable: up to maximum 50 m (150 ft)	


1) UV radiation can impair the cable outer sheath. Protect the cable from direct sunshine where possible.

B: Connecting cable between sensor and transmitter: Proline 500-digital

# Standard cable

A standard cable with the following specifications can be used as the connecting cable.

Design	4, 6, 8 cores (2, 3, 4 pairs); uninsulated stranded CU wires; pair-stranded with common shield	
Shielding	Tin-plated copper braid, optical cover ≥ 85 %	
Capacitance C	Maximum 760 nF IIC, maximum 4.2 μF IIB	
Inductance L	Maximum 26 μH IIC, maximum 104 μH IIB	
Inductance/resistance ratio (L/R)	Maximum 8.9 $\mu H/\Omega$ IIC, maximum 35.6 $\mu H/\Omega$ IIB (e.g. according to IEC 60079-25)	
Loop resistance	Power supply line (+, $-$ ): maximum 5 $\Omega$	
Cable length	Maximum 150 m (450 ft), see the following table.	

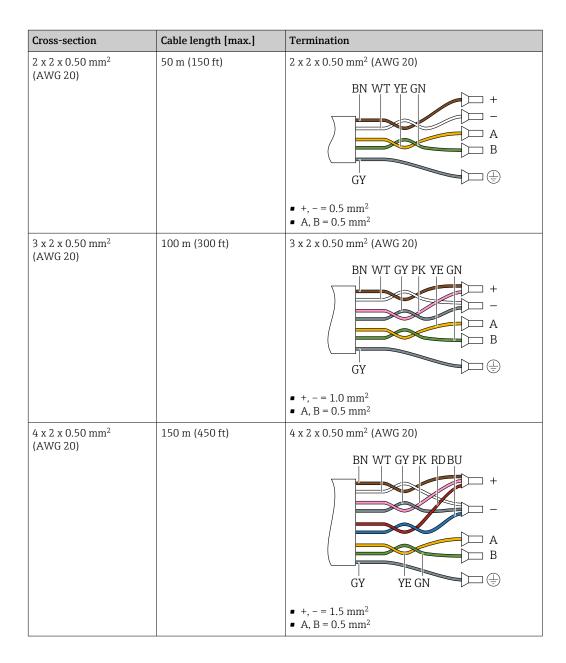

# Optionally available connecting cable

Connecting cable for	Zone 1; Class I, Division 1
Standard cable	$2\times2\times0.5~\text{mm}^2$ (AWG 20) PVC cable $^{1)}$ with common shield (2 pairs, pairstranded)
Flame resistance	According to DIN EN 60332-1-2
Oil-resistance	According to DIN EN 60811-2-1
Shielding	Tin-plated copper braid, optical cover ≥ 85 %
Operating temperature	When mounted in a fixed position: $-50$ to $+105$ °C ( $-58$ to $+221$ °F); when cable can move freely: $-25$ to $+105$ °C ( $-13$ to $+221$ °F)
Available cable length	Fixed: 20 m (60 ft); variable: up to maximum 50 m (150 ft)

1) UV radiation can impair the cable outer sheath. Protect the cable from direct sunshine where possible.

60

C: Connecting cable between sensor and transmitter: Proline 500

Design	$6\times0.38~\text{mm}^2$ PVC cable $^{1)}$ with individual shielded cores and common copper shield
Conductor resistance	$\leq$ 50 $\Omega$ /km (0.015 $\Omega$ /ft)
Capacitance: core/shield	≤ 420 pF/m (128 pF/ft)
Cable length (max.)	20 m (60 ft)
Cable lengths (available for order)	5 m (15 ft), 10 m (30 ft), 20 m (60 ft)
Cable diameter	11 mm (0.43 in) ± 0.5 mm (0.02 in)
Continuous operating temperature	Max. 105 °C (221 °F)

1) UV radiation can impair the cable outer sheath. Protect the cable from direct sunshine where possible.

# Overvoltage protection

Mains voltage fluctuations	→ 🖺 46	
Overvoltage category	Overvoltage category II	
Short-term, temporary overvoltage	Between cable and ground up to 1200 V, for max. 5 s	
Long-term, temporary overvoltage	Between cable and ground up to 500 V	

# Performance characteristics

# Reference operating conditions

- Error limits based on ISO 11631
- Water
  - +15 to +45 °C (+59 to +113 °F)
  - 2 to 6 bar (29 to 87 psi)
- Data as indicated in the calibration protocol
- Accuracy based on accredited calibration rigs according to ISO 17025



# Maximum measurement error

o.r. = of reading;  $1 \text{ g/cm}^3 = 1 \text{ kg/l}$ ; T = medium temperature

#### Base accuracy



Design fundamentals → 🖺 64

Mass flow and volume flow (liquids)

±0.10 % o.r.

Mass flow (gases)

±0.50 % o.r.

Density (liquids)

Under reference conditions	Standard density calibration 1)	Wide-range Density specification <sup>2) 3)</sup>
[g/cm³]	[g/cm³]	[g/cm³]
±0.0005	±0.02	±0.002

- 1) Valid over the entire temperature and density range
- Valid range for special density calibration: 0 to 2  $g/cm^3$ , +5 to +80  $^{\circ}$ C (+41 to +176  $^{\circ}$ F)
- 3) order code for "Application package", option EE "Special density"

# Temperature

 $\pm 0.5 \,^{\circ}\text{C} \pm 0.005 \cdot \text{T} \,^{\circ}\text{C} \, (\pm 0.9 \,^{\circ}\text{F} \pm 0.003 \cdot (\text{T} - 32) \,^{\circ}\text{F})$ 

# Zero point stability

DN		Zero point stability		
[mm] [in]		[kg/h]	[lb/min]	
1	1/24	0.0008	0.00003	
2	1/12	0.002	0.00007	
4	1/8	0.014	0.0005	
6	1/4	0.02	0.0007	

# Flow values

Flow values as turndown parameters depending on nominal diameter.

# SI units

DN	1:1	1:10	1:20	1:50	1:100	1:500
[mm]	[kg/h]	[kg/h]	[kg/h]	[kg/h]	[kg/h]	[kg/h]
1	20	2	1	0.4	0.2	0.04
2	100	10	5	2	1	0.2
4	450	45	22.5	9	4.5	0.9
6	1000	100	50	20	10	2

# US units

DN	1:1	1:10	1:20	1:50	1:100	1:500
[inch]	[lb/min]	[lb/min]	[lb/min]	[lb/min]	[lb/min]	[lb/min]
1/24	0.735	0.074	0.037	0.015	0.007	0.001
1/12	3.675	0.368	0.184	0.074	0.037	0.007
1/8	16.54	1.654	0.827	0.331	0.165	0.033
1/4	36.75	3.675	1.838	0.735	0.368	0.074

# Accuracy of outputs

The outputs have the following base accuracy specifications:

# Current output

Accuracy	+5 ^
Accuracy	± λ μν

# Pulse/frequency output

o.r. = of reading

Accuracy	Max. ±50 ppm o.r. (over the entire ambient temperature range)
----------	---

# Repeatability

o.r. = of reading;  $1 \text{ g/cm}^3 = 1 \text{ kg/l}$ ; T = medium temperature

### Base repeatability



Design fundamentals → 🖺 64

Mass flow and volume flow (liquids)

±0.05 % o.r.

Mass flow (gases)

±0.25 % o.r.

Density (liquids)

 $\pm 0.00025 \text{ g/cm}^3$ 

**Temperature** 

 $\pm 0.25 \,^{\circ}\text{C} \pm 0.0025 \cdot \text{T} \,^{\circ}\text{C} \, (\pm 0.45 \,^{\circ}\text{F} \pm 0.0015 \cdot (\text{T}-32) \,^{\circ}\text{F})$ 

#### Response time

The response time depends on the configuration (damping).

# Influence of ambient temperature

#### **Current output**

Temperature coefficient	Max. 1 μA/°C
-------------------------	--------------

#### Pulse/frequency output

Temperature coefficient	No additional effect. Included in accuracy.
-------------------------	---

# Influence of medium temperature

### Mass flow

o.f.s. = of full scale value


If there is a difference between the temperature during zero adjustment and the process temperature, the additional measurement error of the sensors is typically ±0.0002 %o.f.s./°C (±0.0001 % o. f.s./°F).

The influence is reduced when the zero adjustment is performed at process temperature.

• If there is a difference between the density calibration temperature and the process temperature, the measurement error of the sensors is typically  $\pm 0.00005$  g/cm<sup>3</sup>/°C ( $\pm 0.000025$  g/cm<sup>3</sup>/°F). Field density adjustment is possible.

#### Wide-range density specification (special density calibration)

If the process temperature is outside the valid range ( $\rightarrow \triangleq 61$ ) the measurement error is  $\pm 0.00005 \text{ g/cm}^3 \text{ /°C } (\pm 0.000025 \text{ g/cm}^3 \text{ /°F})$ 

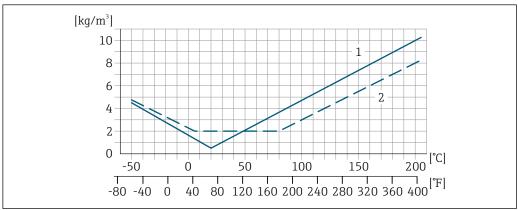

- Field density adjustment, for example at +20 °C (+68 °F)
- Special density calibration

# **Temperature**

 $\pm 0.005 \cdot \text{T} \,^{\circ}\text{C} \, (\pm 0.005 \cdot (\text{T} - 32) \,^{\circ}\text{F})$ 

# Influence of medium pressure

The following shows how the process pressure (gauge pressure) affects the accuracy of the mass flow.

o.r. = of reading



It is possible to compensate for the effect by:

- Reading in the current pressure measured value via the current input or a digital input.
- Specifying a fixed value for the pressure in the device parameters.



DN		[% o.r./bar]	[% o.r./psi]
[mm]	[in]		
1	1/24	-0.001	-0.00007
2	1/12	0	0
4	1/8	-0.005	-0.0004
6	1/4	-0.003	-0.0002

#### Design fundamentals

o.r. = of reading, o.f.s. = of full scale value

BaseAccu = base accuracy in % o.r., BaseRepeat = base repeatability in % o.r.

MeasValue = measured value; ZeroPoint = zero point stability


Calculation of the maximum measured error as a function of the flow rate

Flow rate	Maximum measured error in % o.r.
$\geq \frac{\text{ZeroPoint}}{\text{BaseAccu}} \cdot 100$	± BaseAccu
A0021332	1002355
< ZeroPoint · 100	$\pm \frac{\text{ZeroPoint}}{\text{MeasValue}} \cdot 100$
A0021333	A0021334

Calculation of the maximum repeatability as a function of the flow rate

Flow rate	Maximum repeatability in % o.r.
$\geq \frac{\frac{1}{2} \cdot ZeroPoint}{BaseRepeat} \cdot 100$	± BaseRepeat
A0021335	1002270
$<\frac{\frac{1}{2} \cdot ZeroPoint}{BaseRepeat} \cdot 100$	$\pm \frac{1}{2} \cdot \frac{\text{ZeroPoint}}{\text{MeasValue}} \cdot 100$
A0021336	A0021337


# Example of maximum measurement error

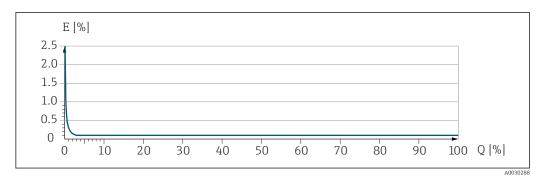

- E Maximum measurement error in % o.r. (example)
- Q Flow rate in % of maximum full scale value

# Installation

# Mounting location

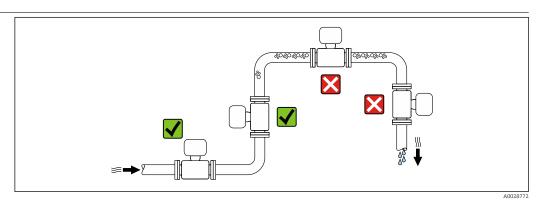


To avoid measurement errors caused by gas bubble formation in the measuring tube, avoid the following installation locations in the pipe:

- Highest point of a pipeline
- Directly upstream of a free pipe outlet in a down pipe

# Installation in down pipes

However, the following installation suggestion allows for installation in an open vertical pipeline. Pipe restrictions or the use of an orifice with a smaller cross-section than the nominal diameter prevent the sensor running empty while measurement is in progress.

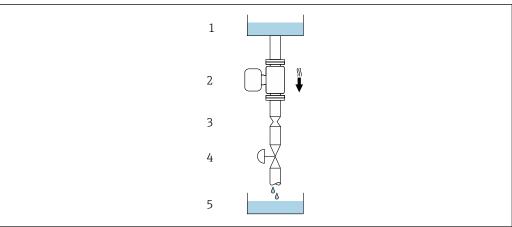

A002877

■ 13 Installation in a down pipe (e.g. for batching applications)

- 1 Supply tank
- 2 Sensor
- 3 Orifice plate, pipe restriction
- 4 Valve
- 5 Filling container

DN/NPS		Ø orifice plate, pipe restriction		
[mm]	[in]	[mm]	[in]	
1	1/24	0.8	0.03	
2	1/12	1.5	0.06	
4	1/8	3.0	0.12	
6	1/4	5.0	0.20	

#### Orientation

The direction of the arrow on the sensor nameplate helps you to install the sensor according to the flow direction (direction of medium flow through the piping).

	Recommendation		
A	Vertical orientation	A0015591	₩₩
В	Horizontal orientation, transmitter at top	A0015589	1)
С	Horizontal orientation, transmitter at bottom	A0015590	<b>✓ ✓</b> <sup>2)</sup>
D	Horizontal orientation, transmitter at side	A0015592	×

- 1) Applications with low process temperatures may reduce the ambient temperature. To maintain the minimum ambient temperature for the transmitter, this orientation is recommended.
- 2) Applications with high process temperatures may increase the ambient temperature. To maintain the maximum ambient temperature for the transmitter, this orientation is recommended.

# Inlet and outlet runs


# Installing the transmitter housing

# Proline 500 - digital transmitter

Pipe mounting

Required tools:

- Open-ended wrench AF 10
- Torx screwdriver TX 25

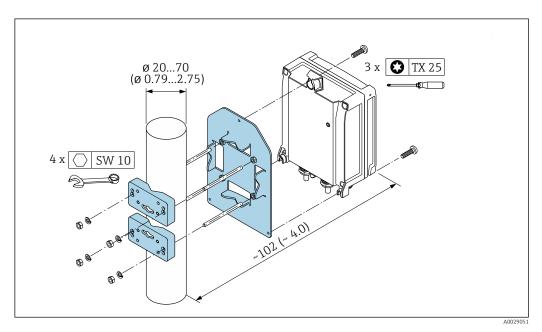


■ 14 Unit mm (in)

Wall mounting

Required tools:

Drill with drill bit Ø 6.0 mm

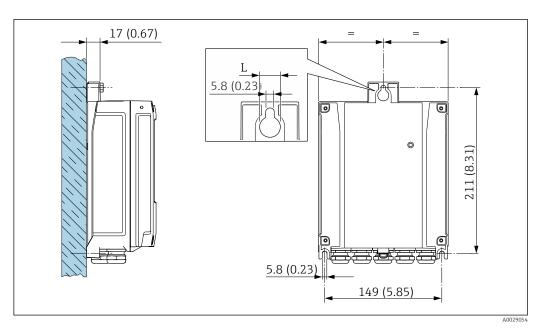

■ 15 Unit mm (in)

L Depends on order code for "Transmitter housing"

Order code for "Transmitter housing"

- Option **A**, aluminum, coated: L = 14 mm (0.55 in)
- Option **D**, polycarbonate: L = 13 mm (0.51 in)

# Proline 500 transmitter

Pipe mounting


Required tools Open-ended wrench AF 13

# **A** WARNING

# Order code for "Transmitter housing", option L "Cast, stainless": cast transmitters are very

They are unstable if they are not mounted on a secure, fixed post.


▶ Only mount the transmitter on a secure, fixed post on a stable surface.

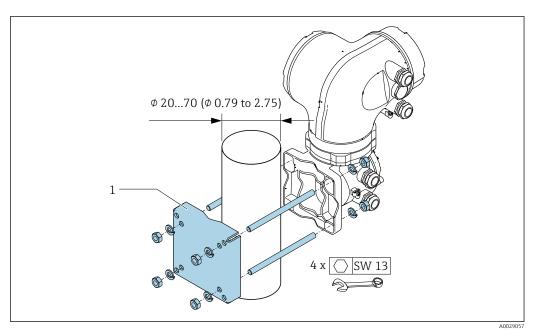

**■** 16 Unit mm (in)

Wall mounting

Required tools Drill with drill bit Ø 6.0 mm

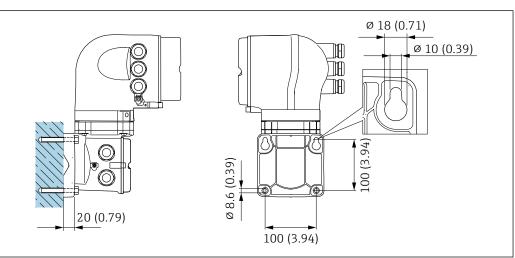

**■** 17 Unit mm (in)

# Special installation instructions

# Hygienic compatibility

When installing in hygienic applications, please refer to the information in the "Certificates and approvals/hygienic compatibility" section

### Rupture disk

Process-related information:  $\rightarrow \blacksquare 75$ .


### **A** WARNING

### Danger from medium escaping!

Medium escaping under pressure can cause injury or material damage.

- ► Take precautions to prevent danger to persons and damage if the rupture disk is actuated.
- ▶ Observe the information on the rupture disk sticker.
- Make sure that the function and operation of the rupture disk is not impeded through the installation of the device.
- ▶ Do not use a heating jacket.
- ▶ Do not remove or damage the rupture disk.

The position of the rupture disk is indicated by a sticker affixed beside it.

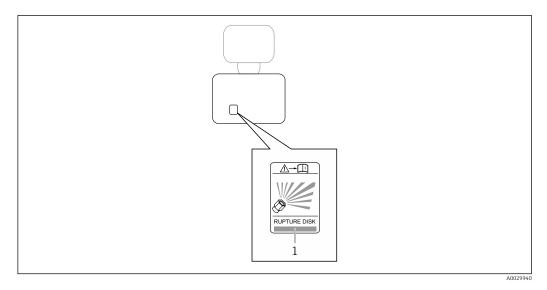

Rupture disk label

#### Zero point verification and zero adjustment

Experience shows that zero adjustment is advisable only in special cases:

- To achieve maximum measurement accuracy even with low flow rates.
- Under extreme process or operating conditions (e.g. very high process temperatures or very highviscosity media).
- For gas applications with low pressure.

For information on checking the zero point and performing a zero adjustment, see the Operating Instructions for the device.

To achieve the highest possible measurement accuracy at low flow rates, the installation must protect the sensor from mechanical stress during operation.

# Wall mounting

#### **▲** WARNING

### Incorrect sensor mounting


Risk of injury if measuring tube breaks

- ▶ The sensor should never be installed in a pipe in a way that it is freely suspended
- ▶ Using the base plate, mount the sensor directly on the floor, wall or ceiling.
- ► Support the sensor on a securely mounted support base (e.g. angle bracket).

The following mounting versions are recommended for the installation.

#### Vertical

- Mounted directly on a wall using the base plate, or
- Device supported on an angle bracket mounted on the wall

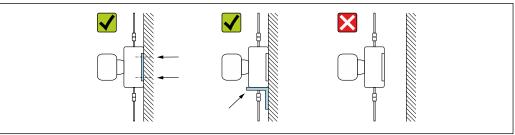

A0030286


#### Horizontal

Device standing on a solid support base



# Mounting plate

The universal mounting plate can be used to affix or place the unit on a flat surface (order code for "Accessories", option PA).

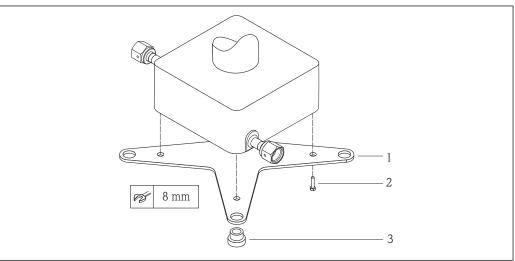


A001976

 $\blacksquare$  18 Mounting kit for Cubemass mounting plate


- 1 1 x Cubemass mounting plate
- 2 4 x screw M5 x 8
- 3 4 x grommet

70

# Protective cover

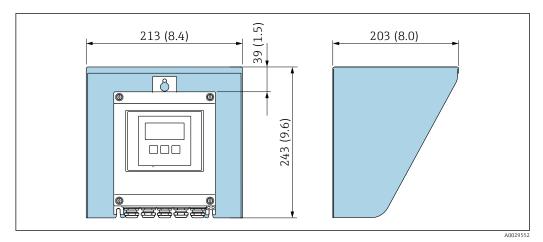

■ 19 Weather protection cover for Proline 500 – digital; unit mm (in)

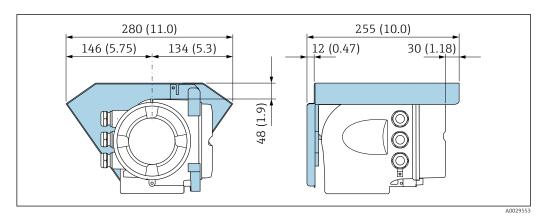

■ 20 Weather protection cover for Proline 500 – unit mm (in)

# **Environment**

Ambient temperature range	Measuring instrument	<ul> <li>-40 to +60 °C (-40 to +140 °F)</li> <li>Order code for "Test, certificate", option JP:</li> <li>-50 to +60 °C (-58 to +140 °F)</li> </ul>
	Readability of the local display	-20 to $+60$ °C ( $-4$ to $+140$ °F) The readability of the display may be impaired at temperatures outside the temperature range.

- ► If operating outdoors:

  Avoid direct sunlight, particularly in warm climatic regions.

Storage temperature	−50 to +80 °C (−58 to +176 °F)	
Climate class	DIN EN 60068-2-38 (test Z/AD)	
Relative humidity	The device is suitable for use in outdoor and indoor areas with a relative humidity of 4 to 95%.	

#### Operating height

According to EN 61010-1 ≤ 2 000 m (6 562 ft)

#### Degree of protection

#### Transmitter

- IP66/67, Type 4X enclosure, suitable for pollution degree 4
- When the housing is open: IP20, Type 1 enclosure, suitable for pollution degree 2
- Display module: IP20, Type 1 enclosure, suitable for pollution degree 2

#### Sensor

- IP66/67, Type 4X enclosure, suitable for pollution degree 4
- When the housing is open: IP20, Type 1 enclosure, suitable for pollution degree 2

#### External WLAN antenna

IP66/67, type 4X enclosure

# Vibration resistance and shock resistance

#### Sinusoidal vibration similar to IEC 60068-2-6

#### Sensor

- 2 to 8.4 Hz, 3.5 mm peak
- 8.4 to 2 000 Hz, 1 g peak

#### Transmitter

- 2 to 8.4 Hz, 7.5 mm peak
- 8.4 to 2000 Hz, 2 g peak

#### Broadband random vibration similar to IEC 60068-2-64

#### Sensor

- 10 to 200 Hz, 0.003 g<sup>2</sup>/Hz
- 200 to 2000 Hz, 0.001 g<sup>2</sup>/Hz
- Total: 1.54 g rms

# Transmitter

- 10 to 200 Hz, 0.01 q<sup>2</sup>/Hz
- 200 to 2000 Hz, 0.003 g<sup>2</sup>/Hz
- Total: 2.70 g rms

#### Half-sine shocks similar to IEC 60068-2-27

- Sensor
  - 6 ms 30 g
- Transmitter6 ms 50 g

#### Rough handling shocks similar to IEC 60068-2-31

# Mechanical load

Transmitter housing and sensor connection housing:

- Protect against mechanical effects, such as shock or impact
- lacksquare Do not use as a ladder or climbing aid

# Electromagnetic compatibility (EMC)


- As per IEC/EN 61326 and NAMUR Recommendation 21 (NE 21), NAMUR Recommendation 21 (NE 21) is fulfilled when the device is installed in accordance with NAMUR Recommendation 98 (NF 98)
- As per IEC/EN 61000-6-2 and IEC/EN 61000-6-4
- Device version with PROFIBUS DP: Complies with emission limits for industry as per EN 50170 Volume 2, IEC 61784
- The following applies for PROFIBUS DP: If baud rates > 1.5 MBaud, an EMC cable entry must be used and the cable shield must continue as far as the terminal wherever possible.
- Details are provided in the Declaration of Conformity.
- This unit is not intended for use in residential environments and cannot guarantee adequate protection of the radio reception in such environments.

### **Process**

#### Medium temperature range

 $-50 \text{ to } +205 ^{\circ}\text{C} (-58 \text{ to } +401 ^{\circ}\text{F})$ 

#### Dependency of ambient temperature on medium temperature

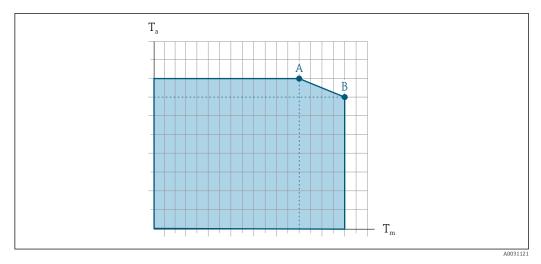

 $lap{1}{2}$  21 Exemplary representation, values in the table below.

- *T<sub>a</sub>* Ambient temperature
- $T_m$  Medium temperature
- A Maximum permitted medium temperature  $T_m$  at  $T_{a max} = 60$  °C (140 °F); higher medium temperatures  $T_m$  require a reduction in the ambient temperature  $T_a$
- B Maximum permitted ambient temperature  $T_a$  for the maximum specified medium temperature  $T_m$  of the sensor
- Values for devices that are used in the hazardous area: Separate Ex documentation (XA) for the device  $\rightarrow \stackrel{\triangle}{=} 118$ .

Not insulated			Insulated					
	A B		В		A		В	
Version	Ta	T <sub>m</sub>	Ta	T <sub>m</sub>	Ta	T <sub>m</sub>	$T_a$	$T_{m}$
Cubemass C 500 – digital	60 °C (140 °F)	205 °C (401 °F)	-	-	60 °C (140 °F)	90 °C (194 °F)	25 °C (77 °F)	205 °C (401 °F)
Cubemass C 500	60 °C (140 °F)	205 °C (401 °F)	-	-	60 °C (140 °F)	160 °C (320 °F)	55 ℃ (131 ℉)	205 °C (401 °F)

#### Seals

For mounting sets with screwed-on connections:

- Viton: -15 to +200 °C (-5 to +392 °F)
- EPDM: -40 to +160 °C (-40 to +320 °F)
- Silicone: -60 to +200 °C (-76 to +392 °F)
- Kalrez: -20 to +275 °C (-4 to +527 °F)

#### Medium density


0 to  $5000 \text{ kg/m}^3$  (0 to 312 lb/cf)

# Pressure-temperature ratings

The following pressure/temperature diagrams apply to all pressure-bearing parts of the device and not just the process connection. The diagrams show the maximum permissible medium pressure depending on the specific medium temperature.

### Flange connection similar to EN 1092-1 (DIN 2501)


Order code for "Mounting kit", option PE

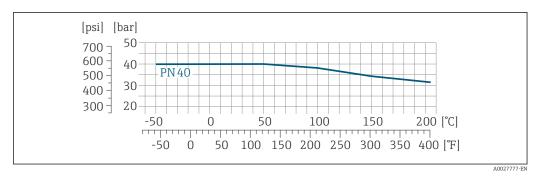

■ 22 With flange material: 1.4539 (904L), Alloy C22; lap joint flanges (not wetted) 1.4404 (316/316L)

### Flange connection similar to ASME B16.5


Order code for "Mounting kit", option PF, PG

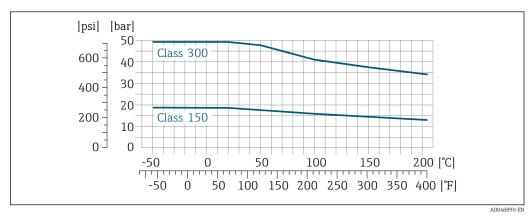

■ 23 With flange material: 1.4539 (904L); lap joint flanges (not wetted) 1.4404 (316/316L)

### Flange connection similar to JIS B2220


Order code for "Mounting kit", option PH

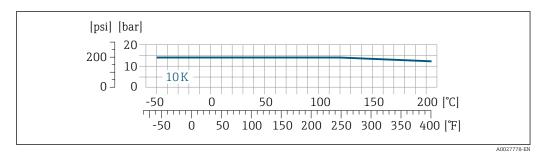

■ 24 With flange material: 1.4539 (904L); lap joint flanges (not wetted): 1.4404 (316/316L)

Process connection 4-VCO-4, ¼ NPTF (DN 1 to 4); 8-VCO-4, ½ NPTF (DN 6)

Order code for "Mounting kit", option PC, PD

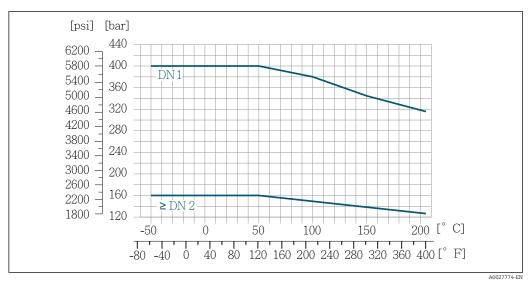

■ 25 4-VCO-4 coupling: 1.4539 (904L); 8-VCO-4 coupling: 1.4539 (904L); NPTF threaded adapter: 1.4539 (904L)

#### Sensor housing

The sensor housing is filled with dry nitrogen gas and protects the electronics and mechanics inside.

#### Rupture disk

To quarantee the safety of the measuring instrument, the device version with a rupture disk with a triggering pressure of 10 to 15 bar (145 to 217.5 psi) is the standard version used. Special installation instructions  $\rightarrow \triangleq 68$ .

#### Internal cleaning

- CIP cleaning
- SIP cleaning

Oil- and grease-free version for wetted parts, without declaration Order code for "Service", option HA 1)


#### Flow limit

Select the nominal diameter by optimizing between the required flow range and permissible pressure



For an overview of the full scale values for the measuring range, see the "Measuring range" section  $\rightarrow$   $\blacksquare$  12

- The minimum recommended full scale value is approx. 1/20 of the maximum full scale value
- For the most common applications, 20 to 50 % of the maximum full scale value can be considered ideal
- A low full scale value must be selected for abrasive media (such as liquids with entrained solids): flow velocity < 1 m/s (< 3 ft/s).
- For gas measurement the following rules apply:
  - The flow velocity in the measuring tubes should not exceed half the speed of sound (0.5 Mach)
  - The maximum mass flow depends on the density of the gas: formula



#### Pressure loss



To calculate the pressure loss, use the *Applicator* sizing tool  $\rightarrow \triangleq 116$ 


### Static pressure

It is important that cavitation does not occur, or that gases entrained in the liquids do not outgas. This is prevented by means of a sufficiently high static pressure.

For this reason, the following mounting locations are recommended:

- At the lowest point in a vertical pipe
- Downstream from pumps (no danger of vacuum)

Cleaning only refers to the measuring instrument. Any accessories that have been supplied are not cleaned.



A002877


#### Thermal insulation

In the case of some fluids, it is important to keep the heat radiated from the sensor to the transmitter to a low level. A wide range of materials can be used for the required insulation.

### NOTICE

#### Electronics overheating on account of thermal insulation!

- Recommended orientation: horizontal orientation, sensor connection housing pointing downwards.
- ▶ Do not insulate the sensor connection housing.
- Maximum permissible temperature at the lower end of the sensor connection housing: 80 °C (176 °F)
- ► Thermal insulation with exposed extension neck: We recommend that you do not insulate the extension neck in order to ensure optimum dissipation of heat.

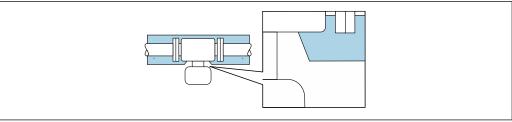

■ 26 Thermal insulation with exposed extension neck

A0034391

#### Heating

Some media require suitable measures to avoid loss of heat at the sensor.

### **Heating options**

- Electrical heating, e.g. with electric band heaters <sup>2)</sup>
- Via pipes carrying hot water or steam
- Via heating jackets

#### **NOTICE**

#### Danger of overheating when heating

- ► Ensure that the temperature at the lower end of the transmitter housing does not exceed 80 °C (176 °F).
- Ensure that sufficient convection takes place at the transmitter neck.
- ► Ensure that a sufficiently large area of the transmitter neck remains exposed. The uncovered part serves as a radiator and protects the electronics from overheating and excessive cooling.
- When using in potentially explosive atmospheres, observe the information in the device-specific Ex documentation. For detailed information on the temperature tables, see the separate document entitled "Safety Instructions" (XA) for the device.

#### **Vibrations**

The high oscillation frequency of the measuring tubes ensures that the correct operation of the measuring system is not influenced by plant vibrations.


<sup>2)</sup> The use of parallel electric band heaters is generally recommended (bidirectional electricity flow). Particular considerations must be made if a single-wire heating cable is to be used. Additional information is provided in the document EA01339D "Installation instructions for electrical trace heating systems" > 119

## Mechanical construction

#### Dimensions in SI units

Housing of Proline 500 - digital transmitter

Non-hazardous area or hazardous area: Zone 2; Class I, Division 2

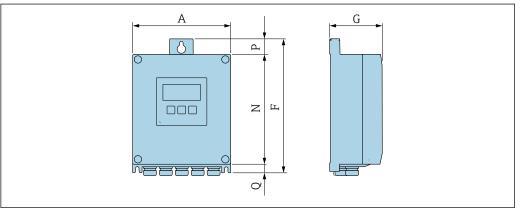

A0033789

Order code for "Transmitter housing", option A "Aluminum, coated" and order code for "Integrated ISEM electronics", option A "Sensor"


A	F	G	N	P	Q
[mm]	[mm]	[mm]	[mm]	[mm]	[mm]
167	232	89	187	24	

 $\label{lem:code} \textit{Order code for "Transmitter housing", option D "Polycarbonate" and order code for "Integrated ISEM electronics", option A "Sensor"$ 

A	F	G	N	P	Q
[mm]	[mm]	[mm]	[mm]	[mm]	[mm]
177	234	89	197	17	

### Housing of Proline 500 transmitter

Hazardous area: Zone 2; Class I, Division 2 or Zone 1; Class I, Division 1

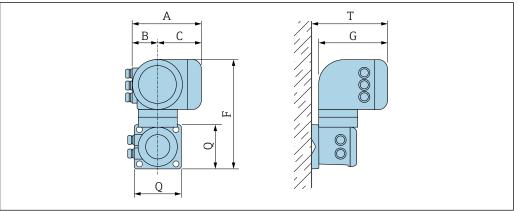

A0033788


Order code for "Transmitter housing", option A "Aluminum, coated" and order code for "Integrated ISEM electronics", option B "Transmitter"

A	B	C	F	G	Q	T
[mm]						
188	85	103	318	217	130	239

 $\label{lem:code} \textit{Order code for "Transmitter housing", option L "Cast, stainless" and order code for "Integrated ISEM electronics", option B "Transmitter"$ 

A [mm]	B [mm]	C [mm]	F [mm]	G [mm]	Q [mm]	T [mm]	
188	85	103	295	217	130	239	

### Sensor connection housing

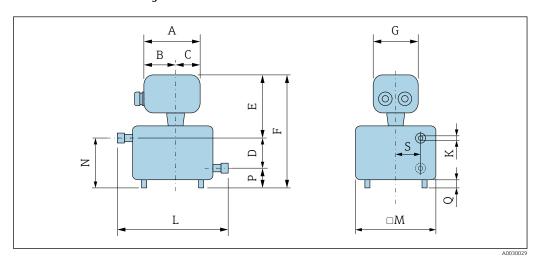

D K P S L DN M N Q [mm] [mm] [mm] [mm] [mm] [mm] [mm] [mm] [mm] 1 30 1.4 121 52 22 10 42.9 175 2 30 2.5 121 52 22 10 42.9 175 4 30 3.9 121 52 22 10 42.9 175 30 5.35 121 52 22 10 175 6 42.9

Order code for "Sensor connection housing", option A "Aluminum, coated"

DN	A 1)	B 1)	С	E	F	G
[mm]						
1-6	148	94	54	162	214	136

1) Depending on the cable gland used: values up to + 30 in

Order code for "Sensor connection housing", option B "Stainless, hygienic"

DN	A 1)	В	С	E	F	G
[mm]						
1-6	137	78	59	158	210	134

1) Depending on the cable gland used: values up to + 30 in

78

### Order code for "Sensor connection housing", option C "Ultra-compact hygienic, stainless"

DN	A 1)	В	С	E	F	G
[mm]						
1-6	124	68	56	157	209	112

1) Depending on the cable gland used: values up to + 30 in


### ${\it Order code for "Sensor connection housing", option L "Cast, stainless"}$

DN	A 1)	В	С	Е	F	G
[mm]						
1-6	145	86	59	185	237	136

1) Depending on the cable gland used: values up to + 30 in

### **Compression fittings**

### VCO coupling

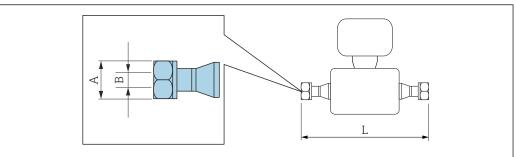

A0015624


Length tolerance for dimension L in mm: +3.0 / -3.0

4-VCO-4 1.4539 (904L): order code for "Process connection", option HAW							
DN [mm]	A [in]	B [mm]	L [mm]				
1	AF <sup>11</sup> / <sub>16</sub>	12.5	175				
2	AF <sup>11</sup> / <sub>16</sub>	12.5	175				
4	AF <sup>11</sup> / <sub>16</sub>	12.5	175				

8-VCO-4 1.4404 (316/316L): order (	8-VCO-4 1.4404 (316/316L): order code for "Process connection", option CVS							
DN [mm]	A [in]	B [mm]	L [mm]					
6	AF 1	20	175					

#### Adapter

Adapter, DN 15 flange to VCO

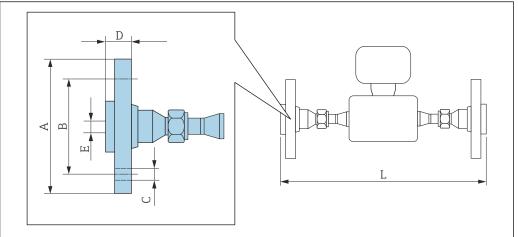

A0019725

Length tolerance for dimension L in mm: +3.0 / -3.0

Flange similar to EN 1092-1 (DIN 2501): PN 40 1.4539 (904L): order code for "Accessories", option PE							
DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]	
1 to 6	95	65	4 × Ø14	28	17.3	278	

DN 1 to 4 with 4-VCO-4, DN 6 with 8-VCO-4

Lap joint flanges (not wetted) made of stainless steel 1.4404 (316/316L)

Sealing sets: order code for "Accessory enclosed", option P1 (Viton), P2 (EPDM), P3 (silicone), P4 (Kalrez)

	Flange similar to ASME B16.5: Class 150 1.4539 (904L): order code for "Accessories", option PF								
DN [mm]									
1 to 6 90.0 66.5 4 × Ø15.7 17.7 15.7 278									

DN 1 to 4 with 4-VCO-4, DN 6 with 8-VCO-4

Lap joint flanges (not wetted) made of stainless steel 1.4404 (316/316L)

Sealing sets: order code for "Accessory enclosed", option P1 (Viton), P2 (EPDM), P3 (silicone), P4 (Kalrez)

	Flange similar to ASME B16.5: Class 300 1.4539 (904L): order code for "Accessories", option PG								
DN [mm]									
1 to 6 95.0 66.5 4 × Ø15.7 20.7 15.7 278									

DN 1 to 4 with 4-VCO-4, DN 6 with 8-VCO-4

Lap joint flanges (not wetted) made of stainless steel 1.4404 (316/316L)


Sealing sets: order code for "Accessory enclosed", option P1 (Viton), P2 (EPDM), P3 (silicone), P4 (Kalrez)

	Flange JIS B2220: 10K 1.4539 (904L): order code for "Accessories", option PH							
DN [mm]								
1 to 6 95 70 4 × Ø15 28 15.0 27								

DN 1 to 4 with 4-VCO-4, DN 6 with 8-VCO-4

Lap joint flanges (not wetted) made of stainless steel 1.4404 (316/316L)
Sealing sets: order code for "Accessory enclosed", option **P1** (Viton), **P2** (EPDM), **P3** (silicone), **P4** (Kalrez)

### Adapter, NPTF to VCO

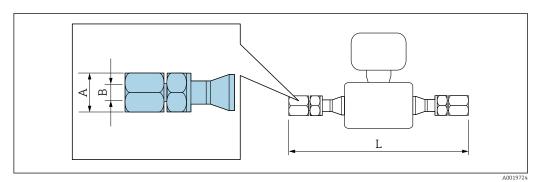


Length tolerance for dimension L in mm: +3.0 / -3.0

<sup>1</sup> / <sub>4</sub> " NPTF to 4-VCO-4 1.4539 (904L): order code for "Accessories", option PC							
DN A B L [mm] [in] [mm]							
1 to 4	AF ¾	½ NPT	246				
Sealing sets: order code for	Sealing sets: order code for "Accessory enclosed", option P1 (Viton), P2 (EPDM), P3 (silicone), P4 (Kalrez)						


1.4539 (904L): order code for "Accessories", option PD							
DN [mm]	A [in]	B [in]	L [mm]				
6 AF <sup>11</sup> / <sub>16</sub> <sup>1</sup> / <sub>2</sub> NPT 246							
Sealing sets: order code for "Accessory enclosed", option P1 (Viton), P2 (EPDM), P3 (silicone), P4 (Kalrez)							

### Accessories

### Protective cover

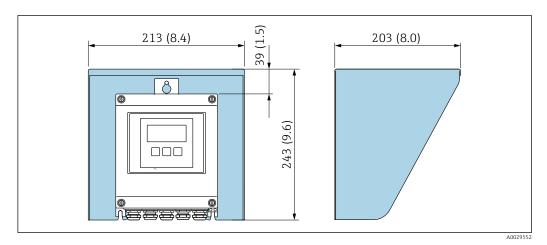

Weather protection cover for Proline 500 – digital; unit mm (in)

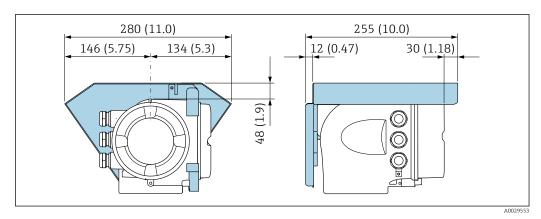


■ 28 Weather protection cover for Proline 500 – unit mm (in)

External WLAN antenna

The external WLAN antenna is not suitable for use in hygienic applications.

Proline 500 – digital


External WLAN antenna mounted on device

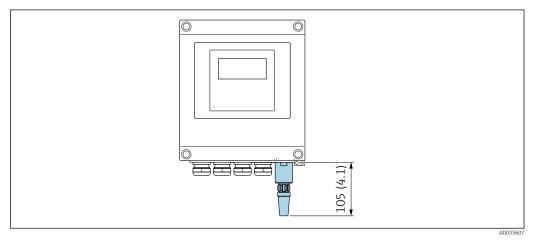

■ 29 Unit mm (in)

External WLAN antenna mounted with cable


The external WLAN antenna can be mounted separately from the transmitter if the transmission/reception conditions at the transmitter mounting location are poor.

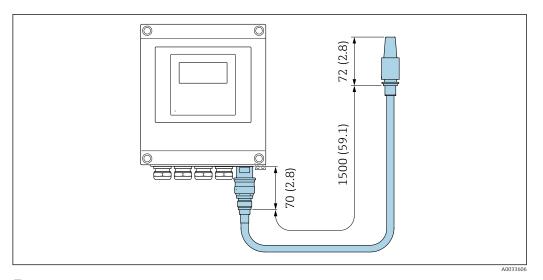

■ 30 Unit mm (in)

Proline 500


External WLAN antenna mounted on device

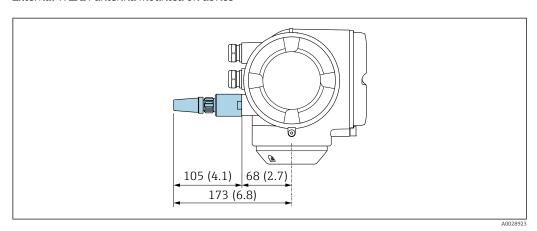

■ 31 Unit mm (in)

External WLAN antenna mounted with cable

The external WLAN antenna can be mounted separately from the transmitter if the transmission/reception conditions at the transmitter mounting location are poor.

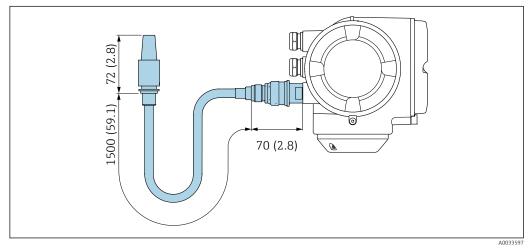


■ 32 Unit mm (in)

#### Dimensions in US units

### Housing of Proline 500 - digital transmitter

Non-hazardous area or hazardous area: Zone 2; Class I, Division 2

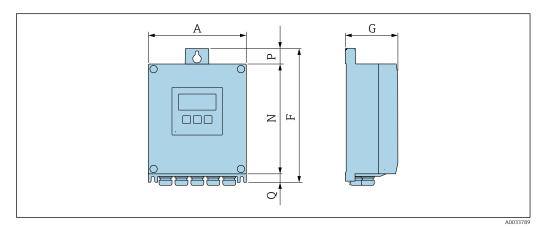

Order code for "Transmitter housing", option A "Aluminum, coated" and order code for "Integrated ISEM electronics", option A "Sensor"


A	F	G	N	P	Q
[in]	[in]	[in]	[in]	[in]	[in]
6.57	9.13	3.50	7.36	0.94	

 ${\it Order\ code\ for\ "Transmitter\ housing",\ option\ D\ "Polycarbonate"\ and\ order\ code\ for\ "Integrated\ ISEM\ electronics",\ option\ A\ "Sensor"$ 

A	F	G	N	P	Q
[in]	[in]	[in]	[in]	[in]	[in]
6.97	9.21	3.50	7.76	0.67	

### Housing of Proline 500 transmitter

Hazardous area: Zone 2; Class I, Division 2 or Zone 1; Class I, Division 1

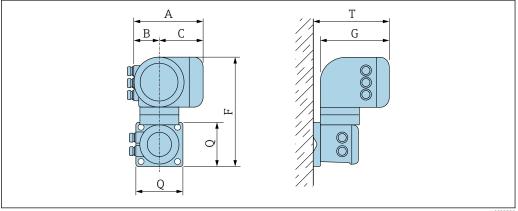

A003378


Order code for "Transmitter housing", option A "Aluminum, coated" and order code for "Integrated ISEM electronics", option B "Transmitter"

A	B	C	F	G	Q	T
[in]						
7.40	3.35	4.06	12.5	8.54	5.12	9.41

 $\label{lem:code} \textit{Order code for "Transmitter housing", option $L$ "Cast, stainless" and order code for "Integrated ISEM electronics", option $B$ "Transmitter"}$ 

A	B	C	F	G	Q	T
[in]						
7.40	3.35	4.06	11.6	8.54	5.12	

### Sensor connection housing

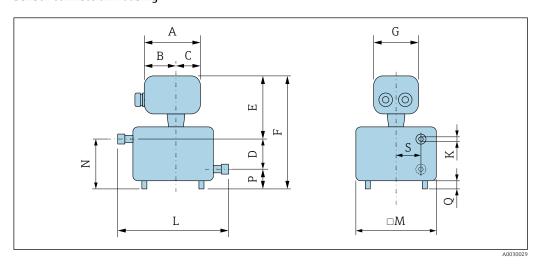

DN D K M N P Q S L [in] [in] [in] [in] [in] [in] [in] [in] [in] 1/24 0.06 0.87 0.39 1.18 4.76 2.05 1.69 6.89 1/12 1.18 0.10 4.76 2.05 0.87 0.39 1.69 6.89 1/8 1.18 0.15 4.76 2.05 0.87 0.39 1.69 6.89 1/4 1.18 0.211 4.76 0.87 0.39 2.05 1.69 6.89

Order code for "Sensor connection housing", option A "Aluminum, coated"

DN	A 1)	B 1)	С	E	F	G
[in]	[in]	[in]	[in]	[in]	[in]	[in]
½4 to ½	5.83	3.70	2.13	6.38	8.43	5.35

1) Depending on the cable gland used: values up to +1.18 in

Order code for "Sensor connection housing", option B "Stainless, hygienic"

DN	A 1)	В	С	Е	F	G
[in]	[in]	[in]	[in]	[in]	[in]	[in]
½4 to ½	5.39	3.07	2.32	6.22	8.27	5.28

1) Depending on the cable gland used: values up to +1.18 in

### Order code for "Sensor connection housing", option C "Ultra-compact hygienic, stainless"

DN	A 1)	В	С	E	F	G
[in]	[in]	[in]	[in]	[in]	[in]	[in]
½4 to ¼	4.88	2.68	2.20	6.18	8.23	4.41

1) Depending on the cable gland used: values up to +1.18 in


### Order code for "Sensor connection housing", option L "Cast, stainless"

DN	A 1)	В	С	Е	F	G
[in]	[in]	[in]	[in]	[in]	[in]	[in]
½4 to ¼	5.71	3.39	2.32	7.28	9.33	5.35

1) Depending on the cable gland used: values up to +1.18 in

### **Compression fittings**

### VCO coupling

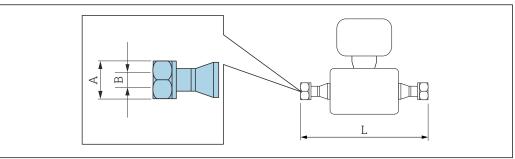

A0015624


Length tolerance for dimension L in inches: +0.12 / -0.12

4-VCO-4 1.4539 (904L): order code for "Process connection", option HAW				
DN [in]	A [in]	B [in]	L [in]	
1/24	AF <sup>11</sup> / <sub>16</sub>	0.49	6.89	
1/12	AF <sup>11</sup> / <sub>16</sub>	0.49	6.89	
1/8	AF <sup>11</sup> / <sub>16</sub>	0.49	6.89	

8-VCO-4 1.4404 (316/316L): order code for "Process connection", option CVS			
DN [in]	A [in]	B [in]	L [in]
1/4	AF 1	0.79	6.89

#### Adapter

Adapter, DN 15 flange to VCO

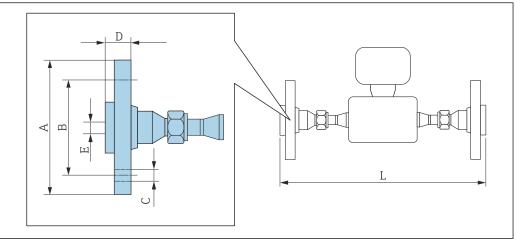

A0019725

Length tolerance for dimension L in inches: +0.12 / -0.12

Flange similar to ASME B16.5: Class 150 1.4539 (904L): order code for "Accessories", option PF						
DN [in]	A [in]	B [in]	C [in]	D [in]	E [in]	L [in]
½4 to ¼	3.54	2.62	4 × Ø0.62	0.7	0.62	10.94

DN  $^{1}\!/_{\!24}$  to  $^{1}\!/_{\!8}$  with 4-VCO-4, DN  $^{1}\!/_{\!4}$  with 8-VCO-4

Lap joint flanges (not wetted) made of stainless steel 1.4404 (316/316L)

Sealing sets: order code for "Accessory enclosed", option P1 (Viton), P2 (EPDM), P3 (silicone), P4 (Kalrez)


Flange similar to ASME B16.5: Class 300 1.4539 (904L): order code for "Accessories", option PG						
DN         A         B         C         D         E         L           [in]         [in]         [in]         [in]         [in]						
½4 to ¼	3.74	2.62	4 × Ø0.62	0.81	0.62	10.94

DN  $^1\!/_{\!24}$  to  $^1\!/_{\!8}$  with 4-VCO-4, DN  $^1\!/_{\!4}$  with 8-VCO-4

Lap joint flanges (not wetted) made of stainless steel 1.4404 (316/316L)

Sealing sets: order code for "Accessory enclosed", option P1 (Viton), P2 (EPDM), P3 (silicone), P4 (Kalrez)

### Adapter, NPTF to VCO

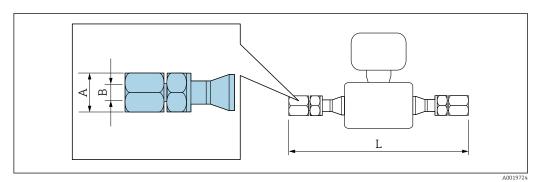


Length tolerance for dimension L in inches: +0.12 / -0.12

1,4" NPTF to 4-VCO-4 1.4539 (904L): order code for "Accessories", option PC					
DN [in]	A [in]	B [in]	L [in]		
<sup>1</sup> / <sub>24</sub> to <sup>1</sup> / <sub>8</sub> AF <sup>3</sup> / <sub>4</sub> NPT 9.69					
Sealing sets: order code for "A	.ccessory enclosed". option <b>P</b>	1 (Viton). <b>P2</b> (EPDM). <b>P3</b> (sil	icone). <b>P4</b> (Kalrez)		


1.4539 (904L): order code for "Accessories", option PD				
DN [in]	A [in]	B [in]	L [in]	
<sup>1</sup> / <sub>4</sub> AF <sup>11</sup> / <sub>16</sub> ½ NPT 9.69				
Sealing sets: order code for "Accessory enclosed", option P1 (Viton), P2 (EPDM), P3 (silicone), P4 (Kalrez)				

#### Accessories

### Protective cover

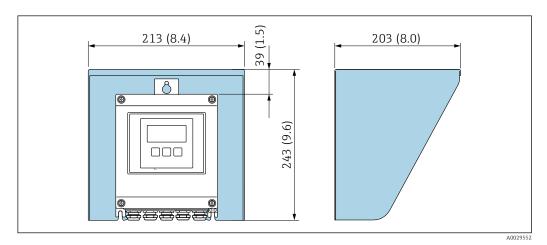

Weather protection cover for Proline 500 – digital; unit mm (in)

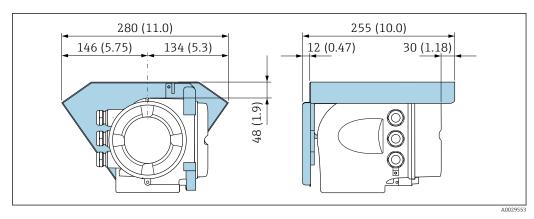


■ 34 Weather protection cover for Proline 500 – unit mm (in)

External WLAN antenna

The external WLAN antenna is not suitable for use in hygienic applications.

Proline 500 – digital


External WLAN antenna mounted on device

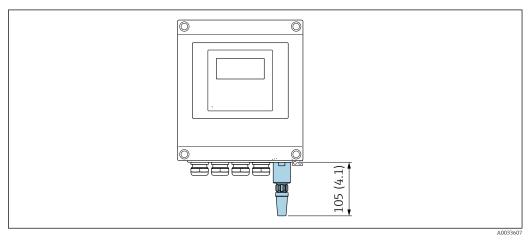

■ 35 Unit mm (in)

External WLAN antenna mounted with cable


The external WLAN antenna can be mounted separately from the transmitter if the transmission/reception conditions at the transmitter mounting location are poor.

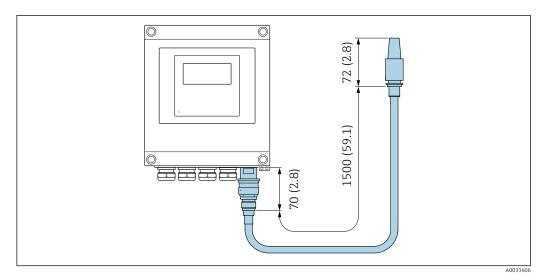

■ 36 Unit mm (in)

#### Proline 500


External WLAN antenna mounted on device

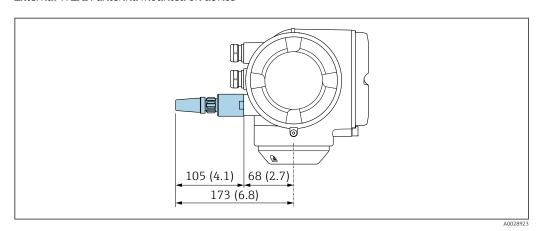

■ 37 Unit mm (in)

#### External WLAN antenna mounted with cable

The external WLAN antenna can be mounted separately from the transmitter if the transmission/reception conditions at the transmitter mounting location are poor.

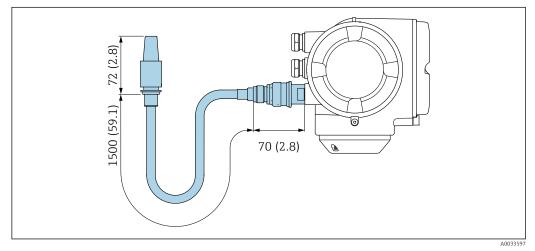

■ 38 Unit mm (in)

#### Weight

All values (weight exclusive of packaging material) refer to devices with VCO couplings.

#### Transmitter

- Proline 500 digital polycarbonate: 1.4 kg (3.1 lbs)
- Proline 500 digital aluminum: 2.4 kg (5.3 lbs)
- Proline 500 aluminum: 6.5 kg (14.3 lbs)
- Proline 500 cast, stainless: 15.6 kg (34.4 lbs)

#### Sensor

- Sensor with cast connection housing version, stainless: +3.7 kg (+8.2 lbs)
- Sensor with aluminum connection housing version:

#### Weight in SI units

DN [mm]	Weight [kg]
1 to 6	3.5

#### Weight in US units

DN [in]	Weight [lbs]
<sup>1</sup> / <sub>24</sub> to <sup>1</sup> / <sub>4</sub>	8

### Materials

#### Transmitter housing

Housing of Proline 500 – digital transmitter

Order code for "Transmitter housing":

- Option A "Aluminum coated": aluminum, AlSi10Mq, coated
- Option **D** "Polycarbonate": polycarbonate

Housing of Proline 500 transmitter

Order code for "Transmitter housing":

- Option **A** "Aluminum coated": aluminum, AlSi10Mg, coated
- Option L "Cast, stainless": cast, stainless steel, 1.4409 (CF3M) similar to 316L

#### Window material

Order code for "Transmitter housing":

- Option **A** "Aluminum, coated": glass
- Option **D** "Polycarbonate": plastic
- Option L "Cast, stainless": glass

Fixing components for pipe mounting


- Screws, threaded bolts, washers, nuts: stainless A2 (chrome-nickel steel)
- Metal plates: stainless steel, 1.4301 (304)

### Sensor connection housing

Order code for "Sensor connection housing":

- Option A "Aluminum coated": aluminum, AlSi10Mg, coated
- Option **B** "Stainless":
  - Stainless steel 1.4301 (304)
  - Optional: Order code for "Sensor feature", option CC "Hygienic version, for maximum corrosion resistance": stainless steel, 1.4404 (316L)
- Option **C** "Ultra-compact, stainless":
  - Stainless steel 1.4301 (304)
  - Optional: Order code for "Sensor feature", option CC "Hygienic version, for maximum corrosion resistance": stainless steel, 1.4404 (316L)
- $\, \bullet \,$  Option L "Cast, stainless": 1.4409 (CF3M) similar to 316L

### Cable entries/cable glands

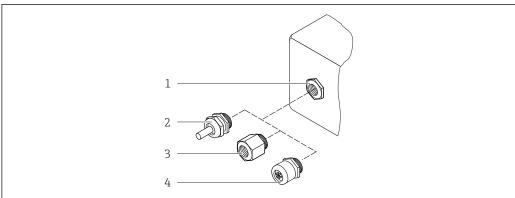

Possible cable entries/cable glands

- Internal thread M20  $\times$  1.5
- Cable gland M20  $\times$  1.5
- Adapter for cable entry with internal thread G  $\frac{1}{2}$ " or NPT  $\frac{1}{2}$ "
- 2 3 4 Device plug

Cable entries and adapters	Material
Cable gland M20 × 1.5	Plastic
■ Adapter for cable entry with female thread G ½" ■ Adapter for cable entry with female thread NPT ½"	Nickel-plated brass
Only available for certain device versions:  Order code for "Transmitter housing":  Option A "Aluminum, coated"  Option D "Polycarbonate"  Order code for "Sensor connection housing":  Proline 500 – digital: Option A "Aluminum coated" Option B "Stainless" Option L "Cast, stainless"  Proline 500: Option B "Stainless" Option L "Cast, stainless"	
<ul> <li>Adapter for cable entry with female thread G ½"</li> <li>Adapter for cable entry with female thread NPT ½"</li> </ul>	Stainless steel, 1.4404 (316L)
Only available for certain device versions:  Order code for "Transmitter housing": Option L "Cast, stainless"  Order code for "Sensor connection housing": Option L "Cast, stainless"	
Adapter for device plug	Stainless steel, 1.4404 (316L)
<ul> <li>Device plug for digital communication:         Only available for certain device versions →          Device plug for connecting cable:         A device plug is always used for the device version, order code for "Sensor connection housing", option C (ultracompact, hygienic, stainless).</li> </ul>	

### Device plug

Electrical connection	Material
Plug M12x1	<ul> <li>Socket: Stainless steel, 1.4404 (316L)</li> <li>Contact housing: Polyamide</li> <li>Contacts: Gold-plated brass</li> </ul>

#### Connecting cable



UV radiation can impair the cable outer sheath. Protect the cable from exposure to sun as much as possible.

Connecting cable for sensor - Proline 500 - digital transmitter

PVC cable with copper shield

Connecting cable for sensor - Proline 500 transmitter

PVC cable with copper shield

#### Sensor housing

- · Acid and alkali-resistant outer surface
- Stainless steel 1.4301 (304)

#### Measuring tubes

Stainless steel, 1.4539 (904L)

#### **Process connections**

VCO connection:

VCO connection: stainless steel, 1.4539 (904L)

Adapter for DN 15 flange similar to EN 1092-1 (DIN2501) / similar to ASME B 16.5 /

as per JIS B2220:

Stainless steel, 1.4539 (904L)

NPTF adapter:

Stainless steel, 1.4539 (904L)



Available process connections → 

97

#### Seals

Welded process connections without internal seals

#### Seals for mounting kit

- Viton
- EPDM
- Silicone
- Kalrez

#### Accessories

Protective cover

Stainless steel, 1.4404 (316L)

External WLAN antenna

- Antenna: ASA plastic (acrylonitrile styrene acrylate) and nickel-plated brass
- Adapter: Stainless steel and nickel-plated brass
- Cable: Polyethylene
- Plug: Nickel-plated brass
- Angle bracket: Stainless steel

#### **Process connections**

- Fixed flange connections:
  - EN 1092-1 (DIN 2512N) flange
  - ASME B16.5 flange
  - JIS B2220 flange
- VCO connections:
  - 4-VCO-4
  - 8-VCO-4
- Adapter for VCO connections:
  - Flange EN 1092-1 (DIN 2501)
  - Flange ASME B16.5
  - Flange JIS B2220
  - NPT



Process connection materials → 🖺 96

#### Surface roughness

All data relate to parts in contact with medium.

The following surface roughness categories can be ordered: Not polished

### Operability

#### Operation concept

#### Operator-oriented menu structure for user-specific tasks

- Commissioning
- Operation
- Diagnosis
- Expert level

#### Quick and safe commissioning

- Guided menus ("Make-it-run" wizards) for applications
- Menu quidance with brief descriptions of the individual parameter functions
- Access to the device via web server
- WLAN access to the device via mobile handheld terminal, tablet or smart phone

#### Reliable operation

- Operation in local language
- Uniform operating philosophy applied to device and operating tools
- If replacing electronic modules, transfer the device configuration via the integrated memory (HistoROM backup) which contains the process and measuring device data and the event logbook. No need to reconfigure.

#### Efficient diagnostics increase measurement reliability

- Troubleshooting measures can be called up via the device and in the operating tools
- Diverse simulation options, logbook for events that occur and optional line recorder functions

#### Languages

Can be operated in the following languages:

- Via local operation
  - English, German, French, Spanish, Italian, Dutch, Portuguese, Polish, Russian, Turkish, Chinese, Japanese, Korean, Vietnamese, Czech, Swedish
- Via web browser
  - English, German, French, Spanish, Italian, Dutch, Portuguese, Polish, Russian, Turkish, Chinese, Japanese, Vietnamese, Czech, Swedish
- Via "FieldCare", "DeviceCare" operating tool: English, German, French, Spanish, Italian, Chinese, Japanese

#### **Onsite operation**


#### Via display module

Equipment level:

- Order code for "Display; operation", option F "4-line, illuminated, graphic display; touch control"
- Order code for "Display; operation", option G "4-line, illuminated, graphic display; touch control +



Information about WLAN interface → 105

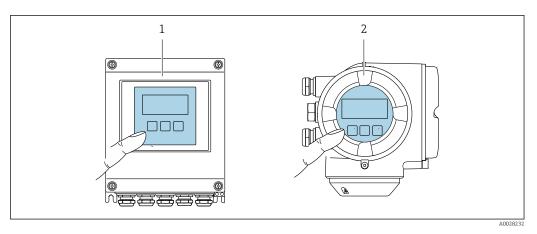

40 Operation with touch control

- 1 Proline 500 digital
- 2 Proline 500

#### Display elements

- 4-line, illuminated, graphic display
- White background lighting; switches to red in event of device errors
- Format for displaying measured variables and status variables can be individually configured


#### Operating elements

- External operation via touch control (3 optical keys) without opening the housing: ±, ⊡, ©
- Operating elements also accessible in the various zones of the hazardous area

#### Remote operation

### Via HART protocol


This communication interface is available in device versions with a HART output.

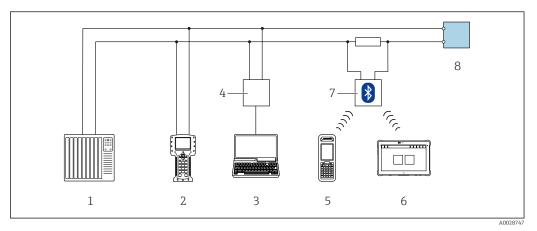

■ 41 Options for remote operation via HART protocol (active)

- 1 Automation system (e.g. PLC)
- 2 Field Communicator 475
- 3 Computer with web browser for accessing the integrated device web server or computer with operating tool (e.g. FieldCare, DeviceCare, AMS Device Manager, SIMATIC PDM) with COM DTM "CDI Communication TCP/IP"
- 4 Commubox FXA195 (USB)
- 5 Field Xpert SFX350 or SFX370
- 6 Field Xpert SMT70
- 7 VIATOR Bluetooth modem with connection cable
- 8 Transmitter

98

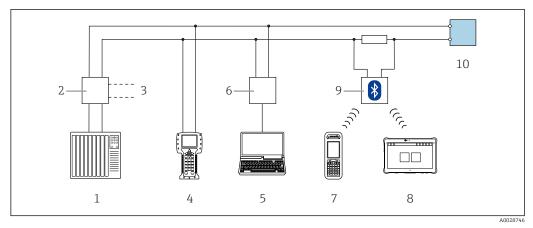


**№** 42 Options for remote operation via HART protocol (passive)

- Automation system (e.g. PLC)
- Transmitter power supply unit, e.g. RN221N (with communication resistor)
- 3 Connection for Commubox FXA195 and Field Communicator 475
- Field Communicator 475
- Computer with web browser for accessing the integrated device web server or computer with operating tool (e.g. FieldCare, DeviceCare, AMS Device Manager, SIMATIC PDM) with COM DTM "CDI Communication TCP/IP"
- Commubox FXA195 (USB)
- Field Xpert SFX350 or SFX370
- Field Xpert SMT70
- VIATOR Bluetooth modem with connection cable
- 10 Transmitter

#### Via FOUNDATION Fieldbus network

This communication interface is available in device versions with FOUNDATION Fieldbus.

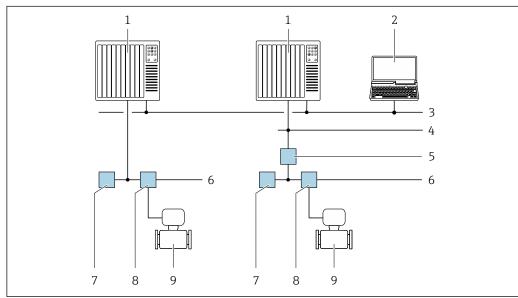


Options for remote operation via FOUNDATION Fieldbus network

- 1 Automation system
- Computer with FOUNDATION Fieldbus network card
- 3 Industry network
- High Speed Ethernet FF-HSE network
- Segment coupler FF-HSE/FF-H1
- 6 FOUNDATION Fieldbus FF-H1 network
- Power supply FF-H1 network
- 8 T-box
- Measuring instrument

#### Via PROFIBUS DP network

This communication interface is available in device versions with PROFIBUS DP.

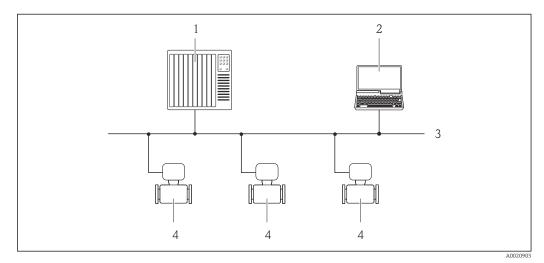


■ 44 Options for remote operation via PROFIBUS DP network

- 1 Automation system
- 2 Computer with PROFIBUS network card
- 3 PROFIBUS DP network
- 4 Measuring instrument

#### Via PROFIBUS PA network

This communication interface is available in device versions with PROFIBUS PA.

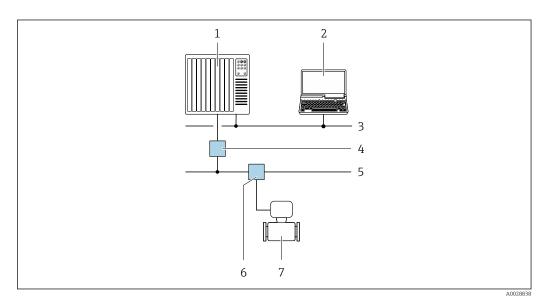


 $\blacksquare$  45 Options for remote operation via PROFIBUS PA network

- 1 Automation system
- 2 Computer with PROFIBUS network card
- 3 PROFIBUS DP network
- 4 Segment coupler PROFIBUS DP/PA
- 5 PROFIBUS PA network
- 6 T-box
- 7 Measuring instrument

### Via Modbus RS485 protocol

This communication interface is available in device versions with a Modbus RS485 output.

100

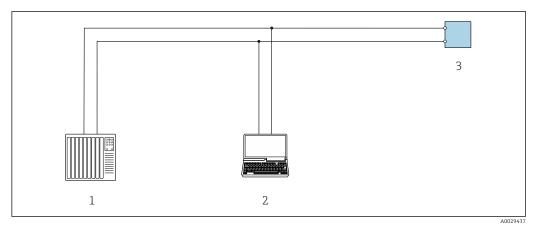


■ 46 Options for remote operation via Modbus RS485 protocol (active)

- 1 Automation system (e.g. PLC)
- 2 Computer with web browser for accessing the integrated device web server or with operating tool (e.g. FieldCare, DeviceCare) with COM DTM "CDI Communication TCP/IP" or Modbus DTM
- 3 Transmitter

#### Via EtherNet/IP network

This communication interface is available in device versions with EtherNet/IP.

#### Star topology

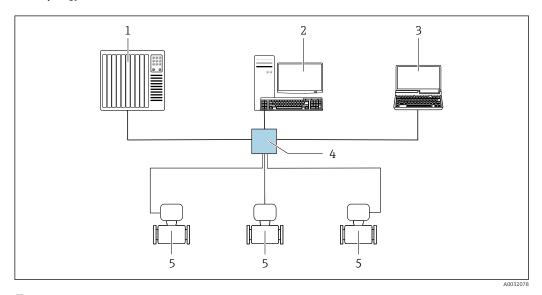


 $\blacksquare$  47 Options for remote operation via Ethernet/IP network: star topology

- 1 Automation system, z.B. "RSLogix" (Rockwell Automation)
- Workstation for measuring instrument operation: with Custom Add-On Profile for "RSLogix 5000" (Rockwell Automation) or with Electronic Data Sheet (EDS)
- 3 Computer with web browser for accessing the integrated web server or computer with operating tool (e.g. FieldCare, DeviceCare) with COM DTM "CDI Communication TCP/IP"
- 4 Standard Ethernet switch, e.g. Scalance X204 (Siemens)
- 5 Measuring instrument

### Ring topology

The device is integrated via the terminal connection for signal transmission (output 1) and the service interface (CDI-RJ45).

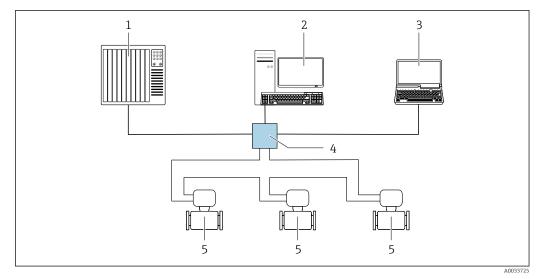


■ 48 Options for remote operation via EtherNet/IP network: ring topology

- 1 Automation system, z. B. "RSLogix" (Rockwell Automation)
- 2 Workstation for measuring instrument operation: with Custom Add-On Profile for RSLogix 5000 (Rockwell Automation) or with Electronic Data Sheet (EDS)
- 3 Computer with web browser for accessing the integrated web server or computer with operating tool (e.g. FieldCare, DeviceCare) with COM DTM "CDI Communication TCP/IP"
- 4 Standard Ethernet switch, e.g. Scalance X204 (Siemens)
- 5 Measuring instrument

#### Via PROFINET network

This communication interface is available in device versions with PROFINET.

### Star topology

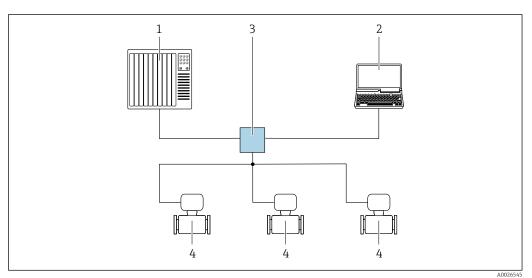


49 Options for remote operation via PROFINET network: star topology

- 1 Automation system, e.g. Simatic S7 (Siemens)
- 2 Computer with web browser for accessing integrated web server or computer with operating tool (e.g. FieldCare, DeviceCare, SIMATIC PDM) with COM DTM "CDI Communication TCP/IP"
- 3 Standard Ethernet switch, e.g. Scalance X204 (Siemens)
- 4 Measuring instrument

### Ring topology

The device is integrated via the terminal connection for signal transmission (output 1) and the service interface (CDI-RJ45).

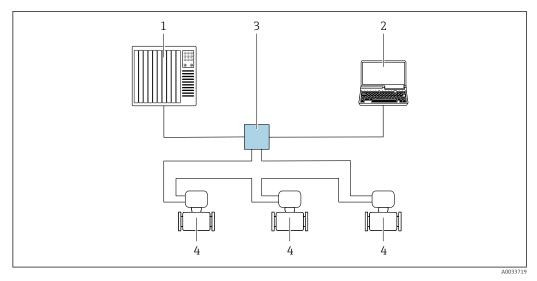


Options for remote operation via PROFINET network: ring topology

- Automation system, e.g., Simatic S7 (Siemens)
- 2 Computer with web browser for accessing integrated web server or computer with operating tool (e.g. FieldCare, DeviceCare, SIMATIC PDM) with COM DTM "CDI Communication TCP/IP"
- Standard Ethernet switch, e.g. Scalance X204 (Siemens)
- Measuring instrument

### Via Modbus TCP over Ethernet-APL 10 Mbit/s, SPE 10 Mbit/s

This communication interface is available on port 1 in device versions with a Modbus TCP over Ethernet-APL output.

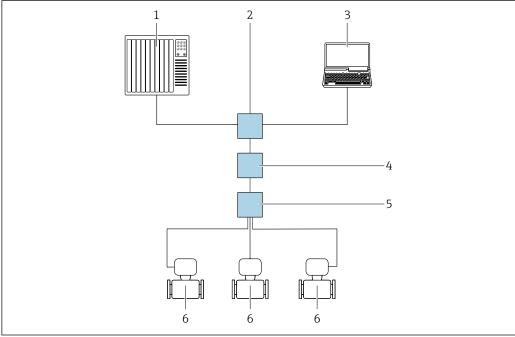

Options for remote operation via Modbus TCP over Ethernet-APL protocol (active)

- 1 Automation system, e.g. Simatic S7 (Siemens)
- Ethernet switch, e.g. Scalance X204 (Siemens)
- 3 Computer with web browser or operating tool
- APL power switch/SPE power switch (optional)
- APL field switch/SPE field switch
- Measuring instrument/communication via port 1 (terminal 26 + 27)


Endress+Hauser 103

A0046117

#### Via Modbus TCP over Ethernet 100 Mbit/s

This communication interface is available on port 2 in device versions with a Modbus TCP over Ethernet-APL output.

Star topology

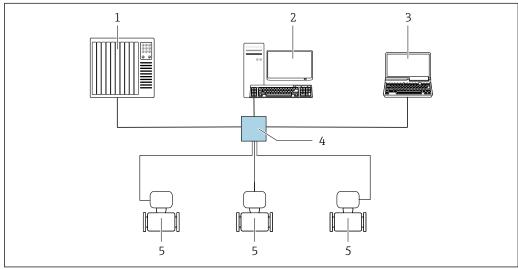

**№** 52 Options for remote operation via Modbus TCP over Ethernet - 100 Mbit/s: Star topology

- Automation system, z. B. RSLogix (Rockwell Automation)
- Workstation for measuring instrument operation: with Custom Add-On Profile for "RSLogix 5000" (Rockwell 2 Automation) or with Electronic Data Sheet (EDS)
- 3 Computer with web browser or operating tool
- Standard Ethernet switch, e.g. Stratix (Rockwell Automation)
- *Measuring instrument/communication via port 2 (RJ45 connector)*

#### Service interface

#### Via service interface (CDI-RJ45)

To configure the device on site, a point-to-point connection can be established. Alternatively, a connection via Modbus TCP can be used. The connection is made with the housing open, directly via the device's service interface (CDI-RJ45).




An adapter for the RJ45 to the M12 connector is optionally available for the non-hazardous area:

Order code for "Accessories", option NB: "Adapter RJ45 M12 (service interface)"

The adapter connects the service interface (CDI-RJ45) to an M12 connector mounted in the cable entry. The connection to the service interface can be established via an M12 connector without opening the device.


#### Proline 500 - digital transmitter

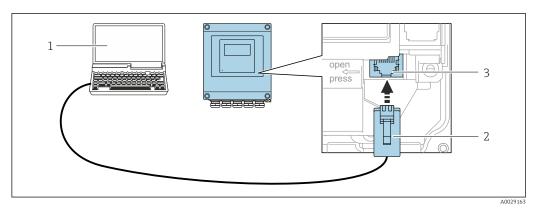

■ 53 Connection via service interface (CDI-RJ45)

- Computer with web browser for accessing the integrated web server or computer with operating tool, e.g. "FieldCare", "DeviceCare" with COM DTM "CDI Communication TCP/IP"or operating tool
- 2 Standard Ethernet connecting cable with RJ45 connector
- 3 Service interface (CDI-RJ45) of the measuring instrument with access to the integrated web server

#### Proline 500 transmitter

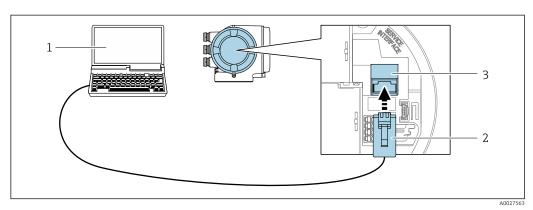


■ 54 Connection via service interface (CDI-RJ45)

- 1 Computer with web browser for accessing integrated web server or with operating tool e.g, "FieldCare", "DeviceCare", with COM DTM "CDI Communication TCP/IP" or Modbus DTM or operating tool
- 2 Standard Ethernet connecting cable with RJ45 connector
- 3 Service interface (CDI-RJ45) of the measuring instrument with access to the integrated web server

#### Via WLAN interface

The optional WLAN interface is available on the following device version: Order code for "Display; operation", option G "4-line, illuminated; touch control + WLAN"

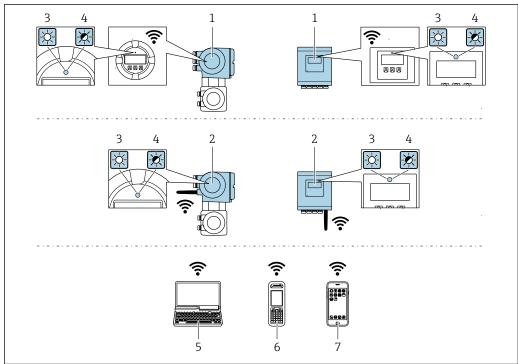

- Transmitter with integrated WLAN antenna
- Transmitter with external WLAN antenna 2
- 3 LED lit constantly: WLAN reception is enabled on measuring instrument
- LED flashing: WLAN connection established between operating unit and measuring instrument
- Computer with WLAN interface and web browser for accessing integrated device web server or with operating tool e.q FieldCare, DeviceCare)
- Mobile handheld terminal with WLAN interface and web browser for accessing integrated device web server or operating tool (e.g. FieldCare, DeviceCare)
- Smartphone or tablet (e.g. Field Xpert SMT70)

MI AN JEEF 000 11 1 / /0 / OU )
WLAN: IEEE 802.11 b/g (2.4 GHz)
• Access point with DHCP server (factory setting)
■ Network
WPA2-PSK AES-128 (in accordance with IEEE 802.11i)
1 to 11
IP66/67
■ Internal antenna
External antenna (optional)
In the event of poor transmission/reception conditions at the place of
installation.
Available as an accessory .
Only 1 antenna is active at any one time!
■ Internal antenna: typically 10 m (32 ft)
External antenna: typically 50 m (164 ft)
Antenna: ASA plastic (acrylonitrile styrene acrylate) and nickel-plated
brass
Adapter: Stainless steel and nickel-plated brass
Cable: Polyethylene
Plug: Nickel-plated brass
Angle bracket: Stainless steel


**Network integration** 

Network integration is only available for the HART communication protocol.

With the optional "OPC UA Server" application package, the device can be integrated into an Ethernet network via the service interface (CDI-RJ45 and WLAN) and communicate with OPC UA clients. If the device is used in this way, IT security must be considered.

For detailed information on connecting transmitters with an Ex de approval, see separate document "Safety instructions" (XA) for the device.

For permanent access to device data and for device configuration via the web server, the device is incorporated directly in a network via the service interface (CDI-RJ45). In this way, the device can be accessed any time from the control station. The measured values are processed separately via the inputs and outputs through the automation system.

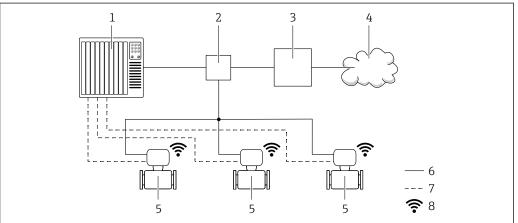

40022616

- 1 Automation system, e.g. Simatic S7 (Siemens)
- 2 Ethernet switch
- 3 Edge Gateway
- 4 Cloud
- 5 Measuring instrument
- 6 Ethernet network
- 7 Measured values via inputs and outputs
- 8 Optional WLAN interface
- i

The optional WLAN interface is available on the following device version: Order code for "Display; operation", option  $\bf G$  "4-line, backlit, graphic display; touch control + WLAN"



Special Documentation for the OPC UA Server application package  $\rightarrow~\cong~119$ .

### Supported operating tools

Different operating tools can be used for local or remote access to the measuring device. Depending on the operating tool used, access is possible with different operating units and via a variety of interfaces.

Supported operating tools	Operating unit	Interface	Additional information
Web browser	Notebook, PC or tablet with web browser	<ul> <li>Service interface CDI-RJ45</li> <li>WLAN interface</li> <li>Ethernet-based fieldbus (EtherNet/IP, PROFINET, Modbus TCP over Ethernet-APL)</li> </ul>	Special Documentation for device → 🖺 119
DeviceCare SFE100	Notebook, PC or tablet with Microsoft Windows system	<ul> <li>Service interface CDI-RJ45</li> <li>WLAN interface</li> <li>Fieldbus protocol</li> <li>Modbus TCP over Ethernet-APL</li> </ul>	→ 🖺 116

Supported operating tools	Operating unit	Interface	Additional information
FieldCare SFE500	Notebook, PC or tablet with Microsoft Windows system	<ul> <li>Service interface CDI- RJ45</li> <li>WLAN interface</li> <li>Fieldbus protocol</li> </ul>	→ 🖺 116
Field Xpert	SMT70/77/50	<ul> <li>All fieldbus protocols</li> <li>WLAN interface</li> <li>Bluetooth</li> <li>Service interface CDI-RJ45</li> </ul>	Operating Instructions BA01202S Device description files: Use update function of handheld terminal

- Other operating tools based on FDT technology with a device driver such as DTM/iDTM or DD/EDD can be used for device operation. These operating tools are available from the individual manufacturers. Integration into the following operating tools, among others, is supported:
  - FactoryTalk AssetCentre (FTAC) from Rockwell Automation → www.rockwellautomation.com
  - Process Device Manager (PDM) from Siemens → www.siemens.com
  - Asset Management Solutions (AMS) from Emerson → www.emersonprocess.com
  - FieldCommunicator 375/475 from Emerson → www.emersonprocess.com
  - Emersons TREX → www.emerson.com
  - Field Device Manager (FDM) from Honeywell → www.process.honeywell.com
  - FieldMate from Yokogawa → www.yokogawa.com
  - PACTWare → www.pactware.com

The related device description files are available: www.endress.com → Download Area

#### Web server

The integrated web server can be used to operate and configure the device via a web browser via Ethernet-APL, via service interface (CDI-RJ45) or via WLAN interface. The structure of the operating menu is the same as for the local display. In addition to the measured values, status information on the device is displayed and can be used to monitor device health. Furthermore the device data can be managed and the network parameters can be configured.

A device that has a WLAN interface (can be ordered as an option) is required for the WLAN connection: order code for "Display; Operation", option G "4-line, illuminated; touch control + WLAN". The device acts as an Access Point and enables communication by computer or a mobile handheld terminal.

#### Supported functions

Data exchange between the operating unit (such as a notebook, for example,) and measuring instrument:

- Upload the configuration from the measuring instrument (XML format, configuration backup)
- Save the configuration to the measuring instrument (XML format, restore configuration)
- Export event list (.csv file)
- Export parameter settings (.csv file or PDF file, document the measuring point configuration)
- Export the Heartbeat Technology verification report (PDF file, only available with the Heartbeat Verification → \( \begin{align\*} \equiv \text{113} \) application package)
- Flash firmware version for device firmware upgrade, for example
- Download driver for system integration
- Visualize up to 1000 saved measured values (only available with the Extended HistoROM application package → 

  113)

### HistoROM data management

The measuring instrument features HistoROM data management. HistoROM data management comprises both the storage and import/export of key device and process data, making operation and servicing far more reliable, secure and efficient.

When the device is delivered, the factory settings of the configuration data are stored as a backup in the device memory. This memory can be overwritten with an updated data record, for example after commissioning.

#### Additional information on the data storage concept

There are different types of data storage units in which device data are stored and used by the device:

	HistoROM backup	T-DAT	S-DAT
Available data	<ul> <li>Event logbook, e.g. diagnostic events</li> <li>Parameter data record backup</li> <li>Device firmware package</li> <li>Driver for system integration for exporting via web server, e.g.:</li> <li>GSD for PROFIBUS DP</li> <li>GSD for PROFIBUS PA</li> <li>GSD for PROFINET</li> <li>EDS for EtherNet/IP</li> <li>DD for FOUNDATION Fieldbus</li> </ul>	Measured value logging ("Extended HistoROM" order option)     Current parameter data record (used by firmware at run time)     Indicator (minimum/maximum values)     Totalizer value	<ul> <li>Sensor data: e.g. nominal diameter</li> <li>Serial number</li> <li>Calibration data</li> <li>Device configuration (e.g. SW options, fixed I/O or multi I/O)</li> </ul>
Storage location	Fixed on the user interface PC board in the connection compartment	Can be plugged into the user interface PC board in the connection compartment	In the sensor plug in the transmitter neck part

#### Data backup

#### **Automatic**

- The most important device data (sensor and transmitter) are automatically saved in the DAT modules
- If the transmitter or measuring device is replaced: once the T-DAT containing the previous device data has been exchanged, the new measuring device is ready for operation again immediately without any errors
- If the sensor is replaced: once the sensor has been replaced, new sensor data are transferred from the S-DAT in the measuring device and the measuring device is ready for operation again immediately without any errors
- If exchanging the electronics module (e.g. I/O electronics module): Once the electronics module has been replaced, the software of the module is compared against the current device firmware. The module software is upgraded or downgraded where necessary. The electronics module is available for use immediately afterwards and no compatibility problems occur.

#### Manual

Additional parameter data record (complete parameter settings) in the integrated device memory HistoROM backup for:

- Data backup function
   Backup and subsequent restoration of a device configuration in the device memory HistoROM backup
- Data comparison function
   Comparison of the current device configuration with the device configuration saved in the device memory HistoROM backup

#### Data transmission

#### Manual

- Transfer of a device configuration to another device using the export function of the specific operating tool, e.g. with FieldCare, DeviceCare or web server: to duplicate the configuration or to store in an archive (e.g. for backup purposes)
- Transmission of the drivers for system integration via web server, e.g.:
  - GSD for PROFIBUS DP
  - GSD for PROFIBUS PA
  - GSD for PROFINET
  - EDS for Ethernet/IP
  - DD for FOUNDATION fieldbus

#### Event list

## Automatic

- Chronological display of up to 20 event messages in the events list
- If the Extended HistoROM application package (order option) is enabled: up to 100 event messages are displayed in the events list along with a time stamp, plain text description and remedial measures
- The events list can be exported and displayed via a variety of interfaces and operating tools e.g. DeviceCare, FieldCare or Web server

### Data logging

#### Manual

If the **Extended HistoROM** application package (order option) is enabled:

- Recording of 1 to 4 channels of up to 1000 measured values (up to 250 measured values per channel)
- User configurable recording interval
- Export the measured value log via a variety of interfaces and operating tools e.g. FieldCare, DeviceCare or web server

# Certificates and approvals

Current certificates and approvals for the product are available at <a href="https://www.endress.com">www.endress.com</a> on the relevant product page:

- 1. Select the product using the filters and search field.
- 2. Open the product page.
- 3. Select **Downloads**.

#### **CE** mark

The device meets the legal requirements of the applicable EU Directives. These are listed in the corresponding EU Declaration of Conformity along with the standards applied.

Endress+Hauser confirms successful testing of the device by affixing to it the CE mark.

#### **UKCA** marking

The device meets the legal requirements of the applicable UK regulations (Statutory Instruments). These are listed in the UKCA Declaration of Conformity along with the designated standards. By selecting the order option for UKCA marking, Endress+Hauser confirms a successful evaluation and testing of the device by affixing the UKCA mark.

Contact address Endress+Hauser UK:

Endress+Hauser Ltd.

Floats Road

Manchester M23 9NF

United Kingdom

www.uk.endress.com

#### RCM marking

The measuring system meets the EMC requirements of the "Australian Communications and Media Authority (ACMA)".

#### Ex approval

The measuring device is certified for use in hazardous areas and the relevant safety instructions are provided in the separate "Safety Instructions" (XA) document. Reference is made to this document on the nameplate.



The separate Ex documentation (XA) containing all the relevant explosion protection data is available from your Endress+Hauser sales center.

#### **Functional safety**

The measuring instrument can be used for flow monitoring systems (min., max., range) up to SIL 2 (single-channel architecture; order code for "Additional approval", option LA) and SIL 3 (multichannel architecture with homogeneous redundancy) and is independently evaluated and certified in accordance with IEC 61508.

The following types of monitoring in safety equipment are possible:

- Mass flow
- Volume flow
- Density



#### **HART** certification

#### **HART** interface

The measuring device is certified and registered by the FieldComm Group. The measuring system meets all the requirements of the following specifications:

- Certified according to HART 7
- The device can also be operated with certified devices of other manufacturers (interoperability)

# FOUNDATION Fieldbus certification

#### FOUNDATION Fieldbus interface

The measuring device is certified and registered by the FieldComm Group. The measuring system meets all the requirements of the following specifications:

- Certified in accordance with FOUNDATION Fieldbus H1
- Interoperability Test Kit (ITK), revision version 6.2.0 (certificate available on request)
- Physical Layer Conformance Test
- The device can also be operated with certified devices of other manufacturers (interoperability)

#### **Certification PROFIBUS**

#### **PROFIBUS** interface

The measuring device is certified and registered by the PNO (PROFIBUS Nutzerorganisation e.V./ PROFIBUS User Organization). The measuring system meets all the requirements of the following specifications:

- Certified according to PA Profile 3.02
- The device can also be operated with certified devices of other manufacturers (interoperability)

#### EtherNet/IP certification

The measuring device is certified and registered by the ODVA (Open Device Vendor Association). The measuring system meets all the requirements of the following specifications:

- Certified in accordance with the ODVA Conformance Test
- EtherNet/IP Performance Test
- EtherNet/IP PlugFest compliance
- The device can also be operated with certified devices of other manufacturers (interoperability)

#### **Certification PROFINET**

#### **PROFINET** interface

The measuring instrument is certified and registered by the PROFIBUS Nutzerorganisation e.V. (PNO). The measuring system meets all the requirements of the following specifications:

- Certified according to:
  - Test specification for PROFINET devices
  - PROFINET Netload Class 2 100 Mbit/s
- The device can also be operated with certified devices of other manufacturers (interoperability).
- The device supports PROFINET S2 system redundancy.

#### PROFINET over Ethernet-APL certification

#### PROFINET interface

The measuring instrument is certified and registered by the PROFIBUS Nutzerorganisation e.V. (PNO). The measuring system meets all the requirements of the following specifications:

- Certified according to:
  - Test specification for PROFINET devices
  - PROFINET PA Profile 4.02
  - PROFINET Netload Robustness Class 2 10 Mbit/s
  - APL conformance test
- The device can also be operated with certified devices of other manufacturers (interoperability)
- The device supports PROFINET S2 system redundancy.

#### Radio approval

The measuring instrument has radio approval.



#### Additional certification

#### CRN approval

Some device versions have CRN approval. A CRN-approved process connection with a CSA approval must be ordered for a CRN-approved device.

#### Tests and certificates

- EN10204-3.1 material certificate, wetted parts and sensor housing (order code for "Test, certificate", option IA)
- Pressure test, internal process, test report (order code for "Test, certificate", option JB)

# External standards and guidelines

■ EN 60529

Degrees of protection provided by enclosure (IP code)

■ IEC/EN 60068-2-6

Environmental influences: Test procedure - Test Fc: vibrate (sinusoidal).

■ IEC/EN 60068-2-31

Environmental influences: Test procedure - Test Ec: shocks due to rough handling, primarily for devices.

■ EN 61010-1

Safety requirements for electrical equipment for measurement, control and laboratory use - general requirements

■ GB 30439.5

Safety requirements for industrial automation products - Part 5: Flowmeter safety requirements

■ EN 61326-1/-2-3

EMC requirements for electrical equipment for measurement, control and laboratory use

■ NAMUR NE 21

Electromagnetic compatibility (EMC) of industrial process and laboratory control equipment

NAMUR NE 32

Data retention in the event of a power failure in field and control instruments with microprocessors

■ NAMUR NE 43

Standardization of the signal level for the breakdown information of digital transmitters with analog output signal.

■ NAMUR NE 53

Software of field devices and signal-processing devices with digital electronics

■ NAMUR NE 105

Specifications for integrating fieldbus devices in engineering tools for field devices

■ NAMUR NE 107

Self-monitoring and diagnostics of field devices

■ NAMUR NE 131

Requirements for field devices for standard applications

■ NAMUR NE 132

Coriolis mass meter

■ ETSI EN 300 328

Guidelines for 2.4 GHz radio components.

■ EN 301489

Electromagnetic compatibility and radio spectrum matters (ERM).

# Ordering information

Detailed ordering information is available from your nearest sales organization www.addresses.endress.com or in the Product Configurator at www.endress.com:

- 1. Select the product using the filters and search field.
- 2. Open the product page.
- Select Configuration.

# Product Configurator - the tool for individual product configuration

- Up-to-the-minute configuration data
- Depending on the device: direct input of information specific to the measuring point, such as the measuring range or operating language
- Automatic verification of exclusion criteria
- Automatic creation of the order code and its breakdown in PDF or Excel output format
- Ability to order directly in the Endress+Hauser Online Shop

# Application packages

Many different application packages are available to enhance the functionality of the device. Such packages might be needed to address safety aspects or specific application requirements.

The application packages can be ordered with the device or subsequently from Endress+Hauser. Detailed information on the order code in question is available from your local Endress+Hauser sales center or on the product page of the Endress+Hauser website: <a href="https://www.endress.com">www.endress.com</a>.



#### Diagnostic functionality

Order code for "Application package", option EA "Extended HistoROM"

Comprises extended functions concerning the event log and the activation of the measured value memory.

Event log:

Memory volume is extended from 20 message entries (standard version) to up to 100 entries.

Data logging (line recorder):

- Memory capacity for up to 1000 measured values is activated.
- 250 measured values can be output via each of the 4 memory channels. The recording interval can
  be defined and configured by the user.
- Measured value logs can be accessed via the local display or operating tool e.g. FieldCare, DeviceCare or Web server.



For detailed information, see the Operating Instructions for the device.

#### **Heartbeat Technology**

Order code for "Application package", option EB "Heartbeat Verification + Monitoring"

#### **Heartbeat Verification**

Meets the requirement for traceable verification in accordance with DIN ISO 9001:2015 Clause 7.6 a) "Control of monitoring and measuring equipment".

- Functional testing in the installed state without interrupting the process.
- Traceable verification results on request, including a report.
- Simple testing process via local operation or other operating interfaces.
- Clear measuring point assessment (pass/fail) with high total test coverage within the framework
  of manufacturer specifications.
- Extension of calibration intervals according to operator's risk evaluation.

#### Heartbeat Monitoring

Continuously supplies data, which are characteristic of the measuring principle, to an external condition monitoring system for the purpose of preventive maintenance or process analysis. These data enable the operator to:

- Draw conclusions using these data and other information about the impact the process influences (e.g. corrosion, abrasion, deposit buildup etc.) have on measuring performance over time.
- Schedule servicing in time.
- Monitor the process or product quality, e.g. gas pockets.



Detailed information on Heartbeat Technology:

Special Documentation → 🖺 118

#### **Concentration measurement**

Order code for "Application package", option ED "Concentration"

Calculation and outputting of fluid concentrations.

The measured density is converted to the concentration of a substance of a binary mixture using the "Concentration" application package:

- Choice of predefined fluids (e.g. various sugar solutions, acids, alkalis, salts, ethanol etc.).
- Common or user-defined units ("Brix, "Plato, % mass, % volume, mol/l etc.) for standard applications.
- Concentration calculation from user-defined tables.



For detailed information, see the Special Documentation for the device.

#### Special density

Order code for "Application package", option EE "Special density"

Many applications use density as a key measured value for monitoring quality or controlling processes. The device measures the density of the fluid as standard and makes this value available to the control system.

The "Special Density" application package offers high-precision density measurement over a wide density and temperature range particularly for applications subject to varying process conditions.

The following information can be found in the calibration certificate supplied:

- Density performance in air
- Density performance in liquids with different density
- Density performance in water with different temperatures



For detailed information, see the Operating Instructions for the device.

#### **OPC-UA Server**

Order code for "Application package", option EL "OPC-UA Server"

The application package provides an integrated OPC-UA server for comprehensive device services for IoT and SCADA applications.



For detailed information, see the Special Documentation for the device.

# Accessories

Various accessories, which can be ordered with the device or subsequently from Endress+Hauser, are available for the device. Detailed information on the order code in question is available from your local Endress+Hauser sales center or on the product page of the Endress+Hauser website: www.endress.com.

#### **Device-specific accessories**

#### For the transmitter

Accessory	Description
Transmitter Proline 500 – digital Proline 500	Transmitter for replacement or storage. Use the order code to define the following specifications:  Approvals  Output  Input  Display/operation  Housing  Software
	<ul> <li>Proline 500 – digital transmitter:         <ul> <li>Order number: 8X5BXX-**********A</li> </ul> </li> <li>Proline 500 transmitter:         <ul> <li>Order number: 8X5BXX-*******</li> </ul> </li> </ul>
	Proline 500 transmitter for replacement: It is essential to specify the serial number of the current transmitter when ordering. On the basis of the serial number, the device-specific data (e.g. calibration factors) of the replaced device can be used for the new transmitter.
	<ul> <li>Proline 500 – digital transmitter: Installation Instructions EA01151D</li> <li>Proline 500 transmitter: Installation Instructions EA01152D</li> </ul>
External WLAN antenna	External WLAN antenna with 1.5 m (59.1 in) connecting cable and two angle brackets. Order code for "Accessory enclosed", option P8 "Wireless antenna wide area".
	<ul> <li>The external WLAN antenna is not suitable for use in hygienic applications.</li> <li>Further information on the WLAN interface → 105.</li> </ul>
	• Order number: 71351317
	Installation Instructions EA01238D
Pipe mounting set	Pipe mounting set for transmitter.
	Proline 500 – digital transmitter Order number: 71346427
	Installation Instructions EA01195D
	Proline 500 transmitter Order number: 71346428

Protective cover Transmitter Proline 500 – digital Proline 500	Is used to protect the measuring instrument from the effects of the weather: e.g. rainwater, excess heating from direct sunlight.  Proline 500 – digital transmitter Order number: 71343504 Proline 500 transmitter Order number: 71343505  Installation Instructions EA01191D
Display guard Proline 500 – digital	Is used to protect the display against impact or scoring, for example from sand in desert areas.  ① Order number: 71228792  ① Installation Instructions EA01093D
Connecting cable Proline 500 – digital Sensor – Transmitter	The connecting cable can be ordered directly with the measuring instrument (order code for "Cable, sensor connection") or as an accessory (order number DK8012).  The following cable lengths are available: order code for "Cable, sensor connection"  Option B: 20 m (65 ft)  Option E: User-configurable up to max. 50 m  Option F: User-configurable up to max. 165 ft  Maximum possible cable length for a Proline 500 – digital connecting cable: 300 m (1000 ft)
Connecting cable Proline 500 Sensor – Transmitter	The connecting cable can be ordered directly with the measuring instrument (order code for "Cable, sensor connection") or as an accessory (order number DK8012).  The following cable lengths are available: order code for "Cable, sensor connection"  Option 1: 5 m (16 ft)  Option 2: 10 m (32 ft)  Option 3: 20 m (65 ft)  Possible cable length for a Proline 500 connecting cable: max. 20 m (65 ft)

# Communication-specific accessories

Accessories	Description		
Commubox FXA195 HART	For intrinsically safe HART communication with FieldCare via the USB interface.  Technical Information TI00404F		
HART loop converter HMX50	Is used to evaluate and convert dynamic HART process variables to analog curre signals or limit values.  Technical Information TI00429F Operating Instructions BA00371F		
Fieldgate FXA42	Transmission of the measured values of connected 4 to 20 mA analog measuring instruments, as well as digital measuring instruments  Technical Information TI01297S Operating Instructions BA01778S Product page: www.endress.com/fxa42		
Field Xpert SMT50	The Field Xpert SMT50 tablet PC for device configuration enables mobile plant asset management in non-hazardous areas. It is suitable for commissioning and maintenance staff to manage field instruments with a digital communication interface and to record progress.  This tablet PC is designed as an all-in-one solution with a preinstalled driver library and is an easy-to-use, touch-sensitive tool which can be used to manage field instruments throughout their entire life cycle.  Technical Information TI01555s  Operating Instructions BA02053S  Product page: www.endress.com/smt50		

Field Xpert SMT70	The Field Xpert SMT70 tablet PC for device configuration enables mobile plant asset management in hazardous and non-hazardous areas. It is suitable for commissioning and maintenance staff to manage field instruments with a digital communication interface and to record progress.  This tablet PC is designed as an all-in-one solution with a preinstalled driver library and is an easy-to-use, touch-sensitive tool which can be used to manage field instruments throughout their entire life cycle.		
	<ul> <li>Technical Information TI01342S</li> <li>Operating Instructions BA01709S</li> <li>Product page: www.endress.com/smt70</li> </ul>		
Field Xpert SMT77	The Field Xpert SMT77 tablet PC for device configuration enables mobile plant asset management in areas categorized as Ex Zone 1.		
	<ul> <li>Technical Information TI01418S</li> <li>Operating Instructions BA01923S</li> <li>Product page: www.endress.com/smt77</li> </ul>		

# Service-specific accessories

Accessory	Description
Applicator	Software for selecting and sizing Endress+Hauser measuring instruments:  Choice of measuring instruments for industrial requirements  Calculation of all the necessary data for identifying the optimum flowmeter: e.g. nominal diameter, pressure loss, flow velocity and measurement accuracy.  Graphic display of the calculation results  Determining the partial order code. Administration, documentation and access to all project-related data and parameters over the entire life cycle of a project.  Applicator is available:
	Via the Internet: https://portal.endress.com/webapp/applicator
Netilion	lloT ecosystem: Unlock knowledge With the Netilion IIoT ecosystem, Endress+Hauser allows you to optimize your plant performance, digitize workflows, share knowledge, and enhance collaboration. Based on decades of experience in process automation, Endress+Hauser offers the process industry an IloT ecosystem that enables you to gain useful insights from data. These insights can be used to optimize processes, leading to increased plant availability, efficiency, and reliability - ultimately resulting in a more profitable plant.  www.netilion.endress.com
FieldCare	FDT-based plant asset management tool from Endress+Hauser. It can configure all intelligent field units in your system and helps you manage them. By using the status information, it is also a simple but effective way of checking their status and condition.  Operating Instructions BA00027S and BA00059S
DeviceCare	Tool to connect and configure Endress+Hauser field devices.  Technical Information: TI01134S Innovation brochure: IN01047S

# System components

Accessories	Description
Memograph M graphic data manager	The Memograph M graphic data manager provides information on all the relevant measured variables. Measured values are recorded correctly, limit values are monitored and measuring points analyzed. The data are stored in the 256 MB internal memory and also on a SD card or USB stick.
	<ul><li>Technical Information TI00133R</li><li>Operating Instructions BA00247R</li></ul>
Cerabar M	The pressure transmitter for measuring the absolute and gauge pressure of gases, steam and liquids. It can be used to read in the operating pressure value.
	<ul> <li>Technical Information TI00426P and TI00436P</li> <li>Operating Instructions BA00200P and BA00382P</li> </ul>

116

Accessories	Description
Cerabar S	The pressure transmitter for measuring the absolute and gauge pressure of gases, steam and liquids. It can be used to read in the operating pressure value.
	<ul><li>Technical Information TI00383P</li><li>Operating Instructions BA00271P</li></ul>
iTEMP	The temperature transmitters can be used in all applications and are suitable for the measurement of gases, steam and liquids. They can be used to read in the medium temperature.
	"Fields of Activity" document FA00006T

# **Documentation**



For an overview of the scope of the associated Technical Documentation, refer to the following:

- Device Viewer (www.endress.com/deviceviewer): Enter the serial number from the nameplate
- Endress+Hauser Operations app: Enter serial number from nameplate or scan matrix code on nameplate.

#### Standard documentation



Supplementary information on the semi-standard options is available in the relevant Special Documentation in the TSP database.

## **Brief Operating Instructions**

Brief Operating Instructions for the sensor

Measuring instrument	Documentation code
Proline Cubemass C	KA01217D

#### *Brief Operating Instructions for the transmitter*

	Documentation code				
Measuring instrument	HART	FOUNDATION Fieldbus	PROFIBUS PA	PROFIBUS DP	Modbus RS485
Proline 500 – digital	KA01315D	KA01233D	KA01392D	KA01390D	KA01319D
Proline 500	KA01314D	KA01291D	KA01391D	KA01389D	KA01318D

## Brief Operating Instructions for the transmitter

	Documentation code				
Measuring instrument	EtherNet/IP	PROFINET	PROFINET over Ethernet-APL	Modbus TCP	
Proline 500 – digital	KA01346D	KA01351D	KA01521D	KA01737D	
Proline 500	KA01347D	KA01350D	KA01520D	KA01736D	

## **Operating Instructions**

Measuring instrument	Documentation code				
	HART	FOUNDATION Fieldbus	PROFIBUS PA	PROFIBUS DP	Modbus RS485
Cubemass C 500	BA01527 D	BA01560D	BA01549D	BA01871D	BA01538D

Measuring		Document	Documentation code		
instrument	EtherNet/IP	PROFINET	PROFINET over Ethernet- APL	Modbus TCP	
Cubemass C 500	BA01748D	BA01759D	BA02123D	BA01538D	

# **Description of Device Parameters**

	Documentation code				
Measuring instrument	HART	FOUNDATION Fieldbus	PROFIBUS PA	PROFIBUS DP	Modbus RS485
Cubemass 500	GP01089D	GP01097D	GP01090D	GP01139D	GP01091D

	Documentation code			
Measuring instrument	EtherNet/IP	PROFINET	PROFINET over Ethernet- APL	Modbus TCP over Ethernet- APL
Cubemass 500	GP01122D	GP01123D	GP01174D	GP01239D

Device-dependent additional documentation

Safety instructions

Safety instructions for electrical equipment for hazardous areas.

Contents	Documentation code
	Measuring instrument
ATEX/IECEx Ex ia	XA01487D
ATEX/IECEx Ex ec	XA01488D
cCSAus IS	XA01489D
cCSAus Ex ia	XA01511D
cCSAus Ex ec	XA01512D
EAC Ex ia	XA03336D
EAC Ex ec	XA03335D
JPN Ex ia	XA01779D
KCs Ex ia	XA03286D
INMETRO Ex ia	XA01491D
INMETRO Ex ec	XA01490D
NEPSI Ex ia	XA01492D
NEPSI Ex ec	XA01493D
UKEX Ex ia	XA02571D
UKEX Ex ec	XA02573D

# **Functional Safety Manual**

Contents	Documentation code
Proline Cubemass 500	SD01728D

#### **Special Documentation**

Contents	Documentation code
Information on the Pressure Equipment Directive	SD01614D
Radio approvals for WLAN interface for A309/A310 display module	SD01793D
OPC UA server 1)	SD02042D
Modbus TCP system integration	SD03383D

1) This Special Documentation is only available for device versions with a HART output.

Contents	Documentation code				
	HART	FOUNDATION Fieldbus	PROFIBUS PA	PROFIBUS DP	Modbus RS485
Web server	SD01674D	SD01677D	SD01676D	SD02234D	SD01675D
Heartbeat Technology	SD01700D	SD01699D	SD01702D	SD02205D	SD01701D
Concentration measurement	SD01716D	SD01717D	SD01719D	SD02215D	SD01718D

Contents	Documentation code			
	PROFINET	EtherNet/IP	PROFINET over Ethernet- APL	Modbus TCP
Web server	SD01975D	SD01974D	SD02770D	-
Heartbeat Technology	SD01991D	SD01985D	SD02734D	SD03353D
Concentration measurement	SD02011D	SD02010D	SD02738D	SD03357D

## **Installation Instructions**

Contents	Note
1 1	The corresponding documentation code is listed with the relevant accessory. $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $

# Registered trademarks

## **HART®**

Registered trademark of the FieldComm Group, Austin, Texas USA  $\,$ 

#### **PROFIBUS**<sup>®</sup>

Registered trademark of the PROFIBUS Nutzerorganisation e.V. (PROFIBUS User Organization), Karlsruhe, Germany

#### FOUNDATION™ fieldbus

Registration-pending trademark of the FieldComm Group, Austin, Texas, USA  $\,$ 

#### Modbus<sup>@</sup>

Registered trademark of SCHNEIDER AUTOMATION, INC.

## Ethernet/IP™

Trademark of ODVA, Inc.

#### Ethernet-APL $^{TM}$

Registered trademark of the PROFIBUS Nutzerorganisation e.V. (PROFIBUS User Organization), Karlsruhe, Germany

#### **PROFINET®**

Registered trademark of the PROFIBUS Nutzerorganisation e.V. (PROFIBUS User Organization), Karlsruhe, Germany

#### TRI-CLAMP®

Registered trademark of Ladish & Co., Inc., Kenosha, USA



www.addresses.endress.com