

# Safety Instructions

## Memosens COS81E

IS Class I Div 1 Groups A, B, C, D

Ex ia op is IIC T6 Ga

Class I Zone 0 AEx ia op is IIC T6 Ga

IS Class II Division 1 Groups E, F, G

Ex ia op is IIIC T90 °C Da

Zone 20 AEx ia op is IIIC T90 °C Da

Safety instructions for electrical apparatus in explosion-hazardous areas




---

# Memosens COS81E

IS Class I Div 1 Groups A, B, C, D  
 Ex ia op is IIC T6 Ga  
 Class I Zone 0 AEx ia op is IIC T6 Ga  
 IS Class II Division 1 Groups E, F, G  
 Ex ia op is IIIC T90 °C Da  
 Zone 20 AEx ia op is IIIC T90 °C Da

## Table of contents

Associated documentation . . . . .	4
Supplementary documentation . . . . .	4
Certificates . . . . .	4
Identification . . . . .	4
Ex-approval . . . . .	4
Safety instructions . . . . .	4
Type code . . . . .	5
Temperature table . . . . .	5
Connection . . . . .	5
Installation conditions . . . . .	6

<b>Associated documentation</b>	This document is an integral part of Operating Instructions BA02066C.
<b>Supplementary documentation</b>	 Competence Brochure CP00021Z <ul style="list-style-type: none"> <li>▪ Explosion Protection: Guidelines and General Principles</li> <li>▪ <a href="http://www.endress.com">www.endress.com</a></li> </ul>
<b>Certificates</b>	<p>The certificates and declarations of conformity are available in the Downloads area of the Endress+Hauser website:</p> <p><a href="http://www.endress.com/download">www.endress.com/download</a></p> <p>CSA C/US certificate, certificate number: CSA20CA80021490X</p>
<b>Identification</b>	<p>The nameplate provides you with the following information on your device:</p> <ul style="list-style-type: none"> <li>▪ Manufacturer identification</li> <li>▪ Order code</li> <li>▪ Extended order code</li> <li>▪ Serial number</li> <li>▪ Safety information and warnings</li> <li>▪ Ex marking on hazardous area versions</li> </ul> <p>► Compare the information on the nameplate with the order.</p>
<b>Ex-approval</b>	<p><b>CSA Ex</b></p> <p>IS Class I Div 1 Groups A, B, C, D</p> <p>Ex ia op is IIC T6 Ga</p> <p>Class I Zone 0 AEx ia op is IIC T6 Ga</p> <p>IS Class II Division 1 Groups E, F, G</p> <p>Ex ia op is IIIC T90 °C Da</p> <p>Zone 20 AEx ia op is IIIC T90 °C Da</p> <p>Details of the fulfilled standards are provided on the certificate.</p>
<b>Safety instructions</b>	<p>The Memosens COS81E oxygen sensor is suitable for use in hazardous areas.</p> <ul style="list-style-type: none"> <li>▪ A maximum ambient temperature of 90 °C (194 °F) must not be exceeded at the sensor head.</li> <li>▪ Oxygen sensors for use in hazardous areas have a special conductive O-ring. The electrical connection of the metallic sensor shaft to the conductive mounting location (such as a metallic assembly) is via the O-ring.</li> <li>▪ Appropriate measures must be taken to connect the assembly or the mounting location to ground in accordance with the Ex guidelines.</li> <li>▪ The plastic housing may only be cleaned with a damp cloth.</li> <li>▪ Hazardous area versions of digital sensors with Memosens technology are marked by an orange/red ring on the plug-in head.</li> <li>▪ The maximum permitted cable length between the sensor and transmitter is 100 m (330 ft).</li> <li>▪ When using devices and sensors, observe the regulations for electrical systems in hazardous areas (EN/IEC 60079-14).</li> <li>▪ The procedures for electrical connection described in the Operating Instructions must be followed.</li> <li>▪ Install the device according to the National Electrical Code (NFPA70) or the Canadian Electrical Code, Part 1 (C22.1), where applicable.</li> <li>▪ Use only as specified in the related manual. Improper use may impair protection.</li> <li>▪ It is the responsibility of the system assembler to ensure the safety of any system that incorporates this equipment.</li> </ul>

Type code


Memosens	COS81E-aabbccdde+g	
	aa	Approval <b>CB</b> CSA C/US IS Cl.1 Div1&2 GP A-D T6 <b>C5</b> CSA C/US IS Cl. I Div 1&2 GP A-D T6 + CSA C/US IS Cl. I Zone 0 AEx ia op is IIC T6 Ga + CSA C/US IS Cl. II Div 1&2 Groups E-G T90 °C+ CSA C/US IS Cl. II Zone 20 AEx ia op is IIIC T90 °C
	bb	Measuring range (all options are certified)
	cc	Cap characteristics AC = Stainless steel C-shape AU = Stainless steel U-shape BC = Titanium C-shape BU = Titanium U-shape CC = Alloy C22 C-shape CU = Alloy C22 U-shape YY = Special version
	dd	Sensor length (all options are certified) max. 600 mm (23,6 in)
	e	Material of O-ring (in the cap)(all options are certified)
	g	Optional = one or more characters determining optional features (all options are certified), e.g. test or other certificates/declarations

Temperature table

Sensor	Process temperature $T_p$	Ambient temperature $T_a$
COS81E	-15 ≤ $T_p$ ≤ 130 °C (T3 rep. T200 °C) -15 ≤ $T_p$ ≤ 120 °C (T4 rep. T135 °C) -15 ≤ $T_p$ ≤ 70 °C (T6 rep. T90°C)	-25 ≤ $T_a$ ≤ 70 °C (T3 rep. T200 °C) -25 ≤ $T_a$ ≤ 90 °C (T4 rep. T135 °C) -25 ≤ $T_a$ ≤ 70 °C (T6 rep. T90°C)

The above temperature table applies only under the following installation conditions, which are described in the following graphic . If the installation conditions cannot be met, the maximum process temperature  $T_p$  must not exceed the maximum ambient temperature  $T_a$ .

Connection

 The sensors can be connected both Class I Division 1 and Class I Division 2: Division 1 equipment can be used in Division 2 as long as they are installed in the same manner as they were intended for Division 1 (NEC 500.8 (B)(2)). This is the case for Memosens sensor with inductive coupling between sensor and cable. There are no different installation methods between sensor and cable. For the cable-transmitter connection the XA of the transmitter must be considered.

Ex specification

The approved Memosens COS81E digital oxygen sensor has an intrinsically safe input with the following parameter set:

Parameter	Value
$P_1$	180 mW


The approved Memosens COS81E digital oxygen sensor uses inherently safe optical radiation:

Parameter	Value
$P_{opt}$ (sensor signal)	≤15 mW

The approved Memosens COS81E digital oxygen sensor must be connected to a Memosens cable or cable transmitter with intrinsically safe output with the following parameter:

Parameter	Value
$P_o$	max. 180 mW

**Installation conditions**

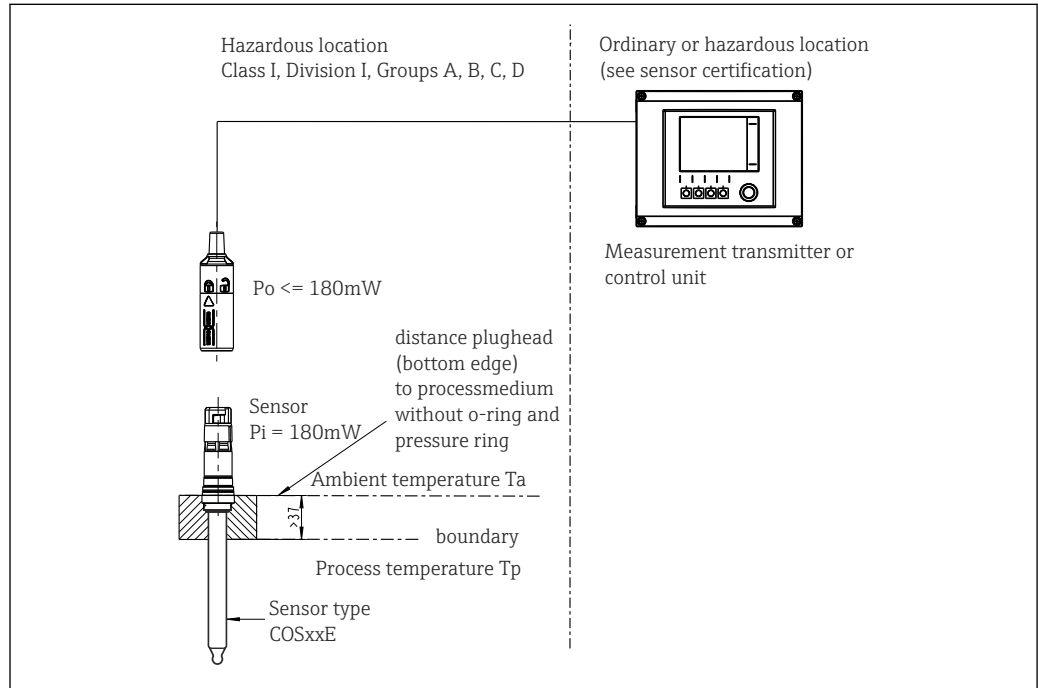

1 Installation conditions

---



[www.addresses.endress.com](http://www.addresses.endress.com)

---