# Technical Information **Proline Promass E 300**

Coriolis flowmeter



# Mid-range Coriolis flowmeter with a compact, easily accessible transmitter

## Application

- Measuring principle operates independently of physical fluid properties such as viscosity or density
- Accurate measurement of liquids and gases for a wide range of standard applications

## Device properties

- Compact dual-tube sensor
- Medium temperature up to +150 °C (+302 °F)
- Process pressure up to 100 bar (1450 psi)
- Compact dual-compartment housing with up to 3 I/Os
- Backlit display with touch control and WLAN access
- Remote display available

## Your benefits

- Cost-effective multipurpose device; an alternative to conventional volumetric flowmeters
- Fewer process measuring points multivariable measurement (flow, density, temperature)
- Space-saving installation no in-/outlet run needs
- Full access to process and diagnostic information numerous, freely combinable I/Os and Ethernet
- Reduced complexity and variety freely configurable I/O functionality
- Integrated verification Heartbeat Technology



# Table of contents

About this document	Environment
Function and system design 5	Climate class
Measuring principle	Relative humidity
Measuring system 6	Operating height
Equipment architecture	Degree of protection
Reliability	Vibration resistance and shock resistance 59
ichabinty	Mechanical load
	Electromagnetic compatibility (EMC) 59
Input	
Measured variable	Process
Measuring range	Medium temperature range
Operable flow range	Medium density 60
Input signal	Pressure/temperature ratings 60
	Sensor housing
Output	Rupture disk
Output and input variants	Internal cleaning
Output signal	Flow limit
Signal on alarm	Pressure loss
Load	Static pressure
Ex connection data	Thermal insulation
Low flow cut off	Heating
Galvanic isolation	Vibrations
Protocol-specific data	
	Mechanical construction 67
Power supply	Dimensions in SI units 67
Terminal assignment	Dimensions in US units
Available device plugs	Weight
Supply voltage	Materials
Power consumption	Process connections
Current consumption	Surface roughness
Power supply failure	Jamase roughness vivivivivivivivivivivivivivi
Overcurrent protection element	0.1111
Electrical connection	Operability
Potential equalization	Operation concept
Terminals	Languages
Cable entries	Local operation
Pin assignment, device plug	Remote operation
Cable specification	Service interface
Overvoltage protection	Network integration
	Supported operating tools
Dowform on an above storieties E1	HistoROM data management
Performance characteristics	
Reference operating conditions	Certificates and approvals 106
Maximum measurement error	CE mark
Repeatability	UKCA marking
Response time	RCM marking
Influence of ambient temperature	Ex approval
Influence of medium temperature	Hygienic compatibility
Influence of medium pressure	Pharmaceutical compatibility
Design fundamentals	Functional safety
	HART certification
Installation	FOUNDATION Fieldbus certification
Mounting location	Certification PROFIBUS
Orientation	EtherNet/IP certification
Inlet and outlet runs	Certification PROFINET
Special installation instructions	PROFINET over Ethernet-APL certification
•	Pressure Equipment Directive

2

Radio approval	109 109 109
Ordering information	110
Application packages Diagnostic functionality Heartbeat Technology Concentration measurement Petroleum Petroleum & locking function OPC-UA Server	110 110 111 111 111 112
Device-specific accessories	112 113 114 114 114
Standard documentation	
Registered trademarks	118

# About this document

# Symbols Electrical symbols

Symbol	Meaning
	Direct current
~	Alternating current
$\overline{}$	Direct current and alternating current
<u></u>	Ground connection A grounded terminal which, as far as the operator is concerned, is grounded via a grounding system.
	Protective earth (PE) Ground terminals that must be connected to ground prior to establishing any other connections.
	The ground terminals are located on the interior and exterior of the device:  Interior ground terminal: protective earth is connected to the mains supply.  Exterior ground terminal: device is connected to the plant grounding system.

# Communication-specific symbols

Symbol	Meaning
<b></b>	Wireless Local Area Network (WLAN) Communication via a wireless, local area network
•	LED LED is off.
<u></u>	LED LED is on.
	LED LED flashing.

# $Symbols \ for \ certain \ types \ of \ information$

Symbol	Meaning
<b>✓</b>	Permitted Procedures, processes or actions that are permitted.
	Preferred Procedures, processes or actions that are preferred.
X	Forbidden Procedures, processes or actions that are forbidden.
i	Tip Indicates additional information.
Ţ <u>i</u>	Reference to documentation
A=	Reference to page
	Reference to graphic
	Visual inspection

## Symbols in graphics

Symbol	Meaning
1, 2, 3,	Item numbers
1., 2., 3.,	Series of steps
A, B, C,	Views
A-A, B-B, C-C,	Sections
EX	Hazardous area
×	Safe area (non-hazardous area)
≋➡	Flow direction

# Function and system design

## Measuring principle

The measuring principle is based on the controlled generation of Coriolis forces. These forces are always present in a system when both translational and rotational movements are superimposed.

 $F_c = 2 \cdot \Delta m (v \cdot \omega)$ 

 $F_c$  = Coriolis force

 $\Delta m = moving mass$ 


 $\omega$  = rotational velocity

 $v = radial \ velocity \ in \ rotating \ or \ oscillating \ system$ 

The amplitude of the Coriolis force depends on the moving mass  $\Delta m$ , its velocity v in the system and thus on the mass flow. Instead of a constant rotational velocity  $\omega$ , the sensor uses oscillation.

In the sensor, two parallel measuring tubes containing flowing medium oscillate in antiphase, acting like a vibrating fork. The Coriolis forces produced at the measuring tubes cause a phase shift in the tube oscillations (see illustration):

- At zero flow (when the medium is at a standstill) the two tubes oscillate in phase (1).
- Mass flow causes deceleration of the oscillation at the inlet of the tubes (2) and acceleration at the outlet (3).

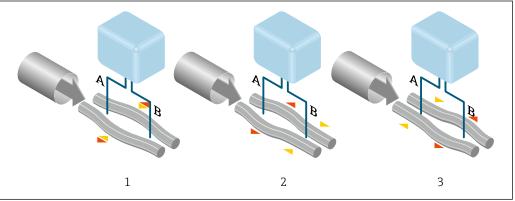

A002885

The phase shift (A-B) increases with increasing mass flow. Electrodynamic sensors register the tube oscillations at the inlet and outlet. System balance is ensured by the antiphase oscillation of the two measuring tubes. The measuring principle operates independently of temperature, pressure, viscosity, conductivity and flow profile.

## Density measurement

The measuring tube is continuously excited at its resonance frequency. A change in the mass and thus the density of the oscillating system (comprising measuring tube and medium) results in a corresponding, automatic adjustment in the oscillation frequency. The resonance frequency is thus a function of the medium density. The microprocessor utilizes this relationship to obtain a density signal.

#### Volume measurement

Together with the measured mass flow, this is used to calculate the volume flow.

## Temperature measurement

The temperature of the measuring tube is determined in order to calculate the compensation factor due to temperature effects. This signal corresponds to the process temperature and is also available as an output signal.

## Gas Fraction Handler (GFH)

The Gas Fraction Handler is a Promass software function that improves measurement stability and repeatability. The function continuously checks for the presence of disturbances in single-phase flow, i.e. gas bubbles in liquids. In the presence of the second phase, flow and density become increasingly unstable. The Gas Fraction Handler function improves measurement stability with respect to the severity of the disturbances, without any effect under single-phase flow conditions.



The Gas Fraction Handler is only available for device versions with HART, Modbus RS485, PROFINET, PROFINET over Ethernet-APL and Modbus TCP over Ethernet-APL.




#### Measuring system

The device consists of a transmitter and a sensor.

The device is available as a compact version:

The transmitter and sensor form a mechanical unit.

#### Transmitter




Device versions and materials:

- Transmitter housing
- Aluminum, coated: aluminum, AlSi10Mg, coated
- Stainless, hygienic: stainless steel, 1.4404
- Material of window in transmitter housing:
  - Aluminum, coated: glass
  - Stainless, hygienic: polycarbonate

#### Configuration:


- External operation via 4-line, illuminated graphic local display (LCD) with touch control and guided menus ("Make-it-run" wizards) for application-specific commissioning.
- Via service interface or WLAN interface:
  - Operating tools (e.g. FieldCare, DeviceCare)
  - Web server (access via web browser)

## Sensor



- Bent dual-tube system
- For standard applications where stable and reliable measurements are required
- Simultaneous measurement of flow, volume flow, density and temperature (multivariable)
- Immune to process influences
- Nominal diameter range: DN 8 to 80 (3/8 to 3")
- Materials:
  - Sensor: stainless steel, 1.4301 (304)
  - Measuring tubes: stainless steel, 1.4539 (904L)
  - Process connections: stainless steel, 1.4404 (316/316L)

## Equipment architecture

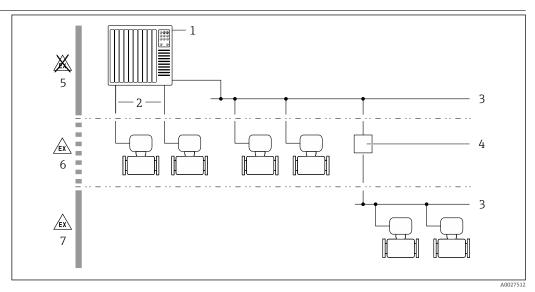

 $\blacksquare 1$  Possibilities for integrating measuring instruments into a system

- 1 Automation system (e.g. PLC)
- 2 Connection cable (0/4 to 20 mA HART etc.)
- 3 Fieldbus
- 4 Coupler
- 5 Non-hazardous area
- 6 Hazardous area: Zone 2; Class I, Division 2
- 7 Hazardous area: Zone 1; Class I, Division 1

# Reliability

## IT security

The manufacturer warranty is valid only if the product is installed and used as described in the Operating Instructions. The product is equipped with security mechanisms to protect it against any inadvertent changes to the settings.

IT security measures, which provide additional protection for the product and associated data transfer, must be implemented by the operators themselves in line with their security standards.

## **Device-specific IT security**

The device offers a range of specific functions to support protective measures on the operator's side. These functions can be configured by the user and guarantee greater in-operation safety if used correctly. The following list provides an overview of the most important functions:

Function/interface	Factory setting	Recommendation
Write protection via hardware write protection switch $\rightarrow \stackrel{ riangle}{ riangle} 8$	Not enabled	On an individual basis following risk assessment
Access code (also applies to web server login or FieldCare connection) → 🖺 8	Not enabled (0000)	Assign a customized access code during commissioning
WLAN (order option in display module)	Enabled	On an individual basis following risk assessment
WLAN security mode	Enabled (WPA2- PSK)	Do not change
WLAN passphrase (Password) → 🖺 8	Serial number	Assign an individual WLAN passphrase during commissioning
WLAN mode	Access point	On an individual basis following risk assessment
Web server → 🖺 8	Enabled	On an individual basis following risk assessment
Service interface CDI-RJ45 → 🖺 9	Enabled	-

Protecting access via hardware write protection

Write access to the parameters of the device via the local display, web browser or operating tool (e.g. FieldCare, DeviceCare) can be disabled via a write protection switch (DIP switch on the main electronics module). When hardware write protection is enabled, only read access to the parameters is possible.

Hardware write protection is disabled when the device is delivered.

## Protecting access via a password

Different passwords are available to protect write access to the device parameters or access to the device via the WLAN interface.

User-specific access code

Protect write access to the device parameters via the local display, web browser or operating tool (e.g. FieldCare, DeviceCare). Access authorization is clearly regulated through the use of a user-specific access code.

WLAN passphrase

The network key protects a connection between an operating unit (e.g. notebook or tablet) and the device via the WLAN interface which can be ordered as an option.

Infrastructure mode

When the device is operated in infrastructure mode, the WLAN passphrase corresponds to the WLAN passphrase configured on the operator side.

User-specific access code

Local display, web browser and operating tool (e.g. FieldCare, DeviceCare)

- Write access to the device parameters via the local display, web browser or operating tool (e.g. FieldCare, DeviceCare) can be protected by the modifiable, user-specific access code.
- When delivered, the device does not have an access code; the default value is 0000 (open).

WLAN passphrase: Operation as WLAN access point

A connection between an operating unit (e.g. notebook or tablet) and the device via the WLAN interface, which can be ordered as an optional extra, is protected by the network key. The WLAN authentication of the network key complies with the IEEE 802.11 standard.

When the device is delivered, the network key is pre-defined depending on the device. It can be changed via the **WLAN settings** submenu in the **WLAN passphrase** parameter.

Infrastructure mode

A connection between the device and WLAN access point is protected by means of an SSID and passphrase on the system side. Please contact the relevant system administrator for access.

General notes on the use of passwords

- The access code and network key supplied with the device should be changed during commissioning for security reasons.
- Follow the general rules for generating a secure password when defining and managing the access code or network kev.
- The user is responsible for the management and careful handling of the access code and network key.

Access via web server

The integrated web server can be used to operate and configure the device via a web browser. The connection is established via the service interface (CDI-RJ45) or WLAN interface . For device versions with the Ethernet/IP and PROFINET communication protocols, the connection can also be established via the terminal connection for signal transmission with Ethernet/IP, PROFINET (RJ45 plug), PROFINET over Ethernet-APL (two-wire) or Modbus TCP over Ethernet-APL.

The web server is enabled when the device is delivered. The web server can be disabled if necessary via the **Web server functionality** parameter (e.g., after commissioning).

The device and status information can be hidden on the login page. This prevents unauthorized access to the information.

For detailed information on device parameters, see: Description of Device Parameters.

## Access via OPC UA



The device can communicate with OPC UA clients using the "OPC UA Server" application package.

The OPC UA server integrated in the device can be accessed via the WLAN access point using the WLAN interface - which can be ordered as an optional extra - or the service interface (CDI-RJ45) via Ethernet network. Access rights and authorization as per separate configuration.

The following Security Modes are supported as per the OPC UA Specification (IEC 62541):

- Without
- Basic128Rsa15 signed
- Basic128Rsa15 signed and encrypted

Access via service interface (port 2): CDI-RJ45

The device can be connected to a network via the service interface. Device-specific functions quarantee the secure operation of the device in a network.

The use of relevant industrial standards and guidelines that have been defined by national and international safety committees, such as IEC/ISA62443 or the IEEE, is recommended. This includes organizational security measures such as the assignment of access authorization as well as technical measures such as network segmentation.



## PROFINET, Ethernet/IP:

The device can be integrated into a ring topology. The device is integrated via the terminal connection for signal transmission, output 1 (port 1) and the terminal connection to the service interface (port  $2) \rightarrow \implies 101$ .



For detailed information on connecting transmitters with an Ex de approval, see separate document "Safety instructions" (XA) for the device.

#### Advanced safety requirements

If the specified requirements for measures cannot be met, alternative measures may need to be put in place. This may involve, for example, mechanical protection of the product against tampering, the cabling, or organizational measures. The Proline measuring instruments can be used in the open field for example. Measures to combat physical tampering of the Proline measuring instruments must be arranged by the customer.

Additional analysis is required if Proline measuring instruments are integrated into a different system. Please note the following:

- The fieldbus network (OT) and company network (IT) must be strictly separated.
- Endress+Hauser recommends the segmentation of the fieldbus networks according to DIN IEC 62443-3-3.

## Network

Pay particular attention to the network components used, the router and switches for example. The operator must guarantee the integrity of the components. Access to the network must be restricted by the operator, if necessary.

## FDI Packages

Signed FDI Packages can be obtained via www.endress.com for the configuration of the field device.

# User training

Depending on the application scenario, users who are not specialized in this area may come in contact with the instrument. We recommend that these users be trained in the safe use of the relevant terminals, components and/or interfaces and be made aware of security issues.

# Input

## Measured variable

## Direct measured variables

- Mass flow
- Density
- Temperature

# Calculated measured variables

- Volume flow
- Corrected volume flow
- Reference density

## Measuring range

# Measuring range for liquids

DN		Measuring range full scale values $\dot{m}_{min(F)}$ to $\dot{m}_{max(F)}$	
[mm]	[in]	[kg/h]	[lb/min]
8	3/8	0 to 2 000	0 to 73.50
15	1/2	0 to 6 500	0 to 238.9
25	1	0 to 18000	0 to 661.5
40	1½	0 to 45 000	0 to 1654
50	2	0 to 70 000	0 to 2 573
80	3	0 to 180 000	0 to 6615

## Measuring range for gases

The full scale value depends on the density and the speed of sound of the gas used. The full scale value can be calculated with the following formulas:

$$\dot{m}_{~max\,(G)}$$
 = minimum of 
$$(\dot{m}_{max(F)}\cdot\rho_G:x~)~and$$
 
$$(\rho_G\cdot(c_G/2)\cdot d_i{}^2\cdot(\pi/4)\cdot 3600\cdot n)$$

m <sub>max(G)</sub>	Maximum full scale value for gas [kg/h]	
m <sub>max(F)</sub>	Maximum full scale value for liquid [kg/h]	
$\dot{m}_{\max(G)} < \dot{m}_{\max(F)}$	$\dot{m}_{max(G)}$ can never be greater than $\dot{m}_{max(F)}$	
$\rho_{G}$	Gas density in [kg/m³] at operating conditions	
х	Limitation constant for max. gas flow [kg/m³]	
$\mathbf{c}_{G}$	Speed of sound (gas) [m/s]	
d <sub>i</sub>	Measuring tube internal diameter [m]	
π	Pi	
n = 2	Number of measuring tubes	

DN		х
[mm]	[in]	[kg/m³]
8	3/8	85
15	1/2	110
25	1	125
40	1½	125

DN		х
[mm]	[in]	[kg/m³]
50	2	125
80	3	155

To calculate the measuring range, use the Applicator sizing tool ightarrow  $\cong$  114

If calculating the full scale value using the two formulas:

- 1. Calculate the full scale value with both formulas.
- 2. The smaller value is the value that must be used.

#### Recommended measuring range



Flow limit  $\rightarrow \triangleq 65$ 

## Operable flow range

Over 1000:1.

Flow rates above the preset full scale value do not override the electronics unit, with the result that the totalizer values are registered correctly.

## Input signal

## Output and input variants

→ 🖺 13

## External measured values

To increase the measurement accuracy of certain measured variables or to calculate the corrected volume flow for gases, the automation system can continuously write different measured values to the measuring instrument:

- Operating pressure to increase measurement accuracy (Endress+Hauser recommends the use of a pressure measuring instrument for absolute pressure, e.g. Cerabar M or Cerabar S)
- Medium temperature to increase measurement accuracy (e.g. iTEMP)
- Reference density for calculating the corrected volume flow for gases
- Various pressure and temperature measuring devices can be ordered from Endress+Hauser: see "Accessories" section  $\Rightarrow riangleq 114$

It is recommended to read in external measured values to calculate the corrected volume flow.

## HART protocol

The measured values are written from the automation system to the measuring device via the HART protocol. The pressure transmitter must support the following protocol-specific functions:

- HART protocol
- Burst mode

## Current input

## Digital communication

The measured values can be written by the automation system via:

- FOUNDATION Fieldbus
- PROFIBUS DP
- PROFIBUS PA
- Modbus RS485
- Modbus TCP over Ethernet-APL
- EtherNet/IP
- PROFINET
- PROFINET over Ethernet-APL

# Current input 0/4 to 20 mA

Current input	0/4 to 20 mA (active/passive)
Current span	<ul> <li>4 to 20 mA (active)</li> <li>0/4 to 20 mA (passive)</li> </ul>
Resolution	1 μΑ
Voltage drop	Typically: 0.6 to 2 V for 3.6 to 22 mA (passive)
Maximum input voltage	≤ 30 V (passive)
Open-circuit voltage	≤ 28.8 V (active)
Possible input variables	<ul><li>Pressure</li><li>Temperature</li><li>Density</li></ul>

# Status input

Maximum input values	■ DC $-3$ to 30 V ■ If status input is active (ON): $R_i > 3 \text{ k}\Omega$
Response time	Configurable: 5 to 200 ms
Input signal level	<ul> <li>Low signal: DC -3 to +5 V</li> <li>High signal: DC 12 to 30 V</li> </ul>
Assignable functions	<ul> <li>Off</li> <li>Reset the individual totalizers separately</li> <li>Reset all totalizers</li> <li>Flow override</li> </ul>

# Output

## Output and input variants

Depending on the option selected for output/input 1, different options are available for the other outputs and inputs. Only one option can be selected for each output/input 1 to 3. The following tables must be read vertically  $(\downarrow)$ .

Example: If the option BA "4-20 mA HART" was selected for output/input 1, one of the options A, B, D, E, F, H, I or J is available for output 2 and one of the options A, B, D, E, F, H, I or J is available for output 3.

## Output/input 1 and options for output/input 2



Options for output/input  $3 \rightarrow 14$ 

Order code for "Output; input 1" (020) →							Poss	ible o	ption	s					
Current output 4 to 20 mA HART	ВА														
Current output 4 to 20 mA HART Ex i passive	<b>4</b>	CA													
Current output 4 to 20 mA HART Ex i active		<b>4</b>	СС												
FOUNDATION fieldbus			<b>4</b>	SA											
FOUNDATION fieldbus Ex i				4	TA										
PROFIBUS DP					<b>\</b>	LA									
PROFIBUS PA						<b>\</b>	GA								
PROFIBUS PA Ex i							<b>\</b>	НА							
Modbus RS485								<b>\</b>	MA						
Ethernet/IP 2-port switch integrated									<b>\</b>	NA					
PROFINET 2-port switch integrated										4	RA				
PROFINET over Ethernet-APL											4	RB			
PROFINET over Ethernet-APL Ex i												1	RC		
Modbus TCP over Ethernet-APL 10 Mbit/s, SPE 10 Mbit/s, Ethernet 100 Mbit/s													<b>\</b>	МВ	
Modbus TCP over Ethernet-APL, Ex i, 10 Mbit/s, Ethernet 100 Mbit/s														4	МС
Order code for "Output; input 2" (021) →	<b>\</b>	4	<b>\</b>	4	<b>\</b>	<b>\</b>	<b>\</b>	<b>\</b>	<b>\</b>	4	1	1	<b>\</b>	<b>\</b>	<b>\</b>
Not used	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α
Current output 4 to 20 mA	В			В		В	В		В	В	В	В		В	
Current output 4 to 20 mA Ex i passive		С	С		С			С					С		С
User-configurable input/output 1)	D			D		D	D		D	D	D	D		D	
Pulse/frequency/switch output	Е			Е		Е	Е		Е	Е	Е	Е		Е	
Double pulse output <sup>2)</sup>	F								F						
Pulse/frequency/switch output Ex i passive		G	G		G			G					G		G
Relay output	Н			Н		Н	Н		Н	Н	Н	Н		Н	
Current input 0/4 to 20 mA	I			I		I	I		I	I	I	I		I	
Status input	J			J		J	J		J	J	J	J		J	

<sup>2)</sup> If double pulse output (F) is selected for output/input 2 (021), only the double pulse output (F) option is available for selection for output/input 3 (022).

# Output/input 1 and options for output/input 3 $\,$

Order code for "Output; input 1" (020) →	Possible options														
Current output 4 to 20 mA HART	ВА														
Current output 4 to 20 mA HART Ex i passive	<b>\</b>	CA													
Current output 4 to 20 mA HART Ex i active		<b>\</b>	СС												
FOUNDATION fieldbus			<b>\</b>	SA											
FOUNDATION fieldbus Ex i				4	TA										
PROFIBUS DP					4	LA									
PROFIBUS PA						4	GA								
PROFIBUS PA Ex i							<b>\</b>	НА							
Modbus RS485								4	MA						
Ethernet/IP 2-port switch integrated									<b>\</b>	NA					
PROFINET 2-port switch integrated										4	RA				
PROFINET over Ethernet-APL 10 Mbit/s, 2-wire											4	RB			
PROFINET over Ethernet-APL Ex i, 10 Mbit/s, 2-wire												4	RC		
Modbus TCP over Ethernet-APL 10 Mbit/s, SPE 10 Mbit/s, Ethernet 100 Mbit/s													4	МВ	
Modbus TCP over Ethernet-APL, Ex i, 10 Mbit/s, Ethernet 100 Mbit/s														4	МС
Order code for "Output; input 3" (022) →	<b>\</b>	<b>\</b>	<b>\</b>	<b>\</b>	<b>\</b>	<b>\</b>	<b>\</b>	<b>\</b>	<b>\</b>	<b>\</b>	<b>\</b>	<b>\</b>	<b>4</b>	<b>\</b>	<b>\</b>
Not used	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α	Α
Current output 4 to 20 mA	В					В			В	В	В	В		В	
Current output 4 to 20 mA Ex i passive		С	С												
User-configurable input/output	D					D			D	D	D	D		D	
Pulse/frequency/switch output	Е					Е			Е	Е	Е	Е		Е	
Double pulse output (slave) 1)	F								F						
Pulse/frequency/switch output Ex i passive		G	G												
Relay output	Н					Н			Н	Н	Н	Н		Н	
Current input 0/4 to 20 mA	I					I			I	I	I	I		I	
Status input	J					J			J	J	J	J		J	

<sup>1)</sup> If double pulse output (F) is selected for output/input 2 (021), only the double pulse output (F) option is available for output/input 3 (022).

14

# Output signal

# Current output 4 to 20 mA HART

Order code	"Output; input 1" (20): Option BA: current output 4 to 20 mA HART
Signal mode	Can be set to: Active Passive
Current range	Can be set to:  4 to 20 mA NAMUR  4 to 20 mA US  4 to 20 mA  0 to 20 mA (only if the signal mode is active)  Fixed current
Open-circuit voltage	DC 28.8 V (active)
Maximum input voltage	DC 30 V (passive)
Load	250 to 700 Ω
Resolution	0.38 μΑ
Damping	Configurable: 0 to 999.9 s
Assignable measured variables	<ul> <li>Mass flow</li> <li>Volume flow</li> <li>Corrected volume flow</li> <li>Density</li> <li>Reference density</li> <li>Temperature</li> <li>Electronics temperature</li> <li>Oscillation frequency 0</li> <li>Oscillation damping 0</li> <li>Signal asymmetry</li> <li>Exciter current 0</li> <li>The range of options increases if the measuring device has one or more application packages.</li> </ul>

# Current output 4 to 20 mA HART Ex i

Order code	"Output; input 1" (20) choose from:  Option CA: current output 4 to 20 mA HART Ex i passive  Option CC: current output 4 to 20 mA HART Ex i active
Signal mode	Depends on the selected order version.
Current range	Can be set to:  4 to 20 mA NAMUR  4 to 20 mA US  4 to 20 mA  0 to 20 mA  for index is active)  Fixed current
Open-circuit voltage	DC 21.8 V (active)
Maximum input voltage	DC 30 V (passive)
Load	<ul> <li>250 to 400 Ω (active)</li> <li>250 to 700 Ω (passive)</li> </ul>
Resolution	0.38 μΑ

Damping	Configurable: 0 to 999.9 s
Assignable measured variables	<ul> <li>Mass flow</li> <li>Volume flow</li> <li>Corrected volume flow</li> <li>Density</li> <li>Reference density</li> <li>Temperature</li> <li>Electronics temperature</li> <li>Oscillation frequency 0</li> <li>Oscillation damping 0</li> <li>Signal asymmetry</li> <li>Exciter current 0</li> <li>The range of options increases if the measuring device has one or more application packages.</li> </ul>

# FOUNDATION Fieldbus

FOUNDATION Fieldbus	H1, IEC 61158-2, galvanically isolated
Data transfer	31.25 kbit/s
<b>Current consumption</b>	10 mA
Permitted supply voltage	9 to 32 V
Bus connection	With integrated reverse polarity protection

# PROFIBUS DP

Signal encoding	NRZ code
Data transfer	9.6 kBaud12 MBaud
Terminating resistor	Integrated, can be activated via DIP switches

# PROFIBUS PA

PROFIBUS PA	In accordance with EN 50170 Volume 2, IEC 61158-2 (MBP), galvanically isolated
Data transmission	31.25 kbit/s
<b>Current consumption</b>	10 mA
Permitted supply voltage	9 to 32 V
Bus connection	With integrated reverse polarity protection

# Modbus RS485

Physical interface	RS485 in accordance with EIA/TIA-485 standard
Terminating resistor	Integrated, can be activated via DIP switches

# Modbus TCP over Ethernet-APL

Port 1: Modbus TCP over Et	hernet-APL 10 Mbit/s
Device usage	Device connection to an APL field switch (terminal 26/27) The device may only be operated according to the following APL port classifications:  If used in hazardous areas: SLAA or SLAC 1)  If used in non-hazardous areas: SLAX
	Connection values of APL field switch (corresponds to APL port classification SPCC or SPAA, for instance):
	<ul> <li>Maximum input voltage: 15 V<sub>DC</sub></li> <li>Minimum output values: 0.54 W</li> </ul>
	Device connection to an SPE switch ■ In non-hazardous areas, the device can be used with an appropriate SPE switch: ■ Maximum output voltage: 30 V <sub>DC</sub> ■ Minimum output power: 1.85 W ■ The SPE switch must support the 10BASE-T1L standard and PoDL power classes 10, 11 or 12 and have a function to disable power class detection.
Standards	According to IEEE 802.3cg, APL port profile specification v1.0, galvanically isolated
Data transfer	Full-duplex (APL/SPE)
Current consumption	Terminal 26/27 max. approx. 45 mA
Permitted supply voltage	9 to 30 V
Bus connection	Terminal 26/27 with integrated reverse polarity protection

 $1) \qquad \hbox{For more information on using the device in the hazardous area, see the Ex-specific Safety Instructions}$ 

Port 2: Modbus TCP over Ethernet 100 Mbit/s					
Device usage	Device connection to a Fast Ethernet (RJ45) switch In non-hazardous areas, the Ethernet switch must support the standard 100BASE-TX.				
Standards	In accordance with IEEE 802.3u				
Data transfer	Half-duplex, full-duplex				
Current consumption	-				
Permitted supply voltage	-				
Bus connection	Service interface (RJ45)				

## EtherNet/IP

Standards	In accordance with IEEE 802.3
-----------	-------------------------------

# PROFINET

Standards	In accordance with IEEE 802.3

# PROFINET over Ethernet-APL

Device use	Device connection to an APL field switch  The device may only be operated according to the following APL port classifications:  ■ If used in hazardous areas: SLAA or SLAC ¹¹  ■ If used in non-hazardous areas: SLAX  Connection values of APL field switch (corresponds to APL port classification SPCC or SPAA, for instance):  ■ Maximum input voltage: 15 V <sub>DC</sub>
	<ul> <li>Minimum output values: 0.54 W</li> <li>Device connection to an SPE switch</li> <li>In non-hazardous areas, the device can be used with an appropriate SPE switch: The device can be connected to an SPE switch with a maximum voltage of 30 V<sub>DC</sub> and a minimum output power of 1.85 W connected.</li> <li>The SPE switch must support the 10BASE-T1L standard and PoDL power classes 10, 11 or 12 and have a function to disable power class detection.</li> </ul>
PROFINET	According to IEC 61158 and IEC 61784
Ethernet-APL	According to IEEE 802.3cg, APL port profile specification v1.0, galvanically isolated
Data transfer	10 Mbit/s
Current consumption	Transmitter  • Max. 400 mA(24 V)  • Max. 200 mA (110 V, 50/60 Hz; 230 V, 50/60 Hz)
Permitted supply voltage	9 to 30 V
Network connection	With integrated reverse polarity protection

For more information on using the device in the hazardous area, see the Ex-specific Safety Instructions 1)

# Current output 4 to 20 mA

Order code	"Output; input 2" (21), "Output; input 3" (022): Option B: current output 4 to 20 mA
Signal mode	Can be set to:  Active Passive
Current range	Can be set to:  4 to 20 mA NAMUR  4 to 20 mA US  4 to 20 mA  0 to 20 mA  for independent of the signal mode is active)  Fixed current
Maximum output values	22.5 mA
Open-circuit voltage	DC 28.8 V (active)
Maximum input voltage	DC 30 V (passive)
Load	$0$ to $700\Omega$
Resolution	0.38 μΑ

Assignable measured variables  - Mass flow - Volume flow - Corrected volume flow - Density - Reference density - Temperature - Electronics temperature - Oscillation frequency 0	Damping	Configurable: 0 to 999.9 s
<ul> <li>Oscillation damping 0</li> <li>Signal asymmetry</li> <li>Exciter current 0</li> <li>The range of options increases if the measuring device has one or more application packages.</li> </ul>	Assignable measured	<ul> <li>Mass flow</li> <li>Volume flow</li> <li>Corrected volume flow</li> <li>Density</li> <li>Reference density</li> <li>Temperature</li> <li>Electronics temperature</li> <li>Oscillation frequency 0</li> <li>Oscillation damping 0</li> <li>Signal asymmetry</li> <li>Exciter current 0</li> <li>The range of options increases if the measuring device has one or more</li> </ul>

# Current output 4 to 20 mA Ex i passive

Order code	"Output; input 2" (21), "Output; input 3" (022): Option C: current output 4 to 20 mA Ex i passive
Signal mode	Passive
Current range	Can be set to:  4 to 20 mA NAMUR  4 to 20 mA US  4 to 20 mA  Fixed current
Maximum output values	22.5 mA
Maximum input voltage	DC 30 V
Load	0 to 700 $\Omega$
Resolution	0.38 μΑ
Damping	Configurable: 0 to 999 s
Assignable measured variables	<ul> <li>Mass flow</li> <li>Volume flow</li> <li>Corrected volume flow</li> <li>Density</li> <li>Reference density</li> <li>Temperature</li> <li>Electronics temperature</li> <li>Oscillation frequency 0</li> <li>Oscillation damping 0</li> <li>Signal asymmetry</li> <li>Exciter current 0</li> <li>The range of options increases if the measuring device has one or more application packages.</li> </ul>

# Pulse/frequency/switch output

Function	Can be configured as pulse, frequency or switch output
Version	Open collector  Can be set to:     Active     Passive     Passive NAMUR  Ex-i, passive
Maximum input values	DC 30 V, 250 mA (passive)
Open-circuit voltage	DC 28.8 V (active)
Voltage drop	For 22.5 mA: ≤ DC 2 V

Pulse output	
Maximum input values	DC 30 V, 250 mA (passive)
Maximum output current	22.5 mA (active)
Open-circuit voltage	DC 28.8 V (active)
Pulse width	Configurable: 0.05 to 2 000 ms
Maximum pulse rate	10 000 Impulse/s
Pulse value	Configurable
Assignable measured variables	<ul> <li>Mass flow</li> <li>Volume flow</li> <li>Corrected volume flow</li> <li>The range of options increases if the measuring device has one or more application packages.</li> </ul>
Frequency output	
Maximum input values	DC 30 V, 250 mA (passive)
Maximum output current	22.5 mA (active)
Open-circuit voltage	DC 28.8 V (active)
Output frequency	Configurable: end value frequency 2 to $10000Hz(f_{max}=12500Hz)$
Damping	Configurable: 0 to 999.9 s
Pulse/pause ratio	1:1
Assignable measured variables	<ul> <li>Mass flow</li> <li>Volume flow</li> <li>Corrected volume flow</li> <li>Density</li> <li>Reference density</li> <li>Temperature</li> <li>Electronics temperature</li> <li>Oscillation frequency 0</li> <li>Oscillation damping 0</li> <li>Signal asymmetry</li> <li>Exciter current 0</li> <li>The range of options increases if the measuring device has one or more application packages.</li> </ul>
Switch output	
Maximum input values	DC 30 V, 250 mA (passive)
Open-circuit voltage	DC 28.8 V (active)
Switching behavior	Binary, conductive or non-conductive

Number of switching cycles	Unlimited
Assignable functions	<ul> <li>Disable</li> <li>On</li> <li>Diagnostic behavior</li> <li>Limit</li> <li>Mass flow</li> <li>Volume flow</li> <li>Corrected volume flow</li> <li>Density</li> <li>Reference density</li> <li>Temperature</li> <li>Totalizer 1-3</li> <li>Flow direction monitoring</li> <li>Status</li> <li>Partially filled pipe detection</li> <li>Low flow cut off</li> <li>The range of options increases if the measuring device has one or more application packages.</li> </ul>

# Double pulse output

Function	Double pulse
Version	Open collector
	Can be set to:  Active Passive Passive NAMUR
Maximum input values	DC 30 V, 250 mA (passive)
Open-circuit voltage	DC 28.8 V (active)
Voltage drop	For 22.5 mA: ≤ DC 2 V
Output frequency	Configurable: 0 to 1000 Hz
Damping	Configurable: 0 to 999 s
Pulse/pause ratio	1:1
Assignable measured variables	<ul> <li>Mass flow</li> <li>Volume flow</li> <li>Corrected volume flow</li> <li>Density</li> <li>Reference density</li> <li>Temperature</li> <li>The range of options increases if the measuring device has one or more application packages.</li> </ul>

# Relay output

Function	Switch output
Version	Relay output, galvanically isolated
Switching behavior	Can be set to: NO (normally open), factory setting NC (normally closed)

Maximum switching capacity (passive)	■ DC 30 V, 0.1 A ■ AC 30 V, 0.5 A
Assignable functions	<ul> <li>Disable</li> <li>On</li> <li>Diagnostic behavior</li> <li>Limit</li> <li>Mass flow</li> <li>Volume flow</li> <li>Corrected volume flow</li> <li>Density</li> <li>Reference density</li> <li>Temperature</li> <li>Totalizer 1-3</li> <li>Flow direction monitoring</li> <li>Status</li> <li>Partially filled pipe detection</li> <li>Low flow cut off</li> </ul>
	The range of options increases if the measuring device has one or more application packages.

## User-configurable input/output

**One** specific input or output is assigned to a user-configurable input/output (configurable I/O) during device commissioning.

The following inputs and outputs are available for assignment:

- Choice of current output: 4 to 20 mA (active), 0/4 to 20 mA (passive)
- Pulse/frequency/switch output
- Choice of current input: 4 to 20 mA (active), 0/4 to 20 mA (passive)
- Status input

The technical values correspond to those of the inputs and outputs described in this section.

# Signal on alarm

Depending on the interface, failure information is displayed as follows:

# **HART** current output

Device diagnostics	Device condition can be read out via HART Command 48
--------------------	--

## PROFIBUS PA

Status and alarm messages	Diagnostics in accordance with PROFIBUS PA Profile 3.02
Failure current FDE (Fault Disconnection Electronic)	0 mA

# PROFIBUS DP

Status and alarm	Diagnostics in accordance with PROFIBUS PA Profile 3.02
messages	

# EtherNet/IP

Device diagnostics	Device condition can be read out in Input Assembly
--------------------	--

## **PROFINET**

# PROFINET over Ethernet-APL

Device diagnostics	Diagnostics according to PROFINET PA Profile 4.02
--------------------	---

# FOUNDATION Fieldbus

Status and alarm messages	Diagnostics in accordance with FF-891
Failure current FDE (Fault Disconnection Electronic)	0 mA

# Modbus RS485

Failure mode	Choose from:
	■ NaN value instead of current value
	■ Last valid value

# Modbus TCP over Ethernet-APL/SPE/Fast Ethernet

Failure mode	Choose from:
	■ NaN value instead of current value
	■ Last valid value

# **Current output**

Current output 4-20 mA	
Failure mode	Configurable:  4 to 20 mA in accordance with NAMUR recommendation NE 43  4 to 20 mA in accordance with US  Min. value: 3.59 mA  Max. value: 22.5 mA  Definable value between: 3.59 to 22.5 mA  Actual value  Last valid value
Current output 4-20 mA	
Failure mode	Configurable:  Maximum alarm: 22 mA  Definable value between: 0 to 20.5 mA

# Pulse/frequency/switch output

Pulse output	
Failure mode	Configurable:  Actual value  No pulses
Frequency output	
Failure mode	Configurable:  Actual value  O Hz  Definable value between: 2 to 12 500 Hz
Switch output	
Failure mode	Configurable:  Current status  Open Closed

## Relay output

Failure mode	Choose from:
	<ul> <li>Current status</li> </ul>
	■ Open
	■ Closed

# Local display

Plain text display	With information on cause and remedial measures	
Backlight	Red lighting indicates a device error.	



Status signal as per NAMUR recommendation NE 107

## Interface/protocol

- Via digital communication:
  - HART protocol
  - FOUNDATION Fieldbus
  - PROFIBUS PA
  - PROFIBUS DP
  - Modbus RS485
  - Modbus TCP over Ethernet-APL
  - EtherNet/IP
  - PROFINET
  - PROFINET over Ethernet-APL
- Via service interface
  - Service interface CDI-RJ45
  - Via service interface/port 2: (RJ45)
  - WLAN interface
- Plain text display
  - With information on cause and remedial actions
  - Modbus TCP



Additional information on remote operation  $\rightarrow \implies 94$ 

# Web browser

Plain text display	With information on cause and remedial measures
--------------------	---

## LEDs

Status information	Status indicated by various LEDs	
	The following information is displayed depending on the device version:  Supply voltage active  Data transmission active  Device alarm/error has occurred  Network available <sup>1)</sup> Connection established <sup>1)</sup> Diagnostic status <sup>2)</sup> PROFINET blinking feature <sup>3)</sup>	

- 1) Only available for PROFINET, PROFINET over Ethernet-APL, Modbus over Ethernet-APL, Ethernet/IP
- 2) Only available for Modbus over Ethernet-APL
- 3) Only available for PROFINET, PROFINET over Ethernet-APL,

Load

# Ex connection data Safety-related values

Order code for Output type		Safety-rela	Safety-related values	
"Output; input 1"		Output; input 1 (Port 1)	Service interface (Port 2)	
Option <b>BA</b>	Current output 4-20 mA HART	$U_N = 30 V_{DC}$ $U_M = 250 V_{AC}$	$U_N = 3.3 V_{AC}$ $U_M = 250 V_{AC}$	
Option <b>GA</b>	PROFIBUS PA	$U_N = 32 V_{DC}$ $U_M = 250 V_{AC}$	$U_N = 3.3 V_{AC}$ $U_M = 250 V_{AC}$	
Option <b>LA</b>	PROFIBUS DP	$U_{N} = 5 V$ $U_{M} = 250 V_{AC}$	$U_N = 3.3 V_{AC}$ $U_M = 250 V_{AC}$	
Option <b>MA</b>	Modbus RS485	$U_{N} = 5 V$ $U_{M} = 250 V_{AC}$	$U_N = 3.3 V_{AC}$ $U_M = 250 V_{AC}$	
Option <b>MB</b>	Modbus TCP over Ethernet-APL 10 Mbit/s, SPE 10 Mbit/s, Ethernet 100 Mbit/s	APL port profile SLAX SPE PoDL classes 10, 11, 12 $U_N = 30 \ V_{DC}$ $U_M = 250 \ V_{AC}$	$U_{\rm N} = 3.3 \ V_{\rm AC}$ $U_{\rm M} = 250 \ V_{\rm AC}$	
Option <b>NA</b>	EtherNet/IP	$U_N = 3.3 V_{AC}$ $U_M = 250 V_{AC}$	U <sub>N</sub> = 3.3 V <sub>AC</sub> U <sub>M</sub> = 250 V <sub>AC</sub>	
Option <b>RA</b>	PROFINET	$U_N = 3.3 V_{AC}$ $U_M = 250 V_{AC}$	$U_N = 3.3 V_{AC}$ $U_M = 250 V_{AC}$	
Option <b>RB</b>	PROFINET over Ethernet-APL/SPE, 10Mbit/s	$ \begin{array}{l} \text{APL port profile SLAX} \\ \text{SPE PoDL classes 10, 11, 12} \\ U_{N} = 30 \ V_{DC} \\ U_{M} = 250 \ V_{AC} \\ \end{array} $	$U_{N} = 3.3 V_{AC}$ $U_{M} = 250 V_{AC}$	
Option <b>SA</b>	FOUNDATION Fieldbus	$U_N = 32 V_{DC}$ $U_M = 250 V_{AC}$	U <sub>N</sub> = 3.3 V <sub>AC</sub> U <sub>M</sub> = 250 V <sub>AC</sub>	
The specifications for U <sub>M</sub> only apply	to devices with Ex i circuits. Zone 1; Cla	ass I, Division 1 devices; Zone 2; Class I	Division 2 devices with Ex i sensor.	

Order code for	Output type	Safety-related values	
"Output; input 2" "Output; input 3"		Output; input 2	Output; input 3
Option <b>B</b>	Current output 4-20 mA	$\begin{array}{l} U_N = 30 \ V_{DC} \\ U_M = 250 \ V_{AC} \end{array}$	
Option <b>D</b>	Configurable I/O initial setting off	$U_{N} = 30 V_{DC}$ $U_{M} = 250 V_{AC}$	
Option <b>E</b>	Pulse/frequency/switch output	$U_N = 30 V_{DC}$ $U_M = 250 V_{AC}$	
Option <b>F</b>	Double pulse output	$U_{\rm N} = 30 \ V_{\rm DC}$ $U_{\rm M} = 250 \ V_{\rm AC}$	
Option <b>H</b>	Relay output	$U_N = 30 V_{DC}$ $I_N = 100 \text{ mA}_{DC} / 500 \text{ mA}_{AC}$ $U_M = 250 V_{AC}$	
Option I	Current input 4-20 mA	$U_{N} = 30 V_{DC}$ $U_{M} = 250 V_{AC}$	
Option <b>J</b>	Status input	$U_{N} = 30 V_{DC}$ $U_{M} = 250 V_{AC}$	

# Intrinsically safe values

Zone 1, Zone 21			
Order code for Output type		Intrinsically safe values	
"Output; input 1"		Output; input 1 (Port 1)	Service interface (Port 2)
Option CA	Current output 4-20mA HART Ex-i passive	$\begin{aligned} &\textbf{Ex ia} \\ &\textbf{U}_i = 30 \ \textbf{V} \\ &\textbf{I}_i = 100 \ \textbf{mA} \\ &\textbf{P}_i = 1.25 \ \textbf{W} \\ &\textbf{L}_i = 0 \ \mu \textbf{H} \\ &\textbf{C}_i = 6 \ \textbf{nF} \end{aligned}$	$\begin{aligned} \textbf{Ex ia} \\ U_i &= 10 \text{ V} \\ I_i &= n. \text{ a.} \\ P_i &= n. \text{ a.} \\ L_i &= 0  \mu\text{H} \\ C_i &= 200  n\text{F} \end{aligned}$
Option CC	Current output 4-20mA HART Ex-i active	$ \begin{aligned} &\textbf{Ex ia} \\ &\textbf{U}_0 = 21.8 \ V \\ &\textbf{I}_0 = 90 \ \text{mA} \\ &\textbf{P}_0 = 491 \ \text{mW} \\ &\textbf{L}_0 = 4.1 \ \text{mH(IIC)/15 mH(IIB)} \\ &\textbf{C}_0 = 160 \ \text{nF(IIC)/1160 nF(IIB)} \\ &\textbf{U}_i = 30 \ \text{V} \\ &\textbf{I}_i = 10 \ \text{mA} \\ &\textbf{P}_i = 0.3 \ \text{W} \\ &\textbf{L}_i = 5 \ \mu\text{H} \\ &\textbf{L}_i = 4.1 \ \mu\text{H} \\ &\textbf{C}_i = 6 \ \text{nF} \end{aligned} $	
Option HA	PROFIBUS PA Ex i (STANDARD + FISCO)	Ex ia $U_i = 30 \text{ V}$ $I_i = 570 \text{ mA}$ $P_i = 8.5 \text{ W}$ $L_i = 10  \mu\text{H}$ $C_i = 5 \text{ nF}$	$ \begin{aligned} \textbf{Ex ia} \\ U_i &= 10 \text{ V} \\ I_i &= n. \text{ a.} \\ P_i &= n. \text{ a.} \\ L_i &= 0  \mu\text{H} \\ C_i &= 200  n\text{F} \end{aligned} $

Zone 1, Zone 21			
Order code for	Output type	Intrinsically safe val	ues
"Output; input 1"		Output; input 1 (Port 1)	Service interface (Port 2)
Option MC	Modbus TCP over Ethernet-APL, Ex-i, 10Mbit/s	2-WISE power load, APL port profile SLAA $^{1)}$ Ex ia $U_i = 17.5 \text{ V}$ $I_i = 380 \text{ mA}$ $P_i = 5.32 \text{ W}$ $L_i = 10 \mu\text{H}$ $C_i = 5 \text{ nF}$ Cable specifications according to 2-WISE: $R_c = 15 \text{ to } 150 \Omega/\text{km}$ $L_c = 0.4 \text{ to } 1 \text{ mH/km}$ $C_c = 45 \text{ to } 200 \text{ nF/km}$ $C_c = C_c \text{ line/line} + 0.5 C_c \text{ line/screen, if both lines are floating, or }C_c = C_c \text{ line/line} + C_c \text{ line/screen, if the screen is connected to one line}$ Length of cable (not including cable stubs): $\leq 200 \text{ m}$ (656.2 ft) Length of cable stubs: $\leq 1 \text{ m}$ (3.3 ft)	$ \begin{aligned} &\textbf{Ex ia} \\ &U_i = 10 \ V \\ &I_i = n. \ a. \\ &P_i = n. \ a. \\ &L_i = 0 \ \mu H \\ &C_i = 200 \ nF \end{aligned} $
Option RC	PROFINET over Ethernet-APL, Ex-i, 10Mbit/s	<b>2-WISE power load, APL port profile SLAA</b> <sup>1)</sup> <b>Ex ia</b> $U_i = 17.5 \text{ V}$ $I_i = 380 \text{ mA}$ $P_i = 5.32 \text{ W}$ $L_i = 10 \text{ μH}$ $C_i = 5 \text{ nF}$ <b>Cable specifications according to 2-WISE:</b> $R_c = 15 \text{ to } 150 \Omega/\text{km}$ $L_c = 0.4 \text{ to } 1 \text{ mH/km}$ $C_c = 45 \text{ to } 200 \text{ nF/km}$ $C_c = C_c \text{ line/line} + 0.5  C_c \text{ line/screen, if both lines are floating, or}$ $C_c = C_c \text{ line/line} + C_c \text{ line/screen, if the screen is connected to one line}$ Length of cable (not including cable stubs): $\leq 200 \text{ m } (656.2 \text{ ft})$ Length of cable stubs: $\leq 1 \text{ m } (3.3 \text{ ft})$	$ \begin{aligned} &\textbf{Ex ia} \\ &U_i = 10 \ V \\ &I_i = n. \ a. \\ &P_i = n. \ a. \\ &L_i = 0 \ \mu H \\ &C_i = 200 \ nF \end{aligned} $
Option TA	FOUNDATION Fieldbus Ex i (STANDARD + FISCO)	Ex ia $U_i = 30 \text{ V}$ $I_i = 570 \text{ mA}$ $P_i = 8.5 \text{ W}$ $L_i = 10  \mu\text{H}$ $C_i = 5 \text{ nF}$	$\begin{aligned} &\textbf{Ex ia} \\ &\textbf{U}_i = 10 \ \textbf{V} \\ &\textbf{I}_i = n. \ a. \\ &\textbf{P}_i = n. \ a. \\ &\textbf{L}_i = 0 \ \mu H \\ &\textbf{C}_i = 200 \ nF \end{aligned}$

<sup>1)</sup> For further options see Ethernet-APL Installation Drawing HE\_01622.

Zone 2	Zone 2		
Order code for "Output; input 1"	Output type	Intrinsically safe values or NIFW values Output; input 1 (Port 1)	
Option HA	PROFIBUS PA Ex i (STANDARD + FISCO)	Ex ic AEx ic, Ex ic, NIFW $U_i = 32 \text{ V}$ $I_i = 570 \text{ mA}$ $P_i = 8.5 \text{ W}$ $L_i = 10 \mu\text{H}$ $C_i = 5 \text{ nF}$	
Option MC	Modbus TCP over Ethernet-APL, Ex-i, 10Mbit/s	2-WISE power load, APL port profile SLAC <sup>1)</sup> Ex ic	
Option RC	PROFINET over Ethernet-APL, Ex-i, 10Mbit/s	AEx ic, Ex ic, NIFW $ U_i = 17.5 \text{ V} $ $ I_i = 380 \text{ mA} $ $ P_i = 5.32 \text{ W} $ $ L_i = 10  \mu\text{H} $ $ C_i = 5 \text{ nF} $ Cable specifications according to 2-WISE: $ R_c = 15 \text{ to } 150  \Omega/\text{km} $ $ L_c = 0.4 \text{ to } 1 \text{ mH/km} $ $ C_c = 45 \text{ to } 200 \text{ nF/km} $ $ C_c = C_c \text{ line/line} + 0.5  C_c \text{ line/screen, if both lines are floating, or } $ $ C_c = C_c \text{ line/line} + C_c \text{ line/screen, if the screen is connected to one line } $ Length of cable (not including cable stubs): $\leq 200 \text{ m } (656.2 \text{ ft}) $ Length of cable stubs: $\leq 1 \text{ m } (3.3 \text{ ft}) $	
Option TA	FOUNDATION Fieldbus Ex i (STANDARD + FISCO)	Ex ic AEx ic, Ex ic, NIFW $U_i = 32 \text{ V}$ $I_i = 570 \text{ mA}$ $P_i = 8.5 \text{ W}$ $L_i = 10 \mu\text{H}$ $C_i = 5 \text{ nF}$	

1) For further options see Ethernet-APL Installation Drawing HE\_01622.

Order code for	, i ji		lues or NIFW values
"Output; input 2" "Output; input 3"		Output; input 2	Output; input 3
Option C	Current output 4-20mA Ex-i passive	$ \begin{aligned} \textbf{Ex ia} \\ \textbf{Ex ic} \\ \textbf{AEx ic, Ex ic, NIFW} \\ \textbf{U}_i &= 30 \text{ V} \\ \textbf{I}_i &= 100 \text{ mA} \\ \textbf{P}_i &= 1.25 \text{ W} \\ \textbf{L}_i &= 0 \\ \textbf{C}_i &= 0 \end{aligned} $	
Option G	Pulse/frequency/switch output Ex-i passive	$ \begin{aligned} \textbf{Ex ia} \\ \textbf{Ex ic} \\ \textbf{AEx ic, Ex ic, NIFW} \\ \textbf{U}_i &= 30 \text{ V} \\ \textbf{I}_i &= 100 \text{ mA} \\ \textbf{P}_i &= 1.25 \text{ W} \\ \textbf{L}_i &= 0 \\ \textbf{C}_i &= 0 \end{aligned} $	

# Low flow cut off

The switch points for low flow cut off are user-selectable.

## Galvanic isolation

The outputs are galvanically isolated:

- from the power supply
- from one another
- from the protective ground connection (PE)

# Protocol-specific data

# HART

Manufacturer ID	0x11
Device type ID	0x3B
HART protocol revision	7
Device description files (DTM, DD)	Information and files under: www.endress.com
HART load	Min. 250 Ω
System integration	Information on system integration: Operating Instructions → 🗎 115.  • Measured variables via HART protocol • Burst Mode functionality

# FOUNDATION Fieldbus

Manufacturer ID	0x452B48 (hex)	
Ident number	0x103B (hex)	
Device revision	1	
DD revision	Information and files under:	
CFF revision	<ul><li>www.endress.com</li><li>www.fieldcommgroup.org</li></ul>	
Interoperability Test Kit (ITK)	Version 6.2.0	
ITK Test Campaign Number	Information:  www.endress.com www.fieldcommgroup.org	
Link Master capability (LAS)	Yes	
Choice of "Link Master" and "Basic Device"	Yes Factory setting: Basic Device	
Node address	Factory setting: 247 (0xF7)	
Supported functions	The following methods are supported:  Restart  ENP Restart  Diagnostic  Set to OOS  Set to AUTO  Read trend data  Read event logbook	
Virtual Communication Relation	onships (VCRs)	
Number of VCRs	44	
Number of link objects in VFD	50	
Permanent entries	1	
Client VCRs	0	
Server VCRs	10	
Source VCRs	43	
Sink VCRs	0	
Subscriber VCRs	43	
Publisher VCRs	43	
Device Link Capabilities		
Slot time	4	
Min. delay between PDU	8	

Max. response delay	16
System integration	Information regarding system integration: Operating Instructions → 🖹 115.  Cyclic data transmission Description of the modules Execution times Methods

# PROFIBUS DP

Manufacturer ID	0x11
Ident number	0x156F
Profile version	3.02
Device description files (GSD, DTM, DD)	Information and files under:  ■ https://www.endress.com/download On the device product page: PRODUCTS → Product Finder → Links ■ https://www.profibus.com
Supported functions	Identification & Maintenance     Simplest device identification on the part of the control system and nameplate     PROFIBUS upload/download     Reading and writing parameters is up to ten times faster with PROFIBUS upload/download     Condensed status     Simplest and self-explanatory diagnostic information by categorizing diagnostic messages that occur
Configuration of the device address	<ul> <li>DIP switches on the I/O electronics module</li> <li>Via operating tools (e.g. FieldCare)</li> </ul>
Compatibility with earlier model	If the device is replaced, the measuring device Promass 300 supports the compatibility of the cyclic data with previous models. It is not necessary to adjust the engineering parameters of the PROFIBUS network with the Promass 300 GSD file.  Previous model: Promass 83 PROFIBUS DP  ■ ID No.: 1529 (hex)  ■ Extended GSD file: EH3x1529.gsd  ■ Standard GSD file: EH3_1529.gsd  Description of the function scope of compatibility: Operating Instructions →   115.
System integration	Information regarding system integration: Operating Instructions → 🖺 115.  Cyclic data transmission Block model Description of the modules

# PROFIBUS PA

Manufacturer ID	0x11
Ident number	0x156D
Profile version	3.02
Device description files (GSD, DTM, DD)	Information and files under:  ■ https://www.endress.com/download On the device product page: PRODUCTS → Product Finder → Links ■ https://www.profibus.com

Supported functions	Identification & Maintenance     Simplest device identification on the part of the control system and nameplate     PROFIBUS upload/download     Reading and writing parameters is up to ten times faster with PROFIBUS upload/download     Condensed status     Simplest and self-explanatory diagnostic information by categorizing diagnostic messages that occur
Configuration of the device address	<ul> <li>DIP switches on the I/O electronics module</li> <li>Local display</li> <li>Via operating tools (e.g. FieldCare)</li> </ul>
Compatibility with earlier model	If the device is replaced, the measuring device Promass 300 supports the compatibility of the cyclic data with previous models. It is not necessary to adjust the engineering parameters of the PROFIBUS network with the Promass 300 GSD file.  Earlier models:  Promass 80 PROFIBUS PA  ID No.: 1528 (hex)  Extended GSD file: EH3x1528.gsd  Standard GSD file: EH3_1528.gsd  Promass 83 PROFIBUS PA  ID No.: 152A (hex)  Extended GSD file: EH3x152A.gsd  Standard GSD file: EH3x152A.gsd  Standard GSD file: EH3_152A.gsd  Description of the function scope of compatibility: Operating Instructions →  115.
System integration	Information regarding system integration: Operating Instructions → 🖺 115.  ■ Cyclic data transmission  ■ Block model  ■ Description of the modules

# Modbus RS485

Protocol	Madhua Amiliantiana Duntagal Charification VI 1
Protocoi	Modbus Applications Protocol Specification V1.1
Response times	<ul> <li>Direct data access: typically 25 to 50 ms</li> <li>Auto-scan buffer (data range): typically 3 to 5 ms</li> </ul>
Device type	Slave
Slave address range	1 to 247
Broadcast address range	0
Function codes	<ul> <li>03: Read holding register</li> <li>04: Read input register</li> <li>06: Write single registers</li> <li>08: Diagnostics</li> <li>16: Write multiple registers</li> <li>23: Read/write multiple registers</li> </ul>
Broadcast messages	Supported by the following function codes:  O6: Write single registers  16: Write multiple registers  23: Read/write multiple registers
Supported baud rate	■ 1200 BAUD ■ 2400 BAUD ■ 4800 BAUD ■ 9600 BAUD ■ 19200 BAUD ■ 38400 BAUD ■ 57600 BAUD ■ 115200 BAUD
Data transmission mode	ASCII     RTU

Data access	Each device parameter can be accessed via Modbus RS485.  For Modbus register information
Compatibility with earlier model	If the device is replaced, the measuring instrument Promass 300 supports the compatibility of the Modbus registers for the process variables and the diagnostic information with the previous model Promass 83. It is not necessary to change the engineering parameters in the automation system.  □ Description of the function scope of compatibility:  Operating Instructions → ■ 115.
System integration	Information regarding system integration: Operating Instructions → 🗎 115.  ■ Modbus RS485 information  ■ Function codes  ■ Register information  ■ Response time  ■ Modbus data map

# Modbus TCP over Ethernet-APL

Port 1: Modbus TCP over Ethernet-APL 10 Mbit/s, SPE 10 Mbit/s	
Protocol	<ul><li>Modbus application protocol V1.1</li><li>TCP</li></ul>
Response times	On Modbus client request: Typically 3 to 5 ms
TCP port	502
Modbus TCP connections	Maximum 4
Communication type	Ethernet Advanced Physical Layer 10BASE-T1L
Data transfer	Full-duplex
Polarity	Automatic correction of crossed "APL signal + " and "APL signal -" signal lines
Device type	Address
Device type ID	0xC43B
Function codes	<ul> <li>03: Read holding register</li> <li>04: Read input register</li> <li>06: Write single registers</li> <li>16: Write multiple registers</li> <li>23: Read/write multiple registers</li> <li>43: Read device identification</li> </ul>
Broadcast support for function codes	<ul> <li>06: Write single registers</li> <li>16: Write multiple registers</li> <li>23: Read/write multiple registers</li> <li>43: Read device identification</li> </ul>
Supported transfer speed	10 Mbit/s (Ethernet-APL)
Supported features	Address can be configured using DHCP, web server or software
Device description files (FDI)	Information and files available at: www.endress.com → Downloads area
Configuration options for measuring instrument	<ul> <li>Asset management software (FieldCare, DeviceCare, Field Expert)</li> <li>Integrated web server via web browser and IP address</li> <li>Onsite operation</li> </ul>

Supported functions	<ul> <li>Device identification using:         Nameplate     </li> <li>Measured value status         The process variables are communicated with a measured value status     </li> <li>Blinking feature via the local display for simple device identification and assignment</li> <li>Device operation via asset management software (e.g. FieldCare, DeviceCare)</li> </ul>
System integration	Information regarding system integration: Operating Instructions → 🗎 115.  ■ Overview and description of the supported function codes  ■ Status coding  ■ Factory setting

Port 2: Modbus TCP over Ethernet 100 Mbit/s	
Protocol	<ul><li>Modbus application protocol V1.1</li><li>TCP</li></ul>
Response times	On Modbus client request: Typically 3 to 5 ms
TCP port	502
Modbus TCP connections	Maximum 4
Communication type	■ 10BASE-T ■ 100BASE-TX
Data transfer	Half-duplex, full-duplex
Polarity	Auto-MDIX
Device type	Address
Device type ID	0xC43B
Function codes	<ul> <li>03: Read holding register</li> <li>04: Read input register</li> <li>06: Write single registers</li> <li>16: Write multiple registers</li> <li>23: Read/write multiple registers</li> <li>43: Read device identification</li> </ul>
Broadcast support for function codes	<ul> <li>06: Write single registers</li> <li>16: Write multiple registers</li> <li>23: Read/write multiple registers</li> <li>43: Read device identification</li> </ul>
Supported transfer speed	<ul><li>10 Mbit/s</li><li>100 Mbit/s (Fast-Ethernet)</li></ul>
Supported features	Address can be configured using DHCP, web server or software
Device description files (FDI)	Information and files available at: www.endress.com → Downloads area
Configuration options for measuring instrument	<ul> <li>Asset management software (FieldCare, DeviceCare, Field Expert)</li> <li>Integrated web server via web browser and IP address</li> <li>Onsite operation</li> </ul>
Supported functions	<ul> <li>Device identification using:         Nameplate     </li> <li>Measured value status         The process variables are communicated with a measured value status     </li> <li>Device operation via asset management software (e.g. FieldCare, DeviceCare)</li> </ul>
System integration	Information regarding system integration: Operating Instructions → 🗎 115.  ■ Overview and description of the supported function codes  ■ Status coding  ■ Factory setting

# EtherNet/IP

Protocol	<ul> <li>The CIP Networks Library Volume 1: Common Industrial Protocol</li> <li>The CIP Networks Library Volume 2: EtherNet/IP Adaptation of CIP</li> </ul>
Communication type	■ 10Base-T ■ 100Base-TX
Device profile	Generic device (product type: 0x2B)
Manufacturer ID	0x000049E
Device type ID	0x103B
Baud rates	Automatic <sup>10</sup> / <sub>100</sub> Mbit with half-duplex and full-duplex detection
Polarity	Auto-polarity for automatic correction of crossed TxD and RxD pairs
Supported CIP connections	Max. 3 connections
Explicit connections	Max. 6 connections
I/O connections	Max. 6 connections (scanner)
Configuration options for measuring device	<ul> <li>DIP switches on the electronics module for IP addressing</li> <li>Manufacturer-specific software (FieldCare)</li> <li>Add-on Profile Level 3 for Rockwell Automation control systems</li> <li>Web browser</li> <li>Electronic Data Sheet (EDS) integrated in the measuring device</li> </ul>
Configuration of the EtherNet interface	<ul> <li>Speed: 10 MBit, 100 MBit, auto (factory setting)</li> <li>Duplex: half-duplex, full-duplex, auto (factory setting)</li> </ul>
Configuration of the device address	<ul> <li>DIP switches on the electronics module for IP addressing (last octet)</li> <li>DHCP</li> <li>Manufacturer-specific software (FieldCare)</li> <li>Add-on Profile Level 3 for Rockwell Automation control systems</li> <li>Web browser</li> <li>EtherNet/IP tools, e.g. RSLinx (Rockwell Automation)</li> </ul>
Device Level Ring (DLR)	Yes
System integration	Information regarding system integration: Operating Instructions $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $
	<ul><li>Cyclic data transmission</li><li>Block model</li><li>Input and output groups</li></ul>

# PROFINET

Protocol	Application layer protocol for decentral device periphery and distributed automation, Version 2.3
Communication type	100 Mbit/s
Conformity class	Conformance class B
Netload Class	Netload Class 2 100 Mbit/s
Baud rates	Automatic 100 Mbit/s with full-duplex detection
Periods	From 8 ms
Polarity	Auto-polarity for automatic correction of crossed TxD and RxD pairs
Media Redundancy Protocol (MRP)	Yes
System redundancy support	System redundancy S2 (2 AR with 1 NAP)
Device profile	Application interface identifier 0xF600 Generic device
Manufacturer ID	0x11
Device type ID	0x843B

Device description files (GSD, DTM, DD)	Information and files available at:  ■ www.endress.com  On the product page for the device: Documents/Software → Device drivers  ■ www.profibus.com
Supported connections	<ul> <li>2 x AR (IO Controller AR)</li> <li>1 x AR (IO-Supervisor Device AR connection allowed)</li> <li>1 x Input CR (Communication Relation)</li> <li>1 x Output CR (Communication Relation)</li> <li>1 x Alarm CR (Communication Relation)</li> </ul>
Configuration options for measuring instrument	<ul> <li>DIP switches on the electronics module, for device name assignment (last part)</li> <li>Asset management software (FieldCare, DeviceCare, Field Xpert)</li> <li>Integrated web server via web browser and IP address</li> <li>Device master file (GSD), can be read out via the integrated web server of the measuring instrument.</li> <li>Onsite operation</li> </ul>
Configuration of the device name	<ul> <li>DIP switches on the electronics module, for device name assignment (last part)</li> <li>DCP protocol</li> <li>Asset management software (FieldCare, DeviceCare, Field Xpert)</li> <li>Integrated web server</li> </ul>
Supported functions	<ul> <li>Identification &amp; Maintenance, simple device identifier via:</li> <li>Control system</li> <li>Nameplate</li> <li>Measured value status         The process variables are communicated with a measured value status     </li> <li>Blinking feature via the local display for simple device identification and assignment</li> <li>Device operation via asset management software (e.g. FieldCare, DeviceCare, SIMATIC PDM)</li> </ul>
System integration	Information regarding system integration: Operating Instructions → 🖺 115.  Cyclic data transmission  Overview and description of the modules  Status coding  Startup configuration  Factory setting

# PROFINET over Ethernet-APL

Protocol	Application layer protocol for decentral device periphery and distributed automation, Version 2.43
Communication type	Ethernet Advanced Physical Layer 10BASE-T1L
Conformance Class	Conformance Class B (PA)
Netload Class	PROFINET Netload Robustness Class 2 10 Mbit/s
Data transfer	10 Mbit/s Full-duplex
Cycle times	64 ms
Polarity	Automatic correction of crossed "APL signal +" and "APL signal -" signal lines
Media Redundancy Protocol (MRP)	Not possible (point-to-point connection to APL field switch)
System redundancy support	System redundancy S2 (2 AR with 1 NAP)
Device profile	PROFINET PA profile 4.02 (Application interface identifier API: 0x9700)
Manufacturer ID	17
Device type ID	0xA43B
Device description files (GSD, DTM, FDI)	Information and files available at:  ■ www.endress.com → Downloads area  ■ www.profibus.com

Supported connections	<ul> <li>2x AR (IO Controller AR)</li> <li>2x AR (IO Supervisor Device AR connection allowed)</li> </ul>
Configuration options for measuring instrument	<ul> <li>DIP switches on the electronics module, for device name assignment (last part)</li> <li>Asset management software (FieldCare, DeviceCare, Field Xpert)</li> <li>Integrated Web server via Web browser and IP address</li> <li>Device master file (GSD), can be read out via the integrated Web server of the measuring instrument.</li> <li>Onsite operation</li> </ul>
Configuration of the device name	<ul> <li>DIP switches on the electronics module, for device name assignment (last part)</li> <li>DCP protocol</li> <li>Asset management software (FieldCare, DeviceCare, Field Xpert)</li> <li>Integrated web server</li> </ul>
Supported functions	<ul> <li>Identification &amp; Maintenance, simple device identifier via:</li> <li>Control system</li> <li>Nameplate</li> <li>Measured value status         The process variables are communicated with a measured value status     </li> <li>Blinking feature via the local display for simple device identification and assignment</li> <li>Device operation via asset management software (e.g. FieldCare, DeviceCare, SIMATIC PDM with FDI package)</li> </ul>
System integration	Information regarding system integration: Operating Instructions → 🗎 115.  Cyclic data transmission Overview and description of the modules Status coding Factory setting

# **Power supply**

# Terminal assignment

Transmitter: supply voltage, input/outputs

#### HART

Supply	Supply voltage		Input/output 1 (Port 1)		Input/output 2		utput 3	Service interface (Port 2)
1 (+)	2 (-)	26 (+)	27 (-)	24 (+)	25 (-)	22 (+)	23 (-)	CDI-RJ45
				The terminal assignment depends on the specific device version ordered $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $				

# FOUNDATION fieldbus

Supply	Supply voltage		utput 1 rt 1)	Input/output 2		Input/output 3		Service interface (Port 2)
1 (+)	2 (-)	26 (A)	27 (B)	24 (+)	25 (-)	22 (+)	23 (-)	CDI-RJ45
				The terminal assignment depends on the specific device version ordered $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $				

### PROFIBUS DP

Supply	Supply voltage		Input/output 1 (Port 1)		Input/output 2		utput 3	Service interface (Port 2)
1 (+)	2 (-)	26 (B)	27 (A)	24 (+)	25 (-)	22 (+)	23 (-)	CDI-RJ45
				The terminal assignment depends on the specific device version ordered $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $				

### PROFIBUS PA

Supply	Supply voltage		Input/output 1 (Port 1)		Input/output 2		output 3	Service interface (Port 2)
1 (+)	2 (-)	26 (B)	27 (A)	24 (+)	25 (-)	22 (+)	23 (-)	CDI-RJ45
				The terminal assignment depends on the specific device version ordered $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $				

### Modbus RS485

Supply	Supply voltage		Input/output 1 (Port 1)		Input/output 2		output 3	Service interface (Port 2)
1 (+)	2 (-)	26 (B)	27 (A)	24 (+)	25 (-)	22 (+)	23 (-)	CDI-RJ45
				The terminal assignment depends on the specific device version ordered $\Rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $				

### Modbus TCP

Supply voltage		Input/output 1 1 (Port <sup>1)</sup> )		Input/output 2		Input/output 3		Service interface (Port 2) 1)
1 (+)	2 (-)	26 (+)	27 (-)	24 (+)	25 (-)	22 (+)	23 (-)	CDI-RJ45
				The terminal assignment depends on the specific device version ordered $\Rightarrow \;  riangleq \; 13.$				

1) For Modbus TCP communication, either port 1 OR port 2 can be used.

#### **PROFINET**

Supply	voltage	Input/output 1 (Port 1) <sup>1)</sup>	Input/o	Input/output 2		output 3	Service interface (Port 2) 1)
1 (+)	2 (-)	RJ45	24 (+)	25 (-)	22 (+)	23 (-)	CDI-RJ45
			The terminal assignment de version order			ecific device	

1) Port can be used for communication or as a service interface (CDI-RJ45).

#### PROFINET over Ethernet-APL

Supply voltage		Input/o (Por	output 1 rt 1)	Input/output 2		Input/output 3		Service interface (Port 2 <sup>1)</sup> )
1 (+)	2 (-)	26 (+)	27 (-)	24 (+)	25 (-)	22 (+)	23 (-)	CDI-RJ45
				The terminal assignment depends on the specific device version ordered $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $				

1) No PROFINET communication available on port 2

#### Ethernet/IP

	Supply voltage		Input/output 1 (Port 1) <sup>1)</sup>	Input/output 2		Input/output 3		Service interface (Port 2) 1)
Ī	1 (+)	2 (-)	RJ45	24 (+)	25 (-)	22 (+)	23 (-)	CDI-RJ45
				The terminal assignment depends on the specific device version ordered $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $				

- 1) Port can be used for communication or as a service interface (CDI-RJ45).

#### Available device plugs

i Dev

Device plugs may not be used in hazardous areas!

# Device plugs for Proline 300:

Order code for "Input; output 1"

- Option **SA** "FOUNDATION Fieldbus"  $\rightarrow$   $\stackrel{ riangle}{ riangle}$  38
- Option **GA** "PROFIBUS PA" → 🖺 39
- Option **NA** "EtherNet/IP" → 🖺 39
- Option **RA** "PROFINET" → 🖺 39
- Option **MB** "Modbus TCP" → 🖺 39

### Device plug for connecting to the service interface:

Order code for "Accessory mounted"

Option **NB**, RJ45 M12 adapter (service interface)  $\rightarrow \triangleq 49$ 

### Order code for "Input; output 1", option SA "FOUNDATION fieldbus"

Order code for	Cable entry/connection → 🗎 41				
"Electrical connection"	2	3			
M, 3, 4, 5	7/8" plug	-			

#### Order code for "Input; output 1", option GA "PROFIBUS PA"

Order code for	Cable entry/connection → 🗎 41				
"Electrical connection"	2	3			
L, N, P, U	Connector M12×1	-			

### Order code for "Input; output 1", option NA "EtherNet/IP"

Order code for	Cable entry/connection → 🖺 41				
"Electrical connection"	2	3			
L, N, P, U	Connector M12×1	_			
R <sup>1) 2)</sup> S <sup>1) 2)</sup> , T <sup>1) 2)</sup> , V <sup>1) 2)</sup>	Connector M12×1	Connector M12×1			

- Not compatible with an external WLAN antenna (order code for "Accessory enclosed", option P8), an RJ45 M12 adapter for the service interface (order code for "Accessory mounted", option NB)
- 2) Suitable for integrating the device into a ring topology.

### Order code for "Input; output 1", option RA "PROFINET"

Order code for	Cable entry/connection → 🖺 41				
"Electrical connection"	2	3			
L, N, P, U	Connector M12×1 –				
R <sup>1) 2)</sup> , S <sup>1) 2)</sup> , T <sup>1) 2)</sup> , V <sup>1) 2)</sup>	Connector M12×1 Connector M12×1				

- Not compatible with an external WLAN antenna (order code for "Accessory enclosed", option P8), an RJ45 M12 adapter for the service interface (order code for "Accessory mounted", option NB)
- 2) Suitable for integrating the device into a ring topology.

#### Order code for "Input; output 1", option RB "PROFINET over Ethernet-APL"

Order code for	Cable entry/connection → 🗎 41				
"Electrical connection"	2	3			
L, N, P, U	Connector M12×1	-			

#### Order code for "Input; output 1", option MB "Modbus TCP over Ethernet-APL"

Order code for	Accessories	Cable entry/connection → 🖺 40			
"Electrical connection"	Accessories	2	3		
L, N, P, U	-	Connector M12×1 A-coded	_		
L, N, P, U	NB <sup>1)</sup>	Connector M12×1 A-coded	Connector M12×1 <sup>1)</sup> D-coded		
1 <sup>2)</sup> , 2 <sup>2)</sup> , 7 <sup>2)</sup> , 8 <sup>2)</sup>	-	-	Connector M12×1 D-coded		

- 1) Cannot be used as a Modbus TCP port.
- 2) Not compatible with an external WLAN antenna (order code for "Accessory enclosed", option P8, an RJ45 M12 adapter for the service interface (order code for "Accessory mounted", option NB) or a remote operating and display module DKX001.

#### Order code for "Accessory mounted", option NB: "Adapter RJ45 M12 (service interface)"

Order code for	Cable entry/connection → 🗎 40			
"Accessory mounted"	Cable entry 2	Cable entry 3		
NB 1)	-	Connector M12×1		

1) Not compatible with electrical connection option 1, 2, 7, 8

#### Supply voltage

Order code for "Power supply"	Terminal voltage		Frequency range
Option <b>D</b>	DC 24 V ±20%		-
Option <b>E</b>	AC 100 to 240 V -15 to 10%		50/60 Hz
Option I	DC 24 V	±20%	-
	AC 100 to 240 V	-15 to 10%	50/60 Hz

#### Power consumption

#### Transmitter

Max. 10 W (active power)

switch-on current	Max. 36 A (<5 ms) as per NAMUR Recommendation NE 21
-------------------	---

#### **Current consumption**

#### **Transmitter**

- Max. 400 mA (24 V)
- Max. 200 mA (110 V, 50/60 Hz; 230 V, 50/60 Hz)

#### Power supply failure

- Totalizers stop at the last value measured.
- Depending on the device version, the configuration is retained in the device memory or in the plug-in memory (HistoROM DAT).
- Error messages (incl. total operated hours) are stored.

# Overcurrent protection element

The device must be operated with a dedicated circuit breaker, as it does not have an ON/OFF switch of its own


- The circuit breaker must be easy to reach and labeled accordingly.
- Permitted nominal current of the circuit breaker: 2 A up to maximum 10 A.

#### **Electrical connection**

#### **Transmitter connection**



- Terminal assignment → 🗎 37
- Device plugs available → 🖺 38

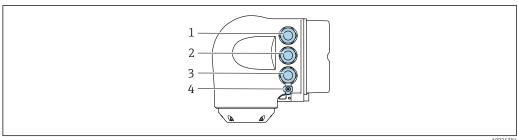

- Terminal connection for supply voltage
- Terminal connection for signal transmission, input/output 2
- Terminal connection for signal transmission, input/output or terminal for network connection via service  $interface\ (CDI-RJ45); Optional: terminal\ connection\ for\ external\ WLAN\ antenna\ or\ connection\ for\ remote$ display and operating module DKX001
- Protective ground connection (PE)
- An adapter for the RJ45 to the M12 connector is optionally available: Order code for "Accessories", option NB: "Adapter RJ45 M12 (service interface)"

The adapter connects the service interface (CDI-RJ45) to an M12 connector mounted in the cable entry. The connection to the service interface can be established via an M12 connector without opening the device.

Network connection via service interface (CDI-RJ45)  $\rightarrow$   $\blacksquare$  101

#### Connecting in a ring topology


Device versions with EtherNet/IP and PROFINET communication protocols can be integrated into a ring topology. The device is integrated via the terminal connection for signal transmission (output 1) and the connection to the service interface (CDI-RJ45).



Integrating the transmitter into a ring topology:

PROFINET




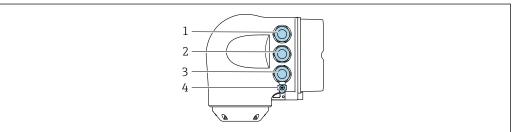

- Terminal connection for supply voltage
- 2 Terminal connection for signal transmission: PROFINET or EtherNet/IP (RJ45 plug)
- 3 Connection to service interface (CDI-RJ45)
- Protective ground connection (PE)
- If the device has additional inputs/outputs, these are routed in parallel via the cable entry for connection to the service interface (CDI-RJ45).

### Connecting the remote display and operating module DKX001

- The remote display and operating module DKX001 is available as an optional extra  $\rightarrow \triangleq 112..$ 
  - The remote display and operating module DKX001 is only available for the following housing version: order code for "Housing": option A "Aluminum, coated"
  - The measuring instrument is always supplied with a dummy cover when the remote display and operating module DKX001 is ordered directly with the measuring instrument. Display or operation at the transmitter is not possible in this case.
  - If ordered subsequently, the remote display and operating module DKX001 may not be connected at the same time as the existing measuring instrument display module. Only one display or operation unit may be connected to the transmitter at any one time.

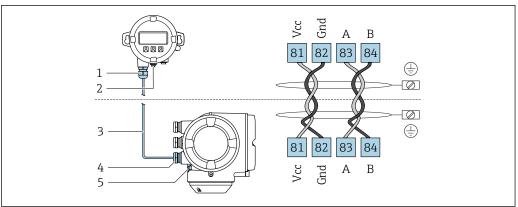


A0027518

- 1 Remote display and operating module DKX001
- 2 Protective ground connection (PE)
- 3 Connecting cable
- 4 Measuring instrument
- 5 Protective ground connection (PE)


#### **Connection examples**

Current output 4 to 20 mA (without HART)



A0055851


- $\blacksquare$  2 Connection example for 4 to 20 mA current output (active)
- 1 Automation system with current input (e.g. PLC)
- 2 Optional additional display unit: Observe maximum load
- *Flowmeter with current output (active)*

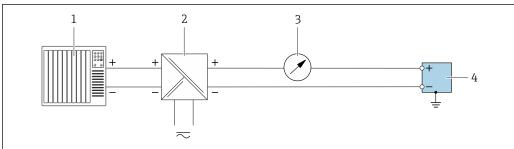

A0055053

- 3 Connection example for 4 to 20 mA current output (passive)
- 1 Automation system with current input (e.g. PLC)
- 2 Power supply
- 3 Optional additional display unit: Observe maximum load
- 4 Transmitter with current output (passive)

#### Current input 4 to 20 mA

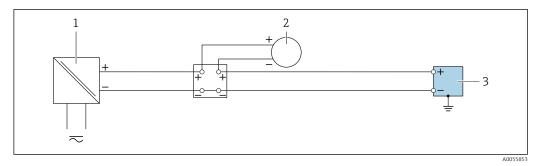


- € 4 Connection example for 4 to 20 mA current input
- Power supply
- 2 External measuring instrument with 4 to 20 mA passive current output. e.g. pressure or temperature)
- 3 Transmitter with 4 to 20 mA current input

### Pulse output/frequency output/switch output




- **№** 5 Connection example for pulse output/frequency output/switch output (active)
- Automation system with pulse input/frequency input/switch input (e.g. PLC)
- Transmitter with pulse output/frequency output/switch output (active)

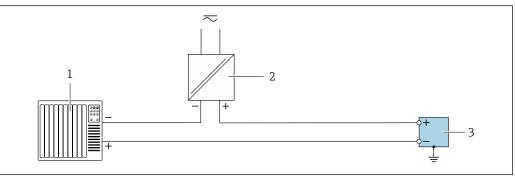

- € 6 Connection example for pulse output/frequency output/switch output (passive)
- Automation system with pulse input/frequency input/switch input (e.g. PLC)
- 2
- 3 *Transmitter with pulse output/frequency output/switch output (passive)*


#### Relay output

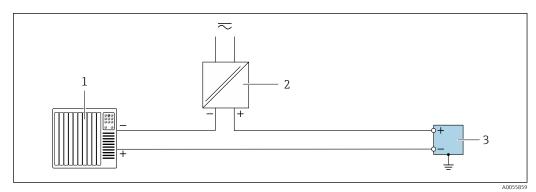

**₽** 7 Connection example for relay output

- Automation system with switch input (e.g. PLC) 1
- 2 Power supply
- 3 Transmitter with relay output


### Status input

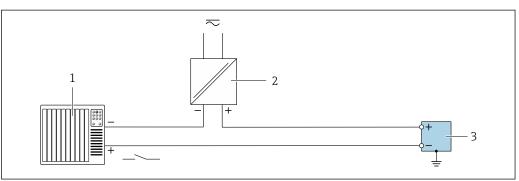

₿ 🗷 Connection example for status input


- Automation system with switch output passive e.g. PLC)
- 2 Power supply
- 3 *Transmitter with status input*

### Current output 4 to 20 mA HART

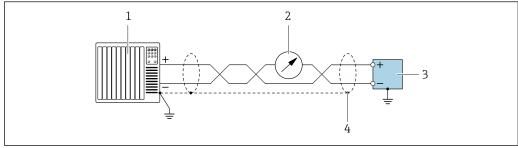

**9** Connection example for 4 to 20 mA current output with HART (active)


- Automation system with 4 to 20 mA current input with HART (e.g. PLC)
- 2 Optional display unit: Note maximum load
- 3 Transmitter with 4 to 20 mA current output with HART (active)
- Ground cable shield at one end. For installations in compliance with NAMUR NE 89, grounding of the cable shield on both sides is required.

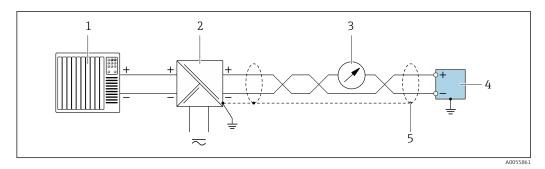

 $\blacksquare$  10 Connection example for 4 to 20 mA current output with HART (passive)

- 1 Automation system with 4 to 20 mA current input with HART (e.g. PLC)
- 2 Power supply
- 3 Optional display unit: Note maximum load
- 4 Transmitter with 4 to 20 mA current output with HART (passive)
- Ground cable shield at one end. For installations in compliance with NAMUR NE 89, grounding of the cable shield on both sides is required.

#### Modbus RS485

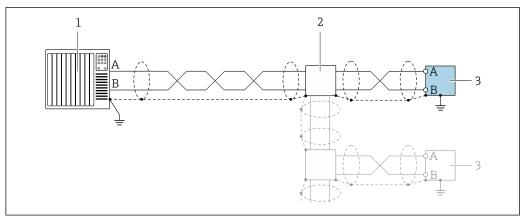

A005586

### ■ 11 Connection example for Modbus RS485

- 1 Automation system with Modbus master (e.g. PLC)
- 2 Optional distribution box
- 3 Transmitter with Modbus RS485


#### PROFIBUS PA

See https://www.profibus.com "PROFIBUS Installation Guidelines".

#### PROFIBUS DP

See https://www.profibus.com "PROFIBUS Installation Guidelines".

#### FOUNDATION Fieldbus

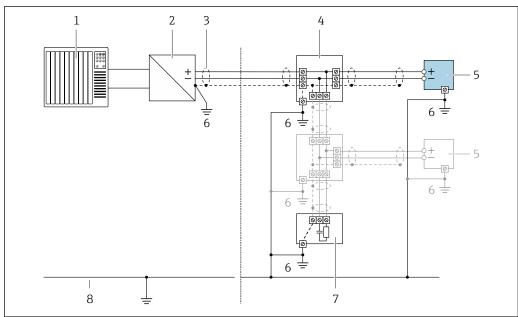

#### ■ 12 Connection example for FOUNDATION Fieldbus

- 1 Automation system (e.g. PLC)
- Power Conditioner (FOUNDATION Fieldbus)
- 3 Cable shield provided at one end. The cable shield must be grounded at both ends to comply with EMC requirements; observe cable specifications
- 4 T-box
- 5 Measuring instrument
- Local grounding 6
- Bus terminator
- Potential equalization conductor

#### **PROFINET**



See https://www.profibus.com "PROFINET Planning guideline".

#### EtherNet/IP



See https://www.odva.org"EtherNet/IP Media Planning & Installation Manual".

#### Ethernet-APL



See https://www.profibus.com Ethernet-APL White Paper "

#### Potential equalization

#### Requirements

For potential equalization:

- Pay attention to in-house grounding concepts
- Take account of operating conditions like the pipe material and grounding
- Connect the medium, sensor and transmitter to the same electric potential
- Use a ground cable with a minimum cross-section of 6 mm<sup>2</sup> (10 AWG) and a cable lug for potential equalization connections

#### **Terminals**

Spring-loaded terminals: Suitable for strands and strands with ferrules. Conductor cross-section 0.2 to 2.5 mm<sup>2</sup> (24 to 12 AWG).

#### Cable entries

- Cable gland: M20  $\times$  1.5 with cable Ø 6 to 12 mm (0.24 to 0.47 in)
- Thread for cable entry:
  - NPT ½"
  - G ½"
  - M20
- Device plug for digital communication: M12 Only available for certain device versions  $\rightarrow \blacksquare 38$ .

# Pin assignment, device plug

### FOUNDATION Fieldbus

	Pin		Assignment	Coding	Plug/socket	
2 / 3	1	+	Signal +	Α	Plug	
1 4	2	-	Signal –			
	3		Cable shield <sup>1</sup>			
	4		Not used			
	Metal plug housing		Cable shield			
		<sup>1</sup> If a cable shield is used				

### PROFIBUS PA

	Pin		Assignment	Coding	Plug/socket
2 / 3	1	+	PROFIBUS PA +	A	Plug
1 4	2		Grounding		
	3	-	PROFIBUS PA -		
	4		Not used		
	Met al plug hous ing		Cable shield		

Recommended plug:

- Binder, series 713, part no. 99 1430 814 04
- Phoenix, part no. 1413934 SACC-FS-4QO SH PBPA SCO

### **PROFINET**


2	Pin		Assignment	Coding	Plug/socket
	1	+	TD +	D	Socket
1 3	2	+	RD +		
	3	-	TD -		
	4	-	RD -		
4 A0032047					
	Metal plug housing		Cable shield		

# Recommended plug:

Binder, series 825, part no. 99 3729 810 04

Phoenix, part no. 1543223 SACC-M12MSD-4Q


#### PROFINET over Ethernet-APL

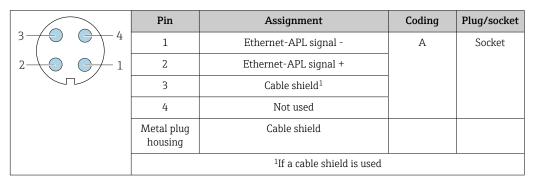

# Recommended plug:

- Binder, series 713, part no. 99 1430 814 04
- Phoenix, part no. 1413934 SACC-FS-4QO SH PBPA SCO

# Modbus TCP over Ethernet-APL 10 Mbit/s

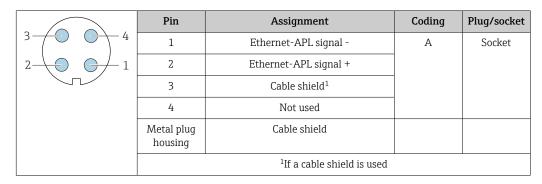

# Recommended plug:

- Binder, series 713, part no. 99 1430 814 04
- Phoenix, part no. 1413934 SACC-FS-4QO SH PBPA SCO

### Modbus TCP over Ethernet 100 Mbit/s

2	Pin		Assignment	Coding	Plug/socket
	1	+	Tx	D	Socket
1 3	2	+	Rx		
	3	-	Tx		
	4	-	Rx		
4 A0032047					

# EtherNet/IP

2	Pin		Assignment	Coding	Plug/socket
	1	+	Tx	D	Socket
1 3	2	+	Rx		
	3	-	Tx		
	4	-	Rx		
<b>4</b> A0032047					
	Met al plug hous ing		Cable shield		

Recommended plug:

- Binder, series 825, part no. 99 3729 810 04
- Phoenix, part no. 1543223 SACC-M12MSD-4Q

#### Service interface

Order code for "Accessory mounted", option NB: "Adapter RJ45 M12 (service interface)"

2	Pin		Assignment	Coding	Plug/socket
	1	+	Tx	D	Socket
1 3	2	+	Rx		
	3	-	Tx		
	4	1	Rx		
4 A0032047					



Recommended plug:

- Binder, series 825, part no. 99 3729 810 04
- Phoenix, part no. 1543223 SACC-M12MSD-4Q

#### Cable specification

#### Permitted temperature range

- The installation guidelines that apply in the country of installation must be observed.
- The cables must be suitable for the minimum and maximum temperatures to be expected.

#### Power supply cable (incl. conductor for the inner ground terminal)

Standard installation cable is sufficient.

#### Protective grounding cable for the outer ground terminal

Conductor cross-section < 6 mm<sup>2</sup> (10 AWG)

Larger cross-sections can be connected using a cable lug.

The grounding impedance must be less than 2  $\Omega$ .

### Signal cable

4 to 20 mA current input

Standard installation cable is sufficient.

Pulse/frequency/switch output

Standard installation cable is sufficient.

Relay output

Standard installation cable is sufficient.

Status input

Standard installation cable is sufficient.

Current output 4 to 20 mA HART

Shielded twisted-pair cable.



See https://www.fieldcommgroup.org "HART PROTOCOL SPECIFICATIONS".

Modbus RS485

Shielded twisted-pair cable.



See https://modbus.org "MODBUS over Serial Line Specification and Implementation Guide".

#### PROFIBUS PA

Shielded twisted-pair cable. Cable type A is recommended.



See https://www.profibus.com "PROFIBUS Installation Guidelines".

#### PROFIBUS DP

Shielded twisted-pair cable. Cable type A is recommended.



See https://www.profibus.com "PROFIBUS Installation Guidelines".

#### **PROFINET**

Only PROFINET cables.



See https://www.profibus.com "PROFINET Planning guideline".

#### EtherNet/IP

Twisted-pair Ethernet CAT 5 or better.



See https://www.odva.org"EtherNet/IP Media Planning & Installation Manual".

#### Ethernet-APL

Shielded twisted-pair cable. Cable type A is recommended.



See https://www.profibus.com Ethernet-APL White Paper "

#### FOUNDATION Fieldbus

Twisted, shielded two-wire cable.



For further information on planning and installing FOUNDATION Fieldbus networks see:

- Operating Instructions for "FOUNDATION Fieldbus Overview" (BA00013S)
- FOUNDATION Fieldbus Guideline
- IEC 61158-2 (MBP)

### Connecting cable for transmitter - remote display and operating module DKX001

#### Standard cable

A standard cable can be used as the connecting cable.

Standard cable 4 cores (2 pairs); pair-stranded with common shield	
Shielding Tin-plated copper-braid, optical cover ≥ 85 %	
Capacitance: core/shield Maximum 1 000 nF for Zone 1; Class I, Division 1	
L/R Maximum 24 $\mu$ H/ $\Omega$ for Zone 1; Class I, Division 1	
Cable length Maximum 300 m (1000 ft), see the following table	

Cross-section	Cable length for use in:  Non-hazardous area  Hazardous area: Zone 2; Class I, Division 2  Hazardous area: Zone 1; Class I, Division 1	
0.34 mm <sup>2</sup> (22 AWG)	80 m (270 ft)	
0.50 mm <sup>2</sup> (20 AWG)	120 m (400 ft)	
0.75 mm <sup>2</sup> (18 AWG)	180 m (600 ft)	
1.00 mm <sup>2</sup> (17 AWG)	240 m (800 ft)	
1.50 mm <sup>2</sup> (15 AWG)	300 m (1000 ft)	

#### Optionally available connecting cable

Standard cable	$2\times2\times0.34~\text{mm}^2$ (22 AWG) PVC cable $^{1)}$ with common shield (2 pairs, pair-stranded)
Flame resistance	According to DIN EN 60332-1-2
Oil-resistance	According to DIN EN 60811-2-1
Shielding	Tin-plated copper-braid, optical cover $\geq$ 85 %
Capacitance: core/shield ≤200 pF/m	
<b>L/R</b> ≤24 μH/Ω	
Available cable length 10 m (35 ft)	
Operating temperature	When mounted in a fixed position: $-50$ to $+105$ °C ( $-58$ to $+221$ °F); when cable can move freely: $-25$ to $+105$ °C ( $-13$ to $+221$ °F)

1) UV radiation can impair the cable outer sheath. Protect the cable from direct sunshine where possible.

#### Overvoltage protection

Mains voltage fluctuations	→ 🖺 40			
Overvoltage category	Overvoltage category II			
Short-term, temporary overvoltage	Between cable and ground up to 1200 V, for max. 5 s			
Long-term, temporary overvoltage	Between cable and ground up to 500 V			

# **Performance characteristics**

# Reference operating conditions

- Error limits based on ISO 11631
- Water
  - +15 to +45 °C (+59 to +113 °F)
  - 2 to 6 bar (29 to 87 psi)
- Data as indicated in the calibration protocol
- Accuracy based on accredited calibration rigs according to ISO 17025



# Maximum measurement error

o.r. = of reading;  $1 \text{ g/cm}^3 = 1 \text{ kg/l}$ ; T = medium temperature

### Base accuracy



Design fundamentals → 🖺 54

Mass flow and volume flow (liquids)

±0.15 % o.r.

 $\pm 0.10$  % o.r. (order code for "Calibration flow", option A, B, C, for mass flow)

Mass flow (gases)

±0.50 % o.r.

Density (liquids)

Under reference conditions	Standard density calibration
[g/cm³]	[g/cm³]
±0.0005	±0.002

### Temperature

 $\pm 0.5 \,^{\circ}\text{C} \pm 0.005 \cdot \text{T} \,^{\circ}\text{C} \, (\pm 0.9 \,^{\circ}\text{F} \pm 0.003 \cdot (\text{T} - 32) \,^{\circ}\text{F})$ 

# Zero point stability

DN		Zero point stability		
[mm]	[mm] [in]		[lb/min]	
8	3/8	0.20	0.007	
15	1/2	0.65	0.024	
25	1	1.80	0.066	
40	1½	4.50	0.165	
50	2	7.0	0.257	
80	3	18.0	0.6615	

### Flow values

Flow values as turndown parameters depending on nominal diameter.

#### SI units

DN	1:1	1:10	1:20	1:50	1:100	1:500
[mm]	[kg/h]	[kg/h]	[kg/h]	[kg/h]	[kg/h]	[kg/h]
8	2 000	200	100	40	20	4
15	6500	650	325	130	65	13
25	18000	1800	900	360	180	36
40	45 000	4500	2 2 5 0	900	450	90
50	70000	7 000	3 500	1400	700	140
80	180 000	18000	9000	3 600	1800	360

#### US units

DN	1:1	1:10	1:20	1:50	1:100	1:500
[inch]	[lb/min]	[lb/min]	[lb/min]	[lb/min]	[lb/min]	[lb/min]
3/8	73.50	7.350	3.675	1.470	0.735	0.147
1/2	238.9	23.89	11.95	4.778	2.389	0.478
1	661.5	66.15	33.08	13.23	6.615	1.323
1½	1654	165.4	82.70	33.08	16.54	3.308
2	2 5 7 3	257.3	128.7	51.46	25.73	5.146
3	6615	661.5	330.8	132.3	66.15	13.23

# Accuracy of outputs

The outputs have the following base accuracy specifications:

Current output

Accuracy	±5 μA
1	·

Pulse/frequency output

o.r. = of reading

**Accuracy** Max

Max. ±50 ppm o.r. (over the entire ambient temperature range)

#### Repeatability

o.r. = of reading;  $1 \text{ g/cm}^3 = 1 \text{ kg/l}$ ; T = medium temperature

#### Base repeatability



Design fundamentals → 🖺 54

Mass flow and volume flow (liquids)

±0.075 % o.r.

±0.05 % o.r. (calibration option, for mass flow)

Mass flow (gases)

 $\pm 0.25$  % o.r. (up to a Mach number of 0.2)

Density (liquids)

 $\pm 0.00025 \text{ g/cm}^3$ 

**Temperature** 

 $\pm 0.25 \,^{\circ}\text{C} \pm 0.0025 \cdot \text{T} \,^{\circ}\text{C} \, (\pm 0.45 \,^{\circ}\text{F} \pm 0.0015 \cdot (\text{T}-32) \,^{\circ}\text{F})$ 

#### Response time

The response time depends on the configuration (damping).

μA/°C

# Influence of ambient temperature

#### **Current output**

Temperature coefficient	Max.	1
-------------------------	------	---

#### Pulse/frequency output

Temperature coefficient	No additional effect. Included in accuracy.
-------------------------	---

# Influence of medium temperature

#### Mass flow


o.f.s. = of full scale value

If there is a difference between the temperature during zero adjustment and the process temperature, the additional measurement error of the sensors is typically  $\pm 0.0002$  %o.f.s./°C ( $\pm 0.0001$  % o.f.s./°F).

The influence is reduced when the zero adjustment is performed at process temperature.

#### Density

If there is a difference between the density calibration temperature and the process temperature, the measurement error of the sensors is typically  $\pm 0.0001$  g/cm<sup>3</sup>/°C ( $\pm 0.00005$  g/cm<sup>3</sup>/°F). Field density adjustment is possible.

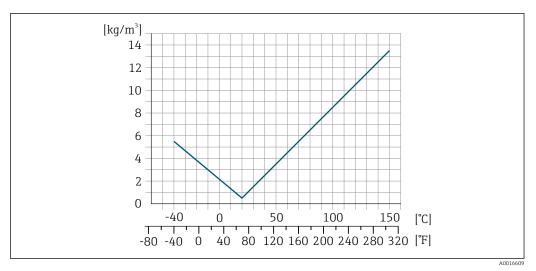

Field density adjustment, for example at +20 °C (+68 °F)

**Temperature** 

 $\pm 0.005 \cdot \text{T} \,^{\circ}\text{C} \, (\pm 0.005 \cdot (\text{T} - 32) \,^{\circ}\text{F})$ 

#### Influence of medium pressure

The following shows how the process pressure (gauge pressure) affects the accuracy of the mass flow.

o.r. = of reading



It is possible to compensate for the effect by:

- Reading in the current pressure measured value via the current input or a digital input.
- Specifying a fixed value for the pressure in the device parameters.



DN		[% o.r./bar]	[% o.r./psi]	
[mm]	[in]			
8	3/8	no effect		
15	1/2	no effect		
25	1	no effect		
40	1½	no effect		
50	2	-0.009 -0.0006		
80	3	-0.020 -0.0014		

# Design fundamentals

o.r. = of reading, o.f.s. = of full scale value

BaseAccu = base accuracy in % o.r., BaseRepeat = base repeatability in % o.r.

MeasValue = measured value; ZeroPoint = zero point stability

Calculation of the maximum measured error as a function of the flow rate


Flow rate	Maximum measured error in % o.r.
$\geq \frac{\text{ZeroPoint}}{\text{BaseAccu}} \cdot 100$	± BaseAccu
A0021332	10012555
< ZeroPoint BaseAccu · 100	± ZeroPoint MeasValue · 100
A0021333	A0021334

54

Calculation of the maximum repeatability as a function of the flow rate

Flow rate		Maximum repeatability in % o.r.
$\geq \frac{\frac{1}{2} \cdot ZeroPoint}{BaseRepeat} \cdot 100$		± BaseRepeat
A00	0021335	10021710
< ½ · ZeroPoint BaseRepeat · 100		$\pm \frac{1}{2} \cdot \frac{\text{ZeroPoint}}{\text{MeasValue}} \cdot 100$
A00	0021336	A0021337


#### Example of maximum measurement error

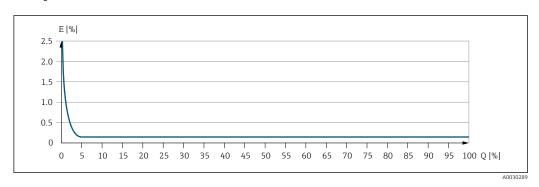

- E Maximum measurement error in % o.r. (example)
- Q Flow rate in % of maximum full scale value

# Installation

### Mounting location

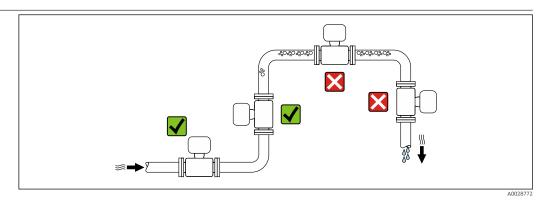


To avoid measurement errors caused by gas bubble formation in the measuring tube, avoid the following installation locations in the pipe:

- Highest point of a pipeline
- Directly upstream of a free pipe outlet in a down pipe

### Installation in down pipes

However, the following installation suggestion allows for installation in an open vertical pipeline. Pipe restrictions or the use of an orifice with a smaller cross-section than the nominal diameter prevent the sensor running empty while measurement is in progress.

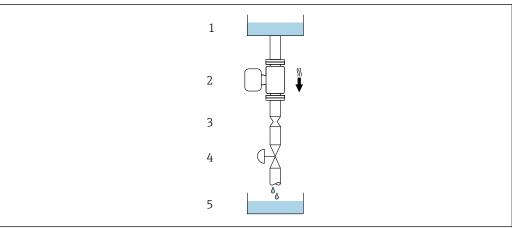

A00287

■ 14 Installation in a down pipe (e.g. for batching applications)

- 1 Supply tank
- 2 Sensor
- 3 Orifice plate, pipe restriction
- 4 Valve
- 5 Filling container

DN/	NPS	Ø orifice plate, pipe restriction			
[mm]	[in]	[mm]	[in]		
8	3/8	6	0.24		
15	1/2	10	0.40		
25	1	14	0.55		
40	1 ½	22	0.87		
50	2	28	1.10		
80	3	50	1.97		


#### Orientation

The direction of the arrow on the sensor nameplate helps you to install the sensor according to the flow direction (direction of medium flow through the piping).

	Orientation										
A	Vertical orientation	A0015591	<b>√ √</b> <sup>1)</sup>								
В	Horizontal orientation, transmitter at top	A0015589	✓ ✓ <sup>2)</sup> Exception: → 🖸 15, 🖺 57								
С	Horizontal orientation, transmitter at bottom	A0015590	<b>√√√</b> <sup>3)</sup> Exception: → <b>1</b> 5, <b>1</b> 5								
D	Horizontal orientation, transmitter at side	A0015592	×								

- 1) This orientation is recommended to ensure self-draining.
- 2) Applications with low process temperatures may reduce the ambient temperature. To maintain the minimum ambient temperature for the transmitter, this orientation is recommended.
- 3) Applications with high process temperatures may increase the ambient temperature. To maintain the maximum ambient temperature for the transmitter, this orientation is recommended.

If a sensor is installed horizontally with a curved measuring tube, match the position of the sensor to the medium properties.

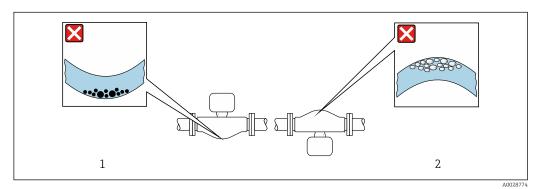

■ 15 Orientation of sensor with curved measuring tube

- 1 Avoid this orientation for media with entrained solids: Risk of solids accumulating
- 2 Avoid this orientation for outgassing media: Risk of gas accumulating

#### Inlet and outlet runs

No special precautions need to be taken for fittings that create turbulence, such as valves, elbows or T-pieces, as long as no cavitation occurs  $\rightarrow \ \cong$  65.

# Special installation instructions

#### **Drainability**

When installed vertically, the measuring tubes can be drained completely and protected against buildup.

#### Hygienic compatibility



- In the case of measuring devices with the order code for "Housing", option B "Stainless, hygienic", to seal the connection compartment cover, screw it closed finger-tight and tighten it by another 45° (corresponds to 15 Nm).

#### Rupture disk

Process-related information:  $\rightarrow \triangleq 65$ .


#### **WARNING**

#### Danger from medium escaping!

Medium escaping under pressure can cause injury or material damage.

- ▶ Take precautions to prevent danger to persons and damage if the rupture disk is actuated.
- ▶ Observe the information on the rupture disk sticker.
- Make sure that the function and operation of the rupture disk is not impeded through the installation of the device.
- Do not use a heating jacket.
- ▶ Do not remove or damage the rupture disk.

The position of the rupture disk is indicated on a sticker applied over it. If the rupture disk is triggered, the sticker is destroyed. The disk can therefore be visually monitored.

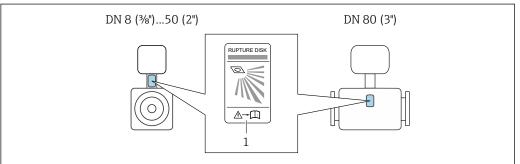

A0029956

Rupture disk label

#### Zero point verification and zero adjustment


Experience shows that zero adjustment is advisable only in special cases:

- To achieve maximum measurement accuracy even with low flow rates.
- Under extreme process or operating conditions (e.g. very high process temperatures or very highviscosity media).
- For gas applications with low pressure.

For information on checking the zero point and performing a zero adjustment, see the Operating Instructions for the device.

To achieve the highest possible measurement accuracy at low flow rates, the installation must protect the sensor from mechanical stress during operation.

#### Protective cover

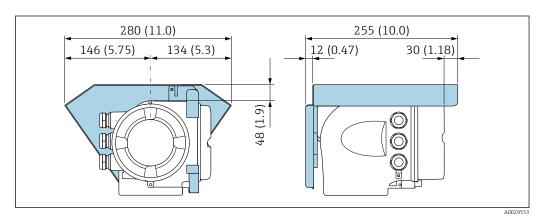

■ 16 Unit mm (in)

# **Environment**

Amhient	temner	ature	range

Measuring instrument	<ul> <li>−40 to +60 °C (−40 to +140 °F)</li> <li>Order code for "Test, certificate", option JP:</li> <li>−50 to +60 °C (−58 to +140 °F)</li> </ul>
Readability of the local display	-20 to $+60$ °C ( $-4$ to $+140$ °F) The readability of the display may be impaired at temperatures outside the temperature range.

- Popendency of ambient temperature on medium temperature  $\rightarrow = 59$
- ► If operating outdoors:

  Avoid direct sunlight, particularly in warm climatic regions.

Storage temperature	−50 to +80 °C (−58 to +176 °F)
Climate class	DIN EN 60068-2-38 (test Z/AD)

# **Relative humidity** The device is suitable for use in outdoor and indoor areas with a relative humidity of 4 to 95%.

# According to EN 61010-1 Operating height $\leq 2000 \text{ m} (6562 \text{ ft})$ Transmitter Degree of protection • IP66/67, Type 4X enclosure, suitable for pollution degree 4 • When the housing is open: IP20, Type 1 enclosure, suitable for pollution degree 2 • Display module: IP20, Type 1 enclosure, suitable for pollution degree 2 Optional Order code for "Sensor options", option CM "IP69" External WLAN antenna IP67 Vibration resistance and Sinusoidal vibration similar to IEC 60068-2-6 shock resistance 2 to 8.4 Hz, 3.5 mm peak 8.4 to 2000 Hz, 1 g peak Broadband random vibration similar to IEC 60068-2-64 ■ 10 to 200 Hz, 0.003 q<sup>2</sup>/Hz ■ 200 to 2000 Hz, 0.001 g<sup>2</sup>/Hz ■ Total: 1.54 g rms Half-sine shocks similar to IEC 60068-2-27 6 ms 30 g Rough handling shocks similar to IEC 60068-2-31 Mechanical load Transmitter housing: Protect against mechanical effects, such as shock or impact • Do not use as a ladder or climbing aid Electromagnetic As per IEC/EN 61326 and NAMUR Recommendation 21 (NE 21), NAMUR Recommendation 21 (NE 21) is fulfilled when the device is installed in accordance with NAMUR Recommendation 98 compatibility (EMC) (NE 98). ■ As per IEC/EN 61000-6-2 and IEC/EN 61000-6-4 Device version with PROFIBUS DP: Complies with emission limits for industry as per EN 50170 Volume 2, IEC 61784 The following applies for PROFIBUS DP: If baud rates > 1.5 MBaud, an EMC cable entry must be used and the cable shield must continue as far as the terminal wherever possible. Details are provided in the Declaration of Conformity. This unit is not intended for use in residential environments and cannot guarantee adequate


# **Process**

**Medium temperature range** -40 to +150 °C (-40 to +302 °F)

Endress+Hauser 59

protection of the radio reception in such environments.

#### Dependency of ambient temperature on medium temperature

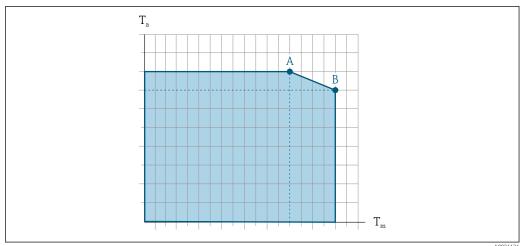

AUU3112

- 17 Exemplary representation, values in the table below.
- *T<sub>a</sub>* Ambient temperature
- $T_m$  Medium temperature
- Maximum permitted medium temperature  $T_m$  at  $T_{a max}$  = 60 °C (140 °F); higher medium temperatures  $T_m$  require a reduction in the ambient temperature  $T_a$
- B Maximum permitted ambient temperature  $T_a$  for the maximum specified medium temperature  $T_m$  of the sensor
- Values for devices that are used in the hazardous area: Separate Ex documentation (XA) for the device  $\rightarrow \stackrel{\triangle}{=} 116$ .

Not insulated				Insulated					
A B				A		В			
T <sub>a</sub>	T <sub>m</sub>	Ta	T <sub>m</sub>	T <sub>a</sub>	T <sub>m</sub>	T <sub>a</sub>	T <sub>m</sub>		
60 °C (140 °F)	150 °C (302 °F)	-	-	60 °C (140 °F)	110 °C (230 °F)	55 ℃ (131 ℉)	150 °C (302 °F)		


#### Medium density

0 to  $5000 \text{ kg/m}^3$  (0 to 312 lb/cf)

# Pressure/temperature ratings


The following pressure/temperature diagrams apply to all pressure-bearing parts of the device and not just the process connection. The diagrams show the maximum permissible medium pressure depending on the specific medium temperature.

### Flange similar to EN 1092-1 (DIN 2501)

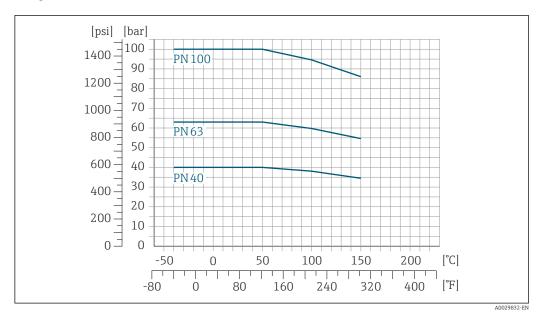


■ 18 With flange material 1.4404 (F316/F316L)

### Flange similar to ASME B16.5

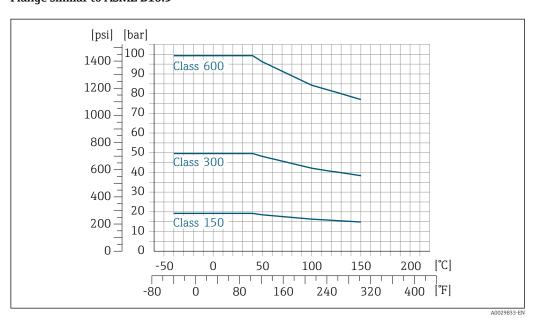


■ 19 With flange material 1.4404 (F316/F316L)

# Flange JIS B2220

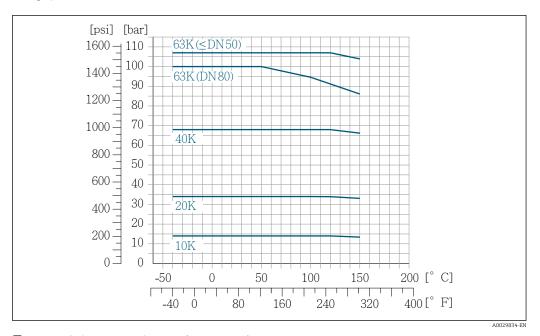


■ 20 With flange material 1.4404 (F316/F316L)

# Flange DIN 11864-2 Form A

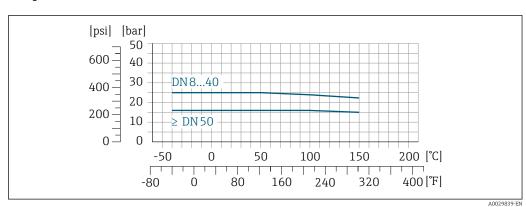

■ 21 With flange material 1.4404 (316/316L)


# Threaded adapter DIN 11851

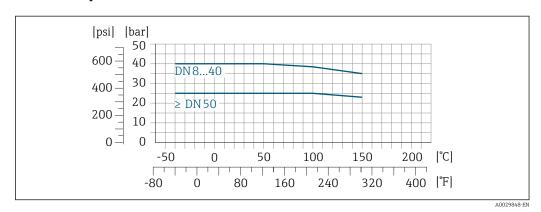

**■** 22 With connection material 1.4404 (316/316L)


DIN 11851 allows for applications up to +140  $^{\circ}$ C (+284  $^{\circ}$ F) if suitable sealing materials are used. Please take this into account when selecting seals and counterparts, as these components can limit the pressure and temperature range.

### Threaded adapter DIN 11864-1 Form A

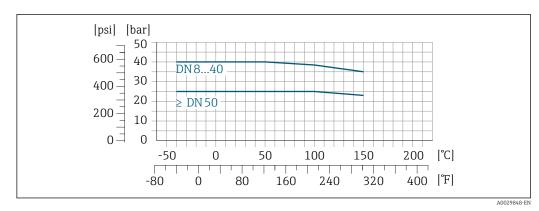


**■** 23 With connection material 1.4404 (316/316L)

### Threaded adapter ISO 2853

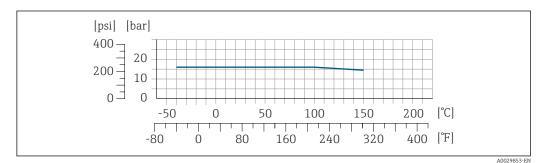


■ 24 With connection material 1.4404 (316/316L)

#### Threaded adapter SMS 1145

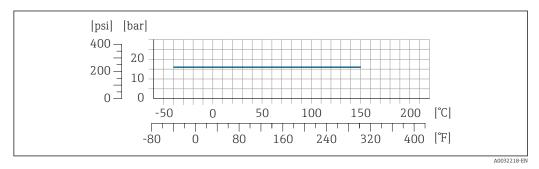


 $\blacksquare$  25 With connection material 1.4404 (316/316L)

#### VCO

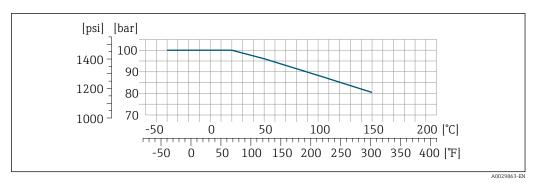

**■** 26 With connection material 1.4404 (316/316L)

#### Tri-Clamp

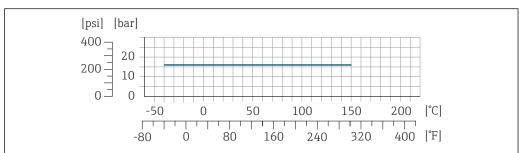

A0032218-EN

The clamp connections are suitable up to a maximum pressure of 16 bar (232 psi). Please observe the operating limits of the clamp and seal used as they can be over 16 bar (232 psi). The clamp and seal are not included in the scope of supply.

#### Sensor housing

The sensor housing is filled with dry nitrogen gas and protects the electronics and mechanics inside.



If a measuring tube fails (e.g. due to process characteristics like corrosive or abrasive fluids), the fluid will initially be contained by the sensor housing.

In the event of a tube failure, the pressure level inside the sensor housing will rise according to the operating process pressure. If the user judges that the sensor housing burst pressure does not provide an adequate safety margin, the device can be fitted with a rupture disk. This prevents excessively high pressure from forming inside the sensor housing. Therefore, the use of a rupture disk is strongly recommended in applications involving high gas pressures, and particularly in applications in which the process pressure is greater than 2/3 of the sensor housing burst pressure.

#### Burst pressure of the sensor housing

If the device is fitted with a rupture disk (order code for "Sensor option", option CA "Rupture disk"), the rupture disk trigger pressure is decisive .

The sensor housing burst pressure refers to a typical internal pressure which is reached prior to mechanical failure of the sensor housing and which was determined during type testing. The corresponding type test declaration can be ordered with the device (order code for "Additional approval", option LN "Sensor housing burst pressure, type test").

D	N	Sensor housing burst pressure				
[mm]	[in]	[bar]	[psi]			
8	3/8	250	3620			
15	1/2	250	3620			
25	1	250	3620			
40	11/2	200	2 900			

64

D	N	Sensor housing burst pressure				
[mm]	[in]	[bar]	[psi]			
50	2	180	2610			
80	3	120	1740			

For information on the dimensions: see the "Mechanical construction" section  $\rightarrow \triangleq 67$ 

#### Rupture disk

To increase the level of safety, a device version with a rupture disk with a trigger pressure of 10 to 15 bar (145 to 217.5 psi) can be used (order code for "Sensor option", option CA "rupture disk").

The use of rupture disks cannot be combined with the separately available heating jacket.


#### Internal cleaning

- CIP cleaning
- SIP cleaning

Oil- and grease-free version for wetted parts, without declaration Order code for "Service", option HA 1)

#### Flow limit

Select the nominal diameter by optimizing between the required flow range and permissible pressure loss.



- The minimum recommended full scale value is approx. 1/20 of the maximum full scale value
- For the most common applications, 20 to 50 % of the maximum full scale value can be considered
- A low full scale value must be selected for abrasive media (such as liquids with entrained solids): flow velocity < 1 m/s (< 3 ft/s).
- For gas measurement the following rules apply:
  - The flow velocity in the measuring tubes should not exceed half the speed of sound (0.5 Mach)
  - The maximum mass flow depends on the density of the gas: formula
- To calculate the flow limit, use the *Applicator* sizing tool  $\rightarrow \implies 114$

#### Pressure loss




To calculate the pressure loss, use the *Applicator* sizing tool  $\rightarrow \triangleq 114$ 

#### Static pressure

It is important that cavitation does not occur, or that gases entrained in the liquids do not outgas. This is prevented by means of a sufficiently high static pressure.

For this reason, the following mounting locations are recommended:

- At the lowest point in a vertical pipe
- Downstream from pumps (no danger of vacuum)



#### Thermal insulation


In the case of some fluids, it is important to keep the heat radiated from the sensor to the transmitter to a low level. A wide range of materials can be used for the required insulation.

Cleaning only refers to the measuring instrument. Any accessories that have been supplied are not cleaned.

#### NOTICE

#### Electronics overheating on account of thermal insulation!

- Recommended orientation: horizontal orientation, transmitter housing pointing downwards.
- ▶ Do not insulate the transmitter housing.
- $\blacktriangleright$  Maximum permissible temperature at the lower end of the transmitter housing: 80 °C (176 °F)
- ► Thermal insulation with exposed extension neck: We recommend that you do not insulate the extension neck in order to ensure optimum dissipation of heat.

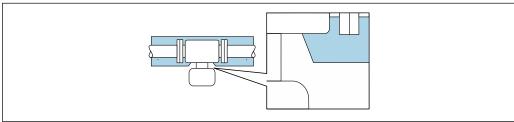

27 Thermal insulation with exposed extension neck

A0034391

### Heating

Some media require suitable measures to avoid loss of heat at the sensor.

#### **Heating options**

- Electrical heating, e.g. with electric band heaters <sup>2)</sup>
- Via pipes carrying hot water or steam
- Via heating jackets
- i

#### **NOTICE**

#### Danger of overheating when heating

- ► Ensure that the temperature at the lower end of the transmitter housing does not exceed 80 °C (176 °F).
- ► Ensure that sufficient convection takes place at the transmitter neck.
- Ensure that a sufficiently large area of the transmitter neck remains exposed. The uncovered part serves as a radiator and protects the electronics from overheating and excessive cooling.
- When using in potentially explosive atmospheres, observe the information in the device-specific Ex documentation. For detailed information on the temperature tables, see the separate document entitled "Safety Instructions" (XA) for the device.
- ► Consider the behavior of the process diagnostics "830 Ambient temperature too high" and "832 Electronics temperature too high" if overheating cannot be avoided by a suitable system design.

### Vibrations

The high oscillation frequency of the measuring tubes ensures that the correct operation of the measuring system is not influenced by plant vibrations.


66

<sup>2)</sup> The use of parallel electric band heaters is generally recommended (bidirectional electricity flow). Particular considerations must be made if a single-wire heating cable is to be used. Additional information is provided in the document EA01339D "Installation instructions for electrical trace heating systems" > 118

# Mechanical construction

#### Dimensions in SI units

### **Compact version**

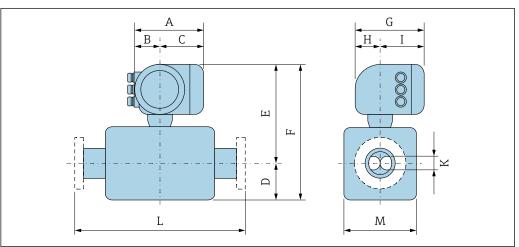

Order code for "Housing", option A "Aluminum, coated"

DN	A 1)	B 1)	С	D	Е	F	G <sup>2)</sup>	Н	I 2)	K	L	М
[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]
8	169	68	101	89	252	341	200	59	141	5.35	3)	45
15	169	68	101	100	252	352	200	59	141	8.30	3)	45
25	169	68	101	102	249	351	200	59	141	12.0	3)	51
40	169	68	101	121	255	376	200	59	141	17.6	3)	65
50	169	68	101	175.5	269.5	445	200	59	141	26.0	3)	95
80	169	68	101	205	288.5	493.5	200	59	141	40.5	3)	127

- Depending on the cable gland used: values up to  $\pm$  30 mm 1)
- 2) 3) For version without local display: values - 30 mm
- Depending on the process connection

### Order code for "Housing", option A "Aluminum, coated"; Ex d

DN	A 1)	B 1)	С	D	Е	F	G <sup>2)</sup>	Н	I 2)	K	L	М
[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]
8	188	85	103	89	253	342	217	58	159	5.35	3)	45
15	188	85	103	100	253	353	217	58	159	8.30	3)	45
25	188	85	103	102	250	352	217	58	159	12.0	3)	51
40	188	85	103	121	256	377	217	58	159	17.6	3)	65
50	188	85	103	175.5	270	445.5	217	58	159	26.0	3)	95
80	188	85	103	205	289	494	217	58	159	40.5	3)	127

- 1) Depending on the cable gland used: values up to + 30 mm
- For version without local display: values 40 mm
- Depending on the process connection


Order code for "Housing", option B "Stainless, hygienic"

DN	A 1)	B 1)	С	D	Е	F	G 2)	Н	I 2)	K	L	M
[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]
8	183	73	110	89	252	341	200	65	135	5.35	3)	45
15	183	73	110	100	252	352	200	65	135	8.30	3)	45
25	183	73	110	102	249	351	200	65	135	12.0	3)	51
40	183	73	110	121	255	376	200	65	135	17.6	3)	65
50	183	73	110	175.5	269.5	445	200	65	135	26.0	3)	95
80	183	73	110	205	288.5	493.5	200	65	135	40.5	3)	127

- Depending on the cable gland used: values up to  $\pm$  30 mm For version without local display: values  $\pm$  13 mm Depending on the process connection
- 1) 2) 3)

#### Flange connections

Fixed flange EN 1092-1, ASME B16.5, JIS B2220

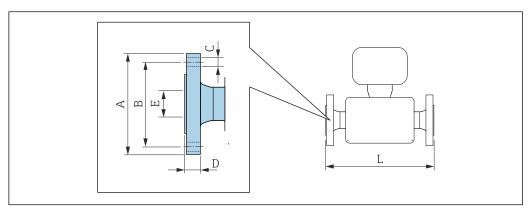

A0015621

i

Length tolerance for dimension L in mm: +1.5/-2.0

#### Flange similar to EN 1092-1 (DIN 2501/DIN 2512N), PN 40

1.4404 (F316/F316L): order code for "Process connection", option D2S

Flange with groove similar to EN 1092-1 Form D (DIN 2512N), PN 40  $\,$ 

1.4404 (F316/F316L): order code for "Process connection", option D6S

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
8 <sup>1)</sup>	95	65	4 × Ø14	16	17.3	232/510 <sup>2)</sup>
15	95	65	4 × Ø14	16	17.3	279/510 <sup>2)</sup>
25	115	85	4 × Ø14	18	28.5	329/600 <sup>2)</sup>
40	150	110	4 × Ø18	18	43.1	445
50	165	125	4 × Ø18	20	54.5	556/715 <sup>2)</sup>
80	200	160	8 × Ø18	24	82.5	611/915 <sup>2)</sup>

Surface roughness (flange): EN 1092-1 Form B1 (DIN 2526 Form C), Ra 3.2 to 12.5  $\mu$ m

- 1) DN 8 with DN 15 flanges as standard
- Installed length in accordance with NAMUR recommendation NE 132 optionally available (order code for "Process connection", option D2N or D6N (with groove))

Flange similar to EN 1092-1 (DIN 2501), PN 40 (with DN 25 flanges) 1.4404 (F316/F316L) Order code for "Process connection", option R2S										
DN         A         B         C         D         E         L           [mm]         [mm]         [mm]         [mm]         [mm]										
8	115	85	4 × Ø14	18	28.5	329				
15 115 85 4 × Ø14 18 28.5 329										
Surface roughn	iess (flange): EN	1092-1 Form F	31 (DIN 2526 Forn	n C), Ra 3.2 to 12	2.5 µm					

Flange similar to EN 1092-1 (DIN 2501/DIN 2512N), PN 63

1.4404 (F316/F316L): order code for "Process connection", option D3S

Flange with groove similar to EN 1092-1 Form D (DIN 2512N), PN 63

1.4404 (F316/F316L): order code for "Process connection", option D7S

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
50	180	135	4 × Ø22	26	54.5	565
80	215	170	8 × Ø22	28	81.7	646

Surface roughness (flange): EN 1092-1 Form B2 (DIN 2526 Form E), Ra 0.8 to 3.2  $\mu m$ 

#### Flange similar to EN 1092-1 (DIN 2501/DIN 2512N), PN 100 1.4404 (F316/F316L)

Order code for "Process connection", option D4S

Flange with groove similar to EN 1092-1 Form D (DIN 2512N) available, PN 100 1.4404 (F316/F316L)

Surface roughness (flange): EN 1092-1 Form B2 (DIN 2526 Form E), Ra 0.8 to 3.2  $\mu m$ 

Order code for "Process connection", option  ${\bf D8S}$ 

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
8 1)	105	75	4 × Ø14	20	17.3	261
15	105	75	4 × Ø14	20	17.3	295
25	140	100	4 × Ø18	24	28.5	360
40	170	125	4 × Ø22	26	42.5	486
50	195	145	4 × Ø26	28	53.9	581
80	230	180	8 × Ø26	32	80.9	656

#### 1) DN 8 with DN 15 flanges as standard

Flange similar to ASME B16.5, Class 150 1.4404 (F316/F316L)

Order code for	Order code for "Process connection", option AAS										
DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]					
8 <sup>1)</sup>	90	60.3	4 × Ø15.7	11.2	15.7	232					
15	90	60.3	4 × Ø15.7	11.2	15.7	279					
25	110	79.4	4 × Ø15.7	14.2	26.7	329					
40	125	98.4	4 × Ø15.7	17.5	40.9	445					
50	150	120.7	4 × Ø19.1	19.1	52.6	556					
80	190	152.4	4 × Ø19.1	23.9	78.0	611					
Surface rough	ness (flange): R	a 3.2 to 6.3 um	1								

DN 8 with DN 15 flanges as standard

#### Flange similar to ASME B16.5, Class 300 1.4404 (F316/F316L) Order code for "Process connection", option ABS DN В С D Ε L [mm] [mm] [mm] [mm] [mm] [mm] [mm] 8 1) 95 66.7 $4 \times \emptyset 15.7$ 14.2 15.7 232 15 95 $4 \times Ø15.7$ 15.7 279 66.7 14.2

#### Flange similar to ASME B16.5, Class 300 1.4404 (F316/F316L)

Order code for "Process connection", option ABS

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
25	125	88.9	4 × Ø19.0	17.5	26.7	329
40	155	114.3	4 × Ø22.3	20.6	40.9	445
50	165	127	8 × Ø19.0	22.3	52.6	556
80	210	168.3	8 × Ø22.3	28.4	78.0	611
Surface rough	ness (flange): R	a 3.2 to 6.3 µm	1			

1) DN 8 with DN 15 flanges as standard  $\,$ 

#### Flange similar to ASME B16.5, Class 600 1.4404 (F316/F316L)

Order code for "Process connection", option ACS

Oraci code joi	order code for Process connection, option Acts											
DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]						
8 <sup>1)</sup>	95	66.7	4 × Ø15.7	20.6	13.9	261						
15	95	66.7	4 × Ø15.7	20.6	13.9	295						
25	125	88.9	4 × Ø19.1	23.9	24.3	380						
40	155	114.3	4 × Ø22.4	28.7	38.1	496						
50	165	127	8 × Ø19.1	31.8	49.2	583						
80	210	168.3	8 × Ø22.4	38.2	73.7	671						
Surface rough	ness (flange): R	Ra 3.2 to 6.3 µm	1									

1) DN 8 with DN 15 flanges as standard

# Flange JIS B2220, 10K 1.4404 (F316/F316L)

Order code for "Process connection", option NDS

	· · · · · · · · · · · · · · · · · · ·										
DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]					
50	155	120	4 × Ø19	16	50	556					
80	185	150	8 × Ø19	18	80	603					

Surface roughness (flange): Ra 3.2 to 6.3 µm

#### Flange JIS B2220, 20K 1.4404 (F316/F316L)

Order code for	Order code for "Process connection", option <b>NES</b>										
DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]					
8 1)	95	70	4 × Ø15	14	15	232					
15	95	70	4 × Ø15	14	15	279					
25	125	90	4 × Ø19	16	25	329					
40	140	105	4 × Ø19	18	40	445					
50	155	120	8 × Ø19	18	50	556					

Flange JIS B2220, 20K 1.4404 (F316/F316L) Order code for "Process connection", option NES								
DN         A         B         C         D         E         L           [mm]         [mm]         [mm]         [mm]         [mm]								
80	80 200 160 8 × Ø23 22 80 603							
Surface roughness (flange): Ra 3.2 to 6.3 μm								

1) DN 8 with DN 15 flanges as standard


Flange JIS B2220, 40K 1.4404 (F316/F316L) Order code for "Process connection", option NGS										
DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]				
8 <sup>1)</sup>	115	80	4 × Ø19	20	15	261				
15	115	80	4 × Ø19	20	15	300				
25	130	95	4 × Ø19	22	25	375				
40	160	120	4 × Ø23	24	38	496				
50	165	130	8 × Ø19	26	50	601				
80	80 210 170 8 × Ø23 32 75 661									
Surface roughr	ness (flange): Ra	3.2 to 6.3 µm								

1) DN 8 with DN 15 flanges as standard

Flange JIS B2220, 63K 1.4404 (F316/F316L) Order code for "Process connection", option NHS						
DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
8 <sup>1)</sup>	120	85	4 × Ø19	23	12	282
15	120	85	4 × Ø19	23	12	315
25	140	100	4 × Ø23	27	22	383
40	175	130	4 × Ø25	32	35	515
50	185	145	4 × Ø23	34	48	616
80	230	185	4 × Ø25	40	73	686
Surface roughness (flange): Ra 3.2 to 6.3 µm						

1) DN 8 with DN 15 flanges as standard

### Fixed flange DIN 11864-2

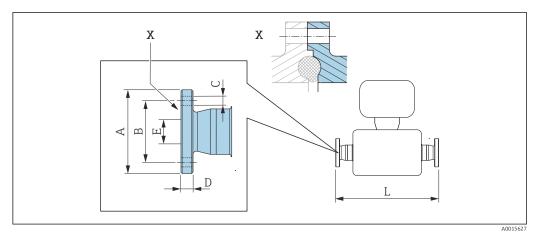

■ 28 Detail X: Asymmetrical process connection; the part shown in blue is provided by the supplier.

Flange DIN11864-2 Form A, for pipe according to DIN11866 series A, flange with notch

Length tolerance for dimension L in mm: +1.5/-2.0

#### 1.4404 (316/316L) Order code for "Process connection", option KCS DN С D E L В [mm] [mm] [mm] [mm] [mm] [mm] [mm] 8 1) 54 37 4 × Ø9 10 10 249 15 59 42 $4 \times Ø9$ 10 16 293 25 70 53 $4 \times Ø9$ 10 26 344 82 456 40 65 $4 \times Ø9$ 10 38 50 94 77 $4 \times Ø9$ 10 50 562 80 133 112 8 × Ø11 12 81 671

3-A version available: order code for "Additional approval", option LP in conjunction with


 $Ra \leq 0.76~\mu m$  order code for "Measuring tube material", option SB, SJ

 $Ra \leq 0.38~\mu m$ : order code for "Measuring tube material", option SC, SK

1) DN 8 with DN 10 flanges as standard

### Clamp connections

# Tri-Clamp

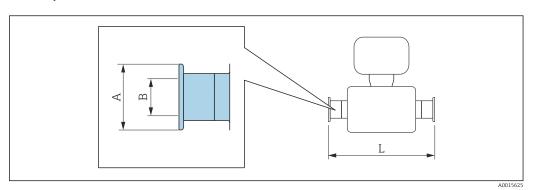

Length tolerance for dimension L in mm: +1.5/-2.0

#### Tri-Clamp ( $\frac{1}{2}$ "), for pipe according to DIN 11866 series C 1.4404 (316/316L) Order code for "Process connection", option FDW DN Clamp В L Α [mm] [in] [mm] [mm] [mm] 8 1/2 25.0 9.5 229 15 1/2 25.0 9.5 273

 $\hbox{3-A version available: order code for "Additional approval", option LP in conjunction with $$ $(1)$ and $(1)$ are also conjunction with $(1)$ and $(1)$ are also conjunction with $(1)$ and $(1)$ are also conjunction with $(1)$ are also conjunction wit$ 

 $Ra \le 0.76 \ \mu m$ : order code for "Measuring tube material", option SB, SJ

 $Ra \leq 0.38~\mu m$ : order code for "Measuring tube material", option SC, SK

Tri-Clamp (≥ 1"), for pipe according to DIN 11866 series C  1.4404 (316/316L)  Order code for "Process connection", option FTS										
DN [mm]	Clamp [in]	A [mm]	B [mm]	L [mm]						
8	1	50.4	22.1	229						
15	1	50.4	22.1	273						
25	1	50.4	22.1	324						
40	11/2	50.4	34.8	456						
50	2	63.9	47.5	562						
80	3	90.9	72.9	671						


3-A version available: order code for "Additional approval", option LP in conjunction with

 $Ra \le 0.76 \ \mu m$ : order code for "Measuring tube material", option SB, SJ

 $Ra \leq 0.38~\mu m$ : order code for "Measuring tube material", option SC, SK

### Threaded couplings

Threaded adapter DIN 11851, DIN11864-1, SMS 1145

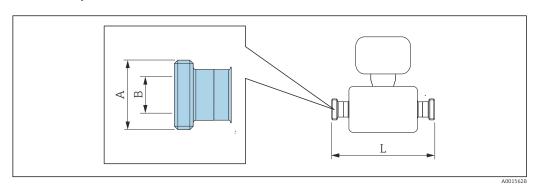

Length tolerance for dimension L in mm: +1.5/-2.0

Threaded adapter DIN 11851, for pipe according to DIN11866 series A 1.4404 (316/316L)  Order code for "Process connection", option FMW									
DN [mm]	A [in]	B [mm]	L [mm]						
8	Rd 34 × ½	16	229						
15	Rd 34 × ½	16	273						
25	Rd 52 × ½	26	324						
40	Rd 65 × ½	38	456						
50	Rd 78 × ½	50	562						
80	Rd 110 × 1/4	81	671						

3-A version available: order code for "Additional approval", option LP in conjunction with

Threaded adapter DIN11864-1 Form A, for pipe according to DIN11866 series A

Ra  $\leq$  0.76 µm: order code for "Measuring tube material", option SB, SJ Ra  $\leq$  0.38 µm: order code for "Measuring tube material", option SC, SK

1.4404 (316/316L) Order code for "Process connection", option FLW									
DN [mm]	A [in]	B [mm]	L [mm]						
8	Rd 28 × ½	10	229						
15	Rd 34 × ⅓	16	273						
25	Rd 52 × <sup>1</sup> ⁄ <sub>6</sub>	26	324						
40	Rd 65 × ½	38	456						
50	Rd 78 × ½	50	562						

671

3-A version available: order code for "Additional approval", option LP in conjunction with

Rd 110 × 1/4

Ra  $\leq 0.76~\mu m$ : order code for "Measuring tube material", option SB, SJ Ra  $\leq 0.38~\mu m$ : order code for "Measuring tube material", option SC, SK


# Threaded adapter SMS 1145 1.4404 (316/316L)

Order code for "Process connection", option SCS

,	, ,		
DN [mm]	A [in]	B [mm]	L [mm]
8	Rd 40 × 1/ <sub>6</sub>	22.5	229
15	Rd 40 × 1/ <sub>6</sub>	22.5	273
25	Rd 40 × 1/ <sub>6</sub>	22.5	324
40	Rd 60 × 1/ <sub>6</sub>	35.5	456
50	Rd 70 × ⅓	48.5	562
80	Rd 98 × 1/ <sub>6</sub>	72.9	671

<sup>3-</sup>A version available: order code for "Additional approval", option LP in conjunction with Ra  $\leq 0.76~\mu m$ : order code for "Measuring tube material", option SB, SJ Ra  $\leq 0.38~\mu m$ : order code for "Measuring tube material", option SC, SK

# Threaded adapter ISO 2853

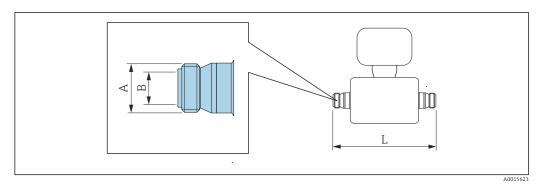

Length tolerance for dimension L in mm:  $\pm 1.5/-2.0$ 


Threaded adapter ISO 2853, for pipe according to ISO 2037 1.4404 (316/316L) Order code for "Process connection", option JSF									
DN [mm]	A 1) [mm]	B [mm]	L [mm]						
8	37.13	22.6	229						
15	37.13	22.6	273						
25	37.13	22.6	324						
40	50.68	35.6	456						
50	64.16	48.6	562						
80	91.19	72.9	671						

<sup>3-</sup>A version available: order code for "Additional approval", option  $\overrightarrow{\text{LP}}$  in conjunction with

Ra  $\leq$  0.76 µm: order code for "Measuring tube material", option SB, SJ Ra  $\leq$  0.38 µm: order code for "Measuring tube material", option SC, SK

Max. thread diameter according to ISO 2853 Annex A

VCO

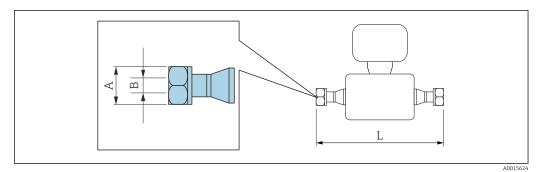


Length tolerance for dimension L in mm: +1.5/-2.0

8-VCO-4 (½") 1.4404 (316/316L) Order code for "Process connection", option CVS									
DN [mm]									
8	AF 1	10.2	252						

12-VCO-4 (¾") 1.4404 (316/316L) Order code for "Process conn								
DN [mm]	A [in]	B [mm]	L [mm]					
15	AF 1½	15.7	305					


# Accessories

# Protective cover

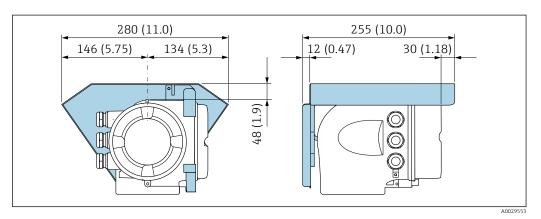

■ 29 Unit mm (in)

### Remote display and operating module DKX001

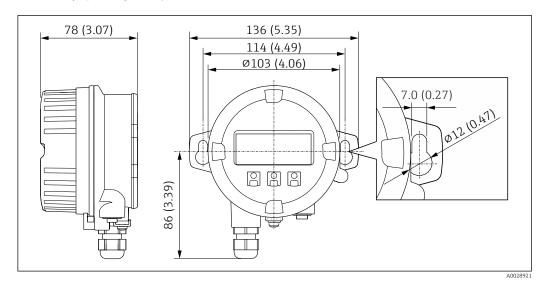


■ 30 Unit mm (in)

# External WLAN antenna

The external WLAN antenna is not suitable for use in hygienic applications.


#### External WLAN antenna mounted on device

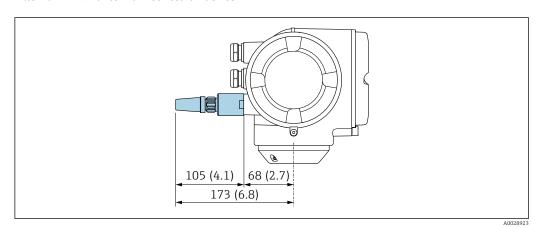

■ 31 Unit mm (in)

### External WLAN antenna mounted with cable


The external WLAN antenna can be mounted separately from the transmitter if the transmission/reception conditions at the transmitter mounting location are poor.

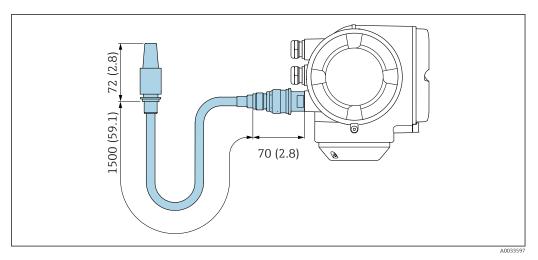

■ 32 Unit mm (in)

# Dimensions in US units

# **Compact version**

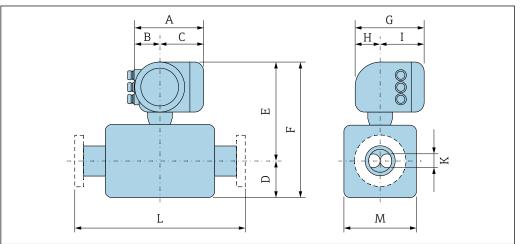

Order code for "Housing", option A "Aluminum, coated"

DN	A 1)	B 1)	С	D	Е	F	G <sup>2)</sup>	Н	I 2)	K	L	M
[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]
3/8	6.65	2.68	3.98	3.5	9.92	13.43	7.87	2.32	5.55	0.21	3)	1.77
1/2	6.65	2.68	3.98	3.94	9.92	13.86	7.87	2.32	5.55	0.33	3)	1.77
1	6.65	2.68	3.98	4.02	9.8	13.82	7.87	2.32	5.55	0.47	3)	2.01
1½	6.65	2.68	3.98	4.76	10.04	14.8	7.87	2.32	5.55	0.69	3)	2.56
2	6.65	2.68	3.98	6.91	10.61	17.52	7.87	2.32	5.55	1.02	3)	3.74
3	6.65	2.68	3.98	8.07	11.36	19.43	7.87	2.32	5.55	1.59	3)	5.00

- Depending on the cable gland used: values up to  $\pm$  1.18 in 1)
- 2) For version without local display: values - 1.18 in
- 3) Depending on the process connection

# Order code for "Housing", option A "Aluminum, coated"; Ex d

DN	A 1)	B 1)	С	D	Е	F	G <sup>2)</sup>	Н	I 2)	K	L	М
[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]
3/8	7.40	3.35	4.06	3.5	9.96	13.46	8.54	2.28	6.26	0.21	3)	1.77
1/2	7.40	3.35	4.06	3.94	9.96	13.9	8.54	2.28	6.26	0.33	3)	1.77
1	7.40	3.35	4.06	4.02	9.84	13.86	8.54	2.28	6.26	0.47	3)	2.01
1½	7.40	3.35	4.06	4.76	10.08	14.84	8.54	2.28	6.26	0.69	3)	2.56
2	7.40	3.35	4.06	6.91	10.63	17.54	8.54	2.28	6.26	1.02	3)	3.74
3	7.40	3.35	4.06	8.07	11.38	19.45	8.54	2.28	6.26	1.59	3)	5.00

- Depending on the cable gland used: values up to  $\pm$  1.18 in 1)
- 2) For version without local display: values - 1.57 in
- Depending on the process connection


Order code for "Housing", option B "Stainless, hygienic"

DN	A 1)	B 1)	С	D	E	F	G 2)	Н	I 2)	K	L	M
[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]
3/8	7.20	2.87	4.33	3.5	9.92	13.43	7.87	2.56	5.31	0.21	3)	1.77
1/2	7.20	2.87	4.33	3.94	9.92	13.86	7.87	2.56	5.31	0.33	3)	1.77
1	7.20	2.87	4.33	4.02	9.8	13.82	7.87	2.56	5.31	0.47	3)	2.01
11/2	7.20	2.87	4.33	4.76	10.04	14.8	7.87	2.56	5.31	0.69	3)	2.56
2	7.20	2.87	4.33	6.91	10.61	17.52	7.87	2.56	5.31	1.02	3)	3.74
3	7.20	2.87	4.33	8.07	11.36	19.43	7.87	2.56	5.31	1.59	3)	5.00

- Depending on the cable gland used: values up to  $\pm$  1.18 in For version without local display: values  $\pm$  0.51 in Depending on the process connection 1) 2) 3)

# Flange connections

Fixed flange ASME B16.5

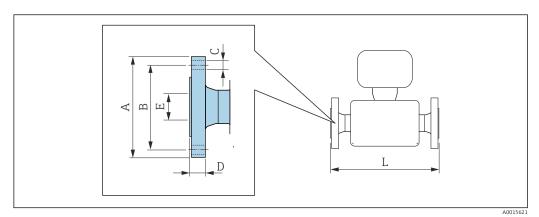

Length tolerance for dimension L in inches: +0.06/-0.08

Flange similar to ASME B16.5, Cl 150 1.4404 (F316/F316L) Order code for "Process connection", option AAS										
DN [in]	A [in]	B [in]	C [in]	D [in]	E [in]	L [in]				
3/8 1)	3.54	2.37	4 × Ø0.62	0.44	0.62	9.13				
1/2	3.54	2.37	4 × Ø0.62	0.44	0.62	10.98				
1	4.33	3.13	4 × Ø0.62	0.56	1.05	12.95				
1½	4.92	3.87	4 × Ø0.62	0.69	1.61	17.52				
2	5.91	4.75	4 × Ø0.75	0.75	2.07	21.89				
3	7.48	6.00	4 × Ø0.75	0.94	3.07	24.06				
Surface roug	ghness (flange	): Ra 126 to 24	48 μin							

1) DN  $\frac{3}{8}$ " with DN  $\frac{1}{2}$ " flanges as standard

Flange similar to ASME B16.5, Class 300 1.4404 (F316/F316L) Order code for "Process connection", option ABS										
DN [in]	A [in]	B [in]	C [in]	D [in]	E [in]	L [in]				
3/8 1)	3.74	2.63	4 × Ø0.62	0.56	0.62	9.13				
1/2	3.74	2.63	4 × Ø0.62	0.56	0.62	10.98				
1	4.92	3.50	4 × Ø0.75	0.69	1.05	12.95				
1½	6.10	4.50	4 × Ø0.88	0.81	1.61	17.52				
2	6.50	5.00	8 × Ø0.75	0.88	2.07	21.89				
3	8.27	6.63	8 × Ø0.88	1.12	3.07	24.06				
Surface rou	ghness (flange	): Ra 126 to 24	48 µin							


1) DN  $\frac{3}{8}$ " with DN  $\frac{1}{2}$ " flanges as standard

1.4404 (F3	Flange similar to ASME B16.5, Class 600 1.4404 (F316/F316L) Order code for "Process connection", option ACS					
DN [in]	A [in]	B [in]	C [in]	D [in]	E [in]	L [in]
3/8 1)	3.74	2.63	4 × Ø0.62	0.81	0.55	10.28
1/2	3.74	2.63	4 × Ø0.62	0.81	0.55	11.61
1	4.92	3.50	4 × Ø0.75	0.94	0.96	14.96
1½	6.10	4.50	4 × Ø0.88	1.13	1.50	19.53
2	6.50	5.00	8 × Ø0.75	1.25	1.94	22.95
3	8.27	6.63	8 × Ø0.88	1.50	2.9	26.42
Surface roug	Surface roughness (flange): Ra 126 to 248 µin					

<sup>1)</sup> DN  $^3\!/\!_8$  with DN  $^4\!/\!_2$  flanges as standard

# **Clamp connections**

# Tri-Clamp

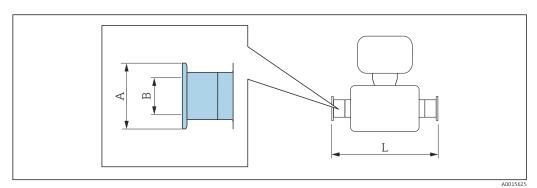

Length tolerance for dimension L in inches: +0.06/-0.08

Tri-Clamp (½"), DIN 11866 series C 1.4404 (316/316L) Order code for "Process connection", option FDW				
DN         Clamp         A         B         L           [in]         [in]         [in]         [in]				
3/8	1/2	0.98	0.37	9.02
1/2	1/2	0.98	0.37	10.75

3-A version available: order code for "Additional approval", option LP in conjunction with Ra  $\leq 30~\mu in$ : order code for "Measuring tube material", option SB, SJ

Ra  $\leq$  30  $\mu$ m: order code for "Measuring tube material", option SD, SJ Ra  $\leq$  15  $\mu$ m: order code for "Measuring tube material", option SC, SK

Tri-Clamp (≥ 1"), DIN 11866 series C 1.4404 (316/316L) Order code for "Process connection", option FTS				
DN [in]	Clamp [in]	A [in]	B [in]	L [in]
3/8	1	1.98	0.87	9.02
1/2	1	1.98	0.87	10.75
1	1	1.98	0.87	12.76
11/2	1½	1.98	1.37	17.95
2	2	2.52	1.87	22.13
3	3	3.58	2.87	26.42


3-A version available: order code for "Additional approval", option LP in conjunction with

 $Ra \le 30~\mu in:$  order code for "Measuring tube material", option SB, SJ

 $Ra \leq 15~\mu in:$  order code for "Measuring tube material", option SC, SK

# Threaded couplings

Threaded adapter SMS 1145

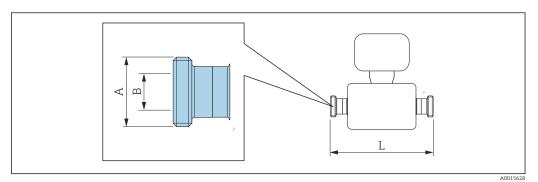


Length tolerance for dimension L in inches: +0.06/-0.08

Threaded adapter SMS 1145 1.4404 (316/316L) Order code for "Process connection", option SCS			
DN [in]	A [in]	B [in]	L [in]
3/8	Rd 40 × 1/ <sub>6</sub>	0.89	9.02
1/2	Rd 40 × 1/ <sub>6</sub>	0.89	10.75
1	Rd 40 × 1/ <sub>6</sub>	0.89	12.76
1½	Rd 60 × 1/ <sub>6</sub>	1.40	17.95
2	Rd 70 × 1/ <sub>6</sub>	1.91	22.13
3	Rd 98 × 1/6	2.87	26.42

3-A version available: order code for "Additional approval", option LP in conjunction with Ra  $\leq 30~\mu in$ : order code for "Measuring tube material", option SB, SJ Ra  $\leq 15~\mu in$ : order code for "Measuring tube material", option SC, SK

86

# VCO

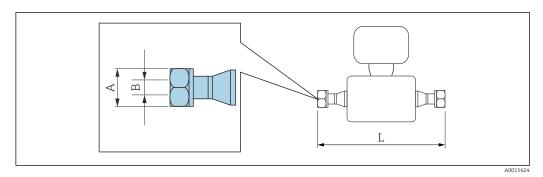


Length tolerance for dimension L in inches: +0.06/-0.08

8-VCO-4 (½") 1.4404 (316/316L) Order code for "Process connection", option CVS			
DN [in]	A [in]	B [in]	L [in]
3/8	AF 1	0.40	9.92

12-VCO-4 (¾") 1.4404 (316/316L) Order code for "Process connection", option CWS			
DN [in]	A [in]	B [in]	L [in]
1/2	AF 1½	0.62	12.01


# Accessories

# Protective cover

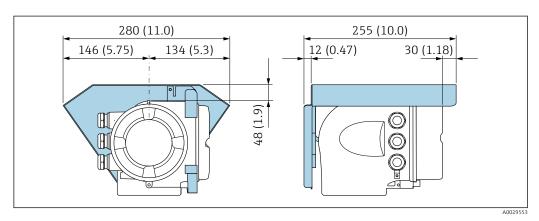

■ 33 Unit mm (in)


# Remote display and operating module DKX001

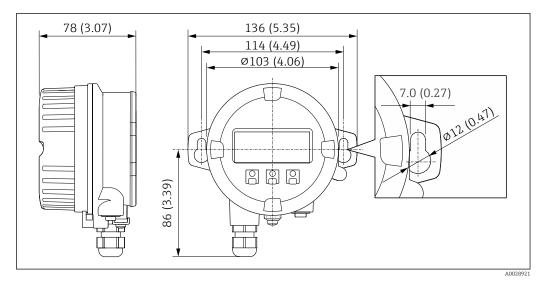

### External WLAN antenna

The external WLAN antenna is not suitable for use in hygienic applications.


#### External WLAN antenna mounted on device

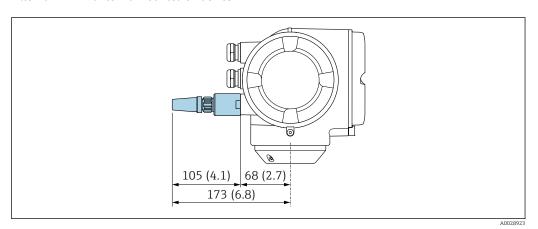

■ 35 Unit mm (in)

### External WLAN antenna mounted with cable

The external WLAN antenna can be mounted separately from the transmitter if the transmission/reception conditions at the transmitter mounting location are poor.

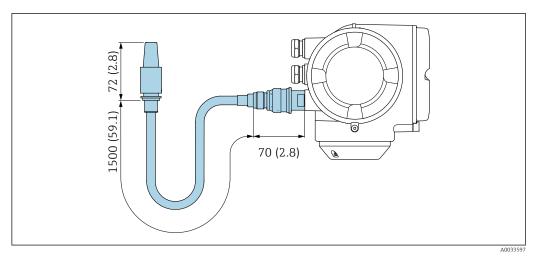

■ 36 Unit mm (in)

# Weight

All values (weight exclusive of packaging material) refer to devices with EN/DIN PN 40 flanges. Weight specifications including transmitter as per order code for "Housing", option A "Aluminum, coated"

Different values due to different transmitter versions:

- Transmitter version for the hazardous area (Order code for "Housing", option A "Aluminum, coated"; Ex d): +2 kg (+4.4 lbs)
- Transmitter version for hygienic area (Order code for "Housing", option B "Stainless, hygienic"): +0.2 kg (+0.44 lbs)

# Weight in SI units

DN [mm]	Weight [kg]
8	5
15	5.5
25	7
40	11
50	16
80	32

# Weight in US units

DN [in]	Weight [lbs]
3/8	11
1/2	12
1	15
1½	24
2	35
3	71

### Materials

# Transmitter housing

Order code for "Housing":

- Option A "Aluminum, coated": aluminum, AlSi10Mg, coated
- Option **B** "Stainless, hygienic": stainless steel, 1.4404 (316L)

Window material

Order code for "Housing":


- Option A "Aluminum, coated": glass
- Option **B** "Stainless, hygienic": polycarbonate

#### Seals

Order code for "Housing":

Option  ${\bf B}$  "Stainless, hygienic": EPDM and silicone

# Cable entries/cable glands

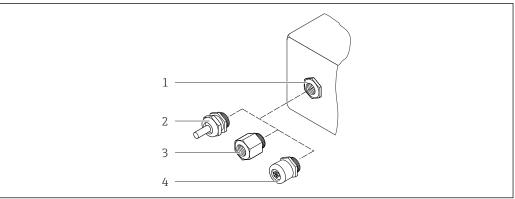

A002835

# ■ 37 Possible cable entries/cable glands

- 1 Internal thread  $M20 \times 1.5$
- 2 Cable gland  $M20 \times 1.5$
- 3 Adapter for cable entry with internal thread G  $\frac{1}{2}$ " or NPT  $\frac{1}{2}$ "
- 4 Device plug

Order code for "Housing", option A "Aluminum, coated"

The various cable entries are suitable for hazardous and non-hazardous areas.

Cable entry/cable gland	Material	
Gland M20 × 1.5	Non-Ex: plastic	
dianu WZO ^ 1.5	Z2, D2, Ex d/de: brass with plastic	
Adapter for cable entry with internal thread G ½"	Nickel-plated brass	
Adapter for cable entry with internal thread NPT ½"		

Order code for "Housing", option B "Stainless, hygienic"

The various cable entries are suitable for hazardous and non-hazardous areas.

Cable entry/cable gland	Material
Cable gland M20 × 1.5	Plastic
Adapter for cable entry with internal thread G ½"	Nickel-plated brass
Adapter for cable entry with internal thread NPT ½"	

# Device plug

Electrical connection	Material
Plug M12x1	<ul> <li>Socket: Stainless steel, 1.4404 (316L)</li> <li>Contact housing: Polyamide</li> <li>Contacts: Gold-plated brass</li> </ul>

#### Sensor housing

- Acid and alkali-resistant outer surface
- Stainless steel 1.4301 (304)

#### Measuring tubes

Stainless steel, 1.4539 (904L); manifold: stainless steel, 1.4404 (316L)

#### **Process connections**

- Flanges similar to EN 1092-1 (DIN2501) / similar to ASME B 16.5 / as per JIS B2220: Stainless steel, 1.4404 (F316/F316L)
- All other process connections:
   Stainless steel, 1.4404 (316/316L)
- Available process connections  $\rightarrow \triangleq 91$

#### Seals

Welded process connections without internal seals

#### Accessories

Protective cover

Stainless steel, 1.4404 (316L)

#### External WLAN antenna


- Antenna: ASA plastic (acrylonitrile styrene acrylate) and nickel-plated brass
- Adapter: Stainless steel and nickel-plated brass
- Cable: Polyethylene
- Plug: Nickel-plated brass
- Angle bracket: Stainless steel

# **Process connections**

- Fixed flange connections:
  - EN 1092-1 (DIN 2501) flange
  - EN 1092-1 (DIN 2512N) flange
  - NAMUR lengths in accordance with NE 132
  - ASME B16.5 flange
  - JIS B2220 flange
  - DIN 11864-2 Form A flange, DIN 11866 series A, flange with notch
- Clamp connections:

Tri-Clamp (OD tubes), DIN 11866 series C

- Thread:
  - DIN 11851 thread, DIN 11866 series A
  - SMS 1145 thread
  - ISO 2853 thread, ISO 2037
  - DIN 11864-1 Form A thread, DIN 11866 series A
- VCO connections:
  - 8-VCO-4
  - 12-VCO-4



#### Surface roughness

All data relate to parts in contact with medium.

The following surface roughness categories can be ordered:

Category	Method	Option(s)/Order code "Measuring tube mat., wetted surface"
Not polished	-	SA
Ra ≤ 0.76 μm (30 μin) <sup>1)</sup>	Mechanically polished <sup>2)</sup>	SB

Category	Method	Option(s)/Order code "Measuring tube mat., wetted surface"
Ra $\leq$ 0.76 µm (30 µin) 1)	Mechanically polished <sup>2)</sup> , welds in as-welded condition	SJ
Ra $\leq$ 0.38 $\mu$ m (15 $\mu$ in) <sup>1)</sup>	Mechanically polished <sup>2)</sup>	SC
Ra ≤ 0.38 μm (15 μin) <sup>1)</sup>	Mechanically polished <sup>2)</sup> , welds in as-welded condition	SK

- 1) 2)
- Ra according to ISO 21920 Inaccessible weld seams between pipe and manifold are excluded  $\,$

# Operability

#### Operation concept

#### Operator-oriented menu structure for user-specific tasks

- Commissioning
- Operation
- Diagnosis
- Expert level

#### Quick and safe commissioning

- Guided menus ("Make-it-run" wizards) for applications
- Menu quidance with brief descriptions of the individual parameter functions
- Access to the device via web server
- WLAN access to the device via mobile handheld terminal, tablet or smart phone

#### Reliable operation

- Operation in local language
- Uniform operating philosophy applied to device and operating tools
- If replacing electronic modules, transfer the device configuration via the integrated memory (HistoROM backup) which contains the process and measuring device data and the event logbook. No need to reconfigure.

#### Efficient diagnostics increase measurement reliability

- Troubleshooting measures can be called up via the device and in the operating tools
- Diverse simulation options, logbook for events that occur and optional line recorder functions

#### Languages

Can be operated in the following languages:

- Via local operation
   English, German, French, Spanish, Italian, Dutch, Portuguese, Polish, Russian, Turkish, Chinese,
   Japanese, Korean, Vietnamese, Czech, Swedish
- Via web browser
   English, German, French, Spanish, Italian, Dutch, Portuguese, Polish, Russian, Turkish, Chinese,
   Japanese, Vietnamese, Czech, Swedish
- Via "FieldCare", "DeviceCare" operating tool: English, German, French, Spanish, Italian, Chinese, Japanese

# Local operation

# Via display module


Equipment level:

- Order code for "Display; operation", option F "4-line, illuminated, graphic display; touch control"
- Order code for "Display; operation", option G "4-line, illuminated, graphic display; touch control + W/I A N"



Information about WLAN interface → 

101

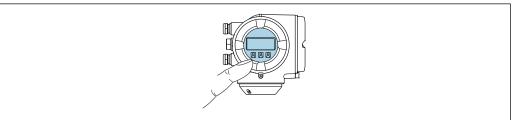

A002678

🖪 38 Operation with touch control

# Display elements

- 4-line, illuminated, graphic display
- White background lighting; switches to red in event of device errors
- Format for displaying measured variables and status variables can be individually configured

# Operating elements


- External operation via touch control (3 optical keys) without opening the housing: ±, □, 国
- Operating elements also accessible in the various zones of the hazardous area

### Via remote display and operating module DKX001



The remote display and operating module DKX001 is available as an optional extra  $\rightarrow \cong 112..$ 

- The remote display and operating module DKX001 is only available for the following housing version: order code for "Housing": option A "Aluminum, coated"
- The measuring instrument is always supplied with a dummy cover when the remote display and operating module DKX001 is ordered directly with the measuring instrument. Display or operation at the transmitter is not possible in this case.
- If ordered subsequently, the remote display and operating module DKX001 may not be connected at the same time as the existing measuring instrument display module. Only one display or operation unit may be connected to the transmitter at any one time.

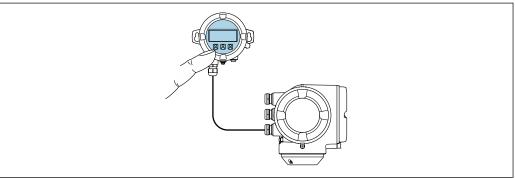

■ 39 Operation via remote display and operating module DKX001

A0026786

### Display and operating elements

#### Housing material

The housing material of the display and operating module DKX001 depends on the choice of transmitter housing material.

Transmitter housing		Remote display and operating module	
Order code for "Housing"	Material	Material	
Option <b>A</b> "Aluminum, coated"	AlSi10Mg, coated	AlSi10Mg, coated	

### Cable entry

Corresponds to the choice of transmitter housing, order code for "Electrical connection".

#### Connecting cable

→ 🖺 50


#### Dimensions

→ 🗎 79

#### Remote operation


# Via HART protocol

This communication interface is available in device versions with a HART output.

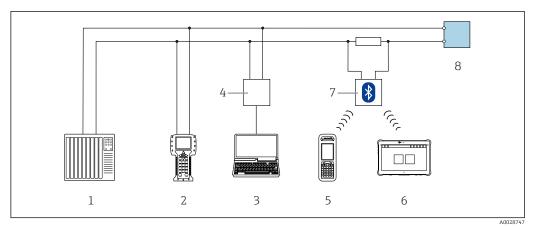

■ 40 Options for remote operation via HART protocol (active)

- 1 Automation system (e.g. PLC)
- 2 Field Communicator 475
- 3 Computer with web browser for accessing the integrated device web server or computer with operating tool (e.g. FieldCare, DeviceCare, AMS Device Manager, SIMATIC PDM) with COM DTM "CDI Communication TCP/IP"
- 4 Commubox FXA195 (USB)
- 5 Field Xpert SFX350 or SFX370
- 6 Field Xpert SMT70
- 7 VIATOR Bluetooth modem with connection cable
- 8 Transmitter

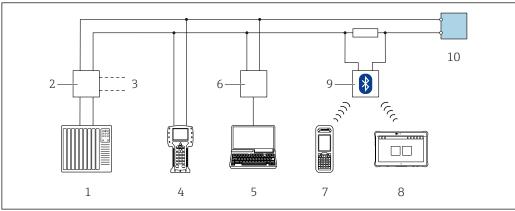


A0028746

■ 41 Options for remote operation via HART protocol (passive)

- 1 Automation system (e.g. PLC)
- 2 Transmitter power supply unit, e.g. RN221N (with communication resistor)
- 3 Connection for Commubox FXA195 and Field Communicator 475
- 4 Field Communicator 475
- 5 Computer with web browser for accessing the integrated device web server or computer with operating tool (e.g. FieldCare, DeviceCare, AMS Device Manager, SIMATIC PDM) with COM DTM "CDI Communication TCP/IP"
- 6 Commubox FXA195 (USB)
- 7 Field Xpert SFX350 or SFX370
- 8 Field Xpert SMT70
- 9 VIATOR Bluetooth modem with connection cable
- 10 Transmitter

#### Via FOUNDATION Fieldbus network

This communication interface is available in device versions with FOUNDATION Fieldbus.

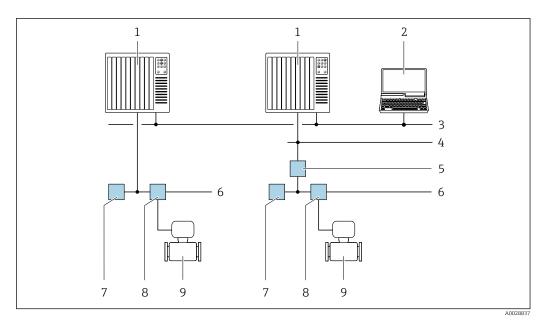


 42 Options for remote operation via FOUNDATION Fieldbus network

- 1 Automation system
- 2 Computer with FOUNDATION Fieldbus network card
- Industry network 3
- 4 High Speed Ethernet FF-HSE network
- Segment coupler FF-HSE/FF-H1 5
- 6 FOUNDATION Fieldbus FF-H1 network
- 7 Power supply FF-H1 network
- 8 T-box
- Measuring instrument

#### Via PROFIBUS DP network

This communication interface is available in device versions with PROFIBUS DP.

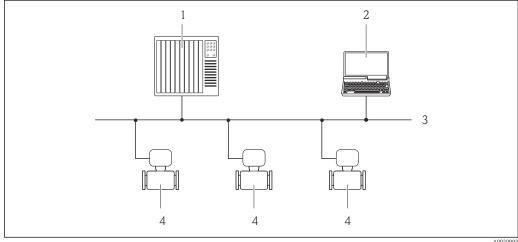


€ 43  ${\it Options for remote operation via PROFIBUS DP\ network}$ 

- Automation system
- Computer with PROFIBUS network card 2
- PROFIBUS DP network 3
- Measuring instrument

# Via PROFIBUS PA network

This communication interface is available in device versions with PROFIBUS PA.

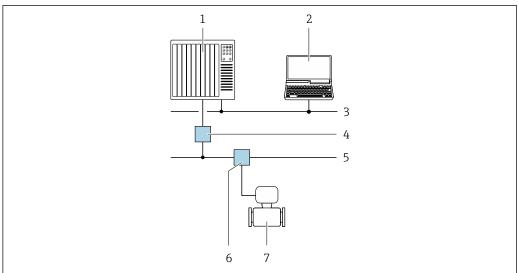


€ 44 Options for remote operation via PROFIBUS PA network

- Automation system
- Computer with PROFIBUS network card 2
- PROFIBUS DP network
- 4 Segment coupler PROFIBUS DP/PA
- 5 PROFIBUS PA network
- 6 T-box
- Measuring instrument

### Via Modbus RS485 protocol

This communication interface is available in device versions with a Modbus RS485 output.

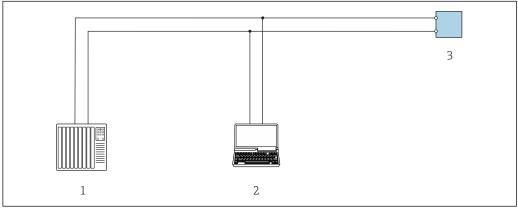


€ 45 Options for remote operation via Modbus RS485 protocol (active)

- Automation system (e.g. PLC)
- Computer with web browser for accessing the integrated device web server or with operating tool (e.g. FieldCare, DeviceCare) with COM DTM "CDI Communication TCP/IP" or Modbus DTM
- Transmitter

# Via Modbus TCP over Ethernet-APL 10 Mbit/s, SPE 10 Mbit/s

This communication interface is available on port 1 in device versions with a Modbus TCP over Ethernet-APL output.

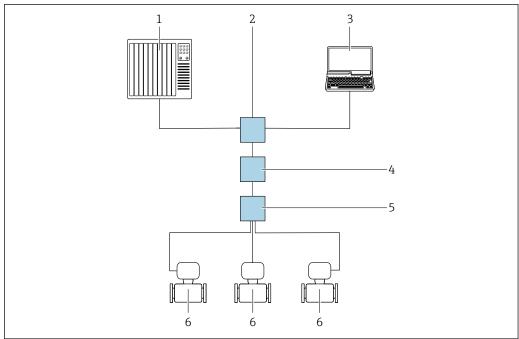


€ 46 Options for remote operation via Modbus TCP over Ethernet-APL protocol (active)

- 1 Automation system, e.g. Simatic S7 (Siemens)
- 2 Ethernet switch, e.g. Scalance X204 (Siemens)
- Computer with web browser or operating tool 3
- 4 APL power switch/SPE power switch (optional)
- APL field switch/SPE field switch 5
- Measuring instrument/communication via port 1 (terminal 26 + 27)

#### Via Modbus TCP over Ethernet 100 Mbit/s

This communication interface is available on port 2 in device versions with a Modbus TCP over Ethernet-APL output.

Star topology

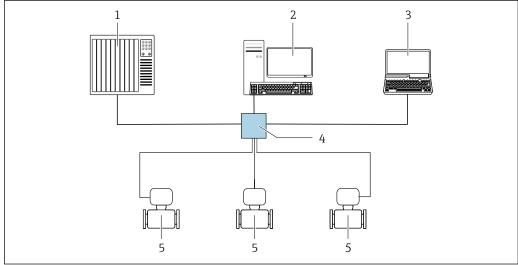

**₽** 47 Options for remote operation via Modbus TCP over Ethernet - 100 Mbit/s: Star topology


- Automation system, z. B. RSLoqix (Rockwell Automation) 1
- Workstation for measuring instrument operation: with Custom Add-On Profile for "RSLogix 5000" (Rockwell 2 Automation) or with Electronic Data Sheet (EDS)
- 3 Computer with web browser or operating tool
- Standard Ethernet switch, e.g. Stratix (Rockwell Automation) 4
- *Measuring instrument/communication via port 2 (RJ45 connector)*

98

#### Via EtherNet/IP network

This communication interface is available in device versions with EtherNet/IP.

#### Star topology

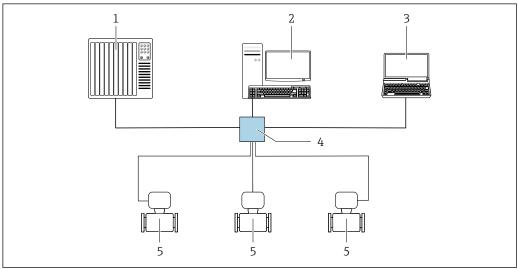


€ 48 Options for remote operation via Ethernet/IP network: star topology

- Automation system, z. B. "RSLogix" (Rockwell Automation)
- Workstation for measuring instrument operation: with Custom Add-On Profile for "RSLogix 5000" (Rockwell 2 Automation) or with Electronic Data Sheet (EDS)
- Computer with web browser for accessing the integrated web server or computer with operating tool (e.g. FieldCare, DeviceCare) with COM DTM "CDI Communication TCP/IP"
- Standard Ethernet switch, e.g. Scalance X204 (Siemens)
- Measuring instrument

# Ring topology

The device is integrated via the terminal connection for signal transmission (output 1) and the service interface (CDI-RJ45).

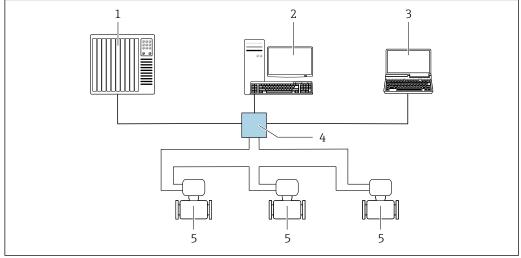

A0033725


Options for remote operation via EtherNet/IP network: ring topology

- Automation system, z.B. "RSLogix" (Rockwell Automation)
- Workstation for measuring instrument operation: with Custom Add-On Profile for RSLogix 5000 (Rockwell Automation) or with Electronic Data Sheet (EDS)
- Computer with web browser for accessing the integrated web server or computer with operating tool (e.g. FieldCare, DeviceCare) with COM DTM "CDI Communication TCP/IP"
- Standard Ethernet switch, e.g. Scalance X204 (Siemens)
- 5 Measuring instrument

#### Via PROFINET network

This communication interface is available in device versions with PROFINET.

# Star topology

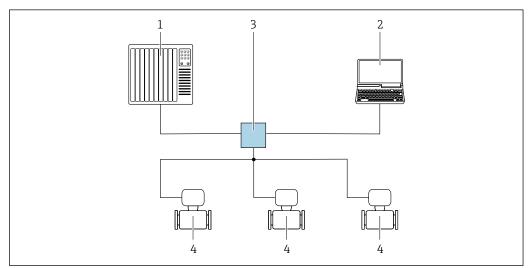


A00265

■ 50 Options for remote operation via PROFINET network: star topology

- 1 Automation system, e.g. Simatic S7 (Siemens)
- 2 Computer with web browser for accessing integrated web server or computer with operating tool (e.g. FieldCare, DeviceCare, SIMATIC PDM) with COM DTM "CDI Communication TCP/IP"
- 3 Standard Ethernet switch, e.g. Scalance X204 (Siemens)
- 4 Measuring instrument

# Ring topology

The device is integrated via the terminal connection for signal transmission (output 1) and the service interface (CDI-RJ45).

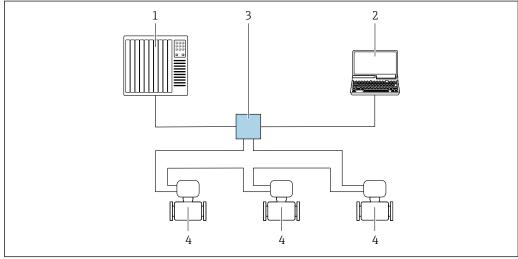

A00337

 $\blacksquare$  51 Options for remote operation via PROFINET network: ring topology

- 1 Automation system, e.g., Simatic S7 (Siemens)
- 2 Computer with web browser for accessing integrated web server or computer with operating tool (e.g. FieldCare, DeviceCare, SIMATIC PDM) with COM DTM "CDI Communication TCP/IP"
- 3 Standard Ethernet switch, e.g. Scalance X204 (Siemens)
- 4 Measuring instrument

#### Service interface

#### Via service interface (CDI-RJ45)


To configure the device on site, a point-to-point connection can be established. Alternatively, a connection via Modbus TCP can be used. The connection is made with the housing open, directly via the device's service interface (CDI-RJ45).



An adapter for the RJ45 to the M12 connector is optionally available for the non-hazardous

Order code for "Accessories", option NB: "Adapter RJ45 M12 (service interface)"

The adapter connects the service interface (CDI-RJ45) to an M12 connector mounted in the cable entry. The connection to the service interface can be established via an M12 connector without opening the device.

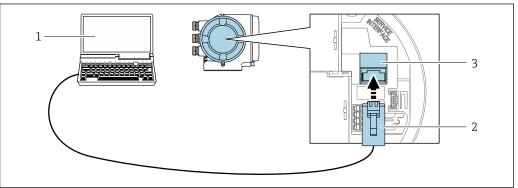


**■** 52 Connection via service interface (CDI-RJ45)

- Computer with web browser for accessing the integrated web server or computer with operating tool, e.g. "FieldCare", "DeviceCare", with COM DTM "CDI Communication TCP/IP" or Modbus DTM or operating tool
- Standard Ethernet connecting cable with RJ45 connector
- Service interface (CDI-RJ45) of the measuring instrument with access to the integrated web server

#### Via WLAN interface

The optional WLAN interface is available on the following device version: Order code for "Display; operation", option G "4-line, illuminated; touch control + WLAN"

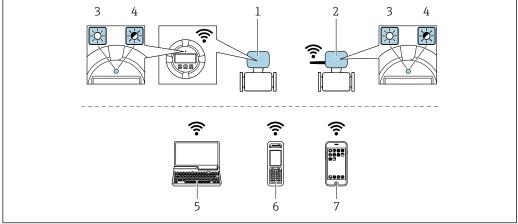

A0034570

- Transmitter with integrated WLAN antenna
- Transmitter with external WLAN antenna
- 3 LED lit constantly: WLAN reception is enabled on measuring instrument
- LED flashing: WLAN connection established between operating unit and measuring instrument
- Computer with WLAN interface and web browser for accessing integrated device web server or with operating tool e.g FieldCare, DeviceCare)
- Mobile handheld terminal with WLAN interface and web browser for accessing integrated device web server or operating tool (e.g. FieldCare, DeviceCare)
- Smartphone or tablet (e.g. Field Xpert SMT70)


Function	WLAN: IEEE 802.11 b/g (2.4 GHz)  • Access point with DHCP server (factory setting)  • Network
Encryption	WPA2-PSK AES-128 (in accordance with IEEE 802.11i)
Configurable WLAN channels	1 to 11
Degree of protection	IP66/67
Available antennas	<ul> <li>Internal antenna</li> <li>External antenna (optional)         In the event of poor transmission/reception conditions at the place of installation.         Available as an accessory .     </li> <li>Only 1 antenna is active at any one time!</li> </ul>
Range	<ul> <li>Internal antenna: typically 10 m (32 ft)</li> <li>External antenna: typically 50 m (164 ft)</li> </ul>
Materials (external antenna)	<ul> <li>Antenna: ASA plastic (acrylonitrile styrene acrylate) and nickel-plated brass</li> <li>Adapter: Stainless steel and nickel-plated brass</li> <li>Cable: Polyethylene</li> <li>Plug: Nickel-plated brass</li> <li>Angle bracket: Stainless steel</li> </ul>

### **Network integration**




Network integration is only available for the HART communication protocol.

With the optional "OPC UA Server" application package, the device can be integrated into an Ethernet network via the service interface (CDI-RJ45 and WLAN) and communicate with OPC UA clients. If the device is used in this way, IT security must be considered.



For permanent access to device data and for device configuration via the web server, the device is incorporated directly in a network via the service interface (CDI-RJ45). In this way, the device can be accessed any time from the control station. The measured values are processed separately via the inputs and outputs through the automation system.

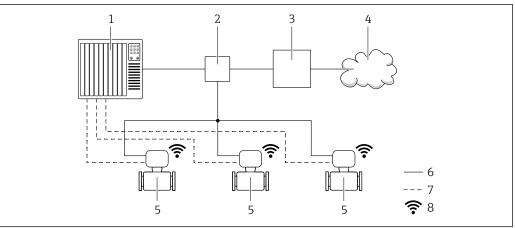

A00336

- 1 Automation system, e.g. Simatic S7 (Siemens)
- 2 Ethernet switch
- 3 Edge Gateway
- 4 Cloud
- 5 Measuring instrument
- 6 Ethernet network
- 7 Measured values via inputs and outputs
- 8 Optional WLAN interface
- The optional WLAN interface is available on the following device version:

  Order code for "Display; operation", option **G** "4-line, backlit, graphic display; touch control + WLAN"
- Special Documentation for the OPC UA Server application package  $\rightarrow \, \stackrel{ riangle}{ riangle} \, 117$ .

# Supported operating tools

Different operating tools can be used for local or remote access to the measuring device. Depending on the operating tool used, access is possible with different operating units and via a variety of interfaces.

Supported operating tools	Operating unit	Interface	Additional information
Web browser	Notebook, PC or tablet with web browser	<ul> <li>Service interface CDI-RJ45</li> <li>WLAN interface</li> <li>Ethernet-based fieldbus (EtherNet/IP, PROFINET, Modbus TCP over Ethernet-APL)</li> </ul>	Special Documentation for device → 🖺 117
DeviceCare SFE100	Notebook, PC or tablet with Microsoft Windows system	<ul> <li>Service interface CDI-RJ45</li> <li>WLAN interface</li> <li>Fieldbus protocol</li> <li>Modbus TCP over Ethernet-APL</li> </ul>	→ 🖺 114

Supported operating tools	Operating unit	Interface	Additional information
FieldCare SFE500	Notebook, PC or tablet with Microsoft Windows system	<ul> <li>Service interface CDI- RJ45</li> <li>WLAN interface</li> <li>Fieldbus protocol</li> </ul>	→ 🖺 114
Field Xpert	SMT70/77/50	<ul> <li>All fieldbus protocols</li> <li>WLAN interface</li> <li>Bluetooth</li> <li>Service interface CDI-RJ45</li> </ul>	Operating Instructions BA01202S Device description files: Use update function of handheld terminal

- Other operating tools based on FDT technology with a device driver such as DTM/iDTM or DD/EDD can be used for device operation. These operating tools are available from the individual manufacturers. Integration into the following operating tools, among others, is supported:
  - FactoryTalk AssetCentre (FTAC) from Rockwell Automation → www.rockwellautomation.com
  - Process Device Manager (PDM) from Siemens → www.siemens.com
  - Asset Management Solutions (AMS) from Emerson → www.emersonprocess.com
  - FieldCommunicator 375/475 from Emerson → www.emersonprocess.com
  - Emersons TREX → www.emerson.com
  - Field Device Manager (FDM) from Honeywell → www.process.honeywell.com
  - FieldMate from Yokogawa → www.yokogawa.com
  - PACTWare → www.pactware.com

The related device description files are available: www.endress.com → Download Area

#### Web server

The integrated web server can be used to operate and configure the device via a web browser via Ethernet-APL, via service interface (CDI-RJ45) or via WLAN interface. The structure of the operating menu is the same as for the local display. In addition to the measured values, status information on the device is displayed and can be used to monitor device health. Furthermore the device data can be managed and the network parameters can be configured.

A device that has a WLAN interface (can be ordered as an option) is required for the WLAN connection: order code for "Display; Operation", option G "4-line, illuminated; touch control + WLAN". The device acts as an Access Point and enables communication by computer or a mobile handheld terminal.

#### Supported functions

Data exchange between the operating unit (such as a notebook, for example,) and measuring instrument:

- Upload the configuration from the measuring instrument (XML format, configuration backup)
- Save the configuration to the measuring instrument (XML format, restore configuration)
- Export event list (.csv file)
- Export parameter settings (.csv file or PDF file, document the measuring point configuration)
- Export the Heartbeat Technology verification report (PDF file, only available with the Heartbeat Verification → \( \begin{align\*} \equiv \text{110} \) application package)
- Flash firmware version for device firmware upgrade, for example
- Download driver for system integration
- Visualize up to 1000 saved measured values (only available with the Extended HistoROM application package → 

  110)

# HistoROM data management

The measuring instrument features HistoROM data management. HistoROM data management comprises both the storage and import/export of key device and process data, making operation and servicing far more reliable, secure and efficient.

When the device is delivered, the factory settings of the configuration data are stored as a backup in the device memory. This memory can be overwritten with an updated data record, for example after commissioning.

104

### Additional information on the data storage concept

There are different types of data storage units in which device data are stored and used by the device:

	HistoROM backup	T-DAT	S-DAT
Available data	<ul> <li>Event logbook, e.g. diagnostic events</li> <li>Parameter data record backup</li> <li>Device firmware package</li> <li>Driver for system integration for exporting via web server, e.g.:</li> <li>GSD for PROFIBUS DP</li> <li>GSD for PROFIBUS PA</li> <li>GSD for PROFINET</li> <li>EDS for EtherNet/IP</li> <li>DD for FOUNDATION Fieldbus</li> </ul>	Measured value logging ("Extended HistoROM" order option)     Current parameter data record (used by firmware at run time)     Indicator (minimum/maximum values)     Totalizer value	<ul> <li>Sensor data: e.g. nominal diameter</li> <li>Serial number</li> <li>Calibration data</li> <li>Device configuration (e.g. SW options, fixed I/O or multi I/O)</li> </ul>
Storage location	Fixed on the user interface PC board in the connection compartment	Can be plugged into the user interface PC board in the connection compartment	In the sensor plug in the transmitter neck part

#### Data backup

#### **Automatic**

- The most important device data (sensor and transmitter) are automatically saved in the DAT modules
- If the transmitter or measuring device is replaced: once the T-DAT containing the previous device data has been exchanged, the new measuring device is ready for operation again immediately without any errors
- If exchanging the electronics module (e.g. I/O electronics module): Once the electronics module has been replaced, the software of the module is compared against the current device firmware. The module software is upgraded or downgraded where necessary. The electronics module is available for use immediately afterwards and no compatibility problems occur.

#### Manual

Additional parameter data record (complete parameter settings) in the integrated device memory HistoROM backup for:

- Data backup function
  - Backup and subsequent restoration of a device configuration in the device memory HistoROM backup
- Data comparison function
  - $\label{thm:comparison} Comparison of the current device configuration with the device configuration saved in the device memory HistoROM backup$

#### Data transmission

#### Manual

- Transfer of a device configuration to another device using the export function of the specific operating tool, e.g. with FieldCare, DeviceCare or web server: to duplicate the configuration or to store in an archive (e.g. for backup purposes)
- Transmission of the drivers for system integration via web server, e.q.:
  - GSD for PROFIBUS DP
  - GSD for PROFIBUS PA
  - GSD for PROFINET
  - EDS for Ethernet/IP
  - DD for FOUNDATION fieldbus

#### **Event list**

#### **Automatic**

- Chronological display of up to 20 event messages in the events list
- If the Extended HistoROM application package (order option) is enabled: up to 100 event messages are displayed in the events list along with a time stamp, plain text description and remedial measures
- The events list can be exported and displayed via a variety of interfaces and operating tools e.g. DeviceCare, FieldCare or Web server

# Data logging

#### Manual

If the **Extended HistoROM** application package (order option) is enabled:

- Recording of 1 to 4 channels of up to 1000 measured values (up to 250 measured values per channel)
- User configurable recording interval
- Export the measured value log via a variety of interfaces and operating tools e.g. FieldCare, DeviceCare or web server

# Certificates and approvals

Current certificates and approvals for the product are available at <a href="https://www.endress.com">www.endress.com</a> on the relevant product page:

- 1. Select the product using the filters and search field.
- 2. Open the product page.
- 3. Select **Downloads**.

#### **CE** mark

The device meets the legal requirements of the applicable EU Directives. These are listed in the corresponding EU Declaration of Conformity along with the standards applied.

Endress+Hauser confirms successful testing of the device by affixing to it the CE mark.

#### **UKCA** marking

The device meets the legal requirements of the applicable UK regulations (Statutory Instruments). These are listed in the UKCA Declaration of Conformity along with the designated standards. By selecting the order option for UKCA marking, Endress+Hauser confirms a successful evaluation and testing of the device by affixing the UKCA mark.

Contact address Endress+Hauser UK:

Endress+Hauser Ltd.

Floats Road

Manchester M23 9NF

United Kingdom

www.uk.endress.com

#### RCM marking

The measuring system meets the EMC requirements of the "Australian Communications and Media Authority (ACMA)".

# Ex approval

The measuring device is certified for use in hazardous areas and the relevant safety instructions are provided in the separate "Safety Instructions" (XA) document. Reference is made to this document on the name plate

Devices with the order code for "Approval; transmitter + sensor", option BA, BB, BC or BD have equipment protection level (EPL) Ga/Gb (Zone 0 in the measuring tube).

The separate Ex documentation (XA) containing all the relevant explosion protection data is available from your Endress+Hauser sales center.

#### Hygienic compatibility

- 3-A approval
  - Only measuring instruments with the order code for "Additional approval", option LP "3A" have 3-A approval.
  - The 3-A approval refers to the measuring instrument.
  - When installing the measuring instrument, ensure that no liquid can accumulate on the outside of the measuring instrument.
    - A remote display module must be installed in accordance with the 3-A Standard.
  - Accessories (e.g. heating jacket, weather protection cover, wall holder unit) must be installed in accordance with the 3-A Standard.
    - Each accessory can be cleaned. Disassembly may be necessary under certain circumstances.
- EHEDG-tested (Type EL Class I)

Only devices with the order code for "Additional approval", option LT "EHEDG" have been tested and meet the requirements of the EHEDG.

To meet the requirements for EHEDG certification, the device must be used with process connections in accordance with the EHEDG position paper entitled "Easy cleanable Pipe couplings and Process connections" (www.ehedq.orq).

To meet the requirements for EHEDG certification, the orientation of the device must ensure drainability.

Test criteria for cleanability according to EHEDG is a flow velocity of 1.5~m/s in the process line. This speed must be ensured for EHEDG-compliant cleaning.

- FDA CFR 21
- Food Contact Materials Regulation (EC) 1935/2004
- Food Contact Materials Regulation GB 4806
- The requirements of the Food Contact Material regulations must be observed when selecting the material versions.



Observe special installation instructions

#### Pharmaceutical compatibility

- FDA 21 CFR 177
- USP <87>
- USP <88> Class VI 121 °C
- TSE/BSE Certificate of Suitability
- cGMP

Devices with the order code for "Test, certificate", option JG "Conformity with cGMP-derived requirements, declaration" comply with the requirements of cGMP with regard to the surfaces of parts in contact with the medium, design, FDA 21 CFR material conformity, USP Class VI tests and TSE/BSE conformity.

A serial number-specific declaration is generated.

#### Functional safety

The measuring instrument can be used for flow monitoring systems (min., max., range) up to SIL 2 (single-channel architecture; order code for "Additional approval", option LA) and SIL 3 (multichannel architecture with homogeneous redundancy) and is independently evaluated and certified in accordance with IEC 61508.

The following types of monitoring in safety equipment are possible:

- Mass flow
- Volume flow
- Density



Functional safety manual with information for the SIL device  $\rightarrow \triangleq 116$ 

#### **HART** certification

# HART interface

The measuring device is certified and registered by the FieldComm Group. The measuring system meets all the requirements of the following specifications:

- Certified according to HART 7
- The device can also be operated with certified devices of other manufacturers (interoperability)

# FOUNDATION Fieldbus certification

#### **FOUNDATION Fieldbus interface**

The measuring device is certified and registered by the FieldComm Group. The measuring system meets all the requirements of the following specifications:

- Certified in accordance with FOUNDATION Fieldbus H1
- Interoperability Test Kit (ITK), revision version 6.2.0 (certificate available on request)
- Physical Layer Conformance Test
- The device can also be operated with certified devices of other manufacturers (interoperability)

#### **Certification PROFIBUS**

#### **PROFIBUS** interface

The measuring device is certified and registered by the PNO (PROFIBUS Nutzerorganisation e.V./ PROFIBUS User Organization). The measuring system meets all the requirements of the following specifications:

- Certified according to PA Profile 3.02
- The device can also be operated with certified devices of other manufacturers (interoperability)

#### EtherNet/IP certification

The measuring device is certified and registered by the ODVA (Open Device Vendor Association). The measuring system meets all the requirements of the following specifications:

- Certified in accordance with the ODVA Conformance Test
- EtherNet/IP Performance Test
- EtherNet/IP PlugFest compliance
- The device can also be operated with certified devices of other manufacturers (interoperability)

#### **Certification PROFINET**

#### **PROFINET** interface

The measuring instrument is certified and registered by the PROFIBUS Nutzerorganisation e.V. (PNO). The measuring system meets all the requirements of the following specifications:

- Certified according to:
  - Test specification for PROFINET devices
  - PROFINET Netload Class 2 100 Mbit/s
- The device can also be operated with certified devices of other manufacturers (interoperability).
- The device supports PROFINET S2 system redundancy.

#### PROFINET over Ethernet-APL certification

#### PROFINET interface

The measuring instrument is certified and registered by the PROFIBUS Nutzerorganisation e.V. (PNO). The measuring system meets all the requirements of the following specifications:

- Certified according to:
  - Test specification for PROFINET devices
  - PROFINET PA Profile 4.02
  - PROFINET Netload Robustness Class 2 10 Mbit/s
  - APL conformance test
- The device can also be operated with certified devices of other manufacturers (interoperability)
- The device supports PROFINET S2 system redundancy.

#### Pressure Equipment Directive

The measuring instruments can be ordered with or without PED or PESR. If a device with PED or PESR is required, this must be ordered explicitly. For devices with nominal diameters less than or equal to DN 25 (NPS 1"), this is neither possible nor necessary. A UK order option must be selected for PESR under the order code for "Approvals".

- With the marking
  - a) PED/G1/x (x = category) or
  - b) PESR/G1/x (x = category)

on the sensor nameplate, Endress+Hauser confirms compliance with the "Essential Safety Requirements"

- a) specified in Annex I of the Pressure Equipment Directive 2014/68/EU or
- b) Schedule 2 of Statutory Instruments 2016 No. 1105.
- Devices bearing this marking (PED or PESR) are suitable for the following types of medium:
  - Media in Group 1 and 2 with a vapor pressure greater than, or smaller and equal to 0.5 bar (7.3 psi)
  - Unstable gases
- Devices not bearing this marking (without PED or PESR) are designed and manufactured according to sound engineering practice. They meet the requirements of
- a) Art. 4, Section 3 of the Pressure Equipment Directive 2014/68/EU or
- b) Part 1, Section 8 of Statutory Instruments 2016 No. 1105.

The scope of application is indicated

- a) in diagrams 6 to 9 in Annex II of the Pressure Equipment Directive 2014/68/EU or
- b) in Schedule 3, Section 2 of Statutory Instruments 2016 No. 1105.

### Radio approval

The measuring instrument has radio approval.



For detailed information on the radio approval, see the Special Documentation  $\rightarrow \triangleq 117$ 

#### Additional certification

#### Marine approval

Currently valid certificates are available:

- In the Downloads area of the Endress+Hauser website: www.endress.com → Downloads
- Specify the following details:
  - Product root, e.g. 8E3B
  - Search: Approval & Certificates → Marine

#### CRN approval

Some device versions have CRN approval. A CRN-approved process connection with a CSA approval must be ordered for a CRN-approved device.

### Tests and certificates

- EN10204-3.1 material certificate, wetted parts and sensor housing (order code for "Test, certificate", option JA)
- Pressure test, internal process, test report (order code for "Test, certificate", option JB)
- Surface roughness test ISO4287/Ra, (wetted parts), test report (option JE)
- Compliance with requirements derived from cGMP, Declaration (option JG)

# External standards and guidelines

■ EN 60529

Degrees of protection provided by enclosure (IP code)

■ IEC/EN 60068-2-6

Environmental influences: Test procedure - Test Fc: vibrate (sinusoidal).

■ IEC/EN 60068-2-31

Environmental influences: Test procedure - Test Ec: shocks due to rough handling, primarily for devices.

■ EN 61010-1

Safety requirements for electrical equipment for measurement, control and laboratory use - general requirements

■ GB 30439.5

Safety requirements for industrial automation products - Part 5: Flowmeter safety requirements

■ EN 61326-1/-2-3

EMC requirements for electrical equipment for measurement, control and laboratory use

■ NAMUR NE 21

Electromagnetic compatibility (EMC) of industrial process and laboratory control equipment

■ NAMUR NE 32

Data retention in the event of a power failure in field and control instruments with microprocessors  $% \left( 1\right) =\left( 1\right) \left( 1\right) \left$ 

NAMUR NE 43

Standardization of the signal level for the breakdown information of digital transmitters with analog output signal.

■ NAMUR NE 53

Software of field devices and signal-processing devices with digital electronics

■ NAMUR NE 80

The application of the pressure equipment directive to process control devices

■ NAMUR NE 105

Specifications for integrating fieldbus devices in engineering tools for field devices

■ NAMUR NE 107

Self-monitoring and diagnostics of field devices

■ NAMUR NE 131

Requirements for field devices for standard applications

■ NAMUR NE 132

Coriolis mass meter

■ ETSI EN 300 328

Guidelines for 2.4 GHz radio components.

■ EN 301489

Electromagnetic compatibility and radio spectrum matters (ERM).

# Ordering information

Detailed ordering information is available from your nearest sales organization www.addresses.endress.com or in the Product Configurator at www.endress.com:

- 1. Select the product using the filters and search field.
- 2. Open the product page.
- 3. Select **Configuration**.


## Product Configurator - the tool for individual product configuration

- Up-to-the-minute configuration data
- Depending on the device: direct input of information specific to the measuring point, such as the measuring range or operating language
- Automatic verification of exclusion criteria
- Automatic creation of the order code and its breakdown in PDF or Excel output format
- Ability to order directly in the Endress+Hauser Online Shop

# Application packages

Many different application packages are available to enhance the functionality of the device. Such packages might be needed to address safety aspects or specific application requirements.

The application packages can be ordered with the device or subsequently from Endress+Hauser. Detailed information on the order code in question is available from your local Endress+Hauser sales center or on the product page of the Endress+Hauser website: <a href="https://www.endress.com">www.endress.com</a>.



### Diagnostic functionality

Order code for "Application package", option EA "Extended HistoROM"

Comprises extended functions concerning the event log and the activation of the measured value memory.

Event log:

Memory volume is extended from 20 message entries (standard version) to up to 100 entries.

Data logging (line recorder):

- Memory capacity for up to 1000 measured values is activated.
- 250 measured values can be output via each of the 4 memory channels. The recording interval can
  be defined and configured by the user.
- Measured value logs can be accessed via the local display or operating tool e.g. FieldCare, DeviceCare or Web server.



For detailed information, see the Operating Instructions for the device.

#### **Heartbeat Technology**

Order code for "Application package", option EB "Heartbeat Verification + Monitoring"

#### Heartheat Verification

Meets the requirement for traceable verification in accordance with DIN ISO 9001:2015 Clause 7.6 a) "Control of monitoring and measuring equipment".

- Functional testing in the installed state without interrupting the process.
- Traceable verification results on request, including a report.
- Simple testing process via local operation or other operating interfaces.
- Clear measuring point assessment (pass/fail) with high total test coverage within the framework of manufacturer specifications.
- Extension of calibration intervals according to operator's risk evaluation.

#### **Heartbeat Monitoring**

Continuously supplies data, which are characteristic of the measuring principle, to an external condition monitoring system for the purpose of preventive maintenance or process analysis. These data enable the operator to:

- Draw conclusions using these data and other information about the impact the process influences (e.g. corrosion, abrasion, deposit buildup etc.) have on measuring performance over time.
- Schedule servicing in time.
- Monitor the process or product quality, e.g. gas pockets.



Detailed information on Heartbeat Technology:

#### Concentration measurement

Order code for "Application package", option ED "Concentration"

Calculation and outputting of fluid concentrations.

The measured density is converted to the concentration of a substance of a binary mixture using the "Concentration" application package:

- Choice of predefined fluids (e.g. various sugar solutions, acids, alkalis, salts, ethanol etc.).
- Common or user-defined units ("Brix, "Plato, % mass, % volume, mol/l etc.) for standard applications.
- Concentration calculation from user-defined tables.



For detailed information, see the Special Documentation for the device.

#### Petroleum

Order code for "Application package", option EJ "Petroleum"

The most important parameters for the Oil & Gas Industry can be calculated and displayed with this application package.

- Corrected volume flow and calculated reference density in accordance with the "API Manual of Petroleum Measurement Standards, Chapter 11.1"
- Water content, based on density measurement
- Weighted mean of the density and temperature



For detailed information, see the Special Documentation for the device.

### Petroleum & locking function

Order code for "Application package", option EM "Petroleum & locking function"

The most important parameters for the Oil & Gas Industry can be calculated and displayed with this application package. It is also possible to lock the settings.

- Corrected volume flow and calculated reference density in accordance with the "API Manual of Petroleum Measurement Standards, Chapter 11.1"
- Water content, based on density measurement
- Weighted mean of the density and temperature



For detailed information, see the Special Documentation for the device.

#### **OPC-UA Server**

Order code for "Application package", option EL "OPC-UA Server"

The application package provides an integrated OPC-UA server for comprehensive device services for IoT and SCADA applications.



For detailed information, see the Special Documentation for the device.

# Accessories

Various accessories, which can be ordered with the device or subsequently from Endress+Hauser, are available for the device. Detailed information on the order code in question is available from your local Endress+Hauser sales center or on the product page of the Endress+Hauser website: www.endress.com.

#### Device-specific accessories

#### For the transmitter

Accessory	Description	
Proline 300 transmitter	Transmitter for replacement or storage. Use the order code to define the follow specifications:  Approvals  Output  Input  Display/operation  Housing  Software  Installation Instructions EA01200D	
Remote display and operating module DKX001	<ul> <li>If ordered directly with the measuring instrument:         Order code for "Display; operation", option O "Remote display 4-line, illuminated;         10 m (30 ft) cable; touch control"</li> <li>If ordered separately:         <ul> <li>Measuring instrument: order code for "Display; operation", option M "W/o, prepared for remote display"</li> <li>DKX001: Via the separate product structure DKX001</li> </ul> </li> <li>If ordered subsequently:         <ul> <li>DKX001: Via the separate product structure DKX001</li> </ul> </li> </ul>	
	Mounting bracket for DKX001 ■ If ordered directly: order code for "Accessory enclosed", option RA "Mounting bracket, pipe 1/2" ■ If ordered subsequently: order number: 71340960	
	Connecting cable (replacement cable) Via the separate product structure: DKX002	
	Further information on display and operating module DKX001 $\rightarrow$ $\bigcirc$ 94.	
	Special Documentation SD01763D	

External WLAN antenna	External WLAN antenna with 1.5 m (59.1 in) connecting cable and two angle brackets. Order code for "Accessory enclosed", option P8 "Wireless antenna wide area".				
	<ul> <li>The external WLAN antenna is not suitable for use in hygienic applications.</li> <li>Further information on the WLAN interface →</li></ul>				
	Order number: 71351317				
	Installation Instructions EA01238D				
Protective cover	Is used to protect the measuring instrument from the effects of the weather: e.g. rainwater, excess heating from direct sunlight.				
	Order number: 71343505				
	Installation Instructions EA01160D				

## For the sensor

Accessories	Description
Heating jacket	Is used to stabilize the temperature of the fluids in the sensor. Water, water vapor and other non-corrosive liquids are permitted for use as fluids.
	If using oil as a heating medium, please consult with Endress+Hauser.
	Heating jackets cannot be used with sensors fitted with a rupture disk. Use the order code with the product root DK8003.
	Special Documentation SD02151D

# Communication-specific accessories

Accessories	Description
Commubox FXA195 HART	For intrinsically safe HART communication with FieldCare via the USB interface.  Technical Information TI00404F
HART loop converter HMX50	Is used to evaluate and convert dynamic HART process variables to analog current signals or limit values.  Technical Information TI00429F Operating Instructions BA00371F
Fieldgate FXA42	Transmission of the measured values of connected 4 to 20 mA analog measuring instruments, as well as digital measuring instruments  Technical Information TI01297S Operating Instructions BA01778S Product page: www.endress.com/fxa42
Field Xpert SMT50	The Field Xpert SMT50 tablet PC for device configuration enables mobile plant asset management in non-hazardous areas. It is suitable for commissioning and maintenance staff to manage field instruments with a digital communication interface and to record progress.  This tablet PC is designed as an all-in-one solution with a preinstalled driver library and is an easy-to-use, touch-sensitive tool which can be used to manage field instruments throughout their entire life cycle.
	<ul> <li>Technical Information TI01555S</li> <li>Operating Instructions BA02053S</li> <li>Product page: www.endress.com/smt50</li> </ul>

Field Xpert SMT70	The Field Xpert SMT70 tablet PC for device configuration enables mobile plant asset management in hazardous and non-hazardous areas. It is suitable for commissioning and maintenance staff to manage field instruments with a digital communication interface and to record progress.  This tablet PC is designed as an all-in-one solution with a preinstalled driver library and is an easy-to-use, touch-sensitive tool which can be used to manage field instruments throughout their entire life cycle.
	<ul> <li>Technical Information TI01342S</li> <li>Operating Instructions BA01709S</li> <li>Product page: www.endress.com/smt70</li> </ul>
Field Xpert SMT77	The Field Xpert SMT77 tablet PC for device configuration enables mobile plant asset management in areas categorized as Ex Zone 1.
	<ul> <li>Technical Information TI01418S</li> <li>Operating Instructions BA01923S</li> <li>Product page: www.endress.com/smt77</li> </ul>

# Service-specific accessories

Accessory	Description
Applicator	Software for selecting and sizing Endress+Hauser measuring instruments:  Choice of measuring instruments for industrial requirements  Calculation of all the necessary data for identifying the optimum flowmeter: e.g. nominal diameter, pressure loss, flow velocity and measurement accuracy.  Graphic display of the calculation results  Determining the partial order code. Administration, documentation and access to all project-related data and parameters over the entire life cycle of a project.  Applicator is available: Via the Internet: https://portal.endress.com/webapp/applicator
Netilion	lloT ecosystem: Unlock knowledge
Nethioli	With the Netilion IIoT ecosystem, Endress+Hauser allows you to optimize your plant performance, digitize workflows, share knowledge, and enhance collaboration.  Based on decades of experience in process automation, Endress+Hauser offers the process industry an IIoT ecosystem that enables you to gain useful insights from data. These insights can be used to optimize processes, leading to increased plant availability, efficiency, and reliability - ultimately resulting in a more profitable plant.  www.netilion.endress.com
FieldCare	FDT-based plant asset management tool from Endress+Hauser. It can configure all intelligent field units in your system and helps you manage them. By using the status information, it is also a simple but effective way of checking their status and condition.
	Operating Instructions BA00027S and BA00059S
DeviceCare	Tool to connect and configure Endress+Hauser field devices.
	<ul><li>Technical Information: TI01134S</li><li>Innovation brochure: IN01047S</li></ul>

## System components

Accessories	Description				
Memograph M graphic data manager	The Memograph M graphic data manager provides information on all the relevant measured variables. Measured values are recorded correctly, limit values are monitored and measuring points analyzed. The data are stored in the 256 MB internal memory and also on a SD card or USB stick.				
	<ul> <li>Technical Information TI00133R</li> <li>Operating Instructions BA00247R</li> </ul>				
Cerabar M	The pressure transmitter for measuring the absolute and gauge pressure of gases, steam and liquids. It can be used to read in the operating pressure value.				
	<ul> <li>Technical Information TI00426P and TI00436P</li> <li>Operating Instructions BA00200P and BA00382P</li> </ul>				

Accessories	Description				
Cerabar S	The pressure transmitter for measuring the absolute and gauge pressure of gases, steam and liquids. It can be used to read in the operating pressure value.				
	<ul><li>Technical Information TI00383P</li><li>Operating Instructions BA00271P</li></ul>				
iTEMP	The temperature transmitters can be used in all applications and are suitable for the measurement of gases, steam and liquids. They can be used to read in the medium temperature.				
	"Fields of Activity" document FA00006T				

# **Documentation**



For an overview of the scope of the associated Technical Documentation, refer to the following:

- *Device Viewer* (www.endress.com/deviceviewer): Enter the serial number from the nameplate
- *Endress+Hauser Operations app*: Enter serial number from nameplate or scan matrix code on nameplate.

### Standard documentation



### **Brief Operating Instructions**

Brief Operating Instructions for the sensor

Measuring instrument	Documentation code
Proline Promass E	KA01260D

### *Brief Operating Instructions for the transmitter*

	Documentation code				
Measuring instrument	HART	FOUNDATION Fieldbus	PROFIBUS PA	PROFIBUS DP	Modbus RS485
Proline 300	KA01309D	KA01229D	KA01227D	KA01386D	KA01311D

### Brief Operating Instructions for the transmitter

	Documentation code			
Measuring instrument	EtherNet/IP	PROFINET	PROFINET over Ethernet-APL	Modbus TCP
Proline 300	KA01339D	KA01341D	KA01517D	KA01733D

### **Operating Instructions**

	Documentation code				
Measuring instrument	HART	FOUNDATION Fieldbus	PROFIBUS PA	PROFIBUS DP	Modbus RS485
Promass E 300	BA01484D	BA01517D	BA01506D	BA01855D	BA01495D

	Documentation code			
Measuring instrument	EtherNet/IP	PROFINET	PROFINET over Ethernet- APL	Modbus TCP
Promass E 300	BA01727D	BA01738D	BA02110D	BA02403D

## **Description of Device Parameters**

	Documentation code				
Measuring instrument	HART	FOUNDATION Fieldbus	PROFIBUS PA	PROFIBUS DP	Modbus RS485
Promass 300	GP01057D	GP01094D	GP01058D	GP01134D	GP01059D

	Documentation code			
Measuring instrument	EtherNet/IP	PROFINET	PROFINET over Ethernet- APL	Modbus TCP
Promass 300	GP01114D	GP01115D	GP01168D	GP01235D

Device-dependent additional documentation

Safety instructions

Safety instructions for electrical equipment for hazardous areas.

Contents	Documentation code
ATEX/IECEx Ex d	XA01405D
ATEX/IECEx Ex ec	XA01439D
cCSAus XP	XA01373D
cCSAus Ex d	XA01372D
cCSAus Ex ec	XA01507D
EAC Ex d	XA01656D
EAC Ex ec	XA01657D
JPN Ex d	XA01778D
KCs Ex d	XA03285D
INMETRO Ex d	XA01468D
INMETRO Ex ec	XA01470D
NEPSI Ex d	XA01469D
NEPSI Ex ec	XA01471D
UKEX Ex d	XA02566D
UKEX Ex ec	XA02568D

## Remote display and operating module DKX001

Contents	Documentation code
ATEX/IECEx Ex i	XA01494D
ATEX/IECEx Ex ec	XA01498D
cCSAus IS	XA01499D
cCSAus Ex nA	XA01513D
EAC Ex i	XA01664D
EAC Ex ec	XA01665D
INMETRO Ex i	XA01500D

Contents	Documentation code
INMETRO Ex ec	XA01501D
JPN	XA01781D
KCs Ex i	XA03280D
NEPSI Ex i	XA01502D
NEPSI Ex nA	XA01503D
UKCA Ex i	XA01494D
UKCA Ex ec	XA01498D

# Functional Safety Manual

Contents	Documentation code
Proline Promass 300	SD01727D

# **Special Documentation**

Contents	Documentation code
Information on the Pressure Equipment Directive	SD01614D
Remote display and operating module DKX001	SD01763D
Radio approvals for WLAN interface for A309/A310 display module	SD01793D
OPC UA server 1)	SD02039D
Modbus TCP system integration	SD03408D

1) This Special Documentation is only available for device versions with a HART output.

Contents	Documentation code				
	HART	FOUNDATION Fieldbus	PROFIBUS PA	PROFIBUS DP	Modbus RS485
Web server	SD01662D	SD01665D	SD01664D	SD02226D	SD01663D
Heartbeat Technology	SD01642D	SD01696D	SD01698D	SD02202D	SD01697D
Concentration measurement	SD01644D	SD01706D	SD01708D	SD02212D	SD01707D
Petroleum	SD02097D	-	SD02291D	SD02216D	SD02098D
Petroleum & locking function	SD02499D	-	-	-	SD02500D
Gas fraction handler	SD02584D	_	-	_	SD02584D

Contents	Documentation code			
	PROFINET	EtherNet/IP	PROFINET over Ethernet- APL	Modbus TCP
Web server	SD01969D	SD01968D	SD02762D	-
Heartbeat Technology	SD01988D	SD01982	SD02731D	SD03350D
Concentration measurement	SD02005D	SD02004D	SD02735D	SD03354D
Petroleum	SD02099D	SD02096D	SD02739D	SD03358D

Contents	Documentation code			
	PROFINET	EtherNet/IP	PROFINET over Ethernet- APL	Modbus TCP
Petroleum & locking function	-	-	SD02739D	-
Gas fraction handler	SD02584D	-	SD02584D	SD02584D

### **Installation Instructions**

Contents	Note
	The corresponding documentation code is listed with the relevant accessory. $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $

# Registered trademarks

#### $HART^{@}$

Registered trademark of the FieldComm Group, Austin, Texas USA

#### **PROFIBUS®**

Registered trademark of the PROFIBUS Nutzerorganisation e.V. (PROFIBUS User Organization), Karlsruhe, Germany

### FOUNDATION™ fieldbus

Registration-pending trademark of the FieldComm Group, Austin, Texas, USA

#### $Modbus^{\otimes}$

Registered trademark of SCHNEIDER AUTOMATION, INC.

# Ethernet/IP™

Trademark of ODVA, Inc.

### $\textbf{Ethernet-APL}^{\intercal M}$

Registered trademark of the PROFIBUS Nutzerorganisation e.V. (PROFIBUS User Organization), Karlsruhe, Germany

### **PROFINET®**

### TRI-CLAMP®

Registered trademark of Ladish & Co., Inc., Kenosha, USA





www.addresses.endress.com