

Technical Information

Cubemass

Coriolis mass flow measuring system



Applications

The Coriolis measuring principle operates independently of physical fluid properties.

- Fluid temperatures up to +200 °C (+392 °F)
- Process pressures up to 400 bar (5800 psi)
- Mass flow measurement up to 1000 kg/h (36.75 lb/min)

Approvals for hazardous area:

- ATEX, NEC/CEC, NEPSI

Connection to commonly used process control systems:

- MODBUS RS485

Your benefits

The Cubemass make it possible to simultaneously record several process variables (mass/density/temperature) for various process conditions during measuring operation.

The **transmitter concept** includes:

- FieldCare for diagnosis
- Very low power consumption

Table of contents

Function and system design	3	Mechanical construction	15
Measuring principle	3	Design/dimensions	15
Measuring system	4	Weight	21
Input	5	Material	22
Measured variable	5	Material load diagram	22
Measuring range	5	Process connections	23
Operable flow range	5	Human interface	24
Output	5	Display elements	24
Output signal	5	Remote operation	24
Signal on alarm	5	Certificates and approvals	24
Load	5	CE mark	24
Galvanic isolation	5	C-Tick symbol	24
Power supply	6	Ex approval	24
Electrical connection Measuring unit	6	Pressure Equipment Directive	24
Electrical connection, terminal assignment	6	Functional safety	24
Supply voltage	6	Other standards and guidelines	24
Cable entries	6	Ordering information	25
Cable specifications	6	Accessories	25
Power consumption	7	Documentation	25
Power supply failure	7	Registered trademarks	25
Potential equalization	7		
Performance characteristics	8		
Reference operating conditions	8		
Maximum measured error	8		
Repeatability	9		
Influence of medium temperature	9		
Influence of medium pressure	9		
Basis for calculations	9		
Operating conditions: Installation	10		
Installation instructions	10		
Inlet and outlet runs	11		
System pressure	11		
Operating conditions: Environment	12		
Ambient temperature range	12		
Storage temperature	12		
Degree of protection	12		
Shock resistance	12		
Vibration resistance	12		
CIP cleaning	12		
SIP cleaning	12		
Electromagnetic compatibility (EMC)	12		
Operating conditions: Process	13		
Medium temperature range	13		
Fluid pressure range (nominal pressure)	13		
Rupture element/disk (optional)	13		
Limiting flow	13		
Pressure loss (SI units)	13		
Pressure loss (US units)	14		

Function and system design

Measuring principle

The measuring principle is based on the controlled generation of Coriolis forces. These forces are always present when both translational and rotational movements are superimposed.

$$F_C = 2 \cdot \Delta m (v \cdot \omega)$$

F_C = Coriolis force

Δm = moving mass


ω = rotational velocity

v = radial velocity in rotating or oscillating system

The amplitude of the Coriolis force depends on the moving mass Δm , its velocity v in the system, and thus on the mass flow. Instead of a constant angular velocity ω , oscillation occurs.

This causes the measuring tube loop through which the fluid is flowing to oscillate. The Coriolis forces produced at the measuring tube loop cause a phase shift in the oscillations of the tube loop (see illustration):

- If there is zero flow, i.e. when the fluid stands still, the oscillation measured at points A and B has the same phase, and thus there is no phase difference (1).
- Mass flow causes deceleration of the oscillation at the inlet of the tube loop (2) and acceleration at the outlet (3).

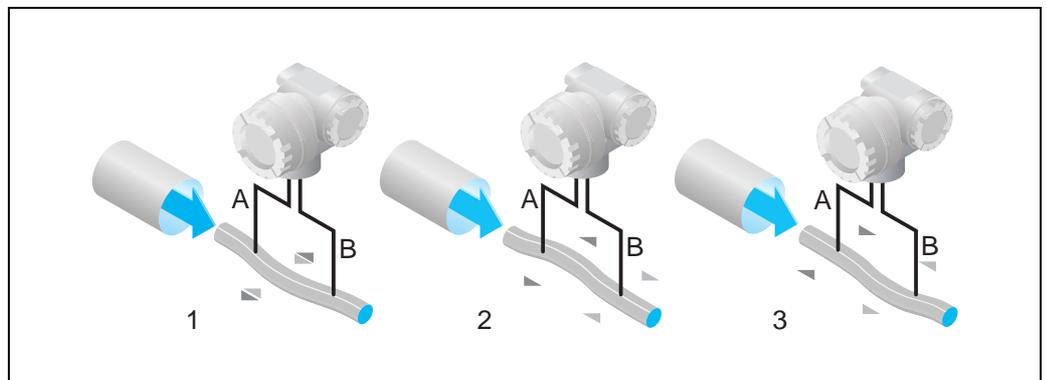

A0013128

The phase difference (A-B) increases with increasing mass flow. Electrodynamical sensors register the tube loop oscillations at the inlet and outlet.

Compared to two-tube systems, other design solutions are required in single-tube systems to ensure system balance. In the case of the Cubemass, an internal reference mass is provided for this purpose.

The measuring principle operates independently of temperature, pressure, viscosity, conductivity and flow profile.

Density measurement

The measuring tube is continuously excited at its resonance frequency. A change in the mass and thus the density of the oscillating system (comprising the measuring tube loop and fluid) results in a corresponding, automatic adjustment in the oscillation frequency. Resonance frequency is thus a function of fluid density. The microprocessor utilizes this relationship to obtain a density signal.

Temperature measurement


The temperature of the measuring tube loop is determined in order to calculate the compensation factor due to temperature effects.

This signal corresponds to the process temperature and is also available as an output.


Measuring system

The measuring system consists of a transmitter and a sensor, which form a mechanical unit.

Transmitter

 <p>A0013123</p>	<ul style="list-style-type: none">■ Configuration via MODBUS RS485, FieldCare■ Mass flow, volume flow, density and temperature measurement as well as calculated variables (e.g. fluid concentrations)
---	---

Sensor

 <p>A0011878</p>	<ul style="list-style-type: none">■ Universal sensor for fluid temperatures up to 200 °C.■ Nominal diameters DN 1 to 6■ Tube material: stainless steel
---	--

Input

Measured variable	<ul style="list-style-type: none"> ■ Mass flow (proportional to the phase difference between two sensors mounted on the measuring tube to register a phase shift in the oscillation) ■ Volume flow (calculated using mass flow and density) ■ Fluid density (proportional to the resonance frequency of the measuring tube) ■ Fluid temperature (measured with temperature sensors)
--------------------------	---

Measuring range

Measuring ranges for liquids

DN		Range for full scale values (liquids) $\dot{m}_{\min(F)}$ to $\dot{m}_{\max(F)}$	
[mm]	[inch]	[kg/h]	[lb/min]
1	1/24"	0 to 20	0 to 0.75
2	1/12"	0 to 100	0 to 3.7
4	1/8"	0 to 450	0 to 16.5
6	1/4"	0 to 1000	0 to 37

Operable flow range	1:100
----------------------------	-------

Output

Output signal

Pulse/frequency output

- passive
- galvanically isolated
- Open Collector
- max. 30 V DC
- max. 25 mA
- Frequency output: end frequency 100 to 5000 Hz, on/off ratio 1:1, pulse width max. 2 s
- Pulse output: pulse value and pulse polarity selectable, pulse width configurable (0.1 to 1000 ms)

Status output

- passive
- Open Collector
- max. 30 V DC
- max. 25 mA

MODBUS RS485

- MODBUS device type: slave
- Address range: 1 to 247
- Functions codes supported: 03, 04, 06, 08, 16, 23
- Broadcast: supported with the function codes 06, 16, 23
- Physical interface: RS485 in accordance with standard EIA/TIA-485
- Baudrate supported: 1200, 2400, 4800, 9600, 19200, 38400, 57600, 115200 Baud
- Transmission mode: RTU or ASCII
- Response time: typically 5 ms

Signal on alarm

Pulse/frequency output

De-energized in the event of fault or power supply failure

Status output

De-energized in the event of fault or power supply failure

MODBUS RS485

De-energized in the event of fault or power supply failure

Load


→ "Output signal"

Galvanic isolation

All circuits for outputs, and power supply are galvanically isolated from each other.

Power supply

Electrical connection Measuring unit

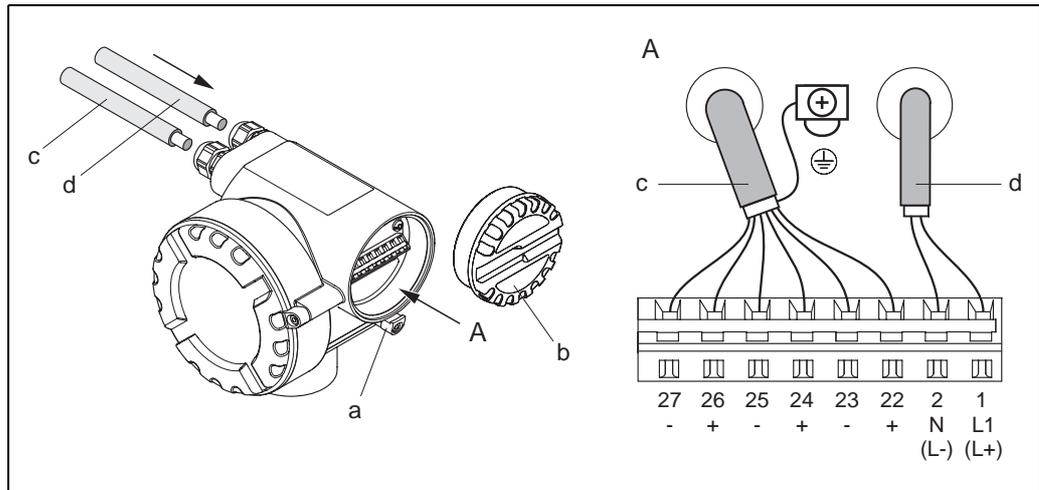

Connecting the transmitter, cable cross-section: max. 2.5 mm² (14 AWG)

A View A

a Safety claw

b Connection compartment cover

c Signal cable: terminal Nos. 22 to 27

(shield for MODBUS RS485 is mandatory; shield for pulse, frequency and status outputs is not required, but recommended)

d Cable for power supply: 20 to 28 V AC, 10 to 30 V DC

– Terminal No. 1: L1 for AC, L+ for DC

– Terminal No. 2: N for AC, L- for DC

Electrical connection, terminal assignment

Order version	Terminal No. (outputs)		
	22 (+) / 23 (-)	24 (+) / 25 (-)	26 (+) / 27 (-)
Fixed communication board (permanent assignment)			
8CM**_**B*****	Pulse / frequency / status output 2	Pulse / frequency / status output 1	MODBUS RS485

Supply voltage

24 V DC nominal voltage (20 to 30 V DC) / 24 V AC nominal voltage (20 to 28 V AC)

Cable entries

Power supply and signal cables (outputs):

- Cable entry M20 × 1.5 (8 to 12 mm / 0.31 to 0.47")
- Threads for cable entries, ½" NPT, G ½"

Cable specifications

Each compatible cable, with a temperature specification at least 20°C (68 °F) higher than the ambient temperature prevailing in the application. We recommend using a cable with a temperature specification of +80°C (176 °F).

MODBUS RS485 (cable type A):

- Characteristic impedance: 135 to 165 Ω at a measuring frequency of 3 to 20 MHz
- Cable capacity: < 30 pF/m (< 9.2 pF/ft)
- Core cross-section: > 0.34 mm² (AWG 22)
- Cable type: twisted pairs
- Loop-resistance: ≤ 110 Ω/km (≤ 0.034 Ω/ft)
- Signal damping: max. 9 dB along the entire length of the cable cross-section
- Shield: Copper braided shielding or braided shielding and foil shielding

Power consumption AC: < 4.0 VA
DC: < 3.2 W

Typical switch-on current at 24 V DC nominal voltage at $R_i = 0.1$ W of the source.

t [ms]	I [A]
0	10.0
0.1	8.0
0.2	7.5
0.5	7.0
1.0	6.0
2.0	4.0
5.0	1.5
10.0	0.125 (operating current)



Note!
The internal resistance of the source may not exceed $R_i = 10$ W.

Power supply failure Lasting min. 20 ms:
■ HistoROM/S-DAT: exchangeable data storage chip which stores the data of the sensor (nominal diameter, serial number, calibration factor, zero point etc.)

Potential equalization No measures necessary.
For explosion-protected equipment → separate Ex-documentation supplied

Performance characteristics

Reference operating conditions

- Error limits following ISO/DIS 11631
- Water, typically 20 to 30 °C (68 to 86 °F); 2 to 4 bar (30 to 60 psi)
- Data as per the calibration report ± 5 °C (± 9 °F) and ± 2 bar (± 30 psi)
- Data on the measured error based on accredited calibration rigs traced back to ISO 17025

Maximum measured error

The values indicated refer to the pulse/frequency output.
The additional measured error for the current output is typically ± 5 μ A. Basis for calculations \rightarrow 9.

o.r. = of reading

Mass flow and volume flow (liquids)

- $\pm 0.10\%$ o.r. (mass flow)
- $\pm 0.10\%$ o.r. (volume flow)

Density (liquids)

- ± 0.001 g/cc (after field density calibration or under reference conditions)
- ± 0.002 g/cc (special density calibration (optional)
Calibration range: 0.0 to 2.0 g/cc, 5 to 80 °C (41 to 176 °F)
Application range: 0.0 to 5.0 g/cc, -50 to 200 °C (-58 to 392 °F)
- ± 0.02 g/cc (standard calibration)

Temperature


± 0.5 °C $\pm 0.005 \cdot T$ °C
(± 1.0 °F $\pm 0.003 \cdot (T - 32)$ °F)

T = Fluid temperature

Zero point stability

DN		Max. full scale value		Zero point stability	
[mm]	[inch]	[kg/h]	[lb/min]	[kg/h]	[lb/min]
1	1/24"	0 to 20	0 to 0.75	0.0008	0.00003
2	1/12"	0 to 100	0 to 3.7	0.002	0.00007
4	1/8"	0 to 450	0 to 16.5	0.014	0.0005
6	1/4"	0 to 1000	0 to 37	0.02	0.0007

Example of maximum measured error

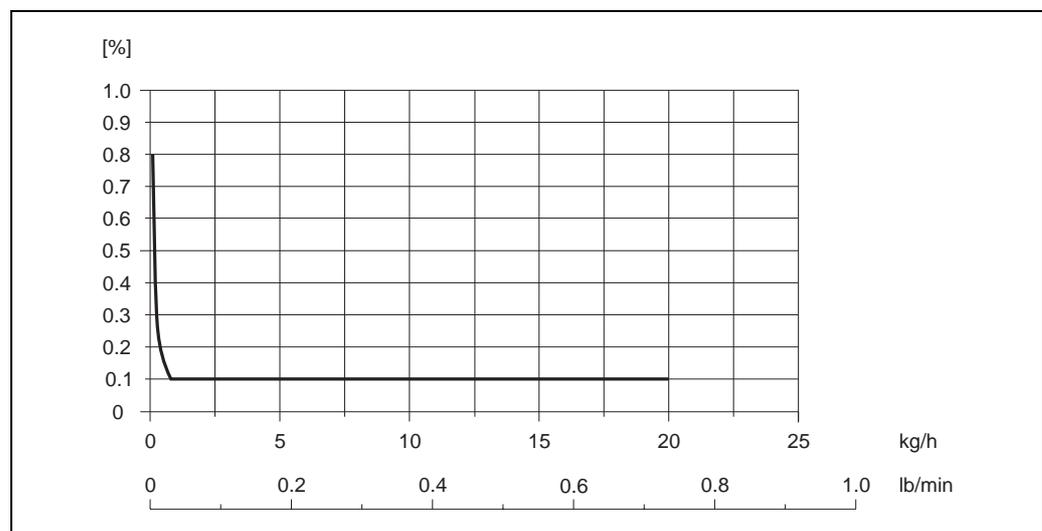

Max. measured error in % o.r. (example: Cubemass, DN 1)

Flow values (examples)

Basis for calculations → 9.

Flow rate		Maximum measured error
[kg/h]	[lb/min]	[% o.r.]
0.1	0.0037	0.8
0.7	0.0257	0.114
2.5	0.0919	0.1
15	0.5513	0.1

Repeatability

Basis for calculations → 9.

o.r. = of reading

Mass flow and volume flow (liquids)

- ±0.05% o.r. (mass flow)
- ±0.05% o.r. (volume flow)

Density (liquids)

- ±0.0005 g/cc

1 g/cc = 1 kg/l

Temperature $\pm 0.25 \text{ }^\circ\text{C} \pm 0.0025 \cdot T \text{ }^\circ\text{C}$ $(\pm 0.5 \text{ }^\circ\text{F} \pm 0.0015 \cdot (T - 32) \text{ }^\circ\text{F})$

T = Fluid temperature

Influence of medium temperature

When there is a difference between the temperature for zero point adjustment and the process temperature, the typical measured error is ±0.0002% of the full scale value / °C (±0.0001% of the full scale value / °F).

Influence of medium pressure

The tables below shows the effect on accuracy of mass flow due to a difference between calibration pressure and process pressure.

DN		Medium pressure	
[mm]	[inch]	[% o.r./bar]	[% o.r./psi]
1	1/24"	-0.001	-0.00007
2	1/12"	0	0
4	1/8"	-0.005	-0.0004
6	¼"	-0.003	-0.0002

o.r. = of reading

Basis for calculations

Depends on the flow:

- Flow \geq zero point stability : (basic accuracy : 100)
 - Max. measured error: \pm basic accuracy in % o.r.
 - Repeatability: $\pm 1/2 \cdot$ basic accuracy in % o.r.
- Flow $<$ zero point stability : (basic accuracy : 100)
 - Max. measured error: \pm (zero point stability : measured value) \cdot 100% o.r.
 - Repeatability: $\pm 1/2 \cdot$ (zero point stability : measured value) \cdot 100% o.r.


o.r. = of reading

Operating conditions: Installation

Installation instructions

Note the following points:

- The measuring device is designed for mounting on tabletops, walls or pipes.
- The high oscillation frequency of the measuring tubes ensures that the correct operation of the measuring system is not influenced by pipe vibrations.
- No special precautions need to be taken for fittings which create turbulence (valves, elbows, T-pieces etc.) as long as no cavitation occurs.

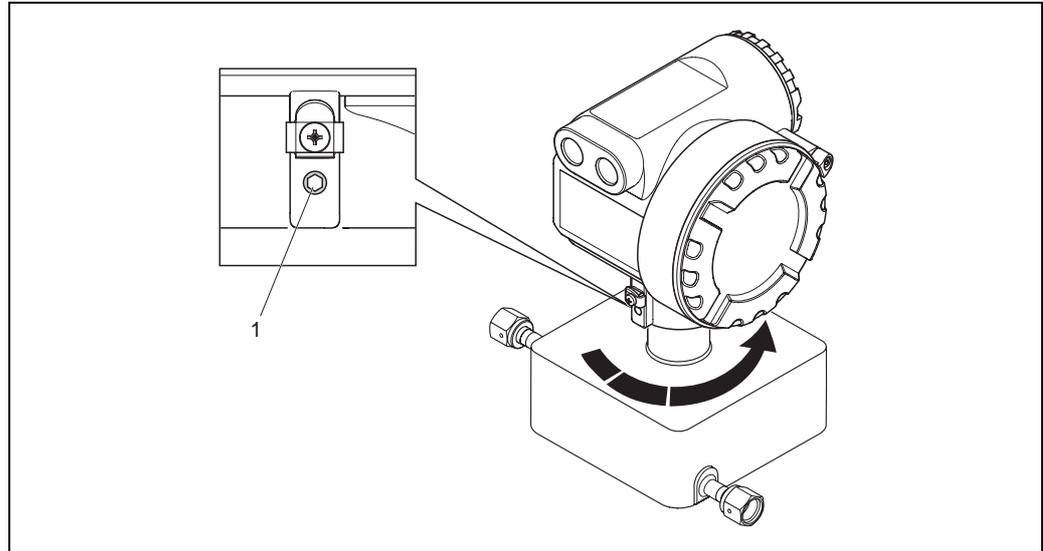

Rotating the transmitter housing


1 = Allen screw

Zero point adjustment

All measuring devices are calibrated using state-of-the-art technology. The zero point obtained in this way is printed on the nameplate. Calibration takes place under reference conditions (→ 8). Therefore, a zero point adjustment is generally **not** required!

If a zero point adjustment is desired, please note the following points before performing one:

- Adjustment can only be performed under stable pressure conditions.
- The zero point adjustment takes place at zero flow. This can be achieved, for example, with shutoff valves upstream and/or downstream of the sensor or by using existing valves and gates.
 - Normal operation → valves 1 and 2 open
 - Zero point adjustment *with* process pressure → Valve 1 open / valve 2 closed
 - Zero point adjustment *without* process pressure → Valve 1 closed / valve 2 open
- A zero point adjustment is **not** possible if an error message is present.

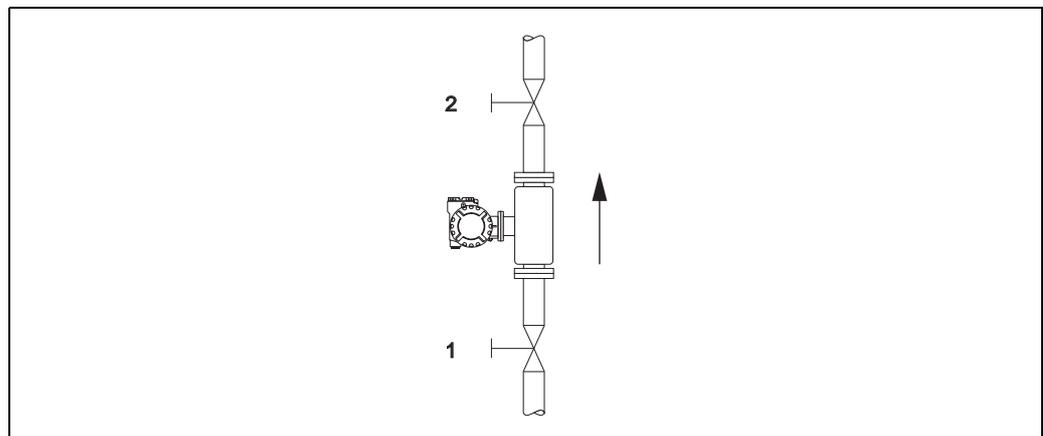

Zero point adjustment and shutoff valves

Inlet and outlet runs

There are no installation requirements regarding inlet and outlet runs. If possible, mount the sensor upstream of fittings such as valves, T-pieces, elbows etc.

System pressure

It is important to ensure that cavitation does not occur as it could influence the oscillation of the measuring tube. No special measures need to be taken for fluids which have properties similar to water under normal conditions.

In the case of liquids with a low boiling point (hydrocarbons, solvents, liquefied gases) or in suction lines, it is important to ensure that pressure does not drop below the vapor pressure and that the liquid does not start to boil. It is also important to ensure that the gases that occur naturally in many liquids do not outgas. Such effects can be prevented when system pressure is sufficiently high.

Consequently, it is generally best to install the sensor:

- On the pump pressure side (no risk of vacuum)
- At the lowest point in a riser

Operating conditions: Environment

Ambient temperature range

Sensor and transmitter:

- Standard: -20 to +60 °C (-4 to +140 °F)
- Optional: -40 to +60 °C (-40 to +140 °F)



Note!

- Install the device in a shady location. Avoid direct sunlight, particularly in warm climatic regions.
-

Storage temperature-40 to +80 °C (-40 to +175 °F), preferably at +20 °C (+68 °F)

Degree of protectionStandard: IP 67 (NEMA 4X) for transmitter and sensor

Shock resistanceAccording to IEC 68-2-31

Vibration resistanceAcceleration up to 1 g, 10 to 150 Hz, following IEC 68-2-6

CIP cleaningYes

SIP cleaningYes

Electromagnetic compatibility (EMC)As per IEC/EN 61326 and NAMUR Recommendation NE 21

Operating conditions: Process

Medium temperature range

Sensor

- -50 to +200 °C (-58 to +392 °F)

Seals

- Only for mounting kits with threaded connections:
 - Viton: -15 to 200 °C (-5 to +392 °F)
 - EPDM: -40 to +160 °C (-40 to +320 °F)
 - Silicone: -60 to +200 °C (-76 to +392 °F)
 - Kalrez: -20 to +275 °C (-4 to +527 °F)

Fluid pressure range (nominal pressure)

DN		Max. nominal pressure	
[mm]	[inch]	[bar]	[psi]
1	1/24"	400	5800
2	1/12"	160	2320
4	1/8"		
6	¼"		

Pressure range of secondary containment

- 25 bar (363 psi)

Rupture element/disk (optional)

Further information → [20](#)

Limiting flow

→ [5](#), "Measuring range"


Pressure loss (SI units)

Pressure loss depends on the fluid properties and on the flow rate. The following formulas can be used to approximately calculate the pressure loss:

Reynolds number	$Re = \frac{4 \cdot \dot{m}}{\pi \cdot d \cdot \nu \cdot \rho}$	A0003381
$Re \geq 2300^{1)}$	$\Delta p = K \cdot \nu^{0.25} \cdot \dot{m}^{1.75} \cdot \rho^{-0.75}$	A0003380
$Re < 2300$	$\Delta p = K1 \cdot \nu \cdot \dot{m}$	A0003379
<p>Δp = pressure loss [mbar] ν = kinematic viscosity [m²/s] \dot{m} = mass flow [kg/s] ρ = density [kg/m³] d = inside diameter of measuring tubes [m] $K, K1$ = constants (depending on nominal diameter) ¹⁾ To compute the pressure loss for gases, always use the formula for $Re \geq 2300$.</p>		

Pressure loss coefficients for Cubemass

DN		d [m]	K	K1
[mm]	[inch]			
1	1/24"	$1.40 \cdot 10^{-3}$	$7.78 \cdot 10^{10}$	$9.50 \cdot 10^{10}$
2	1/12"	$2.50 \cdot 10^{-3}$	$5.04 \cdot 10^9$	$9.51 \cdot 10^9$
4	1/8"	$3.90 \cdot 10^{-3}$	$6.31 \cdot 10^8$	$1.66 \cdot 10^9$
6	1/4"	$5.35 \cdot 10^{-3}$	$1.49 \cdot 10^8$	$4.97 \cdot 10^8$

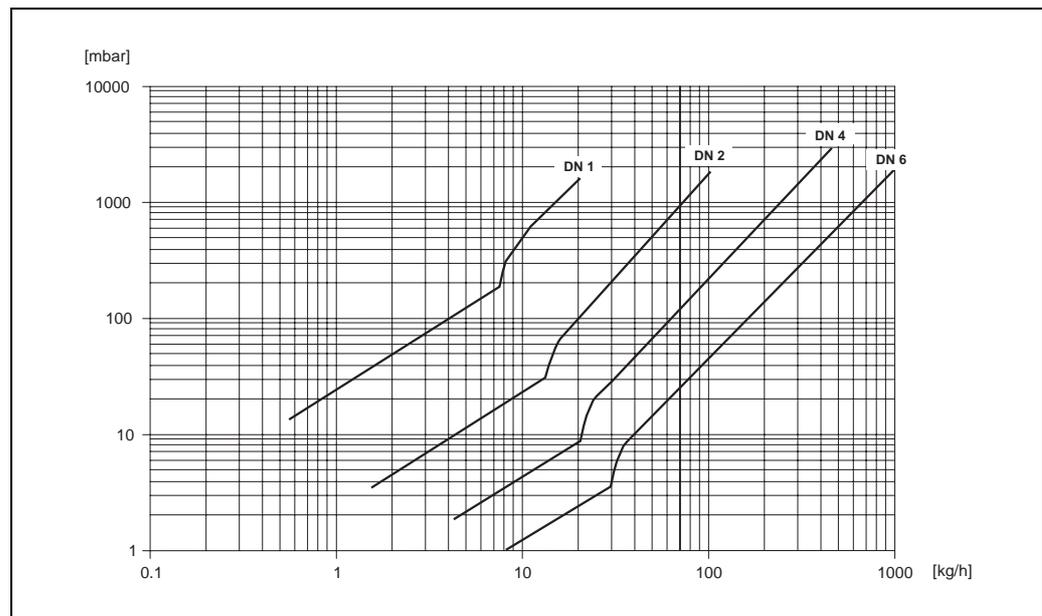

Pressure loss diagram for water

A0011692

Pressure loss (US units)

Pressure loss depends on the nominal diameter and the fluid properties.

The "Applicator" PC software is available from Endress+Hauser and can be used to calculate the pressure loss in US units. The "Applicator" program contains all the important device data which allows the measuring system arrangement to be optimized.

The software is used for the following calculations:


- Nominal diameter of the sensor with fluid properties such as viscosity, density etc.
- Pressure loss downstream from the measuring point
- Conversion of mass flow to volume flow etc.
- Simultaneous display of variables determined by different measuring devices
- Determining measuring ranges

The Applicator program runs on any IBM-compatible PC with Windows.

Mechanical construction

Design/dimensions

Field housing compact version (non-hazardous area II2G / zone 1)

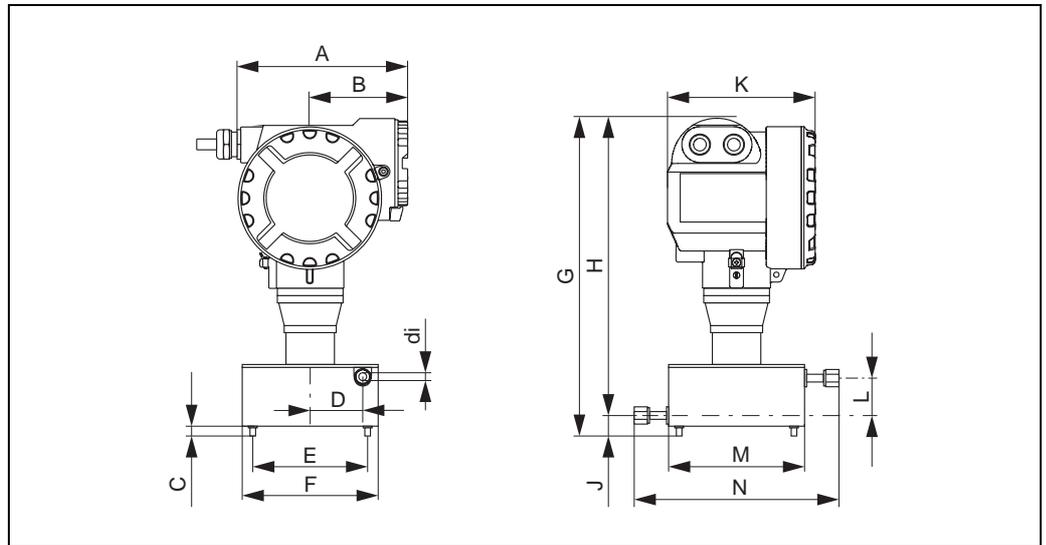

A0013129

Dimensions in SI units

DN	A	B	C	D	E	F	G	H	J	K	L	M	N	di
1	160	92	10	40	90	120	295	273	22	168	30	120	175	1.3
2														2
4														3.9
6														5.35

DN 1 to 4: 4-VCO-4

DN 6: 8-VCO-4

All dimensions in [mm]

Dimensions in US units


DN	A	B	C	D	E	F	G	H	J	K	L	M	N	di
1/24"	6.30	3.62	0.39	1.57	3.54	4.72	11.6	10.8	0.87	6.61	1.18	4.72	6.89	0.05
1/12"														0.08
1/8"														0.15
1/4"														0.21

DN 1/24 to 1/8": 4-VCO-4

DN 1/4": 8-VCO-4

All dimensions in [inch]

4-VCO-4 connection (welded; DN 1 to 4)
8-VCO-4 connection (welded; DN 6)

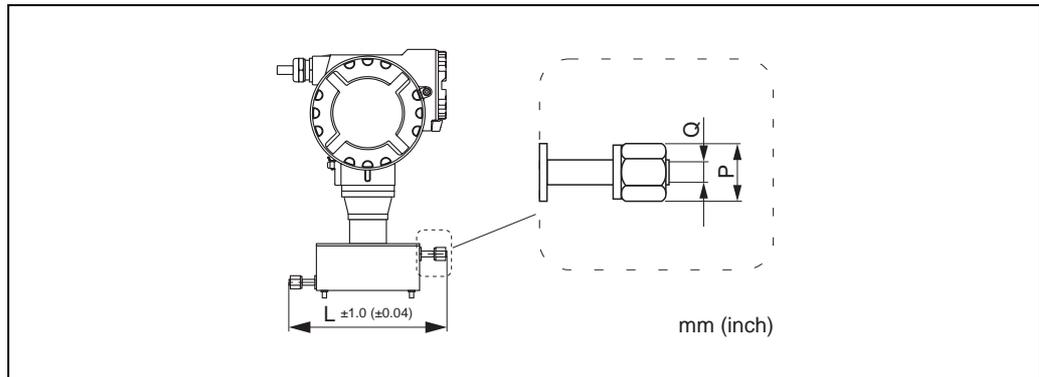

A0013133

Dimensions in SI units

4-VCO-4 / 8-VCO-4 connection: 1.4539/904L			
DN	L	P	Q
1 to 4	175	AF 11/16"	12.5
6	175	AF 1"	20


All dimensions in [mm]

Dimensions in US units

4-VCO-4 / 8-VCO-4 connection: 1.4539/904L			
DN	L	P	Q
1/24 to 1/8"	6.89	AF 11/16"	0.49
1/4"	6.89	AF 1"	0.79

All dimensions in [inch]

4-VCO-4 connection with mounting kit: DN 15 flange (DN 1 to 4)
 8-VCO-4 connection with mounting kit: DN 15 flange (DN 6)

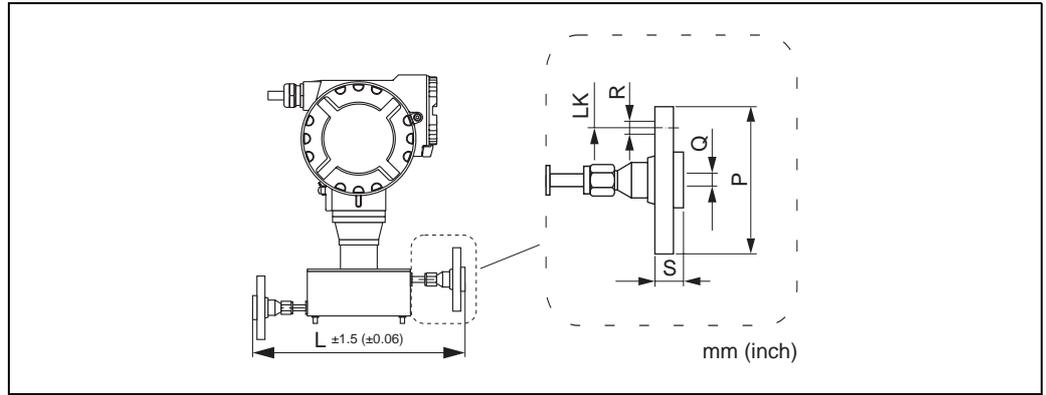

A0013134

Dimensions in SI units

Mounting kit DN 15 flange EN 1092-1 (DIN 2501) PN 40: 1.4539/904L							
DN	PN	L	P	Q	R	S	LK
1 to 6	40	278	95	17.3	4 × Ø 14	28	65

Mounting kit DN 15 flange (JIS): 1.4539/904L							
DN	JIS	L	P	Q	R	S	LK
1 to 6	10K	278	95	15	4 × Ø 15	28	70

Mounting kit ½" flange (ASME): 1.4539/904L							
DN	ASME	L	P	Q	R	S	LK
1 to 6	Cl 150	278	88.9	15.7	4 × Ø 15.7	17.7	60.5
1 to 6	Cl 300	278	95.2	15.7	4 × Ø 15.7	20.7	66.5

Loose flanges (not wetted) made from stainless steel 1.4404/316L
 All dimensions in [mm]

Dimensions in US units


Mounting kit DN 15 flange EN 1092-1 (DIN 2501) PN 40: 1.4539/904L							
DN	PN	L	P	Q	R	S	LK
1/24 to ¼"	40	11	3.74	0.68	4 × Ø 0.55	1.10	2.56

Mounting kit DN 15 flange (JIS): 1.4539/904L							
DN	JIS	L	P	Q	R	S	LK
1/24 to ¼"	10K	11	3.74	0.59	4 × Ø 0.59	1.10	2.76

Mounting kit ½" flange (ASME): 1.4539/904L							
DN	ASME	L	P	Q	R	S	LK
1/24 to ¼"	Cl 150	11	3.50	0.62	4 × Ø 0.62	0.70	2.38
1/24 to ¼"	Cl 300	11	3.75	0.62	4 × Ø 0.62	0.82	2.62

Loose flanges (not wetted) made from stainless steel 1.4404/316L
 All dimensions in [inch]

4-VCO-4 connection with mounting kit: NPT-F (DN 1 to 4)
 8-VCO-4 connection with mounting kit: NPT-F (DN 6)

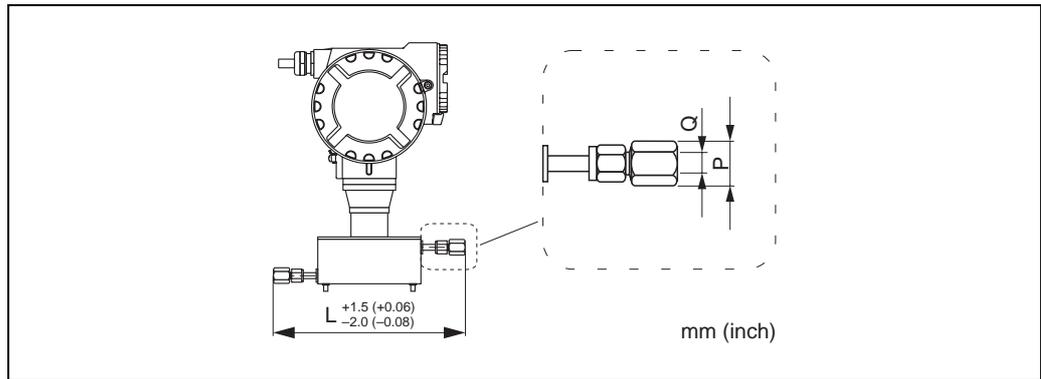

Dimensions in SI units

Mounting kit NPT-F connection: 1.4539/904L			
DN	L	P	Q
1 to 4	265	AF 3/4"	1/4" NPT-F
6	265	AF 1 1/16"	1/2" NPT-F

All dimensions in [mm]


Dimensions in US units

Mounting kit NPT-F connection: 1.4539/904L			
DN	L	P	Q
1/24 to 1/8"	10.43	AF 3/4"	1/4" NPT-F
1/4"	10.43	AF 1 1/16"	1/2" NPT-F

All dimensions in [inch]

Purge connections / secondary containment monitoring**Caution!**

The secondary containment is filled with dry nitrogen (N_2). Do not open the purge connections unless the containment can be filled immediately with a dry inert gas. Use only low overpressure to purge. Maximum pressure 5 bar (73 psi).

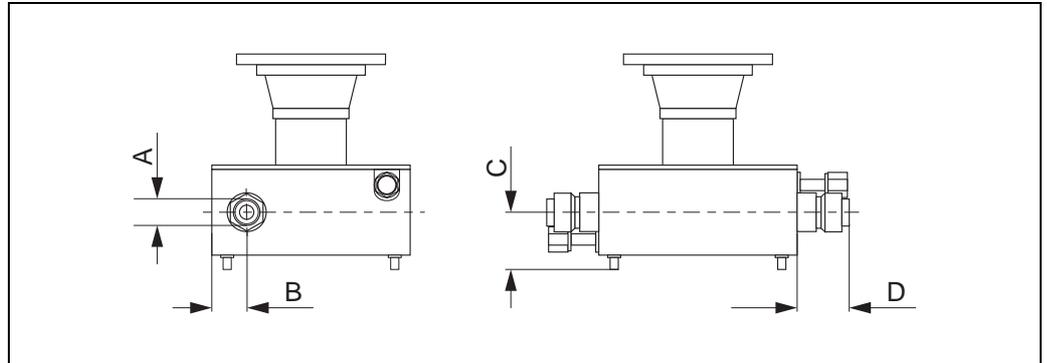*Dimensions in SI units*

DN	A	B	C	D
1 to 6	½" NPT	30	37	33

All dimensions in [mm]

Dimensions in US units

DN	A	B	C	D
1/24 to ¼"	½" NPT	1.18	1.46	1.30

All dimensions in [inch]

Rupture element/disk

The sensor housing is optionally available with an integrated rupture element.



Warning!

- Make sure that the function of the rupture element is not impeded by the installation. The triggering pressure in the housing is indicated on the information notice. Take suitable measures to ensure that no damage can occur if the rupture disk is tripped and personal injury is ruled out.
Triggering pressure in the housing 10 to 15 bar (145 to 217 psi)
- Please note that if a rupture disk is used, the housing can no longer assume a secondary containment function.
- It is not permitted to open the connections or remove the rupture disk.




Caution!

The existing connection nozzles are not designed for a purge or pressure monitoring function.




Note!

- The transportation guard on the rupture disk must be removed prior to commissioning.
- Comply with the information on information notices.

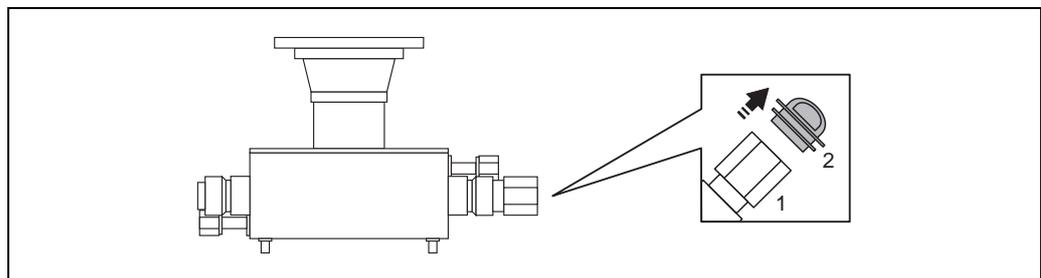

A0012344

1 = Rupture element, 2 = Transportation guard

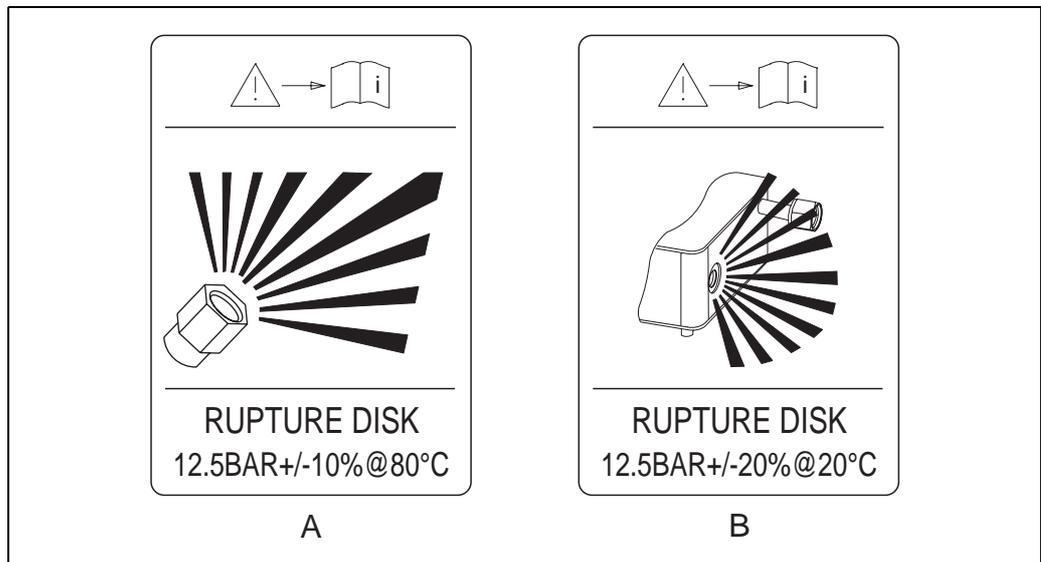

A0011967


Additional sign regarding the position of the rupture disk (RUPTURE DISK)

- A Sensor housing with rupture element (incl. rupture disk) → defined fluid exit
- A Sensor housing with rupture disk → undefined fluid exit



Note!

The location of the rupture disk with undefined fluid exit is covered over by an adhesive label. If the rupture disk is tripped, the adhesive label is destroyed, meaning that a visual check is possible.

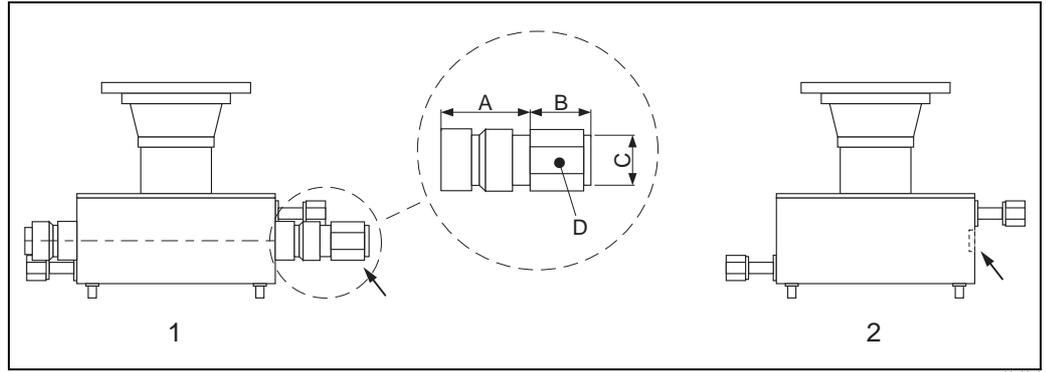

A0012340

Dimensions with rupture element/disk

- 1 Sensor housing with rupture element (incl. rupture disk)
- 2 Sensor housing with rupture disk

Dimensions in SI units

DN	A	B	C	D
1 to 6	33	approx. 42	½" NPT	AF 1"

All dimensions in [mm]

Dimensions in US units

DN	A	B	C	D
1/24 to ¼"	1.30	approx. 1.65	½" NPT	AF 1"

All dimensions in [inch]

Weight

Compact version	
[kg]	[lb]
5.0	11.0

Material**Transmitter housing**

- Aluminum housing; powder-coated die-cast aluminum

Sensor housing / secondary containment

- Acid-resistant and alkali-resistant external surface, stainless steel 1.4301/304

Process connections

Process connections	Material
Mounting set for flanges EN 1092-1 (DIN 2501) / ANSI B16.5 / JIS B2238	Stainless steel 1.4539/904L
Loose flanges	Stainless steel 1.4404/316L
VCO coupling	Stainless steel 1.4539/904L
Mounting set for NPT-F (1/4", 1/2")	Stainless steel 1.4539/904L

Measuring tube

- 1.4539/904L

Seals for mounting set

- Viton
- EPDM
- Silicone
- Kalrez

Material load diagram


Warning!

The following load curves relate to the entire measuring device and not just to the process connection.

Flange connections according to EN 1092-1 (DIN 2501) (mounting kit)

Wetted parts (flange, measuring tube): 1.4539/904L


Loose flanges (not wetted): 1.4404/316L

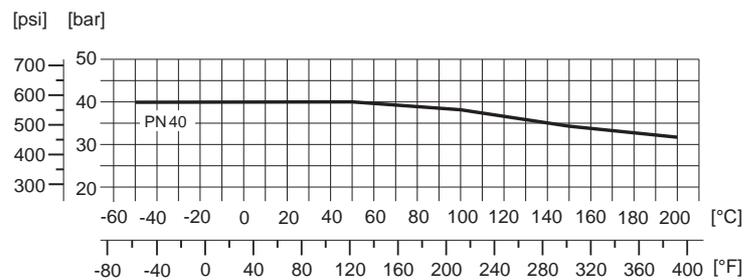

A0012140

Flange connections as per ASME B16.5 (mounting kit)


Wetted parts (flange, measuring tube): 1.4539/904L
 Loose flanges (not wetted): 1.4404/316L

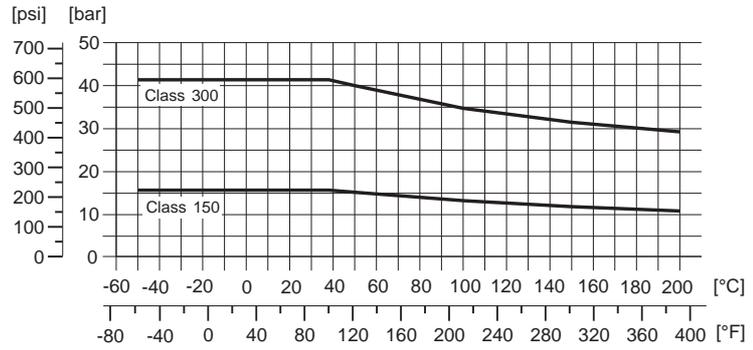

A0012141


Flange connections as per JIS B2220 (mounting kit)

Wetted parts (flange, measuring tube): 1.4539/904L
 Loose flanges (not wetted): 1.4404/316L

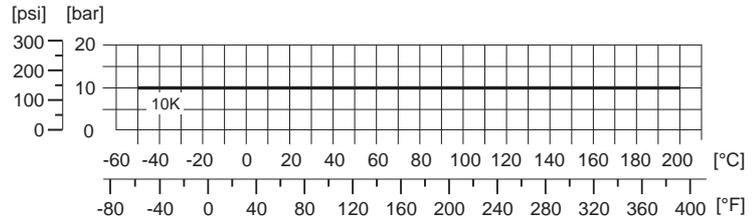

A0012143

**Process connection 4-VCO-4, 1/4" NPT-F (DN 1 to 4),
 8-VCO-4, 1/2" NPT-F (DN 6)**

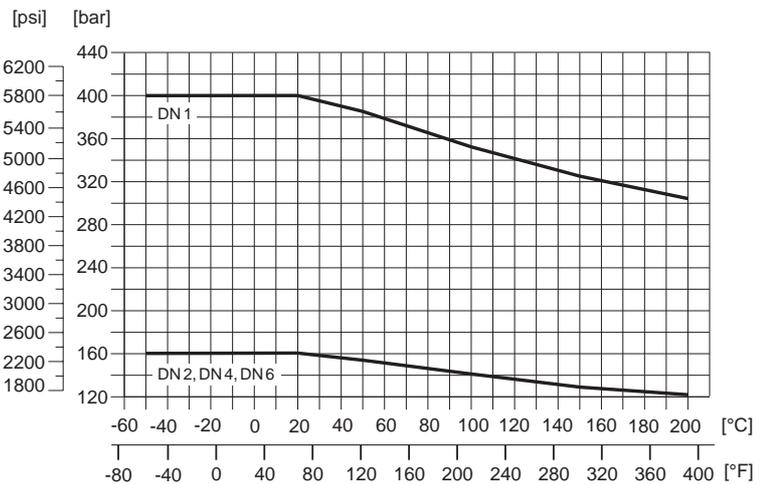

A0011882

Process connections

- Welded process connections
 - 4-VCO-4 -coupling (DN 1 to 4)
 - 8-VCO-4 coupling (DN 6)
- Threaded process connections
 - Flanges according to EN 1092-1 (DIN 2501), JIS, ASME
 - 1/4" NPT-F thread adapter (DN 1 to 4)
 - 1/2" NPT-F thread adapter (DN 6)

Human interface

Display elements	Status LED
Remote operation	Operation takes place using the "FieldCare" configuration and service program from Endress+Hauser and the MODBUS RS485, which can be used to configure parameters for functions and read measuring values.

Certificates and approvals

CE mark	The measuring system is in conformity with the statutory requirements of the EC Directives. Endress+Hauser confirms successful testing of the device by affixing to it the CE mark.
C-Tick symbol	The measuring system meets the EMC requirements of the Australian Communications and Media Authority (ACMA).
Ex approval	Information about currently available Ex versions (ATEX, NEC/CEC etc.) can be supplied by your Endress+Hauser sales office on request. All information relevant to explosion protection is available in separate Ex documents that you can order as necessary.
Pressure Equipment Directive	Measuring devices with a nominal diameter smaller than or equal to DN 25 (1") correspond to Article 3(3) of the EC Directive 97/23/EC (Pressure Equipment Directive) and have been designed and manufactured according to good engineering practice.
Functional safety	SIL 2: in accordance with IEC 61508/IEC 61511-1 (FDIS)
Other standards and guidelines	<ul style="list-style-type: none"> ■ EN 60529: Degrees of protection provided by enclosures (IP code) ■ EN 61010-1: Safety requirements for electrical equipment for measurement, control and laboratory use ■ IEC/EN 61326: Electromagnetic compatibility (EMC requirements) ■ NAMUR Recommendation NE 21: Electromagnetic compatibility (EMC) of industrial process and laboratory control equipment ■ NAMUR Recommendation NE 43: Standardization of the signal level for the breakdown information of digital transmitters with analog output signal. ■ NAMUR Recommendation NE 53: Software of field devices and signal-processing devices with digital electronics

Ordering information

The Endress +Hauser service organization can provide ordering information and detailed information on the order code.

Accessories

Various accessories, which can be ordered separately from Endress+Hauser, are available for the transmitter and the sensor.



Note!

The Endress +Hauser service organization can provide detailed information on the relevant order codes.

Documentation

- Flow measurement (FA005D/06)
- System Information Promass (SI032D/06)
- Operating Instructions MODBUS RS485 (BA142D/06)
- Description of Device Parameters MODBUS RS485 (GP005D/06)
- Ex-Supplementary documentation ATEX (II2G): (XA146D/06)
- Ex-Supplementary documentation NEC/CEC (Div. 1): (XA147D/06)
- Ex-Supplementary documentation NEPSI (Zone 1, Zone 21): (XA148D/06)

Registered trademarks

KALREZ® and VITON®

Registered trademarks of E.I. Du Pont de Nemours & Co., Wilmington, USA

MODBUS®

Registered trademark of the MODBUS Organization

HistoROM™, S-DAT®, FieldCare®, Fieldcheck®, Applicator®

Registered or registration-pending trademarks of Endress+Hauser Flowtec AG, Reinach, CH

Instruments International

Endress+Hauser
Instruments International AG
Kaegenstrasse 2
4153 Reinach
Switzerland

Tel. +41 61 715 81 00
Fax +41 61 715 25 00
www.endress.com
info@ii.endress.com

Endress+Hauser 
People for Process Automation