

Technical Information

Proline Promass U 500

Coriolis flowmeter for single use



Application

- Measuring principle operates independently of physical fluid properties such as viscosity or density
- Highest measurement performance for liquids in single-use processes for the Life Sciences Industry

Device properties

- Standard cable between sensor and transmitter
- Fully traceable cGMP compliance
- One sensor fits four line sizes: $\frac{1}{8}$ to 1"
- Remote version with up to 4 I/Os
- Backlit display with touch control and WLAN access
- Standard cable between sensor and transmitter

Your benefits

- Modern fieldbus communication protocols (2-wire)
- One sensor fits all DN – single variant with 4 disposable line sizes provides highest turndown ratio
- One-hand mounting of disposable – easy commissioning due to intuitive clamping mechanism
- Mounting angle - self drainability or air bubble escape
- Full access to process and diagnostic information – numerous, freely combinable I/Os and Ethernet
- Reduced complexity and variety – freely configurable I/O functionality
- Integrated verification – Heartbeat Technology

Table of contents

About this document	4	Environment	40
Symbols	4	Ambient temperature range	40
Function and system design	5	Storage temperature	40
Measuring principle	5	Shelf life	40
Measuring system	7	Climate class	40
Reliability	8	Relative humidity	40
Input	11	Operating height	40
Measured variable	11	Degree of protection	40
Measuring range	11	Vibration-resistance and shock-resistance	40
Operable flow range	11	Mechanical load	41
Input signal	11	Electromagnetic compatibility (EMC)	41
Output	13	Process	41
Output and input variants	13	Medium temperature range	41
Output signal	15	Medium density	41
Signal on alarm	19	Medium pressure	41
Load	20	Flow limit	41
Low flow cut off	20	Pressure loss	41
Galvanic isolation	21	Static pressure	41
Protocol-specific data	21	Vibrations	41
Power supply	24	Mechanical construction	42
Terminal assignment	24	Dimensions in SI units	42
Available device plugs Proline 500	25	Dimensions in US units	46
Available device plugs Proline 500 digital	25	Weight	49
Pin assignment, device plug	26	Materials	49
Supply voltage	27	Surface roughness	50
Power consumption	27	Display and user interface	50
Current consumption	27	Operation concept	50
Power supply failure	27	Languages	50
Overcurrent protection element	27	Onsite operation	51
Electrical connection	28	Remote operation	51
Potential equalization	32	Service interface	53
Terminals	32	Supported operating tools	55
Cable entries	33	Certificates and approvals	56
Cable specification	33	CE mark	56
Overvoltage protection	34	UKCA marking	56
Performance characteristics	34	RCM marking	56
Reference operating conditions	34	Material certificate	56
Maximum measurement error	34	PROFINET over Ethernet-APL/SPE certification	57
Repeatability	35	Radio approval	57
Response time	36	Additional certification	57
Influence of ambient temperature	36	External standards and guidelines	57
Influence of medium temperature	36	Ordering information	58
Influence of medium pressure	36	Application packages	58
Design fundamentals	36	Accessories	58
Installation	37	Device-specific accessories	58
Installation point	37	Communication-specific accessories	59
Orientation	37	Service-specific accessories	60
Inlet and outlet runs	38		
Installing the transmitter housing	39		
Special installation instructions	39		

Documentation 60
Standard documentation 60
Supplementary device-dependent documentation 61

Registered trademarks 61

About this document

Symbols

Electrical symbols

Symbol	Meaning
	Direct current
	Alternating current
	Direct current and alternating current
	Ground connection A grounded terminal which, as far as the operator is concerned, is grounded via a grounding system.
	Protective earth (PE) Ground terminals that must be connected to ground prior to establishing any other connections. The ground terminals are located on the interior and exterior of the device: ■ Interior ground terminal: protective earth is connected to the mains supply. ■ Exterior ground terminal: device is connected to the plant grounding system.

Communication-specific symbols

Symbol	Meaning
	Wireless Local Area Network (WLAN) Communication via a wireless, local area network
	LED LED is off.
	LED LED is on.
	LED LED flashing.

Symbols for certain types of information

Symbol	Meaning
	Permitted Procedures, processes or actions that are permitted.
	Preferred Procedures, processes or actions that are preferred.
	Forbidden Procedures, processes or actions that are forbidden.
	Tip Indicates additional information.
	Reference to documentation
	Reference to page
	Reference to graphic
	Visual inspection

Symbols in graphics

Symbol	Meaning
1, 2, 3, ...	Item numbers
1, 2, 3, ...	Series of steps
A, B, C, ...	Views
A-A, B-B, C-C, ...	Sections
	Hazardous area
	Safe area (non-hazardous area)
	Flow direction

Function and system design

Measuring principle

The measuring principle is based on the controlled generation of Coriolis forces. These forces are always present in a system when both translational and rotational movements are superimposed.

$$F_c = 2 \cdot \Delta m (v \cdot \omega)$$

F_c = Coriolis force

Δm = moving mass


ω = rotational velocity

v = radial velocity in rotating or oscillating system

The amplitude of the Coriolis force depends on the moving mass Δm , its velocity v in the system and thus on the mass flow. Instead of a constant rotational velocity ω , the sensor uses oscillation.

In the sensor, two parallel measuring tubes containing flowing medium oscillate in antiphase, acting like a vibrating fork. The Coriolis forces produced at the measuring tubes cause a phase shift in the tube oscillations (see illustration):

- At zero flow (when the medium is at a standstill) the two tubes oscillate in phase (1).
- Mass flow causes deceleration of the oscillation at the inlet of the tubes (2) and acceleration at the outlet (3).

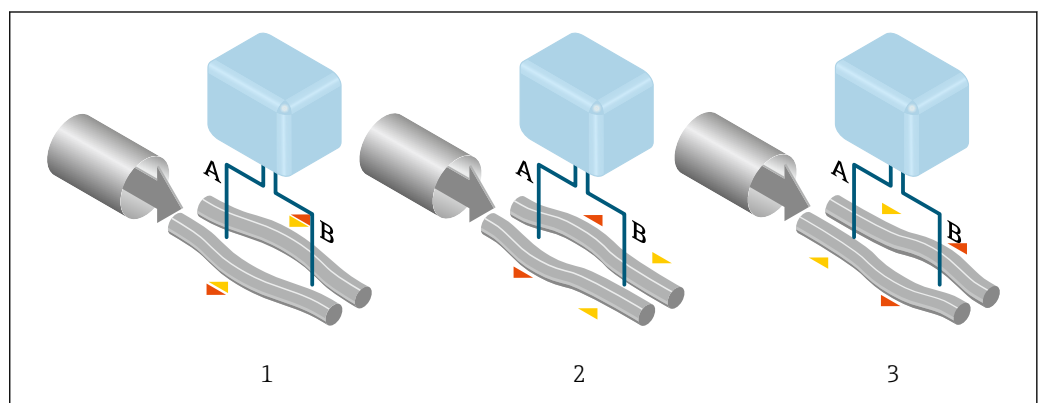

A0028850

The phase shift (A-B) increases with increasing mass flow. Electrodynamic sensors register the tube oscillations at the inlet and outlet. System balance is ensured by the antiphase oscillation of the two measuring tubes. The measuring principle operates independently of temperature, pressure, viscosity, conductivity and flow profile.

Density measurement

The measuring tube is continuously excited at its resonance frequency. A change in the mass and thus the density of the oscillating system (comprising measuring tube and medium) results in a corresponding, automatic adjustment in the oscillation frequency. The resonance frequency is thus a function of the medium density. The microprocessor utilizes this relationship to obtain a density signal.

Volume measurement

Together with the measured mass flow, this is used to calculate the volume flow.

Temperature measurement

The temperature of the measuring tube is determined in order to calculate the compensation factor due to temperature effects. This signal corresponds to the process temperature and is also available as an output signal.

Gas Fraction Handler (GFH)

The Gas Fraction Handler is a Promass software function that improves measurement stability and repeatability. The function continuously checks for the presence of disturbances in single-phase flow, i.e. gas bubbles in liquids. In the presence of the second phase, flow and density become increasingly unstable. The Gas Fraction Handler function improves measurement stability with respect to the severity of the disturbances, without any effect under single-phase flow conditions.



The Gas Fraction Handler is only available for device versions with HART, Modbus RS485, PROFINET, PROFINET over Ethernet-APL and Modbus TCP over Ethernet.



For more detailed information on the Gas Fraction Handler, see the "Gas Fraction Handler" Special Documentation → 61



Measuring system


The measuring system consists of a transmitter, a sensor and a disposable measuring tube.

- The device is available for front panel mounting:
The transmitter and sensor are mounted in physically separate locations and are connected via connecting cables.
- The device is available in a table-top version:
The transmitter and sensor form a mechanical unit.


Proline 500 – digital transmitter

For use in applications not required to meet special requirements due to ambient or operating conditions.

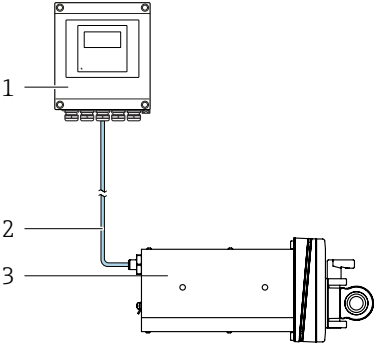Order code for "Device version", option NA "Front panel mounting"  1 Transmitter 2 Connecting cable: cable, separate, standard 3 Sensor ■ Front panel mounting for compact installation in systems ■ Transmitter installation in the protected area ■ GMP-compliant mounting and cleanability ■ Sensor for disposable measuring tube DN 4 to 25 ($\frac{1}{8}$ to 1 ")	Order code for "Device version", option NE "Table version"  1 Transmitter 2 Table version 3 Sensor ■ Compact table unit for stand-alone operation ■ Sensor for disposable measuring tube DN 4 to 25 ($\frac{1}{8}$ to 1 ")
Connecting cable	
Can be ordered in various lengths → 58	-
■ Length: Max. 300 m (1 000 ft) ■ Standard cable with common shield (pair-stranded)	-
Housing versions and materials	
■ Transmitter housing Aluminum, coated: aluminum, AlSi10Mg, coated ■ Material of window in transmitter housing Aluminum, coated: glass	
Configuration	
■ External operation via 4-line, illuminated graphic local display (LCD) with touch control and guided menus ("Make-it-run" wizards) for application-specific commissioning. ■ Via service interface or WLAN interface: ■ Operating tools (e.g. FieldCare, DeviceCare) ■ Web server (access via web browser, e.g. Microsoft Edge)	

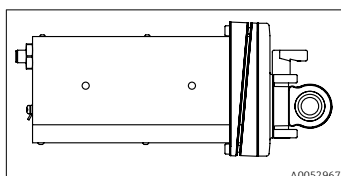Sensor

- Nominal diameter range: DN 4 to 25 ($\frac{1}{8}$ to 1 ")
- Materials:
 - Stainless steel
 - Cast: 1.4409 CF3M - ASTM A 351
 - Seals: EPDM
 - Glass infrared scanner: Silicon optical window
 - Glass camera: Float glass
 - Coil holder: PA6-GF30
 - Wedge: Polycarbonate

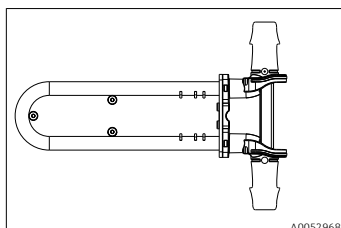Disposable measuring tube

- Bent dual-tube system
- Excellent performance across a wide range of applications
- Simultaneous measurement of flow, volume flow, density and temperature (multivariable)
- Nominal diameter range: DN 4 to 25 ($\frac{1}{8}$ to 1 ")

Materials

- Disposable measuring tube:
 - Measuring tubes: stainless steel 1.4435, 316L
 - Process connections: Makrolon Rx 1805 polycarbonate
 - O-ring: Silicon
- Packaging:
 - Protection blister: PET-G
 - Peel pouch: PET-OPA-PE
 - Double pouch: HDPE

Reliability**IT security**

The manufacturer warranty is valid only if the product is installed and used as described in the Operating Instructions. The product is equipped with security mechanisms to protect it against any inadvertent changes to the settings.

IT security measures, which provide additional protection for the product and associated data transfer, must be implemented by the operators themselves in line with their security standards.

Device-specific IT security

The device offers a range of specific functions to support protective measures on the operator's side. These functions can be configured by the user and guarantee greater in-operation safety if used correctly. The following list provides an overview of the most important functions:

Function/interface	Factory setting	Recommendation
Write protection via hardware write protection switch → 9	Not enabled	On an individual basis following risk assessment
Access code (also applies to web server login or FieldCare connection) → 9	Not enabled (0000)	Assign a customized access code during commissioning
WLAN (order option in display module)	Enabled	On an individual basis following risk assessment
WLAN security mode	Enabled (WPA2-PSK)	Do not change
WLAN passphrase (Password) → 9	Serial number	Assign an individual WLAN passphrase during commissioning
WLAN mode	Access point	On an individual basis following risk assessment
Web server → 9	Enabled	On an individual basis following risk assessment
CDI-RJ45 service interface → 9	Enabled	-

Protecting access via hardware write protection

Write access to the parameters of the device via the local display, Web browser or operating tool (e.g. FieldCare, DeviceCare) can be disabled via a write protection switch (DIP switch on the main electronics module). When hardware write protection is enabled, only read access to the parameters is possible.

Hardware write protection is disabled when the device is delivered.

Protecting access via a password

Different passwords are available to protect write access to the device parameters or access to the device via the WLAN interface.

- **User-specific access code**
Protect write access to the device parameters via the local display, web browser or operating tool (e.g. FieldCare, DeviceCare). Access authorization is clearly regulated through the use of a user-specific access code.
- **WLAN passphrase**
The network key protects a connection between an operating unit (e.g. notebook or tablet) and the device via the WLAN interface which can be ordered as an option.
- **Infrastructure mode**
When the device is operated in infrastructure mode, the WLAN passphrase corresponds to the WLAN passphrase configured on the operator side.

User-specific access code

Write access to the device parameters via the local display, web browser or operating tool (e.g. FieldCare, DeviceCare) can be protected by the modifiable, user-specific access code.

WLAN passphrase: Operation as WLAN access point

A connection between an operating unit (e.g. notebook or tablet) and the device via the WLAN interface, which can be ordered as an optional extra, is protected by the network key. The WLAN authentication of the network key complies with the IEEE 802.11 standard.

When the device is delivered, the network key is pre-defined depending on the device. It can be changed via the **WLAN settings** submenu in the **WLAN passphrase** parameter.

Infrastructure mode

A connection between the device and WLAN access point is protected by means of an SSID and passphrase on the system side. Please contact the relevant system administrator for access.

General notes on the use of passwords

- The access code and network key supplied with the device should be changed during commissioning for safety reasons.
- Follow the general rules for generating a secure password when defining and managing the access code and network key.
- The user is responsible for the management and careful handling of the access code and network key.

Access via web server

The integrated web server can be used to operate and configure the device via a web browser. The connection is established via the service interface (CDI-RJ45) or WLAN interface .

The web server is enabled when the device is delivered. The web server can be disabled if necessary via the **Web server functionality** parameter (e.g., after commissioning).

The device and status information can be hidden on the login page. This prevents unauthorized access to the information.



For detailed information on device parameters, see: Description of Device Parameters.

Access via service interface (port 2): CDI-RJ45

The device can be connected to a network via the service interface. Device-specific functions guarantee the secure operation of the device in a network.

The use of relevant industrial standards and guidelines that have been defined by national and international safety committees, such as IEC/ISA62443 or the IEEE, is recommended. This includes

organizational security measures such as the assignment of access authorization as well as technical measures such as network segmentation.



For detailed information on connecting transmitters with an Ex de approval, see separate document "Safety instructions" (XA) for the device.

Advanced safety requirements

If the specified requirements for measures cannot be met, alternative measures may need to be put in place. This may involve, for example, mechanical protection of the product against tampering, the cabling, or organizational measures. The Proline measuring instruments can be used in the open field for example. Measures to combat physical tampering of the Proline measuring instruments must be arranged by the customer.

Additional analysis is required if Proline measuring instruments are integrated into a different system. Please note the following:

- The fieldbus network (OT) and company network (IT) must be strictly separated.
- Endress+Hauser recommends the segmentation of the fieldbus networks according to DIN IEC 62443-3-3.

Network

Pay particular attention to the network components used, the router and switches for example. The operator must guarantee the integrity of the components. Access to the network must be restricted by the operator, if necessary.

FDI Packages

Signed FDI Packages can be obtained via www.endress.com for the configuration of the field device.

User training

Depending on the application scenario, users who are not specialized in this area may come in contact with the instrument. We recommend that these users be trained in the safe use of the relevant terminals, components and/or interfaces and be made aware of security issues.

Input

Measured variable

Direct measured variables

- Mass flow
- Density
- Temperature

Calculated measured variables

- Volume flow
- Corrected volume flow
- Reference density

Measuring range

Measuring range for liquids

Full scale value defined at 0.2 bar pressure loss.

DN		Measuring range full scale values $\dot{m}_{\min(F)}$ to $\dot{m}_{\max(F)}$	
[mm]	[in]	[kg/min]	[lb/min]
4	$\frac{1}{8}$	0 to 2	0 to 4.4
6	$\frac{1}{4}$	0 to 4.8	0 to 10.6
15	$\frac{1}{2}$	0 to 28.6	0 to 63.1
25	1	0 to 75	0 to 165.3

Recommended measuring range

 Flow limit →  41

Operable flow range

Over 1000 : 1.

Flow rates above the preset full scale value do not override the electronics unit, with the result that the totalizer values are registered correctly.

Input signal

Output and input variants

→  13

External measured values

To increase the measurement accuracy of certain measured variables, the automation system can continuously write various measured values to the measuring instrument:

- pressure to increase measurement accuracy (Endress+Hauser recommends the use of a pressure measuring device for absolute pressure, e.g. Cerabar M or Cerabar S)
- Medium temperature to increase measurement accuracy

Current input

The measured values are written from the automation system to the measuring device via the current input →  11.

Digital communication

The measured values can be written by the automation system via:

- Modbus RS485
- Modbus TCP over Ethernet-APL/SPE
- PROFINET over Ethernet-APL/SPE

Current input 0/4 to 20 mA

Current input	0/4 to 20 mA (active/passive)
Current span	■ 4 to 20 mA (active) ■ 0/4 to 20 mA (passive)

Resolution	1 μ A
Voltage drop	Typically: 0.6 to 2 V for 3.6 to 22 mA (passive)
Maximum input voltage	≤ 30 V (passive)
Open-circuit voltage	≤ 28.8 V (active)
Possible input variables	■ Pressure ■ Temperature ■ Density

Status input

Maximum input values	■ DC -3 to 30 V ■ If status input is active (ON): $R_i > 3$ kΩ
Response time	Configurable: 5 to 200 ms
Input signal level	■ Low signal: DC -3 to +5 V ■ High signal: DC 12 to 30 V
Assignable functions	■ Off ■ Reset the individual totalizers separately ■ Reset all totalizers ■ Flow override

Output

Output and input variants

Depending on the option selected for output/input 1, different options are available for the other outputs and inputs. Only one option can be selected for each output/input 1 to 4. The following tables must be read vertically (↓).

Output/input 1 and options for output/input 2



Options for output/input 3 and 4 → 14

Order code for "Output; input 1" (020) →	Possible options															
Modbus RS485								↓	MA							
PROFINET over Ethernet-APL/SPE											↓	RB				
Order code for "Output; input 2" (021) →	↓	↓	↓	↓	↓	↓	↓	↓	↓	↓	↓	↓	↓	↓	↓	↓
Not used	A	A	A	A	A	A	A	A	A	A	A	A	A	A	A	A
Current output 4 to 20 mA	B			B		B	B		B	B	B	B		B		
User-configurable input/output ¹⁾	D			D		D	D		D	D	D	D		D		
Pulse/frequency/switch output	E			E		E	E		E	E	E	E		E		
Relay output	H			H		H	H		H	H	H	H		H		
Current input 0/4 to 20 mA	I			I		I	I		I	I	I	I		I		
Status input	J			J		J	J		J	J	J	J		J		

1) A specific input or output can be assigned to a user-configurable input/output → 18.

Output/input 1 and options for output/input 3 and 4



Options for output/input 2 → 13

Order code for "Output; input 1" (020) →	Possible options															
Modbus RS485								↓	MA							
PROFINET over Ethernet-APL 10 Mbit/s, 2-wire											↓	RB				
Order code for "Output; input 3" (022), "Output; input 4" (023) ¹⁾ →	↓	↓	↓	↓	↓	↓	↓	↓	↓	↓	↓	↓	↓	↓	↓	↓
Not used	A	A	A	A	A	A	A	A	A	A	A	A	A	A	A	A
Current output 4 to 20 mA	B					B			B	B	B	B		B		
User-configurable input/output	D					D			D	D	D	D		D		
Pulse/frequency/switch output	E					E			E	E	E	E		E		
Relay output	H					H			H	H	H	H		H		
Current input 0/4 to 20 mA	I					I			I	I	I	I		I		
Status input	J					J			J	J	J	J		J		

- 1) The order code for "Output; input 4" (023) is only available for the Proline 500-digital transmitter, order code for "Integrated ISEM electronics", option A.

Output signal

Modbus RS485

Physical interface	RS485 in accordance with EIA/TIA-485 standard
Terminating resistor	Integrated, can be activated via DIP switches

Modbus TCP over Ethernet-APL

Port 1: Modbus TCP over Ethernet-APL 10 Mbit/s

Device usage	Device connection to an APL field switch (terminal 26/27) The device may only be operated according to the following APL port classifications: If used in non-hazardous areas: SLAX Device connection to an SPE switch - In non-hazardous areas, the device can be used with an appropriate SPE switch: - Maximum output voltage: 30 V_{DC} - Minimum output power: 1.85 W - The SPE switch must support the 10BASE-T1L standard and PoDL power classes 10, 11 or 12 and have a function to disable power class detection.
Standards	According to IEEE 802.3cg, APL port profile specification v1.0, galvanically isolated
Data transfer	Full-duplex (APL/SPE)
Current consumption	Terminal 26/27 max. approx. 45 mA
Permitted supply voltage	9 to 30 V
Bus connection	Terminal 26/27 with integrated reverse polarity protection

Port 2: Modbus TCP over Ethernet 100 Mbit/s

Device usage	Device connection to a Fast Ethernet (RJ45) switch In non-hazardous areas, the Ethernet switch must support the standard 100BASE-TX.
Standards	In accordance with IEEE 802.3u
Data transfer	Half-duplex, full-duplex
Current consumption	-
Permitted supply voltage	-
Bus connection	Service interface (RJ45)

PROFINET over Ethernet-APL

Device use	Device connection to an APL field switch The device may only be operated according to the following APL port classifications: If used in non-hazardous areas: SLAX Device connection to an SPE switch - In non-hazardous areas, the device can be used with an appropriate SPE switch: The device can be connected to an SPE switch with a maximum voltage of 30 V_{DC} and a minimum output power of 1.85 W connected. - The SPE switch must support the 10BASE-T1L standard and PoDL power classes 10, 11 or 12 and have a function to disable power class detection.
PROFINET	According to IEC 61158 and IEC 61784
Ethernet-APL	According to IEEE 802.3cg, APL port profile specification v1.0, galvanically isolated
Data transfer	10 Mbit/s

Current consumption	Transmitter - Max. 400 mA(24 V) - Max. 200 mA (110 V, 50/60 Hz; 230 V, 50/60 Hz)
Permitted supply voltage	9 to 30 V
Network connection	With integrated reverse polarity protection

Current output 4 to 20 mA

Signal mode	Can be set to: - Active - Passive
Current range	Can be set to: 4 to 20 mA NAMUR 4 to 20 mA US 4 to 20 mA 0 to 20 mA (only if the signal mode is active) - Fixed current
Maximum output values	22.5 mA
Open-circuit voltage	DC 28.8 V (active)
Maximum input voltage	DC 30 V (passive)
Load	0 to 700 Ω
Resolution	0.38 µA
Damping	Configurable: 0 to 999.9 s
Assignable measured variables	- Mass flow - Volume flow - Corrected volume flow - Density - Reference density - Temperature - Electronics temperature - Oscillation frequency 0 - Oscillation damping 0 - Signal asymmetry - Exciter current 0  The range of options increases if the measuring device has one or more application packages.

Pulse/frequency/switch output

Function	Can be configured as pulse, frequency or switch output
Version	Open collector Can be set to: - Active - Passive - Passive NAMUR  Ex-i, passive
Maximum input values	DC 30 V, 250 mA (passive)
Open-circuit voltage	DC 28.8 V (active)
Voltage drop	For 22.5 mA: ≤ DC 2 V
Pulse output	
Maximum input values	DC 30 V, 250 mA (passive)
Maximum output current	22.5 mA (active)
Open-circuit voltage	DC 28.8 V (active)

Pulse width	Configurable: 0.05 to 2 000 ms
Maximum pulse rate	10 000 Impulse/s
Pulse value	Configurable
Assignable measured variables	■ Mass flow ■ Volume flow ■ Corrected volume flow  The range of options increases if the measuring device has one or more application packages.
Frequency output	
Maximum input values	DC 30 V, 250 mA (passive)
Maximum output current	22.5 mA (active)
Open-circuit voltage	DC 28.8 V (active)
Output frequency	Configurable: end value frequency 2 to 10 000 Hz($f_{\max} = 12\,500\text{ Hz}$)
Damping	Configurable: 0 to 999.9 s
Pulse/pause ratio	1:1
Assignable measured variables	■ Mass flow ■ Volume flow ■ Corrected volume flow ■ Density ■ Reference density ■ Temperature ■ Electronics temperature ■ Oscillation frequency 0 ■ Oscillation damping 0 ■ Signal asymmetry ■ Exciter current 0  The range of options increases if the measuring device has one or more application packages.
Switch output	
Maximum input values	DC 30 V, 250 mA (passive)
Open-circuit voltage	DC 28.8 V (active)
Switching behavior	Binary, conductive or non-conductive
Switching delay	Configurable: 0 to 100 s
Number of switching cycles	Unlimited
Assignable functions	■ Disable ■ On ■ Diagnostic behavior ■ Limit ■ Mass flow ■ Volume flow ■ Corrected volume flow ■ Density ■ Reference density ■ Temperature ■ Totalizer 1-3 ■ Flow direction monitoring ■ Status ■ Partially filled pipe detection ■ Low flow cut off  The range of options increases if the measuring device has one or more application packages.

Double pulse output

Function	Double pulse
Version	Open collector Can be set to: ■ Active ■ Passive ■ Passive NAMUR
Maximum input values	DC 30 V, 250 mA (passive)
Open-circuit voltage	DC 28.8 V (active)
Voltage drop	For 22.5 mA: ≤ DC 2 V
Output frequency	Configurable: 0 to 1 000 Hz
Damping	Configurable: 0 to 999 s
Pulse/pause ratio	1:1
Assignable measured variables	■ Mass flow ■ Volume flow ■ Corrected volume flow ■ Density ■ Reference density ■ Temperature  The range of options increases if the measuring device has one or more application packages.

Relay output

Function	Switch output
Version	Relay output, galvanically isolated
Switching behavior	Can be set to: ■ NO (normally open), factory setting ■ NC (normally closed)
Maximum switching capacity (passive)	■ DC 30 V, 0.1 A ■ AC 30 V, 0.5 A
Assignable functions	■ Disable ■ On ■ Diagnostic behavior ■ Limit ■ Mass flow ■ Volume flow ■ Corrected volume flow ■ Density ■ Reference density ■ Temperature ■ Totalizer 1-3 ■ Flow direction monitoring ■ Status ■ Partially filled pipe detection ■ Low flow cut off  The range of options increases if the measuring device has one or more application packages.

User-configurable input/output

One specific input or output is assigned to a user-configurable input/output (configurable I/O) during device commissioning.

The following inputs and outputs are available for assignment:

- Choice of current output: 4 to 20 mA (active), 0/4 to 20 mA (passive)
- Pulse/frequency/switch output
- Choice of current input: 4 to 20 mA (active), 0/4 to 20 mA (passive)
- Status input

The technical values correspond to those of the inputs and outputs described in this section.

Signal on alarm

Depending on the interface, failure information is displayed as follows:

PROFINET over Ethernet-APL/SPE

Device diagnostics	Diagnostics according to PROFINET PA Profile 4.02
--------------------	---

Modbus RS485

Failure mode	Choose from: ■ NaN value instead of current value ■ Last valid value
--------------	---

Modbus TCP over Ethernet-APL/SPE/Fast Ethernet

Failure mode	Choose from: ■ NaN value instead of current value ■ Last valid value
--------------	---

Current output

Current output 4-20 mA	
Failure mode	Configurable: ■ 4 to 20 mA in accordance with NAMUR recommendation NE 43 ■ 4 to 20 mA in accordance with US ■ Min. value: 3.59 mA ■ Max. value: 22.5 mA ■ Definable value between: 3.59 to 22.5 mA ■ Actual value ■ Last valid value
Current output 4-20 mA	
Failure mode	Configurable: ■ Maximum alarm: 22 mA ■ Definable value between: 0 to 20.5 mA

Pulse/frequency/switch output

Pulse output	
Failure mode	Configurable: ■ Actual value ■ No pulses
Frequency output	
Failure mode	Configurable: ■ Actual value ■ 0 Hz ■ Definable value between: 2 to 12 500 Hz

Switch output	
Failure mode	Configurable: ■ Current status ■ Open ■ Closed

Relay output

Failure mode	Choose from: ■ Current status ■ Open ■ Closed
--------------	---

Local display

Plain text display	With information on cause and remedial measures
Backlight	Red lighting indicates a device error.



Status signal as per NAMUR recommendation NE 107

Interface/protocol

- Via digital communication:
 - Modbus RS485
 - Modbus TCP over Ethernet-APL/SPE
 - PROFINET over Ethernet-APL/SPE
- Via service interface
 - Service interface CDI-RJ45
 - Via service interface/port 2: (RJ45)
 - WLAN interface
- Plain text display
 - With information on cause and remedial action
 - Modbus TCP

Web browser

Plain text display	With information on cause and remedial measures
--------------------	---

LEDs

Status information	Status indicated by various LEDs The following information is displayed depending on the device version: ■ Supply voltage active ■ Data transmission active ■ Device alarm/error has occurred ■ Network available ¹⁾ ■ Connection established ¹⁾ ■ Diagnostic status ²⁾ ■ PROFINET blinking feature ³⁾
--------------------	---

1) Only available for PROFINET over Ethernet-APL, Modbus over Ethernet-APL,

2) Only available for Modbus over Ethernet-APL

3) Only available for PROFINET over Ethernet-APL,

Load Output signal → 15

Low flow cut off The switch points for low flow cut off are user-selectable.

Galvanic isolation

The outputs are galvanically isolated:

- from the power supply
- from one another
- from the potential equalization (PE) connection

Protocol-specific data**Modbus RS485**

Protocol	Modbus Applications Protocol Specification V1.1
Response times	■ Direct data access: typically 25 to 50 ms ■ Auto-scan buffer (data range): typically 3 to 5 ms
Device type	Slave
Slave address range	1 to 247
Broadcast address range	0
Function codes	■ 03: Read holding register ■ 04: Read input register ■ 06: Write single registers ■ 08: Diagnostics ■ 16: Write multiple registers ■ 23: Read/write multiple registers
Broadcast messages	Supported by the following function codes: ■ 06: Write single registers ■ 16: Write multiple registers ■ 23: Read/write multiple registers
Supported baud rate	■ 1 200 BAUD ■ 2 400 BAUD ■ 4 800 BAUD ■ 9 600 BAUD ■ 19 200 BAUD ■ 38 400 BAUD ■ 57 600 BAUD ■ 115 200 BAUD
Data transmission mode	■ ASCII ■ RTU
Data access	Each device parameter can be accessed via Modbus RS485.  For Modbus register information
System integration	Information regarding system integration: Operating Instructions →  61. ■ Modbus RS485 information ■ Function codes ■ Register information ■ Response time ■ Modbus data map

Modbus TCP over Ethernet-APL

Port 1: Modbus TCP over Ethernet-APL 10 Mbit/s, SPE 10 Mbit/s	
Protocol	■ Modbus application protocol V1.1 ■ TCP
Response times	On Modbus client request: Typically 3 to 5 ms
TCP port	502
Modbus TCP connections	Maximum 4
Communication type	Ethernet Advanced Physical Layer 10BASE-T1L
Data transfer	Full-duplex
Polarity	Automatic correction of crossed "APL signal +" and "APL signal -" signal lines
Device type	Address

Device type ID	0xC43B
Function codes	03: Read holding register 04: Read input register 06: Write single registers 16: Write multiple registers 23: Read/write multiple registers 43: Read device identification
Broadcast support for function codes	06: Write single registers 16: Write multiple registers 23: Read/write multiple registers 43: Read device identification
Supported transfer speed	10 Mbit/s (Ethernet-APL)
Supported features	Address can be configured using DHCP, web server or software
Device description files (FDI)	Information and files available at: www.endress.com → Downloads area
Configuration options for measuring instrument	- Asset management software (FieldCare, DeviceCare, Field Expert) - Integrated web server via web browser and IP address - Onsite operation
Supported functions	- Device identification using: Nameplate - Measured value status The process variables are communicated with a measured value status - Blinking feature via the local display for simple device identification and assignment - Device operation via asset management software (e.g. FieldCare, DeviceCare)
System integration	Information regarding system integration: Operating Instructions → 61. - Overview and description of the supported function codes - Status coding - Factory setting

Port 2: Modbus TCP over Ethernet 100 Mbit/s	
Protocol	- Modbus application protocol V1.1 - TCP
Response times	On Modbus client request: Typically 3 to 5 ms
TCP port	502
Modbus TCP connections	Maximum 4
Communication type	10BASE-T 100BASE-TX
Data transfer	Half-duplex, full-duplex
Polarity	Auto-MDIX
Device type	Address
Device type ID	0xC43B
Function codes	03: Read holding register 04: Read input register 06: Write single registers 16: Write multiple registers 23: Read/write multiple registers 43: Read device identification
Broadcast support for function codes	06: Write single registers 16: Write multiple registers 23: Read/write multiple registers 43: Read device identification
Supported transfer speed	10 Mbit/s 100 Mbit/s (Fast-Ethernet)

Supported features	Address can be configured using DHCP, web server or software
Device description files (FDI)	Information and files available at: www.endress.com → Downloads area
Configuration options for measuring instrument	■ Asset management software (FieldCare, DeviceCare, Field Expert) ■ Integrated web server via web browser and IP address ■ Onsite operation
Supported functions	■ Device identification using: Nameplate ■ Measured value status The process variables are communicated with a measured value status ■ Device operation via asset management software (e.g. FieldCare, DeviceCare)
System integration	Information regarding system integration: Operating Instructions → 61. ■ Overview and description of the supported function codes ■ Status coding ■ Factory setting

PROFINET over Ethernet-APL /SPE

Protocol	Application layer protocol for decentral device periphery and distributed automation, Version 2.43
Communication type	Ethernet Advanced Physical Layer 10BASE-T1L
Conformance Class	Conformance Class B (PA)
Netload Class	PROFINET Netload Robustness Class 2 10 Mbit/s
Data transfer	10 Mbit/s Full-duplex
Cycle times	64 ms
Polarity	Automatic correction of crossed "APL signal +" and "APL signal -" signal lines
Media Redundancy Protocol (MRP)	Not possible (point-to-point connection to APL field switch)
System redundancy support	System redundancy S2 (2 AR with 1 NAP)
Device profile	PROFINET PA profile 4.02 (Application interface identifier API: 0x9700)
Manufacturer ID	17
Device type ID	0xA43B
Device description files (GSD, DTM, FDI)	Information and files available at: ■ www.endress.com → Downloads area ■ www.profibus.com
Supported connections	■ 2x AR (IO Controller AR) ■ 2x AR (IO Supervisor Device AR connection allowed)
Configuration options for measuring instrument	■ DIP switches on the electronics module, for device name assignment (last part) ■ Asset management software (FieldCare, DeviceCare, Field Xpert) ■ Integrated Web server via Web browser and IP address ■ Device master file (GSD), can be read out via the integrated Web server of the measuring instrument. ■ Onsite operation
Configuration of the device name	■ DIP switches on the electronics module, for device name assignment (last part) ■ DCP protocol ■ Asset management software (FieldCare, DeviceCare, Field Xpert) ■ Integrated web server

Supported functions	■ Identification & Maintenance, simple device identifier via: ■ Control system ■ Nameplate ■ Measured value status The process variables are communicated with a measured value status ■ Blinking feature via the local display for simple device identification and assignment ■ Device operation via asset management software (e.g. FieldCare, DeviceCare, SIMATIC PDM with FDI package)
System integration	Information regarding system integration: Operating Instructions →  61. ■ Cyclic data transmission ■ Overview and description of the modules ■ Status coding ■ Factory setting

Power supply

Terminal assignment Transmitter: supply voltage, input/outputs

Modbus RS485

Supply voltage		Input/output 1 (port 1)		Input/output 2		Input/output 3		Input/output 4 ¹⁾		Service interface (Port 2)
1 (+)	2 (-)	26 (B)	27 (A)	24 (+)	25 (-)	22 (+)	23 (-)	20 (+)	21 (-)	CDI-RJ45
The terminal assignment depends on the specific device version ordered →  13.										

1) Input/output only available for Proline 500 - digital.

Modbus TCP

Supply voltage		Input/output 1 (Port 1 ¹⁾)		Input/output 2		Input/output 3		Input/output 4 ²⁾		Service interface (Port 2) ¹⁾
1 (+)	2 (-)	26 (+)	27 (-)	24 (+)	25 (-)	22 (+)	23 (-)	20 (+)	21 (-)	CDI-RJ45
The terminal assignment depends on the specific device version ordered →  13.										

1) For Modbus TCP communication, either port 1 OR port 2 can be used.

2) Input/output only available for Proline 500 - digital.

PROFINET over Ethernet-APL

Supply voltage		Input/output 1 (Port 1)		Input/output 2		Input/output 3		Input/output 4 ¹⁾		Service interface (Port 2 ²⁾)
1 (+)	2 (-)	26 (+)	27 (-)	24 (+)	25 (-)	22 (+)	23 (-)	20 (+)	21 (-)	CDI-RJ45
The terminal assignment depends on the specific device version ordered →  13.										

1) Input/output only available for Proline 500 - digital.

2) No PROFINET communication available on port 2

Transmitter and sensor connection housing: connecting cable

The sensor and transmitter, which are mounted in separate locations, are interconnected by a connecting cable. The cable is connected via the sensor connection housing and the transmitter housing.

Terminal assignment and connection of the connecting cable:

Proline 500 – digital →  28

Available device plugs
Proline 500
Device plugs for Proline 500:

Order code for "Input; output 1"

- Option **RB** "PROFINET over Ethernet-APL" → 25
- Option **MB** "Modbus TCP" → 25

Device plug for connecting to the service interface:

Order code for "Accessory mounted"

 Option **NB**, RJ45 M12 adapter (service interface) → 27

Order code for "Input; output 1", option RB "PROFINET over Ethernet-APL"

Order code for "Electrical connection"	Cable entry/connection → 29	
	2	3
L, N, P, U	Connector M12×1	–

Order code for "Input; output 1", option MB "Modbus TCP over Ethernet-APL"

Order code for "Electrical connection"	Accessories	Cable entry/connection → 29	
		2	3
L, N, P, U	–	Connector M12×1 A-coded	–
L, N, P, U	NB ¹⁾	Connector M12×1 A-coded	Connector M12×1 ¹⁾ D-coded
1 ²⁾ , 2 ²⁾ , 7 ²⁾ , 8 ²⁾	–	–	Connector M12×1 D-coded

1) Cannot be used as a Modbus TCP port.

2) Not compatible with an external WLAN antenna (order code for "Accessory enclosed", option P8, an RJ45 M12 adapter for the service interface (order code for "Accessory mounted", option NB)

Order code for "Accessory mounted", option NB: "Adapter RJ45 M12 (service interface)"

Order code for "Accessory mounted"	Cable entry/connection → 29	
	Cable entry 2	Cable entry 3
NB ¹⁾	–	Connector M12×1

1) Not compatible with electrical connection option 1, 2, 7, 8

Available device plugs
Proline 500 digital
Device plugs for Proline 500 digital:

Order code for "Input; output 1"

- Option **RB** "PROFINET over Ethernet-APL" → 25
- Option **MB** "Modbus TCP over Ethernet-APL"

Device plug for connecting to the service interface:

Order code for "Accessory mounted"

 Option **NB**, RJ45 M12 adapter (service interface) → 27

Order code for "Input; output 1", option RB "PROFINET over Ethernet-APL"

Order code for "Electrical connection"	Cable entry/connection → 29			
	2	3	4	5
L, N, P, U	–	Connector M12×1 A-coded	–	–

Order code for "Input; output 1", option MB "Modbus TCP over Ethernet-APL"

Order code for "Electrical connection"	Accessories	Cable entry/connection → 29			
		2	3	4	5
L, N, P, U	-	-	Connector M12×1 A-coded	-	-
L, N, P, U	NB ¹⁾	-	Connector M12×1 A-coded	-	Connector M12×1 ¹⁾ D-coded
1 ²⁾ , 2 ²⁾ , 7 ²⁾ , 8 ²⁾	-	-	-	-	Connector M12×1 D-coded


- 1) Cannot be used as a Modbus TCP port.
 2) Not compatible with an external WLAN antenna (order code for "Accessory enclosed", option P8, an RJ45 M12 adapter for the service interface (order code for "Accessory mounted", option NB)

Order code for "Accessory mounted", option NB: "Adapter RJ45 M12 (service interface)"

Order code for "Electrical connection"	Cable entry/connection → 29			
	2	3	4	5
NB ¹⁾	-	-	-	M12x1 plug D-coded

- 1) Not compatible with electrical connection option 1, 2, 7, 8

Pin assignment, device plug**PROFINET over Ethernet-APL /SPE**


	Pin	Assignment	Coding	Plug/socket
	1	APL signal -	A	Socket
	2	APL signal +		
	3	Cable shield ¹⁾		
	4	Not used		
	Metal plug housing	Cable shield		
¹⁾ If a cable shield is used				



Recommended plug:

- Binder, series 713, part no. 99 1430 814 04
- Phoenix, part no. 1413934 SACC-FS-4QO SH PBPA SCO


Modbus TCP over Ethernet-APL 10 Mbit/s

	Pin	Assignment	Coding	Plug/socket
	1	APL signal -	A	Socket
	2	APL signal +		
	3	Cable shield ¹⁾		
	4	Not used		
	Metal plug housing	Cable shield		
¹⁾ If a cable shield is used				




- Recommended plug:
- Binder, series 713, part no. 99 1430 814 04
 - Phoenix, part no. 1413934 SACC-FS-4QO SH PBPA SCO

Modbus TCP over Ethernet 100 Mbit/s

 A0032047	Pin	Assignment		Coding	Plug/socket
	1	+	Tx	D	Socket
	2	+	Rx		
	3	-	Tx		
	4	-	Rx		

Service interface for

Order code for "Accessories mounted", option **NB**: Adapter RJ45 M12 (service interface)

 A0032047	Pin	Assignment		Coding	Plug/socket
	1	+	Tx	D	Socket
	2	+	Rx		
	3	-	Tx		
	4	-	Rx		



- Recommended plug:
- Binder, series 825, part no. 99 3729 810 04
 - Phoenix, part no. 1543223 SACC-M12MSD-4Q

Supply voltage	Order code for "Power supply"	Terminal voltage		Frequency range
	Option I	DC 24 V	±20%	–
		AC 100 to 240 V	–15 to 10%	50/60 Hz

Power consumption	Transmitter	
	Max. 10 W (active power)	
	switch-on current	Max. 36 A (<5 ms) as per NAMUR Recommendation NE 21


Current consumption	Transmitter	
	■ Max. 400 mA (24 V) ■ Max. 200 mA (110 V, 50/60 Hz; 230 V, 50/60 Hz)	

Power supply failure	■ Totalizers stop at the last value measured. ■ Depending on the device version, the configuration is retained in the device memory or in the plug-in memory (HistoROM DAT). ■ Error messages (incl. total operated hours) are stored.	
----------------------	--	--

Overcurrent protection element	The device must be operated with a dedicated circuit breaker, as it does not have an ON/OFF switch of its own.	
	■ The circuit breaker must be easy to reach and labeled accordingly. ■ Permitted nominal current of the circuit breaker: 2 A up to maximum 10 A.	

Electrical connection


Connection of connecting cable: Proline 500 – digital

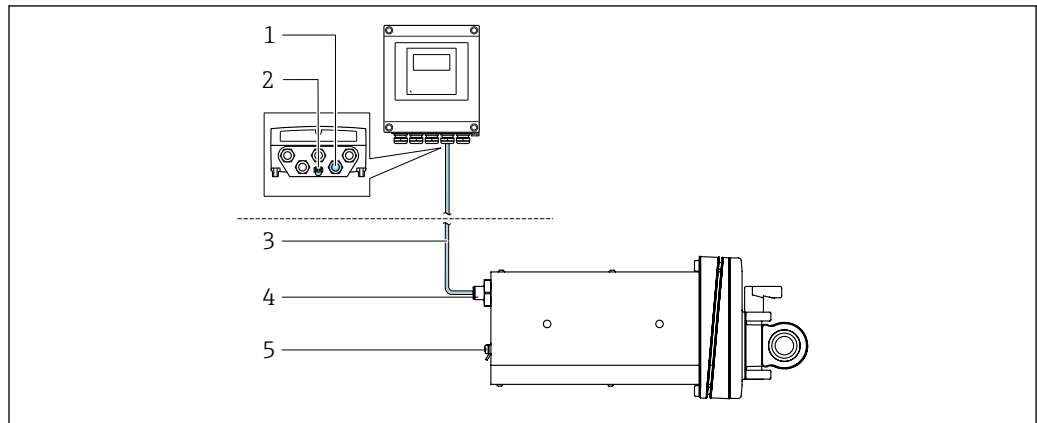

A0053068

1 Order code for "Device version", option NA "Front panel mounting"

- 1 M12 socket for connecting the connecting cable on the transmitter housing
- 2 Terminal connection for potential equalization (PE)
- 3 Connecting cable with M12 plug and M12 socket
- 4 M12 plug for connecting the connecting cable on the sensor
- 5 Terminal connection for potential equalization (PE)

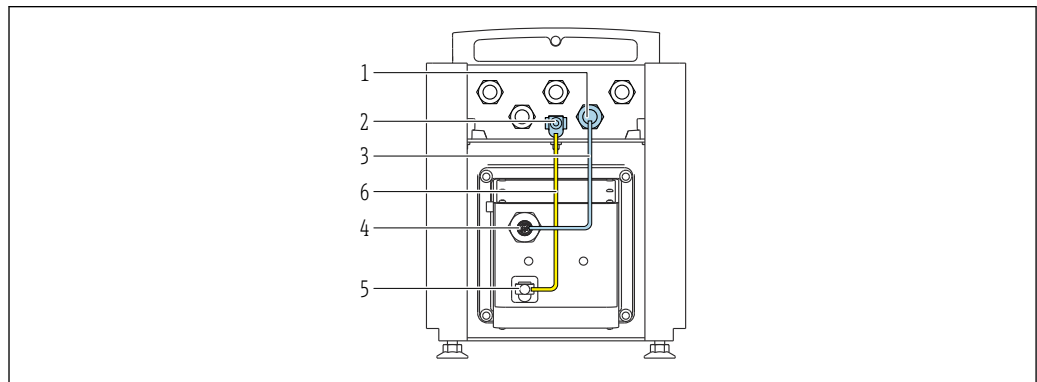


A0053744

2 Order code for "Device version", option NE "Table version"

- 1 M12 socket for connecting the connecting cable on the transmitter housing
- 2 Terminal connection for potential equalization (PE)
- 3 Connecting cable with M12 plug and M12 socket
- 4 M12 plug for connecting the connecting cable on the sensor
- 5 Terminal connection for potential equalization (PE)
- 6 Fixed connection between the potential equalization (PE)

Pin assignment, device plug

Connection at transmitter


	Pin	Color ¹⁾	Assignment		Connection to terminal
	1	Brown	+	Supply voltage	61
	2	White	-		62
	3	Blue	A	ISEM communication	64
	4	Black	B		63
	5	-		-	-

A0053073

	Coding	Plug/socket
	A	Socket

1) Cable colors of connecting cable

Connection on sensor


	Pin	Color ¹⁾	Assignment	
	1	Brown	+	Supply voltage
	2	White	-	
	3	Blue	A	ISEM communication
	4	Black	B	
	5	-		-
Coding			Plug/socket	
A			Plug	

1) Cable colors of connecting cable

Transmitter connection

- Terminal assignment → 24
- Device plug pin assignment → 26

Transmitter connection: Proline 500 – digital

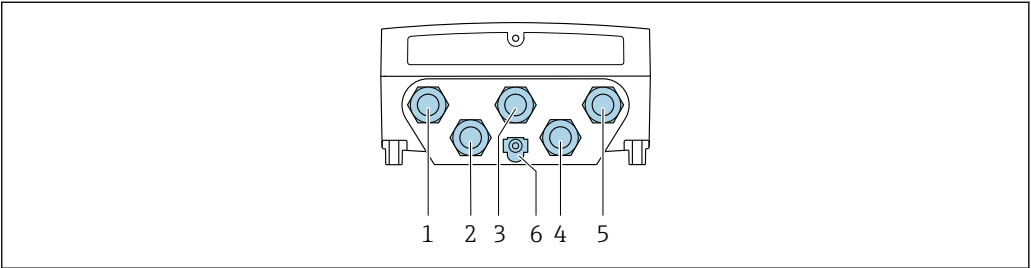

A0028200

- 1 Terminal connection for supply voltage
- 2 Terminal connection for signal transmission, input/output
- 3 Terminal connection for signal transmission, input/output
- 4 Terminal connection for connecting cable between sensor and transmitter
- 5 Terminal connection for signal transmission, input/output; optional: connection for external WLAN antenna
- 6 Terminal connection for potential equalization (PE)


- An adapter for the RJ45 to the M12 plug is optionally available:
Order code for "Accessories", option **NB**: "Adapter RJ45 M12 (service interface)"

The adapter connects the service interface (CDI-RJ45) to an M12 plug mounted in the cable entry. The connection to the service interface can thus be established via an M12 plug without opening the device.

- Network connection (DHCP client) via service interface (CDI-RJ45) → 53


Connection examples

Current output 4 to 20 mA (without HART)

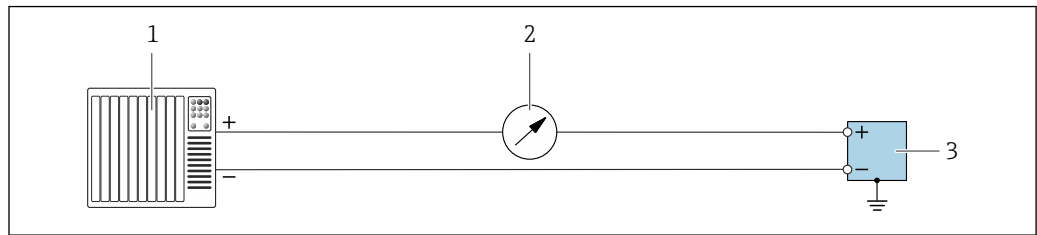

3 Connection example for 4 to 20 mA current output (active)


- 1 Automation system with current input (e.g. PLC)
- 2 Optional additional display unit: Observe maximum load
- 3 Flowmeter with current output (active)

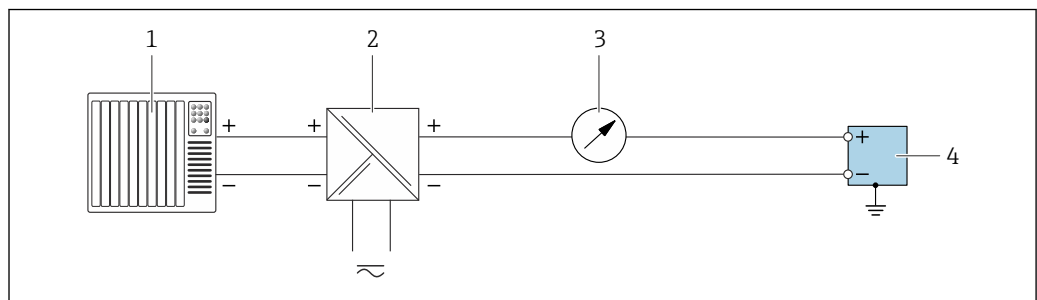

4 Connection example for 4 to 20 mA current output (passive)

- 1 Automation system with current input (e.g. PLC)
- 2 Power supply
- 3 Optional additional display unit: Observe maximum load
- 4 Transmitter with current output (passive)


Current input 4 to 20 mA

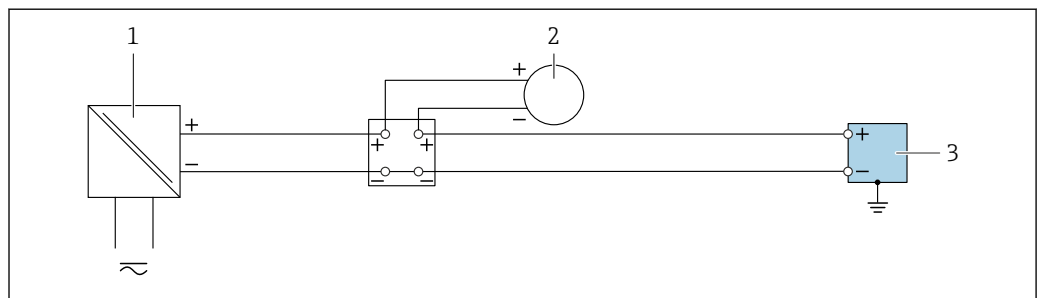

5 Connection example for 4 to 20 mA current input

- 1 Power supply
- 2 External measuring instrument with 4 to 20 mA passive current output. e.g. pressure or temperature)
- 3 Transmitter with 4 to 20 mA current input


Pulse output/frequency output/switch output

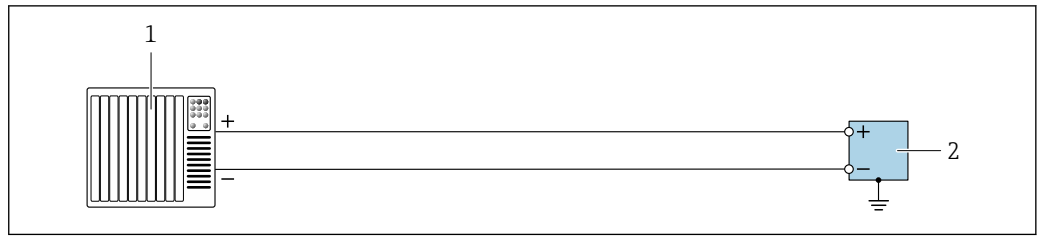

A0055856

6 Connection example for pulse output/frequency output/switch output (active)

- 1 Automation system with pulse input/frequency input/switch input (e.g. PLC)
- 2 Transmitter with pulse output/frequency output/switch output (active)

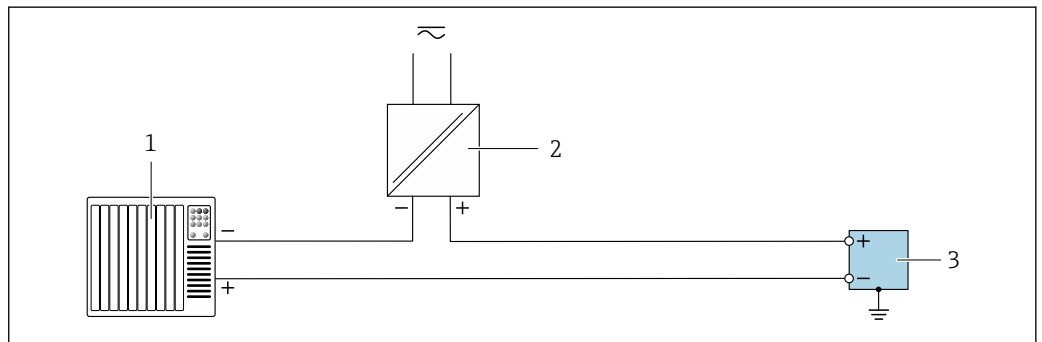


A0055856

7 Connection example for pulse output/frequency output/switch output (passive)

- 1 Automation system with pulse input/frequency input/switch input (e.g. PLC)
- 2 Power supply
- 3 Transmitter with pulse output/frequency output/switch output (passive)

Relay output

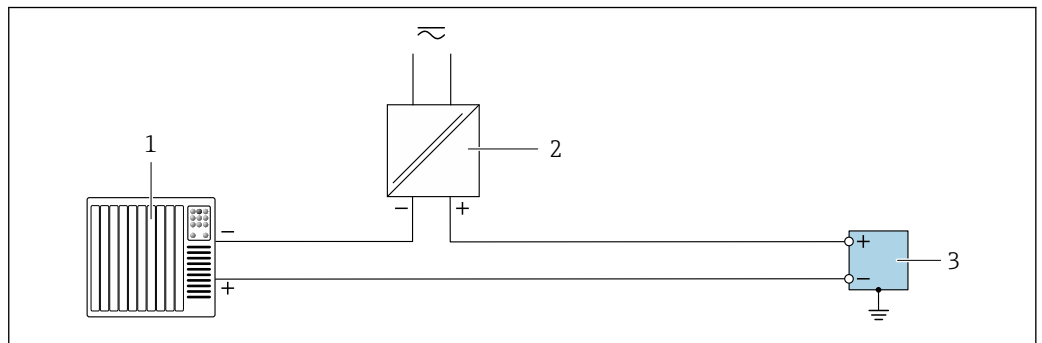


A0055859

8 Connection example for relay output

- 1 Automation system with switch input (e.g. PLC)
- 2 Power supply
- 3 Transmitter with relay output

Status input

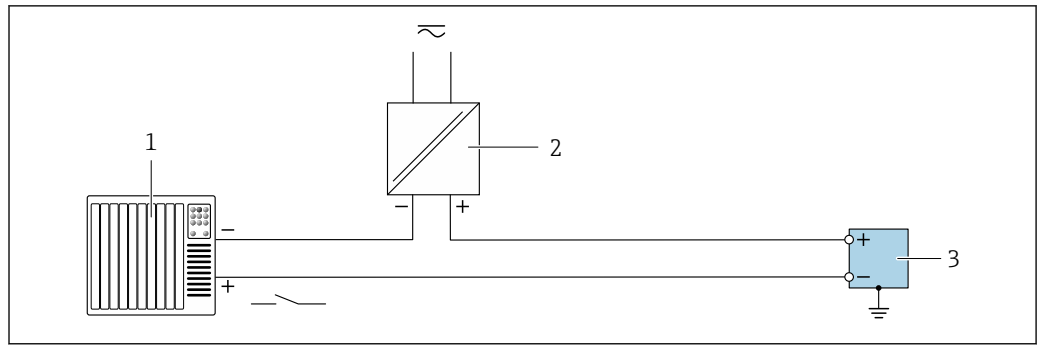


A0055860

9 Connection example for status input

- 1 Automation system with switch output passive e.g. PLC)
- 2 Power supply
- 3 Transmitter with status input

Modbus RS485

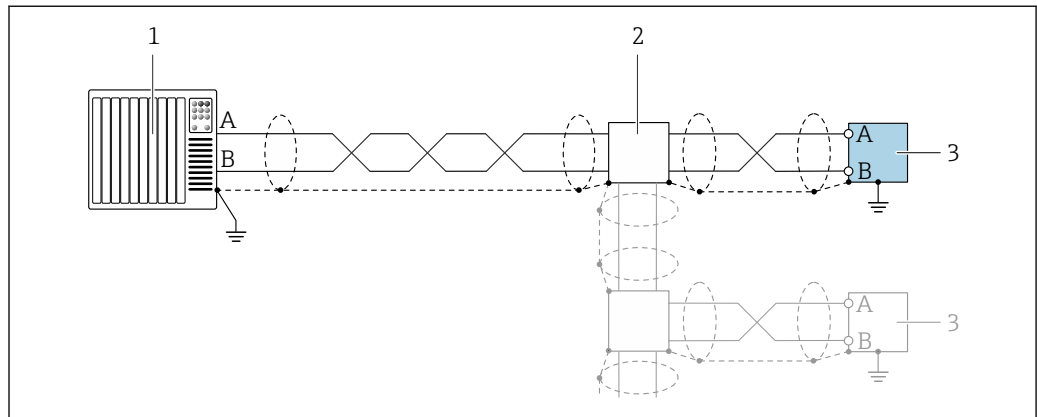

A0055863

10 Connection example for Modbus RS485

- 1 Automation system with Modbus master (e.g. PLC)
- 2 Optional distribution box
- 3 Transmitter with Modbus RS485

Ethernet-APL

See <https://www.profibus.com> Ethernet-APL White Paper "

Potential equalization

Requirements

For potential equalization:

- Pay attention to in-house grounding concepts
- Take account of operating conditions, such as the pipe material and grounding
- Connect the medium, sensor and transmitter to the same electric potential
- For the "device version" order code NE "table top" option, the sensor and transmitter are internally wired
- Use a ground cable with a minimum cross-section of 6 mm² (10 AWG) and a cable lug for potential equalization connections

Terminals

Spring-loaded terminals: Suitable for strands and strands with ferrules.
Conductor cross-section 0.2 to 2.5 mm² (24 to 12 AWG).

Cable entries

- Cable gland: M20 × 1.5 with cable Ø 6 to 12 mm (0.24 to 0.47 in)
- Thread for cable entry:
 - NPT ½"
 - G ½"
 - M20

Cable specification**Permitted temperature range**

- The installation guidelines that apply in the country of installation must be observed.
- The cables must be suitable for the minimum and maximum temperatures to be expected.

Power supply cable (incl. conductor for the inner ground terminal)

Standard installation cable is sufficient.

Protective grounding cable for the outer ground terminal

Conductor cross-section < 6 mm² (10 AWG)

The use of a cable lug enables the connection of larger cross-sections.

The grounding impedance must be less than 2 Ω.

Signal cable

4 to 20 mA current input

Standard installation cable is sufficient.

Pulse/frequency/switch output

Standard installation cable is sufficient.

Relay output

Standard installation cable is sufficient.

Status input

Standard installation cable is sufficient.

Modbus RS485

Shielded twisted-pair cable.

 See <https://modbus.org> "MODBUS over Serial Line Specification and Implementation Guide".

Ethernet-APL

Shielded twisted-pair cable. Cable type A is recommended.

 See <https://www.profibus.com> Ethernet-APL White Paper "

Choice of connecting cable between the transmitter and sensor

A: Connecting cable between sensor and transmitter: Proline 500 – digital

Standard cable

A standard cable with the following specifications can be used as the connecting cable.

Design	2x2 cores (twisted pairs); stranded CU wires with common shield
Shield	Tin-plated copper braid, optical cover ≥ 85 %
Loop resistance	Power supply line (+, -): maximum 10 Ω
Cable length	Maximum 300 m (900 ft), see the following table.
Device plug, side 1	M12 socket, 5-pin, A-coded.
Device plug, side 2	M12 plug, 5-pin, A-coded.

Pins 1+2	Connected cores as twisted pair.
Pins 3+4	Connected cores as twisted pair.

Cross-section	Cable length [max.]
0.34 mm ² (AWG 22)	80 m (240 ft)
0.50 mm ² (AWG 20)	120 m (360 ft)
0.75 mm ² (AWG 18)	180 m (540 ft)
1.00 mm ² (AWG 17)	240 m (720 ft)
1.50 mm ² (AWG 15)	300 m (900 ft)

connecting cable

Design	2 × 2 × 0.34 mm ² PUR cable with common shield
Flame resistance	According to DIN EN 60332-1-2 (60 seconds)
Oil resistance	According to DIN EN 60811-2-1 (for 168h at 90°C)
Shield	Tin-plated copper braid
Continuous operating temperature	When mounted in a fixed position: -40 to +105 °C (-40 to +221 °F); when cable can move freely: -25 to +105 °C (-13 to +221 °F)
Available cable lengths	Fixed: 2 m (6 ft), 5 m (15 ft), 10 m (30 ft)
Device plug, side 1	M12 socket, 5-pin, A-coded
Device plug, side 2	M12 plug, 5-pin, A-coded

Overvoltage protection

Mains voltage fluctuations	→  27
Overvoltage category	Overvoltage category II
Short-term, temporary overvoltage	Between cable and ground up to 1200 V, for max. 5 s
Long-term, temporary overvoltage	Between cable and ground up to 500 V

Performance characteristics

Reference operating conditions

- Error limits based on ISO 11631
 - Water
 - +15 to +45 °C (+59 to +113 °F)
 - 2 to 6 bar (29 to 87 psi)
 - Data as indicated in the calibration protocol
 - Accuracy based on accredited calibration rigs according to ISO 17025
-  To obtain measured errors, use the *Applicator* sizing tool →  60

Maximum measurement error

o.r. = of reading; 1 g/cm³ = 1 kg/l; T = medium temperature

 In non-condensing environment.

Base accuracy

 Design fundamentals →  36

Mass flow and volume flow (liquids)

±0.5 % o.r.

Temperature $\pm 2.5\text{ °C}$ ($\pm 4.5\text{ °F}$)**Zero point stability**

DN		Zero point stability	
[mm]	[in]	[kg/min]	[lb/min]
4	$\frac{1}{8}$	0.0006	0.00132
6	$\frac{1}{4}$	0.0023	0.00507
15	$\frac{1}{2}$	0.0082	0.01808
25	1	0.0227	0.05004

Flow values

Flow values as turndown parameters depending on nominal diameter.

SI units

DN	1:1	1:10	1:20	1:50	1:100	1:500
[mm]	[kg/h]	[kg/h]	[kg/h]	[kg/h]	[kg/h]	[kg/h]
4	450	45	22.5	9	4.5	0.9
6	1 000	100	50	20	10	2
15	6 500	650	325	130	65	13
25	18 000	1 800	900	360	180	36

US units

DN	1:1	1:10	1:20	1:50	1:100	1:500
[inch]	[lb/min]	[lb/min]	[lb/min]	[lb/min]	[lb/min]	[lb/min]
$\frac{1}{8}$	16.54	1.654	0.827	0.331	0.165	0.033
$\frac{1}{4}$	36.75	3.675	1.838	0.735	0.368	0.074
$\frac{1}{2}$	238.9	23.89	11.95	4.778	2.389	0.478
1	661.5	66.15	33.08	13.23	6.615	1.323

Accuracy of outputs

The outputs have the following base accuracy specifications.

Current output

Accuracy	$\pm 5\text{ }\mu\text{A}$
-----------------	----------------------------

Pulse/frequency output

o.r. = of reading

Accuracy	Max. $\pm 50\text{ ppm}$ o.r. (over the entire ambient temperature range)
-----------------	---

Repeatabilityo.r. = of reading; $1\text{ g/cm}^3 = 1\text{ kg/l}$; T = medium temperature

Base repeatability

Design fundamentals → 36

Mass flow and volume flow (liquids) $\pm 0.25\%$ o.r.*Density (liquids)*

■ Basic accuracy:

 $\pm 0.01\text{ g/cm}^3$

■ Repeatability:

 $\pm 0.005\text{ g/cm}^3$ *Temperature* $\pm 0.125\text{ °C}$ ($\pm 0.225\text{ °F}$)**Response time**

The response time depends on the configuration (damping).

Influence of ambient temperature**Current output**

Temperature coefficient	Max. $1\text{ }\mu\text{A/°C}$
--------------------------------	--------------------------------

Pulse/frequency output

Temperature coefficient	No additional effect. Included in accuracy.
--------------------------------	---

Influence of medium temperature**Mass flow**

o.f.s. = of full scale value

If there is a difference between the temperature during zero adjustment and the process temperature, the additional measurement error of the sensors is typically $\pm 0.0002\%$ o.f.s./°C ($\pm 0.0001\%$ o. f.s./°F).

The influence is reduced when the zero adjustment is performed at process temperature.

Density

Density performance is identical across the entire temperature range.

Temperature $\pm 0.005 \cdot T\text{ °C}$ ($\pm 0.005 \cdot (T - 32)\text{ °F}$)**Influence of medium pressure**

A difference between the calibration pressure and process pressure does not affect measurement accuracy.



A pressure of $>0.2\text{ bar}$ is required for an accurate measurement. Pressures lower than this can lead to incorrect measurement results due to cavitation and the formation of air bubbles.

Design fundamentals

o.r. = of reading, o.f.s. = of full scale value

BaseAccu = base accuracy in % o.r., BaseRepeat = base repeatability in % o.r.

MeasValue = measured value; ZeroPoint = zero point stability

Calculation of the maximum measured error as a function of the flow rate

Flow rate	Maximum measured error in % o.r.
$\geq \frac{\text{ZeroPoint}}{\text{BaseAccu}} \cdot 100$ A0021332	$\pm \text{BaseAccu}$ A0021339
$< \frac{\text{ZeroPoint}}{\text{BaseAccu}} \cdot 100$ A0021333	$\pm \frac{\text{ZeroPoint}}{\text{MeasValue}} \cdot 100$ A0021334


Calculation of the maximum repeatability as a function of the flow rate

Flow rate	Maximum repeatability in % o.r.
$\geq \frac{\frac{1}{2} \cdot \text{ZeroPoint}}{\text{BaseRepeat}} \cdot 100$ A0021335	$\pm \text{BaseRepeat}$ A0021340
$< \frac{\frac{1}{2} \cdot \text{ZeroPoint}}{\text{BaseRepeat}} \cdot 100$ A0021336	$\pm \frac{1}{2} \cdot \frac{\text{ZeroPoint}}{\text{MeasValue}} \cdot 100$ A0021337

Installation


Installation point

Front panel mounting

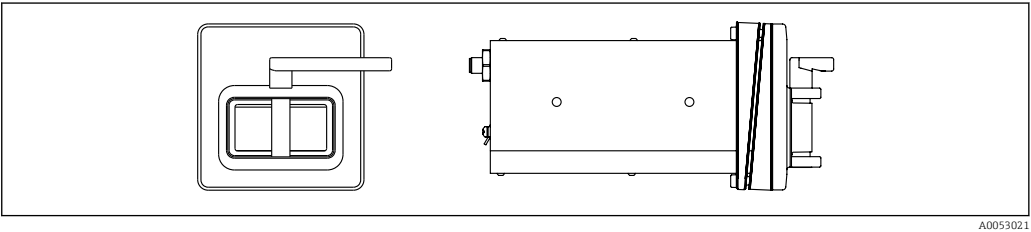

11 Order code for "Device version", option NA "Front panel mounting"



Table version

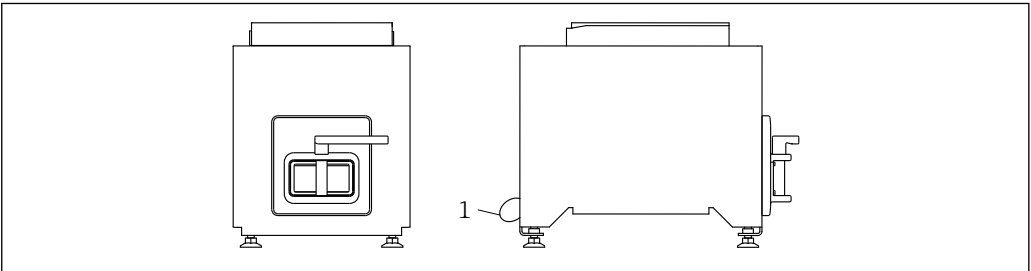

12 Order code for "Device version", option NE "Table version"

1 Secure the device to the table with the supplied cable through the hole on the back.

Orientation

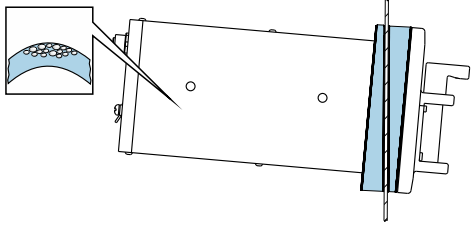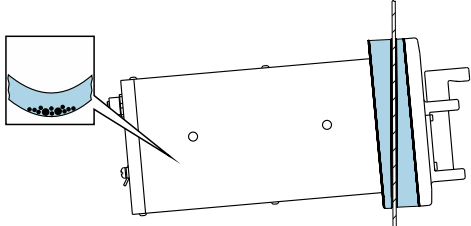Orientation	
Wedge pointing upwards  Gas accumulation in the measuring tube possible. Self-draining.	
Wedge pointing downwards Recommended orientation  Solids accumulation in the measuring tube possible.	

Inlet and outlet runs

No special precautions need to be taken for fittings that create turbulence, such as valves, elbows or T-pieces, as long as no cavitation occurs →  41.


Installing the transmitter housing

Proline 500 – digital transmitter

Wall mounting

Required tools:

Drill with drill bit $\varnothing$ 6.0 mm

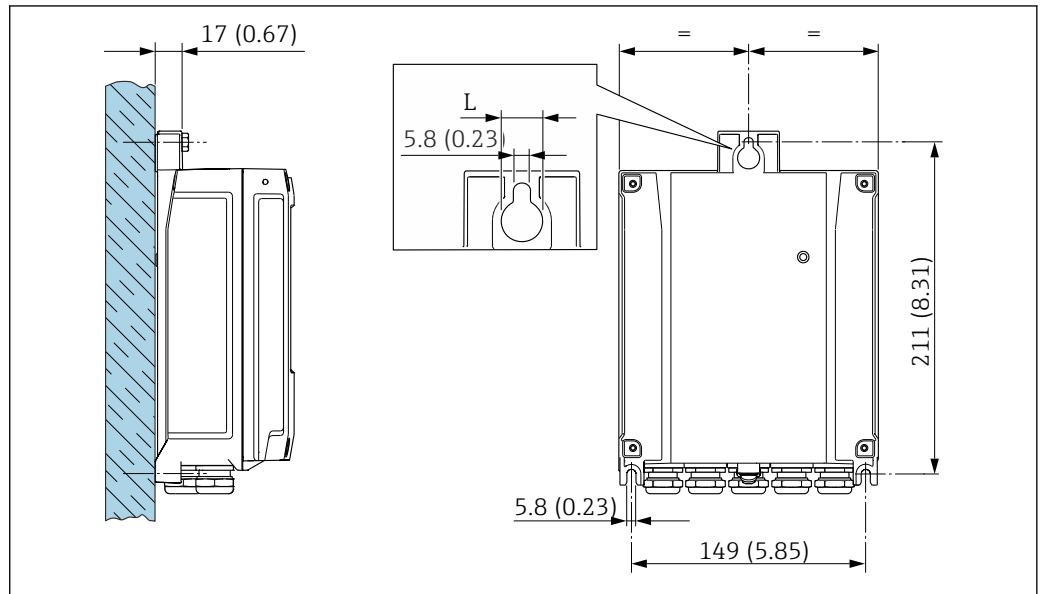

13 Unit mm (in)

L Depends on order code for "Transmitter housing"

Order code for "Transmitter housing"

Option **A**, aluminum, coated: $L = 14$ mm (0.55 in)

Special installation instructions

Drainability

When installed with the wedge pointing upwards, the measuring tubes can be drained completely and protected against buildup.

Sterility



When installing in sterile applications, please refer to the information in the "Certificates and approvals/sterility" section → 56

Biotech



When installing in biotech applications, please refer to the information in the "Certificates and approvals/biotech" section → 56

Zero point verification and zero adjustment

All measuring instruments are calibrated in accordance with state-of-the-art technology. Calibration takes place under reference conditions → 34.

Important parameters such as the calibration factor of the disposable measuring tube and other device information determined during factory calibration must remain unchanged. A zero adjustment of the mounted measuring instrument filled with liquid is required for commissioning to offset the sensor's manufacturing tolerances.

This results in an updated zero point that deviates from the original zero point indicated on the factory calibration certificate and is then documented on the Heartbeat Technology verification report.

For information on checking the zero point and performing a zero adjustment, see the Operating Instructions for the device.



To achieve the highest possible measurement accuracy at low flow rates, the installation must protect the sensor from mechanical stress during operation.

Environment

Ambient temperature range	Measuring instrument	+5 to +40 °C (+41 to +104 °F)
	Readability of the local display	–20 to +60 °C (–4 to +140 °F) The readability of the display may be impaired at temperatures outside the temperature range.



Dependency of ambient temperature on medium temperature → 41

Storage temperature	–40 to +70 °C (–40 to +158 °F)
Shelf life	Disposable measuring tube ■ Maximum 5 years pre-gamma ■ Maximum 2 years post-gamma
Climate class	DIN EN 60068-2-38 (test Z/AD)
Relative humidity	The device is suitable for use in indoor areas with a relative humidity of 5 to 40%.
Operating height	According to EN 61010-1 ■ ≤ 2 000 m (6 562 ft) ■ > 2 000 m (6 562 ft) with additional overvoltage protection (e.g. Endress+Hauser HAW Series)
Degree of protection	Transmitter ■ IP66/67, Type 4X enclosure, suitable for pollution degree 4 ■ When the housing is open: IP20, Type 1 enclosure, suitable for pollution degree 2 ■ Display module: IP20, Type 1 enclosure, suitable for pollution degree 2 Sensor ■ IP54 ■ When the housing is open: IP20 External WLAN antenna IP66/67, type 4X enclosure
Vibration-resistance and shock-resistance	Vibration sinusoidal, in accordance with IEC 60068-2-6 Sensor ■ 2 to 8.4 Hz, 3.5 mm peak ■ 8.4 to 2 000 Hz, 1 g peak Transmitter ■ 2 to 8.4 Hz, 7.5 mm peak ■ 8.4 to 2 000 Hz, 2 g peak Vibration broad-band random, according to IEC 60068-2-64 Transmitter ■ 10 to 200 Hz, 0.01 g²/Hz ■ 200 to 2 000 Hz, 0.003 g²/Hz ■ Total: 2.70 g rms Shock half-sine, according to IEC 60068-2-27 Transmitter 6 ms 50 g Rough handling shocks according to IEC 60068-2-31

Mechanical load	Transmitter housing, sensor and disposable measuring tube: ■ Protect against mechanical effects, such as shock or impact ■ Do not use as a ladder or climbing aid
Electromagnetic compatibility (EMC)	■ As per IEC/EN 61326 and NAMUR Recommendation 21 (NE 21), NAMUR Recommendation 21 (NE 21) is fulfilled when the device is installed in accordance with NAMUR Recommendation 98 (NE 98). ■ As per IEC/EN 61000-6-2 and IEC/EN 61000-6-4  Details are provided in the Declaration of Conformity.  This unit is not intended for use in residential environments and cannot guarantee adequate protection of the radio reception in such environments.


Process

Medium temperature range	3 to 60 °C (37.4 to 140 °F)
Medium density	800 to 1 500 kg/m ³ (1 764 to 3 307 lb/cf)
Medium pressure	6 bar (87 psi)
Flow limit	Select the nominal diameter by optimizing between the required flow range and permissible pressure loss.  For an overview of the full scale values for the measuring range, see the "Measuring range" section →  11 ■ The minimum recommended full scale value is approx. 1/20 of the maximum full scale value ■ For the most common applications, 20 to 50 % of the maximum full scale value can be considered ideal ■ A low full scale value must be selected for abrasive media (such as liquids with entrained solids): flow velocity < 1 m/s (< 3 ft/s).  To calculate the flow limit, use the <i>Applicator</i> sizing tool →  60
Pressure loss	 To calculate the pressure loss, use the <i>Applicator</i> sizing tool →  60
Static pressure	It is important that cavitation does not occur, or that gases entrained in the liquids do not outgas. This is prevented by means of a sufficiently high static pressure. For this reason, the following mounting locations are recommended: Downstream from pumps (no danger of vacuum)
Vibrations	The operational reliability of the measuring system is not affected by plant vibrations.

Mechanical construction

Dimensions in SI units

Housing of Proline 500 – digital transmitter

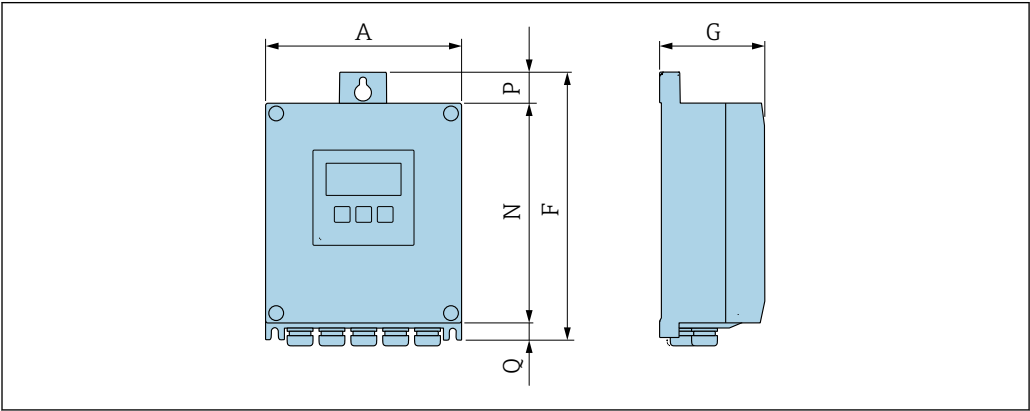


A0033789

Order code for "Transmitter housing", option A "Aluminum, coated" and order code for "Integrated ISEM electronics", option A "Sensor"

A [mm]	F [mm]	G [mm]	N [mm]	P [mm]	Q [mm]
167	232	89	187	24	21

Sensor

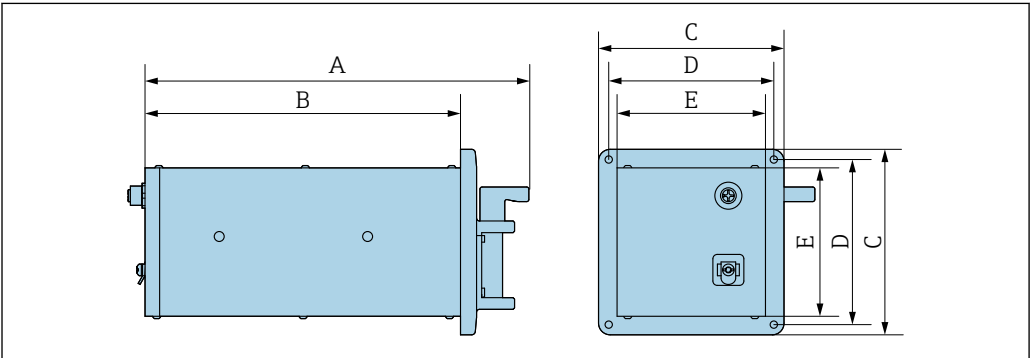


A0053039

Order code for "Device version", option NA "Front panel mounting"

A [mm]	B [mm]	C [mm]	D [mm]	E [mm]
263	216	127	113	101.6

Table version

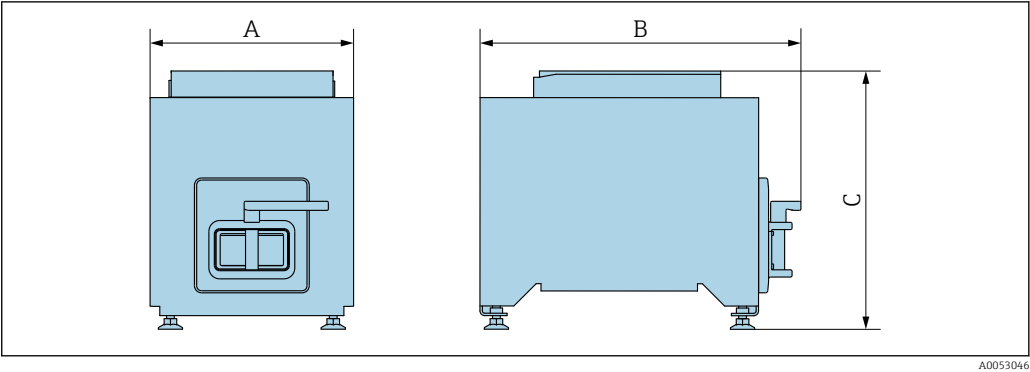


Order code for "Device version", option NE "Table version"

A [mm]	B [mm]	C [mm]
210	345	267


Accessories

Disposable measuring tube

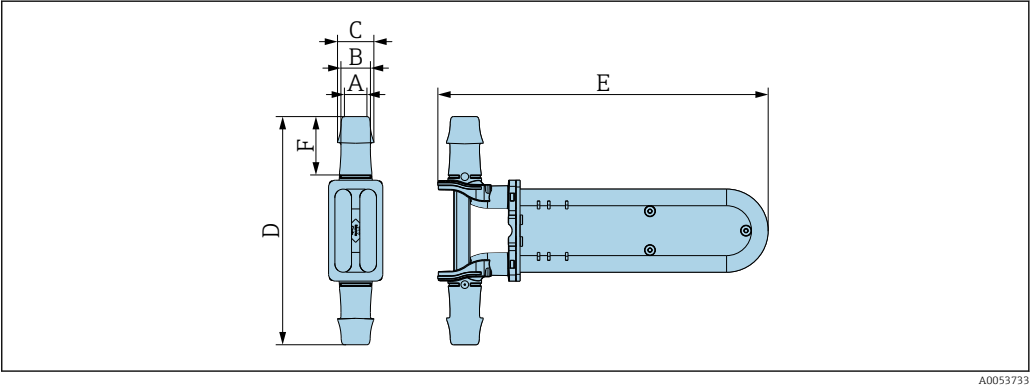

Unpacked

Nominal diameter [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	F [mm]	Dead volume [ml]
4	3	3.8	4.7	95	247	6.4	19
6	5.3	6.4	8.5	111	247	17	21
15	9	11.6	15.5	145	250	29.8	73
25	17.5	21.4	28.4	179	259	50	132

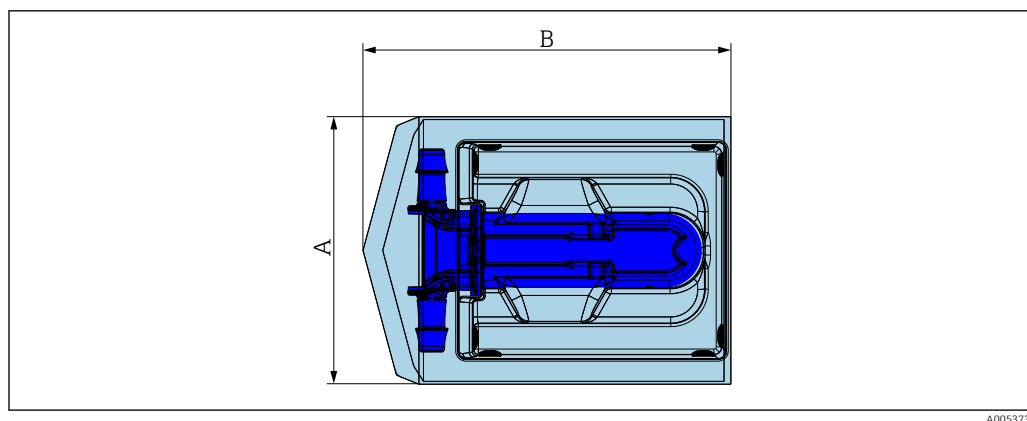


A0053734

Packed

Nominal diameter [mm]	A [mm]	B [mm]
4	275	305
6	275	305
15	275	305
25	275	305

External WLAN antenna

The external WLAN antenna is not suitable for use in hygienic applications.

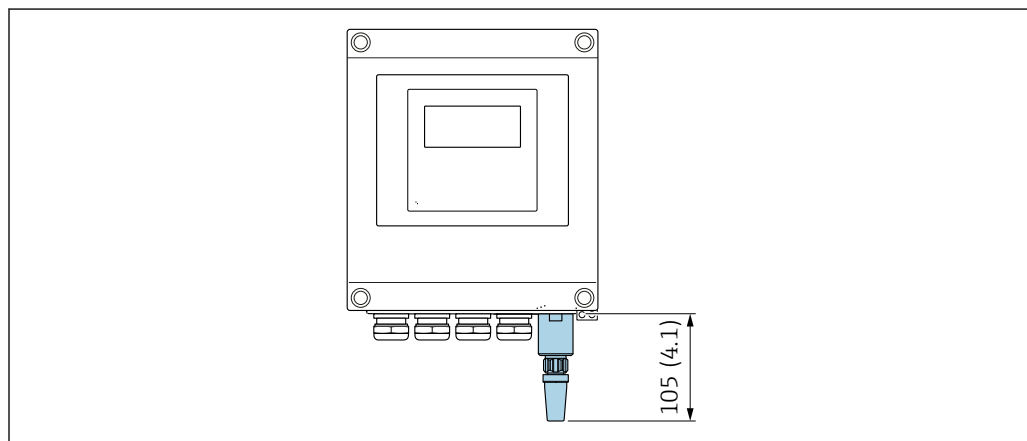
*Proline 500 – digital**External WLAN antenna mounted on device*

A0033607

14 Unit mm (in)

External WLAN antenna mounted with cable

The external WLAN antenna can be mounted separately from the transmitter if the transmission/reception conditions at the transmitter mounting location are poor.

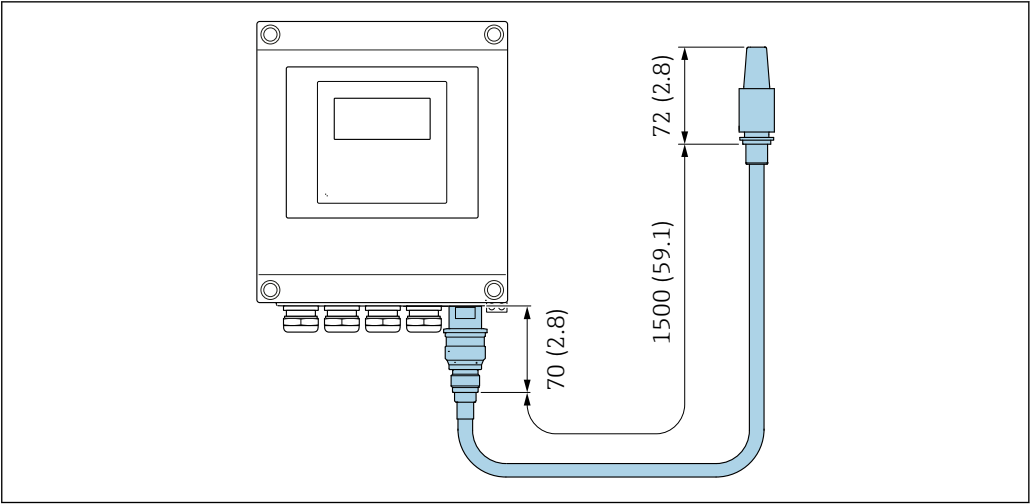


A0033606

15 Unit mm (in)

Dimensions in US units

Housing of Proline 500 – digital transmitter

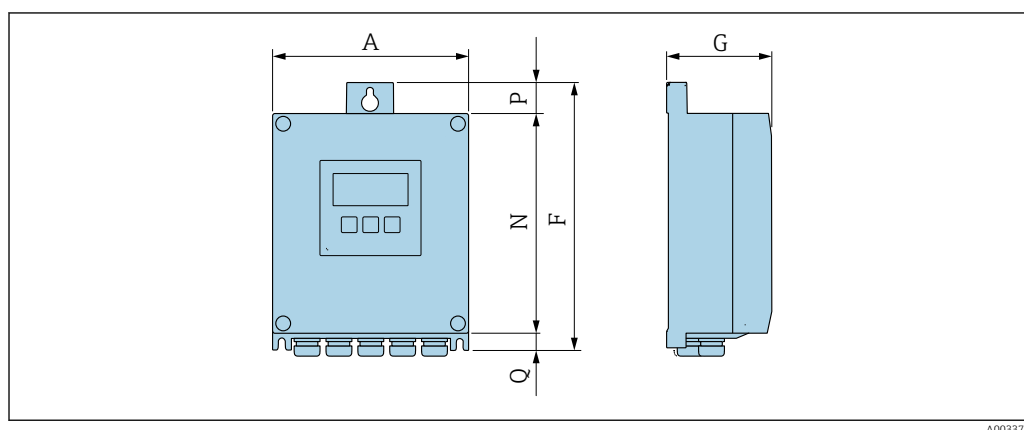


A0033789

Order code for "Transmitter housing", option A "Aluminum, coated" and order code for "Integrated ISEM electronics", option A "Sensor"

A [in]	F [in]	G [in]	N [in]	P [in]	Q [in]
6.57	9.13	3.50	7.36	0.94	0.83

Sensor

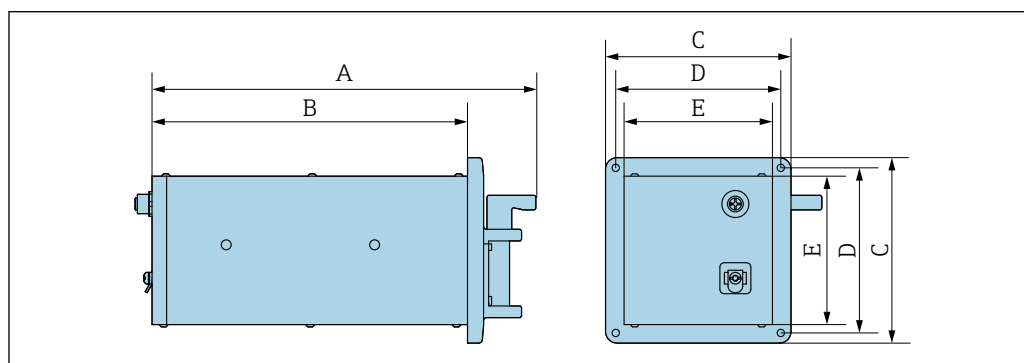


A0053039

Order code for "Device version", option NA "Front panel mounting"

A [in]	B [in]	C [in]	D [in]	E [in]
10.35	8.5	5	4.45	4

Table version

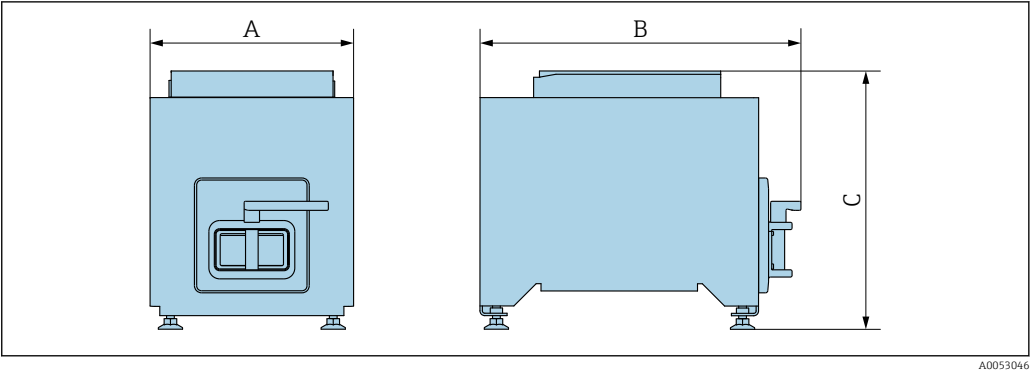


Order code for "Device version", option NE "Table version"

A [in]	B [in]	C [in]
8.27	13.58	10.51


Accessories

Disposable measuring tube

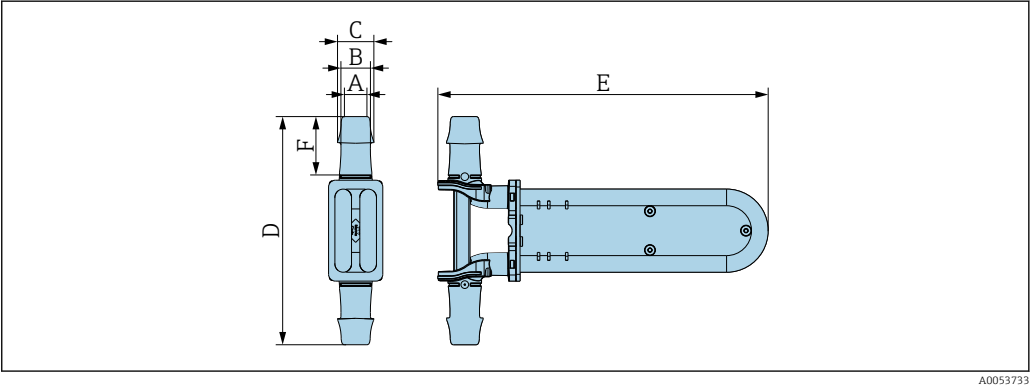

Unpacked

Nominal diameter [in]	A [in]	B [in]	C [in]	D [in]	E [in]	F [in]	Dead volume [fl oz]
1/8	0.118	0.15	0.185	3.74	9.724	0.251	0.64
1/4	0.209	0.252	0.335	4.37	9.724	0.669	0.71
1/2	0.354	0.457	0.61	5.709	9.843	1.172	2.47
1	0.689	0.843	1.118	7.047	10.197	1.968	4.46

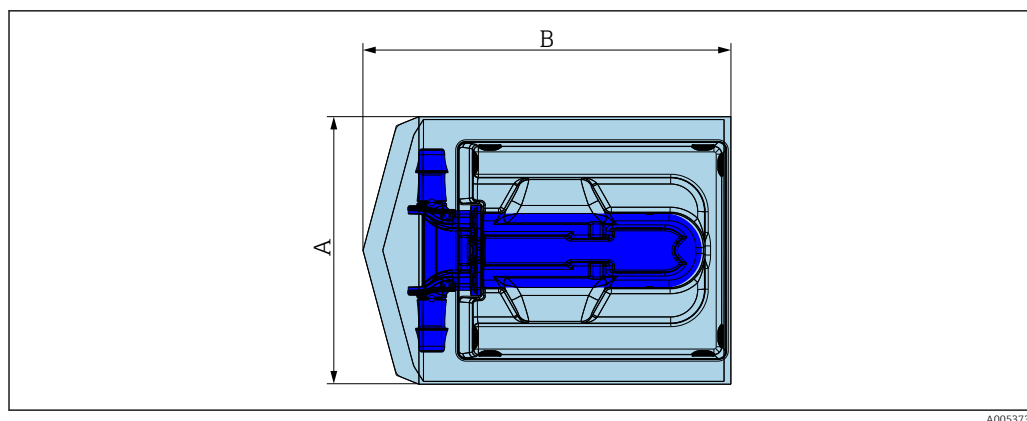


A0053734

Packed

Nominal diameter [in]	A [in]	B [in]
$\frac{1}{8}$	10.8	12
$\frac{1}{4}$	10.8	12
$\frac{1}{2}$	10.8	12
1	10.8	12

External WLAN antenna

The external WLAN antenna is not suitable for use in hygienic applications.

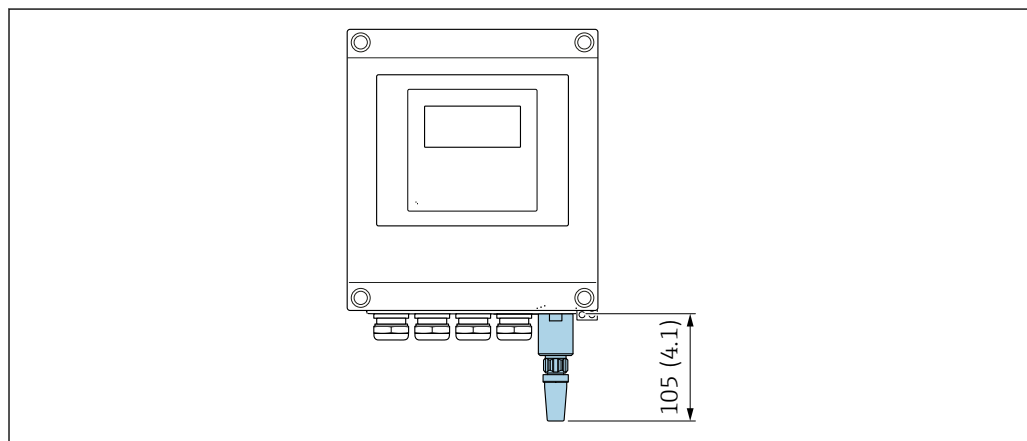
*Proline 500 – digital**External WLAN antenna mounted on device*

A0033607

16 Unit mm (in)

External WLAN antenna mounted with cable

The external WLAN antenna can be mounted separately from the transmitter if the transmission/reception conditions at the transmitter mounting location are poor.

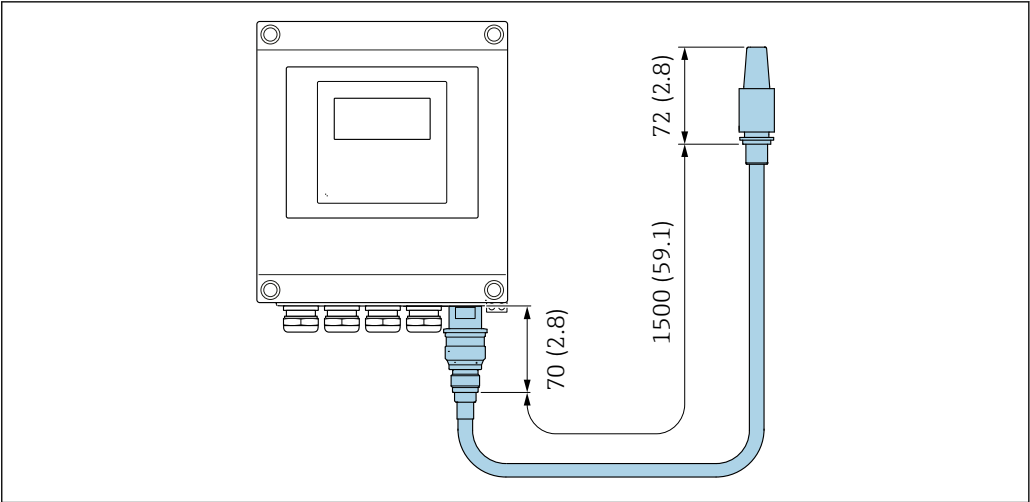

17 Unit mm (in)

Weight

Transmitter
Proline 500 – digital aluminum: 2.4 kg (5.3 lbs)

- Weight in SI units**
- Sensor: 8.65 kg
 - Table version: 12.1 kg
 - Disposable measuring tube: 0.6 kg

- Weight in US units**
- Sensor: 19.07 lbs
 - Table version: 26.68 lbs
 - Disposable measuring tube: 1.32 lbs

Materials

Transmitter housing

Housing of Proline 500 – digital transmitter

Order code for "Transmitter housing":
Option **A** "Aluminum coated": aluminum, AlSi10Mg, coated

Window material

Order code for "Transmitter housing":
Option **A** "Aluminum, coated": glass

Cable entries/cable glands

Cable entries and adapters	Material
Cable gland M20 × 1.5	Plastic
■ Adapter for cable entry with female thread G ½" ■ Adapter for cable entry with female thread NPT ½"	Nickel-plated brass

Connecting cables

 UV radiation can impair the cable outer sheath. Protect the cable from exposure to sun as much as possible.

Connecting cable for sensor - Proline 500 – digital transmitter

PE-X cable with copper shield

Disposable measuring tube

- Measuring tubes:
Stainless steel 1.4435, 316 L
- O-ring:
VMQ silicone
- Hose connection nipple:
Makrolon Rx 1805 polycarbonate



Available process connections

Accessories*External WLAN antenna*

- Antenna: ASA plastic (acrylonitrile styrene acrylate) and nickel-plated brass
- Adapter: Stainless steel and nickel-plated brass
- Cable: Polyethylene
- Plug: Nickel-plated brass
- Angle bracket: Stainless steel

Surface roughness

All data refer to parts in contact with the medium.

The following surface roughness categories can be ordered:

- Steel:
Ra = 0.76 µm (30 µin) mechanically polished
- Plastic:
Ra = 0.76 µm (30 µin)

Display and user interface

Operation concept**Operator-oriented menu structure for user-specific tasks**

- Commissioning
- Operation
- Diagnosis
- Expert level

Quick and safe commissioning

- Guided menus ("Make-it-run" wizards) for applications
- Menu guidance with brief descriptions of the individual parameter functions
- Access to the device via web server
- WLAN access to the device via mobile handheld terminal, tablet or smart phone

Reliable operation

- Operation in local language
- Uniform operating philosophy applied to device and operating tools
- If replacing electronic modules, transfer the device configuration via the integrated memory (HistoROM backup) which contains the process and measuring device data and the event logbook. No need to reconfigure.

Efficient diagnostics increase measurement reliability

- Troubleshooting measures can be called up via the device and in the operating tools
- Diverse simulation options, logbook for events that occur and optional line recorder functions

Languages

Can be operated in the following languages:

- Via local operation
English, German, French, Spanish, Italian, Dutch, Portuguese, Polish, Russian, Turkish, Chinese, Japanese, Korean, Vietnamese, Czech, Swedish
- Via web browser
English, German, French, Spanish, Italian, Dutch, Portuguese, Polish, Russian, Turkish, Chinese, Japanese, Vietnamese, Czech, Swedish
- Via "FieldCare", "DeviceCare" operating tool: English, German, French, Spanish, Italian, Chinese, Japanese

Onsite operation


Via display module

Equipment level:

- Order code for "Display; operation", option F "4-line, illuminated, graphic display; touch control"
- Order code for "Display; operation", option G "4-line, illuminated, graphic display; touch control + WLAN"



Information about WLAN interface → 54

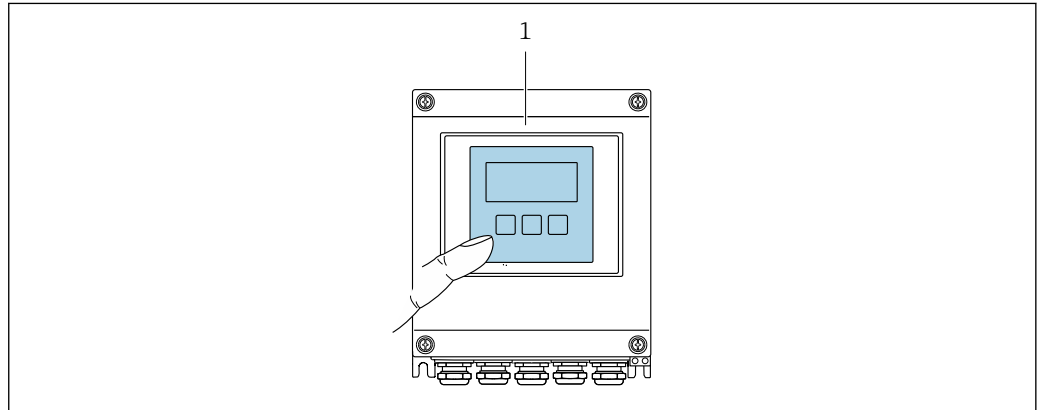

A0037255

18 Operation with touch control

1 Proline 500 – digital

Display elements

- 4-line, illuminated, graphic display
- White background lighting; switches to red in event of device errors
- Format for displaying measured variables and status variables can be individually configured


Operating elements

External operation via touch control (3 optical keys) without opening the housing:

Remote operation

Via Modbus RS485 protocol

This communication interface is available in device versions with a Modbus RS485 output.

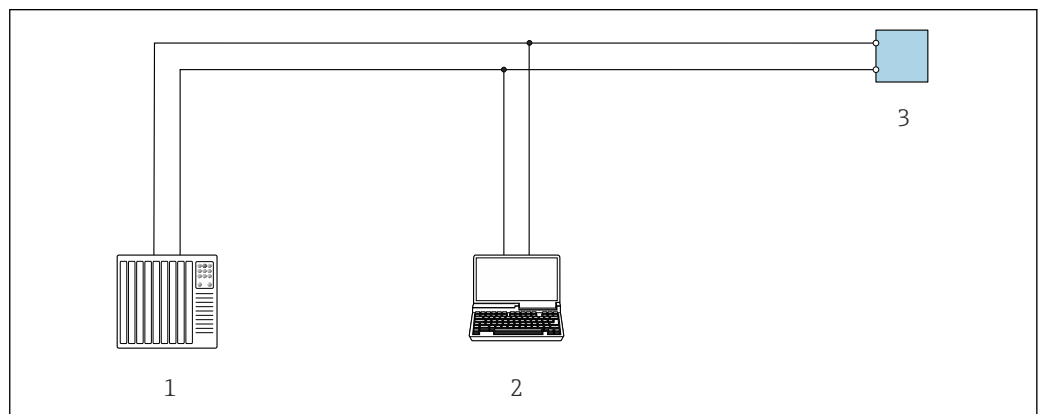


A0029437

19 Options for remote operation via Modbus RS485 protocol (active)

- 1 Automation system (e.g. PLC)
- 2 Computer with web browser for accessing the integrated device web server or with operating tool (e.g. FieldCare, DeviceCare) with COM DTM "CDI Communication TCP/IP" or Modbus DTM
- 3 Transmitter

Via Modbus TCP over Ethernet-APL 10 Mbit/s, SPE 10 Mbit/s

This communication interface is available on port 1 in device versions with a Modbus TCP over Ethernet-APL output.

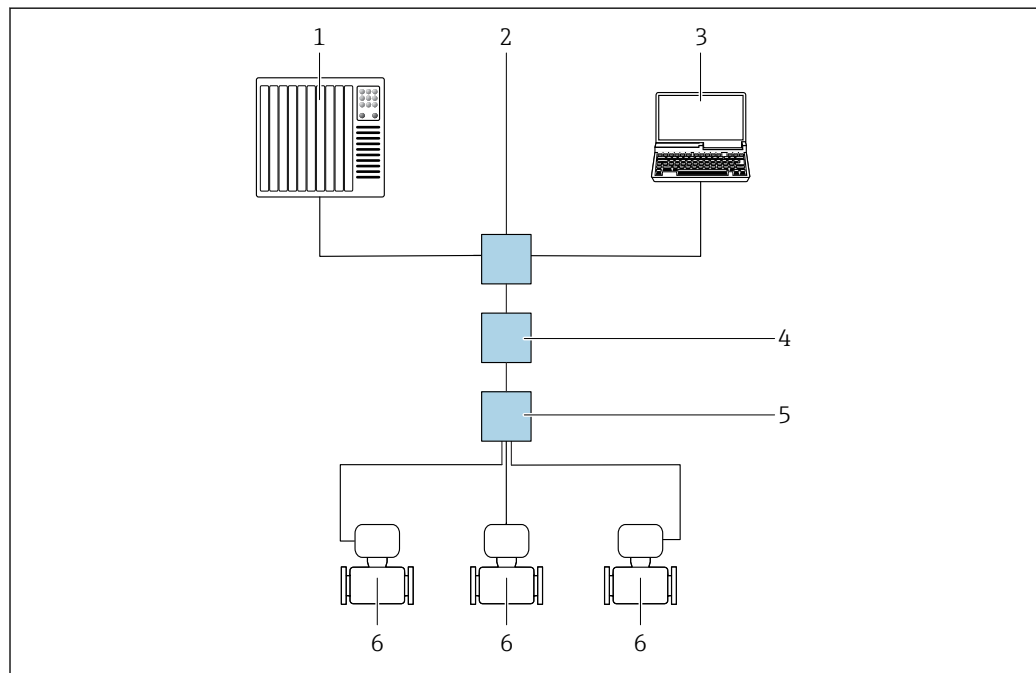


A0046117

20 Options for remote operation via Modbus TCP over Ethernet-APL protocol (active)

- 1 Automation system, e.g. Simatic S7 (Siemens)
- 2 Ethernet switch, e.g. Scalance X204 (Siemens)
- 3 Computer with web browser or operating tool
- 4 APL power switch/SPE power switch (optional)
- 5 APL field switch/SPE field switch
- 6 Measuring instrument/communication via port 1 (terminal 26 + 27)

Via Modbus TCP over Ethernet 100 Mbit/s

This communication interface is available on port 2 in device versions with a Modbus TCP over Ethernet-APL output.

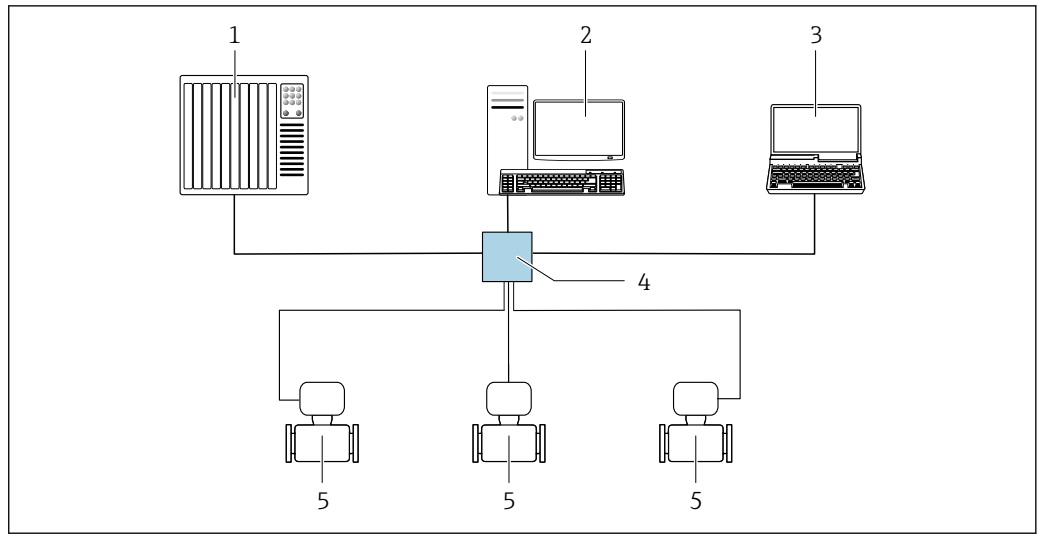Star topology

A0032078

21 Options for remote operation via Modbus TCP over Ethernet - 100 Mbit/s: Star topology

- 1 Automation system, z. B. RSLogix (Rockwell Automation)
- 2 Workstation for measuring instrument operation: with Custom Add-On Profile for "RSLogix 5000" (Rockwell Automation) or with Electronic Data Sheet (EDS)
- 3 Computer with web browser or operating tool
- 4 Standard Ethernet switch, e.g. Stratix (Rockwell Automation)
- 5 Measuring instrument/communication via port 2 (RJ45 connector)

Service interface**Via service interface (CDI-RJ45)**


To configure the device on site, a point-to-point connection can be established. Alternatively, a connection via Modbus TCP can be used. The connection is made with the housing open, directly via the device's service interface (CDI-RJ45).



An adapter for the RJ45 to the M12 plug is optionally available:

Order code for "Accessories", option **NB**: "Adapter RJ45 M12 (service interface)"

The adapter connects the service interface (CDI-RJ45) to an M12 plug mounted in the cable entry. The connection to the service interface can be established via an M12 plug without opening the device.

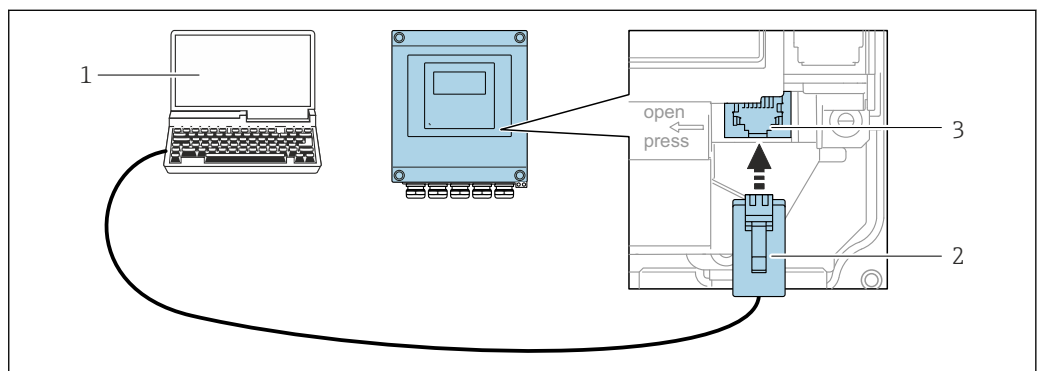Proline 500 – digital transmitter

A0029163


22 Connection via service interface (CDI-RJ45)

- 1 Computer with web browser (e.g. Microsoft Edge, port 2) for accessing the integrated web server or with operating tool "FieldCare", "DeviceCare" with COM DTM "CDI Communication TCP/IP" or Modbus DTM or operating tool
- 2 Standard Ethernet connecting cable with RJ45 connector
- 3 Service interface (CDI-RJ45) of the measuring instrument with access to the integrated web server

Via WLAN interface

The optional WLAN interface is available on the following device version:

Order code for "Display; operation", option G "4-line, illuminated; touch control + WLAN"

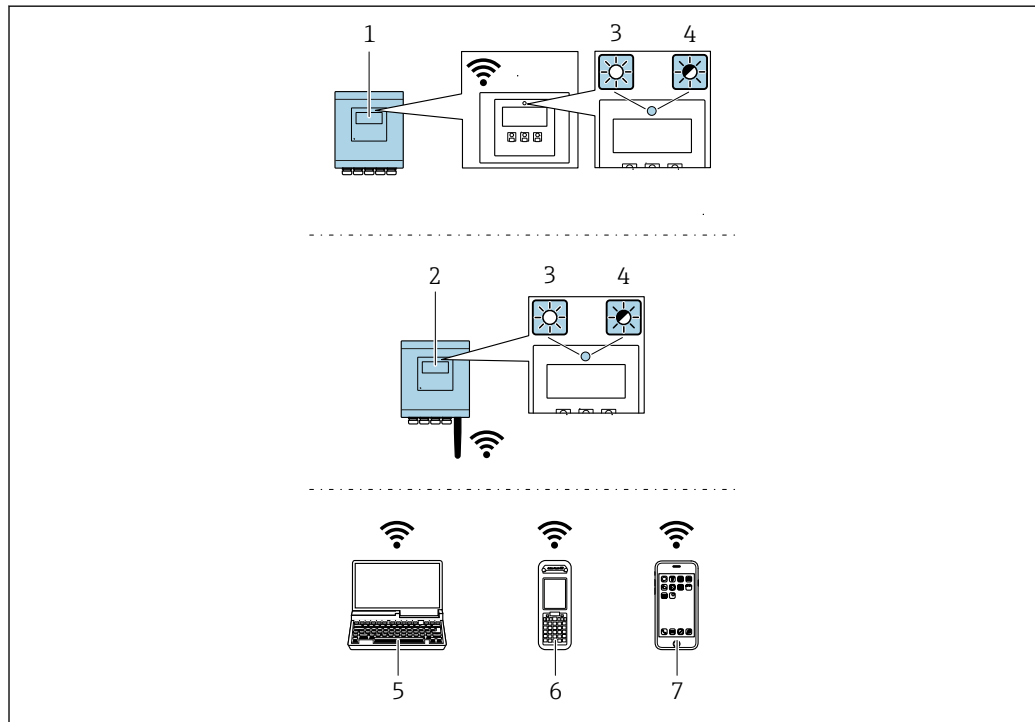

A0037682

- 1 Transmitter with integrated WLAN antenna
- 2 Transmitter with external WLAN antenna
- 3 LED lit constantly: WLAN reception is enabled on measuring instrument
- 4 LED flashing: WLAN connection established between operating unit and measuring instrument
- 5 Computer with WLAN interface and web browser for accessing integrated device web server or with operating tool. e.g. FieldCare, DeviceCare)
- 6 Mobiles handheld terminal with WLAN interface and web browser for accessing integrated device web server or operating tool (e.g. FieldCare, DeviceCare)
- 7 Smartphone or tablet (e.g. Field Xpert SMT70)

Function	WLAN: IEEE 802.11 b/g (2.4 GHz) ■ Access point with DHCP server (factory setting) ■ Network
Encryption	WPA2-PSK AES-128 (in accordance with IEEE 802.11i)
Configurable WLAN channels	1 to 11
Degree of protection	IP66/67
Available antennas	■ Internal antenna ■ External antenna (optional) In the event of poor transmission/reception conditions at the place of installation. Available as an accessory .  Only 1 antenna is active at any one time!
Range	■ Internal antenna: typically 10 m (32 ft) ■ External antenna: typically 50 m (164 ft)
Materials (external antenna)	■ Antenna: ASA plastic (acrylonitrile styrene acrylate) and nickel-plated brass ■ Adapter: Stainless steel and nickel-plated brass ■ Cable: Polyethylene ■ Plug: Nickel-plated brass ■ Angle bracket: Stainless steel

Supported operating tools

Different operating tools can be used for local or remote access to the measuring device. Depending on the operating tool used, access is possible with different operating units and via a variety of interfaces.

Supported operating tools	Operating unit	Interface	Additional information
Web browser	Notebook, PC or tablet with web browser	- Service interface CDI-RJ45 - WLAN interface - Ethernet-based fieldbus (Ethernet/IP, PROFINET, Modbus TCP over Ethernet-APL)	Special Documentation for device → 61
DeviceCare SFE100	Notebook, PC or tablet with Microsoft Windows system	- Service interface CDI-RJ45 - WLAN interface - Fieldbus protocol - Modbus TCP over Ethernet-APL	→ 60
FieldCare SFE500	Notebook, PC or tablet with Microsoft Windows system	- Service interface CDI-RJ45 - WLAN interface - Fieldbus protocol	→ 60
Field Xpert	SMT70/77/50	- All fieldbus protocols - WLAN interface - Bluetooth - Service interface CDI-RJ45	Operating Instructions BA01202S Device description files: Use update function of handheld terminal



Other operating tools based on FDT technology with a device driver such as DTM/iDTM or DD/EDD can be used for device operation. These operating tools are available from the individual manufacturers. Integration into the following operating tools, among others, is supported:

- Emersons TREX → www.emerson.com
- Field Device Manager (FDM) from Honeywell → www.process.honeywell.com
- FieldMate from Yokogawa → www.yokogawa.com
- PACTWare → www.pactware.com

The related device description files are available: www.endress.com → Download Area

Web server

The integrated web server can be used to operate and configure the device via a web browser via Ethernet-APL/SPE, service interface (CDI-RJ45) or via WLAN interface. The structure of the operating menu is the same as for the local display. In addition to the measured values, status information on the device is displayed and can be used to monitor device health. Furthermore the device data can be managed and the network parameters can be configured.

A device that has a WLAN interface (can be ordered as an option) is required for the WLAN connection: order code for "Display; Operation", option G "4-line, illuminated; touch control + WLAN". The device acts as an Access Point and enables communication by computer or a mobile handheld terminal.

Supported functions

Data exchange between the operating unit (such as a notebook, for example,) and measuring instrument:

- Upload the configuration from the measuring instrument (XML format, configuration backup)
- Save the configuration to the measuring instrument (XML format, restore configuration)
- Export event list (.csv file)
- Export parameter settings (.csv file or PDF file, document the measuring point configuration)
- Export the Heartbeat Technology verification report (PDF file, only available with the **Heartbeat Verification** application package)

- Flash firmware version for device firmware upgrade, for example
- Download driver for system integration
- Visualize up to 1000 saved measured values (only available with the **Extended HistoROM** application package)

Certificates and approvals

Current certificates and approvals for the product are available at www.endress.com on the relevant product page:

1. Select the product using the filters and search field.
2. Open the product page.
3. Select **Downloads**.

CE mark	The device meets the legal requirements of the applicable EU Directives. These are listed in the corresponding EU Declaration of Conformity along with the standards applied. Endress+Hauser confirms successful testing of the device by affixing to it the CE mark.
UKCA marking	The device meets the legal requirements of the applicable UK regulations (Statutory Instruments). These are listed in the UKCA Declaration of Conformity along with the designated standards. By selecting the order option for UKCA marking, Endress+Hauser confirms a successful evaluation and testing of the device by affixing the UKCA mark. Contact address Endress+Hauser UK: Endress+Hauser Ltd. Floats Road Manchester M23 9NF United Kingdom www.uk.endress.com
RCM marking	The measuring system meets the EMC requirements of the "Australian Communications and Media Authority (ACMA)".
Material certificate	■ Bioburden ■ Inorganic and organic residues ■ Cytotoxicity growth inhibition ■ Sensitization ■ Systemic toxicity ■ GC/MS fingerprints a. extraction ■ Physico-chemical resistance ■ Biocompatibility of plastics ■ Hemolysis ■ ISO Class 7 clean room ■ Medical devices QM ■ Conformities ■ Ingredients for rubber parts ■ Ingredients for plastic parts ■ Medical packaging ■ Gamma radiation ■ O-ring standard ■ FDA  A comprehensive listing of the serial number-specific disposable measuring tube can be found in the certificate of conformity for single-use requirements in the biopharmaceutical industry.

**PROFINET over Ethernet-
APL/SPE certification****PROFINET interface**

The measuring instrument is certified and registered by the PROFIBUS Nutzerorganisation e.V. (PNO). The measuring system meets all the requirements of the following specifications:

- Certified according to:
 - Test specification for PROFINET devices
 - PROFINET PA Profile 4.02
 - PROFINET Netload Robustness Class 2 10 Mbit/s
 - APL conformance test
- The device can also be operated with certified devices of other manufacturers (interoperability)
- The device supports PROFINET S2 system redundancy.

Radio approval

The measuring instrument has radio approval.



For detailed information on the radio approval, see the Special Documentation → 61

Additional certification**CRN approval**

Some device versions have CRN approval. A CRN-approved process connection with a CSA approval must be ordered for a CRN-approved device.

Tests and certificates

Pressure test, internal process, test report (order code for "Test, certificate", option JB)

**External standards and
guidelines**

- EN 60529
Degrees of protection provided by enclosures (IP code)
- IEC/EN 60068-2-6
Environmental influences: Test procedure - Test Fc: vibrate (sinusoidal).
- IEC/EN 60068-2-31
Environmental influences: Test procedure - Test Ec: shocks due to rough handling, primarily for devices.
- EN 61010-1
Safety requirements for electrical equipment for measurement, control and laboratory use - general requirements
- GB30439.5
Safety requirements for industrial automation products - part 5: Flowmeter safety requirements
- EN 61326-1/-2-3
EMC requirements for electrical equipment for measurement, control and laboratory use
- NAMUR NE 21
Electromagnetic compatibility (EMC) of industrial process and laboratory control equipment
- NAMUR NE 32
Data retention in the event of a power failure in field and control instruments with microprocessors
- NAMUR NE 43
Standardization of the signal level for the breakdown information of digital transmitters with analog output signal.
- NAMUR NE 53
Software of field devices and signal-processing devices with digital electronics
- NAMUR NE 105
Specifications for integrating fieldbus devices in engineering tools for field devices
- NAMUR NE 107
Self-monitoring and diagnostics of field devices
- NAMUR NE 131
Requirements for field devices for standard applications
- NAMUR NE 132
Coriolis mass meter
- ETSI EN 300 328
Guidelines for 2.4 GHz radio components.
- EN 301489
Electromagnetic compatibility and radio spectrum matters (ERM).
- Animal Free (ADI)

Ordering information

Detailed ordering information is available from your nearest sales organization www.addresses.endress.com or in the Product Configurator at www.endress.com:

1. Select the product using the filters and search field.
2. Open the product page.
3. Select **Configuration**.



Product Configurator - the tool for individual product configuration

- Up-to-the-minute configuration data
- Depending on the device: direct input of information specific to the measuring point, such as the measuring range or operating language
- Automatic verification of exclusion criteria
- Automatic creation of the order code and its breakdown in PDF or Excel output format
- Ability to order directly in the Endress+Hauser Online Shop

Application packages

Many different application packages are available to enhance the functionality of the device. Such packages might be needed to address safety aspects or specific application requirements.

The application packages can be ordered with the device or subsequently from Endress+Hauser. Detailed information on the order code in question is available from your local Endress+Hauser sales center or on the product page of the Endress+Hauser website: www.endress.com.



Detailed information on the application packages:
Special Documentation → 61

Accessories

Various accessories, which can be ordered with the device or subsequently from Endress+Hauser, are available for the device. Detailed information on the order code in question is available from your local Endress+Hauser sales center or on the product page of the Endress+Hauser website: www.endress.com.

Device-specific accessories

For the transmitter

Accessories	Description
Transmitter Proline 500 – digital	Transmitter for replacement or storage. Use the order code to define the following specifications: ■ Approvals ■ Output ■ Input ■ Display/operation ■ Housing ■ Software Proline 500 – digital transmitter: Order number: 8X5BXX-*****A Proline 500 – digital transmitter: Installation Instructions EA01151D

External WLAN antenna	External WLAN antenna with 1.5 m (59.1 in) connecting cable and two angle brackets. Order code for "Accessory enclosed", option P8 "Wireless antenna wide area".  The external WLAN antenna is not suitable for use in hygienic applications. - Further information on the WLAN interface →  54  Order number: 71351317  Installation Instructions EA01238D
Connecting cable Proline 500 – digital Sensor – Transmitter	The connecting cable can be ordered directly with the measuring instrument (order code for "Cable, sensor connection) or as an accessory (order number DK8012). The following cable lengths are available: order code for "Cable, sensor connection" - Option C: 2 m (6 ft) - Option J: 5 m (15 ft) - Option L: 10 m (30 ft)  Maximum possible cable length for a Proline 500 – digital connecting cable: 300 m (1 000 ft)

For the sensor

Accessories	Description
Disposable measuring tube	 Order number: - DN 1/8": DK8014-04SBOAADA2 - DN 1/4": DK8014-06SBOABFA2 - DN 1/2": DK8014-15SBOACFA2 - DN 1": DK8014-25SBOADFA2

Communication-specific accessories

Accessories	Description
Fieldgate FXA42	Transmission of the measured values of connected 4 to 20 mA analog measuring instruments, as well as digital measuring instruments  - Technical Information TI01297S - Operating Instructions BA01778S - Product page: www.endress.com/fxa42
Field Xpert SMT50	The Field Xpert SMT50 tablet PC for device configuration enables mobile plant asset management in non-hazardous areas. It is suitable for commissioning and maintenance staff to manage field instruments with a digital communication interface and to record progress. This tablet PC is designed as an all-in-one solution with a preinstalled driver library and is an easy-to-use, touch-sensitive tool which can be used to manage field instruments throughout their entire life cycle.  - Technical Information TI01555S - Operating Instructions BA02053S - Product page: www.endress.com/smt50
Field Xpert SMT70	The Field Xpert SMT70 tablet PC for device configuration enables mobile plant asset management in hazardous and non-hazardous areas. It is suitable for commissioning and maintenance staff to manage field instruments with a digital communication interface and to record progress. This tablet PC is designed as an all-in-one solution with a preinstalled driver library and is an easy-to-use, touch-sensitive tool which can be used to manage field instruments throughout their entire life cycle.  - Technical Information TI01342S - Operating Instructions BA01709S - Product page: www.endress.com/smt70
Field Xpert SMT77	The Field Xpert SMT77 tablet PC for device configuration enables mobile plant asset management in areas categorized as Ex Zone 1.  - Technical Information TI01418S - Operating Instructions BA01923S - Product page: www.endress.com/smt77

Service-specific accessories

Accessories	Description
Applicator	Software for selecting and sizing Endress+Hauser measuring instruments: - Choice of measuring instruments for industrial requirements - Calculation of all the necessary data for identifying the optimum flowmeter: e.g. nominal diameter, pressure loss, flow velocity and measurement accuracy. - Graphic display of the calculation results - Determination of the partial order code, administration, documentation and access to all project-related data and parameters over the entire life cycle of a project. Applicator is available: Via the Internet: https://portal.endress.com/webapp/applicator
Netilion	IIoT ecosystem: Unlock knowledge With the Netilion IIoT ecosystem, Endress+Hauser allows you to optimize your plant performance, digitize workflows, share knowledge, and enhance collaboration. Drawing upon decades of experience in process automation, Endress+Hauser offers the process industry an IIoT ecosystem designed to effortlessly extract insights from data. These insights can be used to optimize processes, leading to increased plant availability, efficiency, and reliability - ultimately resulting in a more profitable plant. www.netilion.endress.com
FieldCare	FDT-based plant asset management tool from Endress+Hauser. It can configure all intelligent field units in your system and helps you manage them. By using the status information, it is also a simple but effective way of checking their status and condition.  Operating Instructions BA00027S and BA00059S
DeviceCare	Tool to connect and configure Endress+Hauser field devices.  Innovation brochure IN01047S

Documentation



For an overview of the scope of the associated Technical Documentation, refer to the following:

- Device Viewer (www.endress.com/deviceviewer): Enter the serial number from the nameplate
- Endress+Hauser Operations app: Enter serial number from nameplate or scan matrix code on nameplate.

Standard documentation



Supplementary information on the semi-standard options is available in the relevant Special Documentation in the TSP database.

Brief operating instructions

Brief Operating Instructions for the sensor

Measuring instrument	Documentation code
Proline Promass U	KA01686D

Brief operating instructions for transmitter

Measuring instrument	Documentation code	
	Modbus RS485	PROFINET over Ethernet-APL
Proline 500 – digital	KA01319D	KA01521D

Operating instructions

Measuring instrument	Documentation code		
	Modbus RS485	PROFINET over Ethernet-APL/SPE	Modbus TCP
Promass U 500	BA02342D	BA02343D	BA02342D

Description of device parameters

Measuring instrument	Documentation code				
	HART	FOUNDATION fieldbus	PROFIBUS PA	PROFIBUS DP	Modbus RS485

Measuring instrument	Documentation code			
	Ethernet/IP	PROFINET	PROFINET over Ethernet-APL	Modbus TCP over Ethernet-APL

Measuring instrument	Documentation code		
	Modbus RS485	PROFINET over Ethernet-APL/SPE	Modbus TCP
Promass 500	GP01062D	GP01173D	GP01236D

Supplementary device-dependent documentation

Special documentation

Contents	Documentation code
Information on the Pressure Equipment Directive	SD01614D
Radio approvals for WLAN interface for A309/A310 display module	SD01793D
Modbus TCP system integration	SD03383D

Installation Instructions

Contents	Note
Installation instructions for spare part sets and accessories	Documentation code: specified for each individual accessory → 58.

Registered trademarks

Modbus®

Registered trademark of SCHNEIDER AUTOMATION, INC.

Ethernet-APL™

Registered trademark of the PROFIBUS Nutzerorganisation e.V. (PROFIBUS User Organization), Karlsruhe, Germany



www.addresses.endress.com
