

# Safety Instructions

## **Deltabar FMD71, FMD72**

4-20 mA HART

Ex db [ia] IIC T6...T4 Ga/Gb

Ex db [ia] IIC T6...T3 Ga/Gb





# Deltabar FMD71, FMD72

4-20 mA HART

## Table of contents

About this document .....	4
Associated documentation .....	4
Supplementary documentation .....	4
Manufacturer's certificates .....	4
Manufacturer address .....	4
Extended order code .....	4
Safety instructions: General .....	6
Safety instructions: Special conditions .....	7
Safety instructions: Installation .....	8
Safety instructions: Zone 0 .....	9
Temperature tables .....	9
Connection data .....	10

**About this document**

This document has been translated into several languages. Legally determined is solely the English source text.

**Associated documentation**

This document is an integral part of the following Operating Instructions:

BA01044P/00

**Supplementary documentation**

Special Documentation for cable gland M20 Ex d: SD02550F/00

Explosion-protection brochure: CP00021Z/11

The Explosion-protection brochure is available:

- In the download area of the Endress+Hauser website:  
[www.endress.com](http://www.endress.com) -> Downloads -> Brochures and Catalogs -> Text Search: CP00021Z
- On the CD for devices with CD-based documentation

**Manufacturer's certificates****Certificate of Conformity**

Certificate number:  
CML 22JPN2275X

Affixing the certificate number certifies conformity with the following standards (depending on the device version):

- JNIO SH-TR-46-1 : 2020
- JNIO SH-TR-46-2 : 2018
- JNIO SH-TR-46-6 : 2015
- IEC 60079-26 : 2014

**Manufacturer address**

Endress+Hauser SE+Co. KG  
Hauptstraße 1  
79689 Maulburg, Germany

Address of the manufacturing plant: See nameplate.

**Extended order code**

The extended order code is indicated on the nameplate, which is affixed to the device in such a way that it is clearly visible. Additional information about the nameplate is provided in the associated Operating Instructions.

## Structure of the extended order code

FMD7x	–	*****	+	A*B*C*D*E*F*G*..
<i>(Device type)</i>		<i>(Basic specifications)</i>		<i>(Optional specifications)</i>

\* = Placeholder

At this position, an option (number or letter) selected from the specification is displayed instead of the placeholders.

### *Basic specifications*

The features that are absolutely essential for the device (mandatory features) are specified in the basic specifications. The number of positions depends on the number of features available.

The selected option of a feature can consist of several positions.

### *Optional specifications*

The optional specifications describe additional features for the device (optional features). The number of positions depends on the number of features available. The features have a 2-digit structure to aid identification (e.g. JA). The first digit (ID) stands for the feature group and consists of a number or a letter (e.g. J = Test, Certificate). The second digit constitutes the value that stands for the feature within the group (e.g. A = 3.1 material (wetted parts), inspection certificate).

More detailed information about the device is provided in the following tables. These tables describe the individual positions and IDs in the extended order code which are relevant to hazardous locations.

## Extended order code: Deltabar



The following specifications reproduce an extract from the product structure and are used to assign:

- This documentation to the device (using the extended order code on the nameplate).
- The device options cited in the document.

### *Device type*

FMD71, FMD72

*Basic specifications*

Position 1, 2 (Approval)		
Selected option		Description
FMD71	JB	JPN Ex db [ia] IIC T6...T4 Ga/Gb JPN Ex db [ia] IIC T6...T3 Ga/Gb
FMD72	JB	JPN Ex db [ia] IIC T6...T4 Ga/Gb

Position 5 (Housing Transmitter)		
Selected option		Description
FMD7x	A	Aluminium T14
	B	Stainless steel T14

*Optional specifications*

No options specific to hazardous locations are available.

**Safety instructions:**  
**General**

- Comply with the installation and safety instructions in the Operating Instructions.
- Staff must meet the following conditions for mounting, electrical installation, commissioning and maintenance of the device:
  - Be suitably qualified for their role and the tasks they perform
  - Be trained in explosion protection
  - Be familiar with national regulations
- Install the device according to the manufacturer's instructions and national regulations.
- Only use the device in media to which the wetted materials have sufficient durability.

**Safety****instructions:****Special conditions**


- For light metal flanges or flange faces (e.g. titanium, zirconium), avoid sparks caused by impact and friction.
- In the case of process connections made of polymeric material or with polymeric coatings, avoid electrostatic charging of the plastic surfaces.
- In the event of additional or alternative special varnishing on the enclosure or other metal parts:
  - Observe the danger of electrostatic charging and discharge.
  - Do not rub surfaces with a dry cloth.
- For repair: Contact the manufacturer for dimensional information on the flameproof joints.
- The sensors can be installed in the boundary wall between Zone 0 and the less hazardous area Zone 1. In this configuration, the process connection is installed in Zone 0, while the sensor enclosure is installed in Zone 1.

*Potential Electrostatic Charging Hazard*

Avoid electrostatic charging:

- Of plastic surfaces (e.g. enclosure, sensor element, special varnishing, attached additional plates, ..)
- Of isolated capacities (e.g. isolated metallic plates)

## Safety instructions: Installation

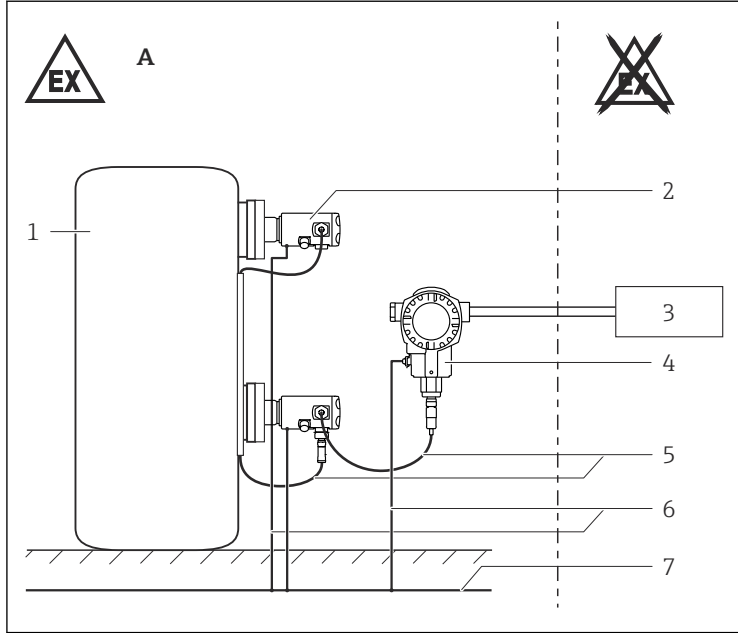

A0032294



- 1 Tank; Zone 0  
 2 Sensor module  
 3 Certified associated apparatus  
 4 Transmitter enclosure (Ex d)  
 5 Ex ia circuits  
 6 Potential equalization line  
 7 Potential equalization

- In potentially explosive atmospheres: Do not open the connection compartment cover and the electronics compartment cover when energized.
- The connection cables to the sensor modules are intrinsically safe circuits (Ex ia). Observe the pertinent guidelines when intrinsically safe plants are installed.
- Sensor modules may only be connected to the transmitter and interconnected to each other. Any further connections are not allowed.



- Transmitter enclosure and sensor modules must have the same ground potential (e.g. transmitter enclosure and sensor modules all mounted to the same metal structure).  
If potential equalisation can not be achieved by the installation, the devices must be interconnected with a suitable bonding conductor using the external ground connections.
- Before operation:
  - Screw in the cover all the way.
  - Tighten the securing clamp on the cover.
- Seal unused entry glands with supplied metal blind plug. Alternative use only suitable, separate approved Ex db blanking elements.
- The plastic sealing plug is used only as transport protection.
- Connect the device:
  - Using suitable cable and wire entries of protection type "Flameproof Enclosure (Ex db)".
  - Using piping systems of protection type "Flameproof Enclosure (Ex db)".
- When connecting through a conduit entry approved for this purpose, mount the associated sealing unit directly at the enclosure.

**Safety instructions:**  
**Zone 0**

- In the event of potentially explosive vapor/air mixtures, only operate the device under atmospheric conditions.
  - Temperature: -20 to +60 °C
  - Pressure: 80 to 110 kPa (0.8 to 1.1 bar)
  - Air with normal oxygen content, usually 21 % (V/V)
- If no potentially explosive mixtures are present, or if additional protective measures have been taken, the device may also be operated under non-atmospheric conditions in accordance with the manufacturer's specifications.

**Temperature tables**

*Device type FMD71*

**Compact version**

Type of protection

Ex db [ia] IIC T6...T4 Ga/Gb

Temperature class	Process temperature $T_p$ (process)	Ambient temperature $T_a$ (ambient): enclosure
T6	$\leq 80\text{ °C}$	$-40\text{ °C} \leq T_a \leq +40\text{ °C}$
T4	$\leq 125\text{ °C}$	$-40\text{ °C} \leq T_a \leq +70\text{ °C}$



The process temperatures refer to the temperature at the separation membrane.

### High-temperature version

Type of protection

Ex db [ia] IIC T6...T3 Ga/Gb

Temperature class	Process temperature $T_p$ (process)	Ambient temperature $T_a$ (ambient): enclosure
T6	$\leq 80\text{ }^\circ\text{C}$	$-40\text{ }^\circ\text{C} \leq T_a \leq +40\text{ }^\circ\text{C}$
T4	$\leq 135\text{ }^\circ\text{C}$	$-40\text{ }^\circ\text{C} \leq T_a \leq +70\text{ }^\circ\text{C}$
T3	$\leq 150\text{ }^\circ\text{C}$	$-40\text{ }^\circ\text{C} \leq T_a \leq +70\text{ }^\circ\text{C}$



The process temperatures refer to the temperature at the separation membrane.

Device type FMD72

Type of protection

Ex db [ia] IIC T6...T4 Ga/Gb

Temperature class	Process temperature $T_p$ (process)	Ambient temperature $T_a$ (ambient): enclosure
T6	$\leq 80\text{ }^\circ\text{C}$	$-40\text{ }^\circ\text{C} \leq T_a \leq +40\text{ }^\circ\text{C}$
T4	$\leq 125\text{ }^\circ\text{C}$	$-40\text{ }^\circ\text{C} \leq T_a \leq +70\text{ }^\circ\text{C}$



- The process temperatures refer to the temperature at the separation membrane.
- Higher temperatures are permitted depending on the type of diaphragm seal.
- Do not exceed the max. ambient temperature at the enclosure.

### Connection data

Electrical data
$U \leq 45\text{ V}_{DC}$ $P \leq 1.1\text{ W}$





71562655

[www.addresses.endress.com](http://www.addresses.endress.com)

---