

Safety Instructions

Solicap S FTI77

Ex ia IIC T80°C T₂₀₀ 130°C Da

Ex ia IIC T80°C T₂₀₀ 130°C Da/Db

Ex ia/tb IIC T90°C Da/Db



Solicap S FTI77

Table of contents

About this document	4
Associated documentation	4
Supplementary documentation	4
Certificates and declarations	4
Manufacturer address	4
Extended order code	4
Safety instructions: General	8
Safety instructions: Specific conditions of use	8
Safety instructions: Installation	9
Temperature tables	12
Connection data	15

About this document

The document number of these Safety Instructions (XA) must match the information on the nameplate.

Associated documentation

All documentation is available on the Internet:

www.endress.com/Deviceviewer

(enter the serial number from the nameplate).

To commission the device, please observe the Operating Instructions pertaining to the device:

BA00381F

Supplementary documentation

Explosion protection brochure: CP00021Z

The explosion protection brochure is available on the Internet:

www.endress.com/Downloads

Certificates and declarations**NEPSI Declaration of Conformity**

Certificate number:

GYJ24.1152X

Affixing the certificate number certifies conformity with the following standards (depending on the device version):

- GB/T 3836.1-2021
- GB/T 3836.4-2021
- GB/T 3836.31-2021

Manufacturer address

Endress+Hauser SE+Co. KG

Hauptstraße 1

79689 Maulburg, Germany

Address of the manufacturing plant: See nameplate.

Extended order code

The extended order code is indicated on the nameplate, which is affixed to the device in such a way that it is clearly visible. Additional information about the nameplate is provided in the associated Operating Instructions.

Structure of the extended order code

FTI77	–	*****	+	A*B*C*D*E*F*G*..
<i>(Device type)</i>		<i>(Basic specifications)</i>		<i>(Optional specifications)</i>

* = Placeholder

At this position, an option (number or letter) selected from the specification is displayed instead of the placeholders.

Basic specifications

The features that are absolutely essential for the device (mandatory features) are specified in the basic specifications. The number of positions depends on the number of features available.

The selected option of a feature can consist of several positions.

Optional specifications

The optional specifications describe additional features for the device (optional features). The number of positions depends on the number of features available. The features have a 2-digit structure to aid identification (e.g. JA). The first digit (ID) stands for the feature group and consists of a number or a letter (e.g. J = Test, Certificate). The second digit constitutes the value that stands for the feature within the group (e.g. A = 3.1 material (wetted parts), inspection certificate).

More detailed information about the device is provided in the following tables. These tables describe the individual positions and IDs in the extended order code which are relevant to hazardous locations.

Extended order code: Solicap S



The following specifications reproduce an extract from the product structure and are used to assign:

- This documentation to the device (using the extended order code on the nameplate).
- The device options cited in the document.

Device type

FTI77

Basic specifications

Position 1 (Approval)		
Selected option		Description
FTI77	1	NEPSI Ex ia IIIC T80°C T ₂₀₀ 130°C Da NEPSI Ex ia IIIC T80°C T ₂₀₀ 130°C Da/Db
	3	NEPSI Ex ia/tb IIIC T90°C Da/Db

Position 2 (Application)		
Selected option		Description
FTI77	1	Solid, fine-grained
	2	Solid, coarse-solids

Position 3 (Inactive Length L3)		
Selected option		Description
FTI77	A	Not selected
	B, C, L, M mm/in, steel
	E, F, G, N, P, R mm/in, 316L
	H, S mm/in, 316L+125mm/5in active build-up protection, 316L

Position 4, 5 (Active Probe Length L1)		
Selected option		Description
FTI77	Ax, Ex mm/in, sword, steel
	Bx, Fx mm/in, sword, 316L
	Cx, Gx mm/in, mm/in rope, steel zinc coated, tension weight steel
	Dx, Hx mm/in, mm/in rope, 316, tension weight 316L

Position 9 (Electronics, Output)		
Selected option		Description
FTI77	Y	Special version: FEI50H
	1 ¹⁾	FEI51; 2-wire 19-253VAC
	2 ¹⁾	FEI52; 3-wire PNP 10-55VDC
	4 ¹⁾	FEI54; relay DPDT, 19-253VAC, 19-55VDC
	5	FEI55; 8/16mA, 11-35VDC
	7 ²⁾	FEI57S; 2-wire PFM
	8 ²⁾	FEI58; NAMUR+test button (H-L signal)

- 1) Only in connection with supply circuit "Non-intrinsically safe"
 2) Only in connection with supply circuit "Intrinsically safe Ex ia"

Position 10 (Housing)		
Selected option		Description
FTI77	1	F15 316L hygiene IP66/67 NEMA4X
	3	F17 Alu IP66/67 NEMA4X
	4	F13 Alu IP66 NEMA4X + gas-tight probe seal
	5	T13 Alu IP66 NEMA4X + gas-tight probe seal + separate conn. compartment
	6	F27 316L IP66/67 NEMA6P + gas-tight probe seal

Position 12 (Type of probe)		
Selected option		Description
FTI77	1	Compact
	2, 3, 4, 5 mm/in L4 cable > separate enclosure

Optional specifications

No options specific to hazardous locations are available.

Safety instructions:
General

- The device is intended to be used in explosive atmospheres as defined in the scope of IEC 60079-0 or equivalent national standards. If no potentially explosive atmospheres are present or if additional protective measures have been taken: The device may be operated according to the manufacturer's specifications.
- Staff must meet the following conditions for mounting, electrical installation, commissioning and maintenance of the device:
 - Be suitably qualified for their role and the tasks they perform
 - Be trained in explosion protection
 - Be familiar with national regulations
- For installation, use and maintenance of the device, users must also observe the requirements stated in the Operating Instructions and the standards:
 - GB 50257-2014: "Code for construction and acceptance of electric device for explosion atmospheres and fire hazard electrical equipment installation engineering".
 - GB/T 3836.13-2021: "Explosive atmospheres, Part 13: Equipment repair, overhaul, reclamation and modification".
 - GB/T 3836.15-2017: "Explosive atmospheres, Part 15: Electrical installations design, selection and erection".
 - GB/T 3836.16-2022: "Explosive atmospheres, Part 16: Electrical installations inspection and maintenance".
 - GB 15577-2018: "Safety regulations for dust explosive prevention and protection". (Only if installed in dust hazardous area.)
- Install the device according to the manufacturer's instructions and national regulations.
- Do not operate the device outside the specified electrical, thermal and mechanical parameters.
- Avoid electrostatic charging:
 - Of plastic surfaces (e.g. enclosure, sensor element, special varnishing, attached additional plates, ...)
 - Of isolated capacities (e.g. isolated metallic plates)

Safety instructions:
Specific conditions of use


Permitted ambient temperature range at the electronics enclosure, permitted process temperature:
 $-50\text{ °C} \leq T_a \leq +70\text{ °C}$

- Observe the information in the temperature tables.
- In the event of additional or alternative special varnishing on the enclosure or other metal parts:
 - Observe the danger of electrostatic charging and discharge.
 - Do not rub surfaces with a dry cloth.

Basic specification, Position 10 = 4, 5 and covers with glass window
 Restriction to $-40\text{ °C} \leq T_a \leq +70\text{ °C}$.

**Safety
instructions:
Installation**

Supply circuit "Intrinsically safe Ex ia"

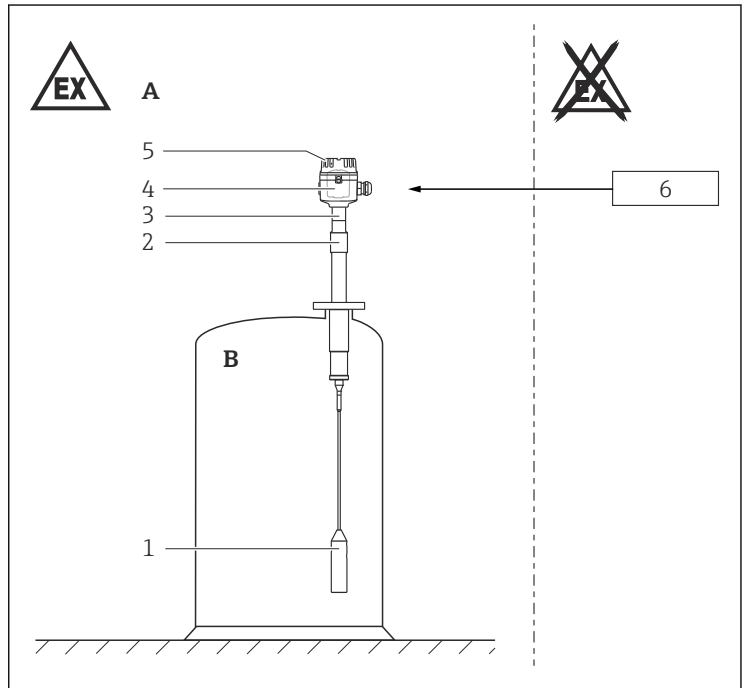


A0033933

1

- A Zone 20, Zone 21
- B Zone 20
- 1 Strut or rope with tensioning weight
- 2 Probe
- 3 Adapter
- 4 Electronic insert
- 5 Enclosure
- 6 Certified associated apparatus

Supply circuit "Non-intrinsically safe"

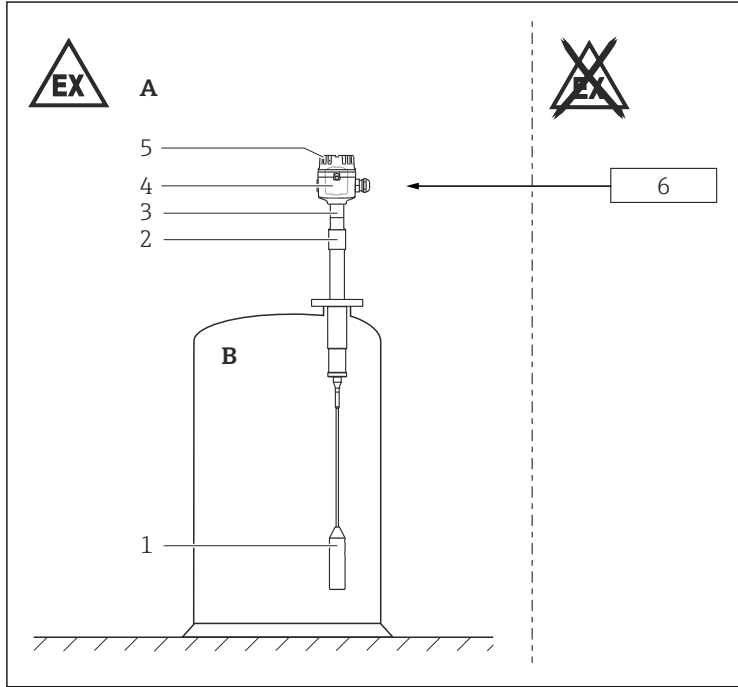

A0033993



- A Zone 21
 B Zone 20
 1 Strut or rope with tensioning weight
 2 Probe
 3 Adapter
 4 Electronic insert
 5 Enclosure
 6 Power supply

- Do not open in a potentially explosive dust atmosphere.
- Observe the maximum process conditions according to the manufacturer's Operating Instructions.
- At high medium temperatures, note flange pressure load capacity as a factor of temperature.
- To maintain the ingress protection of the enclosure:
 - Screw the cover tight.
 - Mount the cable entry correctly.
- After aligning (rotating) the enclosure, retighten the fixing screw (see Operating Instructions).

- Connect the device using suitable cable and wire entries of protection type "Equipment dust ignition protection by enclosure (Ex t)" or "Increased safety (Ex e)" (ingress protection of at least IP65). Lay connecting cable and secure.
- Seal unused entry glands with approved sealing plugs that correspond to the type of protection.
- Install the device to exclude any mechanical damage or friction during the application. Pay particular attention to flow conditions and tank fittings.
- Mechanically fix probes which are more than 3 m (e.g. using guy ropes).
- Maximum rope tensile load:
 - Fine-grained bulk solids: 7.5 kN
 - Coarse-grained bulk solids: 20 kN
- Maximum lateral load including strut:
 - Fine-grained bulk solids: 250 Nm
 - Coarse-grained bulk solids: 800 Nm

Basic specification, Position 10 = 1

Before operation:

- Screw in the cover all the way.
- Tighten the securing clamp on the cover.

Basic specification, Position 10 = 3, 4, 5, 6

Tighten the cover with torque 12 Nm.

Intrinsic safety

Observe the pertinent guidelines when interconnecting intrinsically safe circuits.

Potential equalization

Install potential equalization between the certified associated apparatus (non-hazardous area, X) and the device (explosion-hazardous area, $\triangle\text{Ex}$).


Temperature tables

	Probe and electronics enclosure in Zone 20
	Connection to certified intrinsically safe power circuits
Max. surface temperature at an ambient temperature of 70 °C	80 °C Deposited material with a layer of 200 mm T ₂₀₀ 130 °C

	Probe in Zone 20	Electronics enclosure in Zone 21	
		Connection to certified intrinsically safe power circuits	Connection to non-intrinsically safe power circuits
Max. surface temperature at an ambient temperature of 70 °C	70 °C	80 °C	90 °C
The compact version can also be used for process temperatures between +70 to +400 °C if it can also be ensured that the ambient temperature at the electronics enclosure does not exceed the values as indicated in the temperature graphic.	400 °C	40 °C	40 °C

Compact version

Strut and rope version, partially insulated

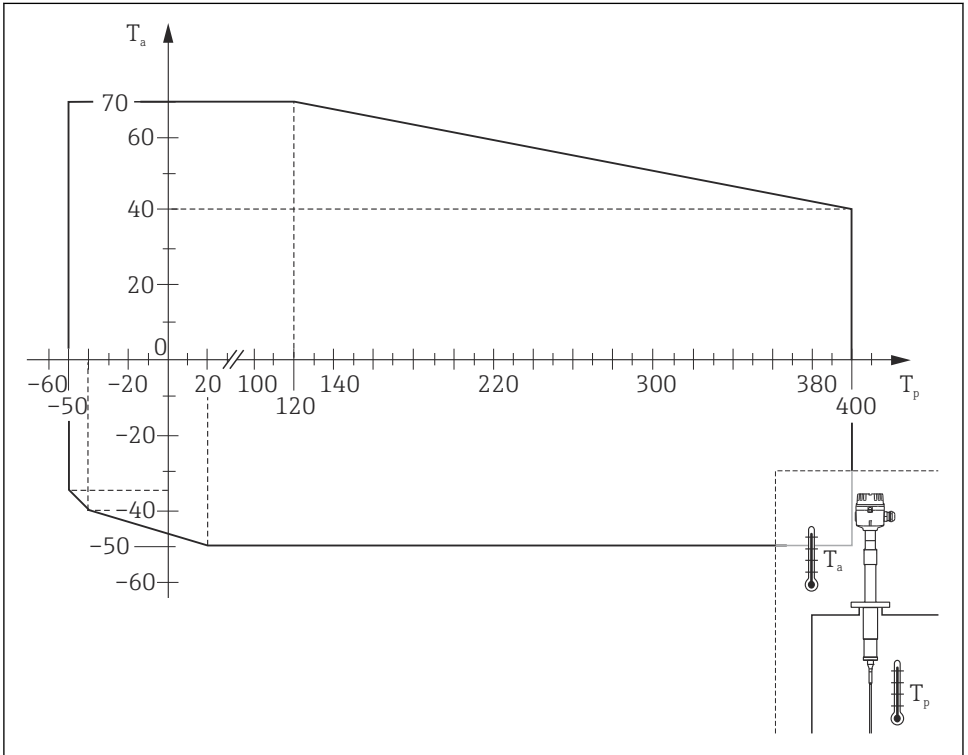


A0033929

3

T_a Ambient temperature in °C

T_p Process temperature in °C

Version with separate enclosure

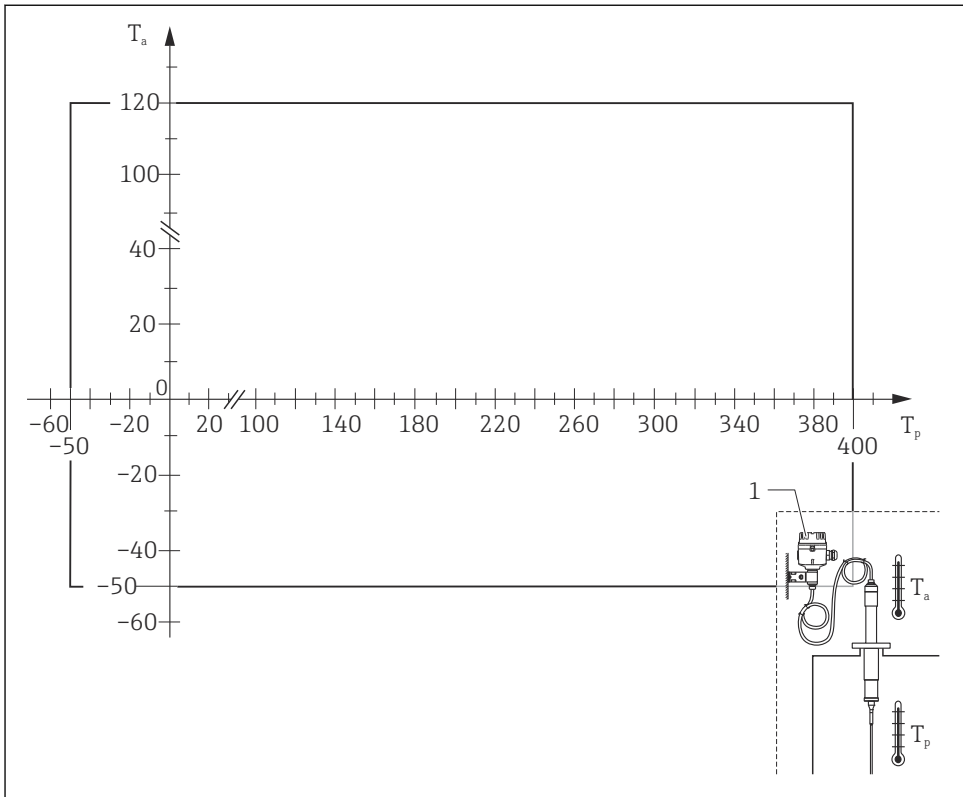

A0033928

 4

T_a Ambient temperature in °C

T_p Process temperature in °C

1 Temperature at the separate enclosure: $-40\text{ °C} \leq T_a \leq +70\text{ °C}$

Connection data Connection to certified intrinsically safe circuits Ex ia (Zone 20)

<i>Basic specification, Position 9</i>	Electrical data
Y	$U_i \leq 30 \text{ V}$ $I_i \leq 120 \text{ mA}$ $P_i \leq 1 \text{ W}$ $C_i \leq 2.4 \text{ nF}$ $L_i \leq 0$
5	$U_i \leq 35 \text{ V}$ $I_i \leq 100 \text{ mA}$ $P_i \leq 1 \text{ W}$ $C_i \leq 2.4 \text{ nF}$ $L_i \leq 0$
7	$U_i \leq 16.1 \text{ V}$ $I_i \leq 100 \text{ mA}$ $P_i \leq 1 \text{ W}$ $C_i \leq 2.4 \text{ nF}$ $L_i \leq 0$
8	$U_i \leq 18 \text{ V}$ $I_i \leq 52 \text{ mA}$ $P_i \leq 170 \text{ mW}$ $C_i/L_i \leq 0$

Connection to non-intrinsically safe circuits (Zone 20/21)


<i>Basic specification, Position 9</i>	Electrical data
Y ¹⁾	$U \leq 35 \text{ V}_{\text{DC}}$
5 ¹⁾	$U \leq 35 \text{ V}_{\text{DC}}$

1) With Basic specification, Position 10 = 5 only with limiting module

<i>Basic specification, Position 9</i>	Power supply	Relay circuit
1	19 to 253 V _{AC}	–
2	10 to 55 V _{DC}	–
4	19 to 253 V _{AC}	253 V _{AC} / 6 A 1500 VA / $\cos \varphi = 1$ 750 VA / $\cos \varphi > 0.7$
	19 to 55 V _{DC}	30 V _{DC} / 4 A 125 V _{DC} / 0.2 A

Cable entry parameters

Thread	Clamping range	Material	Sealing insert	O-ring
M20x1,5	ø 8 to 10.5 mm	Ms, nickel-plated	Silicone	EPDM (ø 17x2)

- 
 - The tightening torque refers to cable glands installed by the manufacturer:
 - Recommended torque to connect the cable gland into the enclosure: 3.75 Nm
 - Recommended torque to tighten the cable into the cable gland: 3.5 Nm
 - Maximum torque to tighten the cable into the cable gland: 10 Nm
 - This value may be different depending on the type of cable. However, the maximum value must not be exceeded.
 - Only suitable for fixed installation. The operator must pay attention to a suitable strain relief of the cable.
 - To maintain the ingress protection of the enclosure: Install the enclosure cover, cable glands and blind plugs correctly.



71646145

www.addresses.endress.com
