



Member of the FM Global Group

FM Approvals  
1151 Boston Providence Turnpike  
P.O. Box 9102 Norwood, MA 02062 USA  
T: 781 762 4300 F: 781-762-9375 www.fmapprovals.com

# CERTIFICATE OF COMPLIANCE

## HAZARDOUS (CLASSIFIED) LOCATION ELECTRICAL EQUIPMENT

This certificate is issued for the following equipment:

**PROMASS abc-defghiknop. Mass Flowmeter.**

XP-IS-DIP / I,II,III / 1 / ABCDEFG / T\*; XP-IS / I / 1 / IIC / T\* - FES0048; Entity, FISCO; Type 4X

Special Conditions of Use:

1. For installation instructions and the Temperature Class (\*) which applies to specific models, ambient temperatures (Ta), and process medium temperatures (Tmed), refer to Control Drawing FES0048.

Entity Parameters:

I/O option S and R HART Current Output or Current Output:

$V_{oc} = 21.8 \text{ V}$ ,  $I_{sc} = 90 \text{ mA}$ ,  $P_o = 0.49 \text{ W}$ ,  $C_a = 150 \text{ nF}$ ,  $L_a = 4.1 \text{ mH}$ ;

$V_{Max} = 30 \text{ V}$ ,  $I_{Max} = 10 \text{ mA}$ ,  $P_i = 0.3 \text{ W}$ ,  $C_i = 6 \text{ nF}$ ,  $L_i = 0$ .

I/O Option S and T Frequency Output:

$V_{Max} = 30 \text{ V}$ ,  $I_{Max} = 300 \text{ mA}$ ,  $P_i = 0.6 \text{ W}$ ,  $C_i = 6 \text{ nF}$ ,  $L_i = 0$ .

I/O option T and U HART Current Output or Current Output:

$V_{Max} = 30 \text{ V}$ ,  $I_{Max} = 100 \text{ mA}$ ,  $P_i = 1.25 \text{ W}$ ,  $C_i = 6 \text{ nF}$ ,  $L_i = 0$ .

I/O Options F and G (Entity, FISCO):

$V_{Max} = 30 \text{ V}$ ,  $I_{Max} = 600 \text{ mA}$ ,  $P_i = 8.5 \text{ W}$ ,  $C_i = 5 \text{ nF}$ ,  $L_i = 10 \mu\text{H}$ .

a = Type of electronic: 40, 80, 83 or 84.

b = Type of sensor: A (with h = N).

b = Type of sensor: E (with h = N or O; (c=80) with h = P)

b = Type of sensor: F [(c = 08, 15, 25, 40, 50, 80, 1H, 1F, 2F) with h = N or O; (c = 80, 1H, 1F, 2F) with h = P].

b = Type of sensor: I [(c = 08, 15, 16, 25, 26, 40, 41, 50, 51, 80) with h = N or O; (c = 41, 50, 51, 80) with h = P].

b = Type of sensor: M [(c = 08, 15, 25, 40, 50, 80) with h = N or O; (c = 80) with h = P].

b = Type of sensor: H [(c = 08, 15, 25, 40, 50) with h = N or O; (c = 50) with h = P].

b = Type of sensor: P [(c = 08, 15, 25, 40, 50) with h = N or O; (c = 50) with h = P].

b = Type of sensor: S [(c = 08, 15, 25, 40, 50) with h = N or O; (c = 50) with h = P].

b = Type of sensor: O [(c = 80, 1H, 1F, 2F) with h = N or O; (c = 80, 1H, 1F, 2F) with h = P]

b = Type of sensor: X. [(c = 3F) with h = N or O; (c = 3F) with h = P]

c = Size: 01, 02, 04, 08, 15, 16, 25, 26, 40, 41, 50, 51, 80, 1H, 1F, 2F, 3F, XX.

d = Material of tube/high pressure version: any single number or letter.

e = Process connection with sealing for Promass M: any triple number or letter (up to 400 bar).

f = Certifications/Treatments: any single number or letter.

- g = Calibration: any single number or letter.
- h = Approvals: N or O (Div. 1, GP A, B, C, D, E, F, G) or P (Div. 1, GP C, D, E, F, G).
- i = Version: A, E, F, J, K, L, M, N, U, V, W, 1, 4, 7 or 8.
- k = Cable gland: B or X.
- n = Version: 0, 1, 2, 3, 4, 5, 7, 8, 9, A, B, C, D, E, F, G, H, K, L, M, N, P, Q, R, S or X.
- o = Software: any single number or letter.
- p = I/O's: A, B, C, D, E, F, G, H, J, K, L, M, N, P, Q, R, S, T, U, V, W, X, 0, 1, 2, 3, 4, 5, 6, 7, 8 or 9.
- \*\* = Option in two digits (none, two or multiple of two digits); any combination of number or letter
- +, # = Signs used as indicator for optional abbreviation of extended order code

AND

**PROMASS abc-defghiknop+\*\*\*#. Mass Flowmeter.**

NI-ANI/1/2/ABCD/T\*; NI-ANI/2/IIC/T\*; DIP/II,III/1/EFG/T\*; Nonincendive Sensor Field Wires and Nonincendive Fieldbus Field Wires — FES0050; Type 4X

Nonincendive Fieldbus Field Wire Parameters:

V<sub>max</sub> = 35V, C<sub>i</sub> = 5nF, L<sub>i</sub> = 10 μH

*Special conditions of use:*

1. For installation instructions and the Temperature Class (\*) which applies to specific models, ambient temperatures (T<sub>a</sub>), and process medium temperatures (T<sub>med</sub>), refer to Control Drawing FES0050.

a = Type of electronic: 40, 80, 83 or 84

b = Type of sensor: A, E, F, H, I, M, P, S, O or X

c = Size: 01, 02, 04, 08, 15, 16, 25, 26, 40, 41, 50, 51, 80, 1H, 1F, 2F, 3F or XX

d = Material of tube/high pressure version: any single number or letter

e = Process connection with sealing for Promass M: any triple number or letter (up to the pressure of 400 bar)

f = Certifications/Treatments: any single number or letter

g = Calibration: any single number or letter

h = Approvals: R (Division 2)

i = Version: A, B, C, D, G, H, 1, 2, 3, 5, or 6

k = Cable gland: A, B, C, D, K, L, M, Q, R, S or X

n = Version: 0, 1, 2, 3, 4, 5, 7, 8, 9, A, B, C, D, E, F, G, H, K, L, M, N, P, Q, R, S or X

o = Software: any single number or letter

p = I/O's: A, B, C, D, E, H, I, J, K, L, M, N, P, Q, V, W, X, 0, 1, 2, 3, 4, 5, 6, 7, 8 or 9

\*\* = Option in two digits (none, two or multiple of two digits); any combination of number or letter

+, # = Signs used as indicator for optional abbreviation of extended order code

AND

**CNGmass DCI 8aFb-cdefghikno+###. Mass Flowmeter.**

XP-IS-DIP / I,II,III / 1 / ABCDEFG / T\*; XP-IS / I / 1 / IIC / T\* - FES0182; Entity, FISCO; Type 4X

Special Conditions of Use:

1. For installation instructions and the Temperature Class (\*) which applies to specific models, ambient temperatures (Ta), and process medium temperatures (Tmed), refer to Control Drawing FES0182.

Entity Parameters:

I/O option S and R HART Current Output or Current Output:

$V_{oc} = 21.8 \text{ V}$ ,  $I_{sc} = 90 \text{ mA}$ ,  $P_o = 0.49 \text{ W}$ ,  $C_a = 150 \text{ nF}$ ,  $L_a = 4.1 \text{ mH}$ ;

$V_{Max} = 30 \text{ V}$ ,  $I_{Max} = 10 \text{ mA}$ ,  $P_i = 0.3 \text{ W}$ ,  $C_i = 6 \text{ nF}$ ,  $L_i = 0$ .

I/O Option S and T Frequency Output:

$V_{Max} = 30 \text{ V}$ ,  $I_{Max} = 300 \text{ mA}$ ,  $P_i = 0.6 \text{ W}$ ,  $C_i = 6 \text{ nF}$ ,  $L_i = 0$ .

I/O option T and U HART Current Output or Current Output:

$V_{Max} = 30 \text{ V}$ ,  $I_{Max} = 100 \text{ mA}$ ,  $P_i = 1.25 \text{ W}$ ,  $C_i = 6 \text{ nF}$ ,  $L_i = 0$ .

I/O Options F and G (Entity, FISCO):

$V_{Max} = 30 \text{ V}$ ,  $I_{Max} = 600 \text{ mA}$ ,  $P_i = 8.5 \text{ W}$ ,  $C_i = 5 \text{ nF}$ ,  $L_i = 10 \mu\text{H}$ .

a = Version: any single number or letter.

b = Size: 08, 15, 25, XX.

c = Material of tube/high pressure version: any single number or letter.

d = Process connection: any triple number or letter (up to 400 bar).

e = Certifications/Treatments: any single number or letter.

f = Calibration: any single number or letter.

g = Approvals: M, N or 8 (Div. 1, GP A, B, C, D, E, F, G).

h = Version: A, E, F, J, K, L, M, N, U, V, W, 1, 4, 7 or 8.

i = Cable gland: B or X.

k = Version: 0, 1, 2, 3, 4, 5, 7, 8, 9, A, B, C, D, E, F, G, H, K, L, M, N, P, Q, R, S or X.

n = Software: any single number or letter.

o = I/O's: A, B, C, D, E, F, G, H, J, K, L, M, N, P, Q, R, S, T, U, V, W, X, 0, 1, 2, 3, 4, 5, 6, 7, 8 or 9.

\*\* = Option in two digits (none, two or multiple of two digits); any combination of number or letter

+, # = Signs used as indicator for optional abbreviation of extended order code

AND

**Cubemass DCI 8Cab-cdefghiknop+###. Mass Flowmeter.**

XP-IS-DIP / I,II,III / 1 / ABCDEFG / T\*; XP-IS / I / 1 / IIC / T\* - FES0183; Entity, FISCO; Type 4X

Special Conditions of Use:

1. For installation instructions and the Temperature Class (\*) which applies to specific models, ambient temperatures (Ta), and process medium temperatures (Tmed), refer to Control Drawing FES0183.

Entity Parameters:

I/O option S and R HART Current Output or Current Output:

$V_{oc} = 21.8 \text{ V}$ ,  $I_{sc} = 90 \text{ mA}$ ,  $P_o = 0.49 \text{ W}$ ,  $C_a = 150 \text{ nF}$ ,  $L_a = 4.1 \text{ mH}$ ;

$V_{Max} = 30 \text{ V}$ ,  $I_{Max} = 10 \text{ mA}$ ,  $P_i = 0.3 \text{ W}$ ,  $C_i = 6 \text{ nF}$ ,  $L_i = 0$ .

I/O Option S and T Frequency Output:

$V_{Max} = 30 \text{ V}$ ,  $I_{Max} = 300 \text{ mA}$ ,  $P_i = 0.6 \text{ W}$ ,  $C_i = 6 \text{ nF}$ ,  $L_i = 0$ .

I/O option T and U HART Current Output or Current Output:

$V_{Max} = 30 \text{ V}$ ,  $I_{Max} = 100 \text{ mA}$ ,  $P_i = 1.25 \text{ W}$ ,  $C_i = 6 \text{ nF}$ ,  $L_i = 0$ .

I/O Options F and G (Entity, FISCO):

$V_{Max} = 30 \text{ V}$ ,  $I_{Max} = 600 \text{ mA}$ ,  $P_i = 8.5 \text{ W}$ ,  $C_i = 5 \text{ nF}$ ,  $L_i = 10 \mu\text{H}$ .

a = Version: any single number or letter.  
b = Size: 01, 02, 04, 06, XX.  
c = Approvals: C3 or 84 (Div. 1, GP A, B, C, D, E, F, G).  
d = I/O's: A, B, C, D, E, F, G, H, J, K, L, M, N, P, Q, R, S, T, U, V, W, X, 0, 1, 2, 3, 4, 5, 6, 7, 8 or 9.  
e = Version: 0, 1, 2, 3, 4, 5, 7, 8, 9, A, B, C, D, E, F, G, H, K, L, M, N, P, Q, R, S or X  
f = Display/Operation: any single number or letter  
g = Operating Language: any single number or letter.  
h = Version: A, E, F, J, K, L, M, N, U, V, W, 1, 4, 7 or 8.  
i = Cable gland: B or X.  
k = Material of tube: any single number or letter.  
n = Process connection: any single number or letter.  
o = Secondary containment: any single number or letter.  
p = Calibration/Treatment: any single number or letter.  
\*\* = Option in two digits (none, two or multiple of two digits); any combination of number or letter  
+, # = Signs used as indicator for optional abbreviation of extended order code

## Equipment Ratings:

Explosionproof for Class I Division 1, Group A, B, C and D and Class I, Zone 1, Group IIC; dust-ignitionproof for Classes II and III Division 1, Groups E, F and G hazardous (classified) outdoor (Type 4X) locations; sensor circuits and signal output circuits (p = I/O options F, G, R, S, T, U) intrinsically safe for Class I, II, III, Division 1, Groups A, B, C, D, E, F and G and Class I Zone 1 Groups IIC when installed in accordance with FM Control Drawing FES0048 (Promass) or FES00182 (CNGmass DCI) or FES0183 (Cubemass DCI)..

Nonincendive for Class I Division 2, Group A, B, C and D and Class I, Zone 2, Group IIC; dust-ignitionproof for Classes II and III Division 1, Group E, F and G hazardous (classified) outdoor (Type 4X) locations; sensor circuits nonincendive for Class I, Division 2, Groups A, B, C and D and Class I, Zone 2, Group IIC. Nonincendive field wiring for Class I Division 2, Group A, B, C and D and Classes II and III Division 1, Group E, F and G hazardous (classified) locations when installed in accordance with FM Control Drawing FES0050 (Promass)..

## FM Approved for:

Endress + Hauser Flowtec AG  
Kaegenstrasse 7  
CH-4153 Reinach, Switzerland



Member of the FM Global Group

This certifies that the equipment described has been found to comply with the following Approval Standards and other documents:

Class 3600	1998
Class 3610	2010
Class 3611	2004
Class 3615	2006
Class 3810	2005
ANSI/NEMA 250	1991


Original Project ID: 3009083

Approval Granted: December 19, 2000

Subsequent Revision Reports / Date Approval Amended

Report Number	Date	Report Number	Date
3012866	December 28, 2001		
3012691	May 7, 2002		
3015235	September 4, 2002		
3016669	February 21, 2003		
3021216	August 31, 2003		
050120	February 28, 2005		
050818	September 1, 2005		
3028484	November 20, 2006		
070130	July 25, 2007		
3030403	November 30, 2007		
070905	December 20, 2007		
071115	December 31, 2007		
3038437	June 9, 2010		
3042811	May 9, 2011		
3043873	September 21, 2011		
110930	<i>January 27, 2011</i>		


FM Approvals LLC

  
 Patrick Byrne  
 Technical Team Manager

*January 27, 2012*  
 Date

### Hazardous Locations

Class I Division 1 Groups ABCD or Class I Zone 1 Groups IIC and Class II and III Division 1 Groups EFG

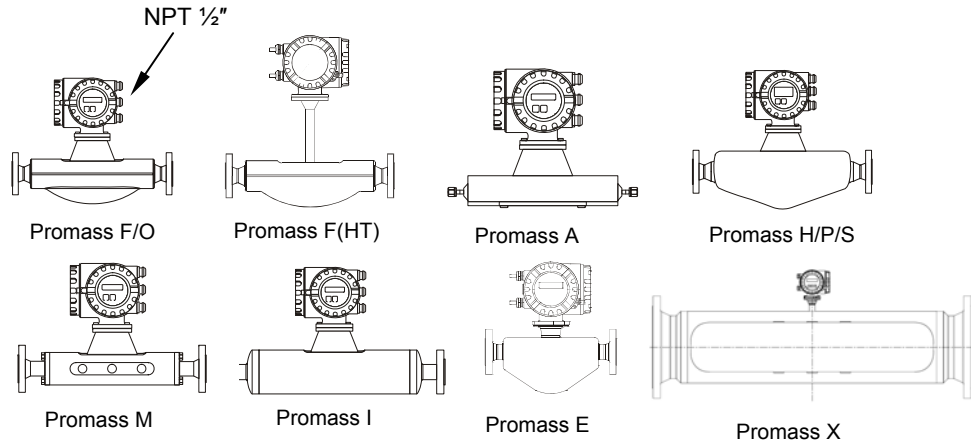

**WARNING: SUBSTITUTION OF COMPONENTS MAY IMPAIR INTRINSIC SAFETY.**

**Notes:**

- Control room equipment shall not use or generate more than 250 V rms.
- Caution: Use supply wires suitable for 5 °C above ambient temperature, but at least for 80 °C / 176 °F.
- Class II Group G: The surface temperature of the apparatus cannot exceed 165 °C / 329 °F. The user must limit the process temperature for Group G to 140 °C.
- Transmitter enclosures Proline G02 and G12 are explosionproof for use in Cl. I Div. 1 Groups A, B, C, D and dust-ignitionproof for Cl. II, III Div. 1 Groups E, F, G
- Transmitter enclosures PROline G02 and G12 are factory sealed for use in Cl. I Div. 1 Groups A, B, C, D. A conduit seal is not required.
- Sensor circuits intrinsically safe for Cl. I, II, III Div. 1 Group A, B, C, D, E, F, G except limited versions of
  - Promass E DN80 (sensor version Group C-D)
  - Promass M DN80 (sensor version Group C-D)
  - Promass I DN41/50/51/80 (sensor version Group C-D)
  - Promass F/F(HT)/O DN80/100/150/250 (sensor version Group C-D)
  - Promass H/P/S DN50 (sensor version Group C-D)
  - Promass X DN350 (sensor version Group C-D)
 which are only suitable for Cl. I, II, III Div. 1 Group C, D, E, F, G
- The minimum medium temperature is -50 °C (-40 °C for Promass E)
- Install all intrinsically safe circuits per NEC ANSI/NFPA 70 and ISA RP 12.6 respecting the Explosionproof Integrity of the enclosure
- The following Sensors are Dual Seal devices in accordance with ANSI/ISA-12.27.01-2003: Promass A, F, F(HT), H, O, P, S and X. Promass E is a Dual Seal device if the optional rupture disk is present.

Temperature table	max. medium temperature [°C]								
	T6	T5	T4A	T4	T3A	T2C	T2B	T2	T1
<b>Ta = 45°C:</b>									
Promass E DN8/15/25/40/50	45	100	120	130	140	140	140	140	140
Promass P/S DN8	45	65	85	100	140	185	200	200	200
<b>Ta = 50°C:</b>									
Promass M DN8/15/25/40/50/80	50	60	85	105	150	150	150	150	150
Promass F DN8/15/25/40	55	70	85	100	150	185 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>
Promass F DN50/80/100/150/250	60	70	85	105	150	185 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>
Promass O DN 80/100/150/250	60	70	85	105	150	185 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>
Promass I DN8/15/16/25	60	95	95	110	150	150	150	150	150
Promass I DN26/40/41/50/51/80	70	85	105	120	150	150	150	150	150
Promass H DN8	50	65	85	100	140	185	200	200	200
Promass H DN15/25/40/50	60	75	100	115	160	200	200	200	200
Promass P/S DN8	---	65	85	100	140	185	200	200	200
Promass P/S DN15/25	50	75	100	115	160	200	200	200	200
Promass P/S DN40	55	75	100	115	160	200	200	200	200
Promass P/S DN50	60	75	95	110	155	200	200	200	200
Promass X DN350	60	70	85	105	150	185 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>
<b>Ta = 60°C:</b>									
Promass A DN1/2/4	60	95	115	130	140	200	200	200	200
Promass M DN8/15/25/40/50/80	---	60	85	100	100	100	100	100	100
Promass F DN8/15/25/40	55	70	85	100	150 <sup>)</sup>	185 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>
Promass F DN50/80/100/150/250	60	70	85	100	150 <sup>)</sup>	185 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>
Promass O DN80/100/150/250	60	70	85	100	150 <sup>)</sup>	185 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>
Promass I DN8/15/16/25	60	95	95	110	150 <sup>)</sup>	150 <sup>)</sup>	150 <sup>)</sup>	150 <sup>)</sup>	150 <sup>)</sup>
Promass I DN26/40/41/50/51/80	70	85	105	120	150 <sup>)</sup>	150 <sup>)</sup>	150 <sup>)</sup>	150 <sup>)</sup>	150 <sup>)</sup>
Promass H DN8	50	65	85	100	140	185 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>
Promass H DN15/25/40/50	60	75	100	115	160	200 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>
Promass E DN8/15/25/40/50	---	100	120	130	140	140	140	140	140
Promass E DN80	60	75	95	110	140	140	140	140	140
Promass F(HT) DN25/50/80	70	85	100	115 <sup>)</sup>	160 <sup>)</sup>	205 <sup>)</sup>	235 <sup>)</sup>	275 <sup>)</sup>	350 <sup>)</sup>
Promass P/S DN8	---	65	85	100	140	185 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>
Promass P/S DN15/25/40	---	75	100	115	160	200 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>
Promass P/S DN50	60	75	95	110	155	200 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>
Promass X DN350	60	70	85	100	150 <sup>)</sup>	185 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>	200 <sup>)</sup>

Device shall not be installed in such way that the transmitter enclosure is located above the sensor.  
 Tm min. is -50°C for Promass A/F/F(HT)/H/I/M/O/P/S/X; Ta min. is -40°C; Tm min. is -40°C for Promass E; Ta min. is -40°C

Communication or other options	Control Drawing
I/O option = F,H,J,Q	see FES 0048 - 0001
I/O option = G,K	see FES 0048 - 0002
I/O option = S,T	see FES 0048 - 0004
I/O option = R,U	see FES 0048 - 0005
Promass 40/80/83/84 E DN80 (optional version)	see FES 0162


Aenderungen:	F	27.04.04/MDI	L	03.08.07/PAM	Alle gesetzlichen Urheberrechte vorbehalten. Diese Zeichnung darf ohne unsere Genehmigung weder vervielfältigt werden noch dritten Personen und Konkurrenzfirmen zugänglich gemacht werden.	<b>Mat.-Nr. 71147429</b>  Ersatz für: Ersteller: FES / <b>ID 1090</b> FILE: M:\ZEICHNUNG\FES0048\PI\FES0048P_110523.doc
	G	06.10.04/MDI	M	05.09.07/BDA		
	H	03.08.05/SCHK	N	11.11.09/SCHK		
	J	15.08.06/BDA	P	05.08.11/SCHK		
	K	20.10.06/BDA				

**FM Control Drawing Div. 1 / Zone 1**  
**Class I Zone 1**  
**Compact Version**  
**Promass 40/80/83/84 A/E/F/H/I/M/O/P/S/X**

Gezeichnet	06.10.00	Bn
Geprüft		
Ex-geprüft	05.08.11	SCHK
Gesehen		

### Hazardous Locations

Class I Division 1 Groups ABCD or Class I Zone 1 Groups IIC  
and Class II and III Division 1 Groups EFG

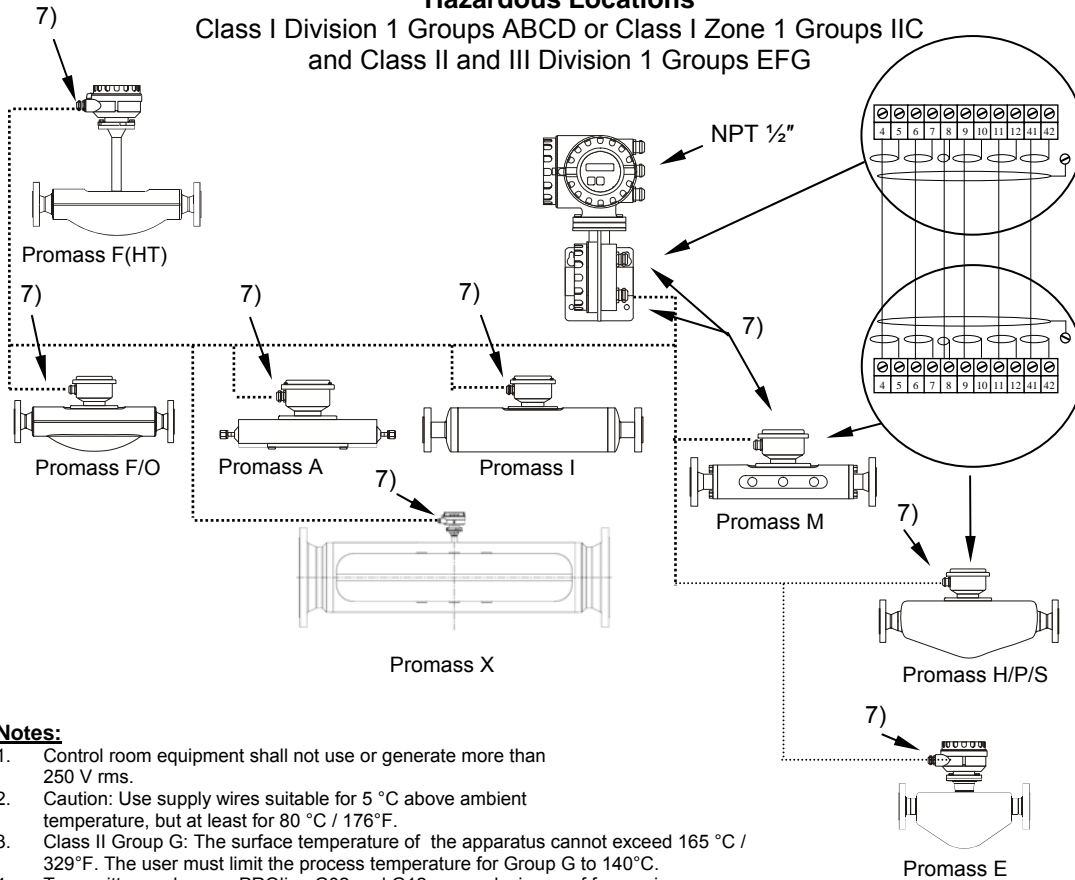

#### Notes:

- Control room equipment shall not use or generate more than 250 V rms.
- Caution: Use supply wires suitable for 5 °C above ambient temperature, but at least for 80 °C / 176°F.
- Class II Group G: The surface temperature of the apparatus cannot exceed 165 °C / 329°F. The user must limit the process temperature for Group G to 140°C.
- Transmitter enclosures PROline G02 and G12 are explosionproof for use in Cl. I Div. 1 Groups A, B, C, D and dust-ignitionproof for Cl. II, III Div. 1 Groups E, F, G
- Transmitter enclosures PROline G02 and G12 are factory sealed for use in Cl. I Div. 1 Groups A, B, C, D. A conduit seal is not required.
- Sensor circuits intrinsically safe for Cl. I, II, III Div. 1 Group A, B, C, D, E, F, G except a limited version of
  - Promass E DN80 (sensor version Group C-D)
  - Promass M DN80 (sensor version Group C-D)
  - Promass I DN41/50/51/80 (sensor version Group C-D)
  - Promass F/F(HT)/O DN80/100/150/250 (sensor version Group C-D)
  - Promass H/P/S DN50 (sensor version Group C-D)
  - Promass X DN350 (sensor version Group C-D)
 which are only suitable for Cl. I, II, III Div. 1 Group C, D, E, F, G
- Allowed cable glands: NPT 1/2", G 1/2", M20x1.5 or PG13.5
- A sensor which was connected to a Promass 60/63/64 transmitter can also be installed to a Promass 8. transmitter. For this case this control drawing is relevant for safe use, except the minimum ambient temperature which is limited to -20°C
- Install all intrinsically safe circuits per NEC ANSI/NFPA 70 and ISA RP 12.6 respecting the Explosionproof Integrity of the enclosure
- The following Sensors are Dual Seal devices in accordance with ANSI/ISA-12.27.01-2003: Promass A, E, F, F(HT), H, O, P, S and X. Promass E is a Dual Seal device if the optional rupture disk is present.

Temperature table	max. medium temperature [°C]								
	T6	T5	T4A	T4	T3A	T2C	T2B	T2	T1
<b>Ta = 45 °C</b>									
Promass E DN25/40/50	45	100	120	130	140	140	140	140	140
Promass P/S DN8	45	65	85	100	140	185	200	200	200
<b>Ta = 50 °C</b>									
Promass P/S DN8	---	65	85	100	140	185	200	200	200
Promass P/S DN15/25	50	75	100	115	160	200	200	200	200
Promass P/S DN40	55	75	100	115	160	200	200	200	200
<b>Ta = 60 °C</b>									
Promass A DN1/2/4	60	95	115	130	140	200	200	200	200
Promass M DN8/15/25/40/50/80	50	60	85	105	150	150	150	150	150
Promass F DN8/15/25/40	55	70	85	100	150	185	200	200	200
Promass F DN50/80/100/150/250	60	70	85	105	150	185	200	200	200
Promass O DN80/100/150/250	60	70	85	105	150	185	200	200	200
Promass I DN8/15/16/25	60	95	95	110	150	150	150	150	150
Promass I DN26/40/41/50/51/80	70	85	105	120	150	150	150	150	150
Promass H DN8	50	65	85	100	140	185	200	200	200
Promass H DN15/25/40/50	60	75	100	115	160	200	200	200	200
Promass E DN8/15/25/40/50	---	100	120	130	140	140	140	140	140
Promass E DN80	60	75	95	110	140	140	140	140	140
Promass F(HT) DN25/50/80	70	85	100	115	160	205	235	275	350
Promass P/S DN8	---	65	85	100	140	185	200	200	200
Promass P/S DN15/25/40	---	75	100	115	160	200	200	200	200
Promass P/S DN50	60	75	95	110	155	200	200	200	200
Promass X DN350	60	70	85	105	150	185	200	200	200

The ambient temperature is -40°C ... +60°C for the transmitter and -40°C ... +60°C for the sensor.

The minimum medium temperature is -50°C . A special version of Promass A/F/F(HT)/H/O/P/S/X is suitable for medium temperatures down to -200°C.

The minimum medium temperature for Promass E is limited to -40 °C.

**WARNING: SUBSTITUTION OF COMPONENTS MAY IMPAIR INTRINSIC SAFETY.**

Aenderungen:	F	27.04.04/MDI	L	03.08.07/PAM	Alle gesetzlichen Urheberrechte vorbehalten. Diese Zeichnung darf ohne unsere Genehmigung weder vervielfältigt werden noch dritten Personen und Konkurrenzfirmen zugänglich gemacht werden.	<b>Mat.-Nr. 71147429</b>  Ersatz für: Ersteller: FES / <b>ID 1090</b> FILE: M:\ZEICHNUNG\FES0048\P\FES0048P_110523.doc
	G	06.10.04/MDI	M	05.09.07/BDA		
	H	03.08.05/SCHK	N	11.11.09/SCHK		
	J	15.08.06/BDA	P	05.08.11/SCHK		
	K	20.10.06/BDA				

FM Control Drawing Div. 1 / Zone 1  
Class I Zone 1  
Remote Version  
Promass 40/80/83/84 A/E/F/H/I/M/O/P/S/X



Flowtec AG, Kägenstrasse 7, CH-4153 Reinach BL1, Postfach

FES0048P


2/2

Gezeichnet	06.10.00	Bn
Geprüft		
Ex-geprüft	05.08.11	SCHK
Gesehen		

**HAZARDOUS LOCATIONS**

- Cl. I Div. 1 Groups A,B,C,D
- Cl. I Zone 1 Group IIC
- Cl. I Div. 2 Group A,B,C,D
- Cl. I Zone 2 Group IIC
- Cl. II, III Div. 1 Group E,F,G

**NON HAZARDOUS LOCATIONS**

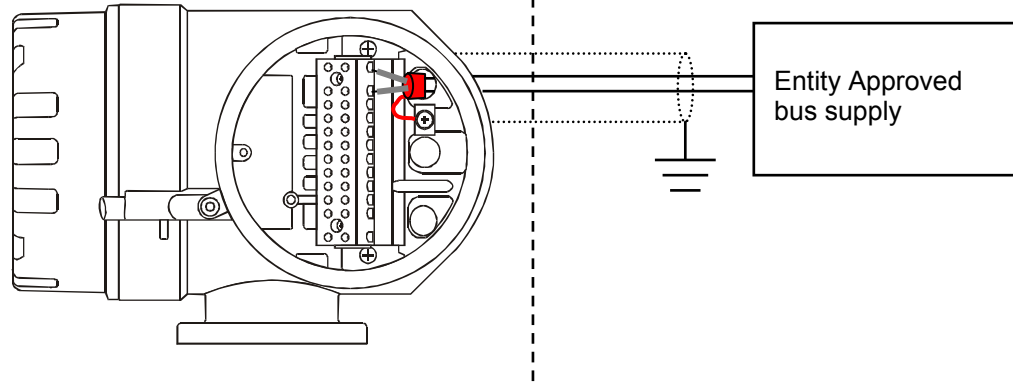

**Notes:**

**Intrinsically safe signal output:**

- 1) Wire intrinsically safe circuits per ISA RP 12.6. or in conduit per NEC ANSI/NFPA 70.
- 2) **WARNING:** SUBSTITUTION OF COMPONENTS MAY IMPAIR INTRINSIC SAFETY.
- 3) Control room equipment may not use or generate more than 250 V rms.

**Type: Promass 8\*\* \*\*\_\*\*\*\*\*F+###**

**Terminals: 26 (+), 27 (-) (Profibus PA):**

Passive intrinsically safe PROFIBUS PA circuit:  
For connecting the intrinsically safe circuit (PROFIBUS PA) according to the FISCO-CONCEPT see FES 0048-0003

**Nonintrinsically safe signal output:**

- 4) Install all intrinsically safe cricuits per NEC ANSI/NFPA 70 and ISA RP 12.6 respecting the Explosionproof Integrity of the enclosure
- 5) **WARNING:** EXPLOSION HAZARD - SUBSTITUTION OF COMPONENTS MAY IMPAIR SUITABILITY FOR CLASS I, DIVISION 1.
- 6) Control room equipment may not use or generate over 250 Vrms.

**Type: Promass 8\*\* \*\*\_\*\*\*\*\*H+###**

**Terminals 26 (+),27 (-) (PROFIBUS PA)**

V 9...32V; I = 12mA

**Type: Promass 8\*\* \*\*\_\*\*\*\*\*J+### (PROFIBUS DP)**

**Promass 8\*\* \*\*\_\*\*\*\*\*Q+### (MODBUS RS)**

**Terminals 24 (+5V),25 (GND), 26 (DPA/RSA), 27 (DPB/RSB)**

Terminals: +5V, GNO, DPA, DPB

V = 5 V, I = 100 mA

Aenderungen:	F	27.04.04/MDI	L	03.08.07/PAM	Alle gesetzlichen Urheberrechte vorbehalten. Diese Zeichnung darf ohne unsere Genehmigung weder vervielfältigt werden noch dritten Personen und Konkurrenzfirmen zugänglich gemacht werden.	<b>Mat.-Nr. 71147429</b>  Ersatz für: Ersteller: FES / <b>ID 1090</b> FILE: M:\ZEICHN\G\FES0048\PI\FES0048P_110523.doc
	G	06.10.04/MDI	M	05.09.07/BDA		
	H	03.08.05/SCHK	N	11.11.09/SCHK		
	J	15.08.06/BDA	P	05.08.11/SCHK		
	K	20.10.06/BDA				

FM Control Drawing Div. 1 / Zone 1  
Promass 40/80/83/84 A/E/F/H/I/M/O/P/S/X  
PROFIBUS PA / IS installation  
PROFIBUS PA / DP or MODBUS RS non-IS installation

Gezeichnet	06.10.00	Bn
Geprüft		
Ex-geprüft	05.08.11	SCHK
Gesehen		



Flowtec AG, Kägenstrasse 7, CH-4153 Reinach BL1, Postfach


**FES0048-0001P**



**HAZARDOUS LOCATIONS**

- Cl. I Div. 1 Groups A,B,C,D
- Cl. I Zone 1 Group IIC
- Cl. I Div. 2 Group A,B,C,D
- Cl. I Zone 2 Group IIC
- Cl. II, III Div. 1 Group E,F,G

**NON HAZARDOUS LOCATIONS**

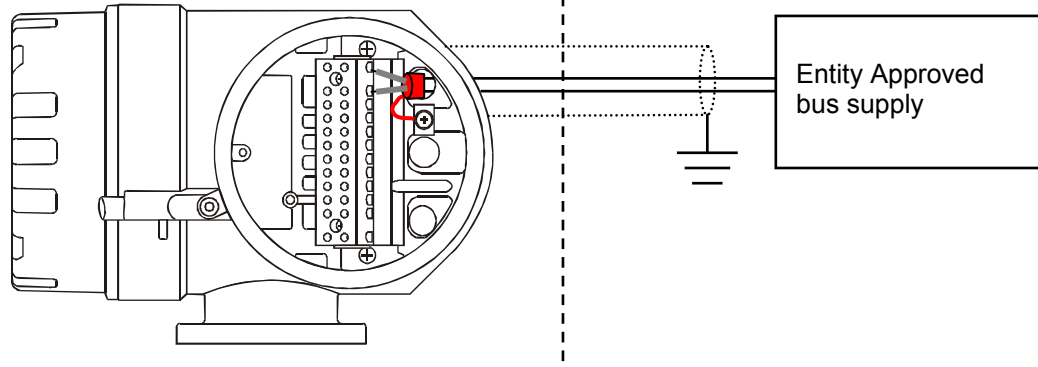

**Notes:**

**Intrinsically safe signal output:**

- 1) Wire all intrinsically circuits per ISA RP 12.6. or in conduit per NEC ANSI/NFPA 70
- 2) **WARNING: SUBSTITUTION OF COMPONENTS MAY IMPAIR INTRINSIC SAFETY.**
- 3) Control room equipment may not use or generate more than 250 Vrms.

**Type: Promass 8\*\* \*\*\_\*\*\*\*\*G+###**

**Terminals: 26, 27 (Foundation Fieldbus):**

Intrinsically safe circuit:

$V_{max} / U_i$	$I_{max} / I_i$	$P_{max} / P_i$	$C_i$	$L_i$
30 V	600 mA	8.5 W	$\leq 5 \text{ nF}$	$\leq 10 \mu\text{H}$

Connect to entity approved associated apparatus with

$I_{sc}, I_t \text{ or } I_o \leq I_{max} \text{ or } I_i$  and

$V_{oc}, V_t \text{ or } U_o \leq V_{max} \text{ or } U_i$

$(P_o \leq P_{max} \text{ or } P_i)$

Cable parameters for Intrinsic Safety:

$C_{cable} \leq C_a / C_o - \sum C_i$

$L_{cable} \leq L_a / L_o - \sum L_i \text{ or}$

$L/R_{cable} \leq L/R_{Associated Apparatus}$  and  $L_i$  of each I.S. apparatus  $\leq 10 \mu\text{H}$

Alternatively the intrinsically safe circuit ( Fieldbus Foundation) can be connected according to the FISCO – Concept ( see FES 0048–0003 ).

**Nonintrinsically safe signal output:**

- 4) Install all intrinsically safe cricuits per NEC ANSI/NFPA 70 and ISA RP 12.6 respecting the Explosionproof Integrity of the enclosure
- 5) **WARNING: EXPLOSION HAZARD - SUBSTITUTION OF COMPONENTS MAY IMPAIR SUITABILITY FOR CLASS I, DIVISION 1.**
- 6) Control room equipment may not use or generate over 250 Vrms.

**Type: Promass 8\*\* \*\*\_\*\*\*\*\*K+###**

**Terminals 26,27 (FIELDBUS FOUNDATION NON I.S.)**

$V 9...32V ; I = 12mA$

Aenderungen:	F	27.04.04/MDI	L	03.08.07/PAM	Alle gesetzlichen Urheberrechte vorbehalten. Diese Zeichnung darf ohne unsere Genehmigung weder vervielfältigt werden noch dritten Personen und Konkurrenzfirmen zugänglich gemacht werden.	<b>Mat.-Nr. 71147429</b>  Ersatz für: Ersteller: FES / <b>ID 1090</b> FILE: M:\ZEICHN\GFES0048\PFES0048P_110523.doc
	G	06.10.04/MDI	M	05.09.07/BDA		
	H	03.08.05/SCHK	N	11.11.09/SCHK		
	J	15.08.06/BDA	P	05.08.11/SCHK		
	K	20.10.06/BDA				

FM Control Drawing Div. 1 / Zone 1  
 Promass 40/80/83/84 A/E/F/H/I/M/O/P/S/X  
 Fieldbus Foundation IS installation  
 Fieldbus Foundation non-IS installation

Gezeichnet	06.10.00	Bn
Geprüft		
Ex-geprüft	05.08.11	SCHK
Gesehen		



Flowtec AG, Kägenstrasse 7, CH-4153 Reinach BL1, Postfach

**FES0048-0002P**

**FISCO CONCEPT**

The FISCO Concept allows interconnection of intrinsically safe apparatus to associated apparatus not specially examined in such combination. The criteria for interconnection is that the voltage ( $U_i$  or  $V_{max}$ ), the current ( $I_i$  or  $I_{max}$ ), and the power ( $P_i$  or  $P_{max}$ ) which intrinsically safe apparatus can receive and remain intrinsically safe, considering faults, must be equal or greater than the voltage ( $U_o$ ,  $V_{oc}$  or  $V_t$ ), the current ( $I_o$ ,  $I_{sc}$  or  $I_t$ ) and the power ( $P_o$  or  $P_{max}$ ) levels which can be delivered by the associated apparatus, considering faults and applicable factors. In addition, the maximum unprotected capacitance ( $C_i$ ) and inductance ( $L_i$ ) of each apparatus (other than the termination) connected to the fieldbus must be less than or equal to 5 nF and 10 µH respectively.

In each segment only one active device, normally the associated apparatus, is allowed to provide the necessary energy for the fieldbus system. The voltage  $U_o$  (or  $V_{oc}$  or  $V_t$ ) of the associated apparatus is limited to a range of 14V to 24Vd.c. All other equipment connected to the bus cable has to be passive, meaning that they are not allowed to provide energy to the system, except a leakage current of 50µA for each connected device. Separately powered equipment needs a galvanic isolation to assure that the intrinsically safe fieldbus circuit remains passive.

The cable used to interconnect the devices needs to have the parameter in the following range:

Loop Resistance  $R'$  : 15...150 Ohm/km  
 Inductance per unit length  $L'$  : 0.4...1 mH/km  
 Capacitance per unit length  $C'$  : 80...200 nF

$C' = C' \text{ line/line} + 0.5 C' \text{ line/screen}$ , if both lines are floating, or  
 $C' = C' \text{ line/line} + C' \text{ line/screen}$ , if the screen is connected to one line  
 Length of trunk cable: ≤ 1000 m  
 Length of spur cable: ≤ 30 m  
 Length of splice: ≤ 1 m

At each end of the trunk cable an approved infallible line termination with following parameters is suitable:

$R = 90...100 \text{ Ohm}$        $C = 0...2.2 \text{ µF}$

One of the allowed terminations might already be integrated in the associated apparatus. The number of passive apparatus connected to the bus segment is not limited due to I.S. reasons. If the above rules are respected, up to a total length of 1000 m (sum of trunk and all spur cables), the inductance and the capacitance of the cable will not impair the intrinsic safety of the installation.

**Notes:**

Intrinsically safe Class I, Div.1, Groups A, B, C, D


- Approved associated apparatus must be installed in accordance with manufacturers instructions.
- FM approved associated apparatus must meet the following parameters:  
 $U_o$  or  $V_{oc}$  or  $V_t \leq U_i$  ( $V_{max}$ ) and  $I_o$  or  $I_{sc}$  or  $I_t \leq I_i$  ( $I_{max}$ ) and  $P_o$  or  $P_{max} \leq P_i$  ( $P_{max}$ )
- The maximum non-hazardous area voltage must not exceed 250V
- The installation must be in accordance with the National Electrical Code NFPA 70, and ANSI/ISA-Rp 12.6. (except chapter 5).
- Multiple earthing of screen is allowed only, if high integrity equipotential system is realized between the points of bonding (see drawing No. FES 0014 ).
- Caution: Use only supply wires suitable for 5°C above surrounding temperature.
- Warning : Substitution of components may impair intrinsic safety.
- The polarity for connection PA+ (26) and PA- (27) is of no importance due to an internal rectifier.

**HAZARDOUS (CLASSIFIED) LOCATION**

Class I, Division 1, Groups A,B,C,D  
 Class II, Division 1, Groups E,F,G  
 Class III, Division 1

**NONHAZARDOUS LOCATION**

Promass \*\*\*\*\*F/G+##\*\*#

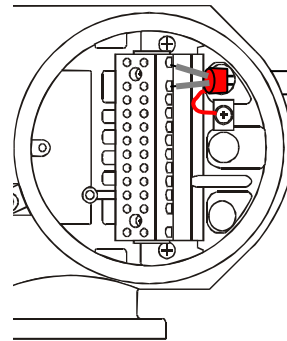


Any FM Approved Intrinsically Safe Apparatus suitable for FISCO Concept

Promass 8** *...*****F/G+##**#	
Terminal 26 (+) Terminal 27 (-) (FISCO-Model)	
$U_i$ ( $V_{max}$ ) = 30 V	$C_i \leq 5 \text{ nF}$
$I_i$ ( $I_{max}$ ) = 600 mA	$L_i \leq 10 \text{ µH}$
$P_i$ ( $P_{max}$ ) = 8.5 W	
Leakage current : ≤ 50µA	
Apparatus provides galvanic isolation up to 250V rms between fieldbus circuit and any other circuit	
Temperature Classification: T6	
Max. ambient Temperature: 60°C / 140°F	

Any FM Approved Termination with  
 $R = 90...100 \Omega$   
 $C = 0...2.2 \text{ µF}$

Keine Änderungen ohne vorherige Factory Mutual Genehmigung

Any FM Approved Associated Apparatus Suitable for Fisco concept

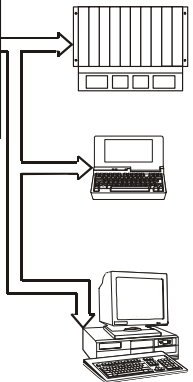

Änderungen:	F	27.04.04/MDI	L	03.08.07/PAM	Alle gesetzlichen Urheberrechte vorbehalten. Diese Zeichnung darf ohne unsere Genehmigung weder vervielfältigt werden noch dritten Personen und Konkurrenzfirmen zugänglich gemacht werden.	<b>Mat.-Nr. 71147429</b>  Ersatz für: Ersteller: FES / <b>ID 1090</b> FILE: M\ZEICHN\G\FES0048\PI\FES0048P_110523.doc
	G	06.10.04/MDI	M	05.09.07/BDA		
	H	03.08.05/SCHK	N	11.11.09/SCHK		
	J	15.08.06/BDA	P	05.08.11/SCHK		
	K	20.10.06/BDA				


FM Control Drawing Div. 1 / Zone 1  
 Promass 40/80/83/84 A/E/F/H/I/M/O/P/S/X  
 Intrinsically safe PROFIBUS PA  
 Foundation Fieldbus  
 FISCO-Concept

Gezeichnet	06.10.00	Bn
Geprüft		
Ex-geprüft	05.08.11	SCHK
Gesehen		

**NON HAZARDOUS LOCATION**

**HAZARDOUS LOCATION**

Cl. I, Zone 1 IIC  
 Cl. I, II, III Div. 1 Group A,B,C,D,E,F,G or  
 Cl. I Div. 2 Group A,B,C,D, and Cl.II,III Div.1 Group E,F,G

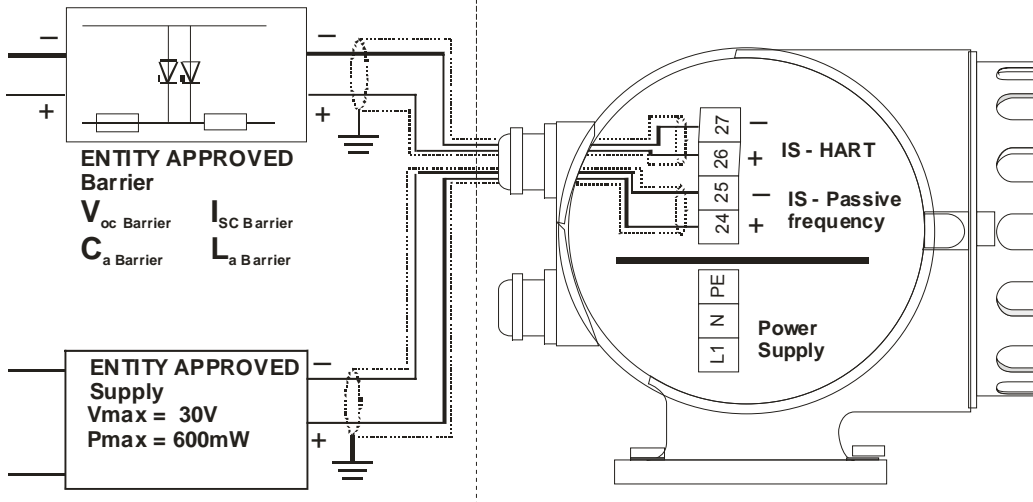

**Notes:**

- 1) Use supply wires suitable for 5 °C above surrounding ambient, but at least for 80°C/176°F
- 2) **Intrinsically safe signal output:** Install all intrinsically safe circuits per NEC ANSI/NFPA 70 and ISA RP 12.6 respecting the Explosionproof Integrity of the enclosure
- 3) **WARNING:** SUBSTITUTION OF COMPONENTS MAY IMPAIR INTRINSIC SAFETY.
- 4) Control room equipment may not use or generate more than 250 Vrms.

**Type: Promass 8\*\* \*\_\*\*\*\*\*S+###**

**Promass 40\* \*\_\*\*\*\*\*S+###**

**Terminals: 26, 27 (HART current output):**

Active intrinsically safe circuit:

V <sub>oc</sub> / U <sub>o</sub>	I <sub>sc</sub> / I <sub>o</sub>	P <sub>max</sub> / P <sub>o</sub>	C <sub>a</sub> / C <sub>o</sub>	L <sub>a</sub> / L <sub>o</sub>
21.8 V	90 mA	490 mW	0.15 µF	4.1 mH

V <sub>max</sub> / U <sub>i</sub>	I <sub>max</sub> / I <sub>i</sub>	P <sub>max</sub> / P <sub>i</sub>	C <sub>i</sub>	L <sub>i</sub>
30 V	10 mA	300 mW	6 nF	0

Cable parameters for Intrinsic Safety:

$$C_{\text{cable}} \leq 0.15 \mu\text{F} \quad \text{if } V_{\text{oc}} \text{ (of Barrier)} \leq 21.8 \text{ V}$$

$$C_{\text{cable}} \leq C_a \text{ Barrier} - 6 \text{ nF} \quad \text{if } V_{\text{oc}} \text{ (of Barrier)} \geq 21.8 \text{ V}$$

$$L_{\text{cable}} \leq 4.1 \text{ mH}$$

**Terminals 24, 25 (Passive intrinsically safe circuit):**

V <sub>max</sub> / U <sub>i</sub>	I <sub>max</sub> / I <sub>i</sub>	P <sub>max</sub> / P <sub>i</sub>	C <sub>i</sub>	L <sub>i</sub>
30 V	300 mA	600mW	6 nF	0

Entity approved supply must meet the following requirements:

$$V_{\text{oc}}, V_t \text{ or } U_o \leq V_{\text{max}} \quad P_{\text{max}} \text{ or } P_o \leq P_{\text{max}} / P_i$$

Cable parameters for Intrinsic Safety:

$$C_{\text{cable}} \leq C_a (C_o) - 6\text{nF} \quad L_{\text{cable}} \leq L_a (L_o)$$

**Type: Promass 8\*\* \*\_\*\*\*\*\*T+###**

**Promass 40\* \*\_\*\*\*\*\*T+###**

**Terminals: 26, 27 (HART current output):**

Passive intrinsically safe circuit:

V <sub>max</sub> / U <sub>i</sub>	I <sub>max</sub> / I <sub>i</sub>	P <sub>max</sub> / P <sub>i</sub>	C <sub>i</sub>	L <sub>i</sub>
30 V	100 mA	1.25 W	6 nF	negligible

Connect to entity approved Barrier with

$$V_{\text{oc}}, V_t \text{ or } U_o \leq V_{\text{max}} / U_i$$

$$I_{\text{sc}}, I_t \text{ or } I_o \leq I_{\text{max}} / I_i$$

Cable parameters for Intrinsic Safety:

$$C_{\text{cable}} \leq C_a \text{ Barrier or } C_o \text{ Barrier} - 6 \text{ nF}$$

$$L_{\text{cable}} \leq L_a \text{ Barrier or } L_o \text{ Barrier}$$

**Terminals 24, 25 (Passive intrinsically safe circuit):**

V <sub>max</sub> / U <sub>i</sub>	I <sub>max</sub> / I <sub>i</sub>	P <sub>max</sub> / P <sub>i</sub>	C <sub>i</sub>	L <sub>i</sub>
30 V	300 mA	600mW	6 nF	0

Entity approved apparatus must meet the following requirements:

$$V_{\text{oc}}, V_t \text{ or } U_o \leq V_{\text{max}} \quad P_{\text{max}} \text{ or } P_o \leq P_{\text{max}} / P_i$$


Cable parameters for Intrinsic Safety:

$$C_{\text{cable}} \leq C_a (C_o) - 6 \text{ nF} \quad L_{\text{cable}} \leq L_a (L_o)$$

Aenderungen:	F	27.04.04/MDI	L	03.08.07/PAM	Alle gesetzlichen Urheberrechte vorbehalten. Diese Zeichnung darf ohne unsere Genehmigung weder vervielfältigt werden noch dritten Personen und Konkurrenzfirmen zugänglich gemacht werden.	<b>Mat.-Nr. 71147429</b>  Ersatz für: Ersteller: FES / <b>ID 1090</b> FILE: M:\ZEICHN\GIFES0048\VFES0048P_110523.doc
	G	06.10.04/MDI	M	05.09.07/BDA		
	H	03.08.05/SCHK	N	11.11.09/SCHK		
	J	15.08.06/BDA	P	05.08.11/SCHK		
	K	20.10.06/BDA				


FM Control Drawing Cl. I, Div. 1			Gezeichnet	06.10.00	Bn
Promass 40/80/83/84 A/E/F/H/I/M/O/P/S/X			Geprüft		
Entity concept Commodul HART IS (Option S/T)			Ex-geprüft	05.08.11	SCHK
			Gesehen		

**NON HAZARDOUS LOCATION**

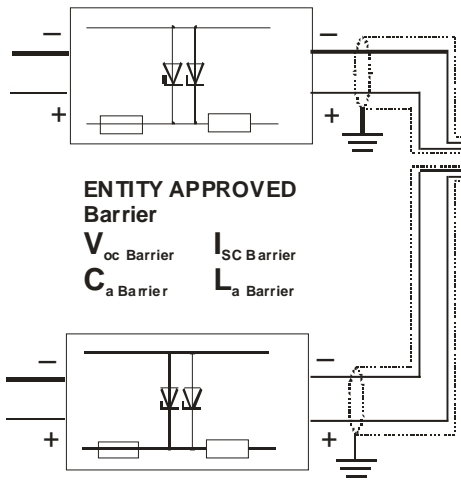

**HAZARDOUS LOCATION**

Cl. I, Zone 1 IIC  
 Cl. I, II, III Div. 1 Group A,B,C,D,E,F,G or  
 Cl. I Div. 2 Group A,B,C,D, and Cl.II,III Div.1 Group E,F,G

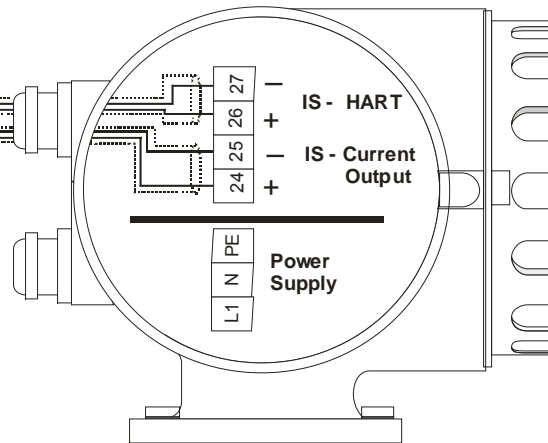

**Notes:**

- 1) Use supply wires suitable for 5 °C above surrounding ambient, but at least for 80°C/176°F
- 2) **Intrinsically safe signal output:** Install all intrinsically safe circuits per NEC ANSI/NFPA 70 and ISA RP 12.6 respecting the Explosionproof Integrity of the enclosure
- 3) **WARNING:** SUBSTITUTION OF COMPONENTS MAY IMPAIR INTRINSIC SAFETY.
- 4) Control room equipment may not use or generate more than 250 Vrms.

**Type: Promass 8\*\* \*\_\*\*\*\*\*R+###**

**Promass 40\* \*\_\*\*\*\*\*R+###**

**Terminals: 26, 27 (HART current output):**

**Terminals: 24, 25 (current output):**

**Active:**

$V_{oc} / U_o$	$I_{sc} / I_o$	$P_{max} / P_o$	$C_a / C_o$	$L_a / L_o$
21.8 V	90 mA	490 mW	0.15 µF	4.1 mH

$V_{max} / U_i$	$I_{max} / I_i$	$P_{max} / P_i$	$C_i$	$L_i$
30 V	10 mA	300 mW	6 nF	0

**Cable parameters for Intrinsic Safety:**

- $C_{cable} \leq 0.15 \mu F$  if  $V_{oc} \text{ (of Barrier)} \leq 21.8 V$
- $C_{cable} \leq C_a \text{ Barrier} - 6 nF$  if  $V_{oc} \text{ (of Barrier)} \geq 21.8 V$
- $L_{cable} \leq 4.1 mH$

**Type: Promass 8\*\* \*\_\*\*\*\*\*U+###**

**Promass 40\* \*\_\*\*\*\*\*U+###**

**Terminals: 26, 27 (HART current output)**

**Terminals: 24, 25 (current output)**

**Passive:**

$V_{max} / U_i$	$I_{max} / I_i$	$P_{max} / P_i$	$C_i$	$L_i$
30 V	100 mA	1.25 W	6 nF	negligible

Connect to entity approved Barrier with

$V_{OC}, V_t \text{ or } U_o \leq V_{max} / U_i$

$I_{sc}, I_t \text{ or } I_o \leq I_{max} / I_i$

Cable parameters for Intrinsic Safety:

$C_{cable} \leq C_a \text{ Barrier or } C_o \text{ Barrier} - 6 nF$

$L_{cable} \leq L_a \text{ Barrier or } L_o \text{ Barrier}$

Aenderungen:	F	27.04.04/MDI	L	03.08.07/PAM	Alle gesetzlichen Urheberrechte vorbehalten. Diese Zeichnung darf ohne unsere Genehmigung weder vervielfältigt werden noch dritten Personen und Konkurrenzfirmen zugänglich gemacht werden.	<b>Mat.-Nr. 71147429</b>  Ersatz für: Ersteller: FES / <b>ID 1090</b> FILE: M:\ZEICHN\GIFES0048\PI\FES0048P_110523.doc
	G	06.10.04/MDI	M	05.09.07/BDA		
	H	03.08.05/SCHK	N	11.11.09/SCHK		
	J	15.08.06/BDA	P	05.08.11/SCHK		
	K	20.10.06/BDA				

FM Control Drawing Cl. I, Div. 1 Promass 40/80/83/84 A/E/F/H/I/M/O/P/S/X Entity concept Commodul HART IS (Option R/U)	Gezeichnet	06.10.00	Bn
	Geprüft		
	Ex-geprüft	05.08.11	SCHK
	Gesehen		



Flowtec AG, Kägenstrasse 7, CH-4153 Reinach BL1, Postfach

**FES0048-0005P**